

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042723\
 Data File : VX035335.D
 Acq On : 27 Apr 2023 12:52
 Operator : JC/MD
 Sample : 02485-01 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 33992

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M

Title : SW846 8260

Signal : TIC: VX035335.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	694	705	721	rBV2	130847	387405	32.24%	5.696%
2	5.550	721	732	751	rVB	242204	693857	57.75%	10.202%
3	5.958	789	799	808	rBV	144642	384850	32.03%	5.659%
4	6.037	808	812	825	rVB2	16815	44965	3.74%	0.661%
5	6.763	920	931	946	rBV	373546	892062	74.25%	13.117%
6	8.647	1233	1240	1247	rBV	759654	1201446	100.00%	17.666%
7	8.720	1247	1252	1264	rVB	100000	160429	13.35%	2.359%
8	10.055	1465	1471	1490	rBV	751868	1031981	85.89%	15.174%
9	10.305	1505	1512	1520	rBV	31875	48346	4.02%	0.711%
10	10.640	1561	1567	1577	rBV	48759	67300	5.60%	0.990%
11	11.079	1634	1639	1649	rBV	607287	792125	65.93%	11.647%
12	11.378	1682	1688	1697	rBV3	6177	14499	1.21%	0.213%
13	12.024	1788	1794	1801	rBV	725529	928929	77.32%	13.659%
14	12.085	1801	1804	1811	rVB	11197	14847	1.24%	0.218%
15	13.292	1994	2002	2009	rBV3	7182	15748	1.31%	0.232%
16	14.481	2193	2197	2207	rVB7	6111	15611	1.30%	0.230%
17	14.615	2215	2219	2224	rBV5	10574	16294	1.36%	0.240%
18	14.755	2234	2242	2246	rBV2	20579	25994	2.16%	0.382%
19	15.487	2357	2362	2368	rBV	22917	37387	3.11%	0.550%
20	16.377	2500	2508	2513	rBV2	14250	26944	2.24%	0.396%




Sum of corrected areas: 6801019

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042723\
Data File : VX035335.D
Acq On : 27 Apr 2023 12:52
Operator : JC/MD
Sample : 02485-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

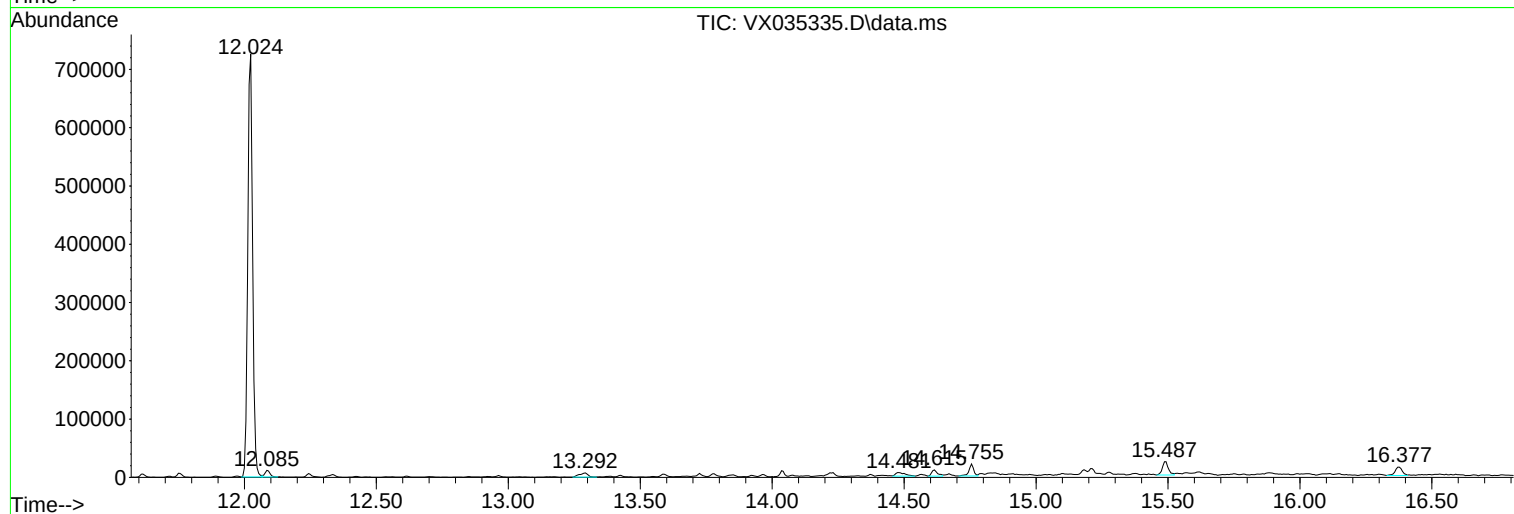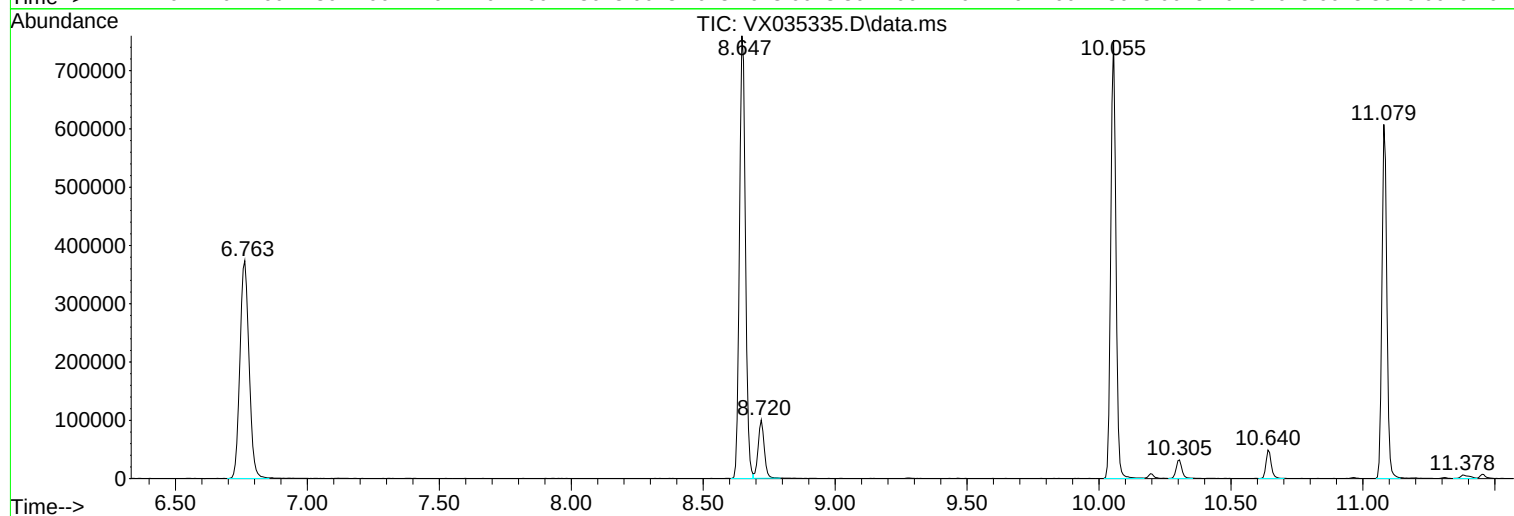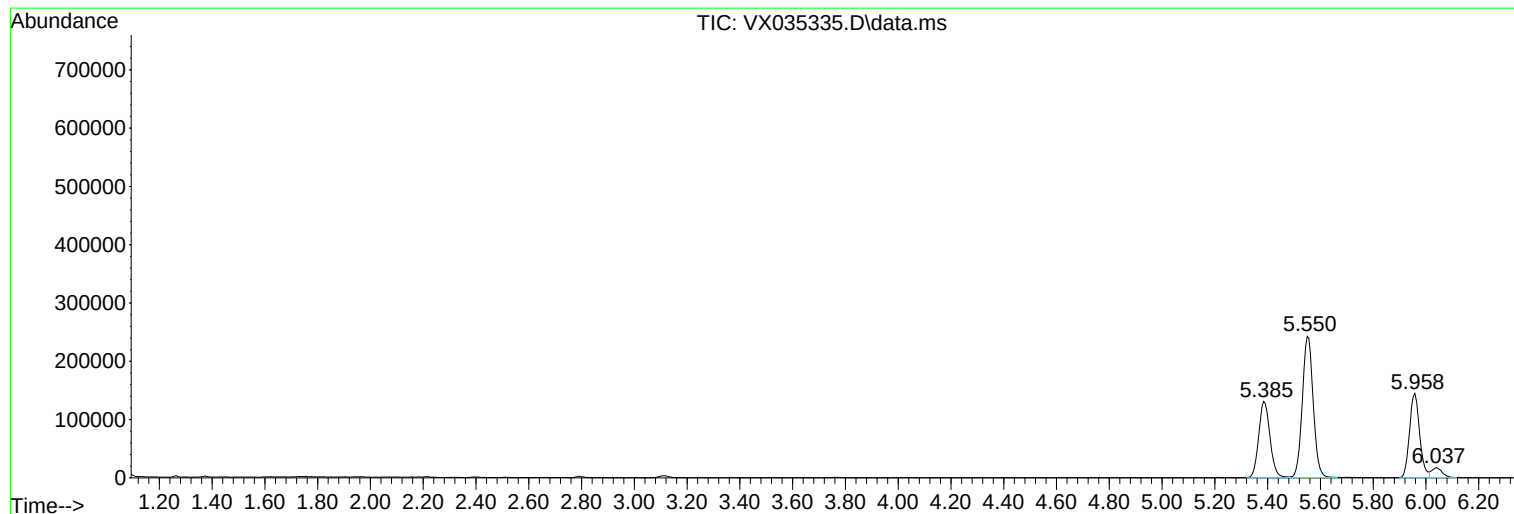

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042723\
Data File : VX035335.D
Acq On : 27 Apr 2023 12:52
Operator : JC/MD
Sample : 02485-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042723\
Data File : VX035335.D
Acq On : 27 Apr 2023 12:52
Operator : JC/MD
Sample : 02485-01 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
33992

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------