

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042723\  
Data File : VX035343.D  
Acq On : 27 Apr 2023 15:58  
Operator : JC/MD  
Sample : 02492-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-041

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042523W.M

Title : SW846 8260

Signal : TIC: VX035343.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 4.489       | 544           | 558         | 589          | rBV      | 4413834        | 12106504      | 20.93%          | 16.074%       |
| 2         | 5.550       | 721           | 732         | 749          | rVB      | 232938         | 668148        | 1.16%           | 0.887%        |
| 3         | 6.763       | 920           | 931         | 948          | rBV      | 361927         | 865793        | 1.50%           | 1.150%        |
| 4         | 7.141       | 978           | 993         | 1021         | rBV      | 24314697       | 57830568      | 100.00%         | 76.784%       |
| 5         | 8.647       | 1234          | 1240        | 1258         | rBV      | 737302         | 1175425       | 2.03%           | 1.561%        |
| 6         | 10.055      | 1465          | 1471        | 1493         | rBV      | 721998         | 1001334       | 1.73%           | 1.330%        |
| 7         | 11.079      | 1634          | 1639        | 1658         | rBV      | 581167         | 770599        | 1.33%           | 1.023%        |
| 8         | 12.024      | 1788          | 1794        | 1807         | rBV      | 694949         | 897340        | 1.55%           | 1.191%        |




Sum of corrected areas: 75315711

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042723\  
Data File : VX035343.D  
Acq On : 27 Apr 2023 15:58  
Operator : JC/MD  
Sample : 02492-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

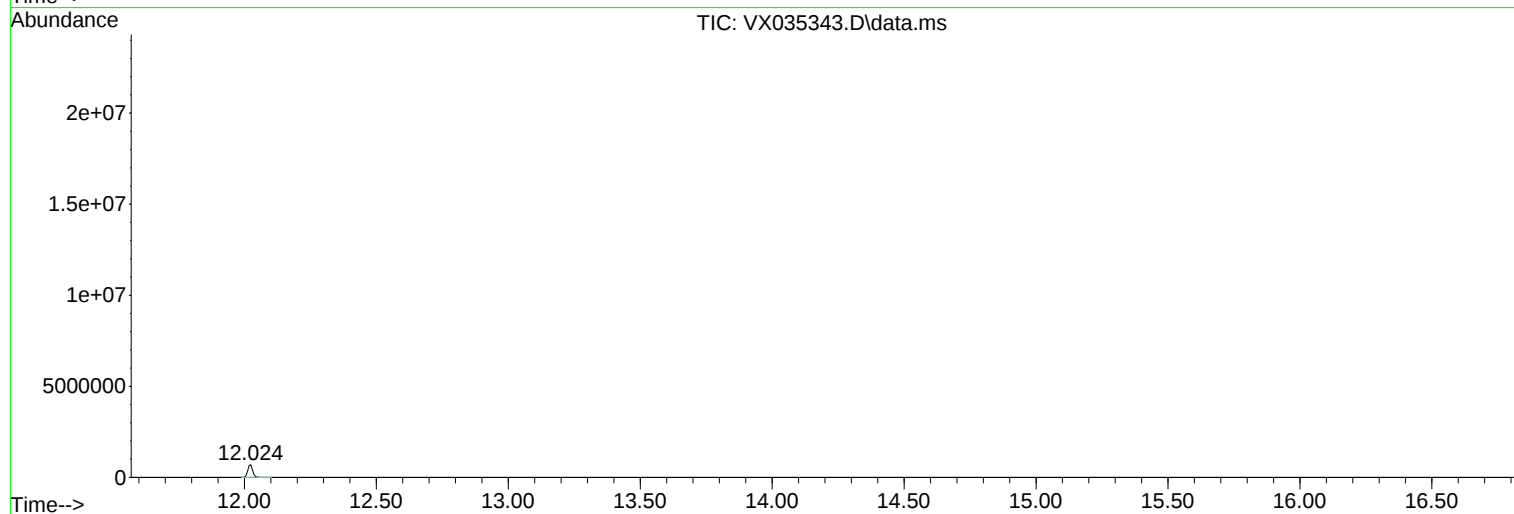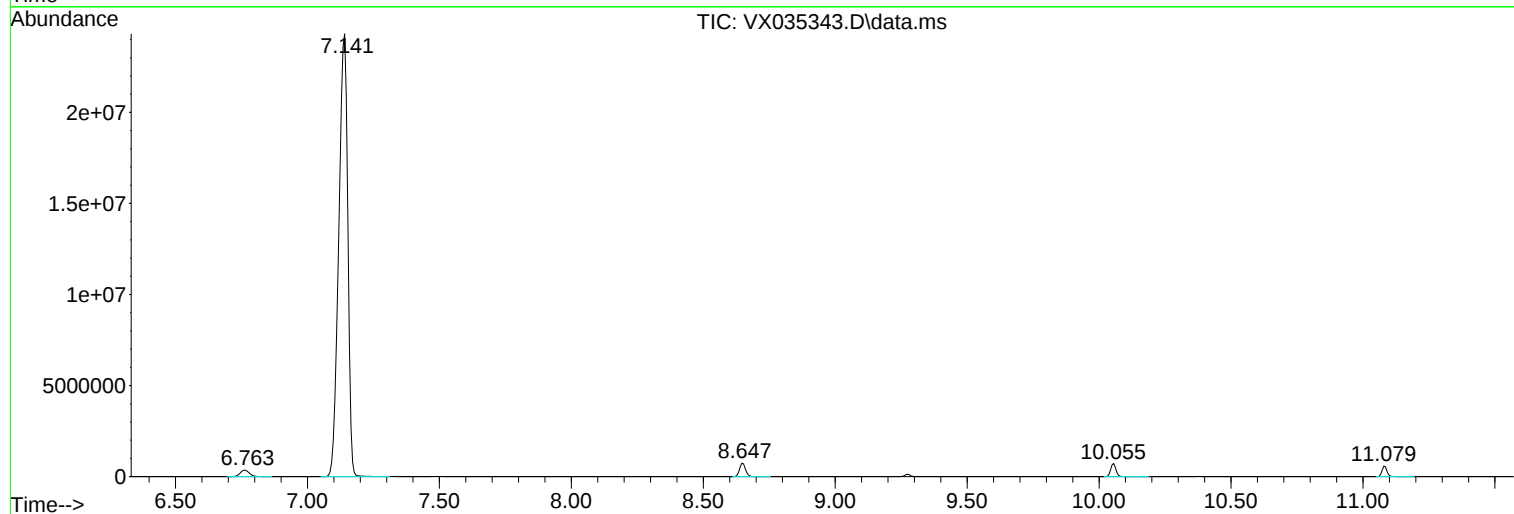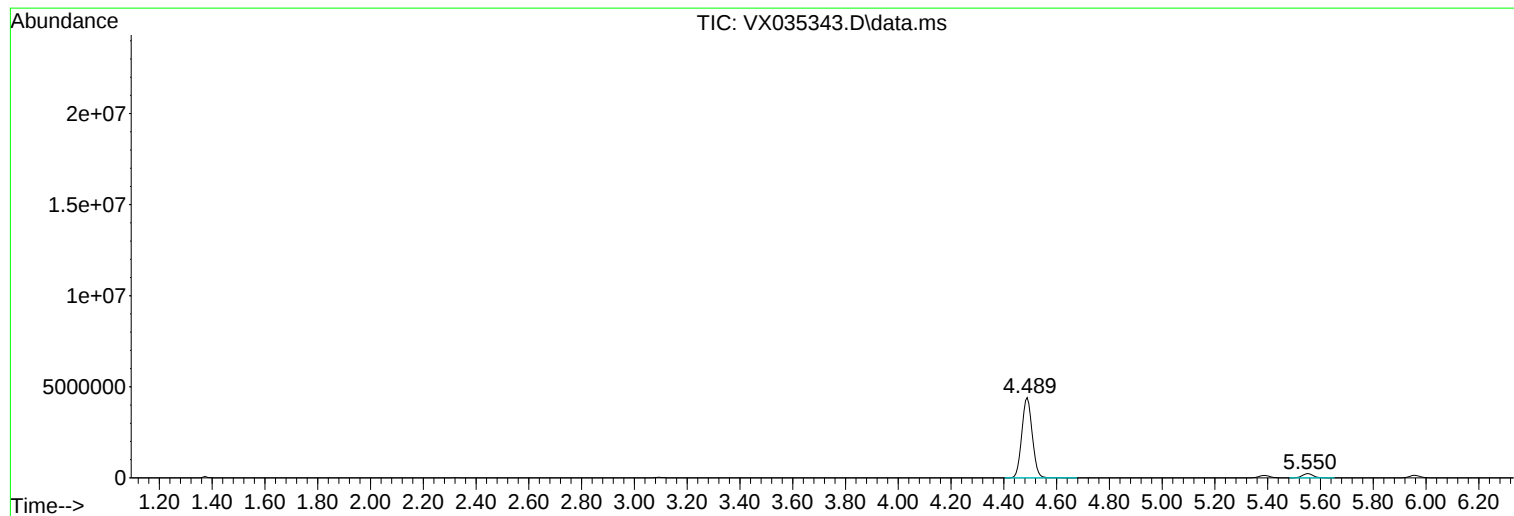

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042723\  
Data File : VX035343.D  
Acq On : 27 Apr 2023 15:58  
Operator : JC/MD  
Sample : 02492-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042723\  
Data File : VX035343.D  
Acq On : 27 Apr 2023 15:58  
Operator : JC/MD  
Sample : 02492-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 18 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
22-MW-041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042523W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|