
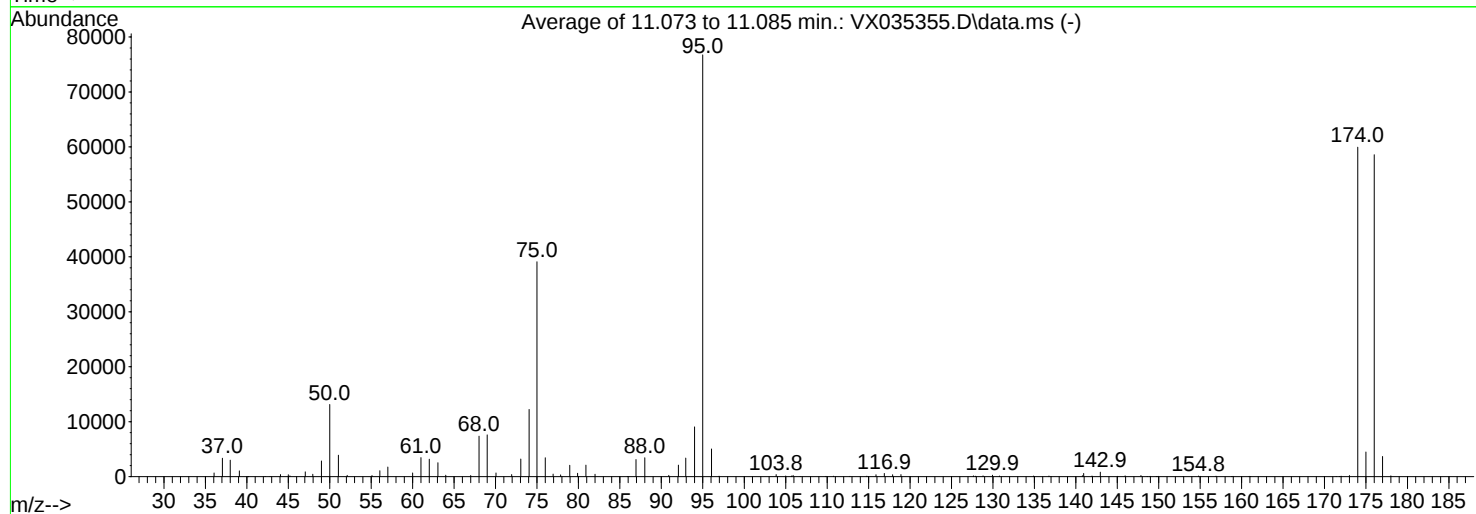


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042723\
Data File : VX035355.D
Acq On : 28 Apr 2023 00:04
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y042423S.M
Title : SW846 8260
Last Update : Tue Apr 25 02:39:58 2023

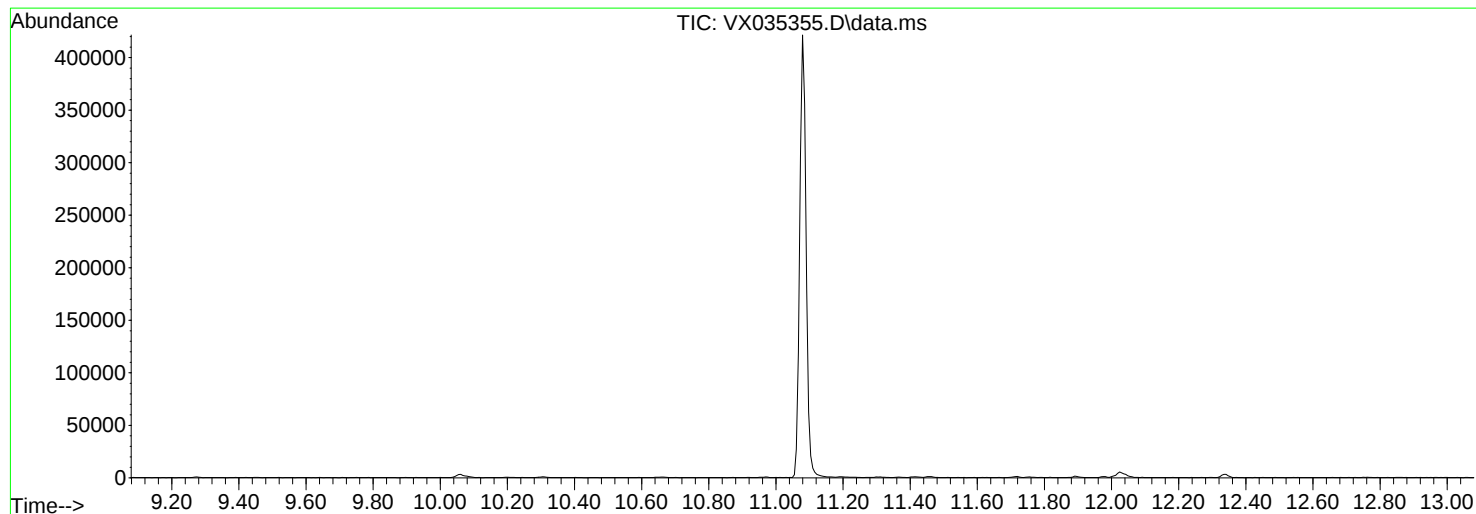

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	13123	PASS
75	95	30	60	50.9	39104	PASS
95	95	100	100	100.0	76752	PASS
96	95	5	9	6.6	5039	PASS
173	174	0.00	2	0.3	207	PASS
174	95	50	100	78.1	59939	PASS
175	174	5	9	7.5	4495	PASS
176	174	95	101	97.8	58595	PASS
177	176	5	9	6.3	3680	PASS