



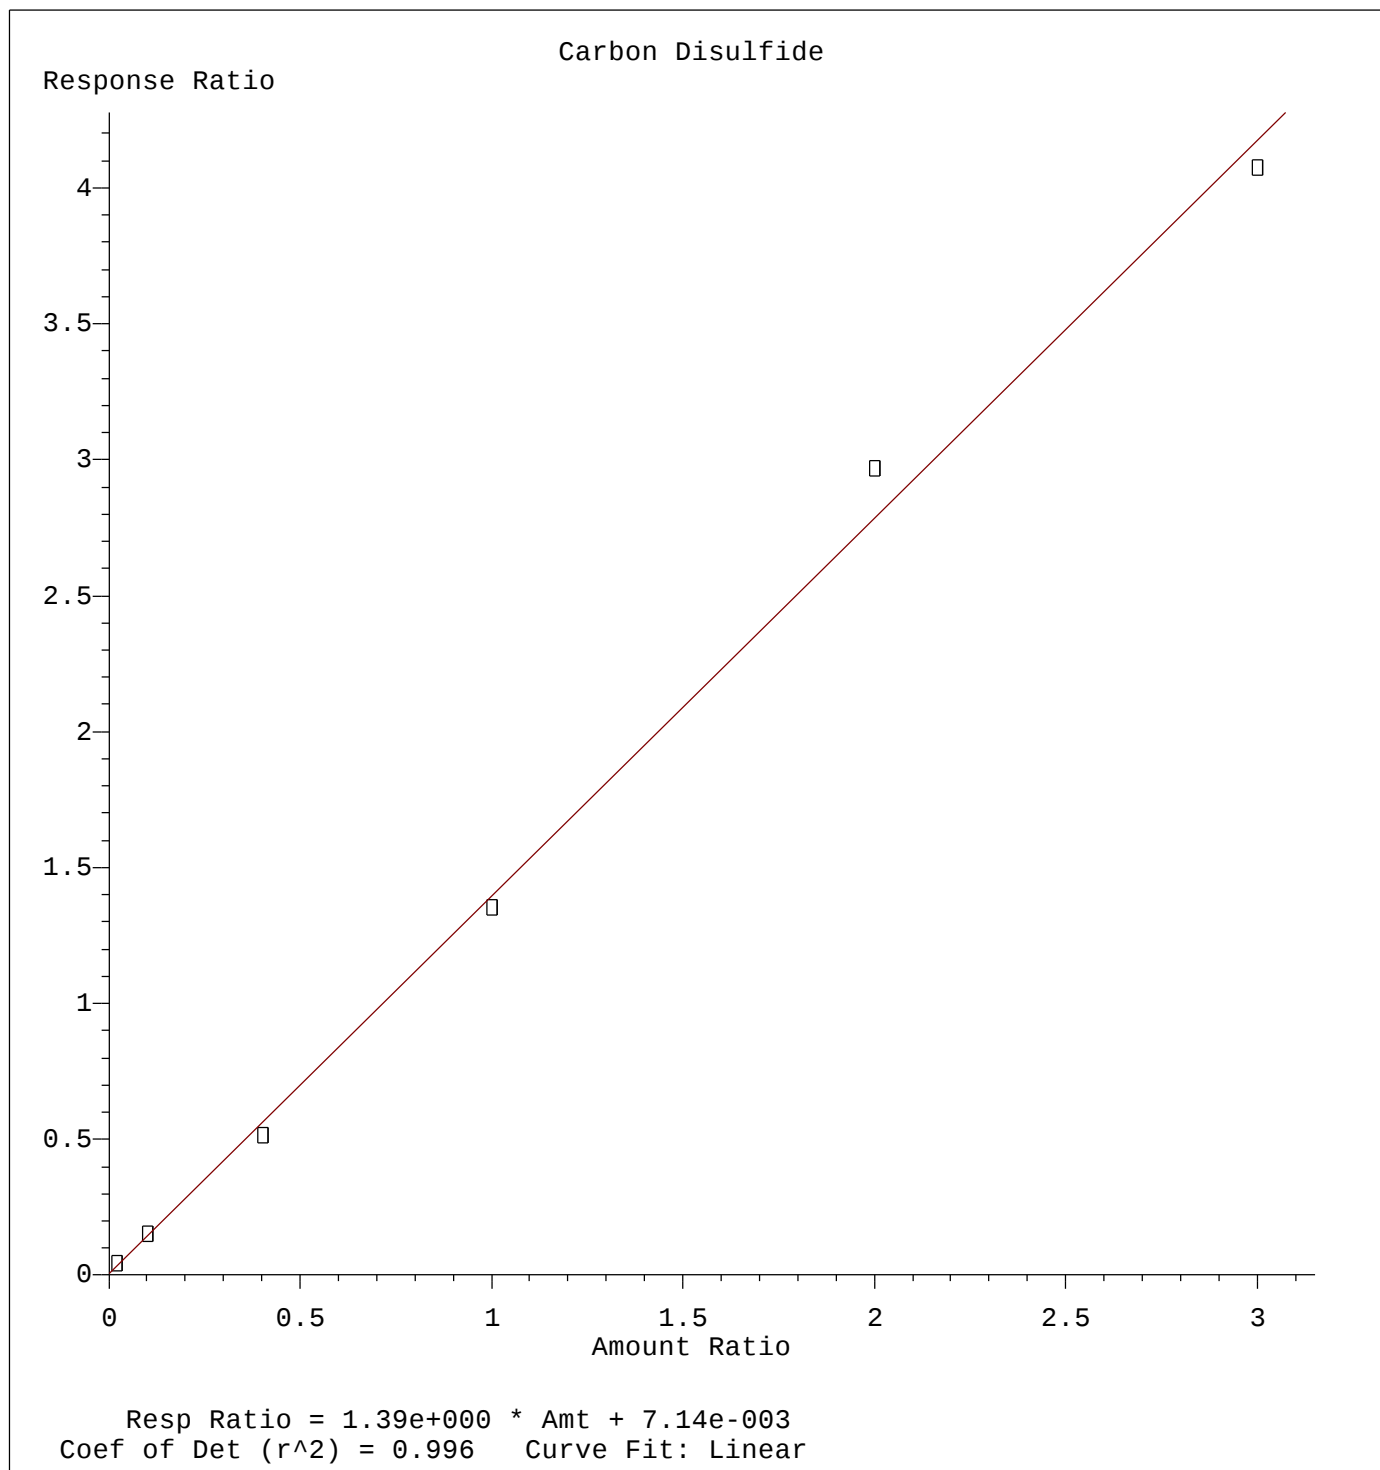


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Calibration Table Last Updated: Tue Apr 28 17:30:11 2020

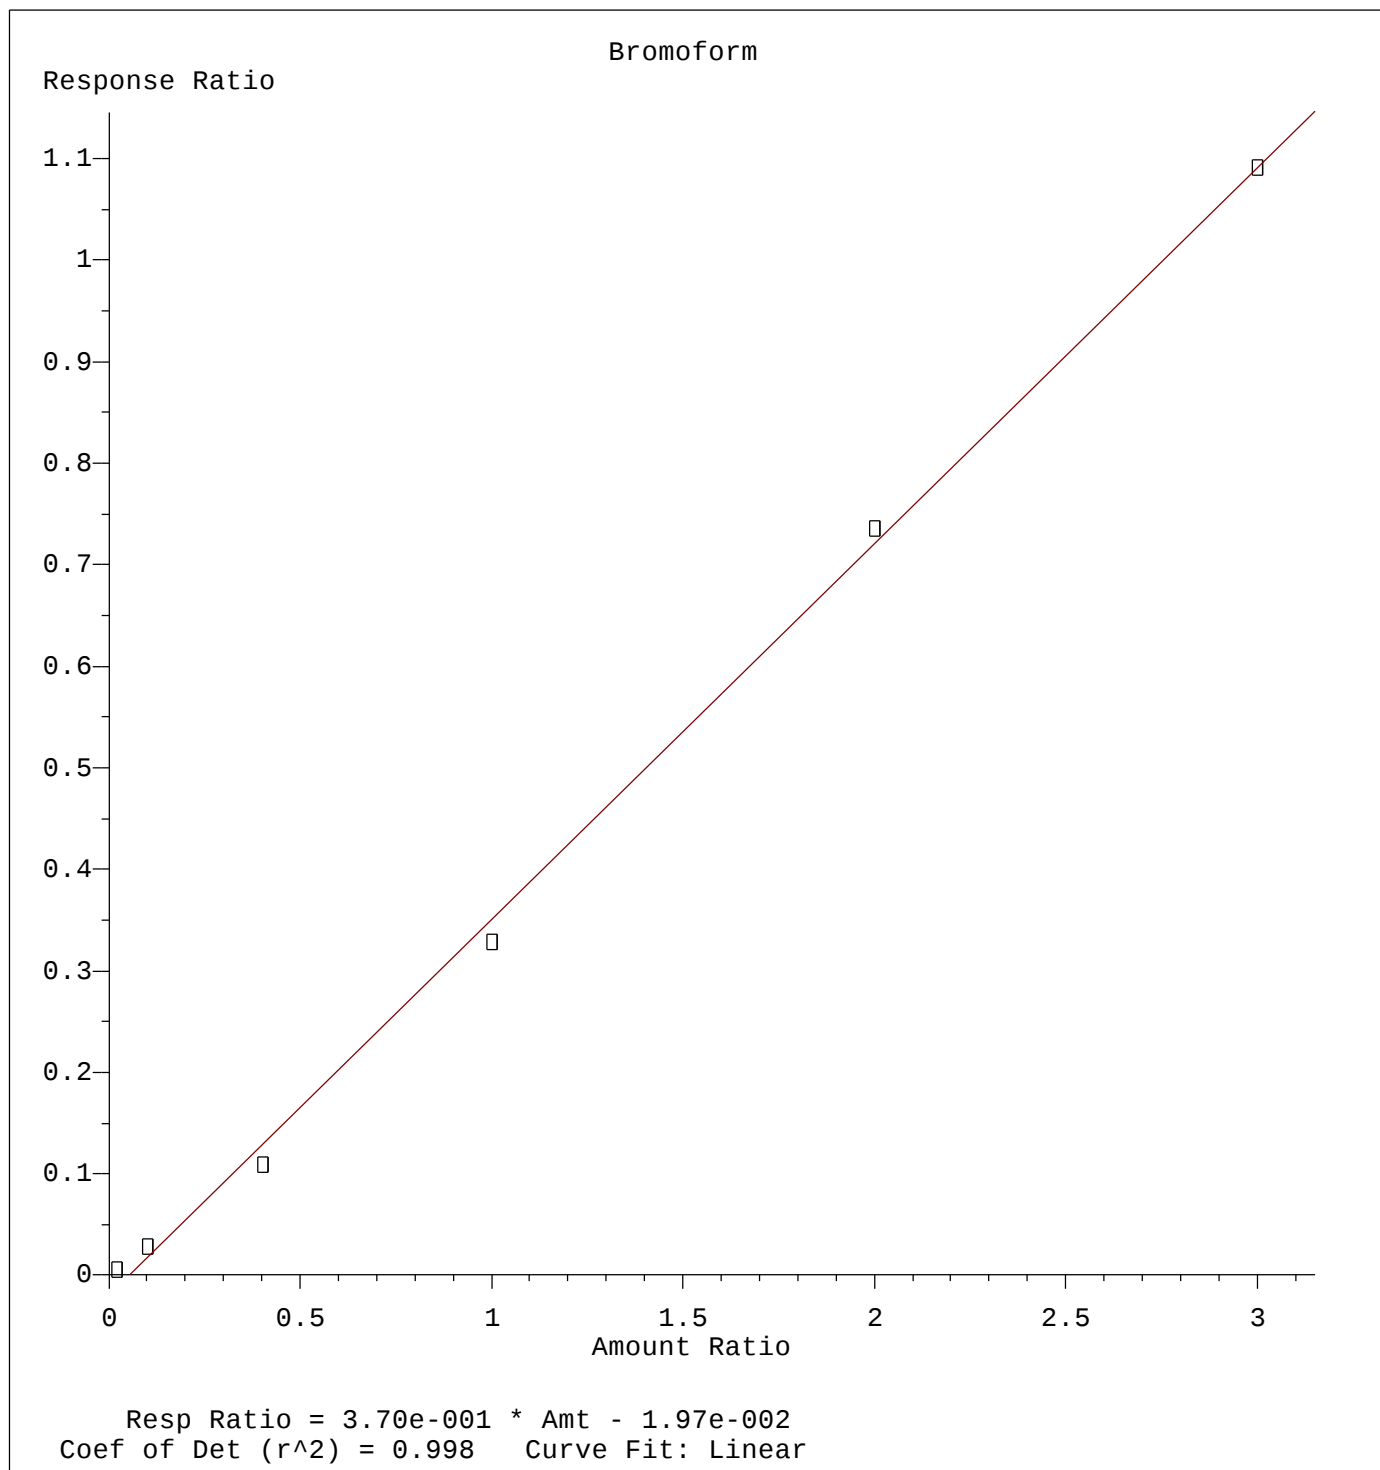

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Calibration Table Last Updated: Tue Apr 28 17:30:11 2020

1,1,2,2-Tetrachloroethane

Response Ratio

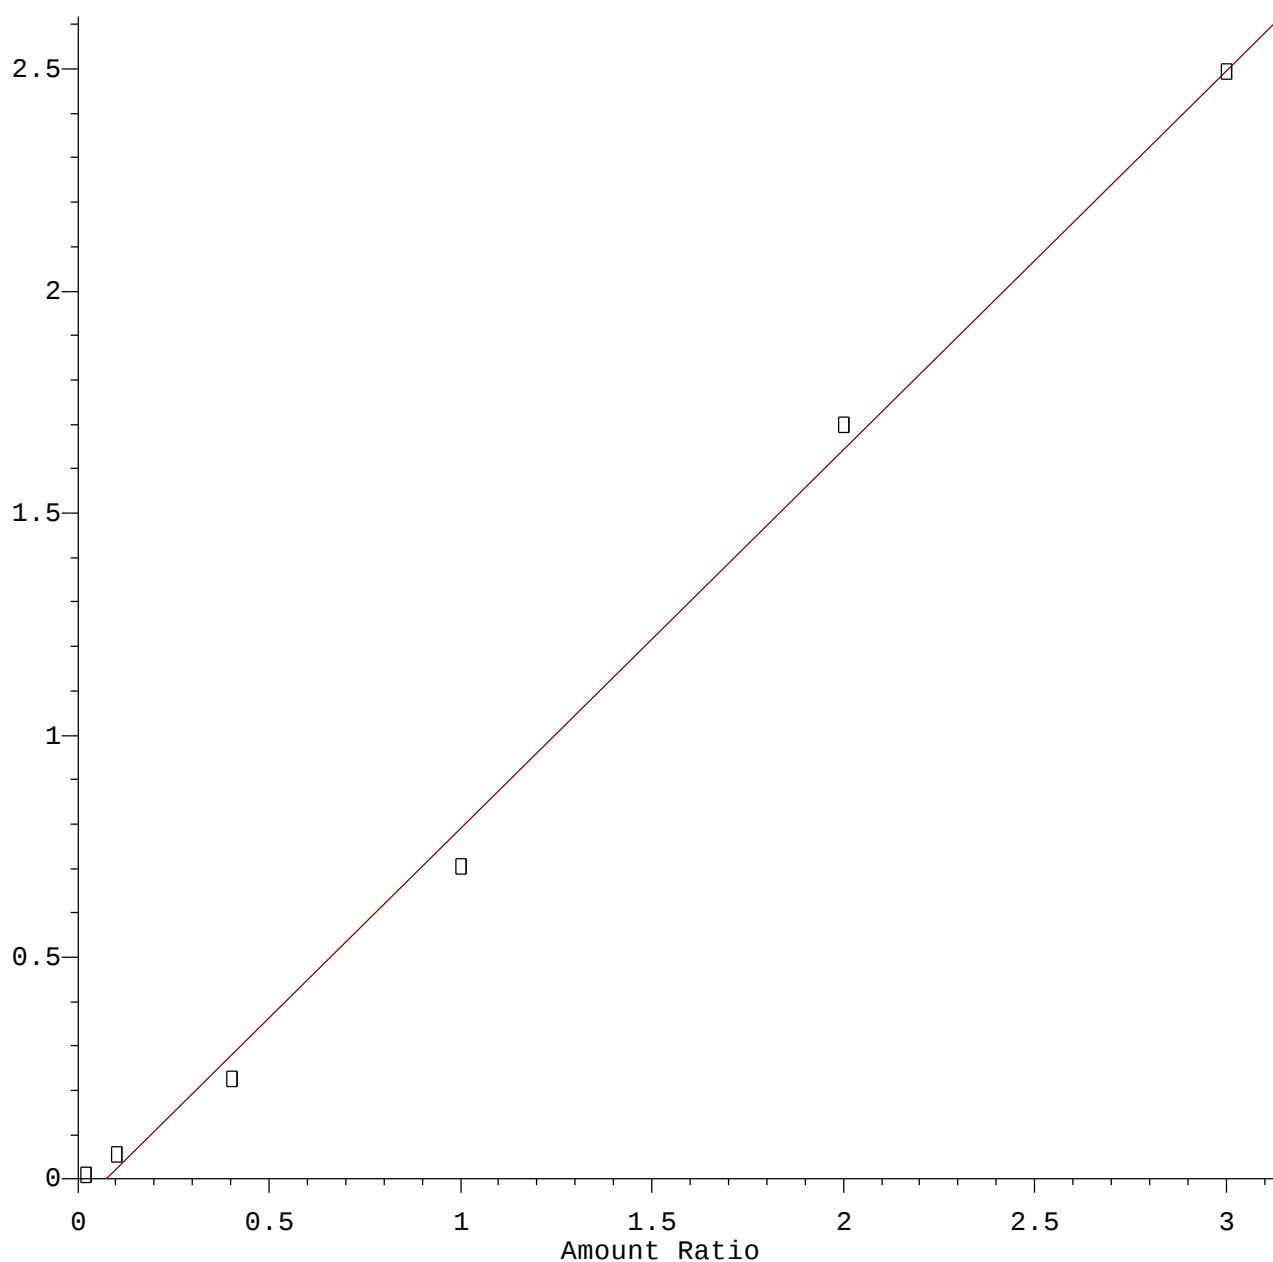

Resp Ratio = $8.53 \times 10^{-1} \times \text{Amt} - 6.31 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Calibration Table Last Updated: Tue Apr 28 17:30:11 2020