


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042820\  
 Data File : VX015960.D  
 Acq On : 28 Apr 2020 14:32  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X042820W.M  
 Title : SW846 8260  
 Last Update : Tue Apr 28 17:30:11 2020

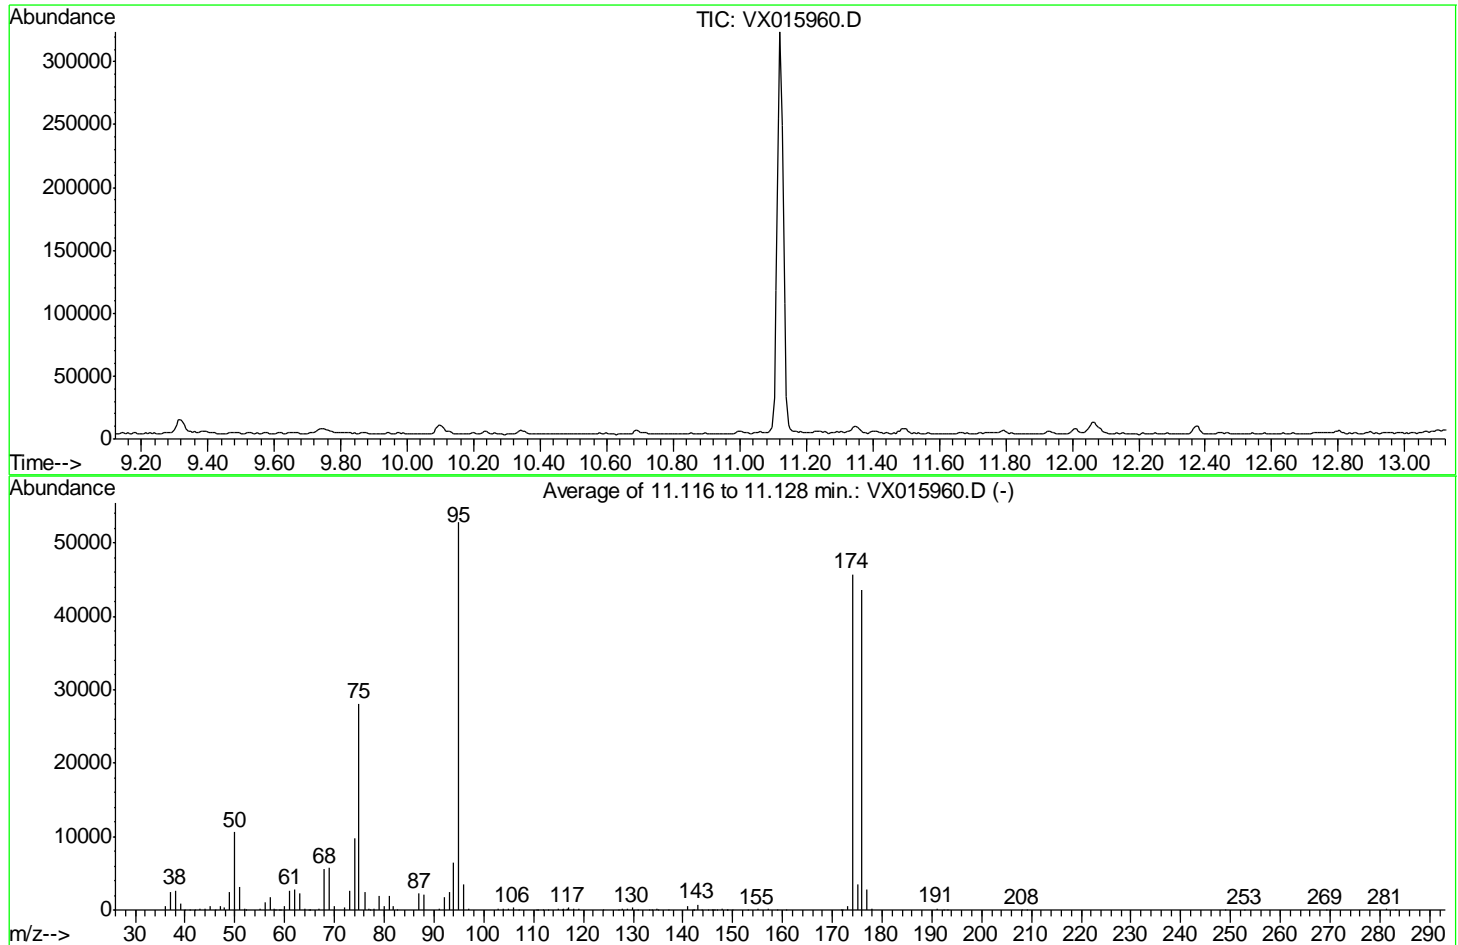

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	10601	PASS
75	95	30	60	53.3	28121	PASS
95	95	100	100	100.0	52786	PASS
96	95	5	9	6.7	3526	PASS
173	174	0.00	2	1.2	528	PASS
174	95	50	100	86.6	45717	PASS
175	174	5	9	7.6	3482	PASS
176	174	95	101	95.2	43512	PASS
177	176	5	9	6.3	2753	PASS