
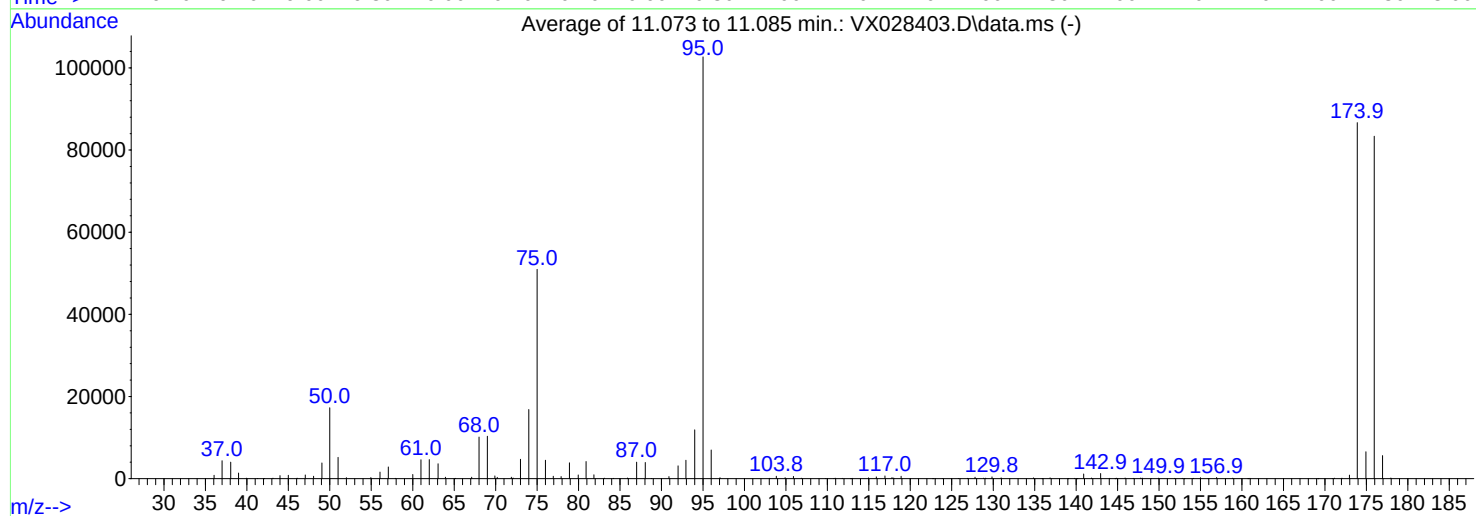


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042822\
 Data File : VX028403.D
 Acq On : 28 Apr 2022 16:17
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X042822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 29 06:09:36 2022

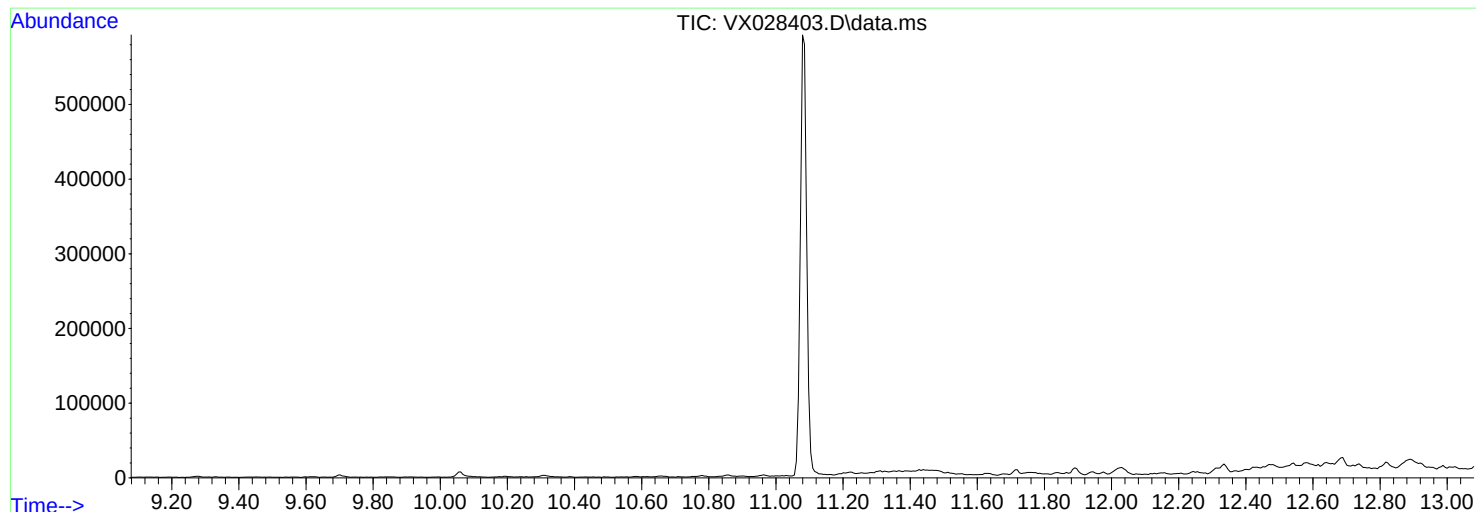

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	17269	PASS
75	95	30	60	49.6	50949	PASS
95	95	100	100	100.0	102693	PASS
96	95	5	9	6.8	6977	PASS
173	174	0.00	2	1.0	873	PASS
174	95	50	100	84.4	86677	PASS
175	174	5	9	7.5	6531	PASS
176	174	95	101	96.2	83379	PASS
177	176	5	9	6.7	5626	PASS