

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
 Data File : VX035404.D
 Acq On : 28 Apr 2023 20:21
 Operator : JC/MD
 Sample : 02495-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PZ-02

Quant Time: Apr 29 00:44:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	238419	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	394894	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	363087	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	173207	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	142132	49.413	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.820%
35) Dibromofluoromethane	5.391	113	120877	49.872	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.740%
50) Toluene-d8	8.647	98	463850	50.732	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.460%
62) 4-Bromofluorobenzene	11.079	95	177388	51.574	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	103.140%
Target Compounds						
					Qvalue	
16) Acetone	2.392	43	6912	5.533	ug/l #	84
22) Diisopropyl ether	3.757	45	1659	0.206	ug/l #	61
68) m/p-Xylenes	10.305	106	1333	0.256	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035404.D
Acq On : 28 Apr 2023 20:21
Operator : JC/MD
Sample : 02495-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PZ-02

Quant Time: Apr 29 00:44:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration




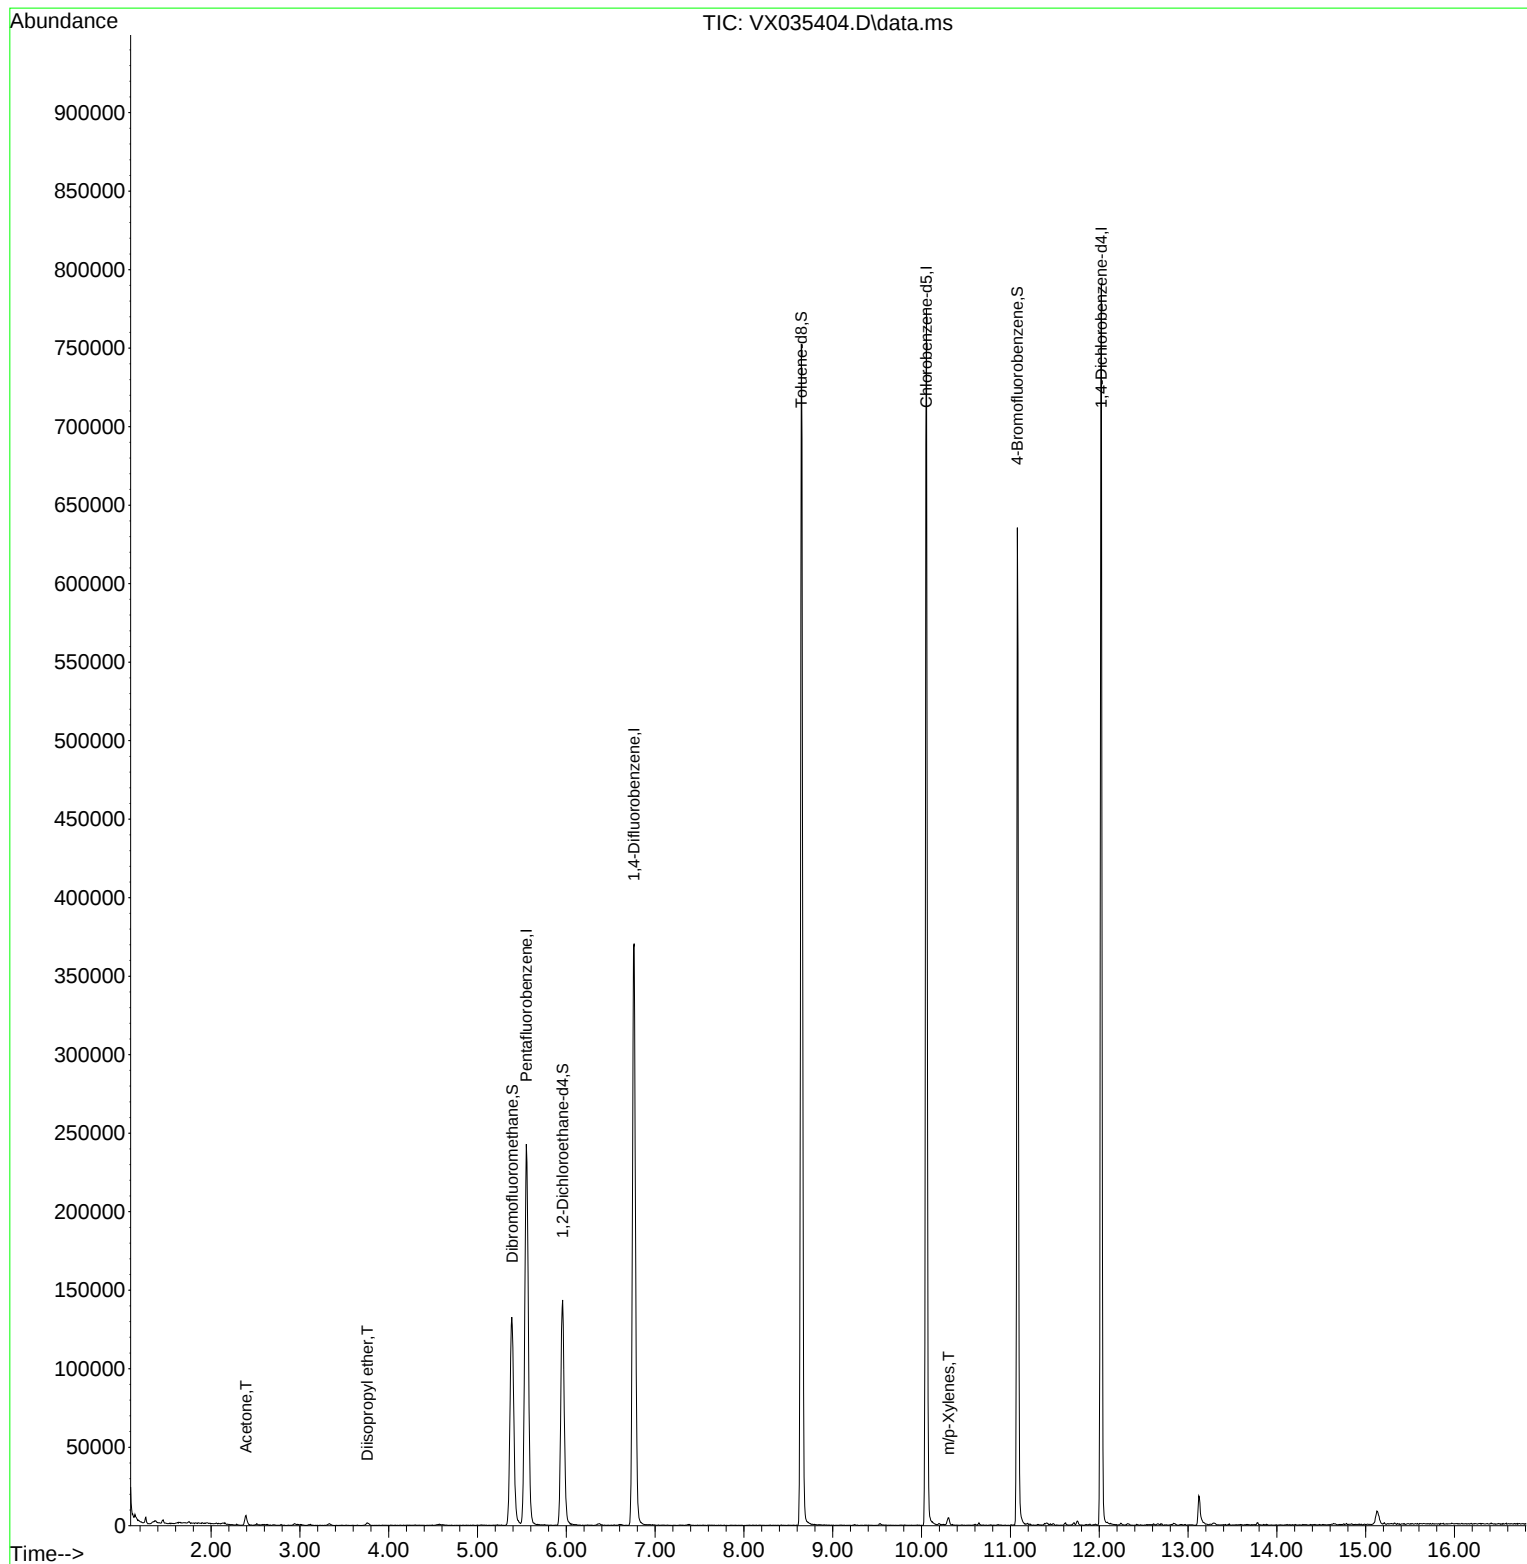


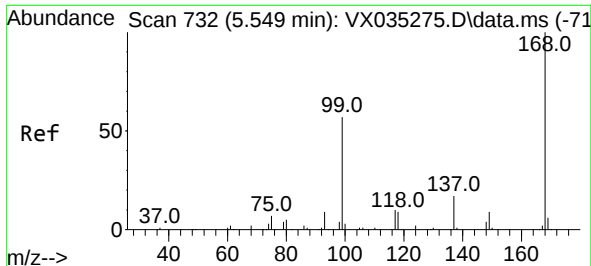

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21




Instrument :
MSVOA_X
ClientSampleId :
PZ-02


Tgt Ion:168 Resp: 238419
Ion Ratio Lower Upper
168 100
99 57.2 45.7 68.5

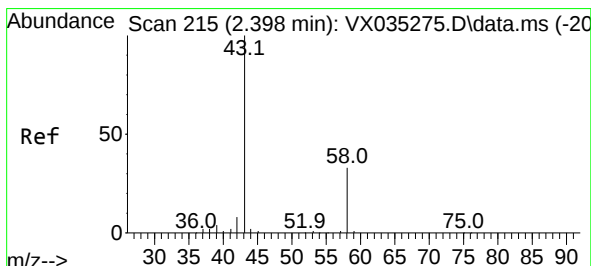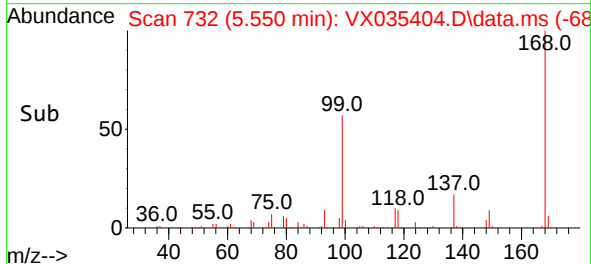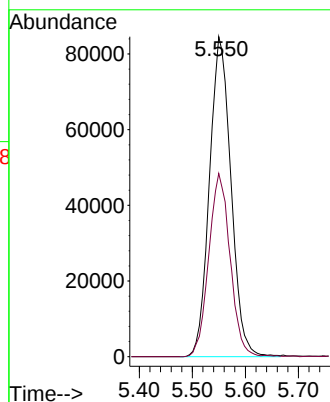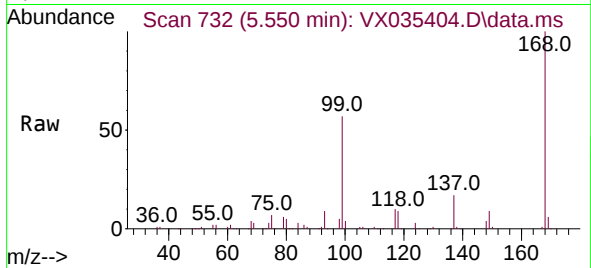

#16
Acetone
Concen: 5.533 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.006 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21

Tgt Ion: 43 Resp: 6912
Ion Ratio Lower Upper
43 100
58 39.5 24.7 37.1#


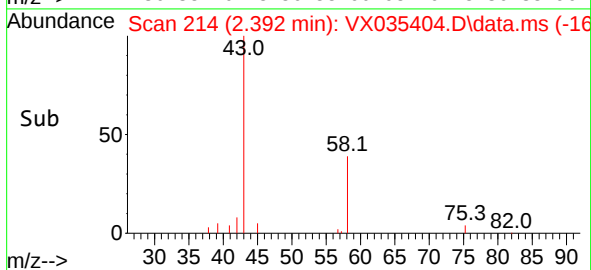
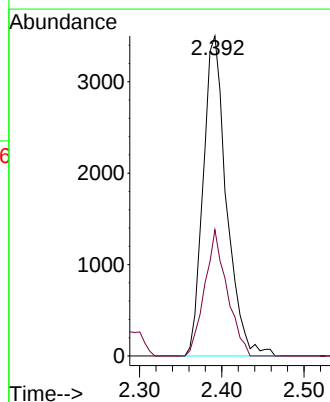
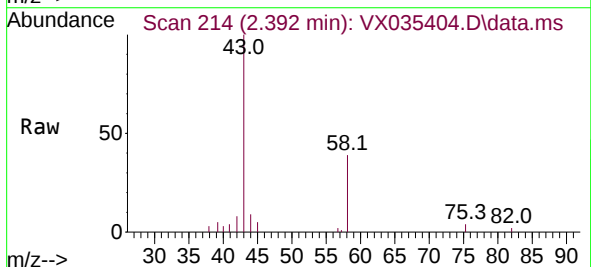


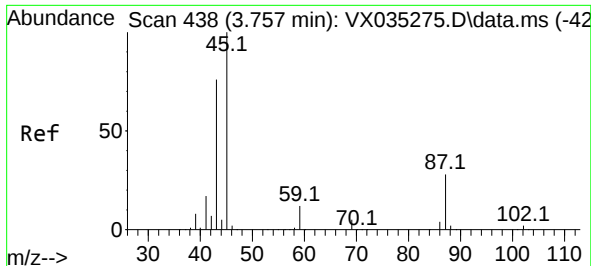

#22
Diisopropyl ether
Concen: 0.206 ug/l
RT: 3.757 min Scan# 41
Delta R.T. 0.000 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21




Instrument :
MSVOA_X
ClientSampleId :
PZ-02


Tgt Ion: 45 Resp: 1659
Ion Ratio Lower Upper
45 100
43 38.7 65.4 98.2#
87 30.4 20.6 31.0
59 27.2 9.0 13.6#

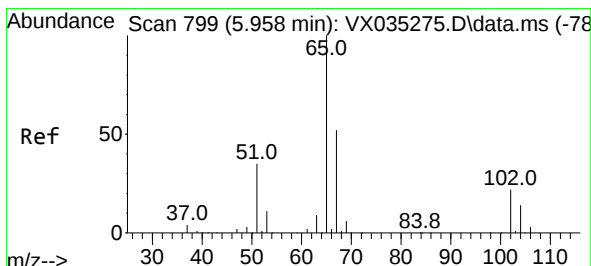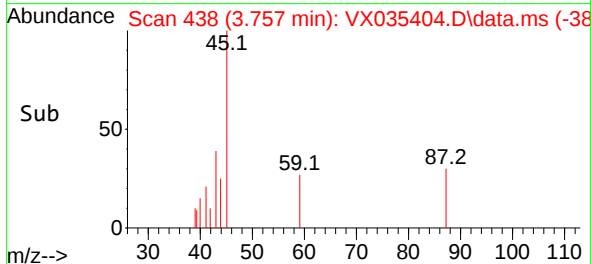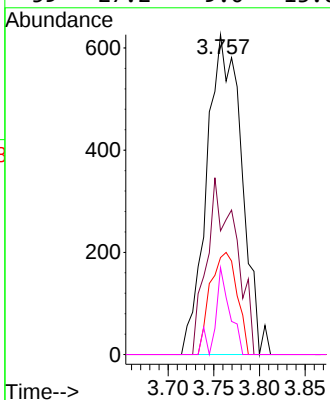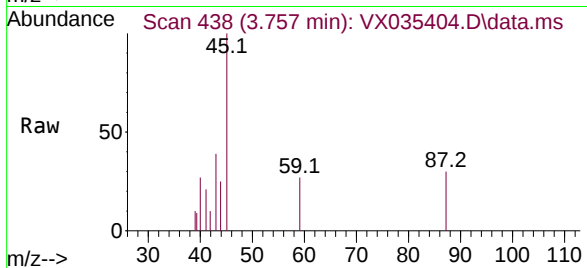

#33
1,2-Dichloroethane-d4
Concen: 49.413 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21

Tgt Ion: 65 Resp: 142132
Ion Ratio Lower Upper
65 100
67 51.7 0.0 104.0


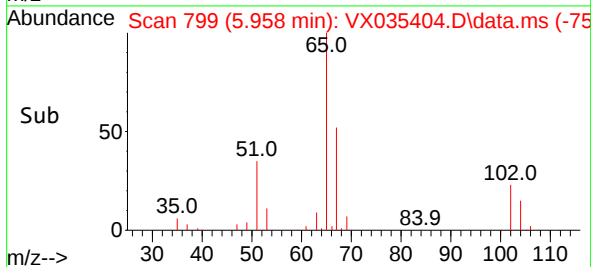
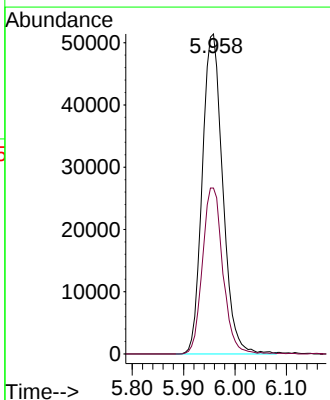
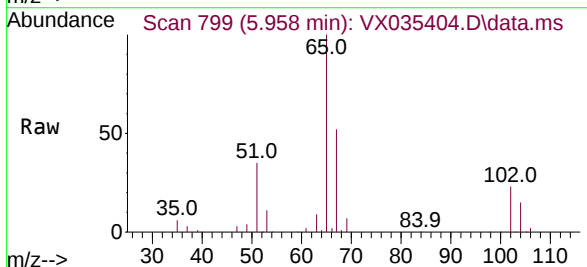


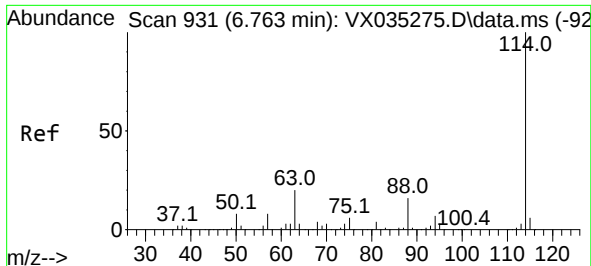

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.763 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: VX035404.D
 Acq: 28 Apr 2023 20:21




Instrument :
 MSVOA_X
 ClientSampleId :
 PZ-02


Tgt Ion:114 Resp: 394894
 Ion Ratio Lower Upper
 114 100
 63 19.6 0.0 42.2
 88 16.1 0.0 33.2

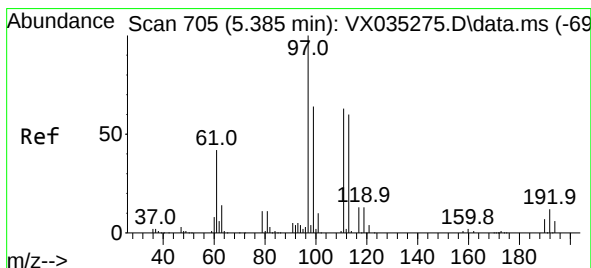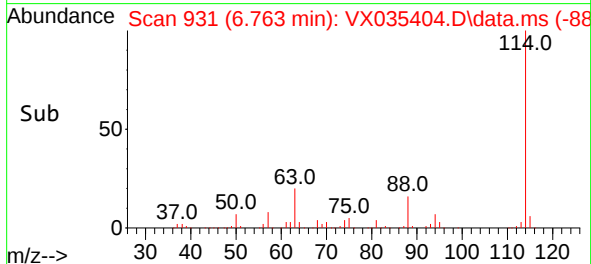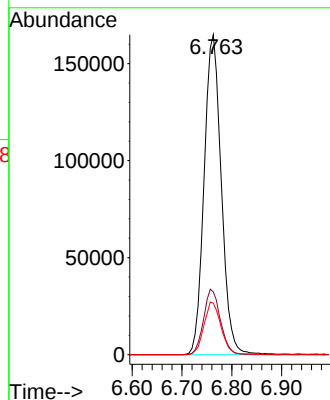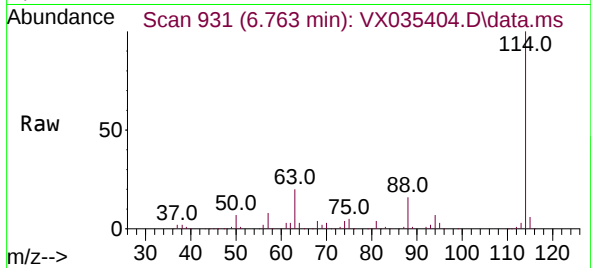

#35
 Dibromofluoromethane
 Concen: 49.872 ug/l
 RT: 5.391 min Scan# 706
 Delta R.T. 0.006 min
 Lab File: VX035404.D
 Acq: 28 Apr 2023 20:21

Tgt Ion:113 Resp: 120877
 Ion Ratio Lower Upper
 113 100
 111 101.3 83.7 125.5
 192 20.4 15.4 23.2


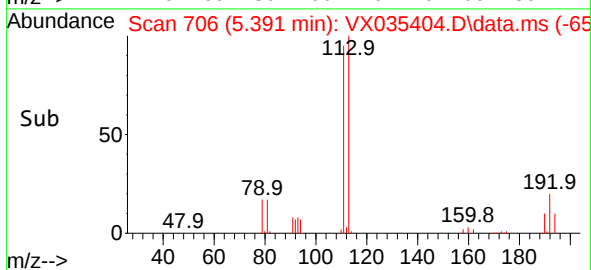
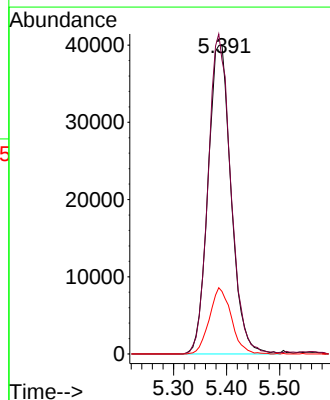
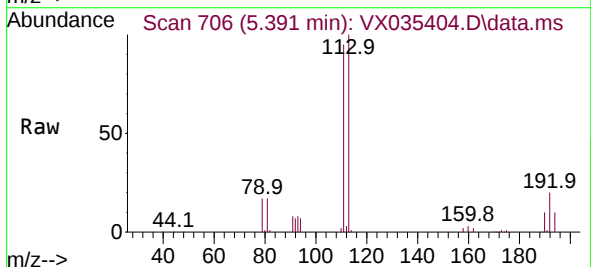


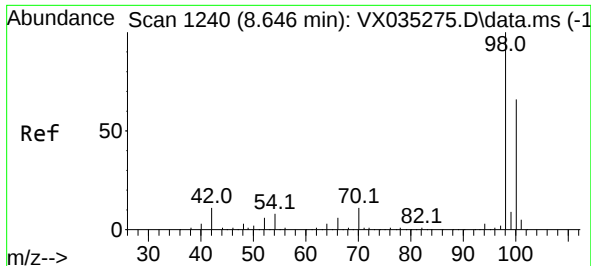

#50
Toluene-d8
Concen: 50.732 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.001 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21




Instrument :
MSVOA_X
ClientSampleId :
PZ-02


Tgt Ion: 98 Resp: 463850
Ion Ratio Lower Upper
98 100
100 66.7 52.5 78.7

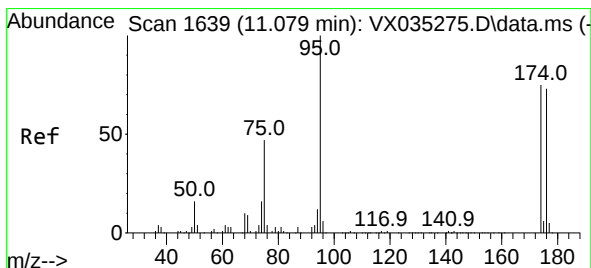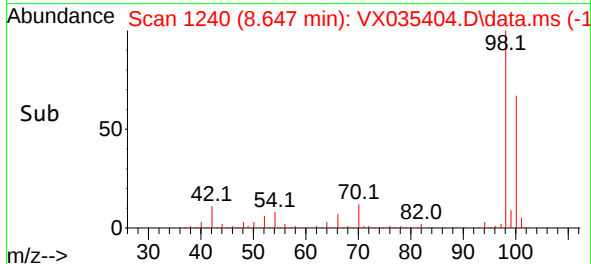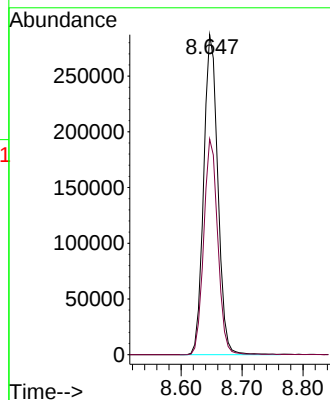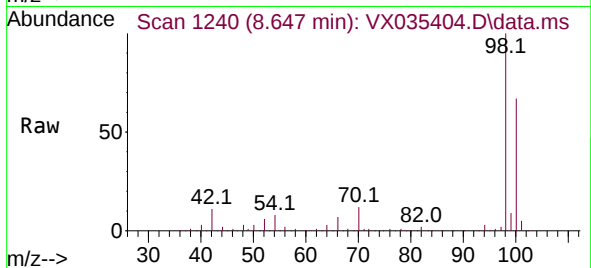

#62
4-Bromofluorobenzene
Concen: 51.574 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21

Tgt Ion: 95 Resp: 177388
Ion Ratio Lower Upper
95 100
174 78.1 0.0 147.4
176 77.2 0.0 140.6


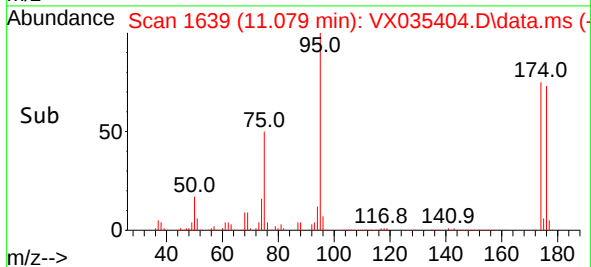
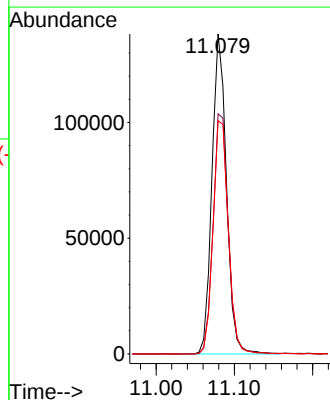
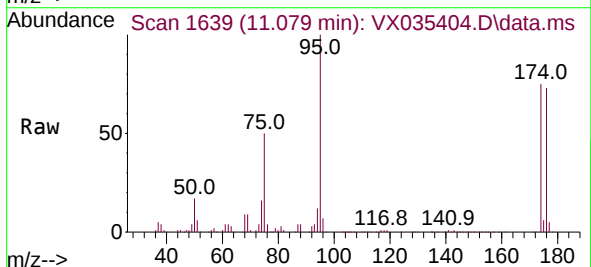


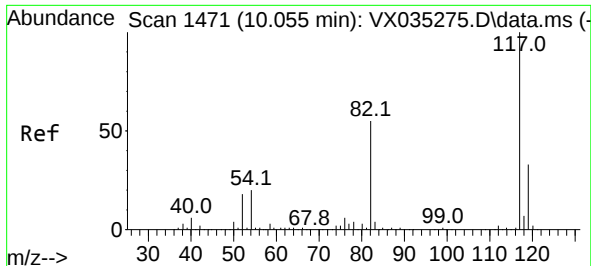

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21




Instrument :
MSVOA_X
ClientSampleId :
PZ-02


Tgt Ion:117 Resp: 363087
Ion Ratio Lower Upper
117 100
82 55.1 45.0 67.4
119 33.0 26.0 39.0

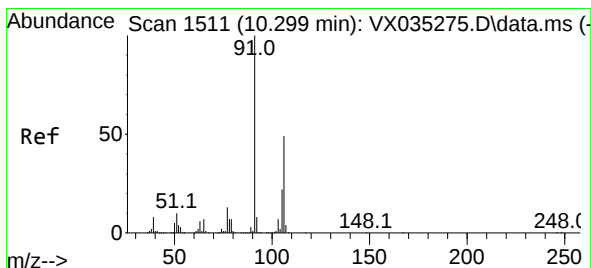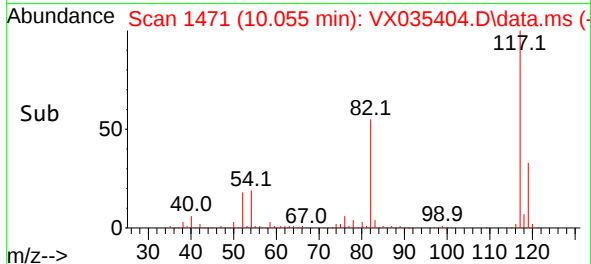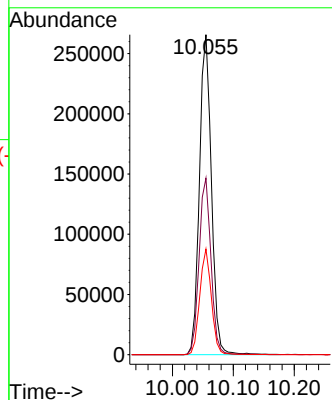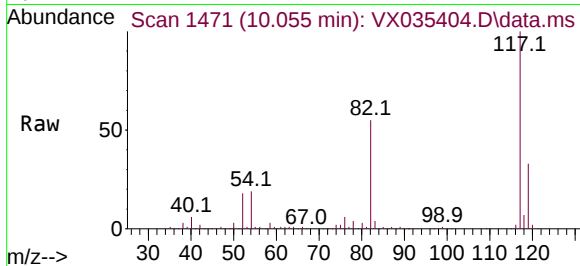

#68
m/p-Xylenes
Concen: 0.256 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. 0.006 min
Lab File: VX035404.D
Acq: 28 Apr 2023 20:21

Tgt Ion:106 Resp: 1333
Ion Ratio Lower Upper
106 100
91 187.6 164.0 246.0

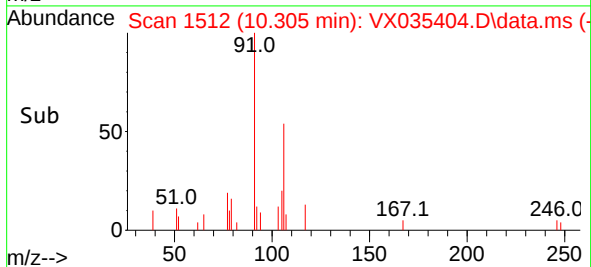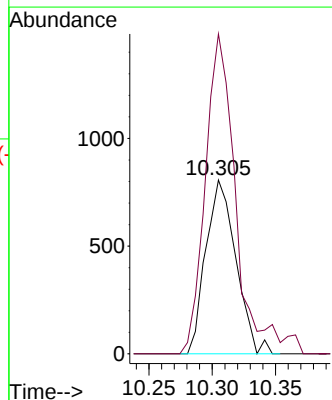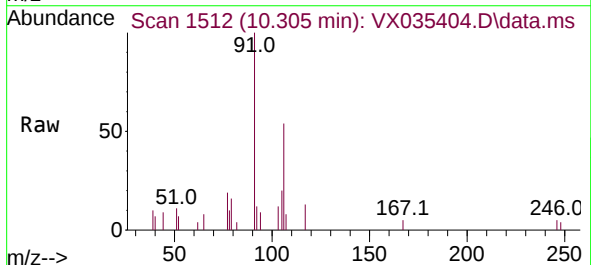

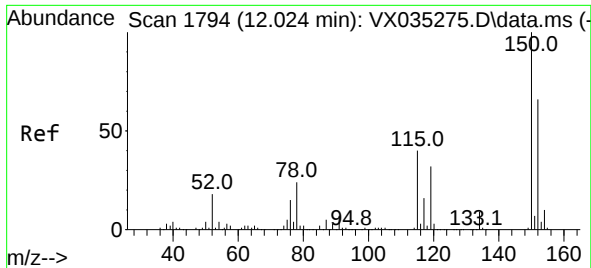

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX035404.D


Acq: 28 Apr 2023 20:21

Instrument :

MSVOA_X

ClientSampleId :

PZ-02

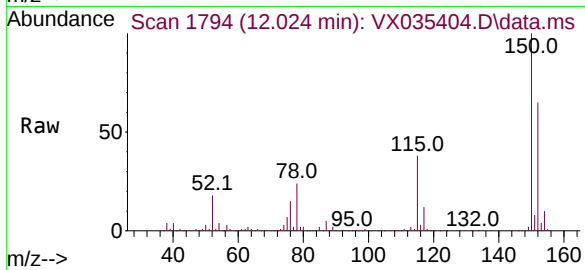

Tgt Ion:152 Resp: 173207

Ion Ratio Lower Upper

152 100

115 60.2 45.0 135.0

150 156.1 0.0 352.4

