

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
 Data File : VX035398.D
 Acq On : 28 Apr 2023 18:02
 Operator : JC/MD
 Sample : 02473-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M

Title : SW846 8260

Signal : TIC: VX035398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	721	rBV	135562	393184	32.15%	5.385%
2	5.550	721	732	754	rVB	246973	702016	57.41%	9.614%
3	5.958	789	799	817	rBV2	146226	394583	32.27%	5.404%
4	6.763	921	931	948	rBV	375612	904764	73.99%	12.391%
5	8.647	1234	1240	1256	rBV	776924	1222868	100.00%	16.747%
6	10.055	1465	1471	1489	rBV	765505	1059801	86.67%	14.514%
7	11.079	1634	1639	1650	rBV	639649	827223	67.65%	11.329%
8	12.024	1788	1794	1804	rBV	769029	990765	81.02%	13.569%
9	14.633	2215	2222	2227	rBV10	5257	12946	1.06%	0.177%
10	15.133	2289	2304	2322	rBV2	267197	793751	64.91%	10.870%




Sum of corrected areas: 7301901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035398.D
Acq On : 28 Apr 2023 18:02
Operator : JC/MD
Sample : 02473-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

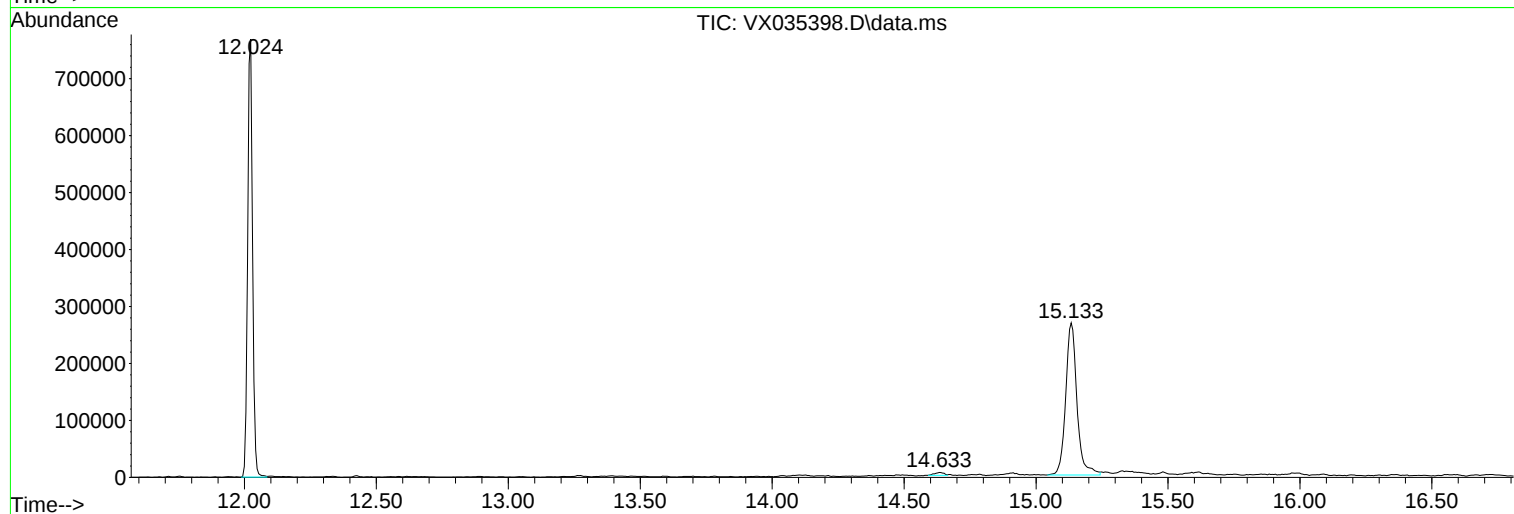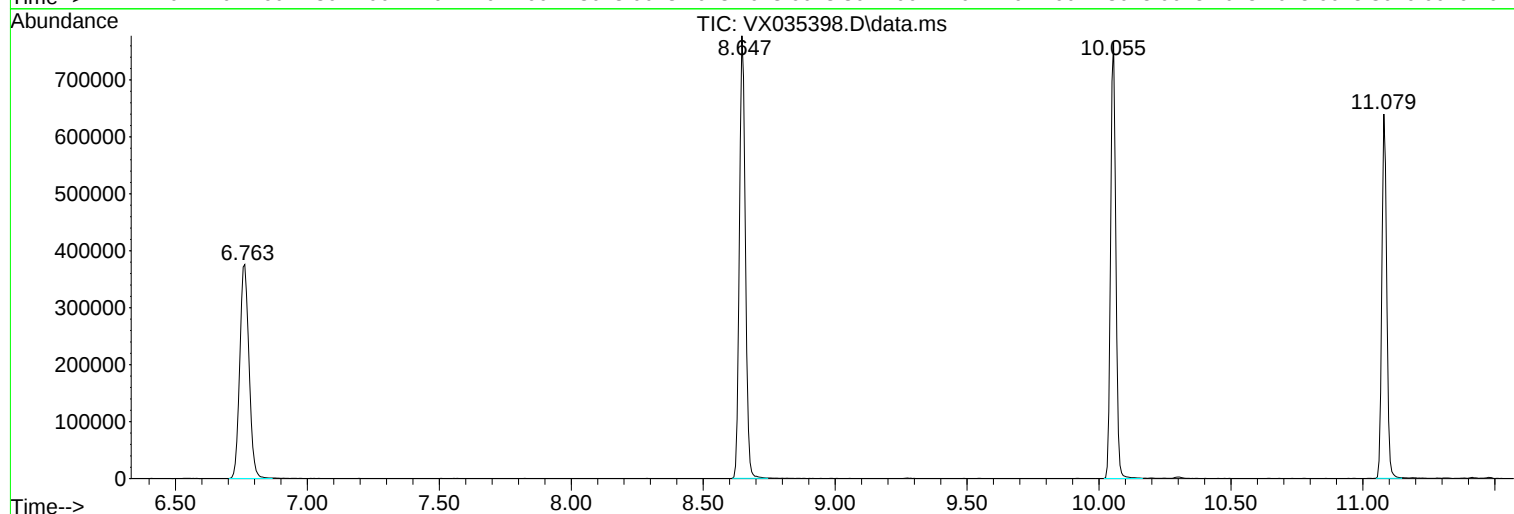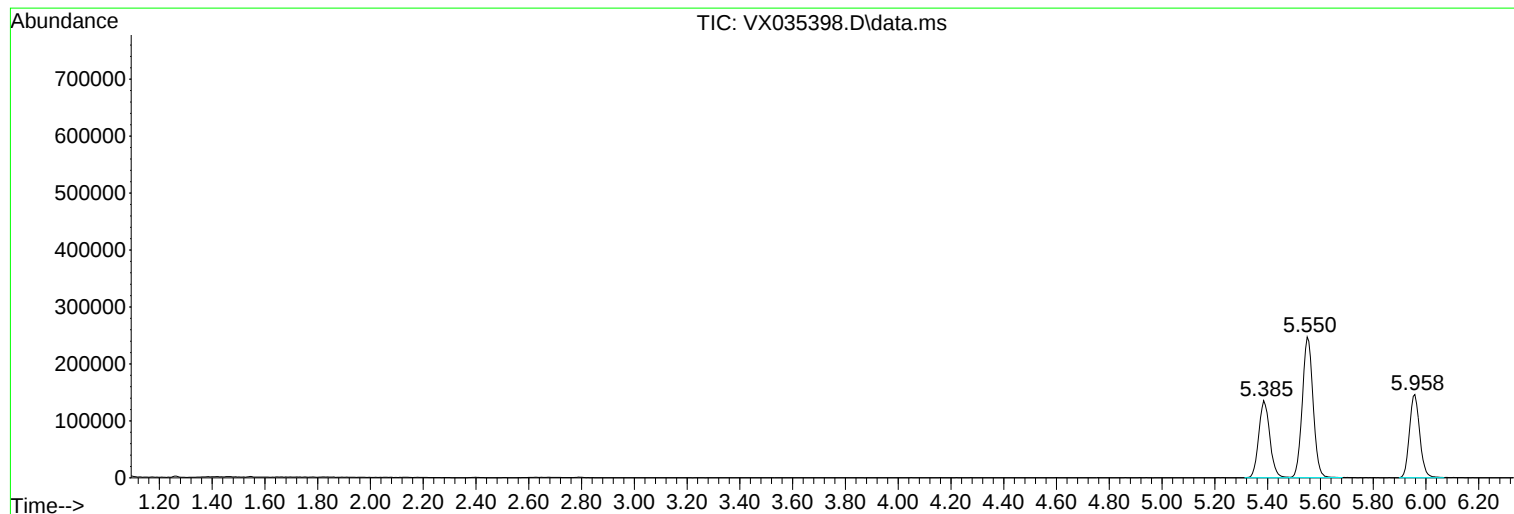

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035398.D
Acq On : 28 Apr 2023 18:02
Operator : JC/MD
Sample : 02473-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1H-Indene, 2,3-dihydro-1,1,... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.133	40.06 ug/l	793751	1,4-Dichlorobenzene-d4	12.024

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1H-Indene, 2,3-dihydro-1,1,3-tri...	236	C18H20	003910-35-8	98
2			2-Pentene, 4-methyl-2,4-diphenyl-	236	C18H20	006258-73-7	96
3			1-Methyl-4-phenyl-3,4-dihydroiso...	221	C16H15N	1000211-01-5	47
4			(Dimethylphenylsilyl)phenylacety...	236	C16H16Si	1000434-31-1	43
5			Benzo[h]quinoline, 2,3,4-trimethyl-	221	C16H15N	063042-66-0	43

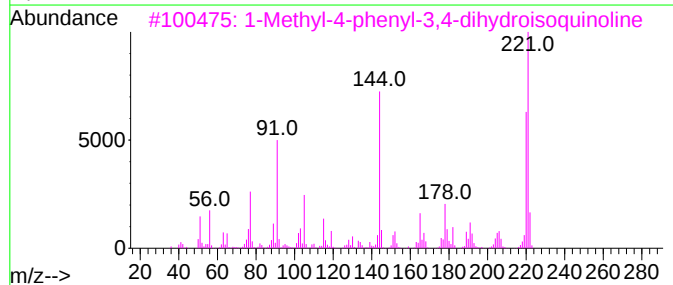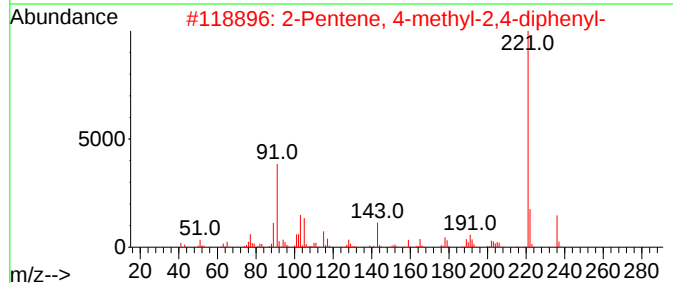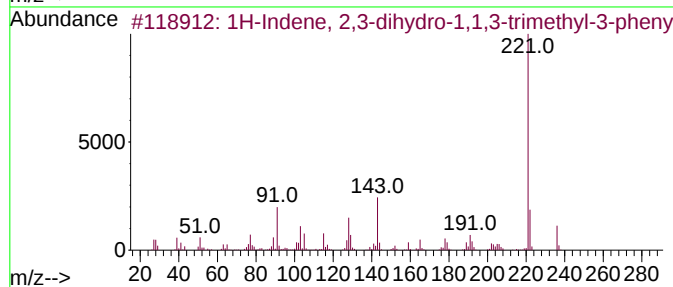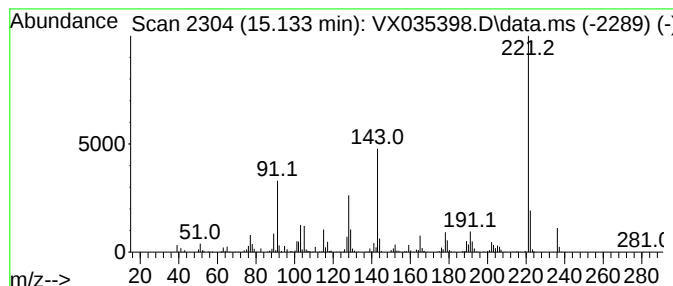

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035398.D
Acq On : 28 Apr 2023 18:02
Operator : JC/MD
Sample : 02473-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1H-Indene, 2,3-...	15.133	40.1	ug/l	793751	4	12.024	990765	50.0