

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
 Data File : VX035401.D
 Acq On : 28 Apr 2023 19:12
 Operator : JC/MD
 Sample : 02522-06DL 10X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

Signal : TIC: VX035401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.385	693	705	722	rBV2	139999	416672	27.08%	2.841%
2	5.550	722	732	753	rVB	252629	721583	46.90%	4.921%
3	5.958	788	799	809	rBV	149133	403128	26.20%	2.749%
4	6.044	809	813	826	rVB4	8398	20493	1.33%	0.140%
5	6.763	918	931	955	rBV	382875	937981	60.96%	6.396%
6	7.379	1022	1032	1044	rVB4	7267	18308	1.19%	0.125%
7	8.647	1234	1240	1247	rBV	788707	1257114	81.70%	8.572%
8	8.720	1247	1252	1265	rVB	226533	356412	23.16%	2.430%
9	10.055	1465	1471	1480	rBV	800349	1102274	71.64%	7.517%
10	10.195	1488	1494	1504	rBV	897866	1173538	76.27%	8.002%
11	10.305	1505	1512	1520	rVV	461674	636298	41.35%	4.339%
12	10.640	1562	1567	1579	rVB	216982	284329	18.48%	1.939%
13	10.963	1615	1620	1626	rBV	50604	63249	4.11%	0.431%
14	11.079	1634	1639	1652	rBV	691061	879404	57.15%	5.997%
15	11.305	1671	1676	1683	rBV	94122	115973	7.54%	0.791%
16	11.402	1683	1692	1696	rVV	83756	146279	9.51%	0.997%
17	11.451	1696	1700	1708	rVB	221263	270348	17.57%	1.844%
18	11.610	1720	1726	1734	rBV	254306	326373	21.21%	2.226%
19	11.750	1744	1749	1756	rBV	1286539	1538644	100.00%	10.492%
20	12.018	1788	1793	1800	rBV	846700	1084730	70.50%	7.397%
21	12.085	1800	1804	1811	rVB	423183	511783	33.26%	3.490%
22	12.244	1824	1830	1837	rBV	437147	549570	35.72%	3.748%
23	12.317	1837	1842	1852	rVB2	51476	77761	5.05%	0.530%
24	12.414	1852	1858	1862	rBV2	38259	52538	3.41%	0.358%
25	12.463	1862	1866	1872	rVB	26166	33633	2.19%	0.229%
26	12.530	1872	1877	1879	rBV	57340	71795	4.67%	0.490%
27	12.555	1879	1881	1886	rVV	45263	50339	3.27%	0.343%
28	12.616	1886	1891	1894	rVV	80086	104754	6.81%	0.714%
29	12.646	1894	1896	1900	rVV	23572	24767	1.61%	0.169%
30	12.701	1900	1905	1913	rVB2	88197	127407	8.28%	0.869%
31	12.847	1925	1929	1934	rVB2	28962	36719	2.39%	0.250%
32	12.920	1934	1941	1944	rBV	69765	83132	5.40%	0.567%
33	12.963	1944	1948	1954	rVB	75162	93222	6.06%	0.636%
34	13.170	1978	1982	1987	rVB	59888	71081	4.62%	0.485%
35	13.292	1997	2002	2007	rVB2	138780	183160	11.90%	1.249%
36	13.420	2019	2023	2030	rVB	21270	30384	1.97%	0.207%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035401.D
Acq On : 28 Apr 2023 19:12
Operator : JC/MD
Sample : 02522-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M

Title : SW846 8260

37	13.542	2039	2043	2046	rBV2	13863	17538	1.14%	0.120%
38	13.579	2046	2049	2055	rVB3	15717	24945	1.62%	0.170%
39	13.664	2060	2063	2068	rVB2	13801	21183	1.38%	0.144%
40	13.774	2075	2081	2087	rBV	426351	522484	33.96%	3.563%
41	13.871	2092	2097	2101	rVB	22380	32342	2.10%	0.221%
42	14.640	2218	2223	2230	rVB	57024	77755	5.05%	0.530%
43	14.780	2241	2246	2253	rVB	39266	50033	3.25%	0.341%
44	15.133	2294	2304	2313	rBV3	22691	63207	4.11%	0.431%




Sum of corrected areas: 14664662

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035401.D
Acq On : 28 Apr 2023 19:12
Operator : JC/MD
Sample : 02522-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

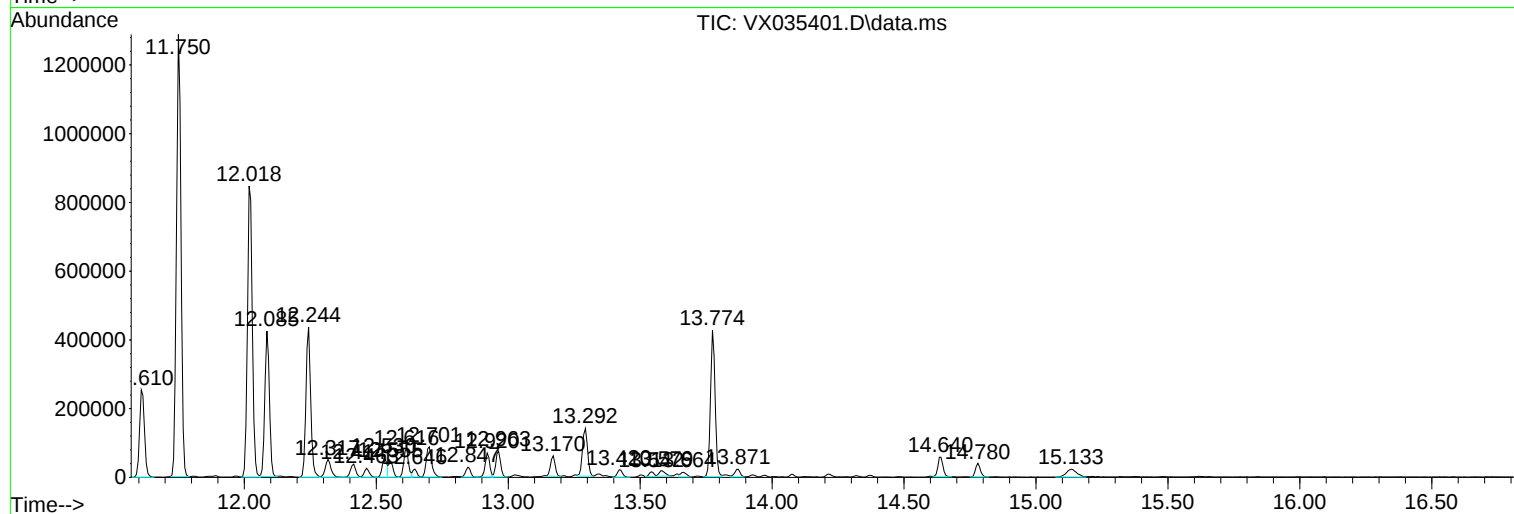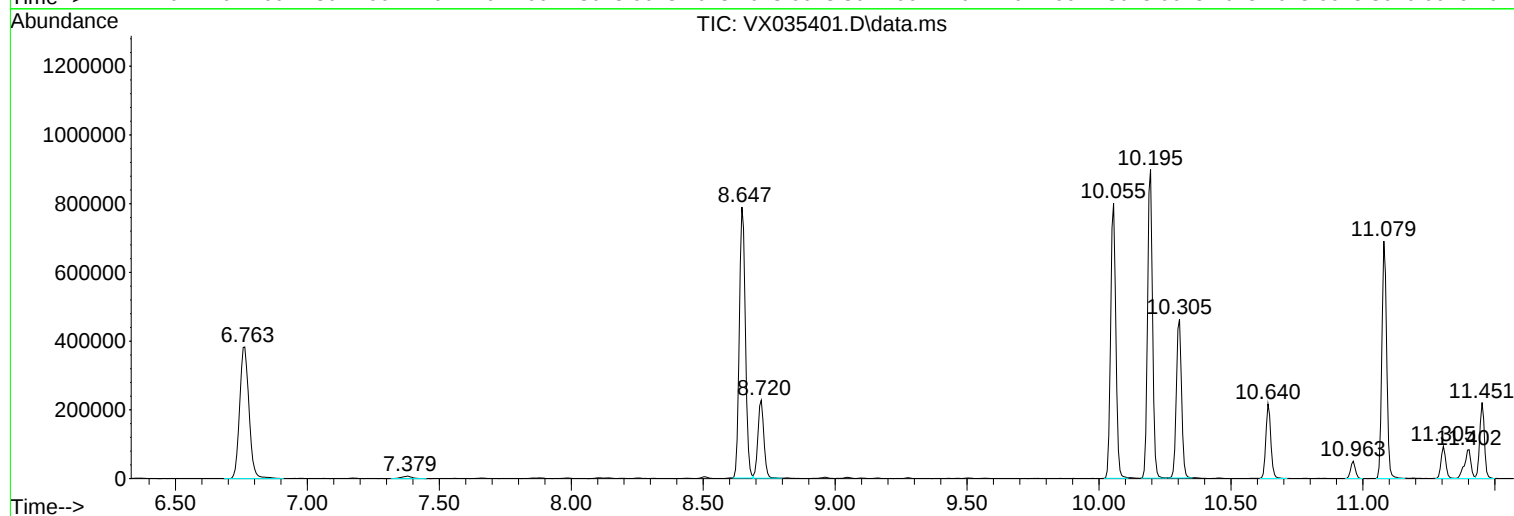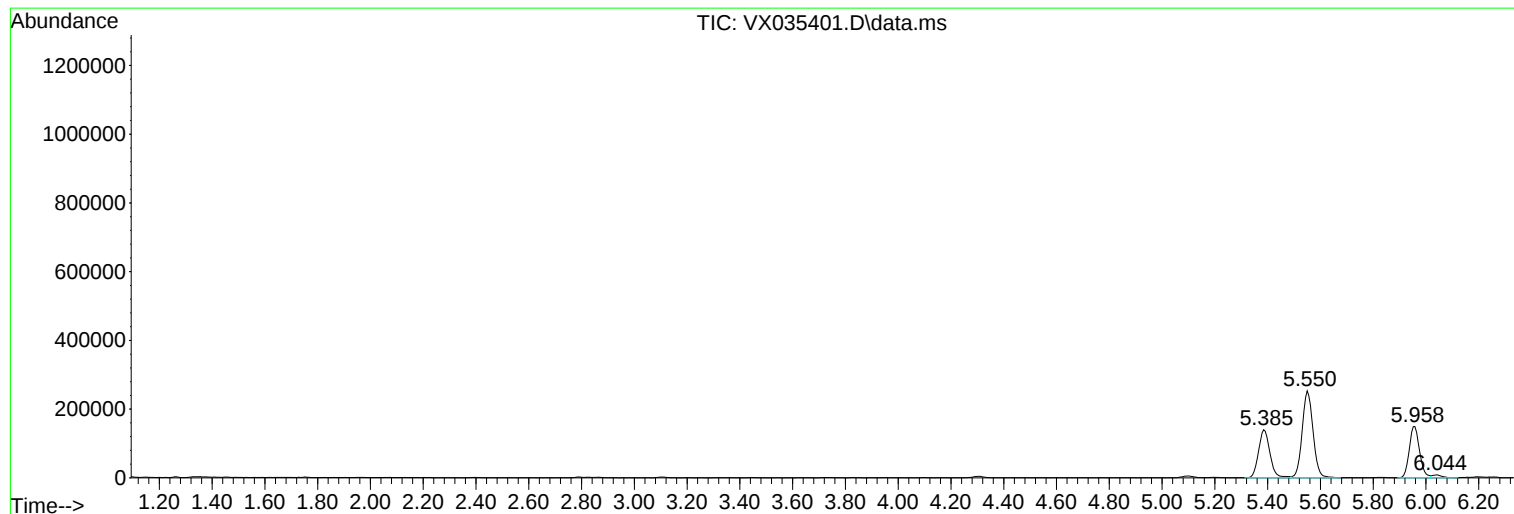

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035401.D
Acq On : 28 Apr 2023 19:12
Operator : JC/MD
Sample : 02522-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035401.D
Acq On : 28 Apr 2023 19:12
Operator : JC/MD
Sample : 02522-06DL 10X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc