
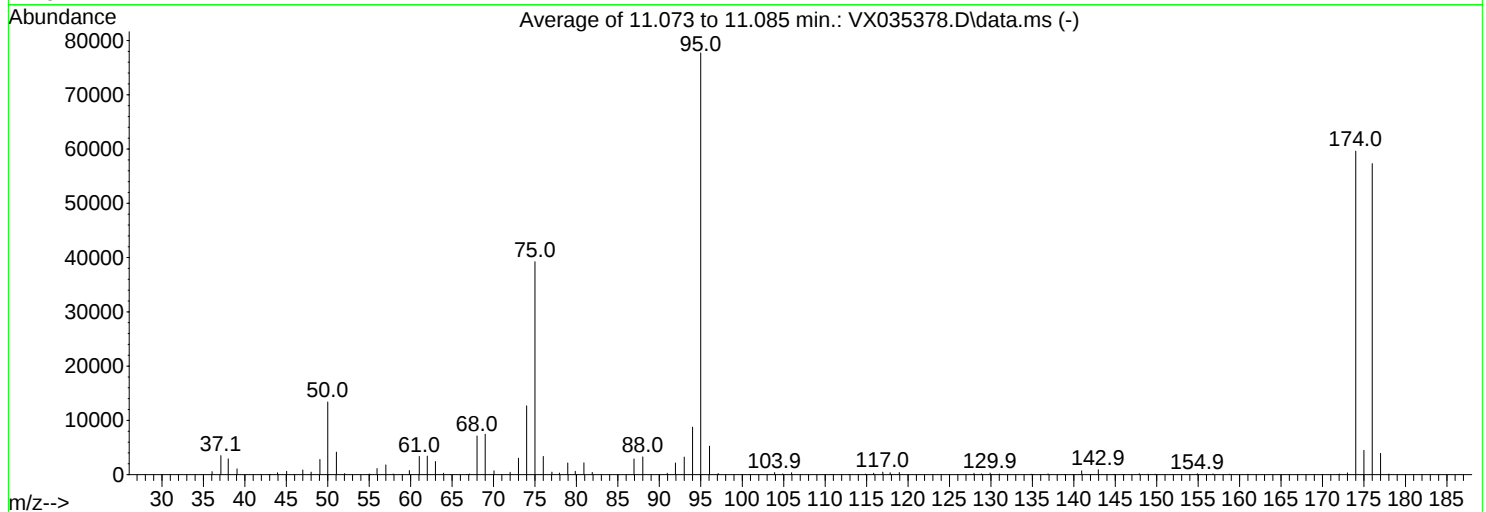


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042823\  
Data File : VX035378.D  
Acq On : 28 Apr 2023 10:03  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042523W.M  
Title : SW846 8260  
Last Update : Tue Apr 25 16:31:40 2023

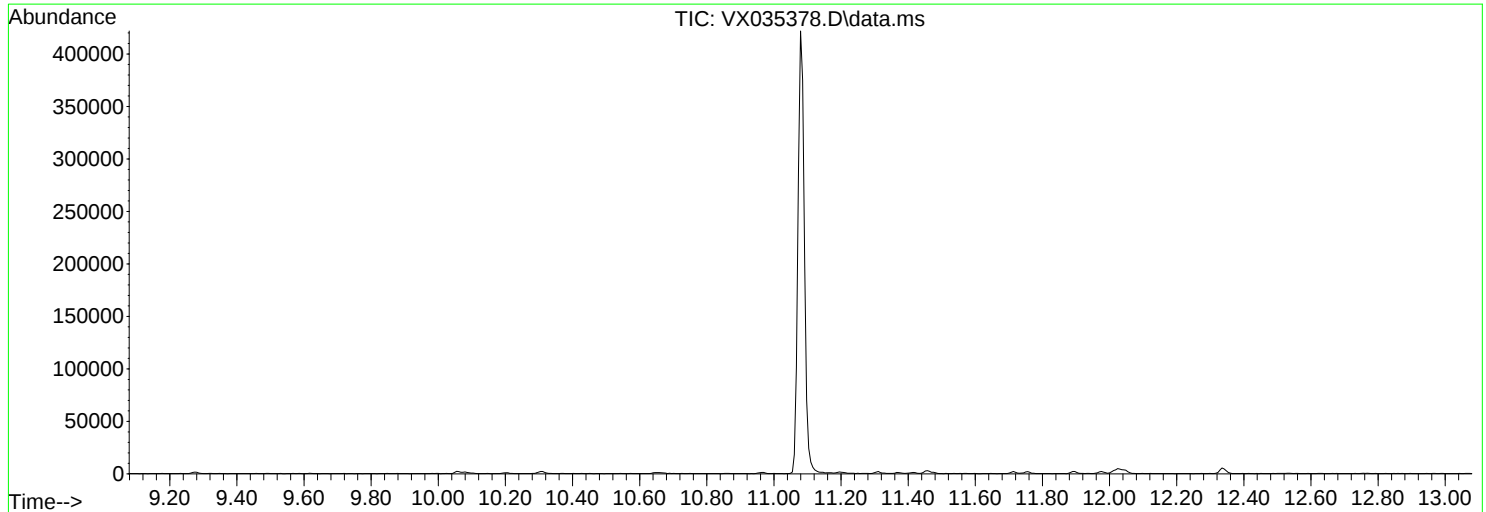

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 17.2  | 13381 | PASS      |
| 75     | 95      | 30     | 60     | 50.5  | 39243 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 77728 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 5236  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.5   | 319   | PASS      |
| 174    | 95      | 50     | 100    | 76.7  | 59632 | PASS      |
| 175    | 174     | 5      | 9      | 7.5   | 4495  | PASS      |
| 176    | 174     | 95     | 101    | 96.1  | 57317 | PASS      |
| 177    | 176     | 5      | 9      | 6.8   | 3918  | PASS      |