


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042823\
Data File : VX035408.D
Acq On : 28 Apr 2023 22:17
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Title : SW846 8260
Last Update : Tue Apr 25 16:31:40 2023

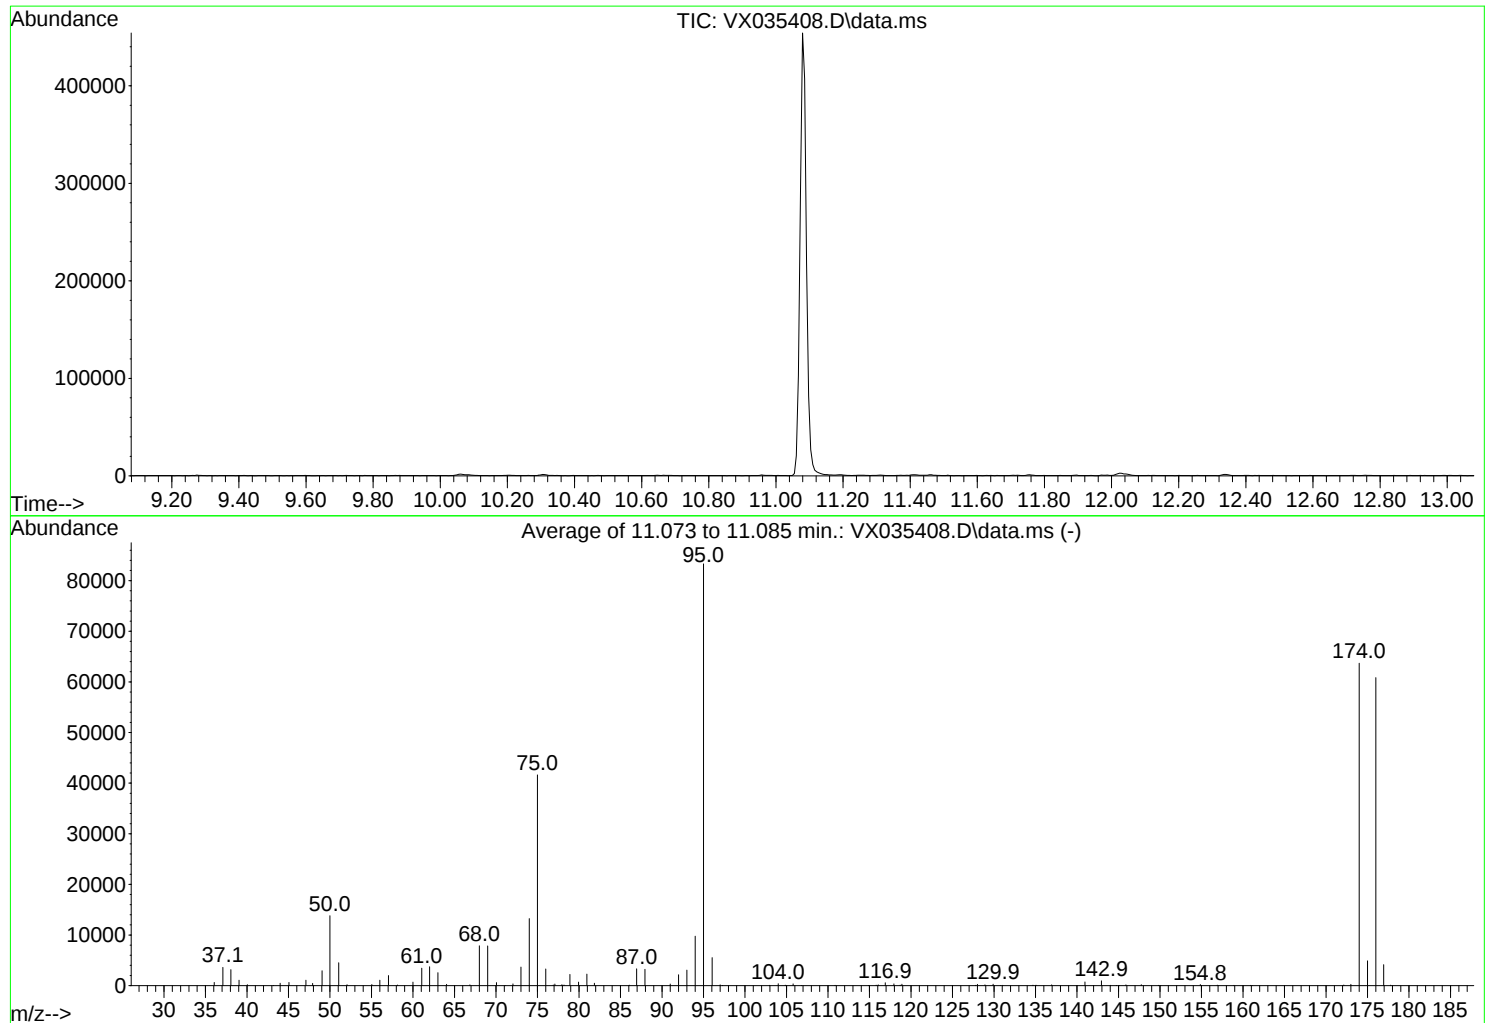

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	13808	PASS
75	95	30	60	50.0	41621	PASS
95	95	100	100	100.0	83315	PASS
96	95	5	9	6.7	5542	PASS
173	174	0.00	2	0.4	243	PASS
174	95	50	100	76.4	63683	PASS
175	174	5	9	7.7	4907	PASS
176	174	95	101	95.5	60848	PASS
177	176	5	9	6.8	4134	PASS