

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042825\
 Data File : VX045957.D
 Acq On : 28 Apr 2025 15:26
 Operator : JC/MD
 Sample : Q1891-04
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-C

Quant Time: Apr 29 01:34:45 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.544	168	63272	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	128718	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	123117	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53117	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	64415	55.670	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	111.340%
35) Dibromofluoromethane	5.379	113	46385	50.791	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.580%
50) Toluene-d8	8.647	98	162646	51.024	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.040%
62) 4-Bromofluorobenzene	11.079	95	63454	54.650	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	109.300%
Target Compounds						
					Qvalue	
16) Acetone	2.380	43	58428	122.973	ug/l	99
18) Methyl Acetate	2.709	43	2017	1.844	ug/l	95
20) Methylene Chloride	2.782	84	2657	2.987	ug/l	92
25) 2-Butanone	4.580	43	4430	6.370	ug/l #	84
43) Isopropyl Acetate	6.348	43	11517	4.890	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042825\
Data File : VX045957.D
Acq On : 28 Apr 2025 15:26
Operator : JC/MD
Sample : Q1891-04
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-C

Quant Time: Apr 29 01:34:45 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration



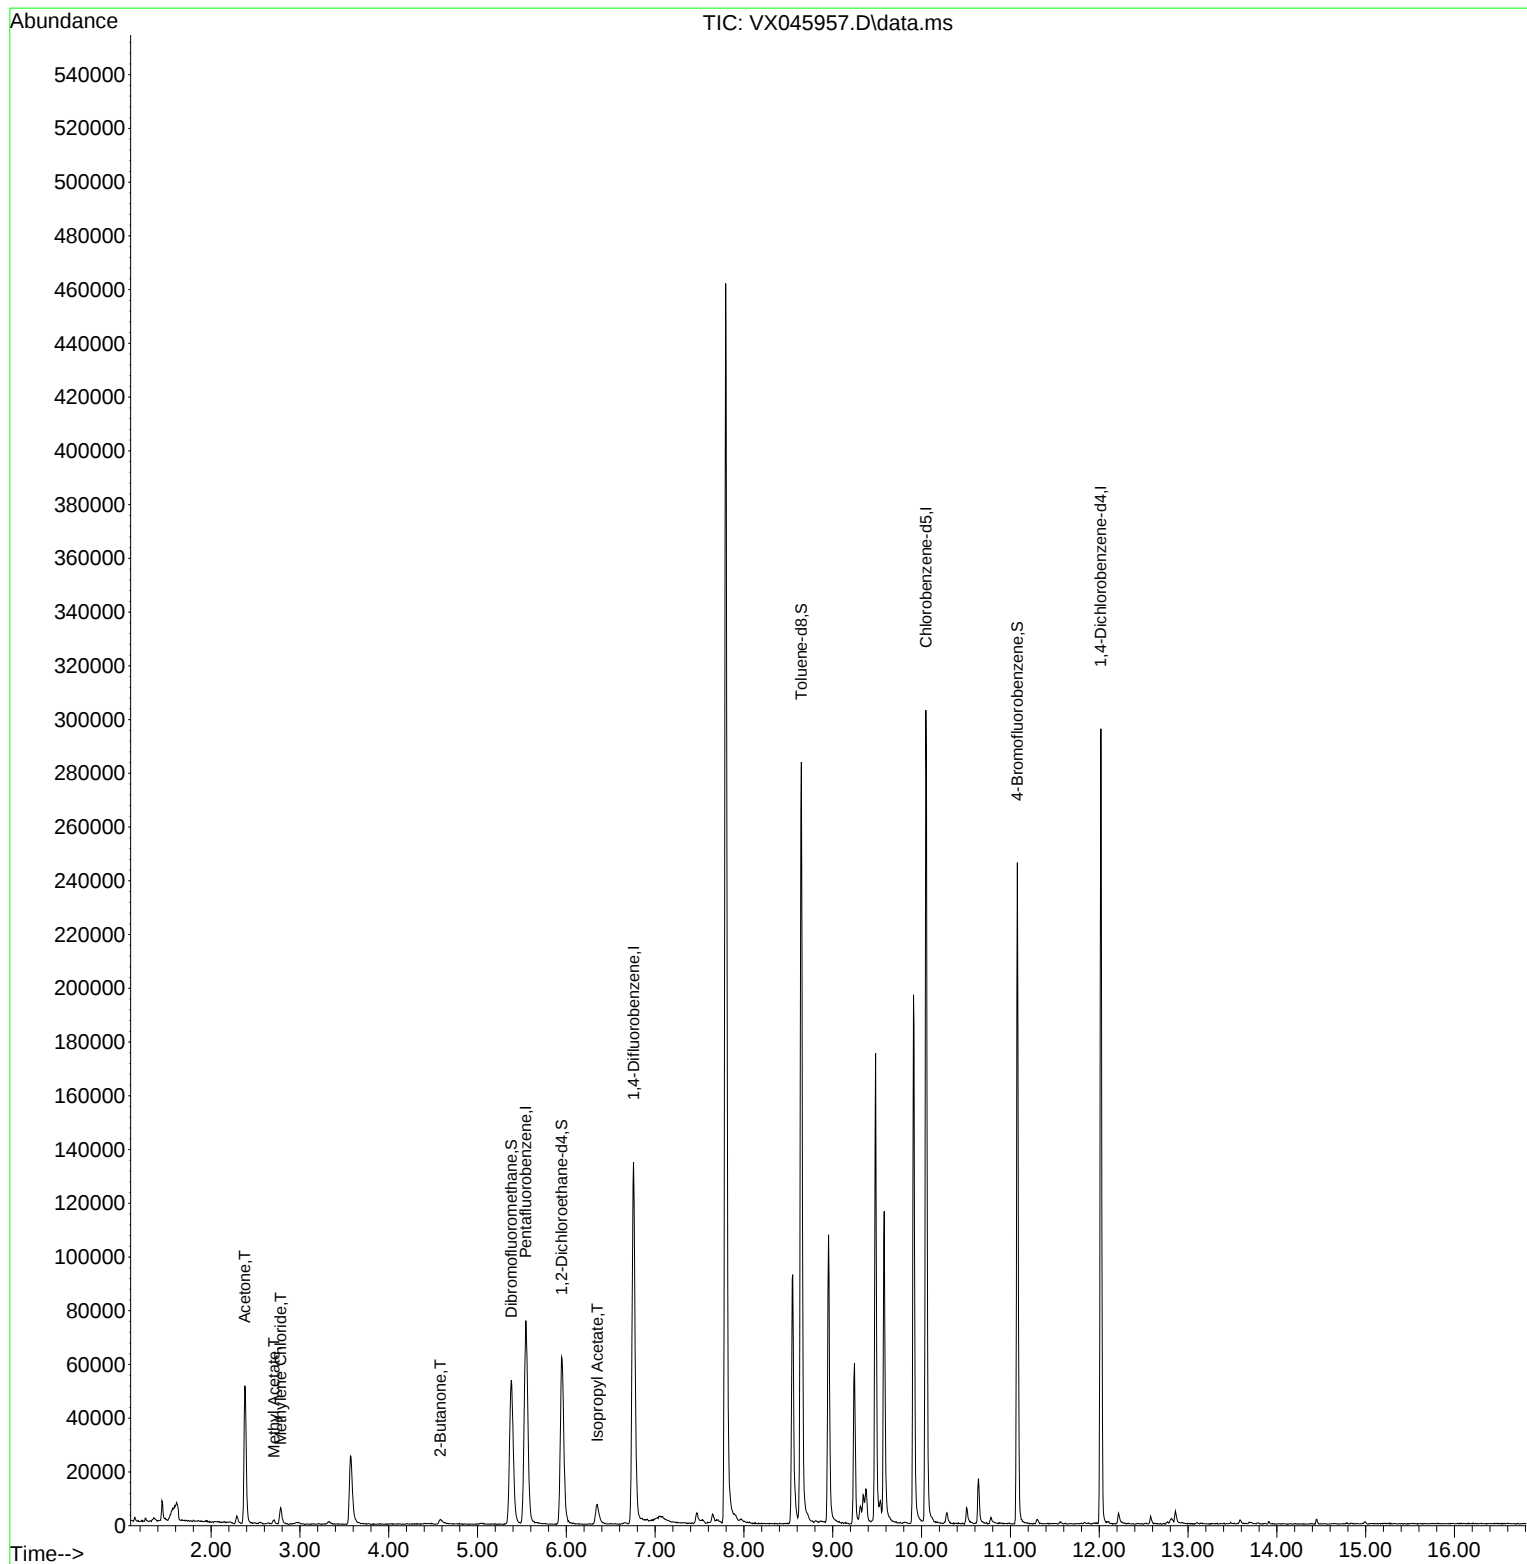




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C

Tgt Ion:168 Resp: 63272
Ion Ratio Lower Upper
168 100
99 74.1 52.3 78.5

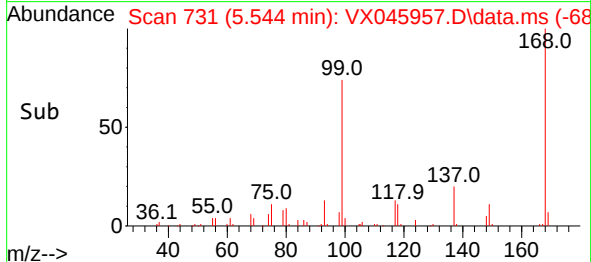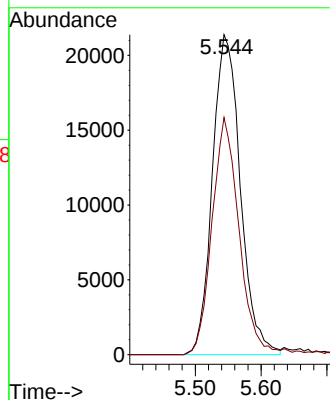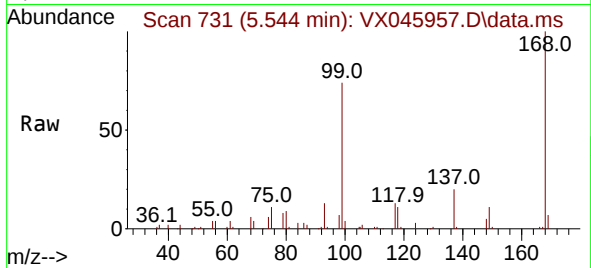

#16
Acetone
Concen: 122.973 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion: 43 Resp: 58428
Ion Ratio Lower Upper
43 100
58 27.5 22.3 33.5

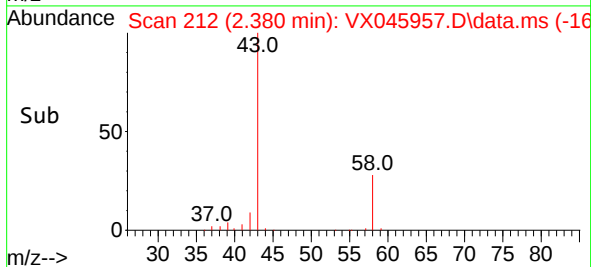
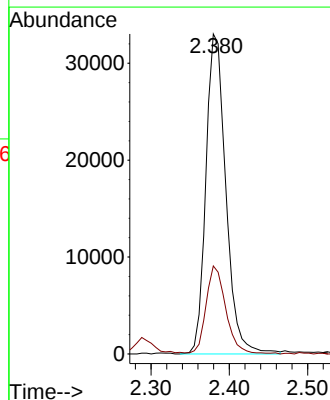
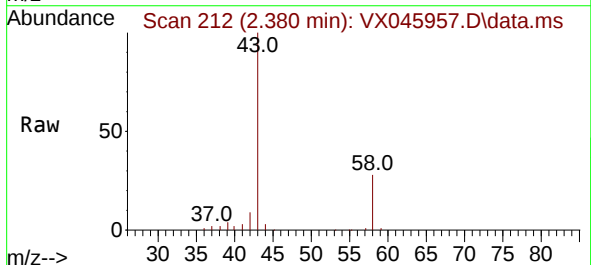




#18
Methyl Acetate
Concen: 1.844 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C

Tgt Ion: 43 Resp: 2017
Ion Ratio Lower Upper
43 100
74 19.3 17.5 26.3

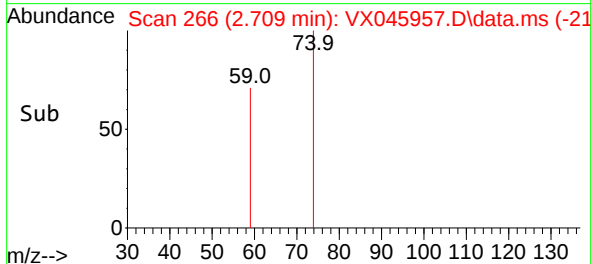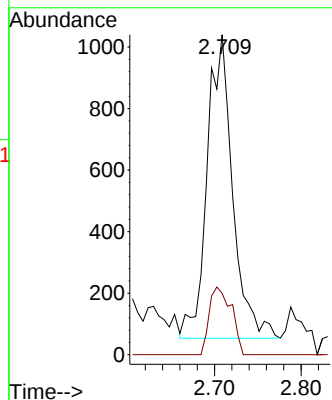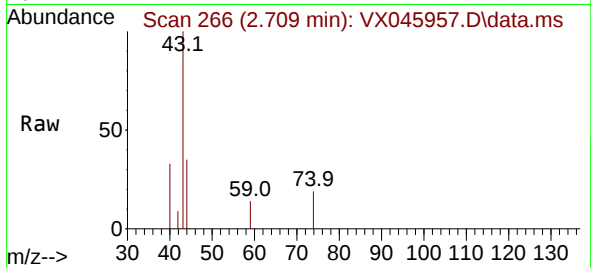

#20
Methylene Chloride
Concen: 2.987 ug/l
RT: 2.782 min Scan# 278
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion: 84 Resp: 2657
Ion Ratio Lower Upper
84 100
49 144.1 107.5 161.3
51 48.0 33.0 49.6
86 58.9 50.1 75.1

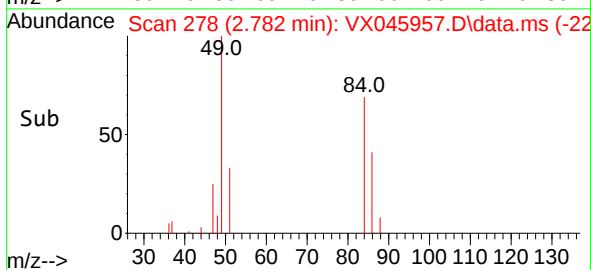
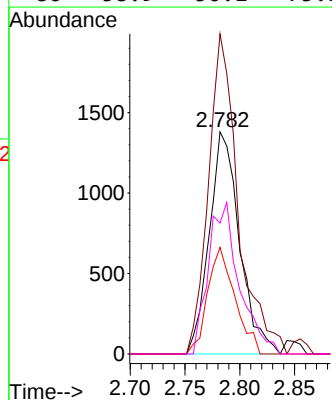
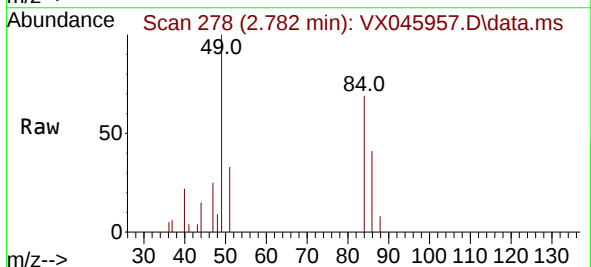




#25
2-Butanone
Concen: 6.370 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.024 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C

Tgt Ion: 43 Resp: 4430
Ion Ratio Lower Upper
43 100
72 15.7 18.6 28.0#

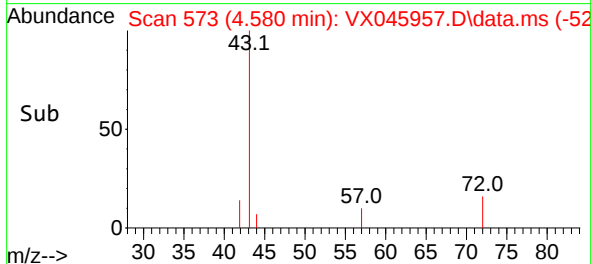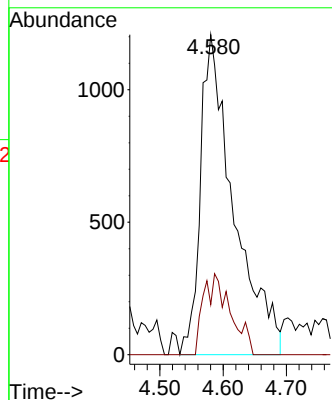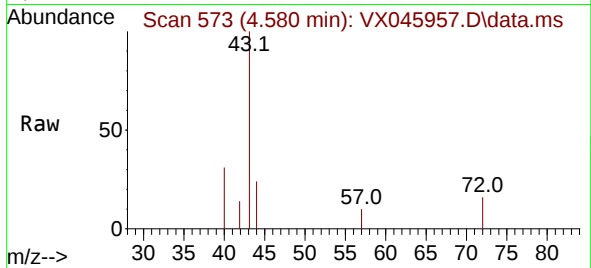

#33
1,2-Dichloroethane-d4
Concen: 55.670 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion: 65 Resp: 64415
Ion Ratio Lower Upper
65 100
67 49.7 0.0 99.0

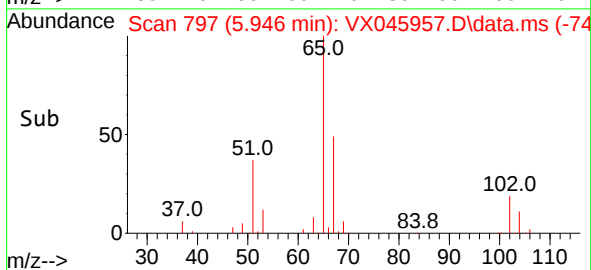
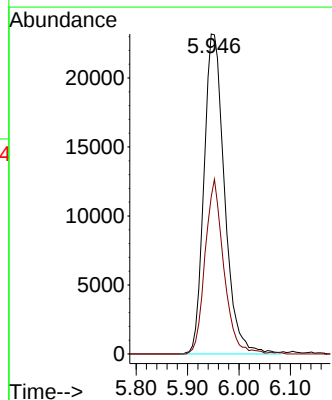
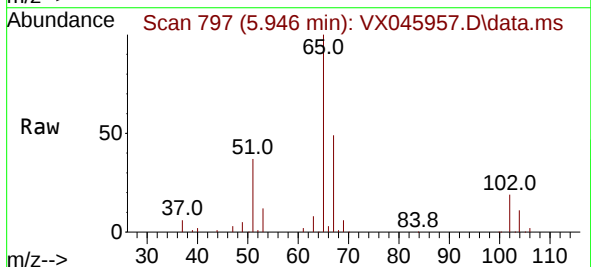




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C

Tgt Ion:114 Resp: 128718
Ion Ratio Lower Upper
114 100
63 24.8 0.0 46.8
88 17.5 0.0 35.4

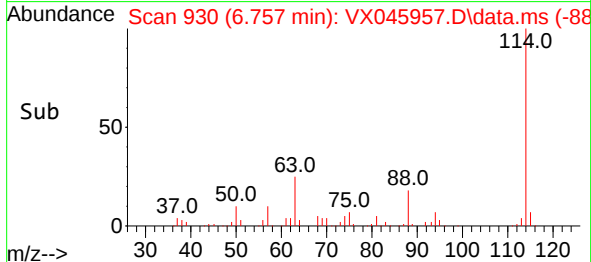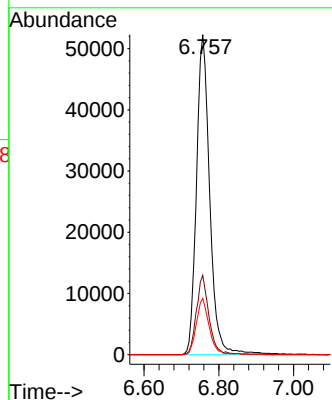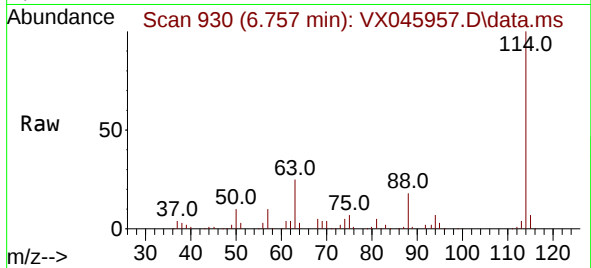

#35
Dibromofluoromethane
Concen: 50.791 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion:113 Resp: 46385
Ion Ratio Lower Upper
113 100
111 104.3 81.8 122.6
192 16.7 13.8 20.6

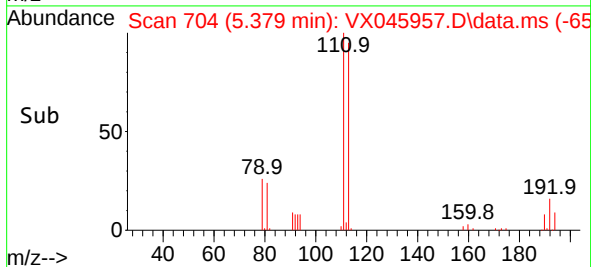
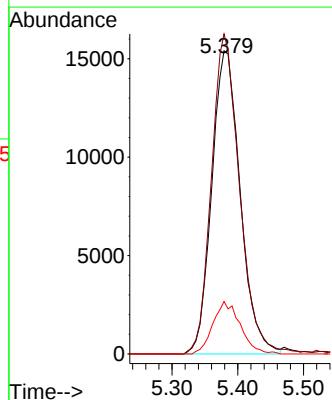
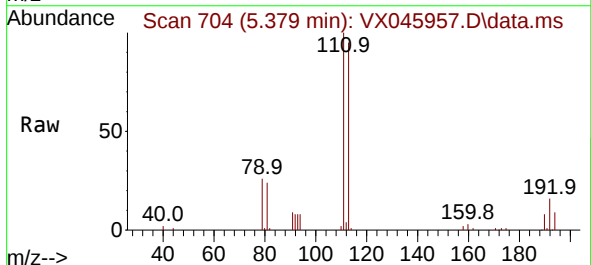




#43
Isopropyl Acetate
Concen: 4.890 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C

Tgt Ion: 43 Resp: 11517
Ion Ratio Lower Upper
43 100
61 16.9 14.1 21.1
87 11.2 9.2 13.8

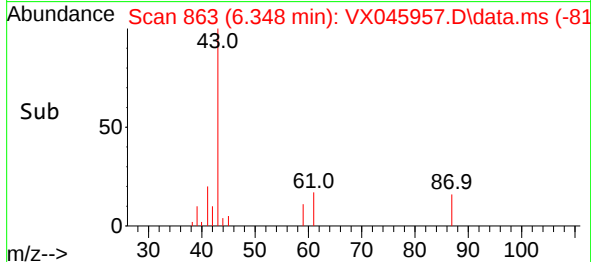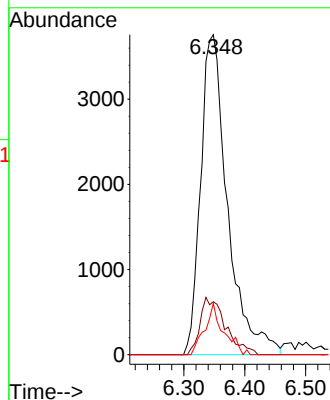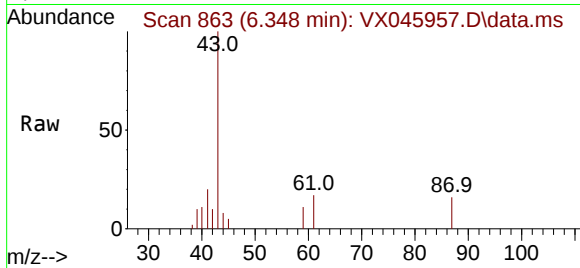

#50
Toluene-d8
Concen: 51.024 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion: 98 Resp: 162646
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.4

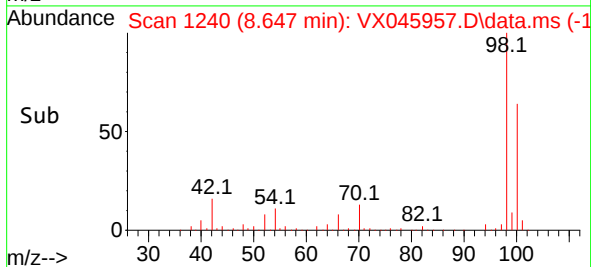
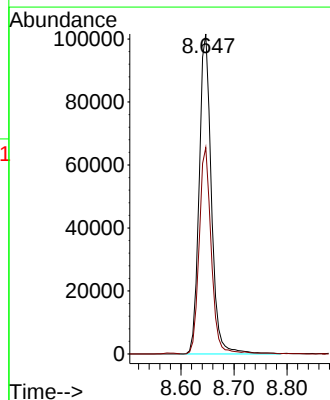
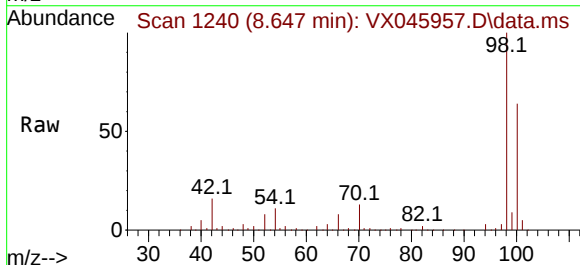




#62
4-Bromofluorobenzene
Concen: 54.650 ug/l
RT: 11.079 min Scan# 1
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26




Instrument :
MSVOA_X
ClientSampleId :
MH-C


Tgt Ion: 95 Resp: 63454
Ion Ratio Lower Upper
95 100
174 66.8 0.0 135.8
176 64.1 0.0 131.4

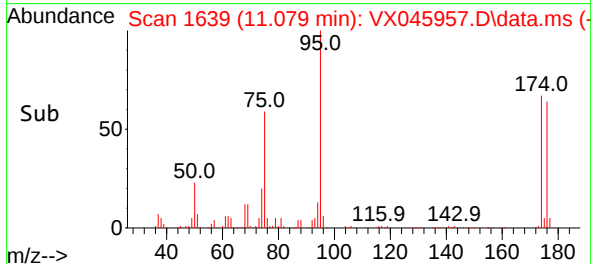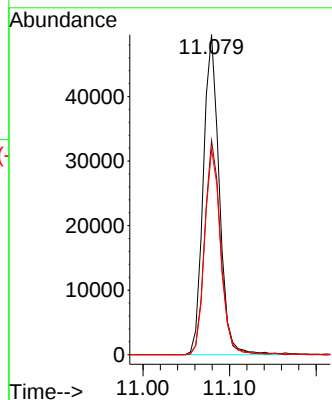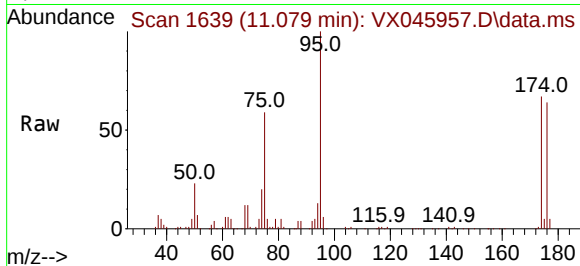

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX045957.D
Acq: 28 Apr 2025 15:26

Tgt Ion: 117 Resp: 123117
Ion Ratio Lower Upper
117 100
82 63.9 49.2 73.8
119 30.6 25.1 37.7

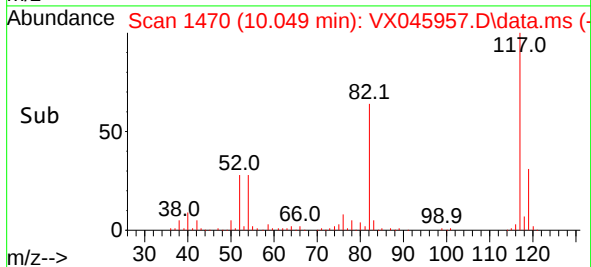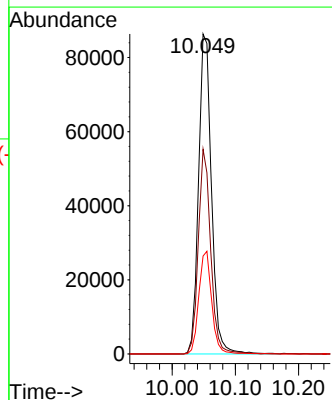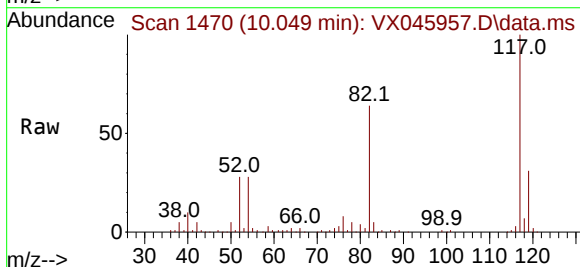

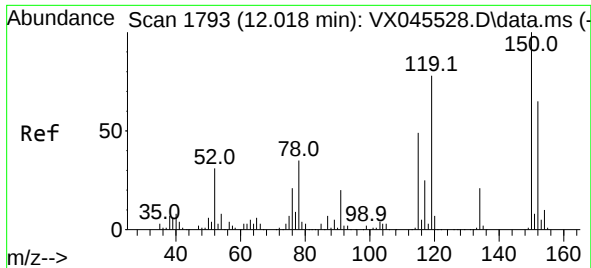

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX045957.D


Acq: 28 Apr 2025 15:26

Instrument :

MSVOA_X

ClientSampleId :

MH-C

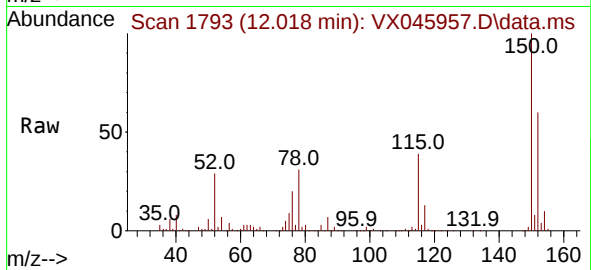

Tgt Ion:152 Resp: 53117

Ion Ratio Lower Upper

152 100

115 64.2 46.9 140.7

150 158.6 0.0 349.4

