



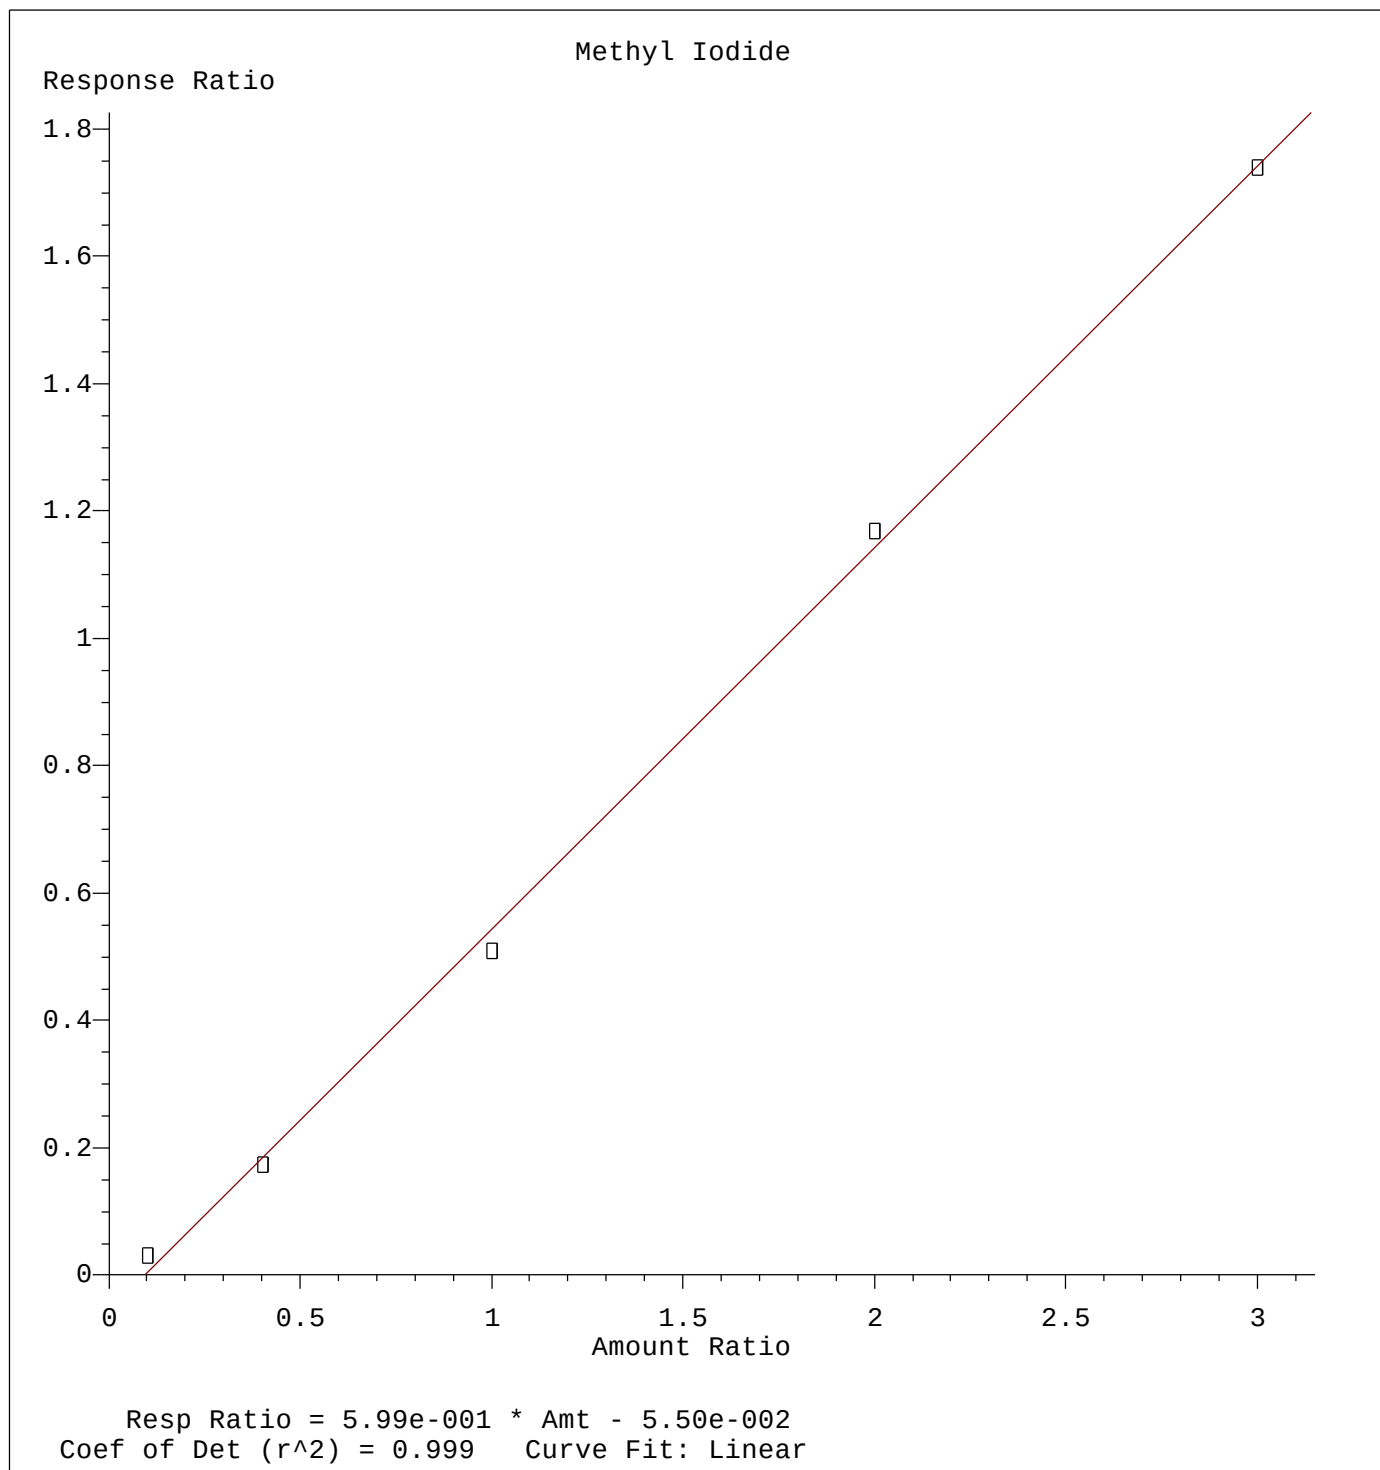

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Calibration Table Last Updated: Tue Apr 30 07:03:14 2019

Bromochloromethane

Response Ratio

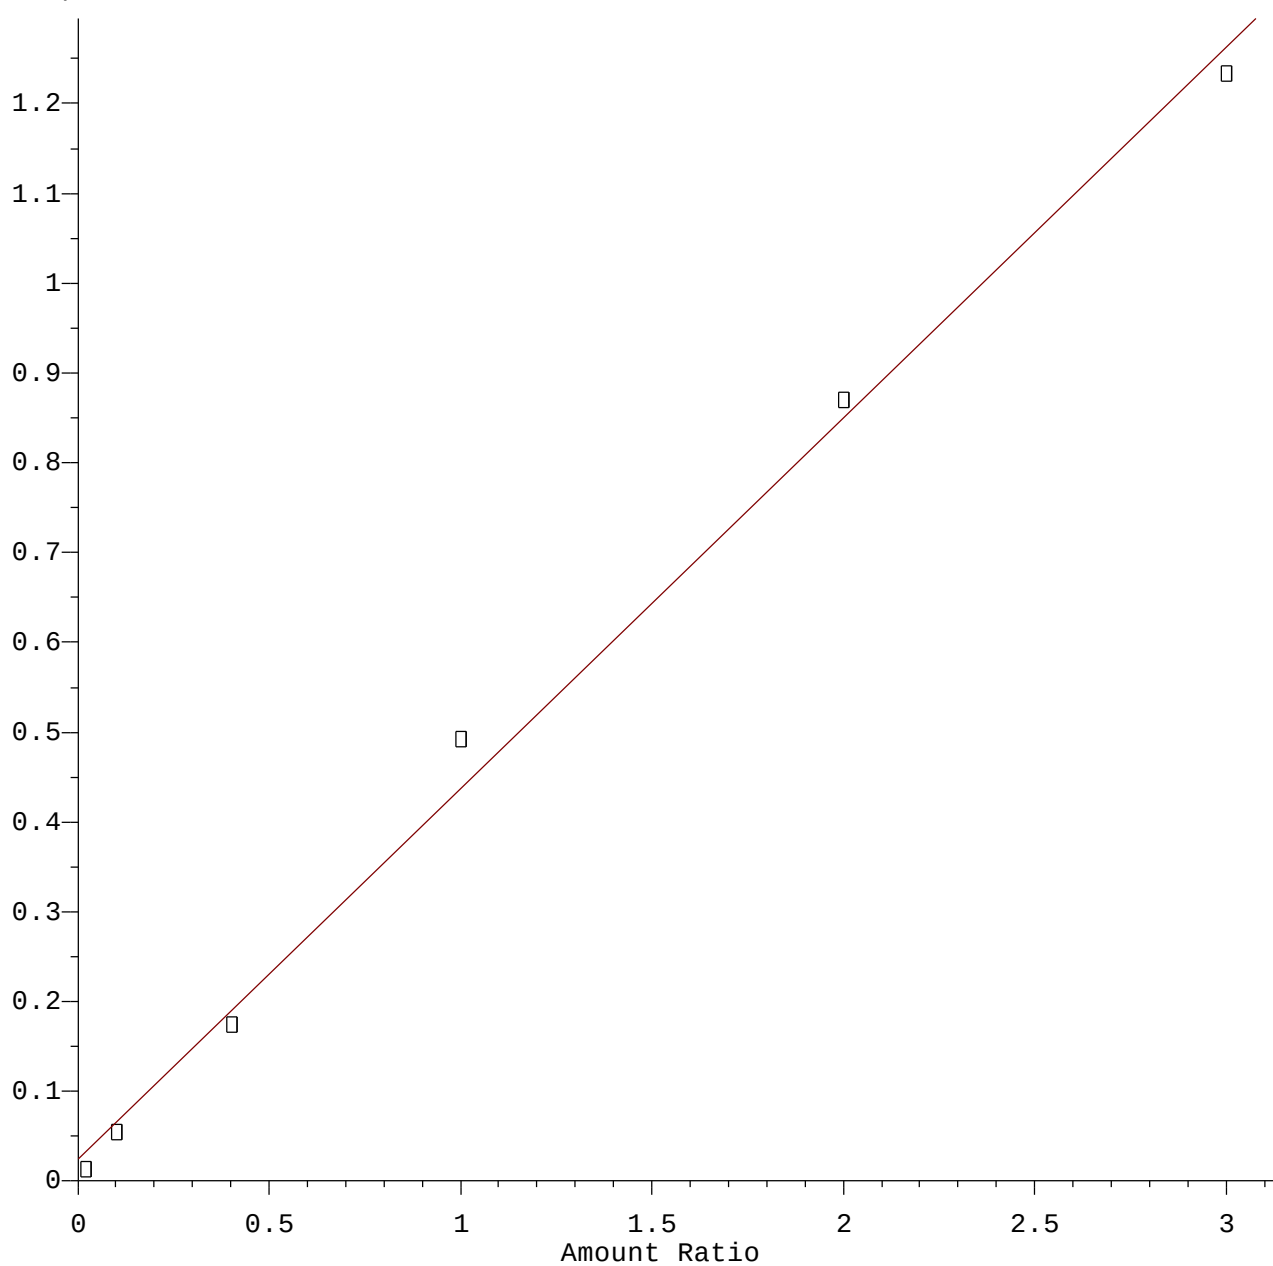

Resp Ratio = $4.13 \times 10^{-1} \times \text{Amt} + 2.39 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Calibration Table Last Updated: Tue Apr 30 07:03:50 2019