


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX042919\
Data File : VX009207.D
Acq On : 29 Apr 2019 15:02
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Title : SW846 8260
Last Update : Tue Apr 30 07:03:50 2019

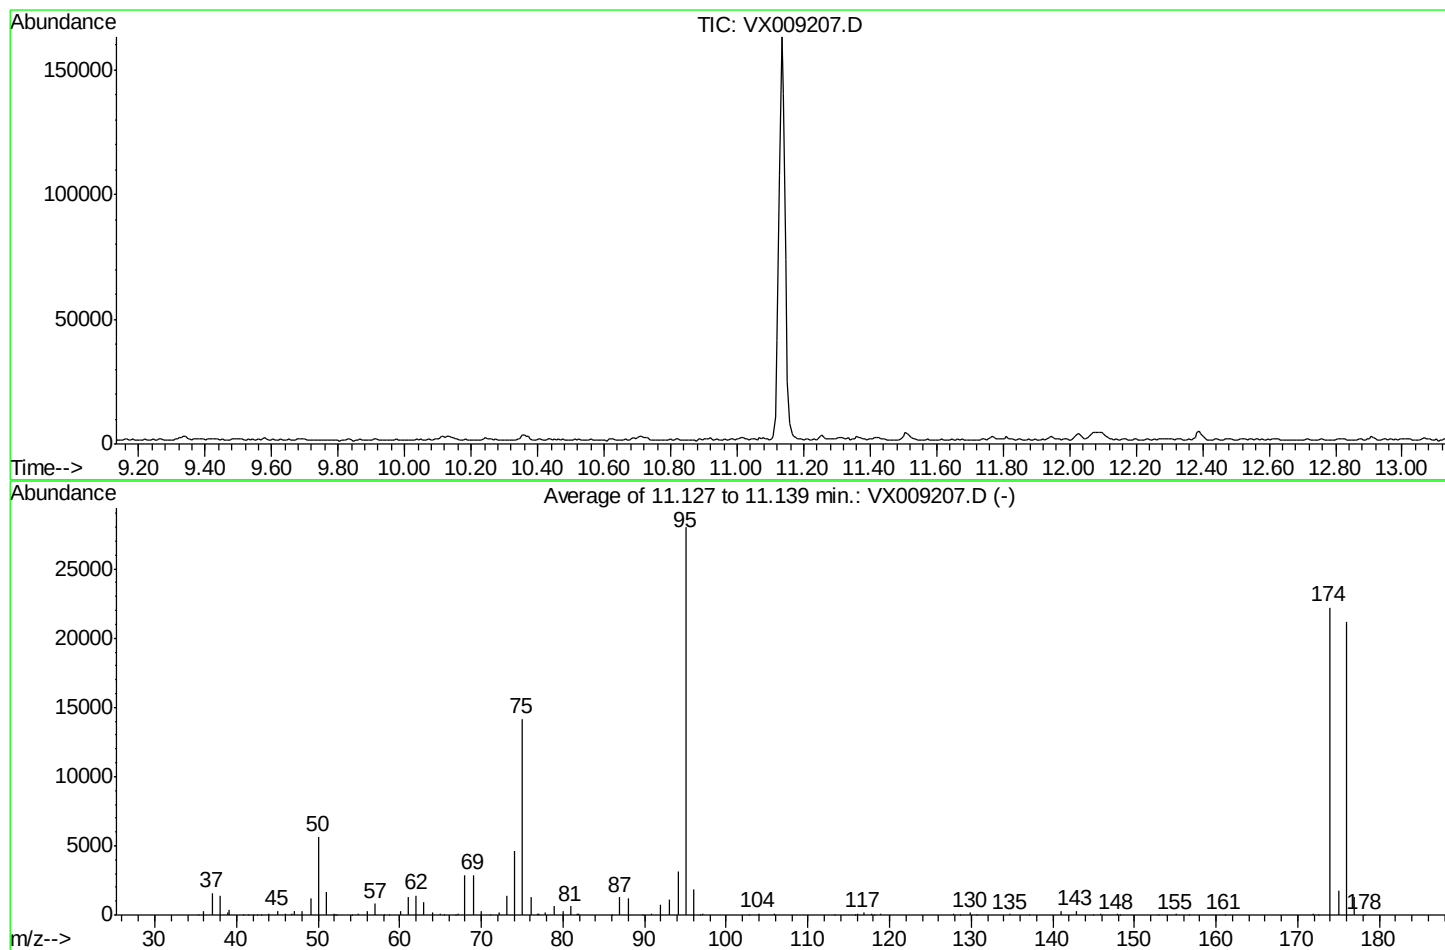

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	5657	PASS
75	95	30	60	50.6	14157	PASS
95	95	100	100	100.0	28000	PASS
96	95	5	9	6.6	1843	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.4	22231	PASS
175	174	5	9	8.1	1805	PASS
176	174	95	101	95.2	21161	PASS
177	176	5	9	6.3	1331	PASS