

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX042920\  
 Data File : VX015980.D  
 Acq On : 29 Apr 2020 16:25  
 Operator : JC/SP  
 Sample : L2405-08  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BLIND-DUPLICATE

## Integration Parameters: RTEINT.P

Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X042820W.M  
 Title : SW846 8260

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.575       | 236           | 244         | 252          | rBV2     | 8156           | 17839         | 1.27%           | 0.230%        |
| 2         | 5.470       | 706           | 719         | 731          | rBV      | 154173         | 437432        | 31.20%          | 5.651%        |
| 3         | 5.635       | 734           | 746         | 763          | rVB      | 280617         | 778889        | 55.55%          | 10.063%       |
| 4         | 6.037       | 801           | 812         | 825          | rBV      | 173359         | 456700        | 32.57%          | 5.900%        |
| 5         | 6.836       | 933           | 943         | 962          | rBV      | 424200         | 1012630       | 72.22%          | 13.082%       |
| 6         | 8.695       | 1241          | 1248        | 1257         | rBV      | 907237         | 1402163       | 100.00%         | 18.115%       |
| 7         | 10.098      | 1471          | 1478        | 1487         | rBV      | 946141         | 1257899       | 89.71%          | 16.251%       |
| 8         | 11.122      | 1639          | 1646        | 1654         | rBV      | 846894         | 1040965       | 74.24%          | 13.448%       |
| 9         | 12.061      | 1795          | 1800        | 1808         | rBV      | 1087665        | 1335880       | 95.27%          | 17.259%       |


Sum of corrected areas: 7740397

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX042920\  
Data File : VX015980.D  
Acq On : 29 Apr 2020 16:25  
Operator : JC/SP  
Sample : L2405-08  
Misc : 5.0mL/MSVOA X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042820W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

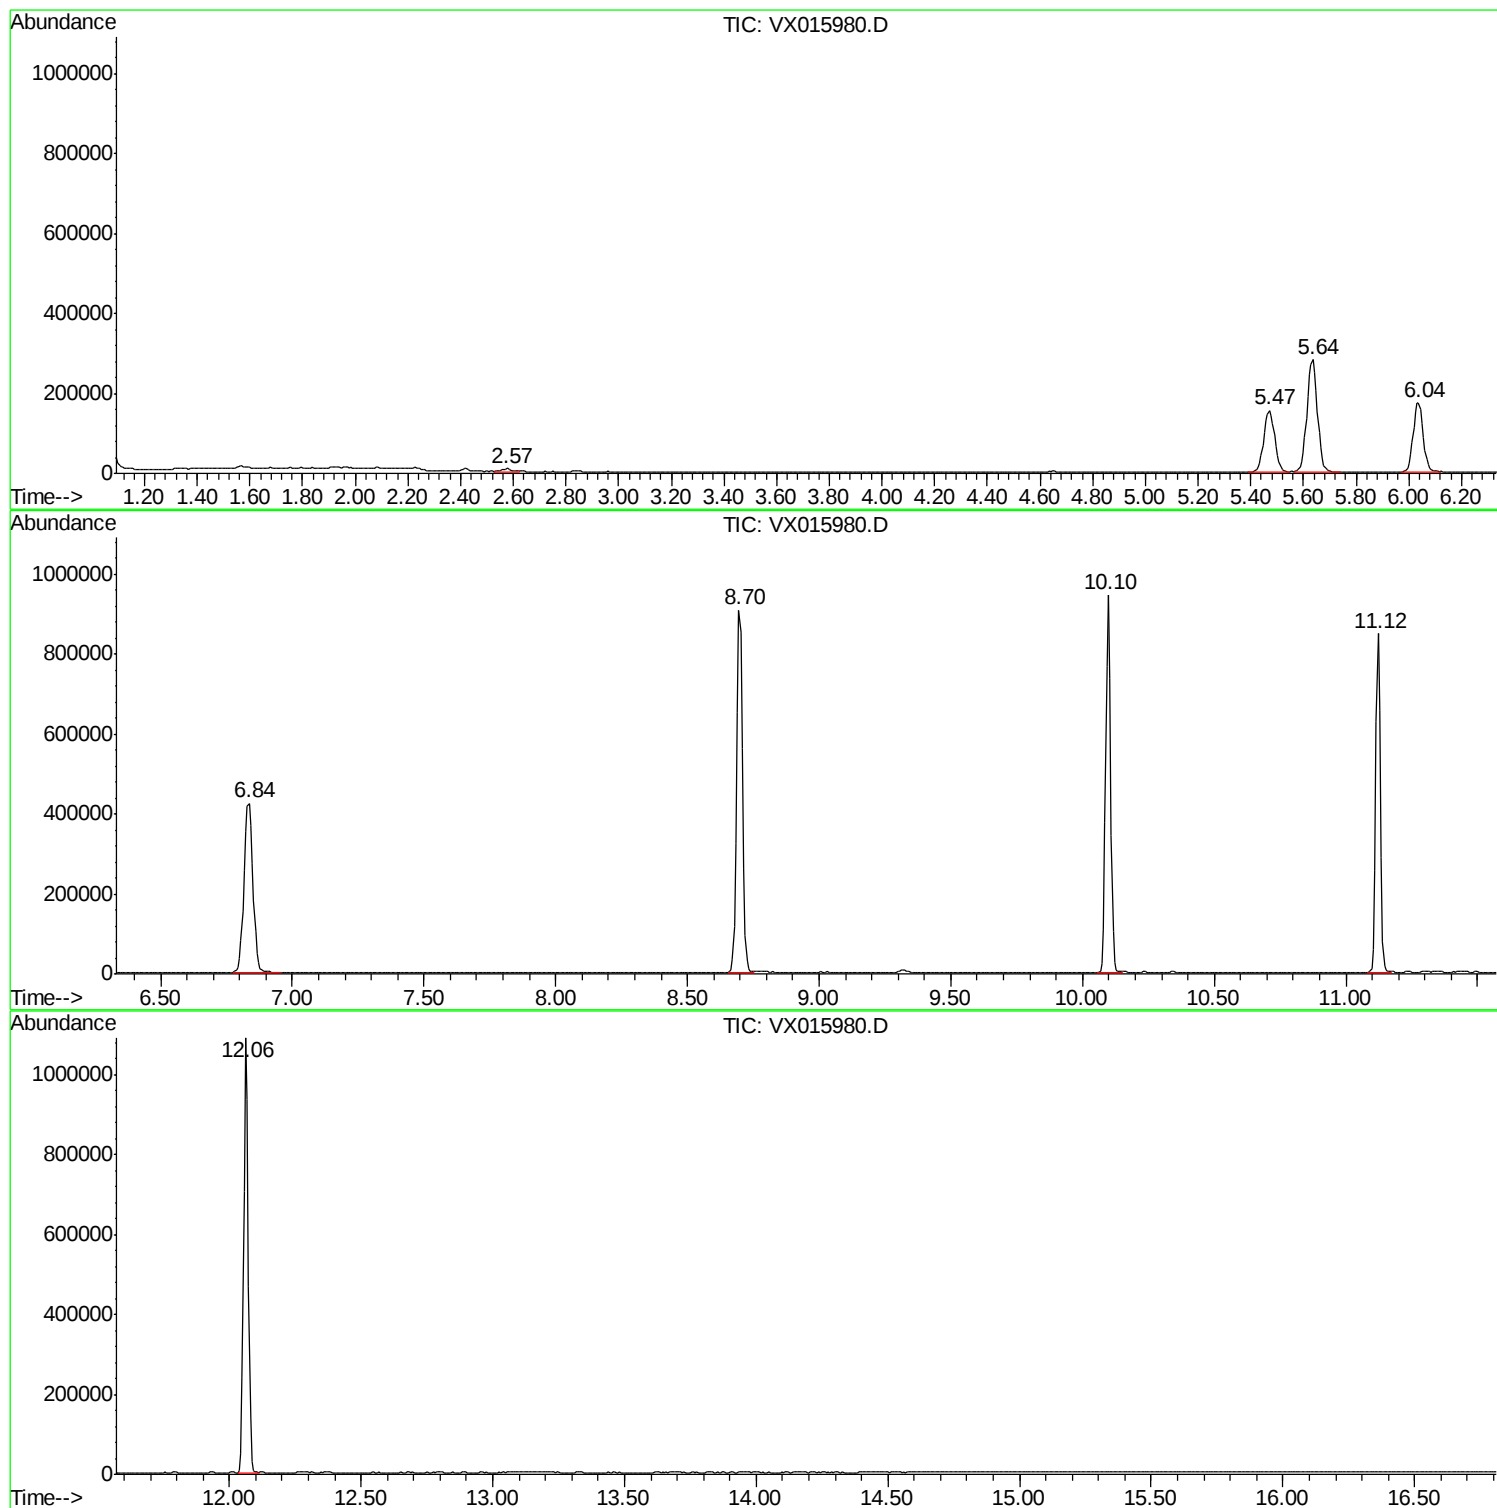

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX042920\  
Data File : VX015980.D  
Acq On : 29 Apr 2020 16:25  
Operator : JC/SP  
Sample : L2405-08  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042820W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA\_X\DATA\VX042920\  
Data File : VX015980.D  
Acq On : 29 Apr 2020 16:25  
Operator : JC/SP  
Sample : L2405-08  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BLIND-DUPLICATE

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA\_X\METHOD\82X042820W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |
|------------------|----|---------|-------|----------|-----------------------|
|                  |    |         |       |          | # RT Resp Conc        |