

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
 Data File : VX028431.D
 Acq On : 29 Apr 2022 18:09
 Operator : JC/MD
 Sample : N2640-07
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MWBR3-B-117-137-042922

Quant Time: Apr 30 09:16:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	390066	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	674233	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	652767	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	311304	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	282201	55.486	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 110.980%	
35) Dibromofluoromethane	5.391	113	254115	53.743	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 107.480%	
50) Toluene-d8	8.653	98	947466	52.171	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 104.340%	
62) 4-Bromofluorobenzene	11.079	95	344458	49.606	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 99.220%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	1.142	85	841	0.334	ug/l	96
3) Chloromethane	1.294	50	532	Below Cal		99
4) Vinyl Chloride	1.374	62	1333	0.339	ug/l #	86
5) Bromomethane	1.617	94	887	Below Cal		81
6) Chloroethane	1.697	64	1144	Below Cal	#	82
8) Diethyl Ether	2.325	74	44	Below Cal	#	7
10) Methyl Iodide	2.459	142	485	5.335	ug/l #	89
11) Tert butyl alcohol	2.940	59	693	Below Cal	#	72
12) 1,1-Dichloroethene	2.325	96	190888	63.677	ug/l	95
14) Allyl chloride	2.532	41	3910	0.777	ug/l #	65
16) Acetone	2.379	43	8437	4.058	ug/l	98
18) Methyl Acetate	2.703	43	994	0.220	ug/l #	59
20) Methylene Chloride	2.788	84	1383	0.366	ug/l #	74
21) trans-1,2-Dichloroethene	3.093	96	13739	3.370	ug/l	96
24) 1,1-Dichloroethane	3.611	63	31194	4.611	ug/l	97
27) cis-1,2-Dichloroethene	4.489	96	129482	26.636	ug/l	85
29) Tetrahydrofuran	5.025	42	429	0.218	ug/l #	46
30) Chloroform	5.092	83	2567	0.316	ug/l	93
31) Cyclohexane	5.556	56	7710	1.244	ug/l #	1
36) 1,1-Dichloropropene	5.556	75	28336	4.594	ug/l #	50
38) Carbon Tetrachloride	5.556	117	40212	5.775	ug/l #	16
39) Methylcyclohexane	7.129	83	9009	1.158	ug/l #	1
42) 1,2-Dichloroethane	6.086	62	19449	2.902	ug/l	100
44) Trichloroethene	7.129	130	811557	155.010	ug/l	99
49) 1,4-Dioxane	7.671	88	2516	20.112	ug/l	99
51) 4-Methyl-2-Pentanone	8.647	43	3577	0.547	ug/l #	1
52) Toluene	8.720	92	3745	0.299	ug/l	92
60) Dibromochloromethane	9.275	129	3635	0.654	ug/l #	9
64) Tetrachloroethene	9.275	164	4326	0.848	ug/l	90
76) 1,2,3-Trichloropropane	11.079	75	176975	28.886	ug/l #	38
81) trans-1,4-Dichloro-2-b...	11.079	75	176975	85.842	ug/l #	15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
Data File : VX028431.D
Acq On : 29 Apr 2022 18:09
Operator : JC/MD
Sample : N2640-07
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922

Quant Time: Apr 30 09:16:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




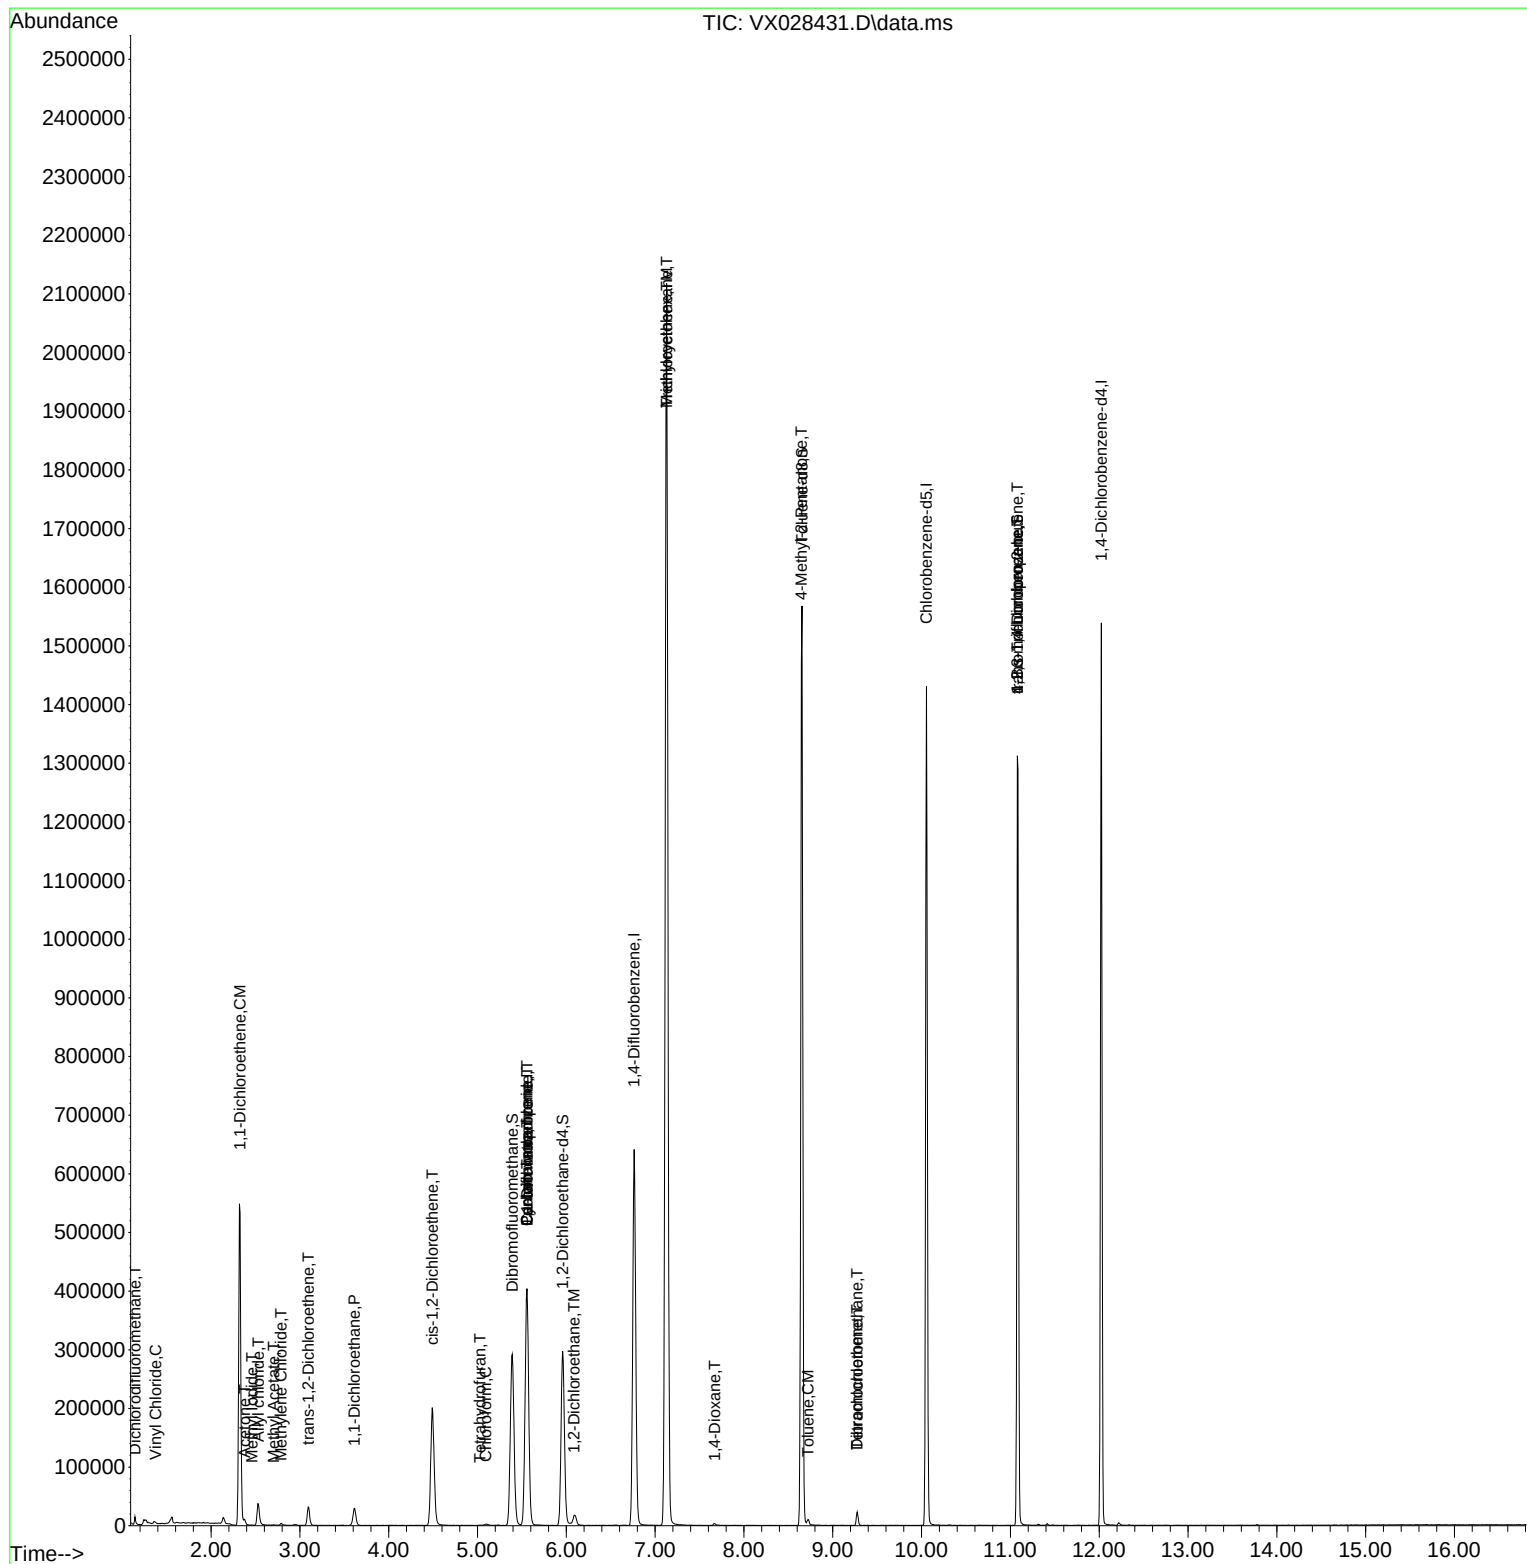




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument : MSVOA_X
ClientSampleId : MWBR3-B-117-137-042922


Tgt Ion:168 Resp: 390066
Ion Ratio Lower Upper
168 100
99 54.0 41.7 62.5

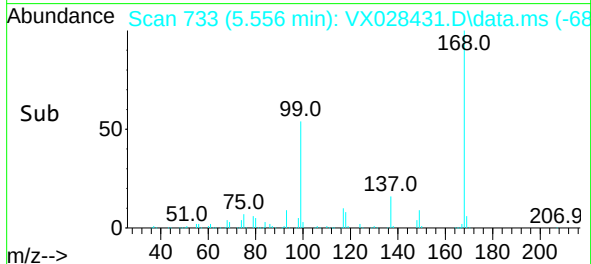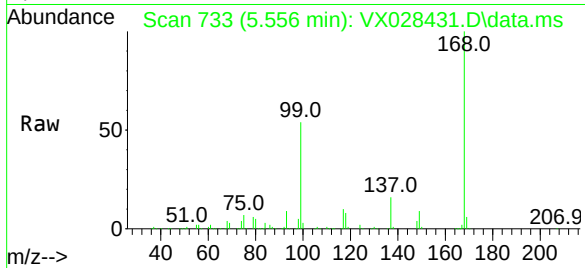

#2
Dichlorodifluoromethane
Concen: 0.334 ug/l
RT: 1.142 min Scan# 9
Delta R.T. -0.024 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 85 Resp: 841
Ion Ratio Lower Upper
85 100
87 30.4 16.2 48.6


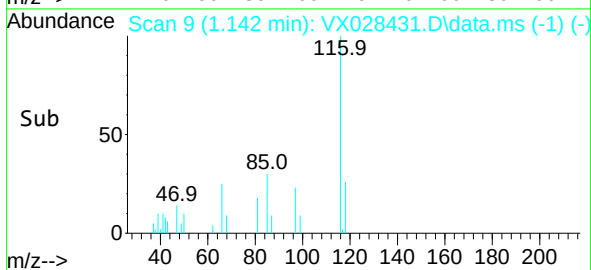

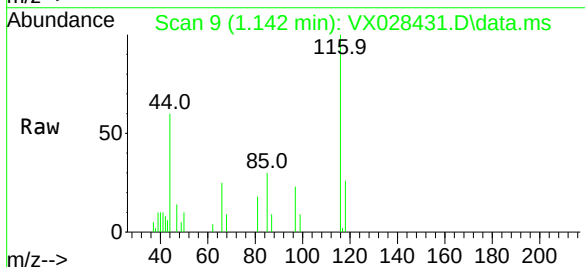


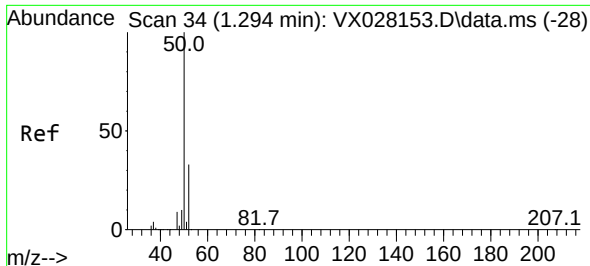

#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 50 Resp: 532
Ion Ratio Lower Upper
50 100
52 32.2 26.4 39.6

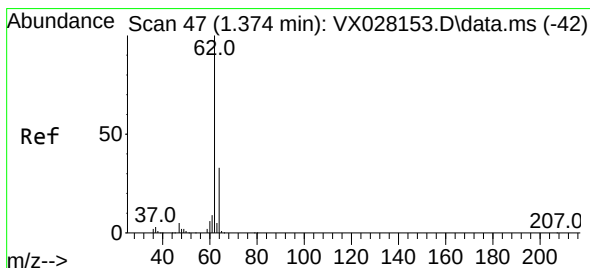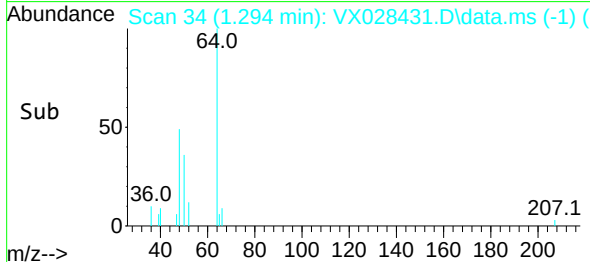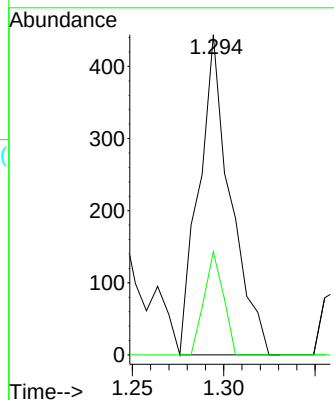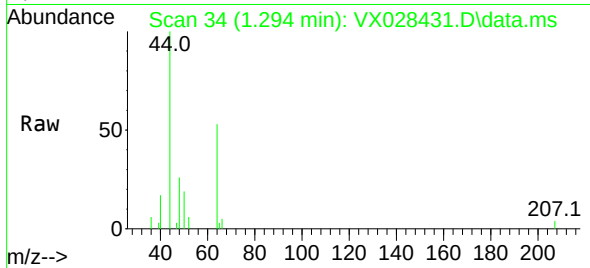

#4
Vinyl Chloride
Concen: 0.339 ug/l
RT: 1.374 min Scan# 47
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 62 Resp: 1333
Ion Ratio Lower Upper
62 100
64 24.3 25.5 38.3#


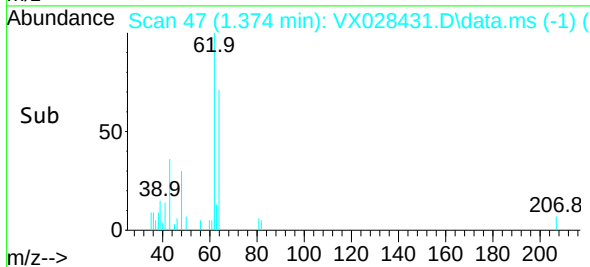
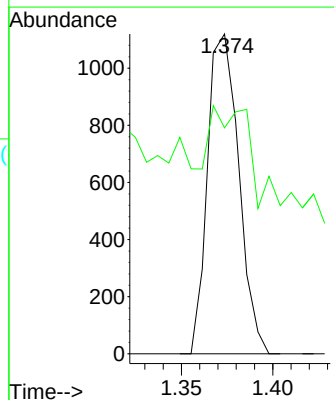
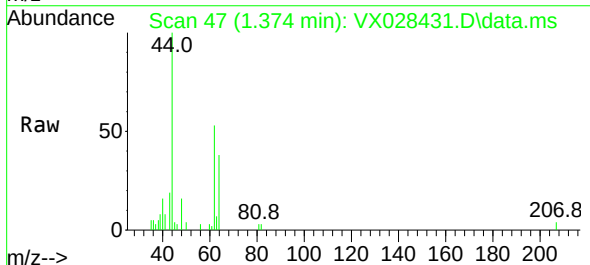


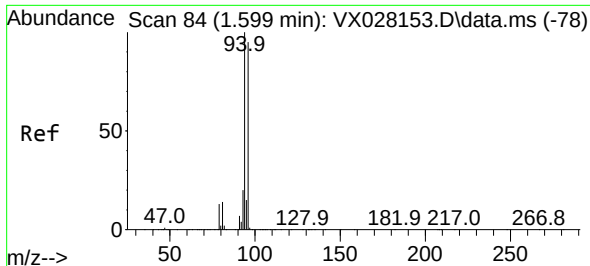

#5
Bromomethane
Concen: Below Cal
RT: 1.617 min Scan# 81
Delta R.T. 0.018 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 94 Resp: 887
Ion Ratio Lower Upper
94 100
96 76.0 75.3 112.9

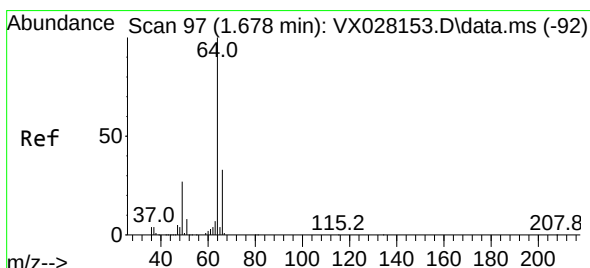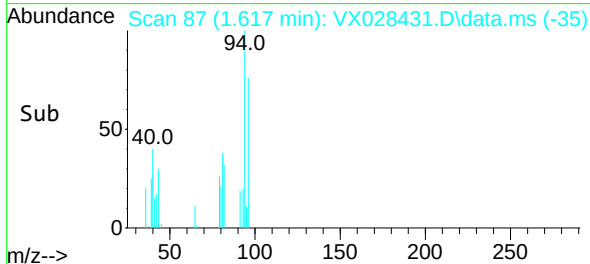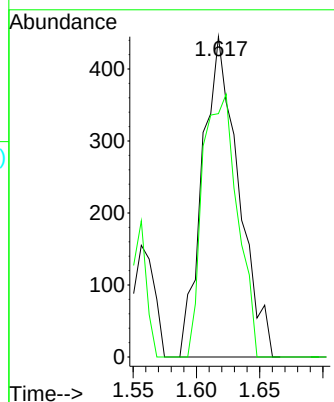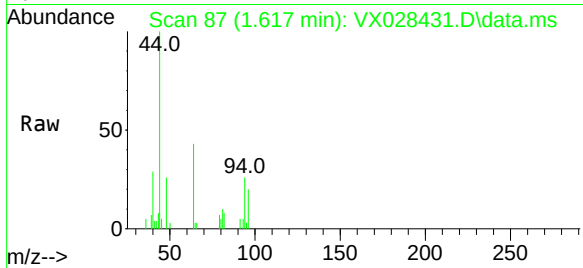

#6
Chloroethane
Concen: Below Cal
RT: 1.697 min Scan# 100
Delta R.T. 0.019 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 64 Resp: 1144
Ion Ratio Lower Upper
64 100
66 21.6 25.3 37.9#


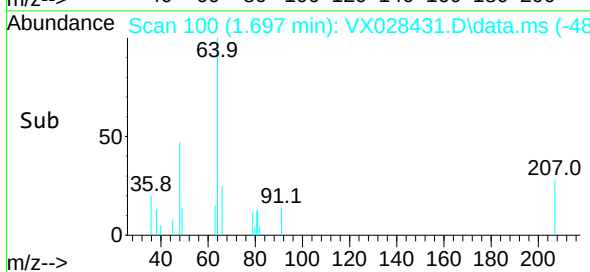
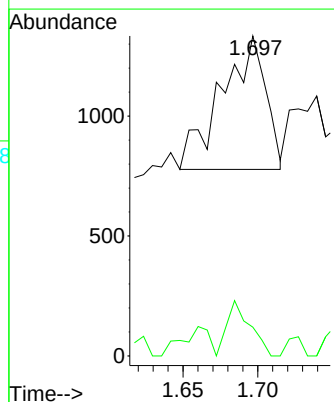
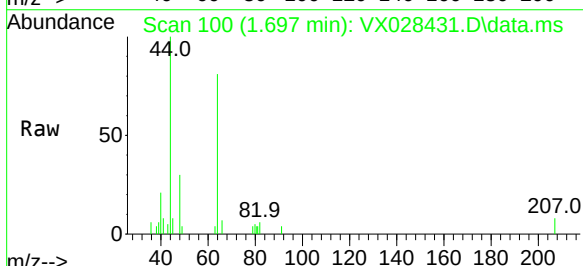




#8
Diethyl Ether
Concen: Below Cal
RT: 2.325 min Scan# 20
Delta R.T. 0.195 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 74 Resp: 44
Ion Ratio Lower Upper
74 100
45 0.0 42.0 126.0#

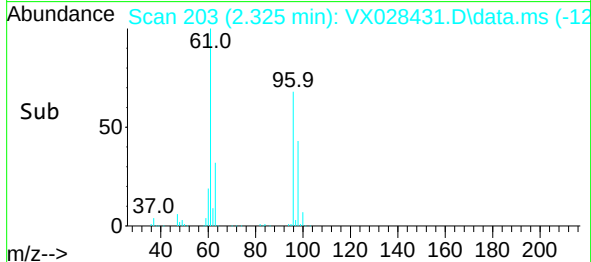

#10
Methyl Iodide
Concen: 5.335 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion:142 Resp: 485
Ion Ratio Lower Upper
142 100
127 49.5 33.9 50.9
141 10.1 11.4 17.2#

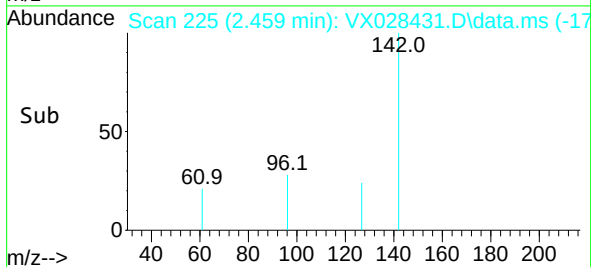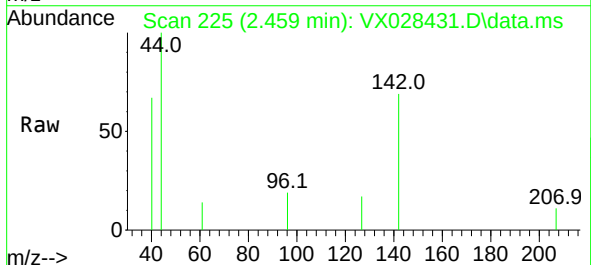

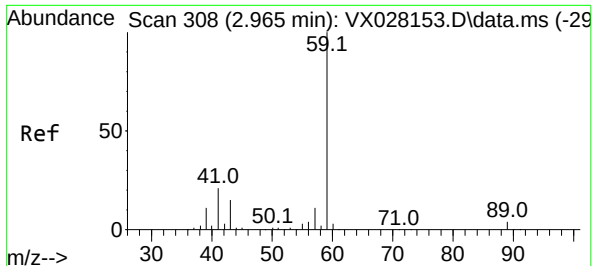

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.940 min Scan# 308

Delta R.T. -0.025 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09

Instrument :

MSVOA_X

ClientSampleId :





MWBR3-B-117-137-042922

Tgt Ion: 59 Resp: 693

Ion Ratio Lower Upper

59 100

57 0.0 8.3 12.5#

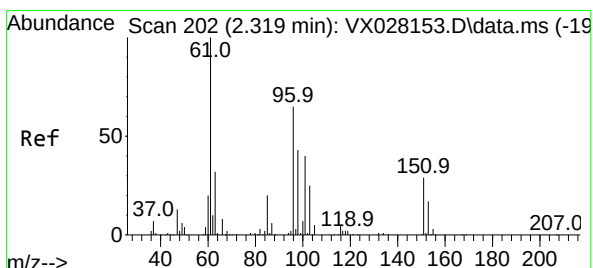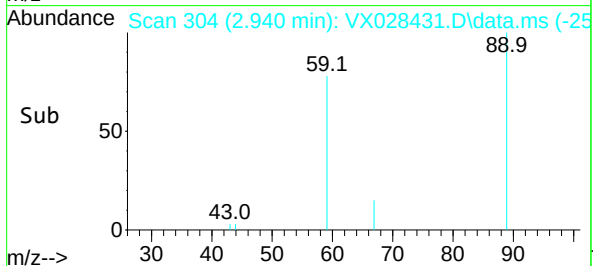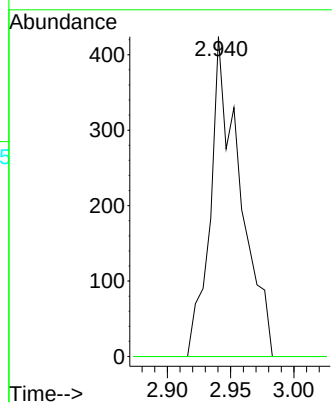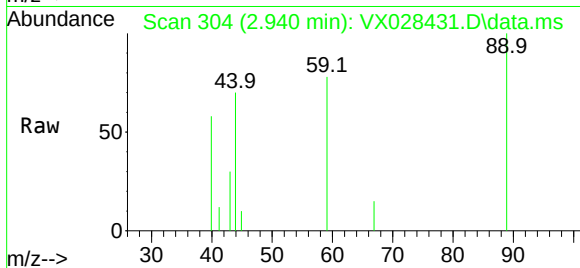

#12

1,1-Dichloroethene

Concen: 63.677 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09




Tgt Ion: 96 Resp: 190888


Ion Ratio Lower Upper

96 100

61 146.4 124.6 187.0

98 63.2 51.0 76.4


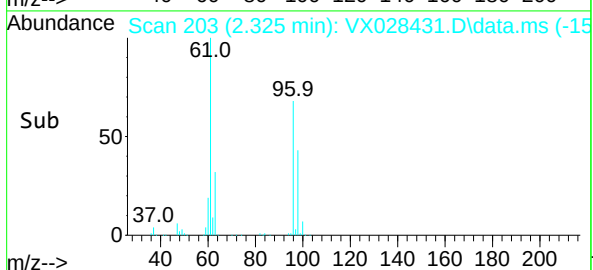

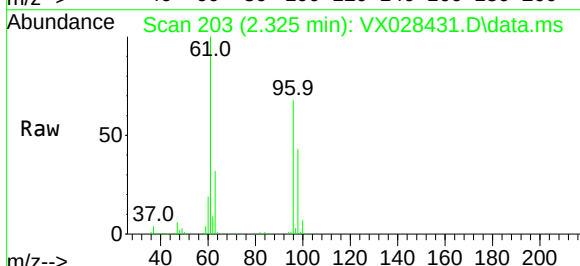




#14
 Allyl chloride
 Concen: 0.777 ug/l
 RT: 2.532 min Scan# 21
 Delta R.T. -0.134 min
 Lab File: VX028431.D
 Acq: 29 Apr 2022 18:09




Instrument :
 MSVOA_X
 ClientSampleId :
 MWBR3-B-117-137-042922


Tgt Ion: 41 Resp: 3910
 Ion Ratio Lower Upper
 41 100
 39 92.7 50.4 75.6#
 76 21.4 32.7 49.1#

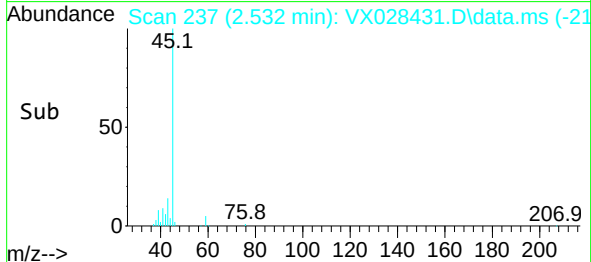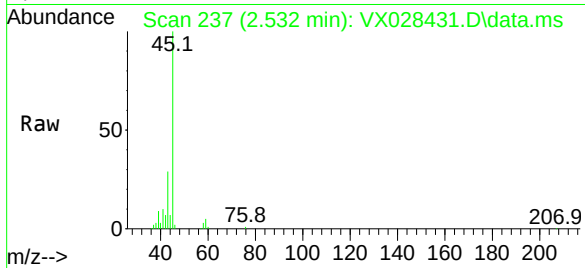

#16
 Acetone
 Concen: 4.058 ug/l
 RT: 2.379 min Scan# 212
 Delta R.T. -0.001 min
 Lab File: VX028431.D
 Acq: 29 Apr 2022 18:09

Tgt Ion: 43 Resp: 8437
 Ion Ratio Lower Upper
 43 100
 58 34.9 28.8 43.2


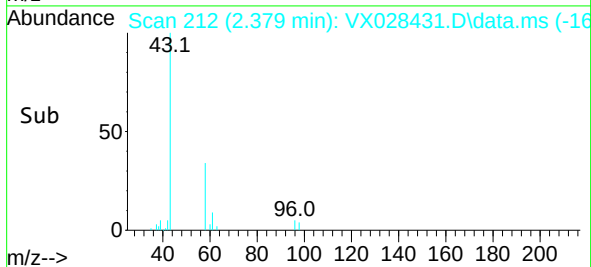

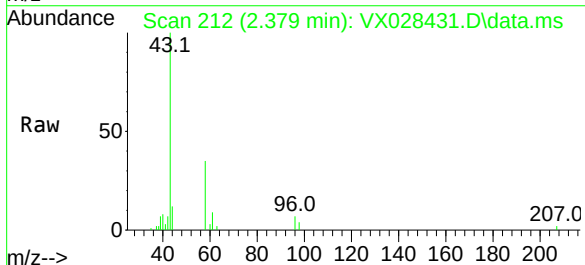




#18
Methyl Acetate
Concen: 0.220 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 43 Resp: 994
Ion Ratio Lower Upper
43 100
74 6.6 22.8 34.2#

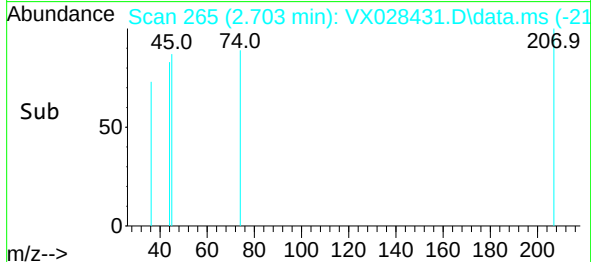

#20
Methylene Chloride
Concen: 0.366 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 84 Resp: 1383
Ion Ratio Lower Upper
84 100
49 143.7 85.5 128.3#
51 47.8 26.6 39.8#
86 72.5 51.5 77.3


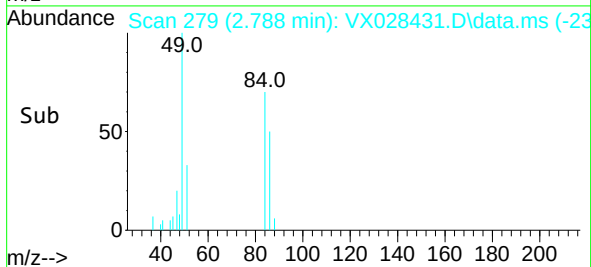

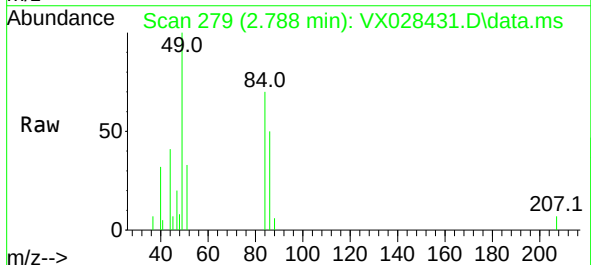




#21
trans-1,2-Dichloroethene
Concen: 3.370 ug/l
RT: 3.093 min Scan# 31
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument : MSVOA_X
ClientSampleId : MWBR3-B-117-137-042922


Tgt Ion: 96 Resp: 13739
Ion Ratio Lower Upper
96 100
61 129.2 105.4 158.2
98 68.6 50.0 75.0

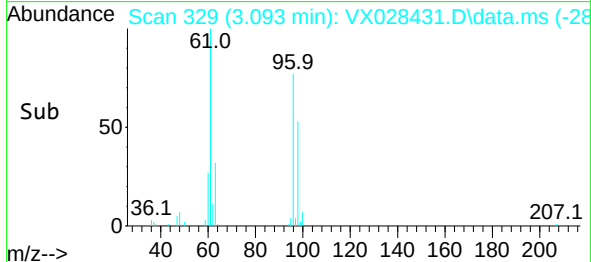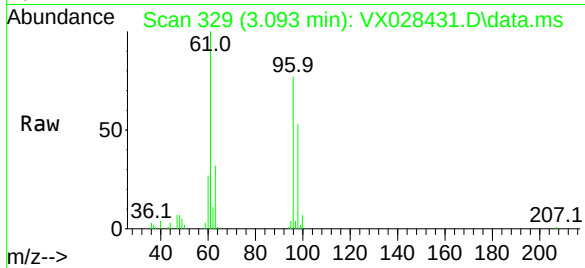

#24
1,1-Dichloroethane
Concen: 4.611 ug/l
RT: 3.611 min Scan# 414
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 63 Resp: 31194
Ion Ratio Lower Upper
63 100
98 9.1 3.9 11.7
100 5.6 2.4 7.2

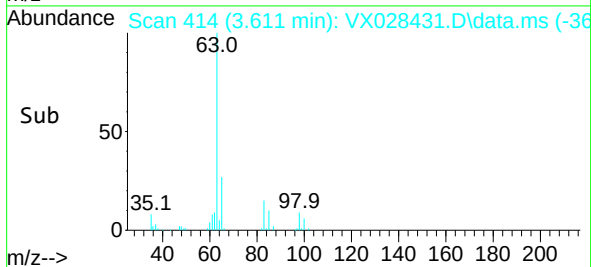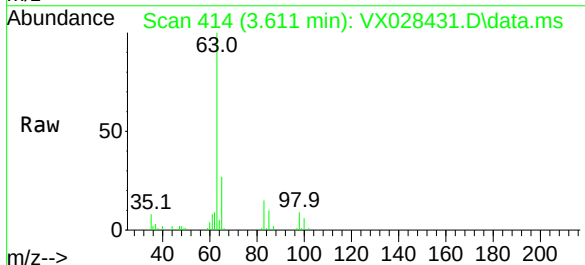



#27

cis-1,2-Dichloroethene

Concen: 26.636 ug/l

RT: 4.489 min Scan# 51

Delta R.T. -0.000 min

Lab File: VX028431.D


Acq: 29 Apr 2022 18:09

Instrument :

MSVOA_X

ClientSampleId :

MWBR3-B-117-137-042922

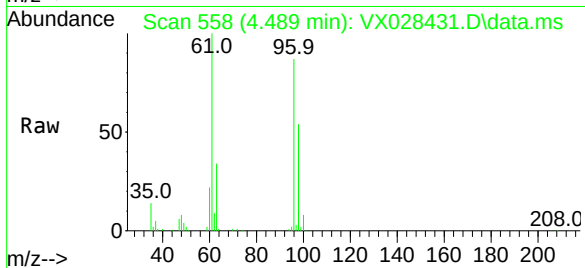




Tgt Ion: 96 Resp: 129482

Ion Ratio Lower Upper

96 100

61 115.1 0.0 283.8

98 65.0 0.0 129.8

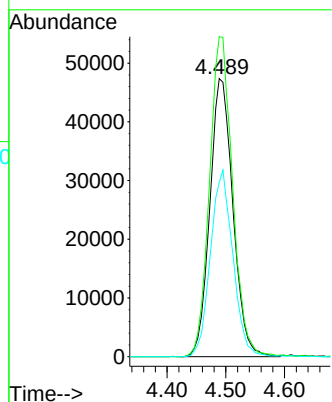

#29

Tetrahydrofuran

Concen: 0.218 ug/l

RT: 5.025 min Scan# 646

Delta R.T. 0.018 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09




Tgt Ion: 42 Resp: 429


Ion Ratio Lower Upper

42 100

72 6.3 44.1 66.1#

71 23.8 40.5 60.7#


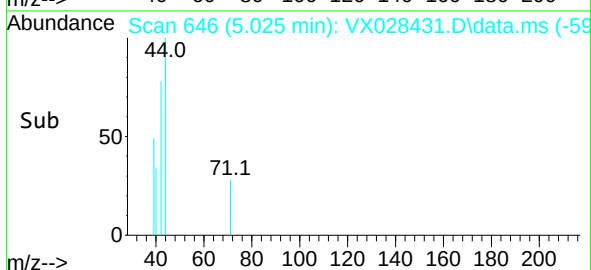

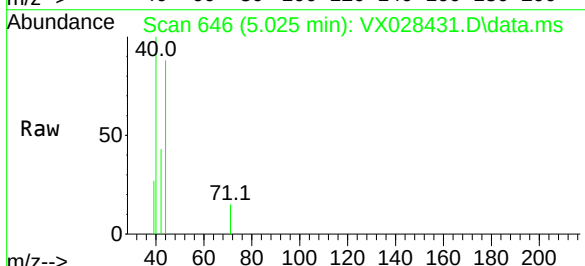




#30
Chloroform
Concen: 0.316 ug/l
RT: 5.092 min Scan# 61
Delta R.T. -0.007 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 83 Resp: 2567
Ion Ratio Lower Upper
83 100
85 71.2 52.7 79.1

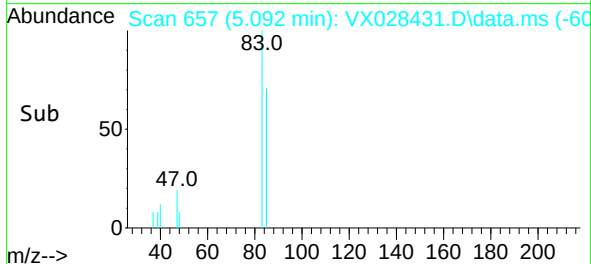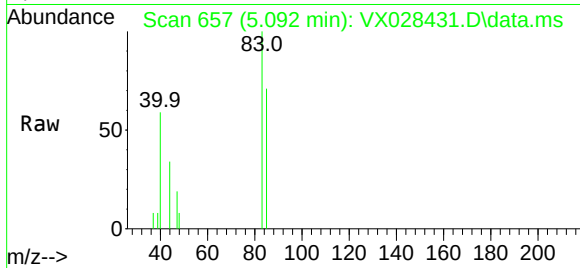

#31
Cyclohexane
Concen: 1.244 ug/l
RT: 5.556 min Scan# 733
Delta R.T. 0.086 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 56 Resp: 7710
Ion Ratio Lower Upper
56 100
69 174.2 26.7 40.1#
84 146.4 77.2 115.8#

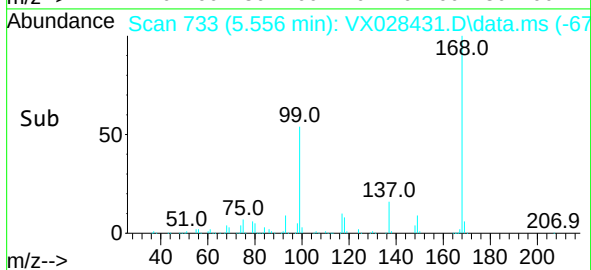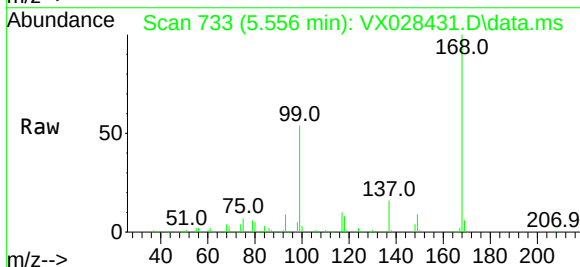



#33

1,2-Dichloroethane-d4

Concen: 55.486 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09

Instrument :

MSVOA_X

ClientSampleId :





MWBR3-B-117-137-042922

Tgt Ion: 65 Resp: 282201

Ion Ratio Lower Upper

65 100

67 51.6 0.0 107.4

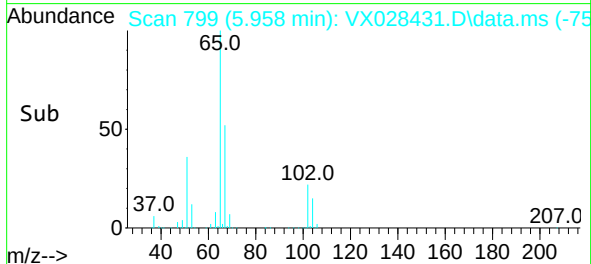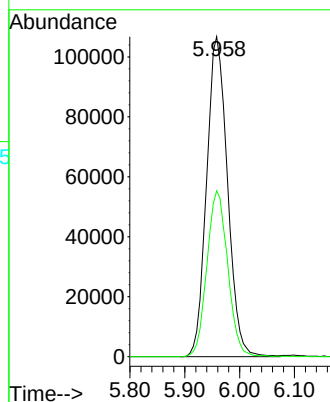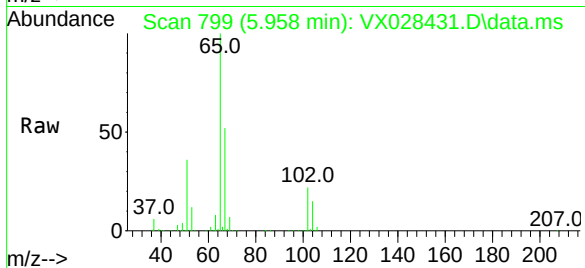

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09




Tgt Ion: 114 Resp: 674233


Ion Ratio Lower Upper

114 100

63 18.0 0.0 36.8

88 15.0 0.0 32.4

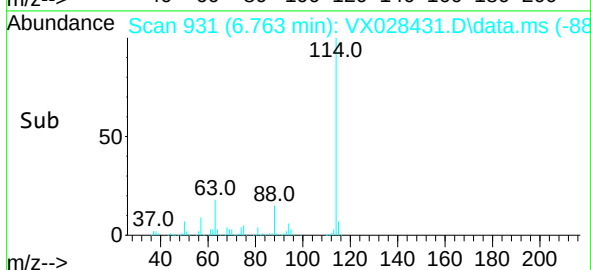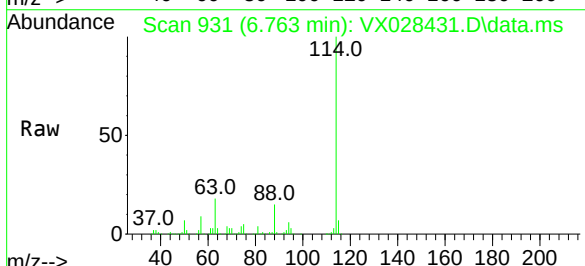

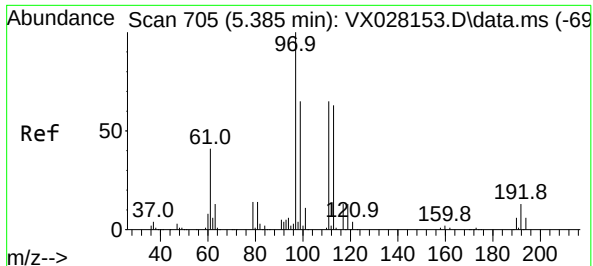

#35

Dibromofluoromethane

Concen: 53.743 ug/l

RT: 5.391 min Scan# 705

Delta R.T. 0.006 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09

Instrument :

MSVOA_X

ClientSampleId :

MWBR3-B-117-137-042922





Tgt Ion:113 Resp: 254115

Ion Ratio Lower Upper

113 100

111 102.9 82.8 124.2

192 20.0 16.9 25.3

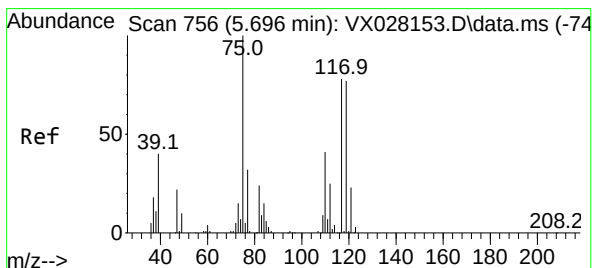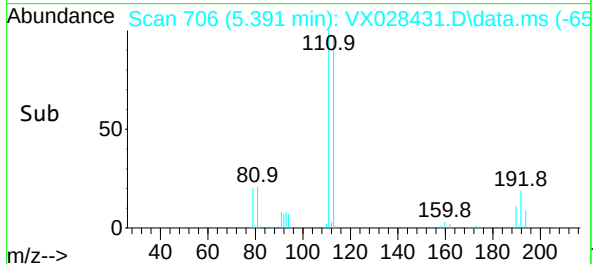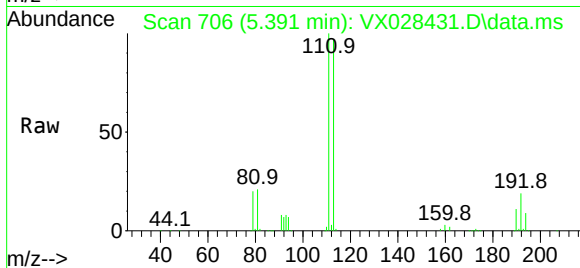

#36

1,1-Dichloropropene

Concen: 4.594 ug/l

RT: 5.556 min Scan# 733

Delta R.T. -0.140 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09




Tgt Ion: 75 Resp: 28336


Ion Ratio Lower Upper

75 100

110 9.9 18.3 54.8#

77 0.0 24.8 37.2#


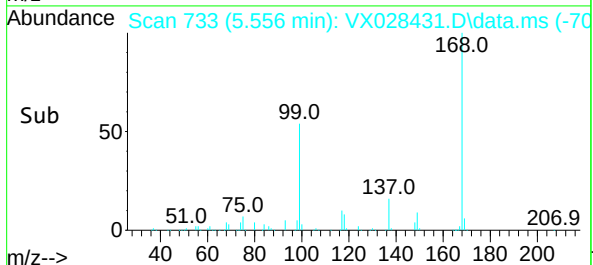
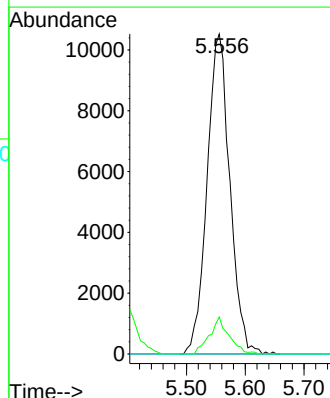
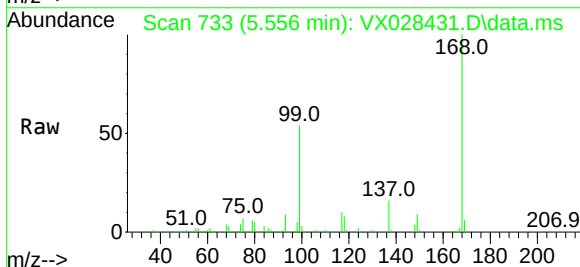




#38
Carbon Tetrachloride
Concen: 5.775 ug/l
RT: 5.556 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion:117 Resp: 40212
Ion Ratio Lower Upper
117 100
119 5.3 77.3 115.9#
121 0.0 24.2 36.2#

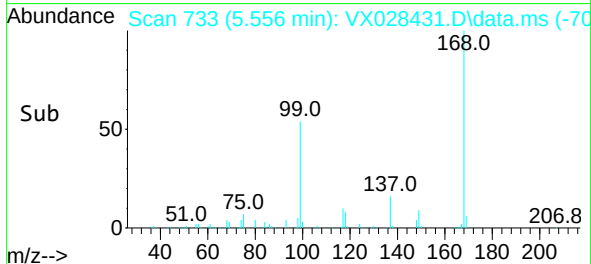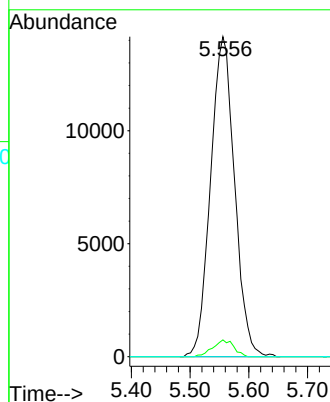

#39
Methylcyclohexane
Concen: 1.158 ug/l
RT: 7.129 min Scan# 991
Delta R.T. -0.256 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 83 Resp: 9009
Ion Ratio Lower Upper
83 100
55 0.0 54.6 81.8#
98 195.8 37.4 56.2#

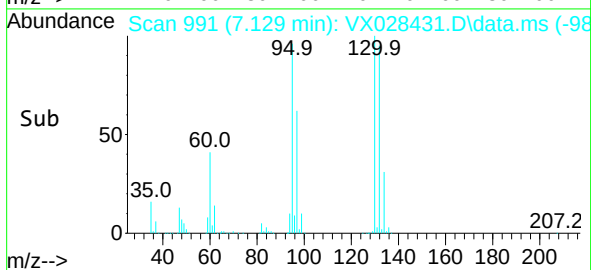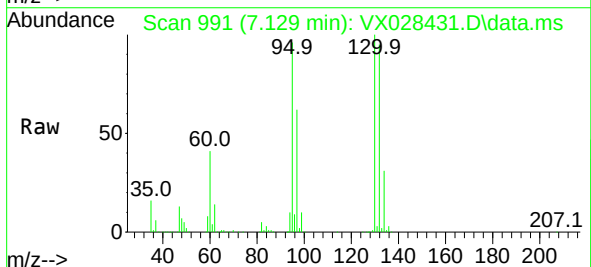



#42

1,2-Dichloroethane

Concen: 2.902 ug/l

RT: 6.086 min Scan# 81

Delta R.T. -0.006 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09

Instrument :

MSVOA_X

ClientSampleId :





MWBR3-B-117-137-042922

Tgt Ion: 62 Resp: 19449

Ion Ratio Lower Upper

62 100

98 10.2 0.0 20.4

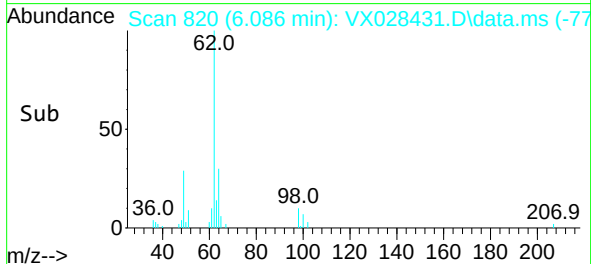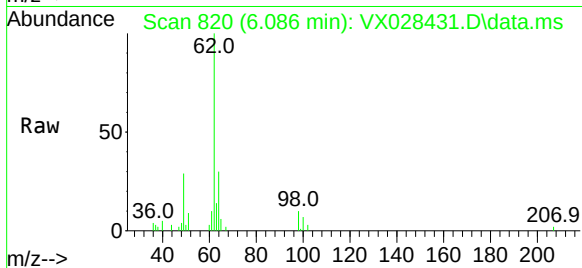

#44

Trichloroethene

Concen: 155.010 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.000 min

Lab File: VX028431.D




Acq: 29 Apr 2022 18:09


Tgt Ion:130 Resp: 811557

Ion Ratio Lower Upper

130 100

95 95.7 0.0 188.8

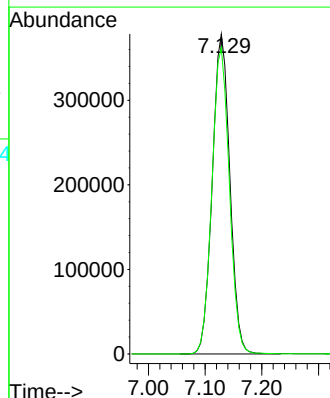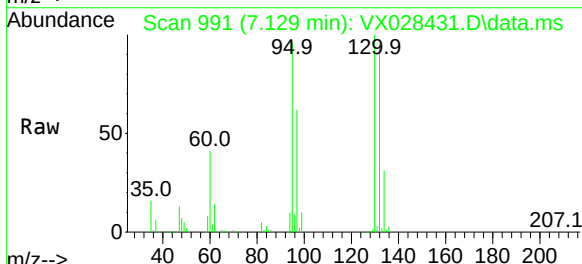

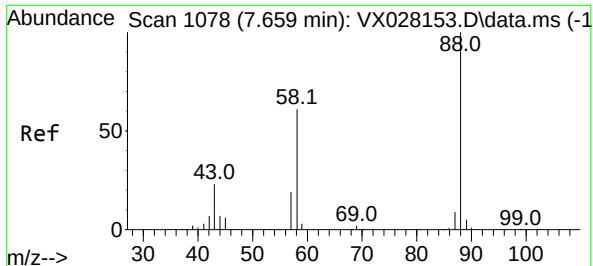

#49

1,4-Dioxane

Concen: 20.112 ug/l

RT: 7.671 min Scan# 1080

Delta R.T. 0.012 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09





Instrument :

MSVOA_X

ClientSampleId :

MWBR3-B-117-137-042922

Tgt Ion:	88	Resp:	2516
Ion	Ratio	Lower	Upper
88	100		
43	26.8	21.9	32.9
58	68.4	53.7	80.5

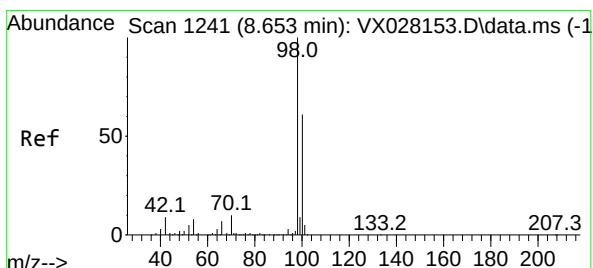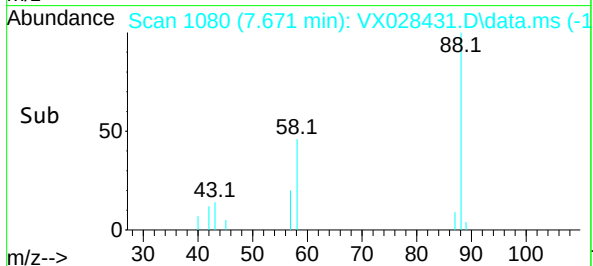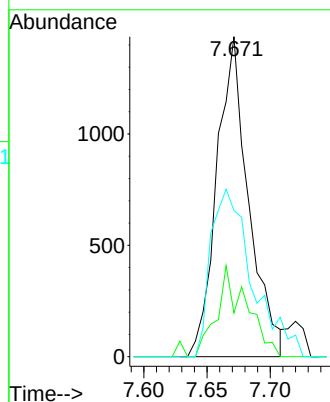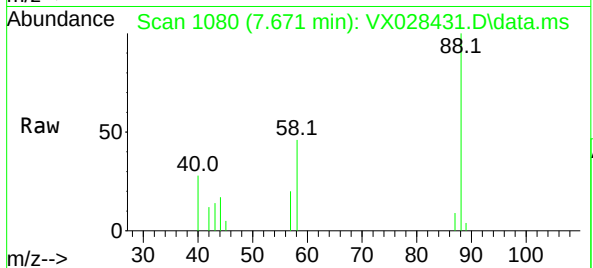

#50

Toluene-d8

Concen: 52.171 ug/l




RT: 8.653 min Scan# 1241


Delta R.T. -0.000 min

Lab File: VX028431.D

Acq: 29 Apr 2022 18:09

Tgt Ion:	98	Resp:	947466
Ion	Ratio	Lower	Upper
98	100		
100	65.7	52.6	78.8


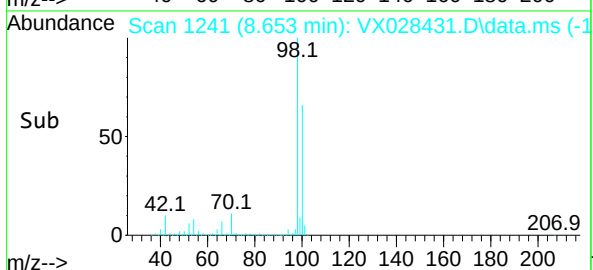

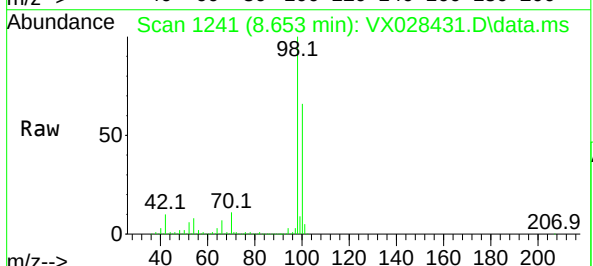


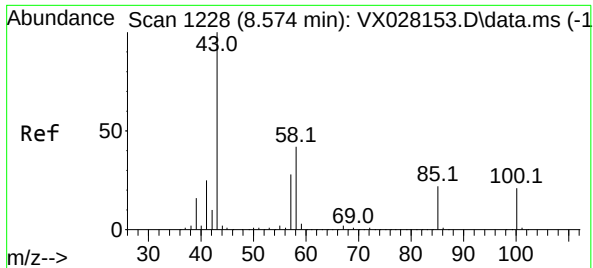

#51
4-Methyl-2-Pentanone
Concen: 0.547 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.073 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion: 43 Resp: 3577
Ion Ratio Lower Upper
43 100
58 195.9 36.1 54.1#

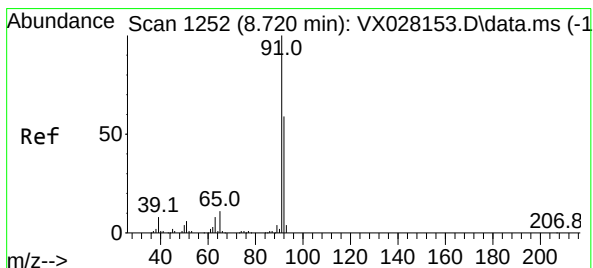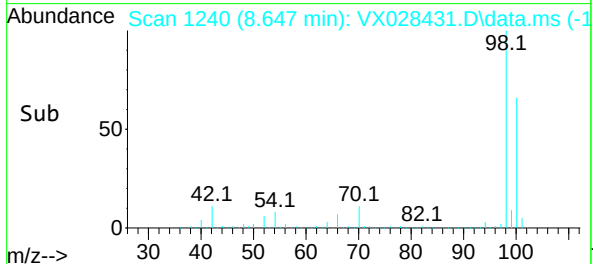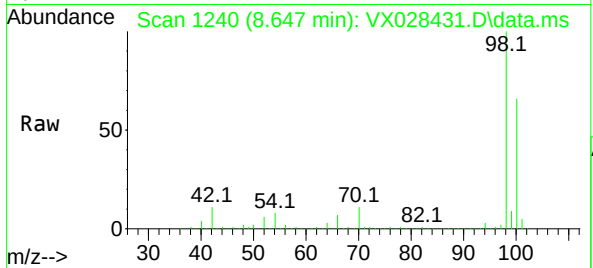

#52
Toluene
Concen: 0.299 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 92 Resp: 3745
Ion Ratio Lower Upper
92 100
91 161.4 137.5 206.3


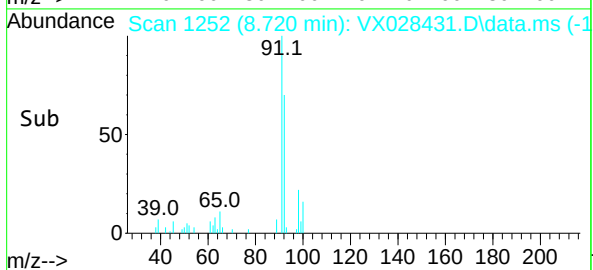

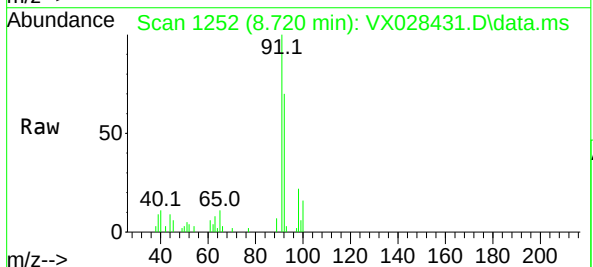


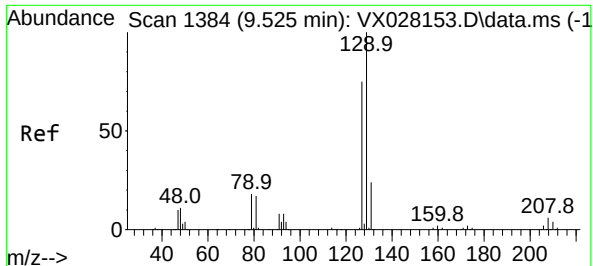

#60
Dibromochloromethane
Concen: 0.654 ug/l
RT: 9.275 min Scan# 11
Delta R.T. -0.250 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument :
MSVOA_X
ClientSampleId :
MWBR3-B-117-137-042922


Tgt Ion:129 Resp: 3635
Ion Ratio Lower Upper
129 100
127 0.0 40.3 120.8#

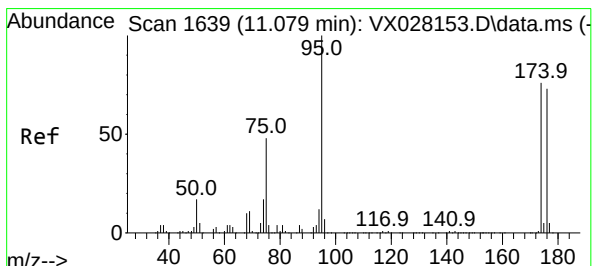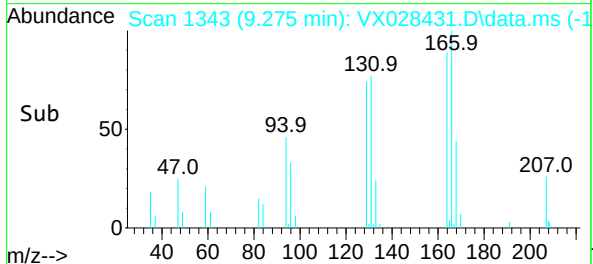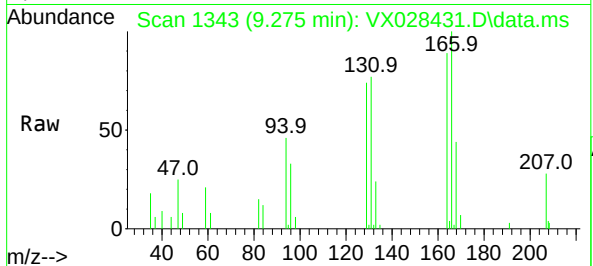

#62
4-Bromofluorobenzene
Concen: 49.606 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion: 95 Resp: 344458
Ion Ratio Lower Upper
95 100
174 84.0 0.0 163.0
176 81.0 0.0 155.0


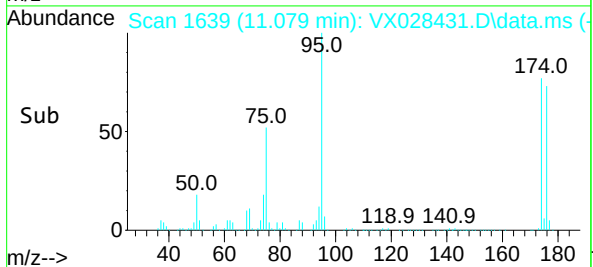

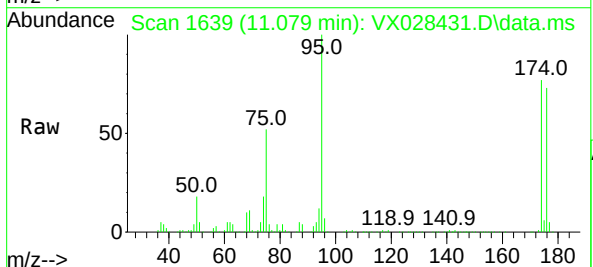




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09




Instrument : MSVOA_X
ClientSampleId : MWBR3-B-117-137-042922


Tgt Ion:117 Resp: 652767
Ion Ratio Lower Upper
117 100
82 52.6 41.8 62.8
119 32.5 24.8 37.2

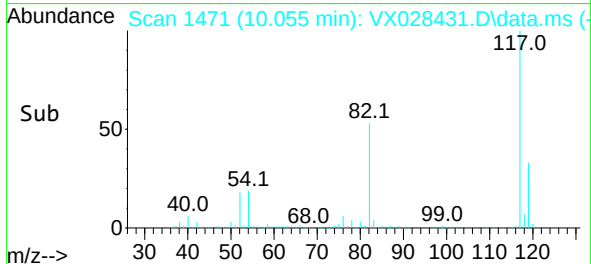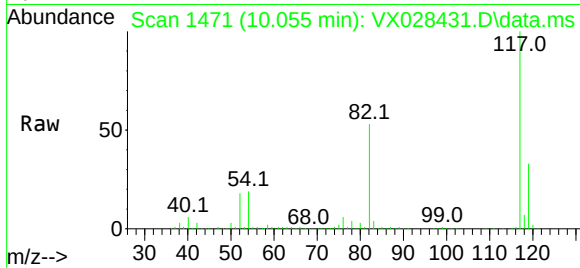

#64
Tetrachloroethene
Concen: 0.848 ug/l
RT: 9.275 min Scan# 1343
Delta R.T. -0.000 min
Lab File: VX028431.D
Acq: 29 Apr 2022 18:09

Tgt Ion:164 Resp: 4326
Ion Ratio Lower Upper
164 100
166 112.2 101.2 151.8
129 82.7 73.0 109.4
131 86.7 74.2 111.2


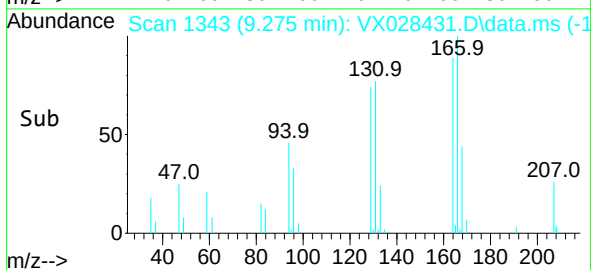

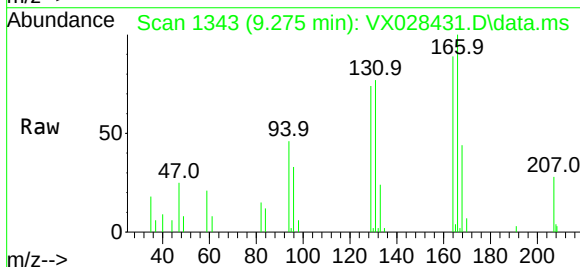




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VX028431.D
 Acq: 29 Apr 2022 18:09




Instrument :
 MSVOA_X
 ClientSampleId :
 MWBR3-B-117-137-042922


Tgt Ion:152 Resp: 311304
 Ion Ratio Lower Upper
 152 100
 115 58.3 37.5 112.7
 150 156.6 0.0 338.2

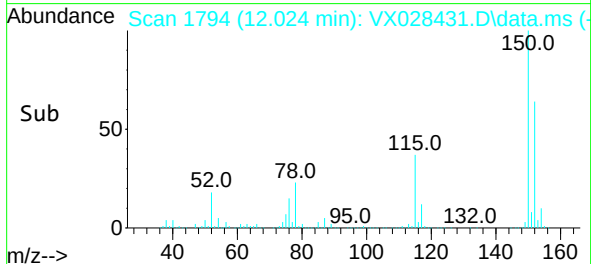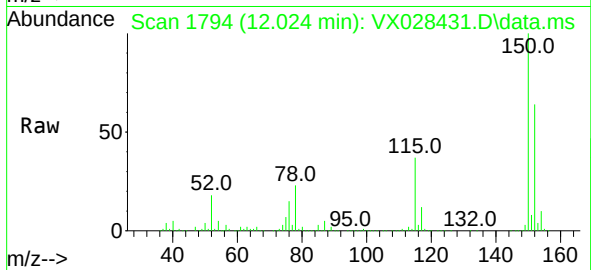

#76
 1,2,3-Trichloropropane
 Concen: 28.886 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.165 min
 Lab File: VX028431.D
 Acq: 29 Apr 2022 18:09


Tgt Ion: 75 Resp: 176975
 Ion Ratio Lower Upper
 75 100
 77 1.0 19.4 58.2#

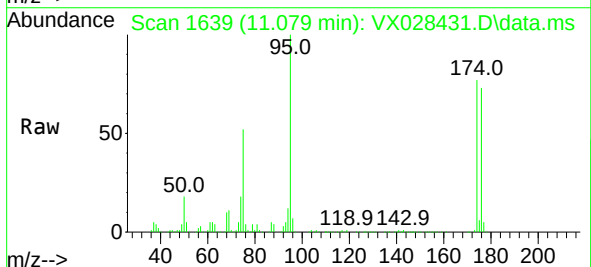



#81
 trans-1,4-Dichloro-2-butene
 Concen: 85.842 ug/l
 RT: 11.079 min Scan# 1
 Delta R.T. 0.061 min
 Lab File: VX028431.D
 Acq: 29 Apr 2022 18:09

Instrument :
 MSVOA_X
 ClientSampleId :
 MWBR3-B-117-137-042922

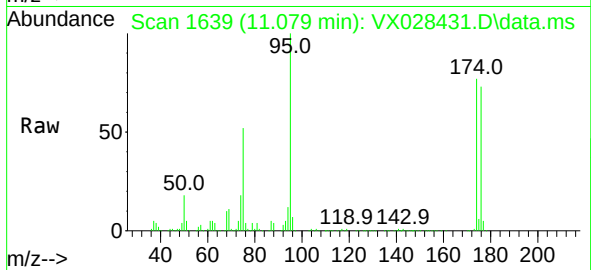

Tgt Ion: 75 Resp: 176975
 Ion Ratio Lower Upper
 75 100
 53 0.0 69.0 103.4#
 89 0.0 37.0 55.6#

