

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
 Data File : VX028434.D
 Acq On : 29 Apr 2022 19:19
 Operator : JC/MD
 Sample : N2609-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-1

Quant Time: Apr 30 09:17:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	444539	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	750754	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	752065	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	350508	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	302574	52.201	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 104.400%	
35) Dibromofluoromethane	5.391	113	280224	53.224	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 106.440%	
50) Toluene-d8	8.653	98	1055799	52.211	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 104.420%	
62) 4-Bromofluorobenzene	11.079	95	388149	50.201	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 100.400%	

Target Compounds				Qvalue		
3) Chloromethane	1.294	50	544	Below Cal	96	
5) Bromomethane	1.611	94	2004	Below Cal	85	
6) Chloroethane	1.703	64	1178	Below Cal	#	49
8) Diethyl Ether	2.130	74	77	Below Cal	#	1
10) Methyl Iodide	2.459	142	2237	5.641	ug/l	96
11) Tert butyl alcohol	2.947	59	3616	Below Cal	#	76
12) 1,1-Dichloroethene	2.325	96	907	0.265	ug/l	# 52
13) Acrolein	2.233	56	301	0.424	ug/l	# 65
15) Acrylonitrile	3.068	53	766	0.324	ug/l	86
16) Acetone	2.380	43	12554	5.727	ug/l	94
17) Carbon Disulfide	2.514	76	3477	0.378	ug/l	# 94
18) Methyl Acetate	2.703	43	1961	0.381	ug/l	# 88
20) Methylene Chloride	2.788	84	7622	1.772	ug/l	89
25) 2-Butanone	4.562	43	3775	1.100	ug/l	# 73
29) Tetrahydrofuran	5.032	42	449	0.201	ug/l	# 79
31) Cyclohexane	5.544	56	7220	1.022	ug/l	# 9
36) 1,1-Dichloropropene	5.550	75	31053	4.522	ug/l	# 50
38) Carbon Tetrachloride	5.556	117	43279	5.582	ug/l	# 16
43) Isopropyl Acetate	6.348	43	28168	2.484	ug/l	99
44) Trichloroethene	7.129	130	3604	0.618	ug/l	73
48) Methyl methacrylate	7.598	41	7570	1.454	ug/l	# 7
49) 1,4-Dioxane	7.805	88	381	2.735	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.549	43	104988	14.426	ug/l	# 45
54) cis-1,3-Dichloropropene	8.549	75	56441	6.666	ug/l	# 68
57) 1,3-Dichloropropane	9.482	76	34846	3.805	ug/l	# 43
59) 2-Hexanone	9.482	43	390552	69.277	ug/l	# 45
76) 1,2,3-Trichloropropane	11.079	75	190801	27.659	ug/l	# 38
81) trans-1,4-Dichloro-2-b...	11.079	75	190801	82.196	ug/l	# 15
89) n-Butylbenzene	12.335	91	3784	0.212	ug/l	97
90) Hexachloroethane	12.542	117	259	1.878	ug/l	60
93) 1,2,4-Trichlorobenzene	13.591	180	2766	0.397	ug/l	95
94) Hexachlorobutadiene	13.725	225	2873	0.924	ug/l	93
95) Naphthalene	13.780	128	7166	0.309	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	2880	0.421	ug/l	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
Data File : VX028434.D
Acq On : 29 Apr 2022 19:19
Operator : JC/MD
Sample : N2609-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
WC-1


Quant Time: Apr 30 09:17:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Quant Time: Apr 30 09:17:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




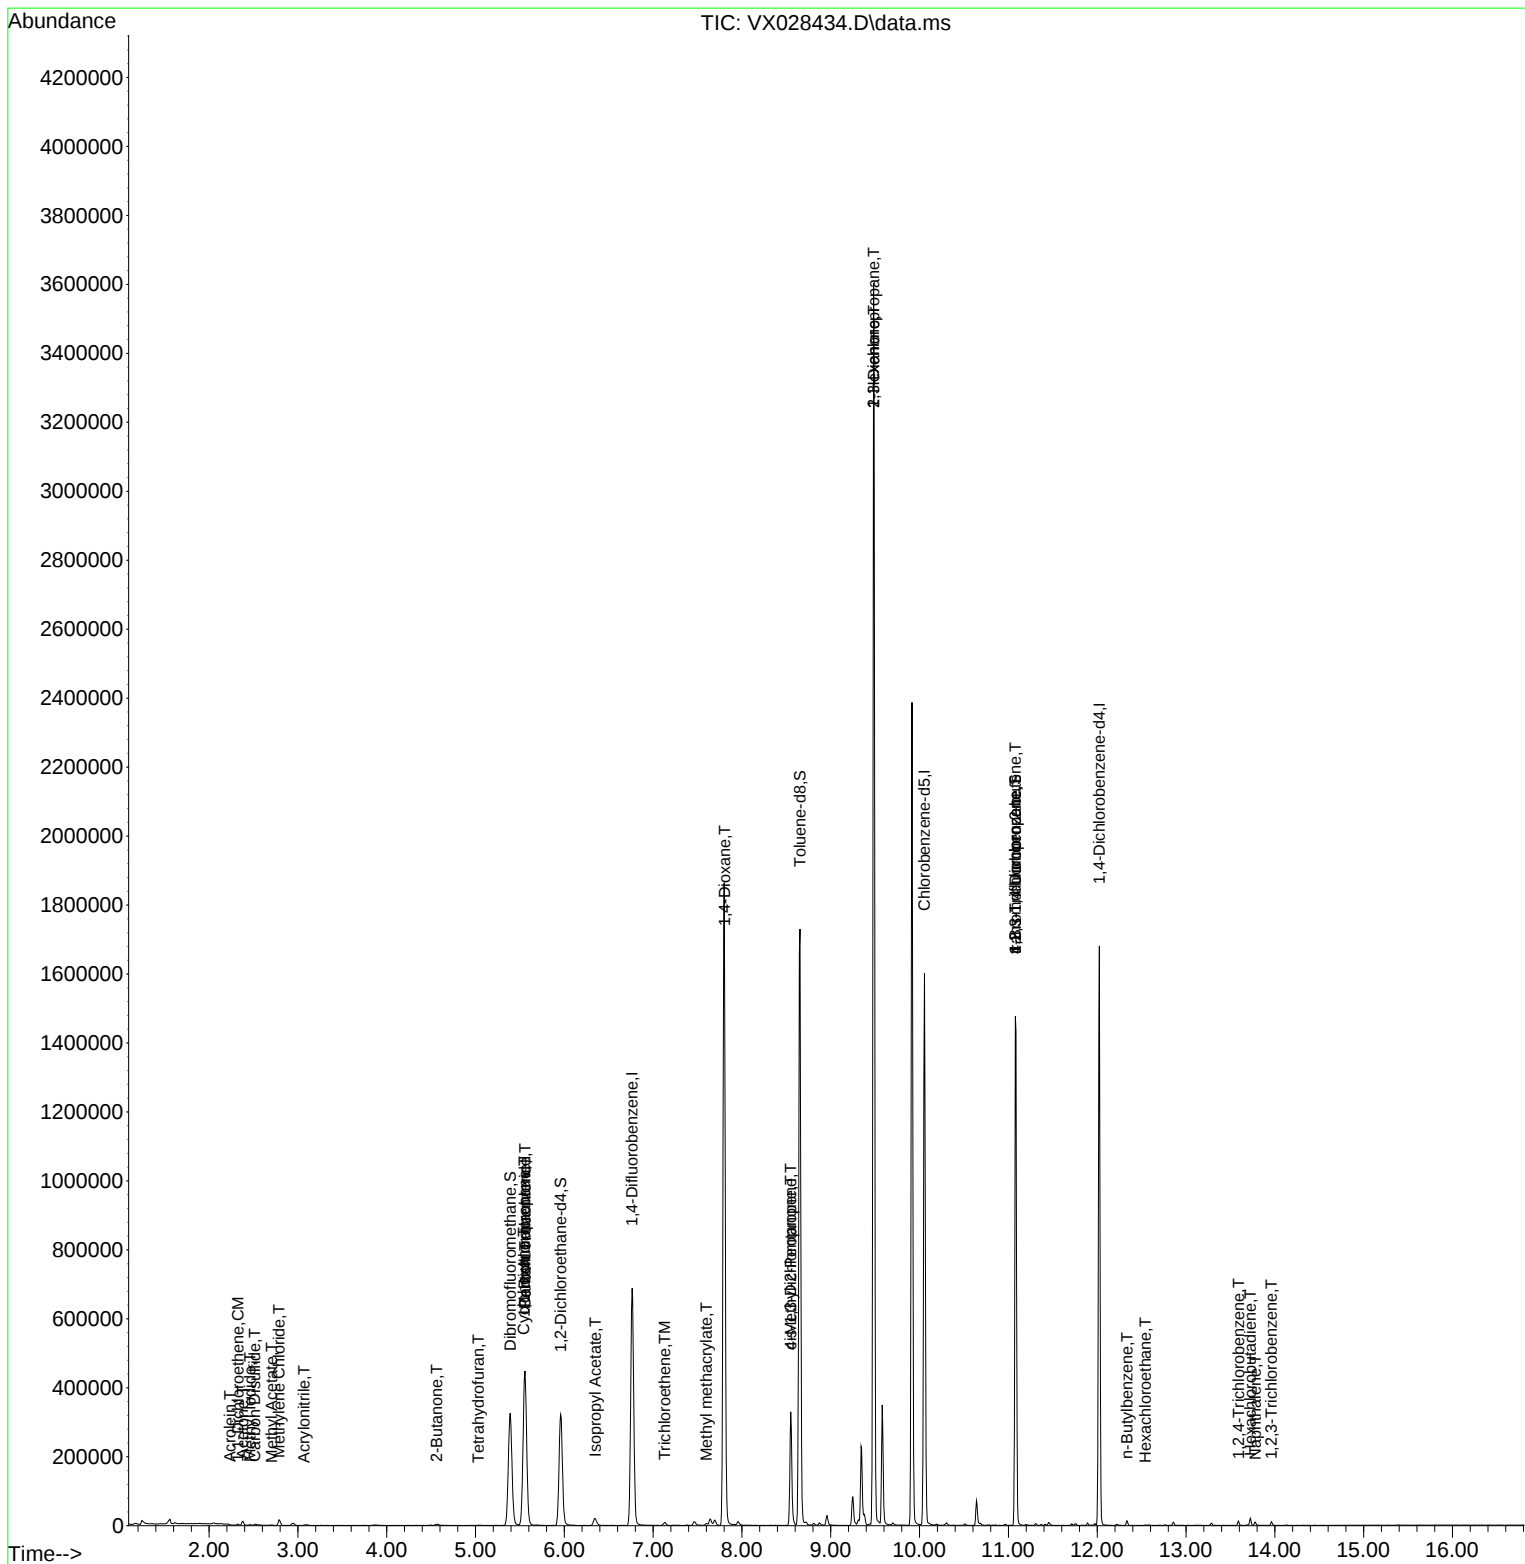




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1

Tgt Ion:168 Resp: 444539
Ion Ratio Lower Upper
168 100
99 53.2 41.7 62.5



#3
Chloromethane
Concen: Below Cal
RT: 1.294 min Scan# 34
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 50 Resp: 544
Ion Ratio Lower Upper
50 100
52 35.2 26.4 39.6









#5
Bromomethane
Concen: Below Cal
RT: 1.611 min Scan# 80
Delta R.T. 0.012 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 94 Resp: 2004
Ion Ratio Lower Upper
94 100
96 79.9 75.3 112.9

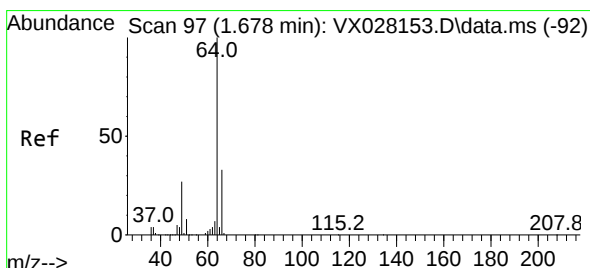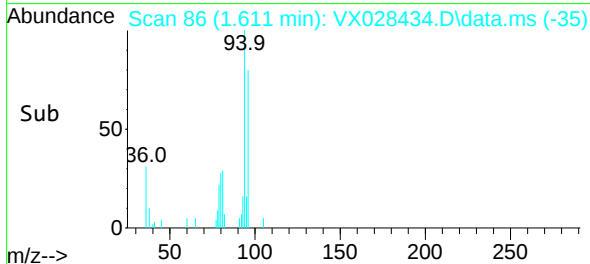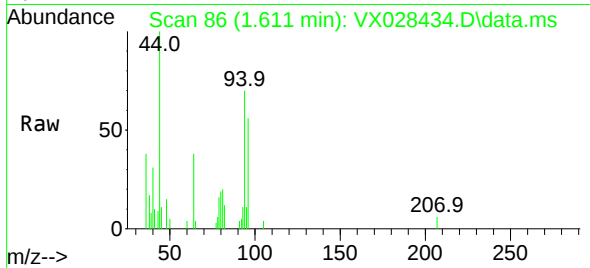

#6
Chloroethane
Concen: Below Cal
RT: 1.703 min Scan# 101
Delta R.T. 0.025 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19


Tgt Ion: 64 Resp: 1178
Ion Ratio Lower Upper
64 100
66 3.1 25.3 37.9

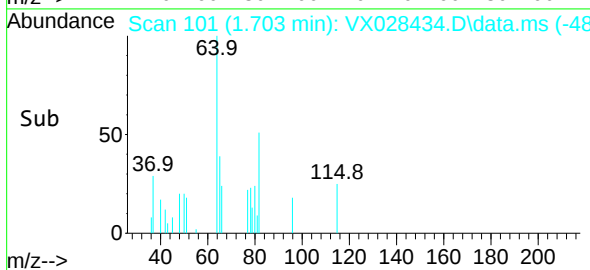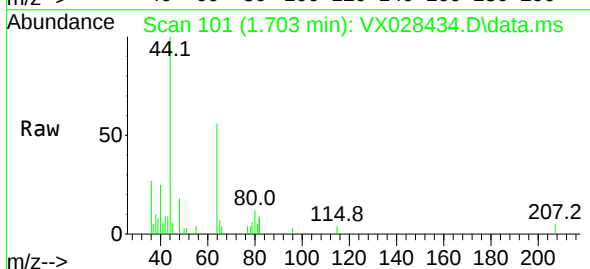






#8
Diethyl Ether
Concen: Below Cal
RT: 2.130 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Instrument :
MSVOA_X
ClientSampleId :
WC-1



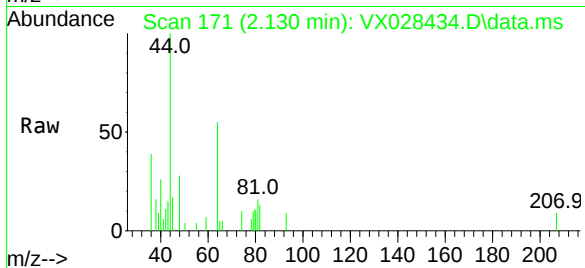



Tgt Ion: 74 Resp: 77
Ion Ratio Lower Upper
74 100
45 481.8 42.0 126.0#



#10
Methyl Iodide
Concen: 5.641 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 142 Resp: 2237
Ion Ratio Lower Upper
142 100
127 45.5 33.9 50.9
141 14.3 11.4 17.2

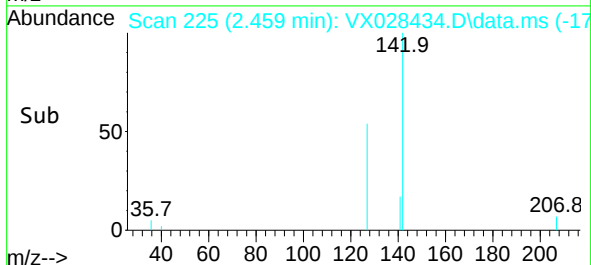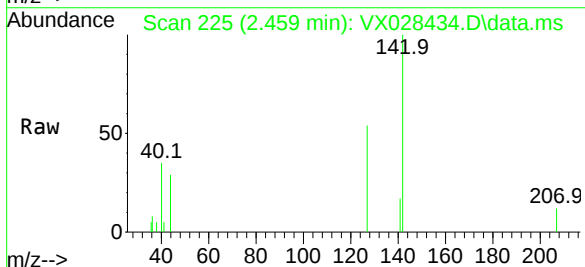

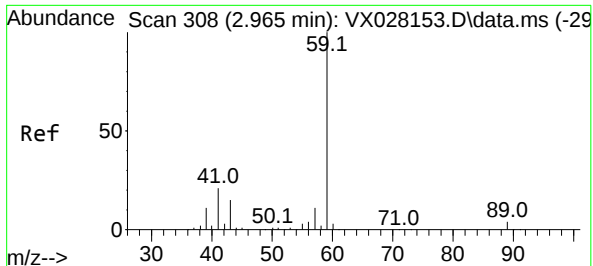

#11

Tert butyl alcohol

Concen: Below Cal

RT: 2.947 min Scan# 30

Delta R.T. -0.018 min

Lab File: VX028434.D

Acq: 29 Apr 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :





WC-1

Tgt Ion: 59 Resp: 3616

Ion Ratio Lower Upper

59 100

57 1.4 8.3 12.5#

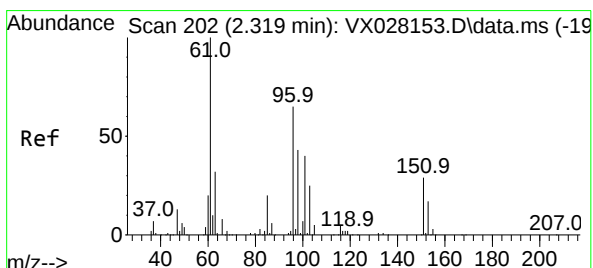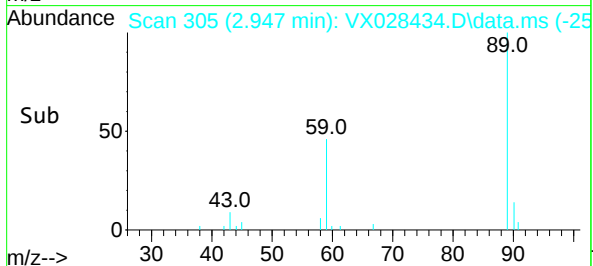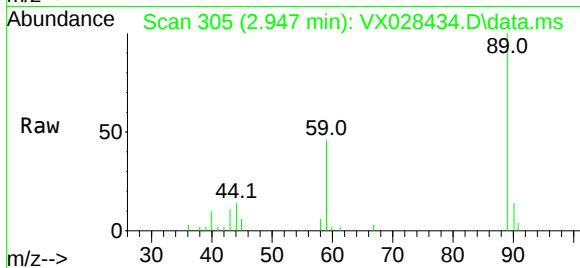

#12

1,1-Dichloroethene

Concen: 0.265 ug/l

RT: 2.325 min Scan# 203

Delta R.T. 0.006 min

Lab File: VX028434.D

Acq: 29 Apr 2022 19:19




Tgt Ion: 96 Resp: 907


Ion Ratio Lower Upper

96 100

61 77.0 124.6 187.0#

98 51.6 51.0 76.4


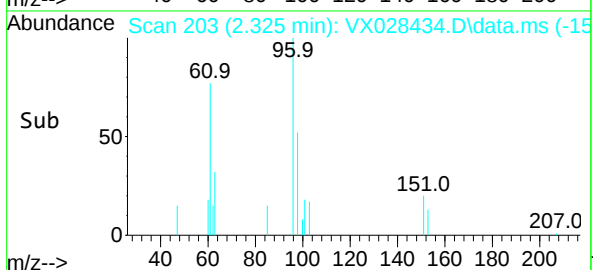

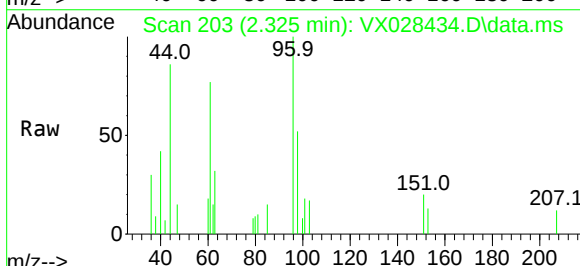




#13
Acrolein
Concen: 0.424 ug/l
RT: 2.233 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 56 Resp: 301
Ion Ratio Lower Upper
56 100
55 97.0 55.0 82.6#

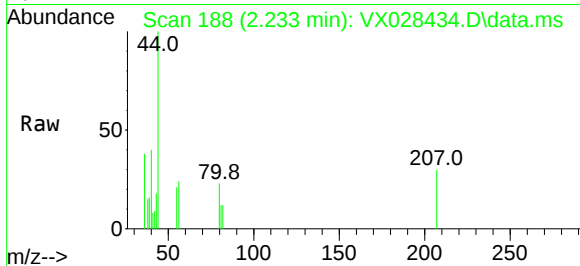

#15
Acrylonitrile
Concen: 0.324 ug/l
RT: 3.068 min Scan# 325
Delta R.T. 0.006 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 53 Resp: 766
Ion Ratio Lower Upper
53 100
52 97.3 65.7 98.5
51 31.2 28.4 42.6




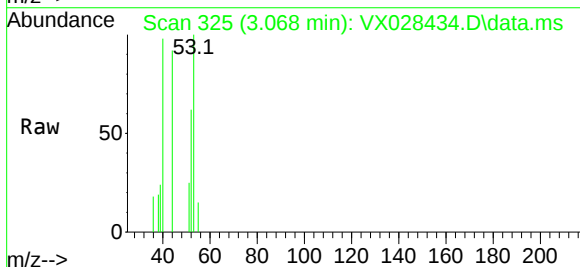


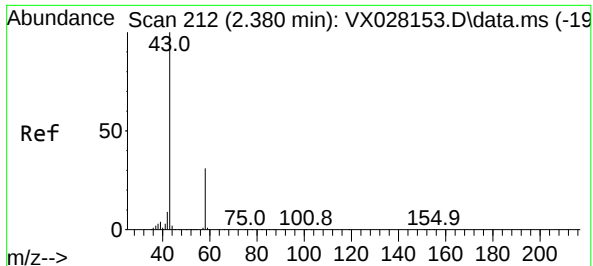

#16
Acetone
Concen: 5.727 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 43 Resp: 12554
Ion Ratio Lower Upper
43 100
58 32.7 28.8 43.2

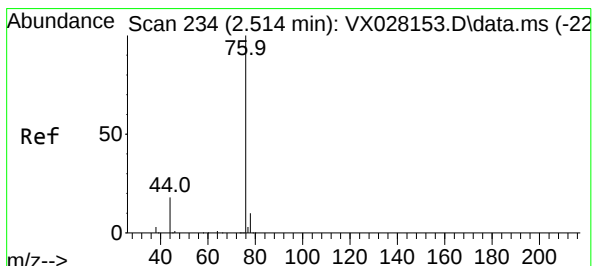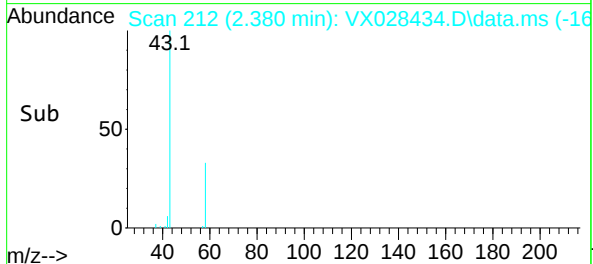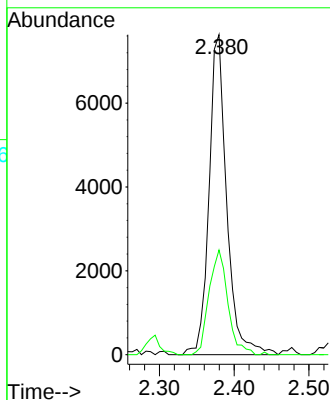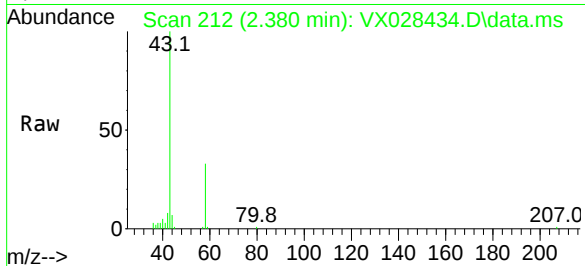

#17
Carbon Disulfide
Concen: 0.378 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 76 Resp: 3477
Ion Ratio Lower Upper
76 100
78 6.9 7.2 10.8#


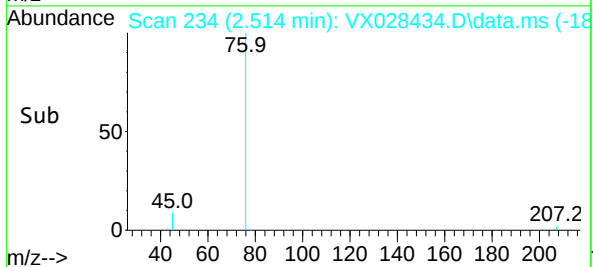
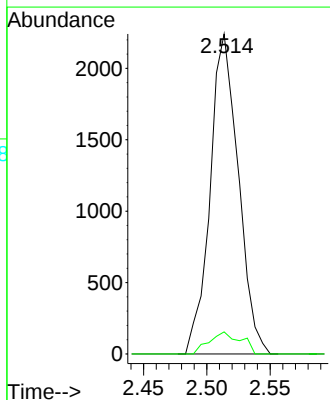
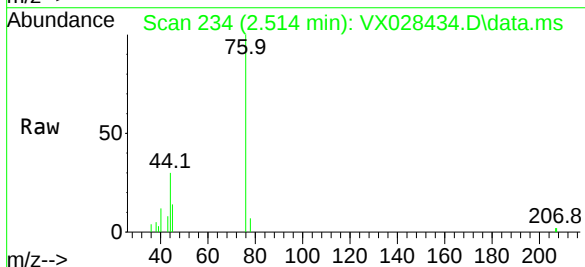




#18
Methyl Acetate
Concen: 0.381 ug/l
RT: 2.703 min Scan# 265
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 43 Resp: 1961
Ion Ratio Lower Upper
43 100
74 22.4 22.8 34.2#

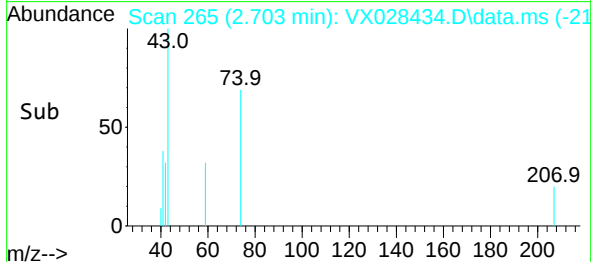

#20
Methylene Chloride
Concen: 1.772 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 84 Resp: 7622
Ion Ratio Lower Upper
84 100
49 119.3 85.5 128.3
51 30.7 26.6 39.8
86 74.6 51.5 77.3




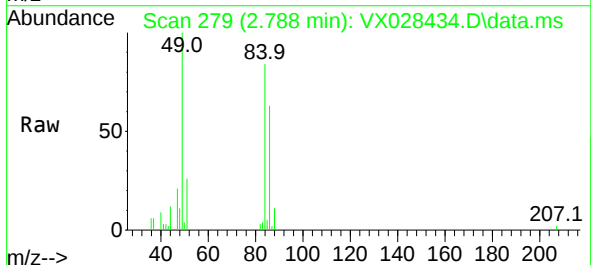




#25
2-Butanone
Concen: 1.100 ug/l
RT: 4.562 min Scan# 51
Delta R.T. 0.006 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 43 Resp: 3775
Ion Ratio Lower Upper
43 100
72 15.9 24.4 36.6#



#29
Tetrahydrofuran
Concen: 0.201 ug/l
RT: 5.032 min Scan# 647
Delta R.T. 0.025 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19


Tgt Ion: 42 Resp: 449
Ion Ratio Lower Upper
42 100
72 71.9 44.1 66.1#
71 38.3 40.5 60.7#

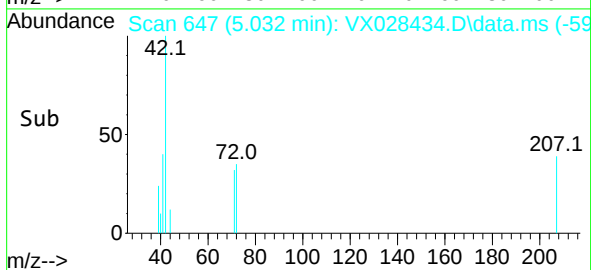



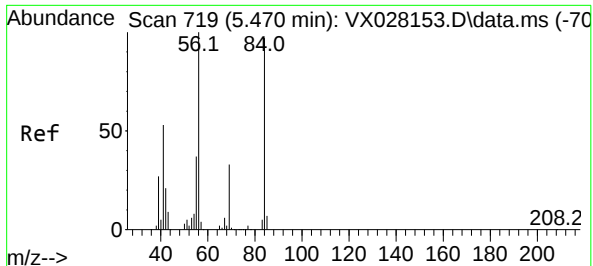


#31
Cyclohexane
Concen: 1.022 ug/l
RT: 5.544 min Scan# 719
Delta R.T. 0.074 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19


Instrument :
MSVOA_X
ClientSampleId :
WC-1

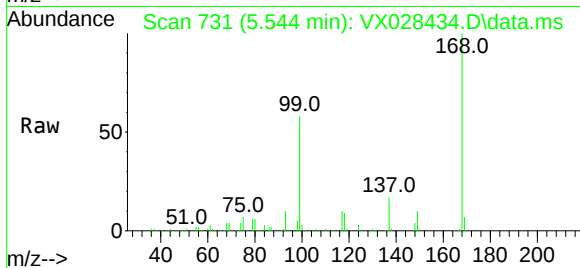



Tgt Ion: 56 Resp: 7220
Ion Ratio Lower Upper
56 100
69 172.4 26.7 40.1#
84 133.5 77.2 115.8#

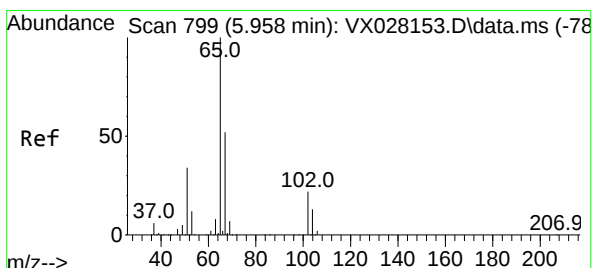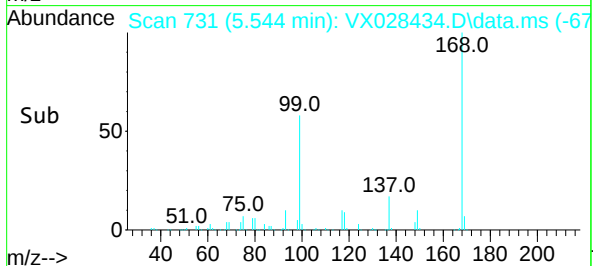


#33
1,2-Dichloroethane-d4
Concen: 52.201 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

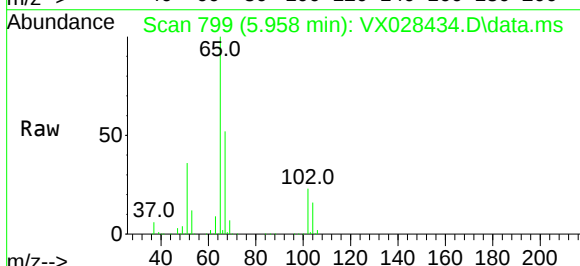

Tgt Ion: 65 Resp: 302574
Ion Ratio Lower Upper
65 100
67 52.7 0.0 107.4




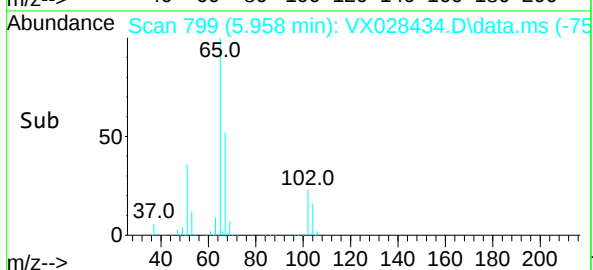




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion:114 Resp: 750754
Ion Ratio Lower Upper
114 100
63 17.1 0.0 36.8
88 15.1 0.0 32.4

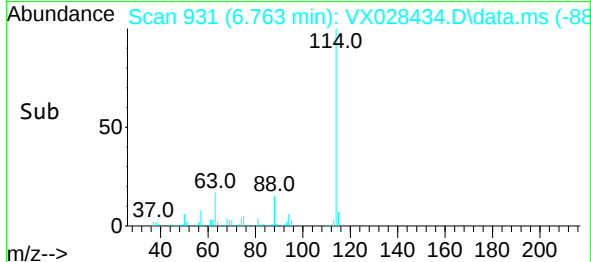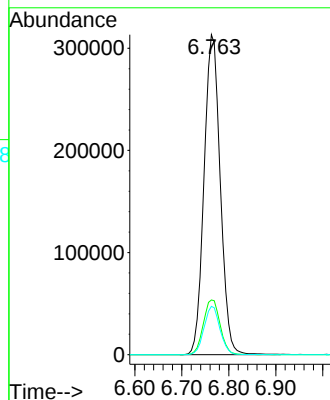

#35
Dibromofluoromethane
Concen: 53.224 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion:113 Resp: 280224
Ion Ratio Lower Upper
113 100
111 102.7 82.8 124.2
192 20.4 16.9 25.3



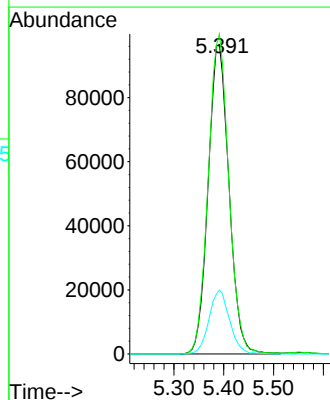
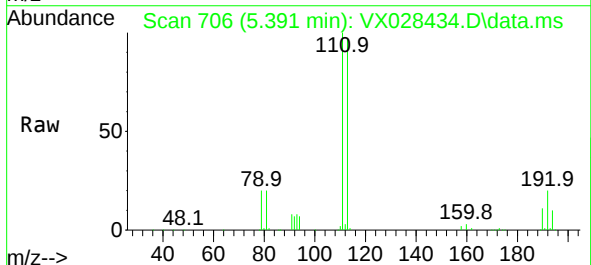




#36
1,1-Dichloropropene
Concen: 4.522 ug/l
RT: 5.550 min Scan# 710
Delta R.T. -0.146 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 75 Resp: 31053
Ion Ratio Lower Upper
75 100
110 9.6 18.3 54.8#
77 0.0 24.8 37.2#



#38
Carbon Tetrachloride
Concen: 5.582 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.128 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 117 Resp: 43279
Ion Ratio Lower Upper
117 100
119 5.6 77.3 115.9#
121 0.0 24.2 36.2#





#43

Isopropyl Acetate

Concen: 2.484 ug/l

RT: 6.348 min Scan# 863

Delta R.T. 0.012 min

Lab File: VX028434.D

Acq: 29 Apr 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :

WC-1





Tgt Ion: 43 Resp: 28168

Ion Ratio Lower Upper

43 100

61 22.7 18.5 27.7

87 15.4 13.0 19.6

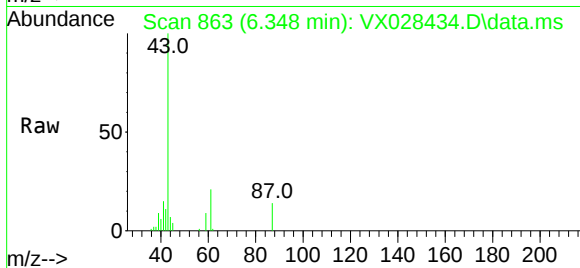

#44

Trichloroethene

Concen: 0.618 ug/l

RT: 7.129 min Scan# 991

Delta R.T. -0.000 min

Lab File: VX028434.D




Acq: 29 Apr 2022 19:19


Tgt Ion:130 Resp: 3604

Ion Ratio Lower Upper

130 100

95 68.2 0.0 188.8


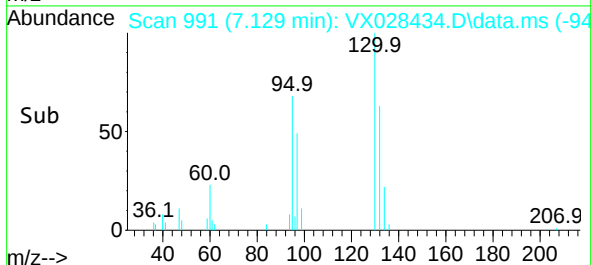
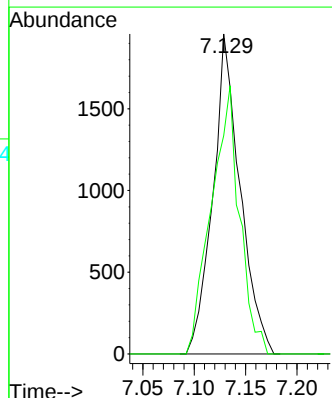
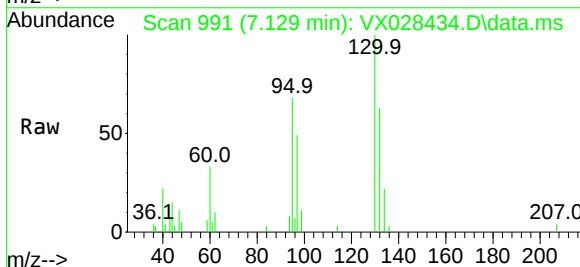




#48
Methyl methacrylate
Concen: 1.454 ug/l
RT: 7.598 min Scan# 1102
Delta R.T. -0.098 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 41 Resp: 7570
Ion Ratio Lower Upper
41 100
69 0.0 82.5 123.7#
39 0.0 43.8 65.8#

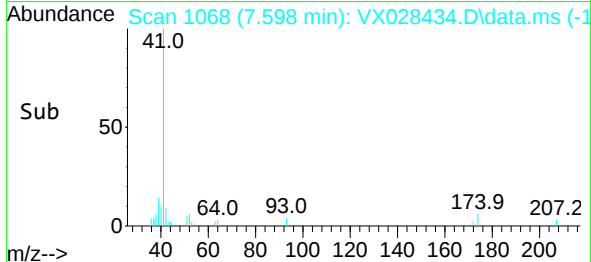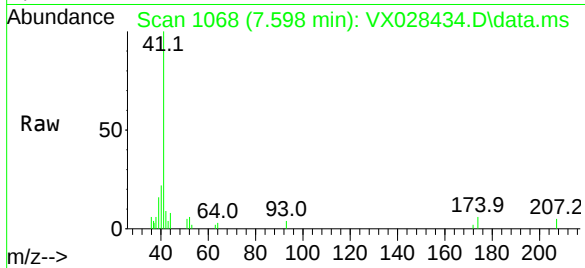

#49
1,4-Dioxane
Concen: 2.735 ug/l
RT: 7.805 min Scan# 1102
Delta R.T. 0.146 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 88 Resp: 381
Ion Ratio Lower Upper
88 100
43 425835.4 21.9 32.9#
58 2001.0 53.7 80.5#




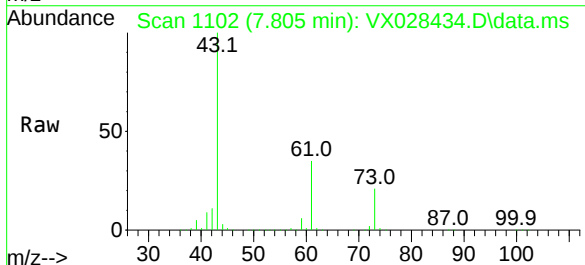




#50
Toluene-d8
Concen: 52.211 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 98 Resp: 1055799
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8

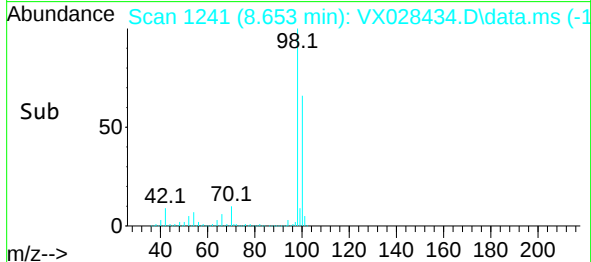

#51
4-Methyl-2-Pentanone
Concen: 14.426 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 43 Resp: 104988
Ion Ratio Lower Upper
43 100
58 8.8 36.1 54.1#




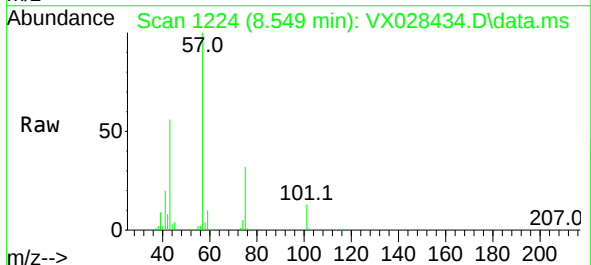


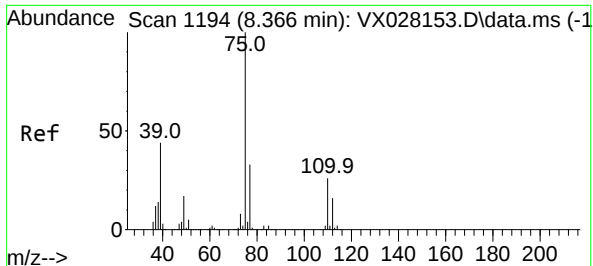

#54
 cis-1,3-Dichloropropene
 Concen: 6.666 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX028434.D
 Acq: 29 Apr 2022 19:19




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-1


Tgt Ion: 75 Resp: 56441
 Ion Ratio Lower Upper
 75 100
 77 0.5 24.8 37.2#
 39 29.5 29.6 44.4#

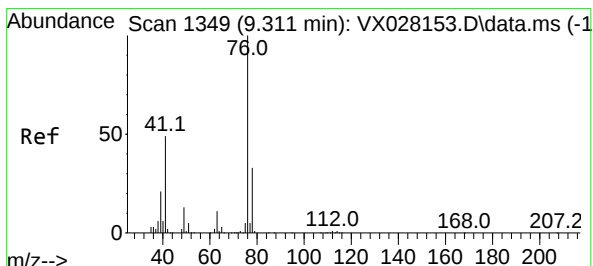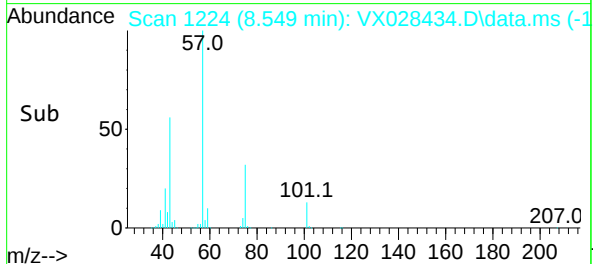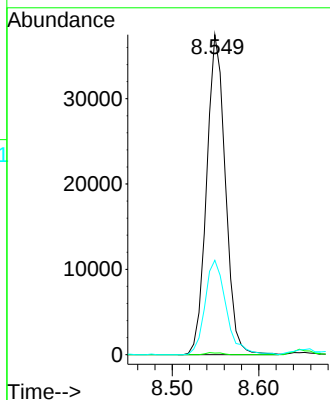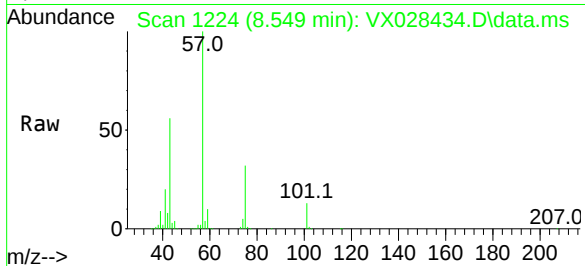

#57
 1,3-Dichloropropane
 Concen: 3.805 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.171 min
 Lab File: VX028434.D
 Acq: 29 Apr 2022 19:19

Tgt Ion: 76 Resp: 34846
 Ion Ratio Lower Upper
 76 100
 78 0.6 25.8 38.8#

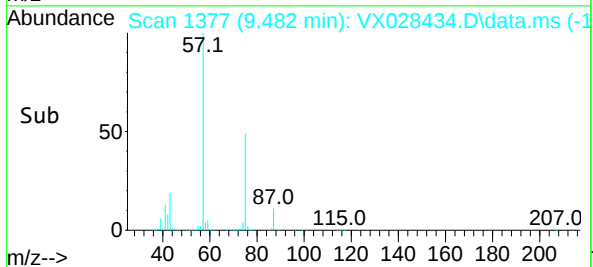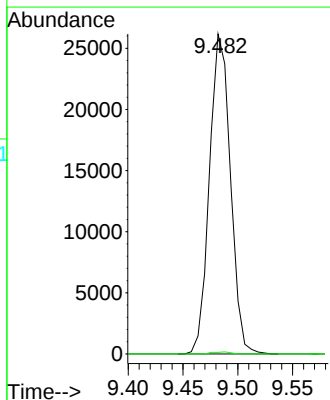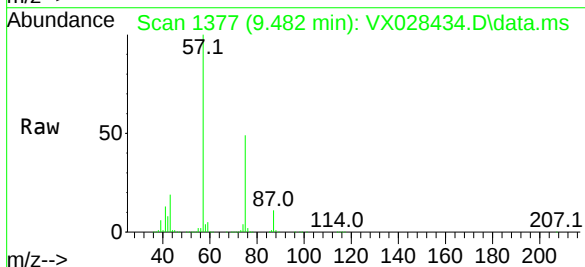



#59

2-Hexanone

Concen: 69.277 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.049 min

Lab File: VX028434.D

Acq: 29 Apr 2022 19:19

Instrument :

MSVOA_X

ClientSampleId :





WC-1

Tgt Ion: 43 Resp: 390552

Ion Ratio Lower Upper

43 100

58 20.6 31.9 95.7#

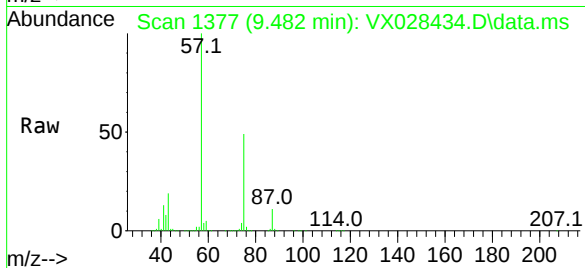

#62

4-Bromofluorobenzene

Concen: 50.201 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX028434.D

Acq: 29 Apr 2022 19:19




Tgt Ion: 95 Resp: 388149


Ion Ratio Lower Upper

95 100

174 87.3 0.0 163.0

176 84.9 0.0 155.0


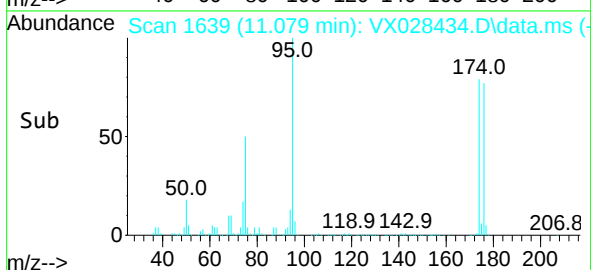

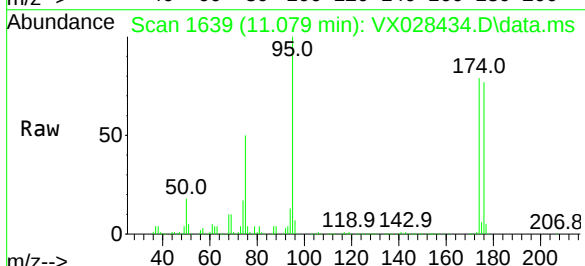




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion:117 Resp: 752065
Ion Ratio Lower Upper
117 100
82 50.8 41.8 62.8
119 31.8 24.8 37.2

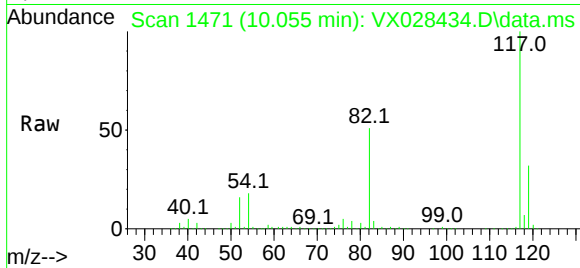

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion:152 Resp: 350508
Ion Ratio Lower Upper
152 100
115 58.1 37.5 112.7
150 158.4 0.0 338.2


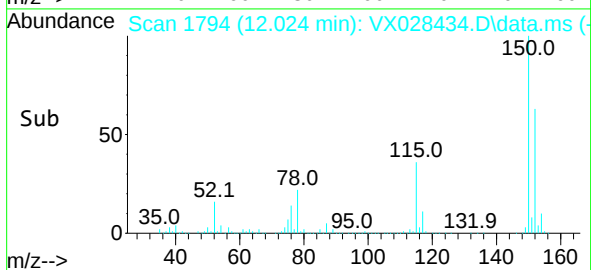

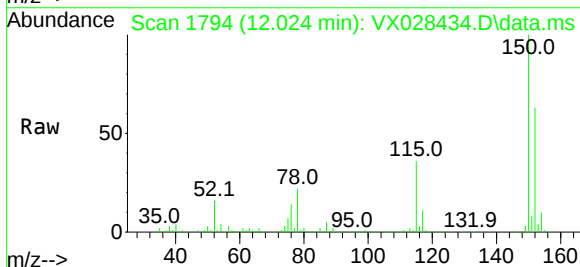


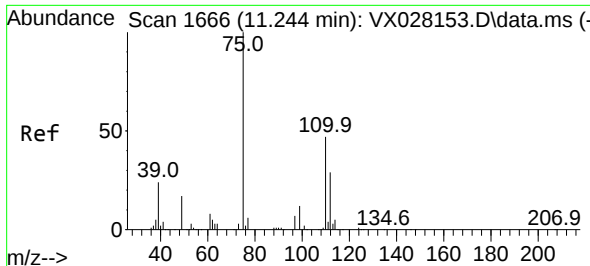

#76
1,2,3-Trichloropropane
Concen: 27.659 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.165 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion: 75 Resp: 190801
Ion Ratio Lower Upper
75 100
77 1.3 19.4 58.2#

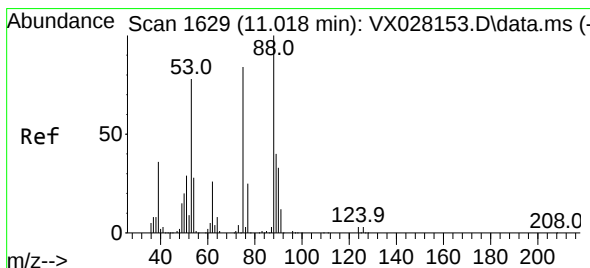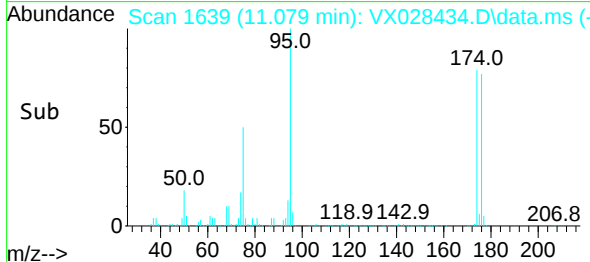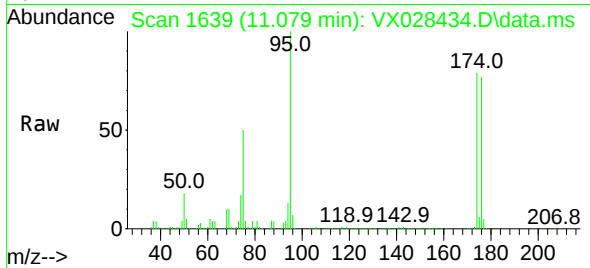

#81
trans-1,4-Dichloro-2-butene
Concen: 82.196 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion: 75 Resp: 190801
Ion Ratio Lower Upper
75 100
53 0.0 69.0 103.4#
89 0.0 37.0 55.6#


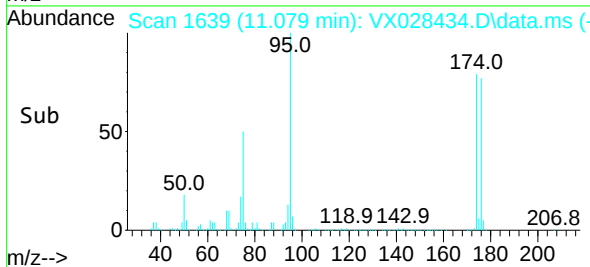

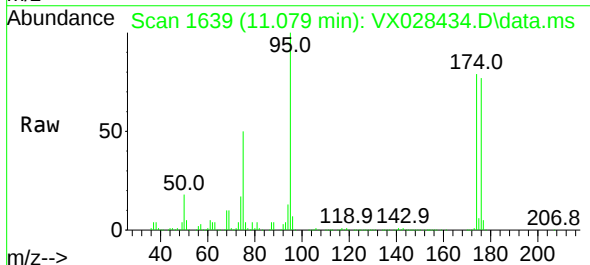




#89
n-Butylbenzene
Concen: 0.212 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19




Instrument :
MSVOA_X
ClientSampleId :
WC-1


Tgt Ion:	91	Resp:	3784
Ion	Ratio	Lower	Upper
91	100		
92	56.6	27.8	83.3
134	28.9	13.3	39.8

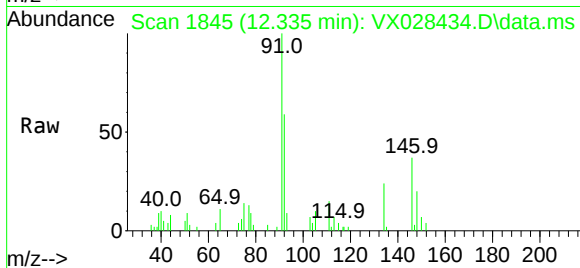

#90
Hexachloroethane
Concen: 1.878 ug/l
RT: 12.542 min Scan# 1879
Delta R.T. 0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion:	117	Resp:	259
Ion	Ratio	Lower	Upper
117	100		
201	44.0	39.5	118.5




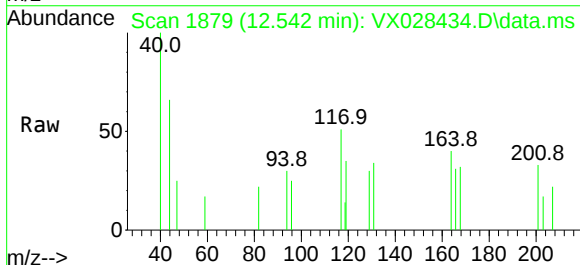


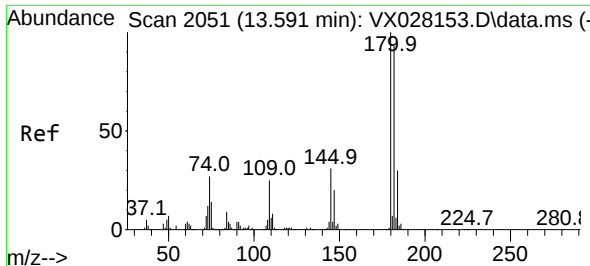

#93
 1,2,4-Trichlorobenzene
 Concen: 0.397 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. -0.000 min
 Lab File: VX028434.D
 Acq: 29 Apr 2022 19:19




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-1


Tgt Ion:180 Resp: 2766
 Ion Ratio Lower Upper
 180 100
 182 101.0 47.7 143.1
 145 32.2 15.2 45.5

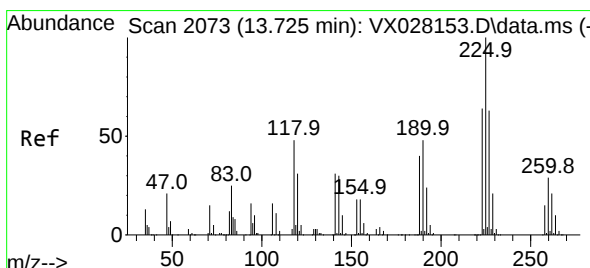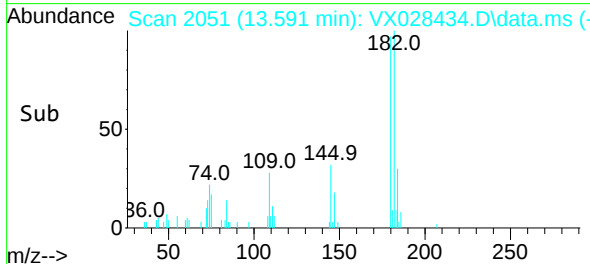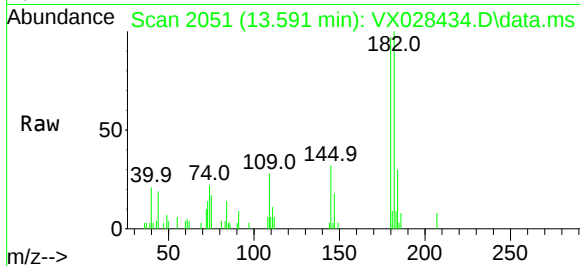

#94
 Hexachlorobutadiene
 Concen: 0.924 ug/l
 RT: 13.725 min Scan# 2073
 Delta R.T. 0.000 min
 Lab File: VX028434.D
 Acq: 29 Apr 2022 19:19

Tgt Ion:225 Resp: 2873
 Ion Ratio Lower Upper
 225 100
 223 62.6 34.2 102.5
 227 72.9 33.9 101.7


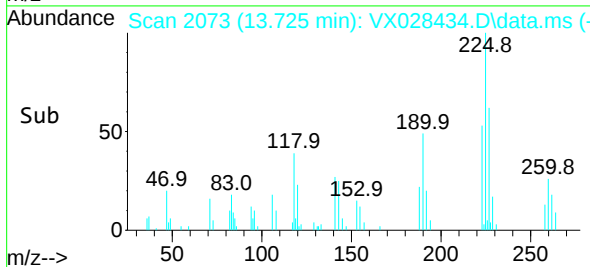

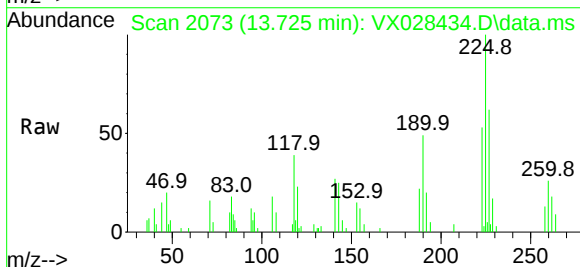


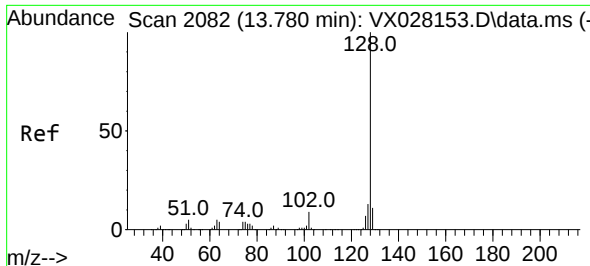

#95
Naphthalene
Concen: 0.309 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Instrument :
MSVOA_X
ClientSampleId :
WC-1

Tgt Ion:128	Resp:	7166
Ion	Ratio	Lower Upper
128	100	
127	12.3	10.2 15.4
129	10.4	8.7 13.1

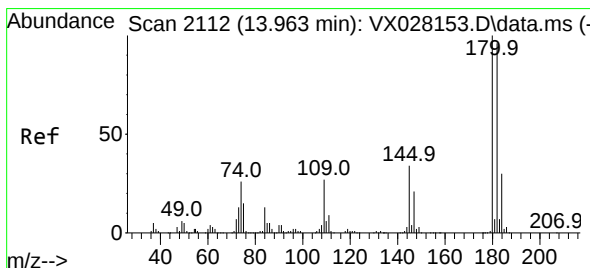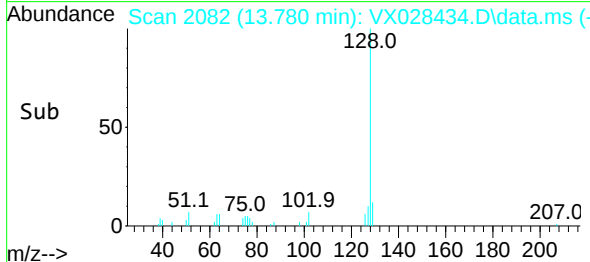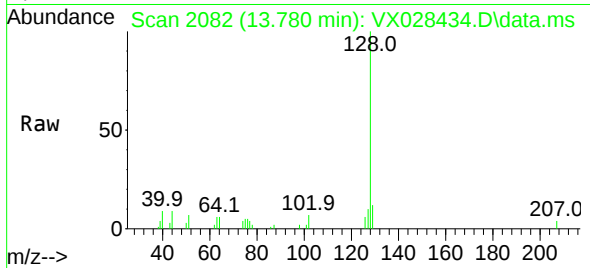

#96
1,2,3-Trichlorobenzene
Concen: 0.421 ug/l
RT: 13.963 min Scan# 2112
Delta R.T. -0.000 min
Lab File: VX028434.D
Acq: 29 Apr 2022 19:19

Tgt Ion:180	Resp:	2880
Ion	Ratio	Lower Upper
180	100	
182	92.2	50.0 149.8
145	34.4	16.2 48.5

