

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
 Data File : VX028427.D
 Acq On : 29 Apr 2022 16:36
 Operator : JC/MD
 Sample : N2640-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-042922

Quant Time: Apr 30 09:15:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	404497	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	703516	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	685316	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	320373	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	282289	53.523	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 107.040%	
35) Dibromofluoromethane	5.385	113	254768	51.638	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 103.280%	
50) Toluene-d8	8.653	98	943945	49.814	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 99.620%	
62) 4-Bromofluorobenzene	11.079	95	348339	48.077	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 96.160%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
Data File : VX028427.D
Acq On : 29 Apr 2022 16:36
Operator : JC/MD
Sample : N2640-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-042922

Quant Time: Apr 30 09:15:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




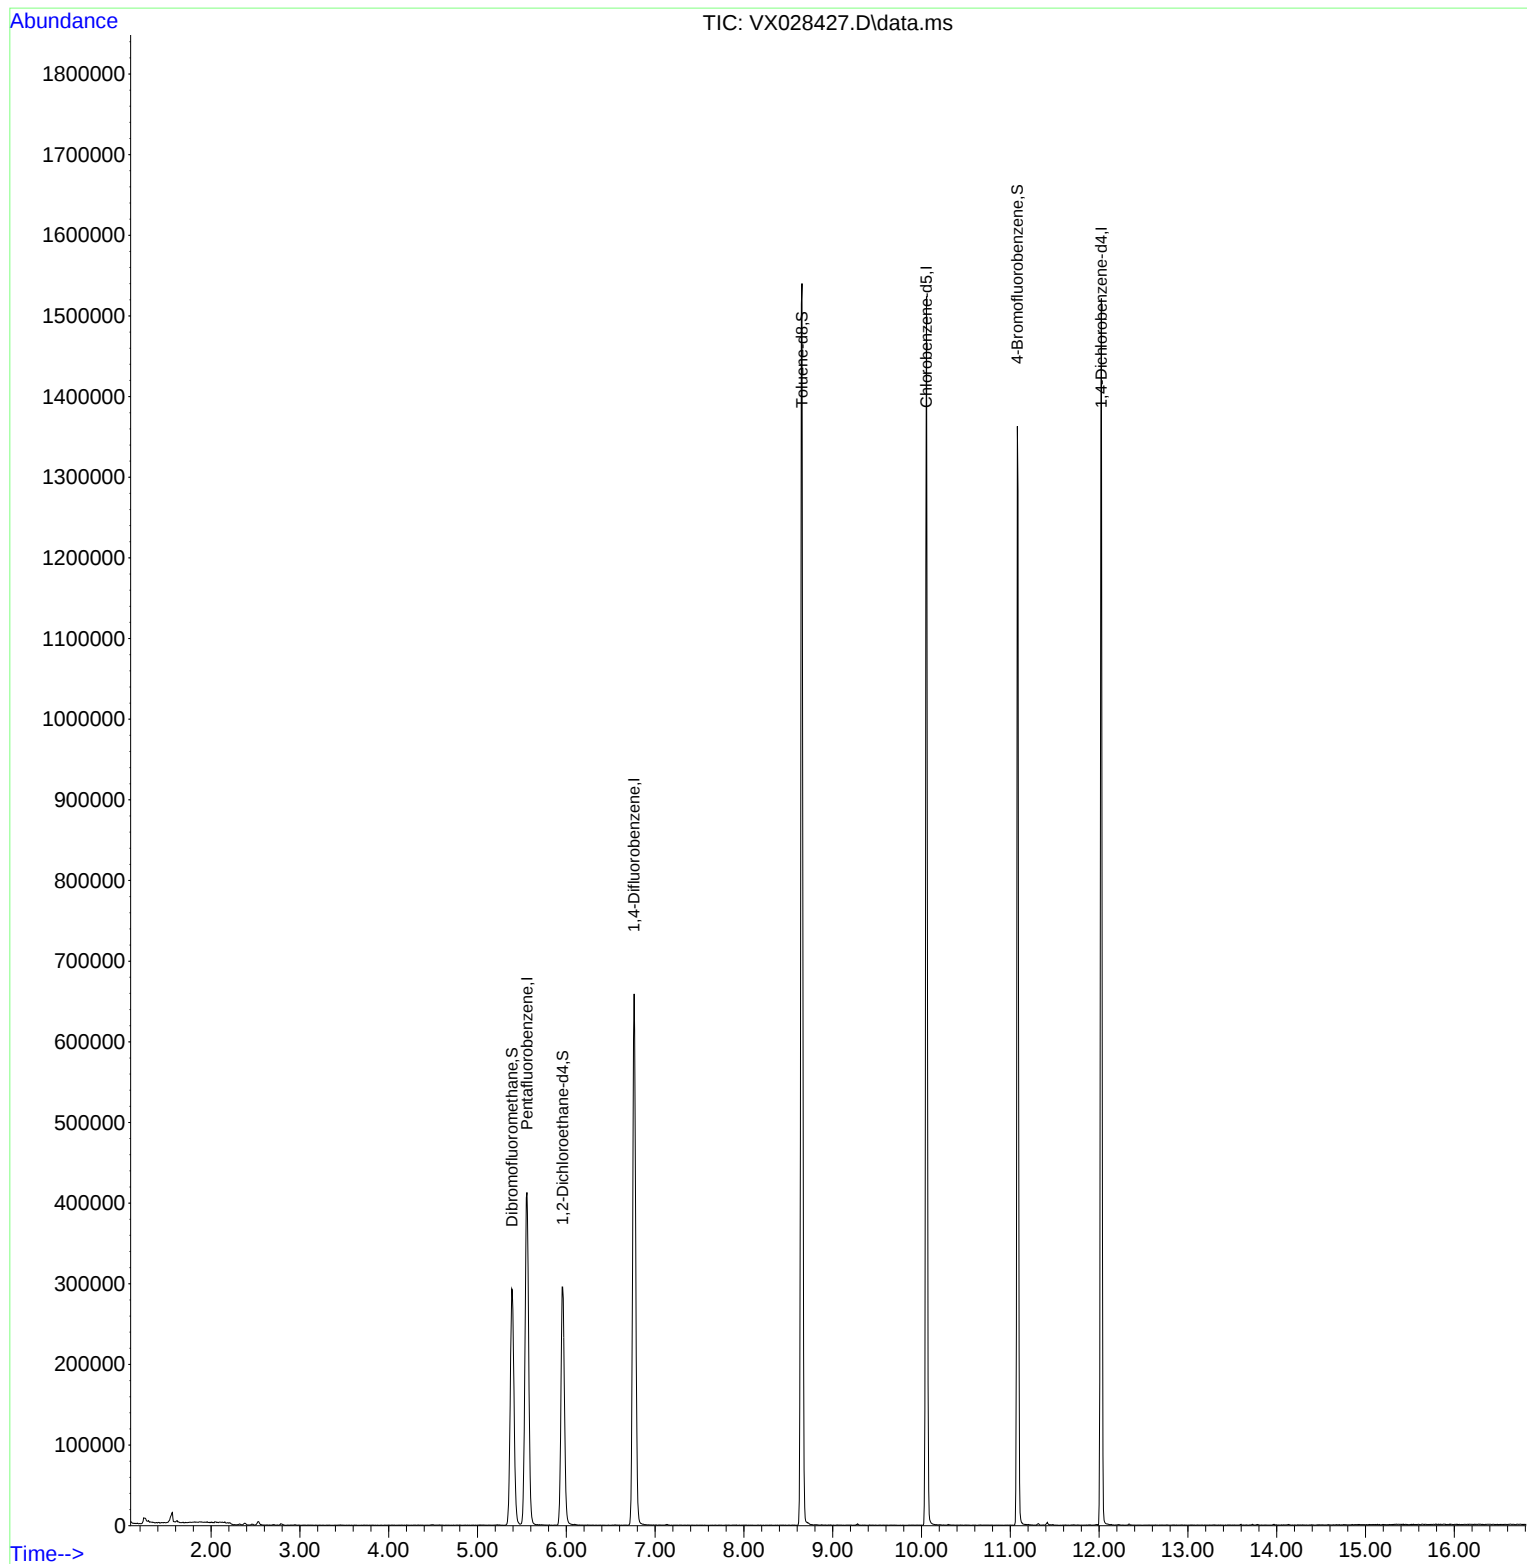




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. -0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36




Instrument :
MSVOA_X
ClientSampleId :
TB-01-042922


Tgt Ion:168 Resp: 404497
Ion Ratio Lower Upper
168 100
99 56.4 41.7 62.5

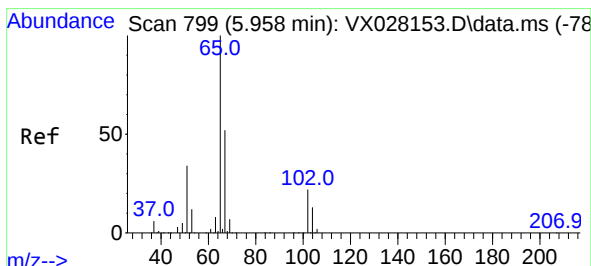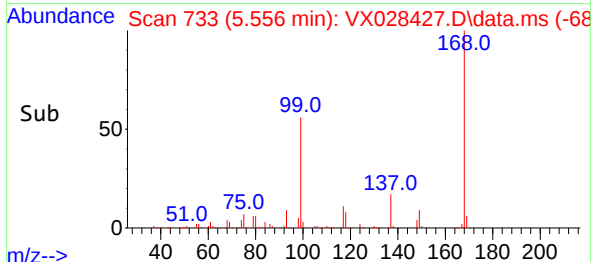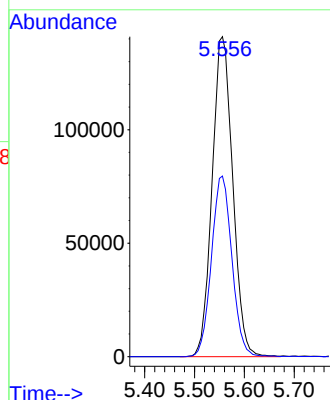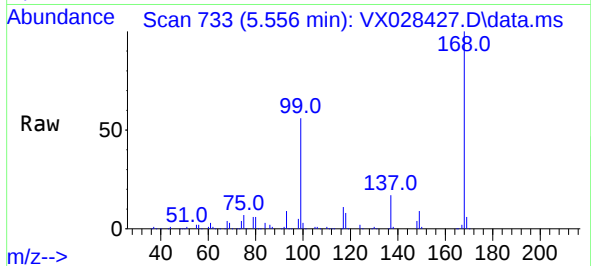

#33
1,2-Dichloroethane-d4
Concen: 53.523 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36


Tgt Ion: 65 Resp: 282289
Ion Ratio Lower Upper
65 100
67 51.7 0.0 107.4

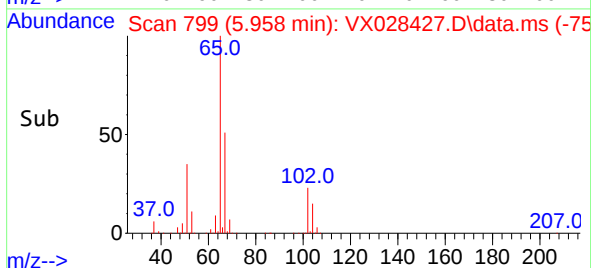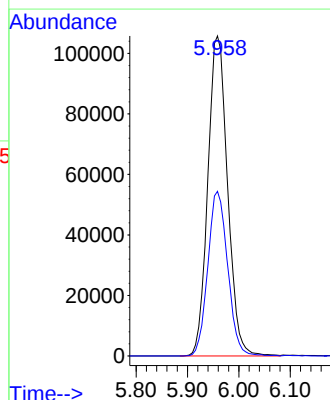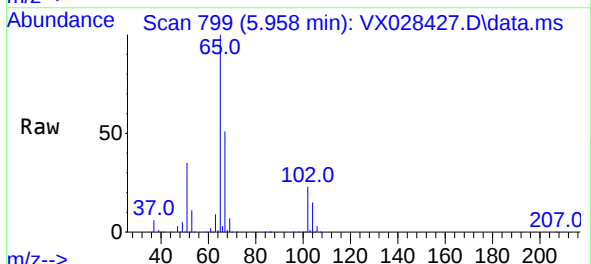



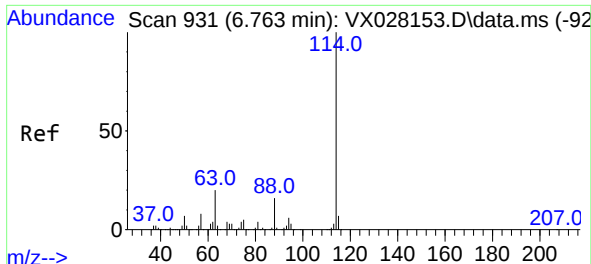


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36

Instrument :
MSVOA_X
ClientSampleId :
TB-01-042922



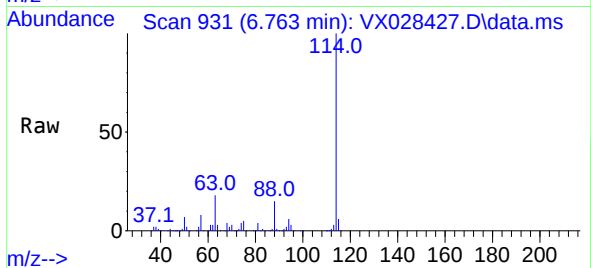


Tgt Ion:114 Resp: 703516
Ion Ratio Lower Upper
114 100
63 18.3 0.0 36.8
88 15.1 0.0 32.4

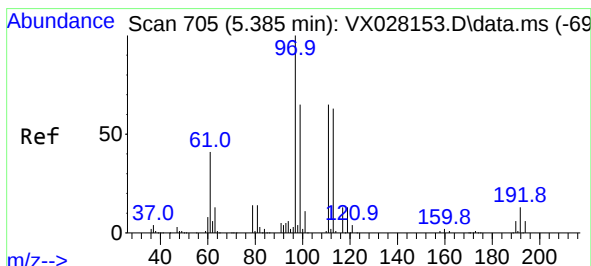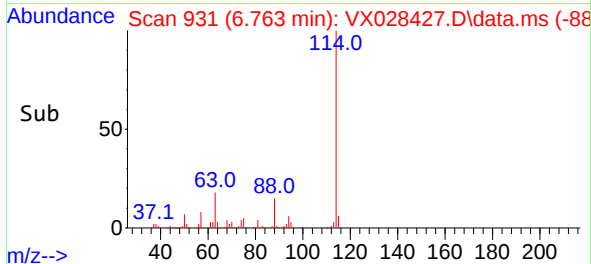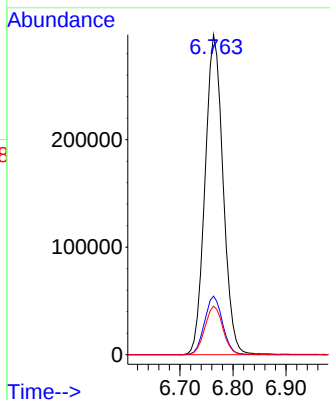

#35
Dibromofluoromethane
Concen: 51.638 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36

Tgt Ion:113 Resp: 254768
Ion Ratio Lower Upper
113 100
111 102.9 82.8 124.2
192 20.3 16.9 25.3


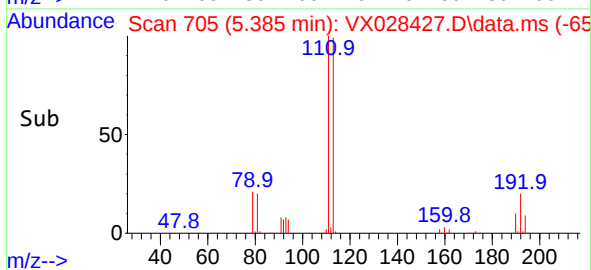
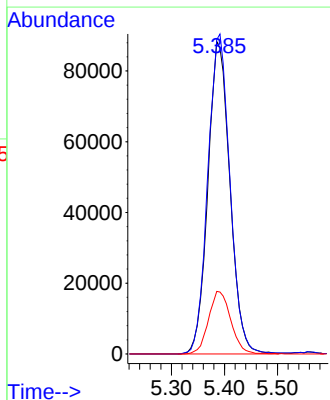
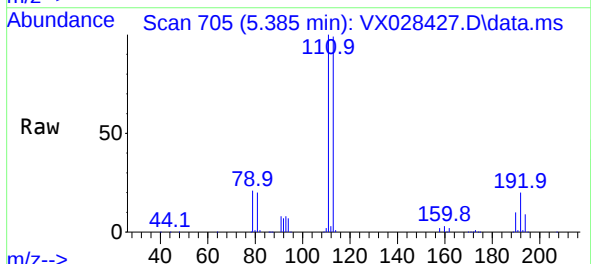




#50
Toluene-d8
Concen: 49.814 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36




Instrument :
MSVOA_X
ClientSampleId :
TB-01-042922


Tgt Ion: 98 Resp: 943945
Ion Ratio Lower Upper
98 100
100 66.3 52.6 78.8

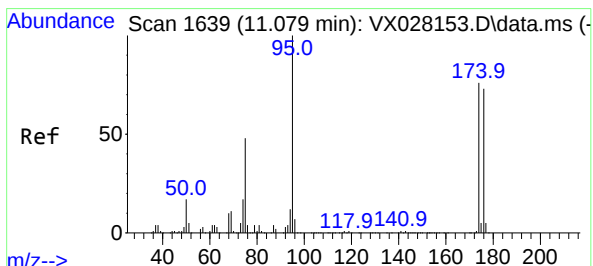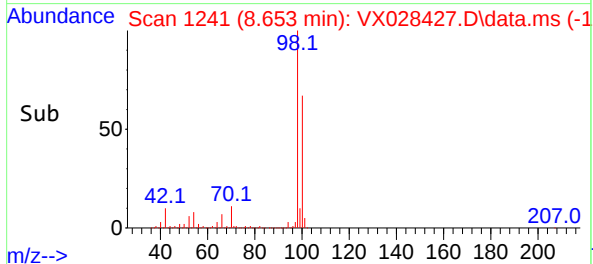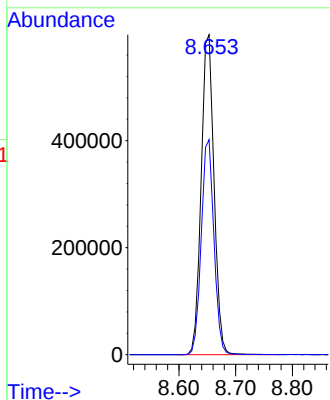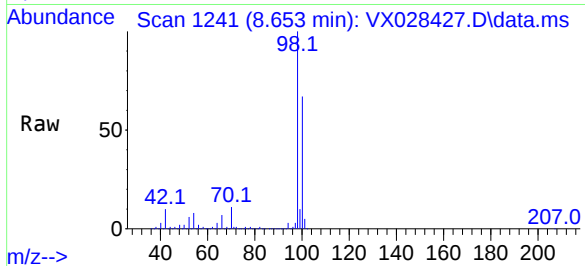

#62
4-Bromofluorobenzene
Concen: 48.077 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36

Tgt Ion: 95 Resp: 348339
Ion Ratio Lower Upper
95 100
174 84.2 0.0 163.0
176 80.6 0.0 155.0


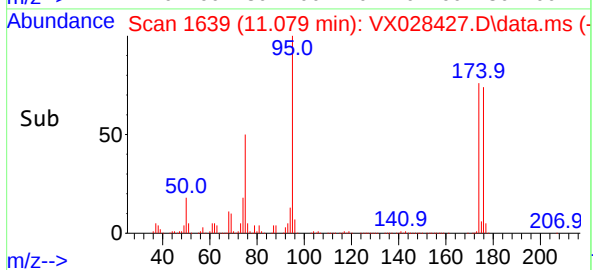
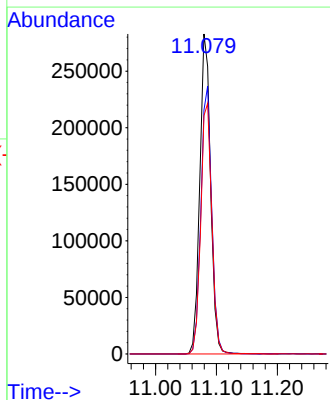
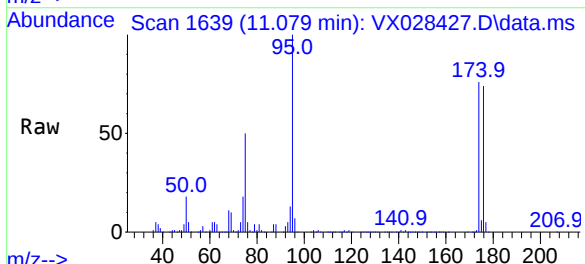


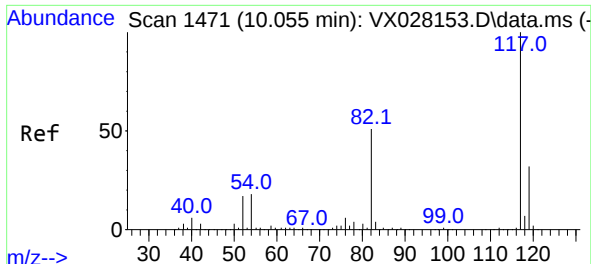

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36

Instrument :
MSVOA_X
ClientSampleId :
TB-01-042922

Tgt Ion:117 Resp: 685316
Ion Ratio Lower Upper
117 100
82 51.0 41.8 62.8
119 32.2 24.8 37.2

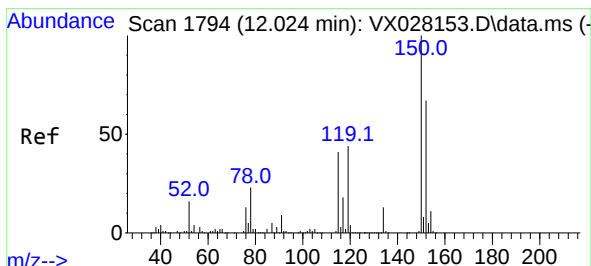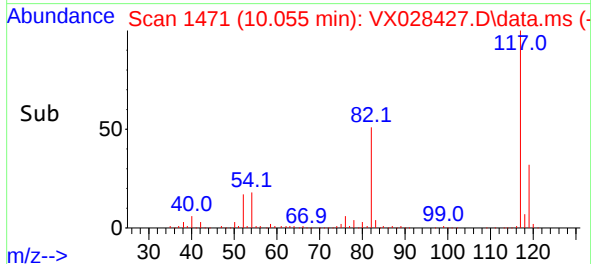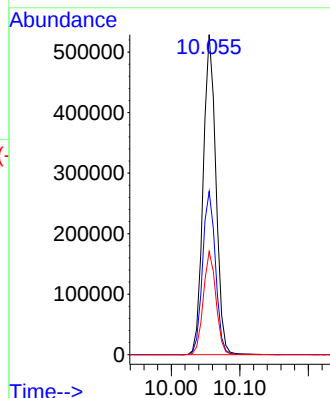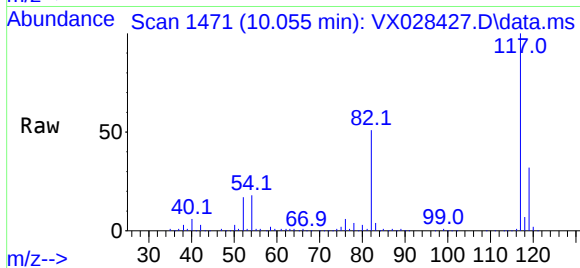

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028427.D
Acq: 29 Apr 2022 16:36

Tgt Ion:152 Resp: 320373
Ion Ratio Lower Upper
152 100
115 58.3 37.5 112.7
150 156.0 0.0 338.2

