

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
 Data File : VX028464.D
 Acq On : 30 Apr 2022 07:42
 Operator : JC/MD
 Sample : N2616-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MH-18D

Quant Time: Apr 30 09:25:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	381364	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	679272	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	697510	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	317919	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	290099	58.340	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 116.680%	
35) Dibromofluoromethane	5.391	113	255904	53.720	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 107.440%	
50) Toluene-d8	8.653	98	975874	53.337	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 106.680%	
62) 4-Bromofluorobenzene	11.079	95	359687	51.415	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 102.820%	
Target Compounds						Qvalue
16) Acetone	2.380	43	11013	5.888	ug/l	92
20) Methylene Chloride	2.788	84	8066	2.186	ug/l	98
43) Isopropyl Acetate	6.342	43	27251	2.656	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
Data File : VX028464.D
Acq On : 30 Apr 2022 07:42
Operator : JC/MD
Sample : N2616-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MH-18D

Quant Time: Apr 30 09:25:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




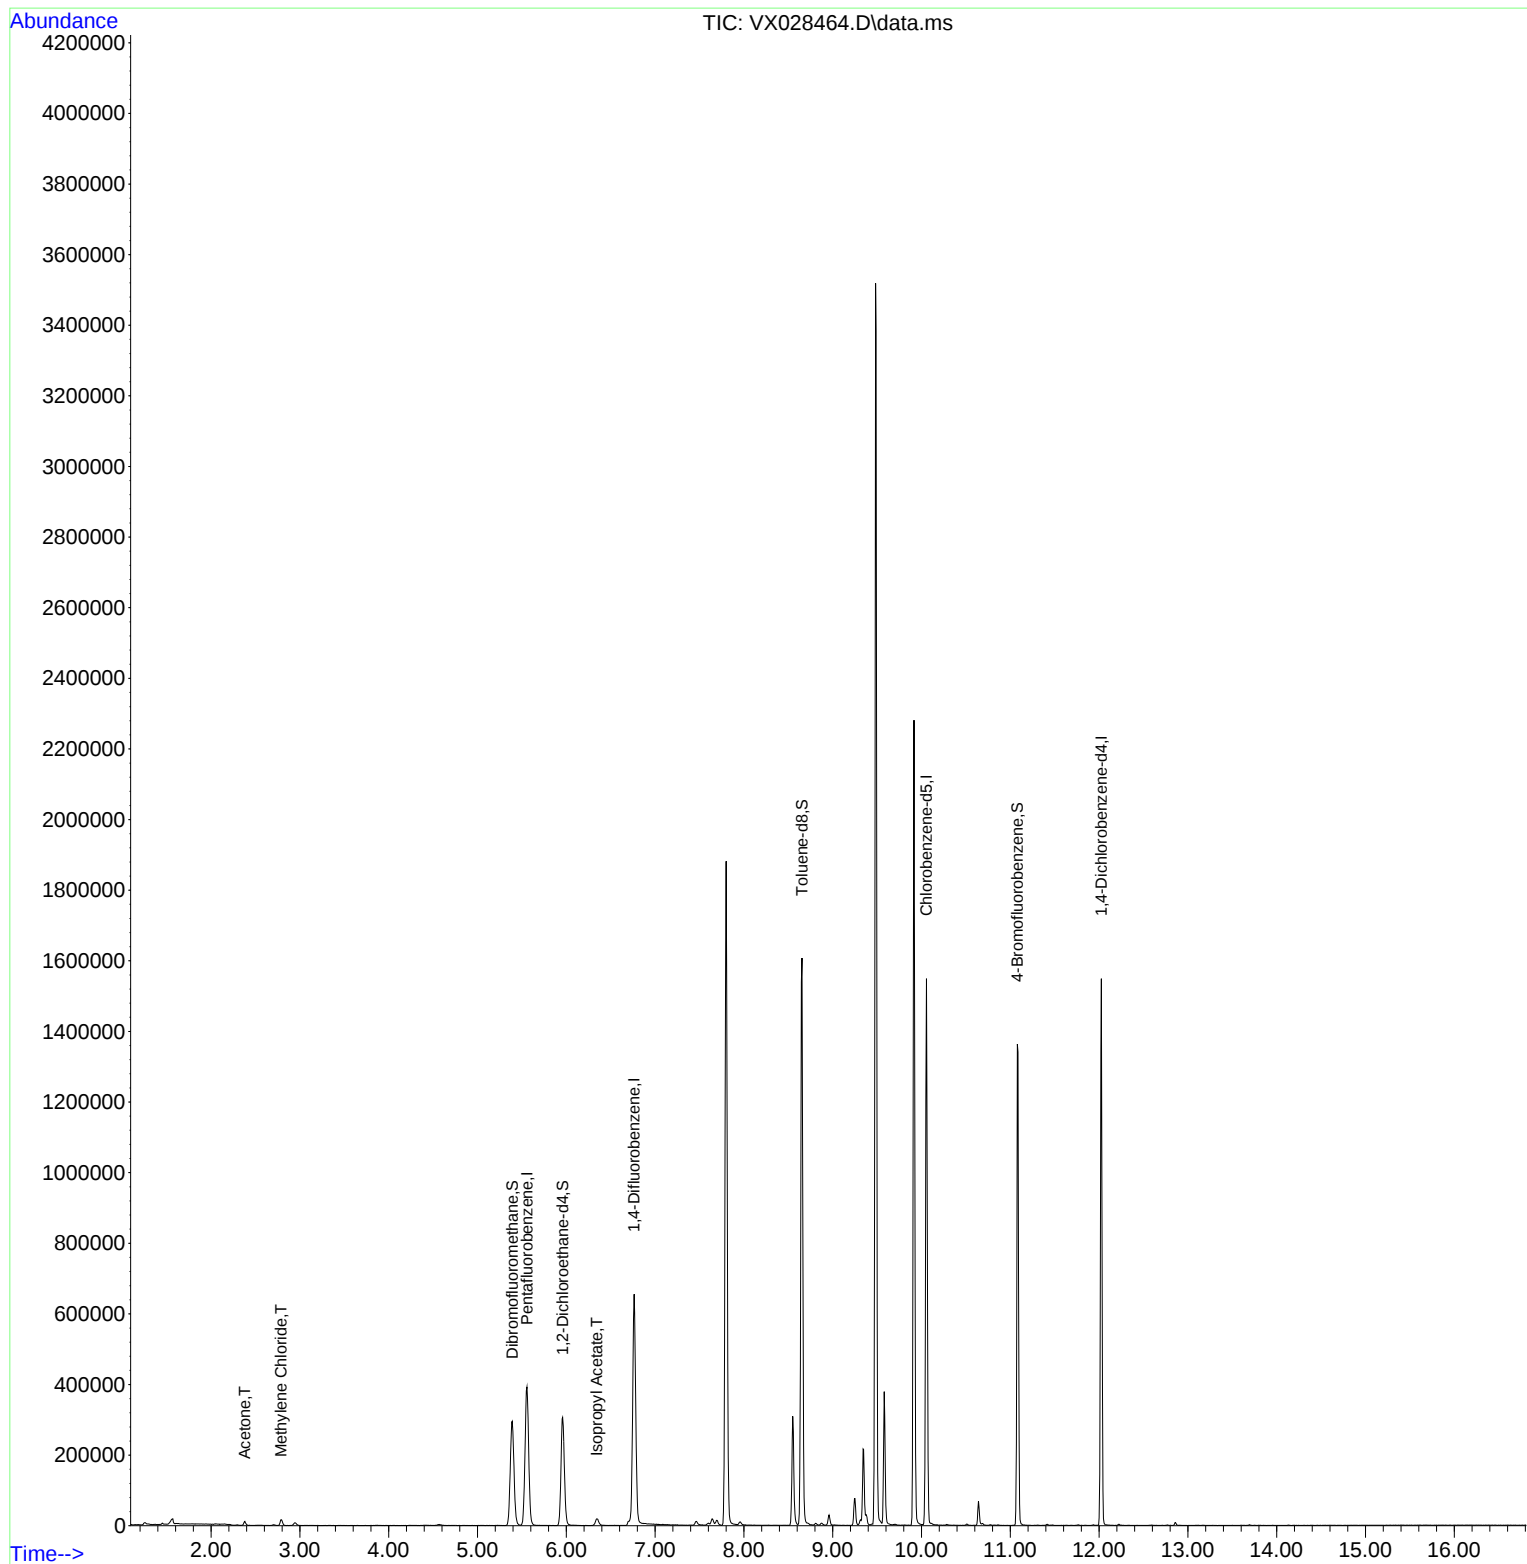


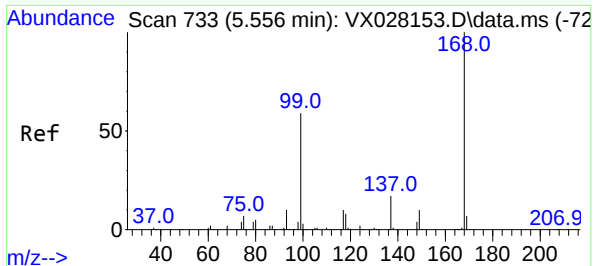

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42




Instrument :
MSVOA_X
ClientSampleId :
MH-18D


Tgt Ion:168 Resp: 381364
Ion Ratio Lower Upper
168 100
99 57.0 41.7 62.5

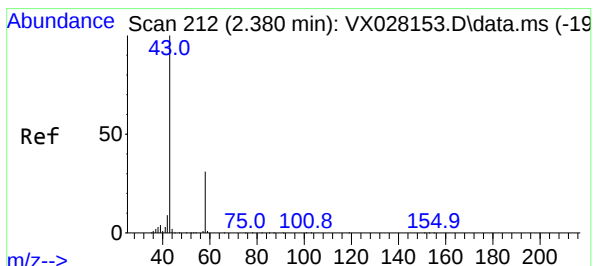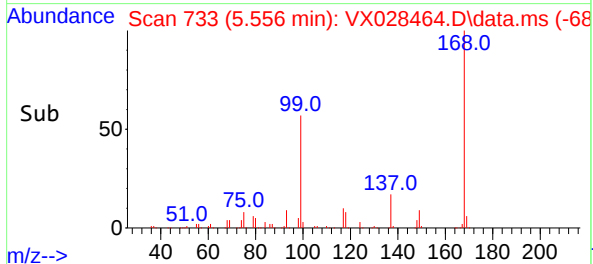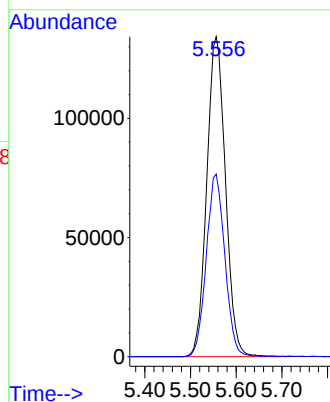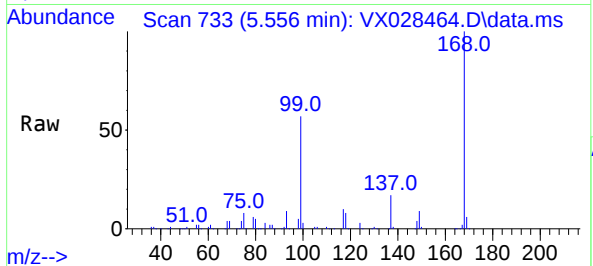

#16
Acetone
Concen: 5.888 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Tgt Ion: 43 Resp: 11013
Ion Ratio Lower Upper
43 100
58 31.2 28.8 43.2

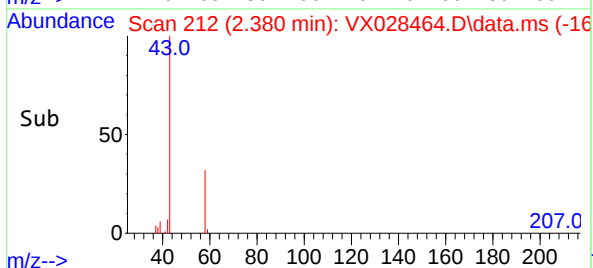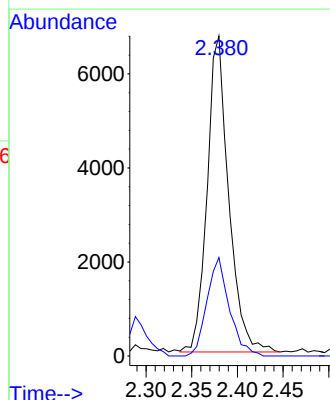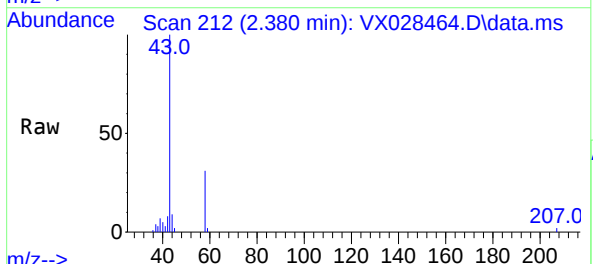




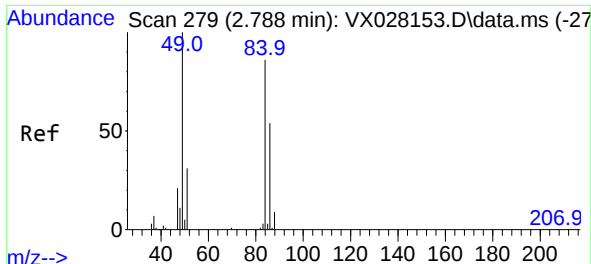


#20
Methylene Chloride
Concen: 2.186 ug/l
RT: 2.788 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Instrument :
MSVOA_X
ClientSampleId :
MH-18D

Tgt Ion: 84 Resp: 8066




Ion	Ratio	Lower	Upper
84	100		
49	110.4	85.5	128.3
51	33.4	26.6	39.8
86	64.3	51.5	77.3

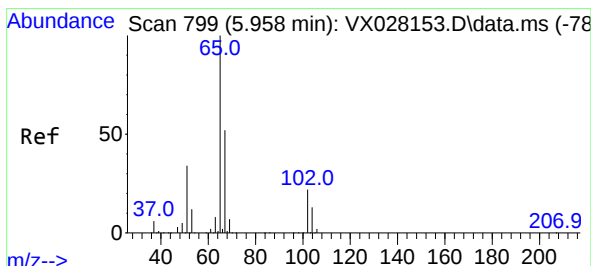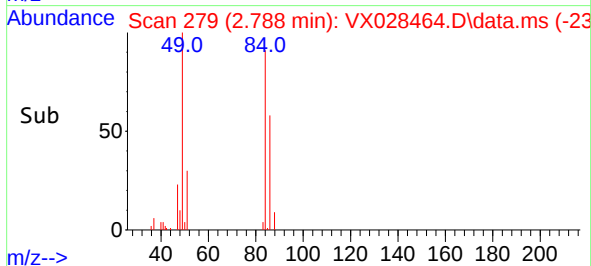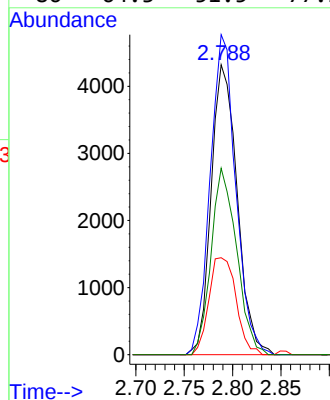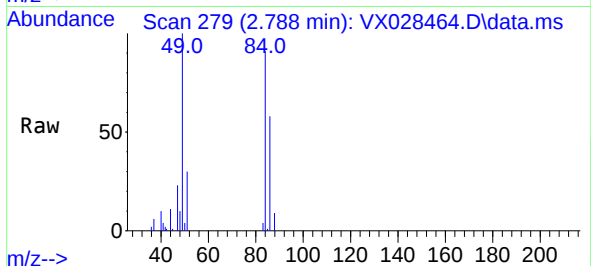


#33
1,2-Dichloroethane-d4
Concen: 58.340 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Tgt Ion: 65 Resp: 290099


Ion	Ratio	Lower	Upper
65	100		
67	51.9	0.0	107.4

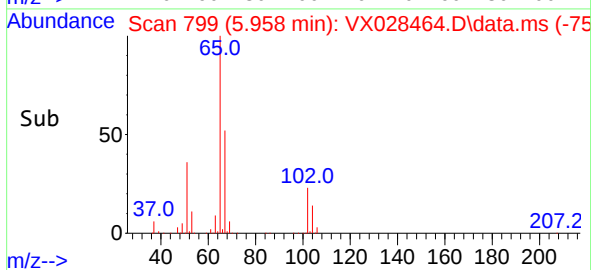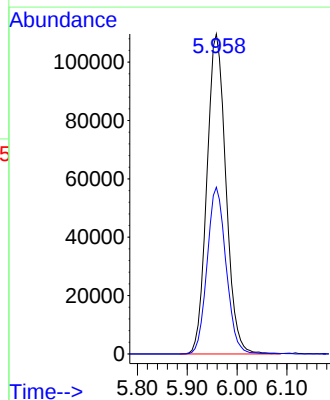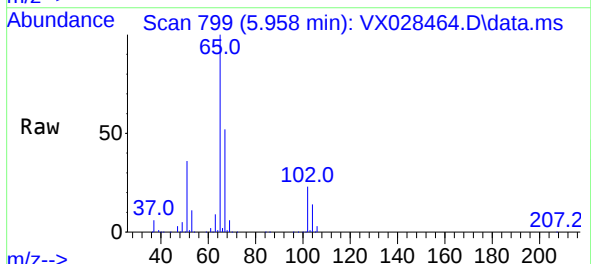



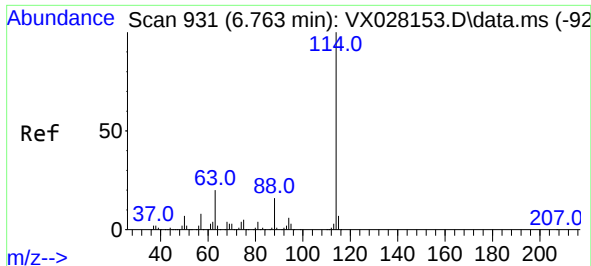


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Instrument :
MSVOA_X
ClientSampleId :
MH-18D



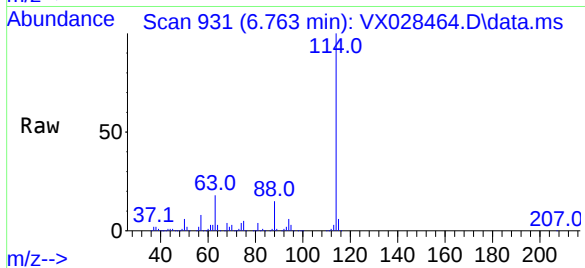



Tgt Ion:114 Resp: 679272
Ion Ratio Lower Upper
114 100
63 18.2 0.0 36.8
88 15.1 0.0 32.4

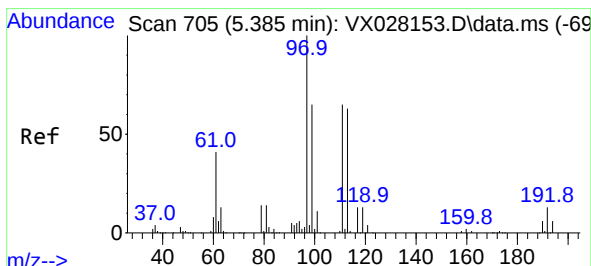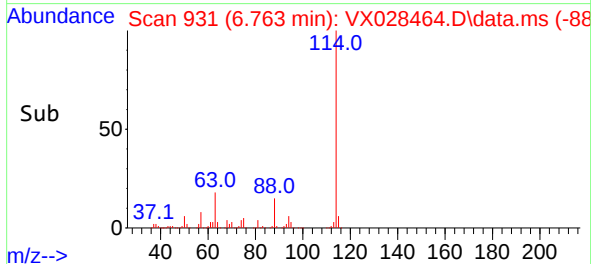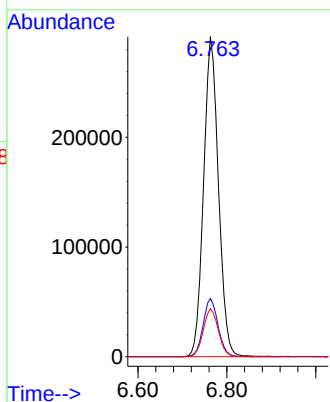

#35
Dibromofluoromethane
Concen: 53.720 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Tgt Ion:113 Resp: 255904
Ion Ratio Lower Upper
113 100
111 102.8 82.8 124.2
192 19.8 16.9 25.3


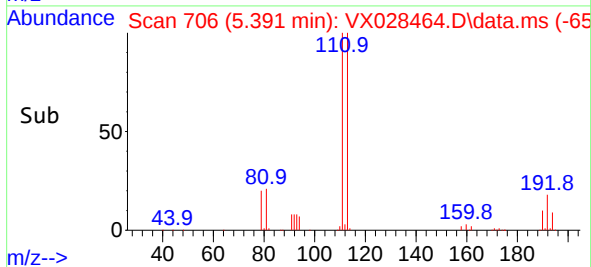
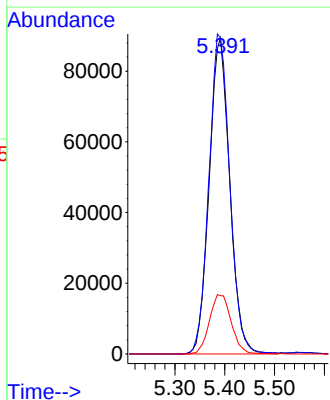
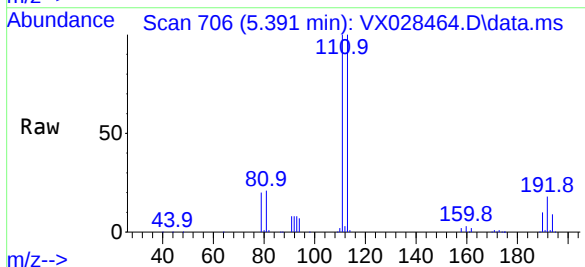


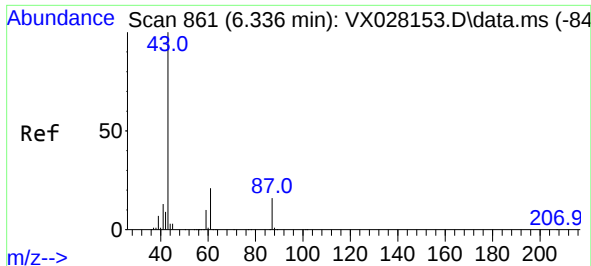

#43
Isopropyl Acetate
Concen: 2.656 ug/l
RT: 6.342 min Scan# 861
Delta R.T. 0.006 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42




Instrument :
MSVOA_X
ClientSampleId :
MH-18D


Tgt Ion: 43 Resp: 27251
Ion Ratio Lower Upper
43 100
61 20.3 18.5 27.7
87 15.9 13.0 19.6

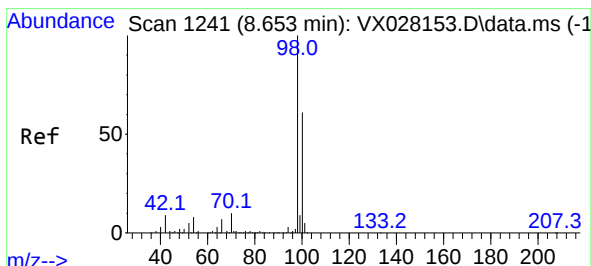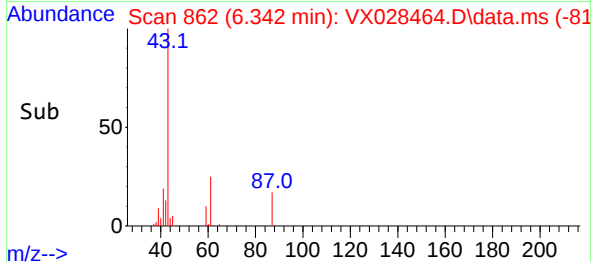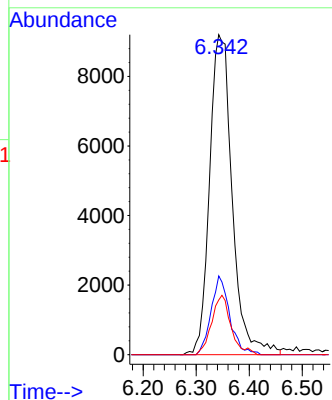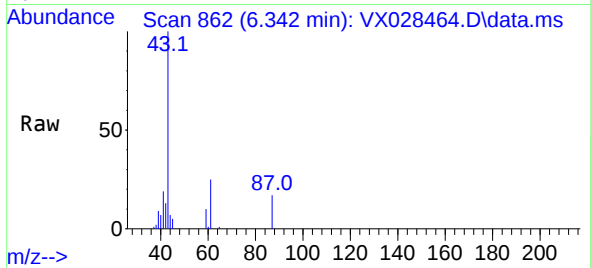

#50
Toluene-d8
Concen: 53.337 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Tgt Ion: 98 Resp: 975874
Ion Ratio Lower Upper
98 100
100 66.4 52.6 78.8


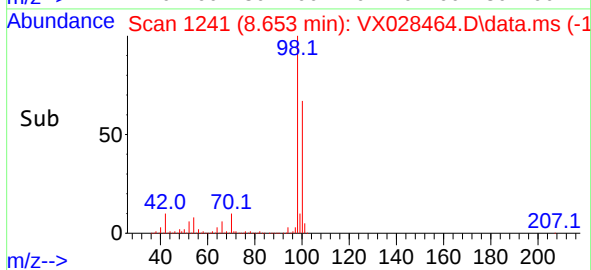
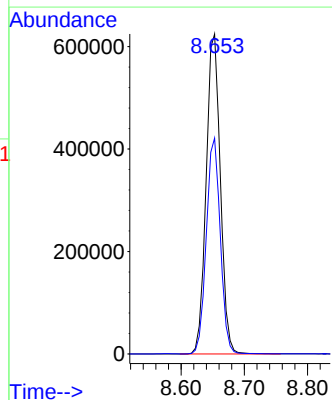
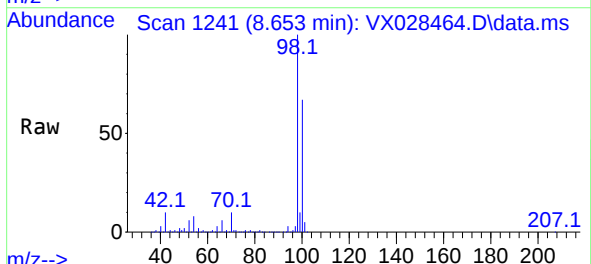


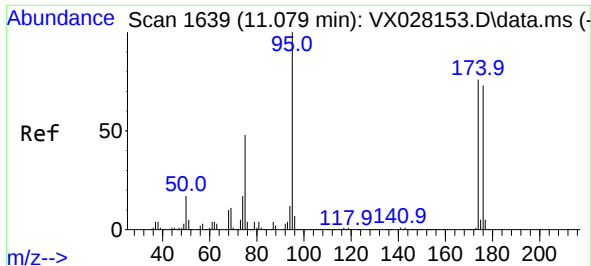

#62
4-Bromofluorobenzene
Concen: 51.415 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42




Instrument :
MSVOA_X
ClientSampleId :
MH-18D

Tgt Ion: 95 Resp: 359687
Ion Ratio Lower Upper
95 100
174 85.1 0.0 163.0
176 81.7 0.0 155.0

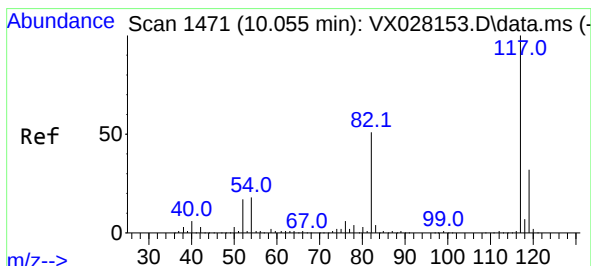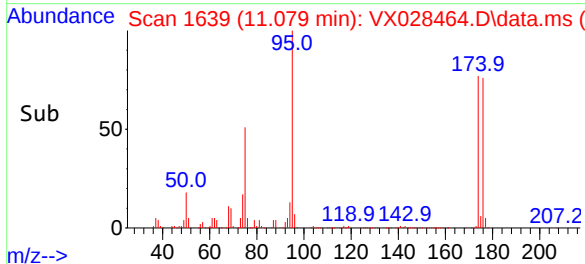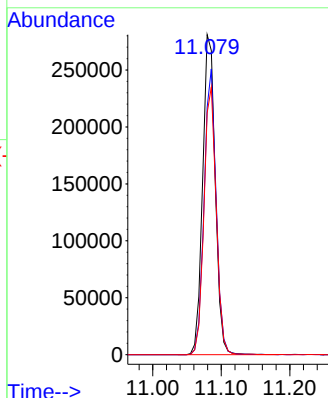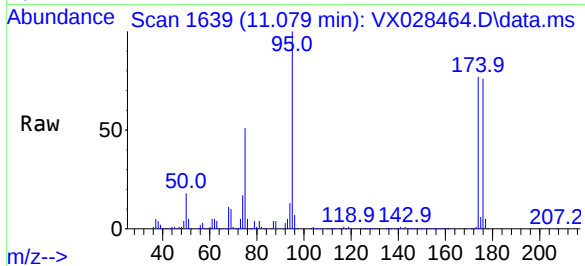


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Tgt Ion: 117 Resp: 697510
Ion Ratio Lower Upper
117 100
82 52.3 41.8 62.8
119 32.2 24.8 37.2

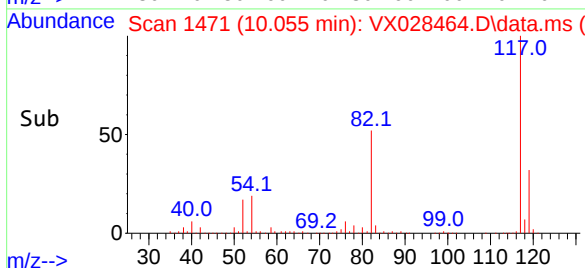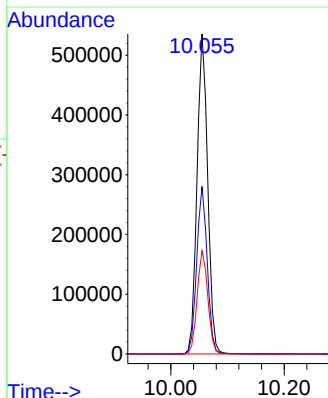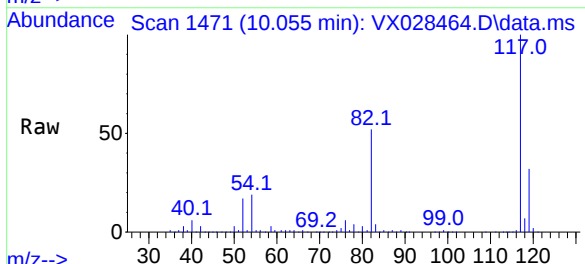


Abundance Scan 1794 (12.024 min): VX028153.D\data.ms (-

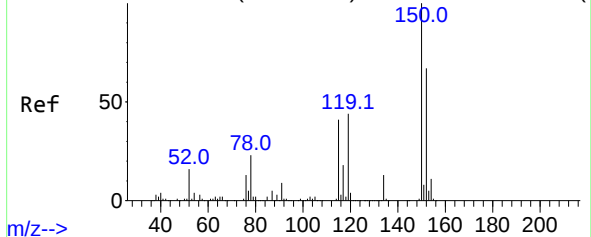

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX028464.D
Acq: 30 Apr 2022 07:42

Instrument :
MSVOA_X
ClientSampleId :
MH-18D

Abundance Scan 1794 (12.024 min): VX028464.D\data.ms

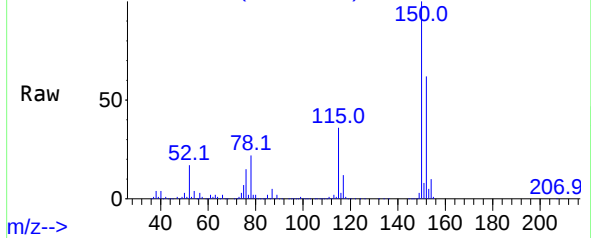

Tgt Ion:	152	Resp:	317919
Ion	Ratio	Lower	Upper
152	100		
115	58.3	37.5	112.7
150	158.1	0.0	338.2

Abundance Scan 1794 (12.024 min): VX028464.D\data.ms (-

