


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX042922\
 Data File : VX028411.D
 Acq On : 29 Apr 2022 09:36
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X042822W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 29 06:09:36 2022

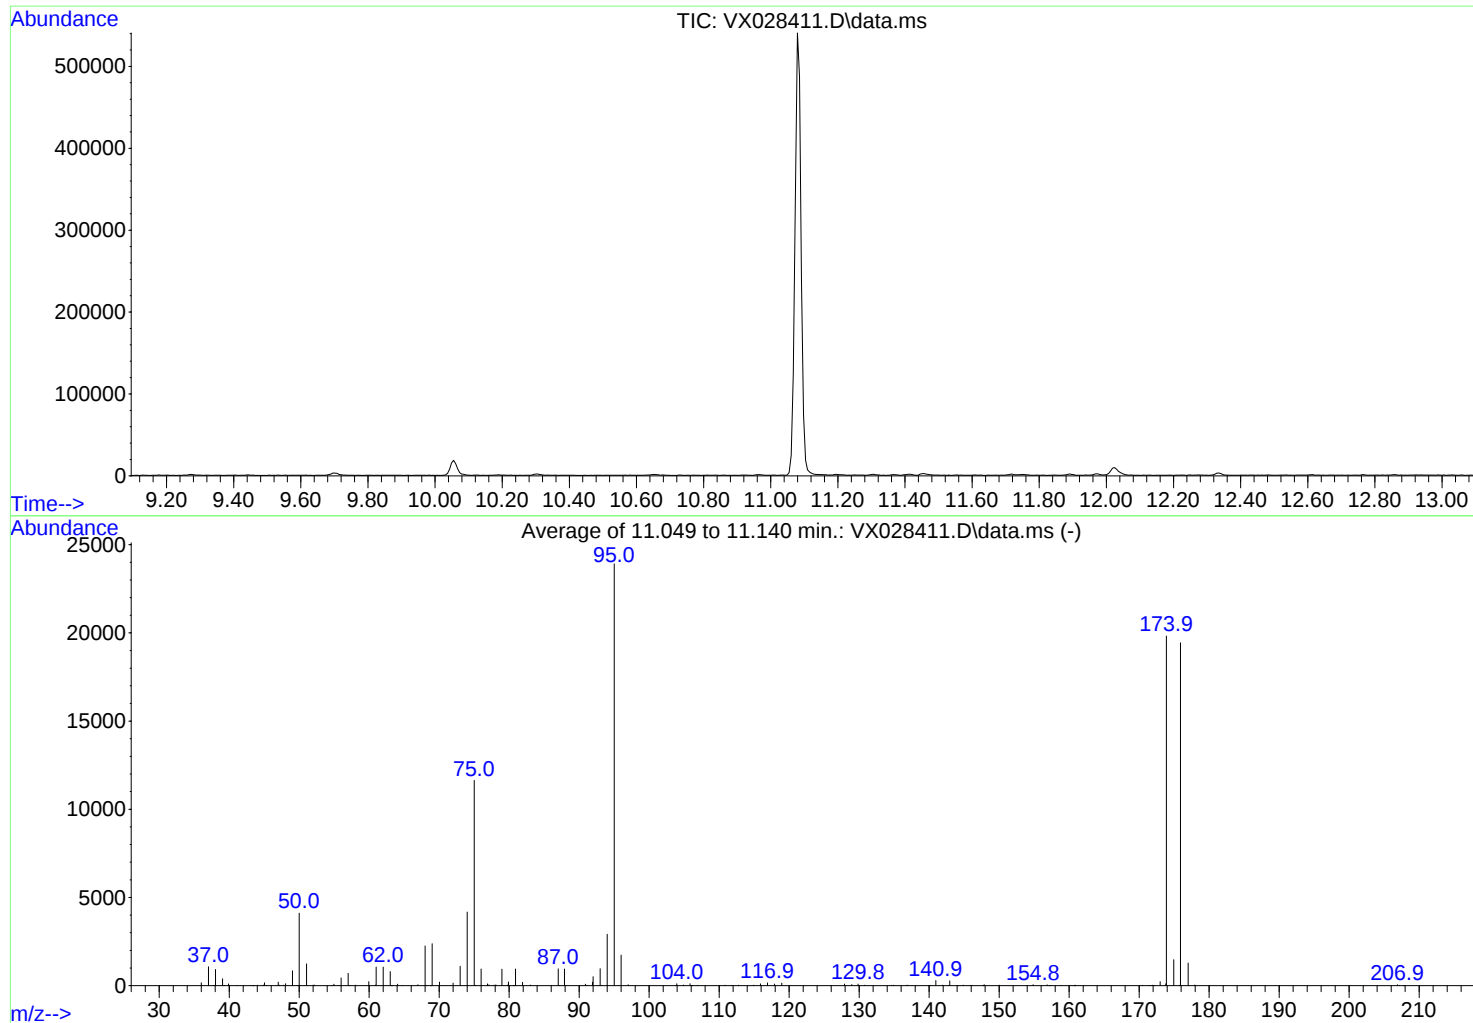

AutoFind: Averaged scan 1634 to 1649; Bkg corrected with scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	4110	PASS
75	95	30	60	48.7	11637	PASS
95	95	100	100	100.0	23915	PASS
96	95	5	9	7.2	1730	PASS
173	174	0.00	2	1.1	226	PASS
174	95	50	100	82.9	19826	PASS
175	174	5	9	7.4	1470	PASS
176	174	95	101	98.0	19438	PASS
177	176	5	9	6.6	1279	PASS