

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042924\  
 Data File : VX041269.D  
 Acq On : 29 Apr 2024 11:53  
 Operator : JC/MD  
 Sample : VX0429MBL01  
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :

Quant Time: Apr 30 02:06:27 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042224W.M  
 Quant Title : SW846 8260  
 QLast Update : Tue Apr 23 05:30:28 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units       | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|-------------|----------|
| -----                         |        |       |          |          |             |          |
| Internal Standards            |        |       |          |          |             |          |
| 1) Pentafluorobenzene         | 5.550  | 168   | 148578   | 50.000   | ug/l        | # 0.00   |
| 34) 1,4-Difluorobenzene       | 6.757  | 114   | 215463   | 50.000   | ug/l        | 0.00     |
| 63) Chlorobenzene-d5          | 10.055 | 117   | 201717   | 50.000   | ug/l        | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 12.024 | 152   | 105999   | 50.000   | ug/l        | 0.00     |
| System Monitoring Compounds   |        |       |          |          |             |          |
| 33) 1,2-Dichloroethane-d4     | 5.952  | 65    | 77724    | 54.954   | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 78 - 117 | Recovery | = 109.900%  |          |
| 35) Dibromofluoromethane      | 5.385  | 113   | 67156    | 51.239   | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 75 - 124 | Recovery | = 102.480%  |          |
| 50) Toluene-d8                | 8.647  | 98    | 250830   | 56.724   | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 92 - 112 | Recovery | = 113.440%# |          |
| 62) 4-Bromofluorobenzene      | 11.079 | 95    | 92901    | 56.920   | ug/l        | 0.00     |
| Spiked Amount                 | 50.000 | Range | 83 - 123 | Recovery | = 113.840%  |          |
| Target Compounds              |        |       |          |          |             |          |
|                               |        |       |          |          |             | Qvalue   |
| 3) Chloromethane              | 1.294  | 50    | 337      | 0.265    | ug/l        | 95       |
| 5) Bromomethane               | 1.599  | 94    | 996      | 1.390    | ug/l        | 98       |
| 6) Chloroethane               | 1.672  | 64    | 197      | 0.408    | ug/l        | # 1      |
| 10) Methyl Iodide             | 2.440  | 142   | 806      | 0.576    | ug/l        | # 75     |
| 11) Tert butyl alcohol        | 2.940  | 59    | 1204     | 4.752    | ug/l        | # 78     |
| 13) Acrolein                  | 2.245  | 56    | 174      | 0.612    | ug/l        | # 35     |
| 15) Acrylonitrile             | 3.087  | 53    | 667      | 1.030    | ug/l        | # 87     |
| 16) Acetone                   | 2.392  | 43    | 4406     | 8.558    | ug/l        | 98       |
| 17) Carbon Disulfide          | 2.501  | 76    | 1369     | 0.605    | ug/l        | 95       |
| 18) Methyl Acetate            | 2.709  | 43    | 649      | 0.426    | ug/l        | # 67     |
| 20) Methylene Chloride        | 2.782  | 84    | 1062     | 0.845    | ug/l        | # 88     |
| 21) trans-1,2-Dichloroethene  | 3.081  | 96    | 299      | 0.250    | ug/l        | # 58     |
| 23) Vinyl Acetate             | 3.751  | 43    | 957      | 0.294    | ug/l        | # 73     |
| 25) 2-Butanone                | 4.611  | 43    | 215      | 0.245    | ug/l        | # 51     |
| 29) Tetrahydrofuran           | 5.044  | 42    | 359      | 0.599    | ug/l        | # 71     |
| 31) Cyclohexane               | 5.537  | 56    | 2585     | 1.358    | ug/l        | # 1      |
| 36) 1,1-Dichloropropene       | 5.544  | 75    | 9210     | 5.492    | ug/l        | # 51     |
| 38) Carbon Tetrachloride      | 5.544  | 117   | 12943    | 6.910    | ug/l        | # 17     |
| 41) Methacrylonitrile         | 5.038  | 41    | 192      | 0.200    | ug/l        | # 36     |
| 51) 4-Methyl-2-Pentanone      | 8.580  | 43    | 706      | 0.381    | ug/l        | 98       |
| 59) 2-Hexanone                | 9.457  | 43    | 517      | 0.363    | ug/l        | 89       |
| 76) 1,2,3-Trichloropropane    | 11.079 | 75    | 47368    | 27.736   | ug/l        | # 39     |
| 81) trans-1,4-Dichloro-2-b... | 11.079 | 75    | 47368    | 78.251   | ug/l        | # 5      |
| 93) 1,2,4-Trichlorobenzene    | 13.597 | 180   | 1021     | 0.426    | ug/l        | 80       |
| 95) Naphthalene               | 13.780 | 128   | 4092     | 0.595    | ug/l        | # 95     |
| 96) 1,2,3-Trichlorobenzene    | 13.963 | 180   | 1113     | 0.441    | ug/l        | 92       |
| -----                         |        |       |          |          |             |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX042924\  
Data File : VX041269.D  
Acq On : 29 Apr 2024 11:53  
Operator : JC/MD  
Sample : VX0429MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_X/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :


Quant Time: Apr 30 02:06:27 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X042224W.M  
Quant Title : SW846 8260  
QLast Update : Tue Apr 23 05:30:28 2024  
Response via : Initial Calibration

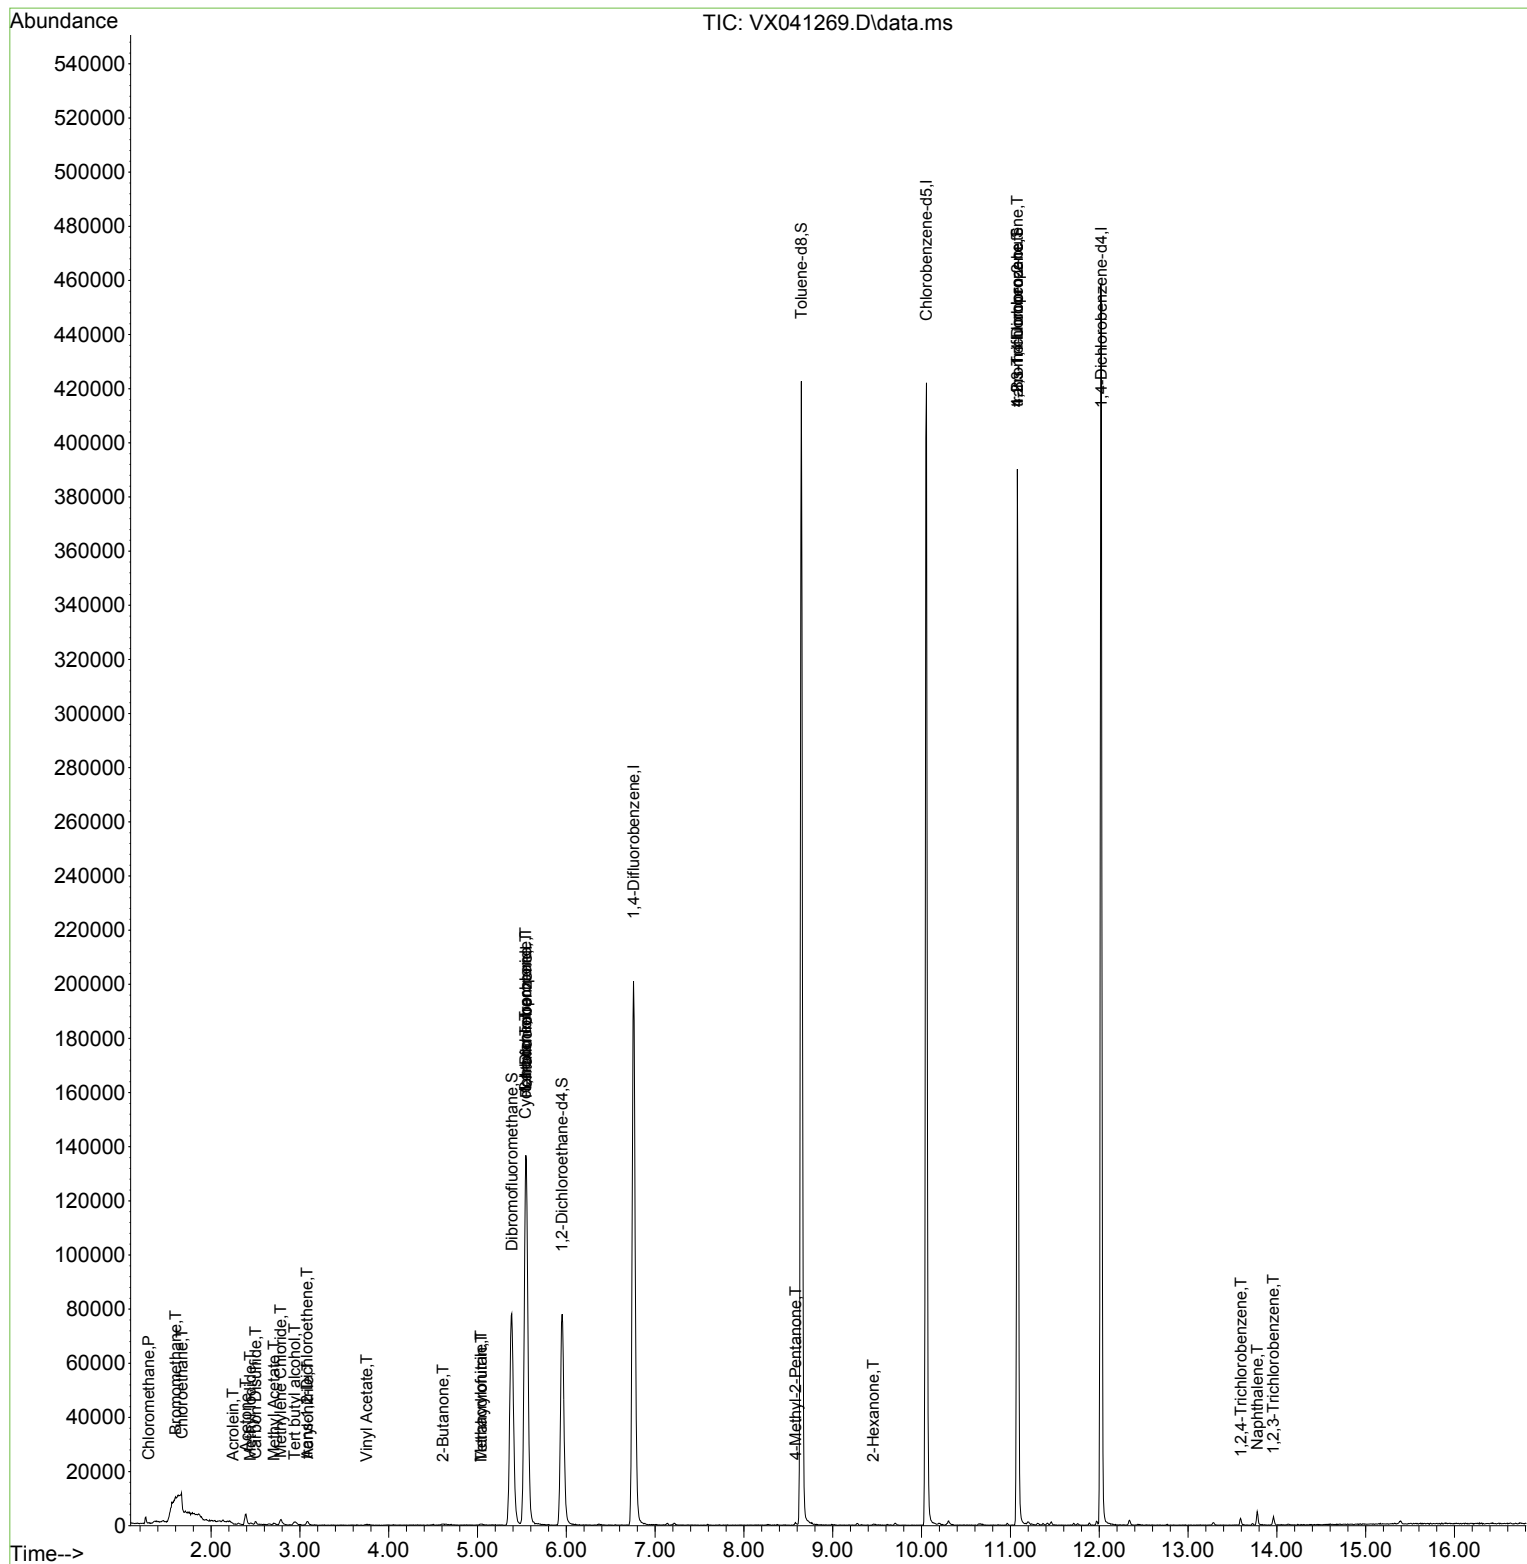






#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 5.550 min Scan# 71  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :



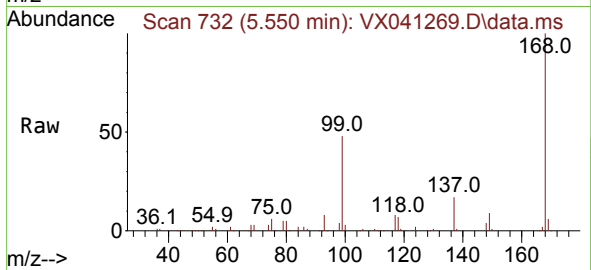



Tgt Ion:168 Resp: 148578  
Ion Ratio Lower Upper  
168 100  
99 48.0 56.6 85.0#

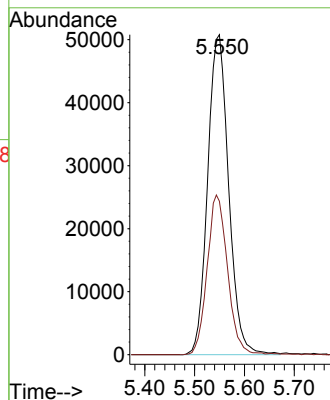

#3  
Chloromethane  
Concen: 0.265 ug/l  
RT: 1.294 min Scan# 34  
Delta R.T. -0.006 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 50 Resp: 337  
Ion Ratio Lower Upper  
50 100  
52 28.9 25.5 38.3


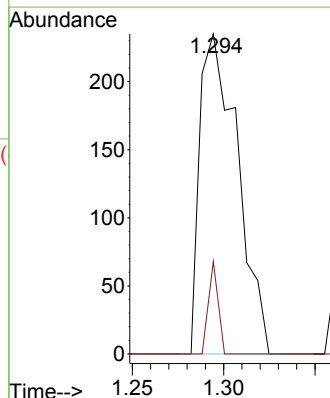

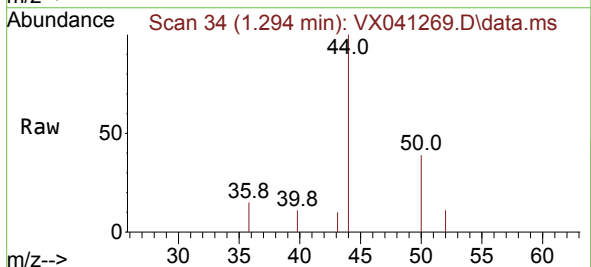


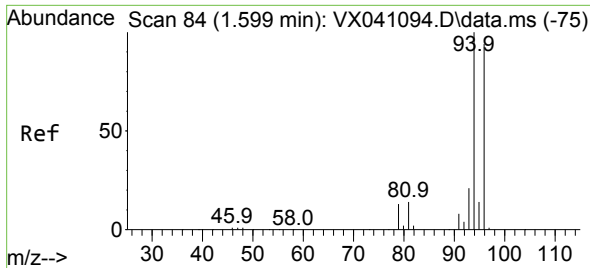

#5  
Bromomethane  
Concen: 1.390 ug/l  
RT: 1.599 min Scan# 84  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 94 Resp: 996  
Ion Ratio Lower Upper  
94 100  
96 95.5 74.6 111.8

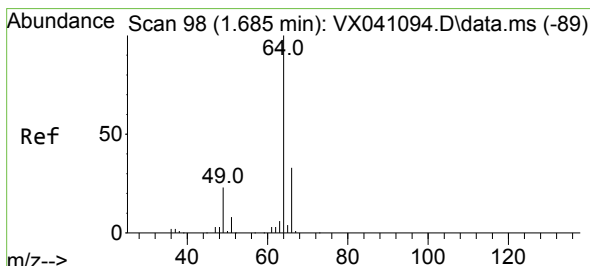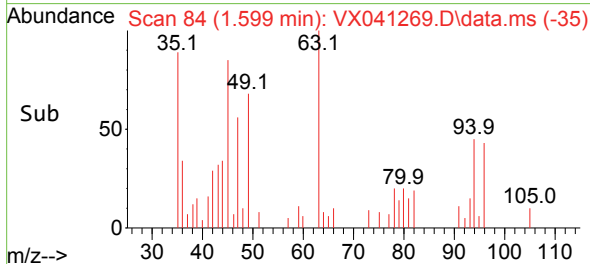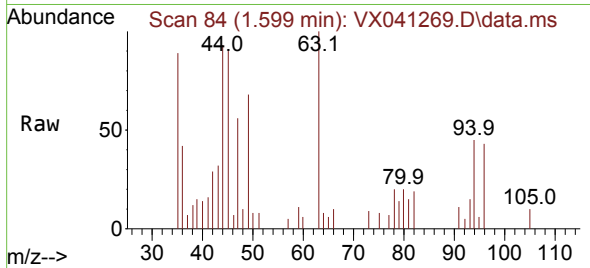

#6  
Chloroethane  
Concen: 0.408 ug/l  
RT: 1.672 min Scan# 96  
Delta R.T. 0.006 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion: 64 Resp: 197  
Ion Ratio Lower Upper  
64 100  
66 146.5 25.1 37.7#

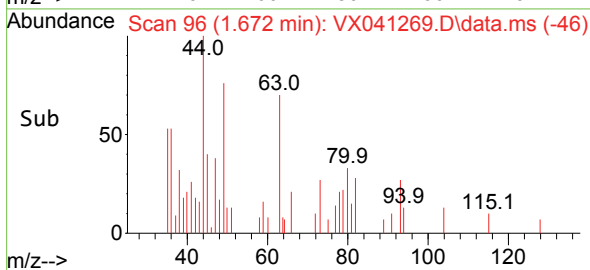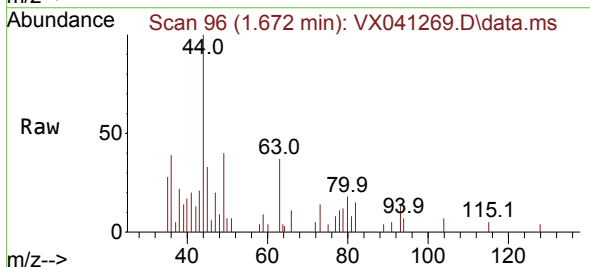






#10  
Methyl Iodide  
Concen: 0.576 ug/l  
RT: 2.440 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion:142 Resp: 806  
Ion Ratio Lower Upper  
142 100  
127 36.8 41.6 62.4#  
141 0.0 11.6 17.4#

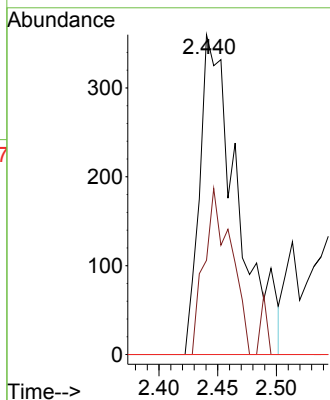

#11  
Tert butyl alcohol  
Concen: 4.752 ug/l  
RT: 2.940 min Scan# 304  
Delta R.T. -0.122 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 59 Resp: 1204  
Ion Ratio Lower Upper  
59 100  
57 0.0 6.0 9.0#

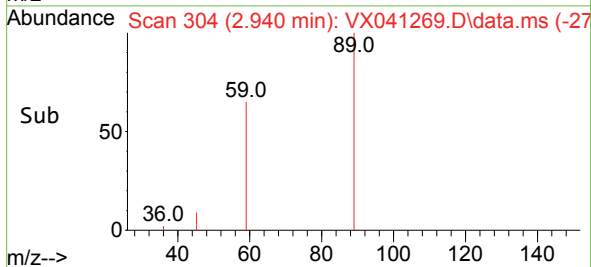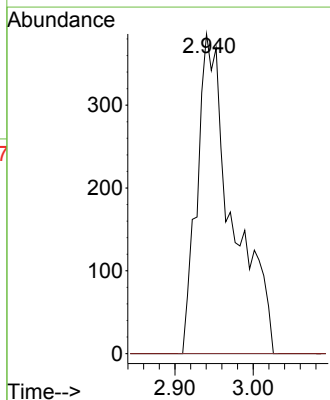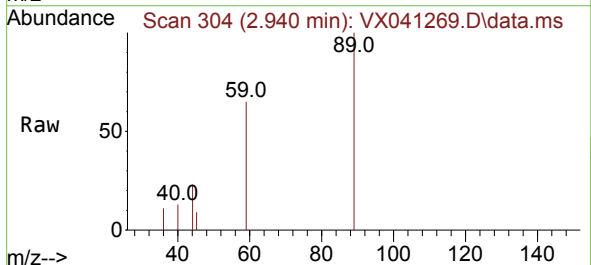



#13

Acrolein

Concen: 0.612 ug/l

RT: 2.245 min Scan# 19

Delta R.T. 0.006 min

Lab File: VX041269.D

Acq: 29 Apr 2024 11:53

Instrument :

MSVOA\_X





ClientSampleId :

Tgt Ion: 56 Resp: 174

Ion Ratio Lower Upper

56 100

55 125.3 57.1 85.7#

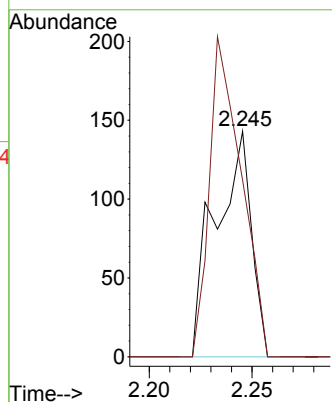

#15

Acrylonitrile

Concen: 1.030 ug/l

RT: 3.087 min Scan# 328

Delta R.T. 0.012 min

Lab File: VX041269.D

Acq: 29 Apr 2024 11:53




Tgt Ion: 53 Resp: 667


Ion Ratio Lower Upper

53 100

52 72.1 66.0 99.0

51 27.1 29.8 44.6#


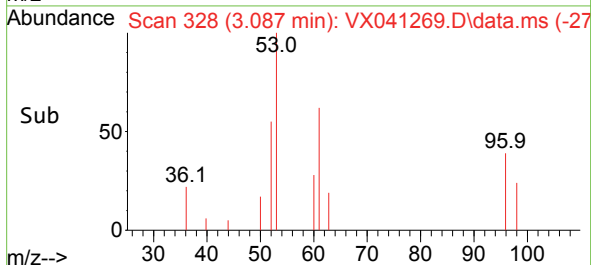

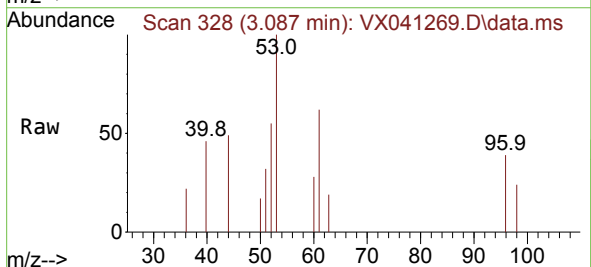




#16  
Acetone  
Concen: 8.558 ug/l  
RT: 2.392 min Scan# 212  
Delta R.T. -0.006 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 4406  
Ion Ratio Lower Upper  
43 100  
58 28.3 21.9 32.9

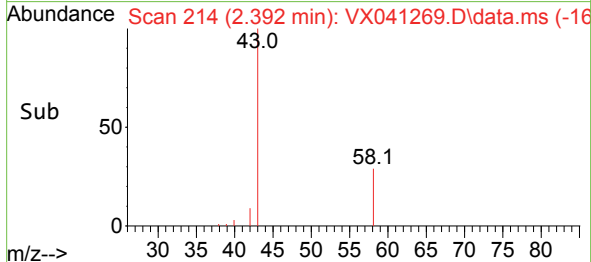

#17  
Carbon Disulfide  
Concen: 0.605 ug/l  
RT: 2.501 min Scan# 232  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion: 76 Resp: 1369  
Ion Ratio Lower Upper  
76 100  
78 7.2 7.0 10.6

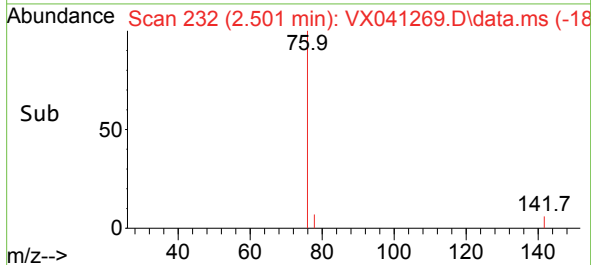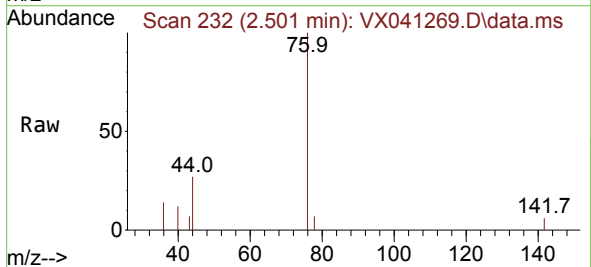






#18  
Methyl Acetate  
Concen: 0.426 ug/l  
RT: 2.709 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :



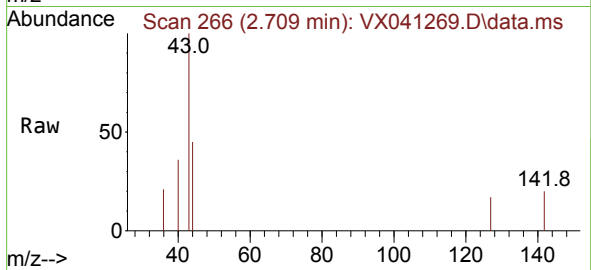



Tgt Ion: 43 Resp: 649  
Ion Ratio Lower Upper  
43 100  
74 6.5 17.8 26.8#

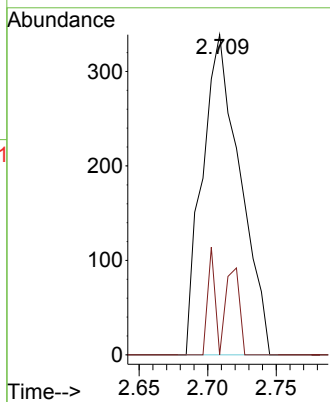

#20  
Methylene Chloride  
Concen: 0.845 ug/l  
RT: 2.782 min Scan# 278  
Delta R.T. -0.006 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion: 84 Resp: 1062  
Ion Ratio Lower Upper  
84 100  
49 120.2 103.6 155.4  
51 23.5 33.8 50.6#  
86 55.3 49.4 74.0

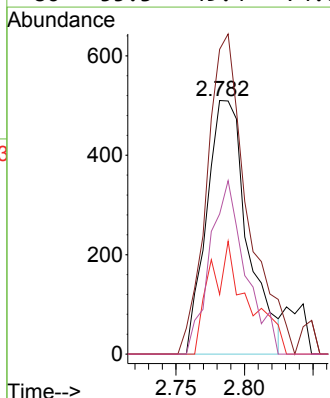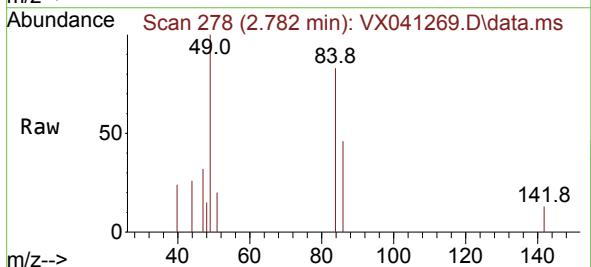






#21  
trans-1,2-Dichloroethene  
Concen: 0.250 ug/l  
RT: 3.081 min Scan# 31  
Delta R.T. -0.006 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 96 Resp: 299  
Ion Ratio Lower Upper  
96 100  
61 100.5 119.2 178.8#  
98 22.7 48.7 73.1#

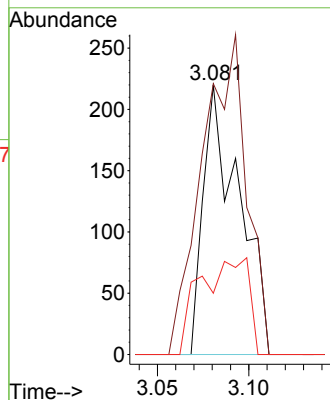

#23  
Vinyl Acetate  
Concen: 0.294 ug/l  
RT: 3.751 min Scan# 437  
Delta R.T. 0.030 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 43 Resp: 957  
Ion Ratio Lower Upper  
43 100  
86 0.0 7.8 11.8#


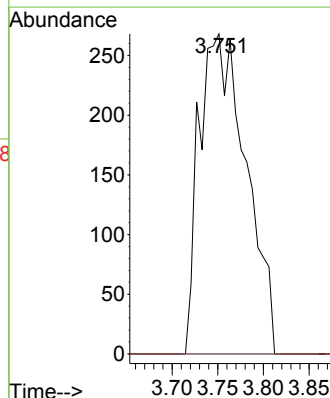






#25  
2-Butanone  
Concen: 0.245 ug/l  
RT: 4.611 min Scan# 51  
Delta R.T. 0.043 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 215  
Ion Ratio Lower Upper  
43 100  
72 0.0 19.4 29.2#

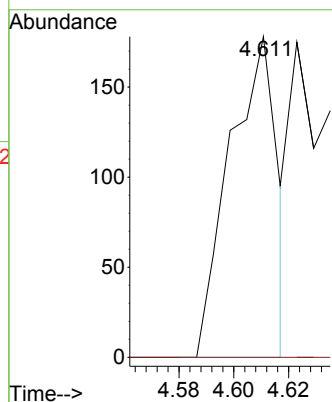

#29  
Tetrahydrofuran  
Concen: 0.599 ug/l  
RT: 5.044 min Scan# 649  
Delta R.T. 0.030 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion: 42 Resp: 359  
Ion Ratio Lower Upper  
42 100  
72 10.9 34.2 51.4#  
71 35.7 32.2 48.2

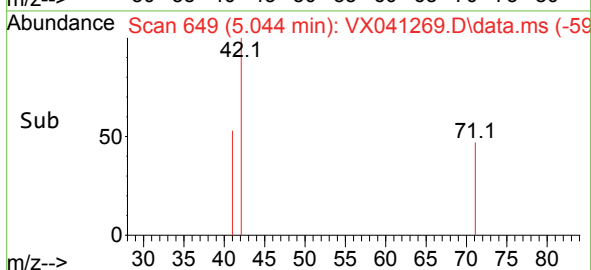






#31  
Cyclohexane  
Concen: 1.358 ug/l  
RT: 5.537 min Scan# 719  
Delta R.T. 0.073 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 56 Resp: 2585  
Ion Ratio Lower Upper  
56 100  
69 160.3 23.4 35.2#  
84 124.8 65.9 98.9#



#33  
1,2-Dichloroethane-d4  
Concen: 54.954 ug/l  
RT: 5.952 min Scan# 798  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 65 Resp: 77724  
Ion Ratio Lower Upper  
65 100  
67 50.7 0.0 100.2


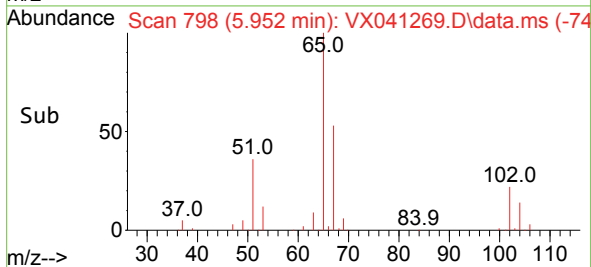

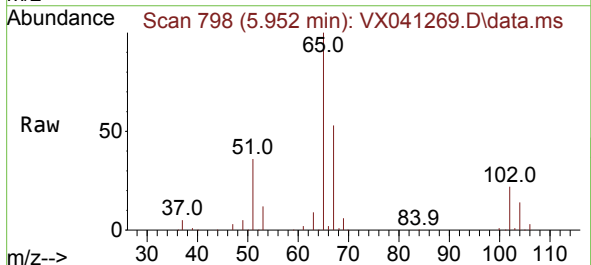




#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 6.757 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion:114 Resp: 215463  
Ion Ratio Lower Upper  
114 100  
63 19.2 0.0 45.0  
88 16.1 0.0 36.6



#35  
Dibromofluoromethane  
Concen: 51.239 ug/l  
RT: 5.385 min Scan# 705  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion:113 Resp: 67156  
Ion Ratio Lower Upper  
113 100  
111 102.0 82.9 124.3  
192 25.6 13.3 19.9#

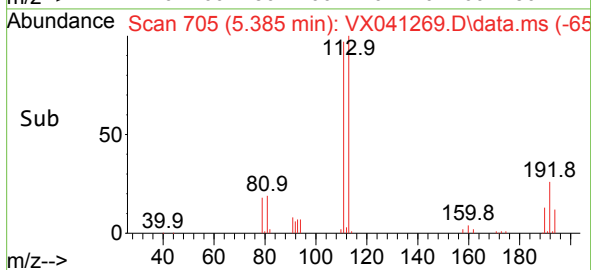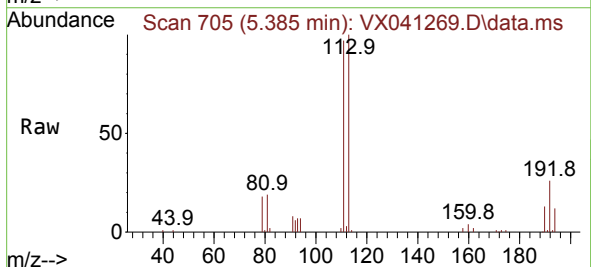






#36  
1,1-Dichloropropene  
Concen: 5.492 ug/l  
RT: 5.544 min Scan# 71  
Delta R.T. -0.146 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Instrument :  
MSVOA\_X  
ClientSampleId :







Tgt Ion: 75 Resp: 9210  
Ion Ratio Lower Upper  
75 100  
110 10.1 17.0 50.9#  
77 0.0 24.7 37.1#



#38  
Carbon Tetrachloride  
Concen: 6.910 ug/l  
RT: 5.544 min Scan# 731  
Delta R.T. -0.128 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 117 Resp: 12943  
Ion Ratio Lower Upper  
117 100  
119 7.0 78.2 117.2#  
121 0.0 24.4 36.6#


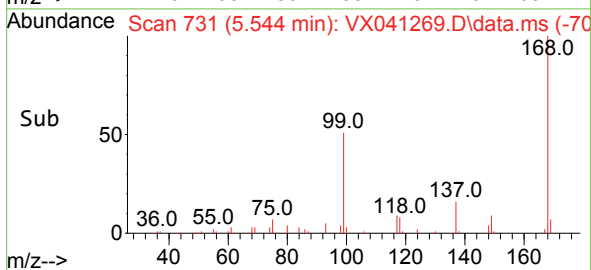






#41  
Methacrylonitrile  
Concen: 0.200 ug/l  
RT: 5.038 min Scan# 64  
Delta R.T. 0.110 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 41 Resp: 192  
Ion Ratio Lower Upper  
41 100  
39 21.4 45.2 67.8#  
67 0.0 52.6 78.8#  
52 0.0 22.7 34.1#

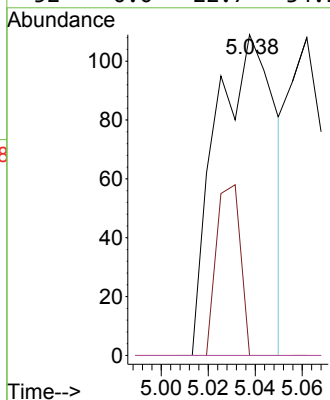

#50  
Toluene-d8  
Concen: 56.724 ug/l  
RT: 8.647 min Scan# 1240  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion: 98 Resp: 250830  
Ion Ratio Lower Upper  
98 100  
100 65.7 53.1 79.7


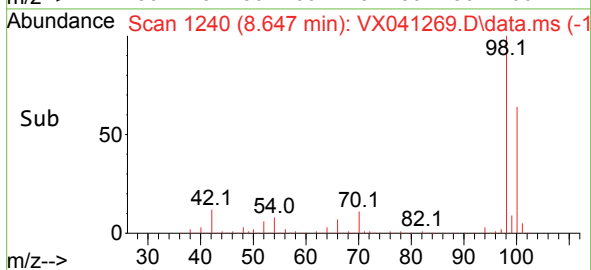
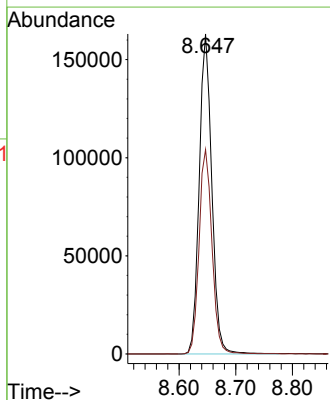





#51  
4-Methyl-2-Pentanone  
Concen: 0.381 ug/l  
RT: 8.580 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 43 Resp: 706  
Ion Ratio Lower Upper  
43 100  
58 36.7 30.4 45.6

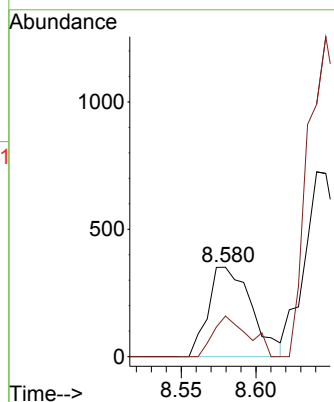

#59  
2-Hexanone  
Concen: 0.363 ug/l  
RT: 9.457 min Scan# 1373  
Delta R.T. 0.024 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Tgt Ion: 43 Resp: 517  
Ion Ratio Lower Upper  
43 100  
58 44.3 26.2 78.5

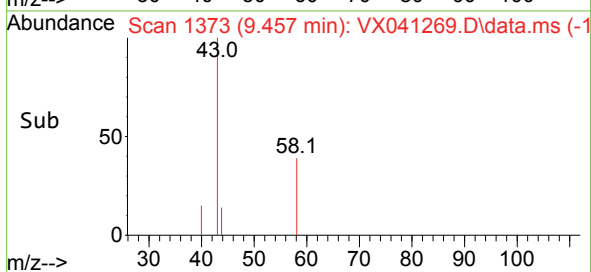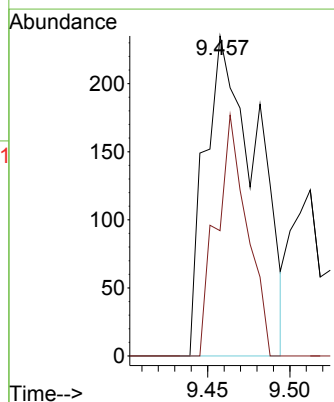






#62  
4-Bromofluorobenzene  
Concen: 56.920 ug/l  
RT: 11.079 min Scan# 1639  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53


Instrument :  
MSVOA\_X  
ClientSampleId :





Tgt Ion: 95 Resp: 92901  
Ion Ratio Lower Upper  
95 100  
174 99.0 0.0 135.6  
176 96.3 0.0 131.0

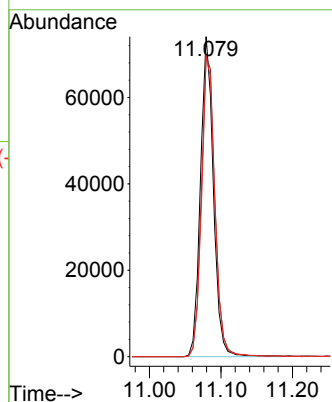


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 10.055 min Scan# 1471  
Delta R.T. -0.000 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Tgt Ion: 117 Resp: 201717  
Ion Ratio Lower Upper  
117 100  
82 49.2 46.2 69.4  
119 33.8 25.5 38.3

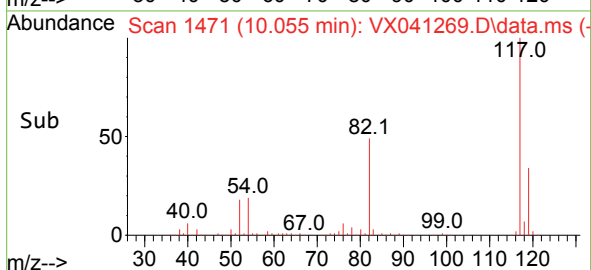






#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.000 ug/l  
 RT: 12.024 min Scan# 11  
 Delta R.T. -0.000 min  
 Lab File: VX041269.D  
 Acq: 29 Apr 2024 11:53


Instrument :  
 MSVOA\_X  
 ClientSampleId :

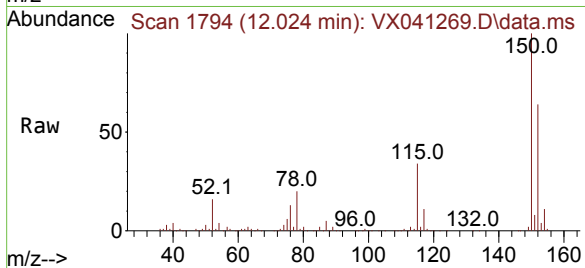



Tgt Ion:152 Resp: 105999  
 Ion Ratio Lower Upper  
 152 100  
 115 53.5 43.3 129.9  
 150 155.1 0.0 345.0

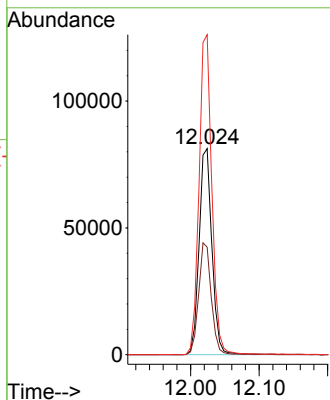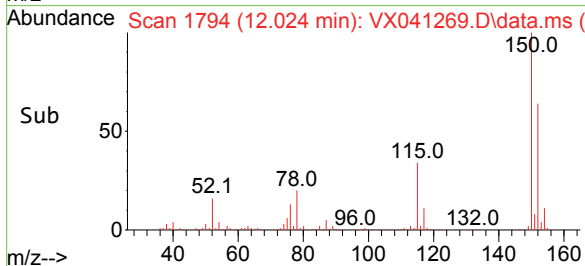


#76  
 1,2,3-Trichloropropane  
 Concen: 27.736 ug/l  
 RT: 11.079 min Scan# 1639  
 Delta R.T. -0.159 min  
 Lab File: VX041269.D  
 Acq: 29 Apr 2024 11:53

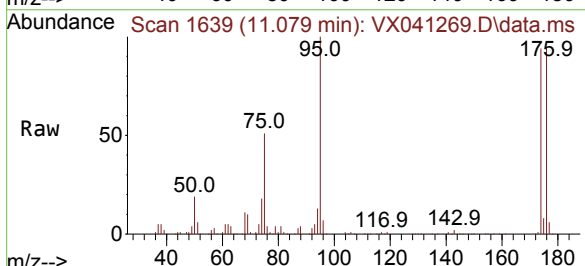

Tgt Ion: 75 Resp: 47368  
 Ion Ratio Lower Upper  
 75 100  
 77 1.3 19.1 57.5#



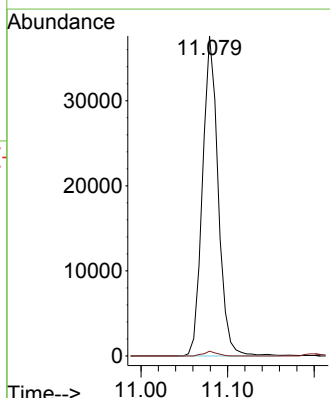
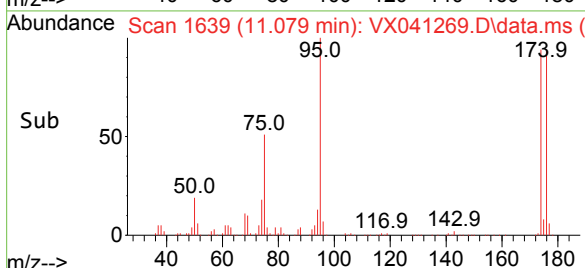




#81  
trans-1,4-Dichloro-2-butene  
Concen: 78.251 ug/l  
RT: 11.079 min Scan# 1  
Delta R.T. 0.061 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53




Instrument :  
MSVOA\_X  
ClientSampleId :


Tgt Ion: 75 Resp: 47368  
Ion Ratio Lower Upper  
75 100  
53 0.0 90.5 135.7#  
89 0.0 36.9 55.3#

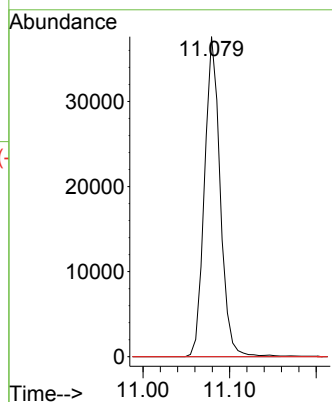

#93  
1,2,4-Trichlorobenzene  
Concen: 0.426 ug/l  
RT: 13.597 min Scan# 2052  
Delta R.T. 0.012 min  
Lab File: VX041269.D  
Acq: 29 Apr 2024 11:53

Tgt Ion:180 Resp: 1021  
Ion Ratio Lower Upper  
180 100  
182 76.5 48.3 144.8  
145 23.9 18.0 54.0

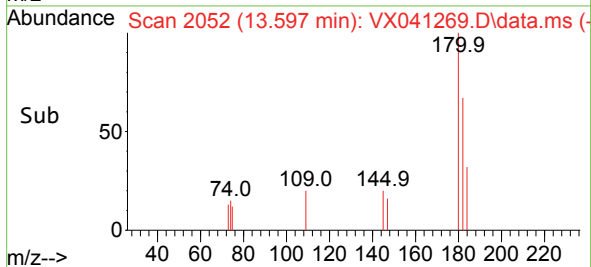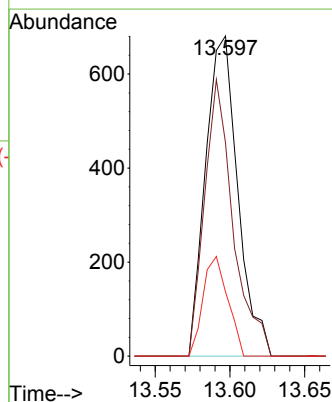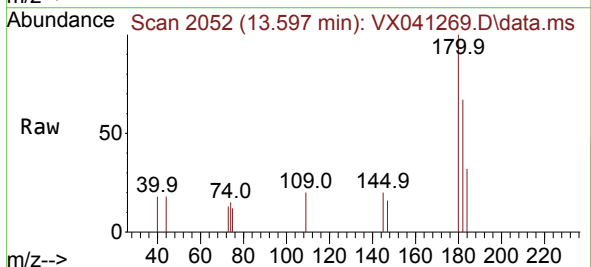



#95

Naphthalene

Concen: 0.595 ug/l

RT: 13.780 min Scan# 2081

Delta R.T. 0.006 min

Lab File: VX041269.D





Acq: 29 Apr 2024 11:53

Instrument :

MSVOA\_X

ClientSampleId :

|             |       |           |
|-------------|-------|-----------|
| Tgt Ion:128 | Resp: | 4092      |
| Ion Ratio   | Lower | Upper     |
| 128         | 100   |           |
| 127         | 11.2  | 10.3 15.5 |
| 129         | 8.4   | 8.8 13.2# |

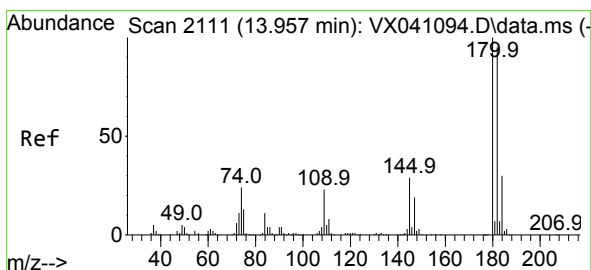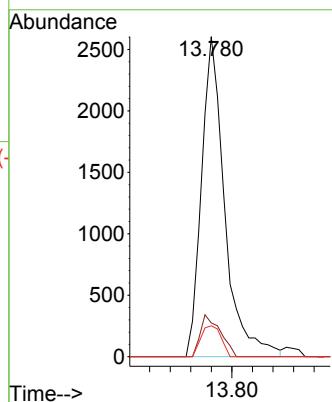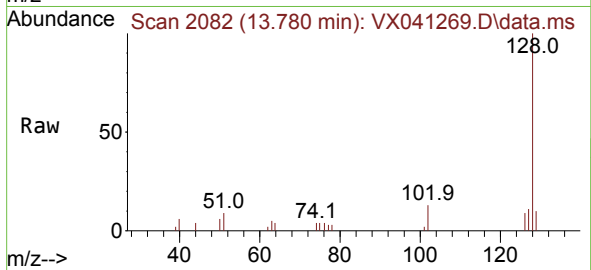

#96

1,2,3-Trichlorobenzene

Concen: 0.441 ug/l

RT: 13.963 min Scan# 2112

Delta R.T. -0.000 min

Lab File: VX041269.D

Acq: 29 Apr 2024 11:53

|             |       |            |
|-------------|-------|------------|
| Tgt Ion:180 | Resp: | 1113       |
| Ion Ratio   | Lower | Upper      |
| 180         | 100   |            |
| 182         | 99.3  | 46.9 140.6 |
| 145         | 26.8  | 17.8 53.5  |

