


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX043020\
 Data File : VX015986.D
 Acq On : 30 Apr 2020 10:04
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X043020W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Thu Apr 30 12:42:44 2020

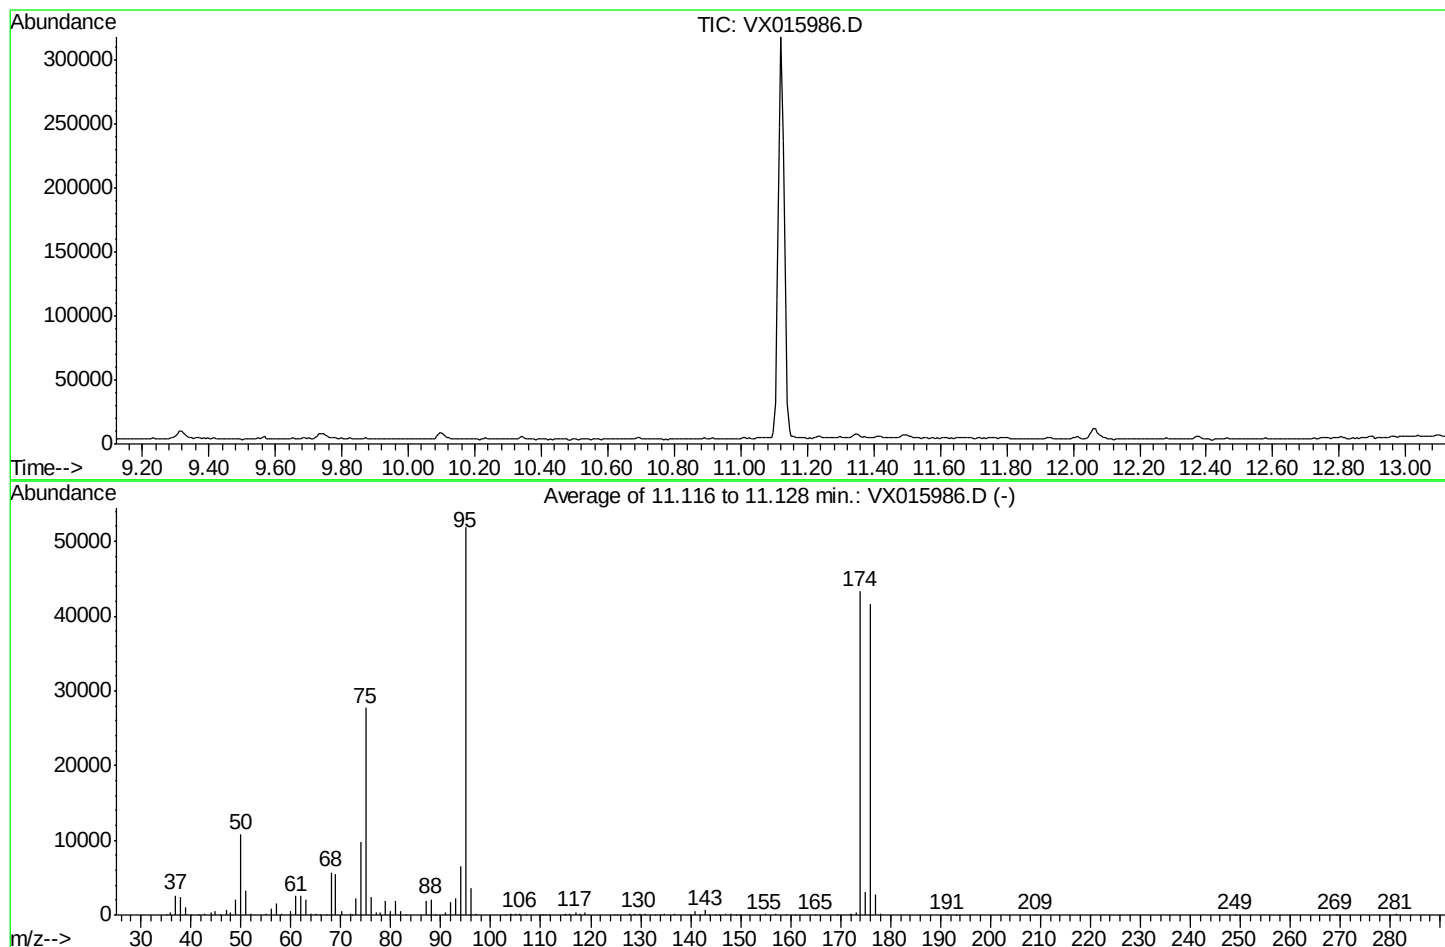

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1640

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10791	PASS
75	95	30	60	53.4	27701	PASS
95	95	100	100	100.0	51882	PASS
96	95	5	9	6.8	3545	PASS
173	174	0.00	2	0.8	345	PASS
174	95	50	100	83.5	43328	PASS
175	174	5	9	7.3	3166	PASS
176	174	95	101	96.0	41600	PASS
177	176	5	9	6.7	2771	PASS