

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043024\
 Data File : VX041308.D
 Acq On : 30 Apr 2024 18:35
 Operator : JC/MD
 Sample : P2264-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 01 02:50:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 02:38:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	181737	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	268177	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	252022	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	133438	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	98176	49.622	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	99.240%		
35) Dibromofluoromethane	5.385	113	80310	44.191	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.380%		
50) Toluene-d8	8.647	98	262970	45.717	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	91.440%#		
62) 4-Bromofluorobenzene	11.079	95	116287	52.225	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.440%		
Target Compounds						
						Qvalue
3) Chloromethane	1.295	50	345	0.223	ug/l	92
5) Bromomethane	1.599	94	218	0.236	ug/l	# 37
11) Tert butyl alcohol	3.008	59	975	2.462	ug/l	# 78
15) Acrylonitrile	3.123	53	867	0.959	ug/l	# 23
16) Acetone	2.398	43	6961	4.143	ug/l	92
18) Methyl Acetate	2.709	43	406	0.201	ug/l	# 53
19) Methyl tert-butyl Ether	3.117	73	80313	15.644	ug/l	99
20) Methylene Chloride	2.794	84	864	0.503	ug/l	# 85
25) 2-Butanone	4.629	43	290	0.226	ug/l	# 51
31) Cyclohexane	5.465	56	7251	3.037	ug/l	86
36) 1,1-Dichloropropene	5.544	75	10834	4.985	ug/l	# 51
38) Carbon Tetrachloride	5.544	117	15633	6.280	ug/l	# 15
39) Methylcyclohexane	7.373	83	2702	1.058	ug/l	86
51) 4-Methyl-2-Pentanone	8.641	43	1311	0.536	ug/l	# 1
55) 1,1,2-Trichloroethane	9.098	97	1445	0.916	ug/l	# 20
69) o-Xylene	10.646	106	896	0.277	ug/l	90
73) Isopropylbenzene	10.964	105	70230	8.622	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	58256	26.789	ug/l	# 39
78) n-propylbenzene	11.305	91	14965	1.749	ug/l	99
79) 2-Chlorotoluene	11.305	91	14965	2.715	ug/l	# 42
81) trans-1,4-Dichloro-2-b...	11.079	75	58256	72.970	ug/l	# 5
82) 4-Chlorotoluene	11.305	91	14965	2.391	ug/l	# 46
83) tert-Butylbenzene	11.713	119	16075	2.261	ug/l	98
84) 1,2,4-Trimethylbenzene	11.890	105	62714	9.387	ug/l	# 33
85) sec-Butylbenzene	11.890	105	62714	7.696	ug/l	# 75
86) p-Isopropyltoluene	12.177	119	41896	5.725	ug/l	96
89) n-Butylbenzene	12.329	91	6890	1.171	ug/l	# 68
90) Hexachloroethane	12.616	117	34527	28.211	ug/l	# 17
92) 1,2-Dibromo-3-Chloropr...	12.920	75	2524	4.092	ug/l	# 10
95) Naphthalene	13.792	128	2597	0.284	ug/l	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043024\
Data File : VX041308.D
Acq On : 30 Apr 2024 18:35
Operator : JC/MD
Sample : P2264-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 01 02:50:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 01 02:38:17 2024
Response via : Initial Calibration




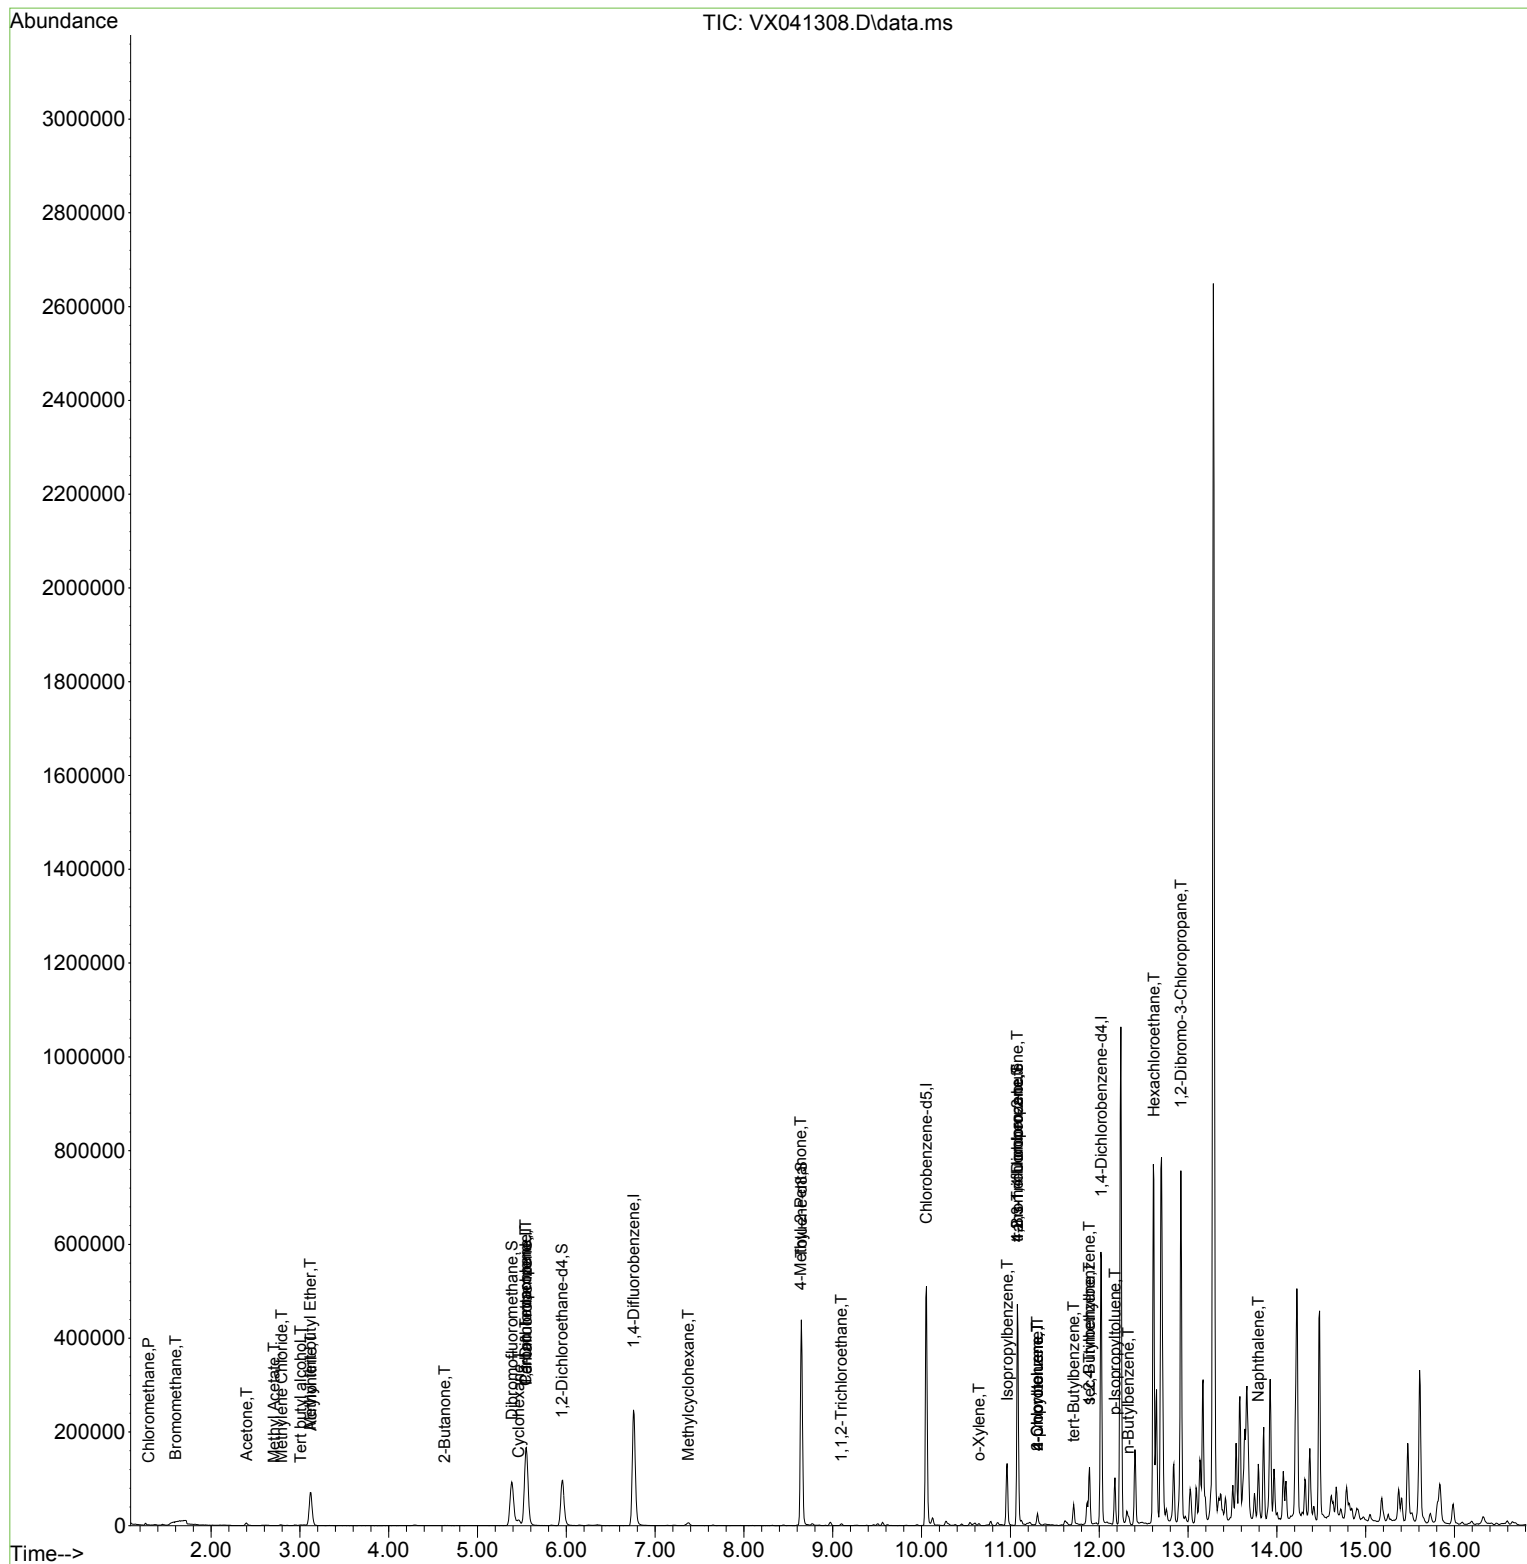




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 181737
Ion Ratio Lower Upper
168 100
99 47.6 56.6 85.0#

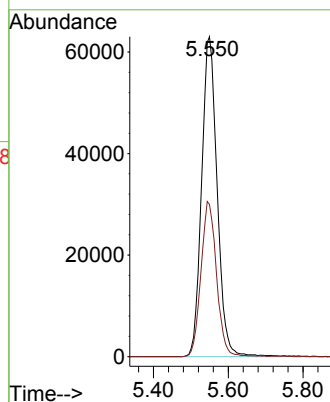

#3
Chloromethane
Concen: 0.223 ug/l
RT: 1.295 min Scan# 34
Delta R.T. -0.006 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 50 Resp: 345
Ion Ratio Lower Upper
50 100
52 27.3 25.5 38.3

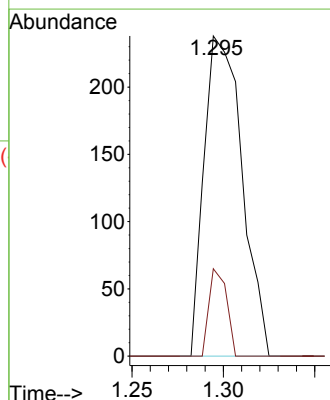

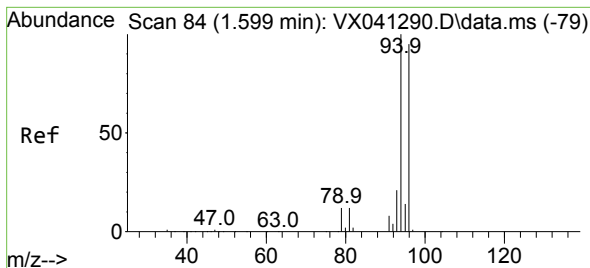

#5

Bromomethane

Concen: 0.236 ug/l

RT: 1.599 min Scan# 84

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 94 Resp: 218

Ion Ratio Lower Upper

94 100

96 154.0 74.6 111.8#

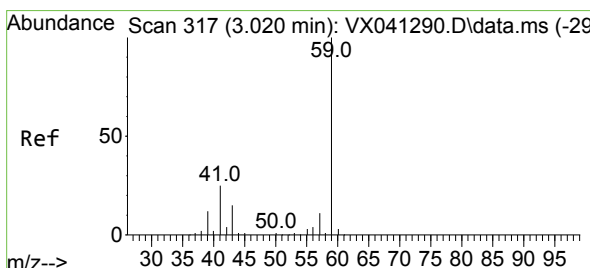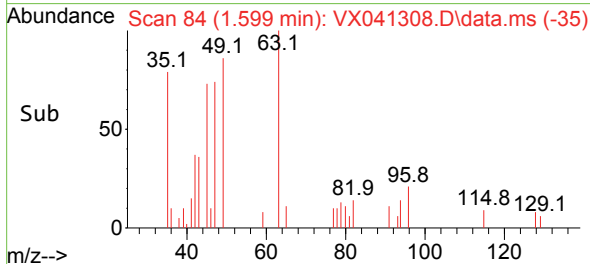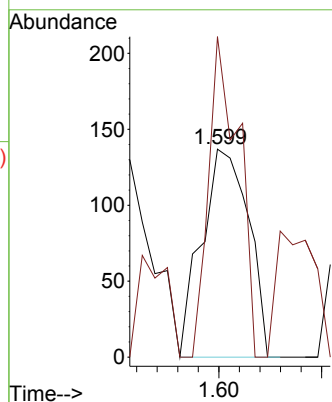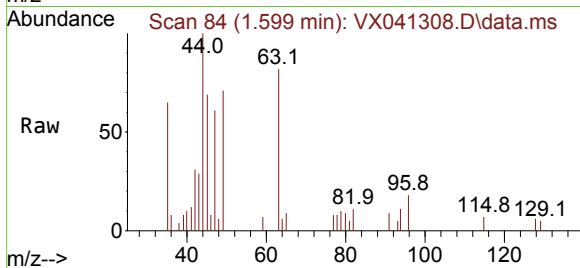

#11

Tert butyl alcohol

Concen: 2.462 ug/l

RT: 3.008 min Scan# 315

Delta R.T. -0.012 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 59 Resp: 975

Ion Ratio Lower Upper

59 100


57 0.0 6.0 9.0#

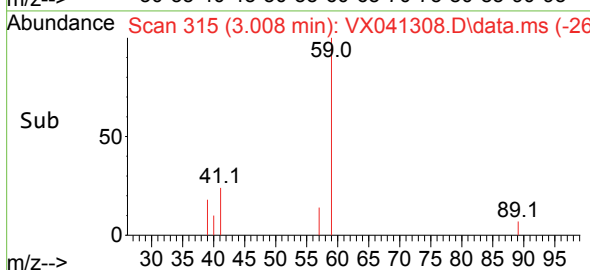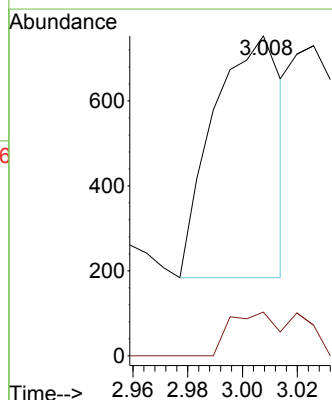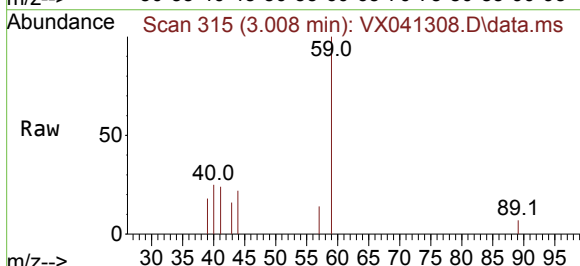






#15
Acrylonitrile
Concen: 0.959 ug/l
RT: 3.123 min Scan# 31
Delta R.T. 0.049 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 53 Resp: 867
Ion Ratio Lower Upper
53 100
52 6.1 66.0 99.0#
51 72.3 29.8 44.6#

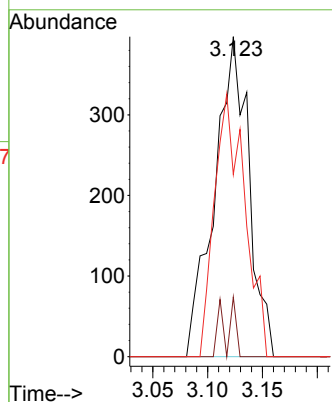

#16
Acetone
Concen: 4.143 ug/l
RT: 2.398 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 43 Resp: 6961
Ion Ratio Lower Upper
43 100
58 31.5 21.9 32.9

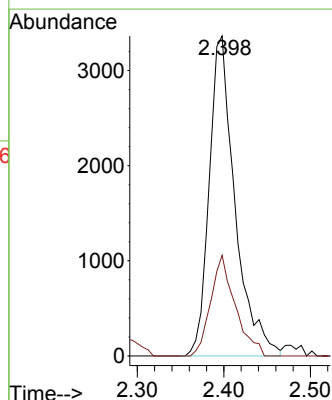



#18

Methyl Acetate

Concen: 0.201 ug/l

RT: 2.709 min Scan# 2

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 43 Resp: 406

Ion Ratio Lower Upper

43 100

74 0.0 17.8 26.8#

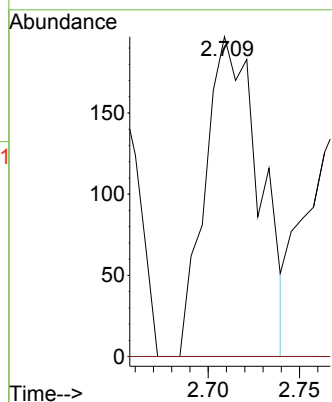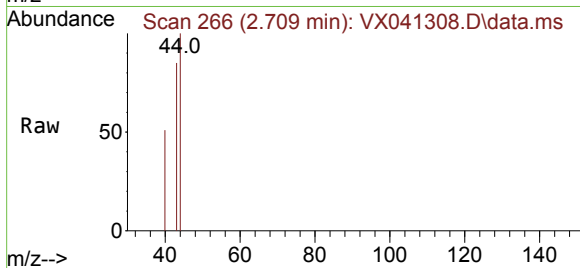

#19

Methyl tert-butyl Ether

Concen: 15.644 ug/l

RT: 3.117 min Scan# 333

Delta R.T. 0.000 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 73 Resp: 80313

Ion Ratio Lower Upper

73 100

57 21.9 17.3 25.9

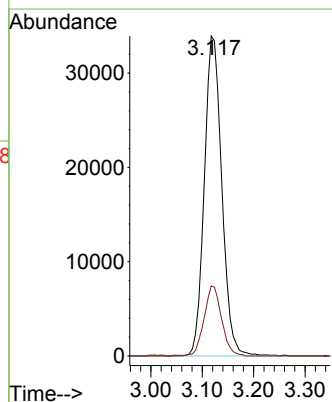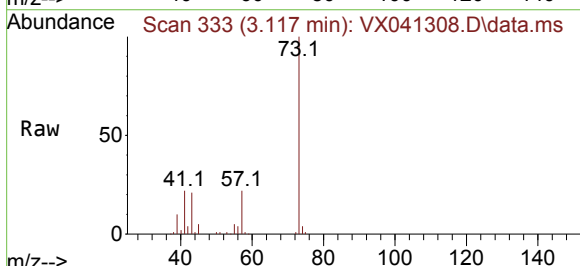



#20

Methylene Chloride

Concen: 0.503 ug/l

RT: 2.794 min Scan# 21

Delta R.T. 0.006 min


Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 84 Resp: 864




Ion Ratio Lower Upper

84 100

49 100.0 103.6 155.4#

51 38.9 33.8 50.6

86 60.9 49.4 74.0

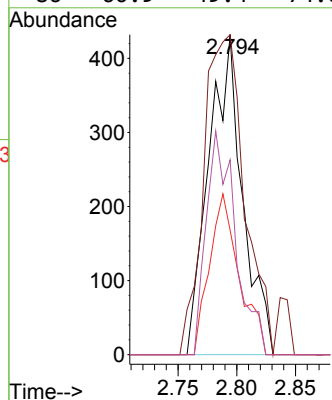

#25

2-Butanone

Concen: 0.226 ug/l

RT: 4.629 min Scan# 581

Delta R.T. 0.061 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 43 Resp: 290

Ion Ratio Lower Upper

43 100


72 0.0 19.4 29.2#

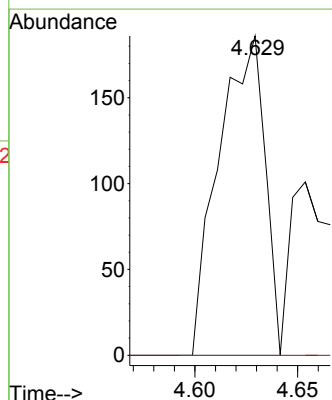



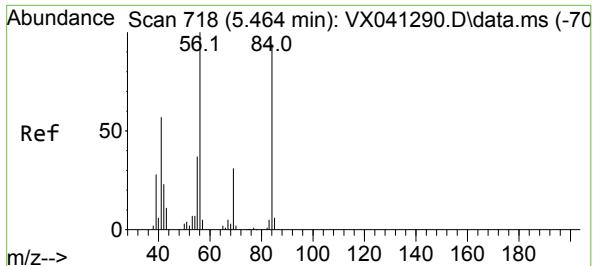


#31
Cyclohexane
Concen: 3.037 ug/l
RT: 5.465 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :



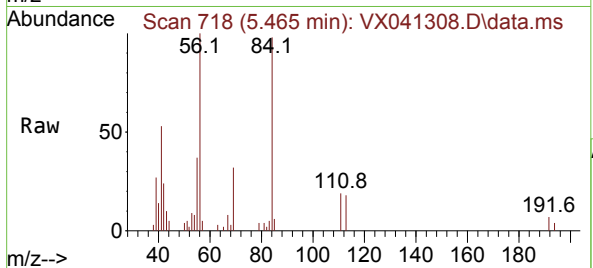



Tgt Ion: 56 Resp: 7251
Ion Ratio Lower Upper
56 100
69 32.1 23.4 35.2
84 98.0 65.9 98.9

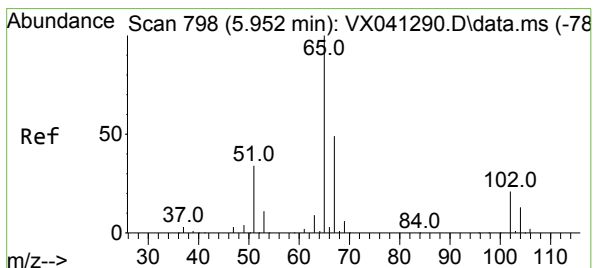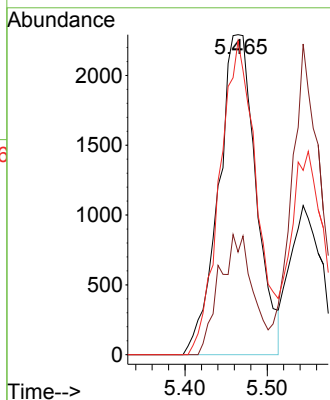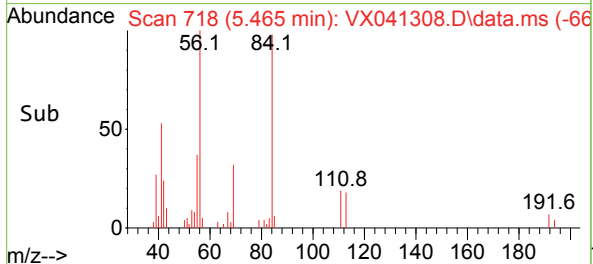

#33
1,2-Dichloroethane-d4
Concen: 49.622 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 65 Resp: 98176
Ion Ratio Lower Upper
65 100
67 50.4 0.0 100.2


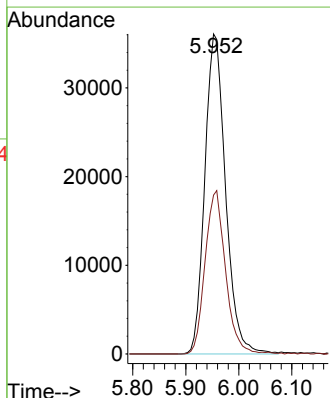
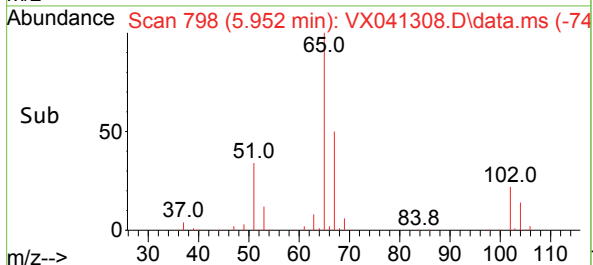
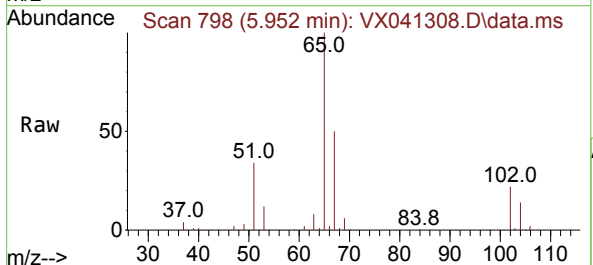




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 268177
Ion Ratio Lower Upper
114 100
63 19.1 0.0 45.0
88 16.0 0.0 36.6

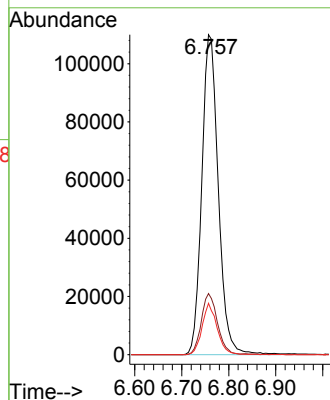

#35
Dibromofluoromethane
Concen: 44.191 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35


Tgt Ion:113 Resp: 80310
Ion Ratio Lower Upper
113 100
111 103.8 82.9 124.3
192 25.3 13.3 19.9#

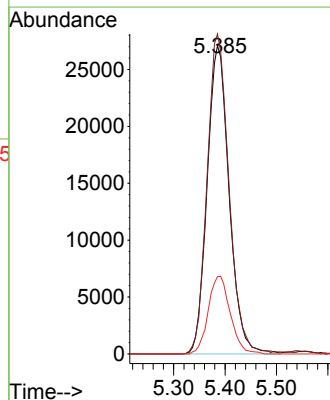






#36
1,1-Dichloropropene
Concen: 4.985 ug/l
RT: 5.544 min Scan# 711
Delta R.T. -0.146 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35


Instrument :
MSVOA_X
ClientSampleId :





Tgt Ion: 75 Resp: 10834
Ion Ratio Lower Upper
75 100
110 10.1 17.0 50.9#
77 0.0 24.7 37.1#

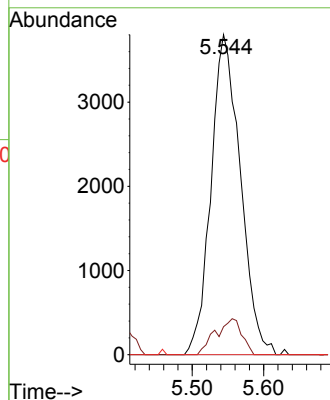


#38
Carbon Tetrachloride
Concen: 6.280 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.128 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35



Tgt Ion: 117 Resp: 15633
Ion Ratio Lower Upper
117 100
119 5.3 78.2 117.2#
121 0.0 24.4 36.6#

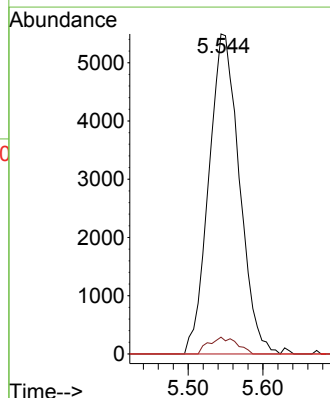



#39

Methylcyclohexane

Concen: 1.058 ug/l

RT: 7.373 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 2702

Ion Ratio Lower Upper

83 100

55 95.5 64.6 97.0

98 40.6 36.7 55.1

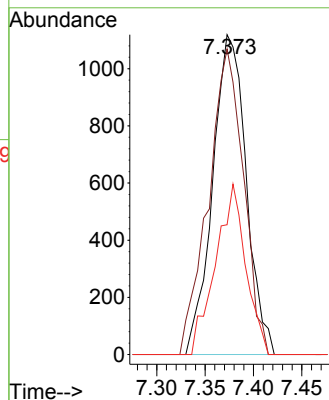

#50

Toluene-d8

Concen: 45.717 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 98 Resp: 262970

Ion Ratio Lower Upper

98 100

100 66.4 53.1 79.7


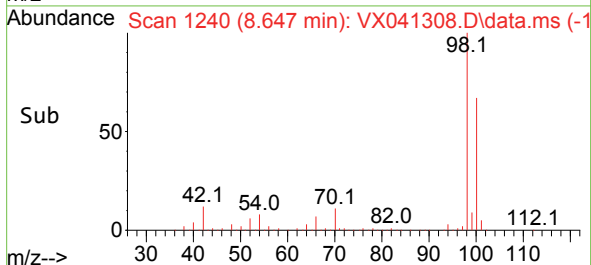
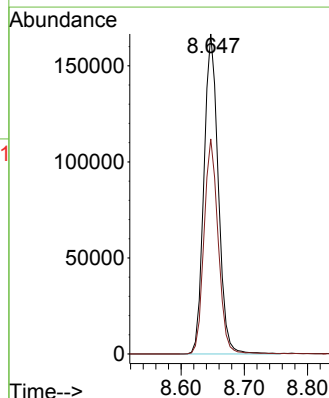
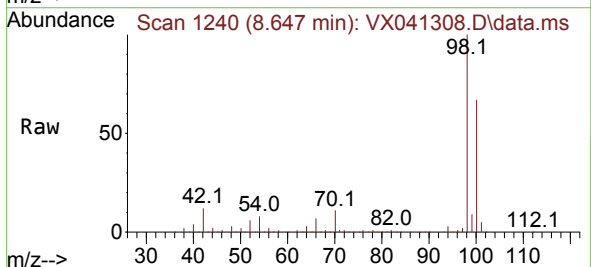




#51
4-Methyl-2-Pentanone
Concen: 0.536 ug/l
RT: 8.641 min Scan# 1311
Delta R.T. 0.061 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1311
Ion Ratio Lower Upper
43 100
58 156.2 30.4 45.6#

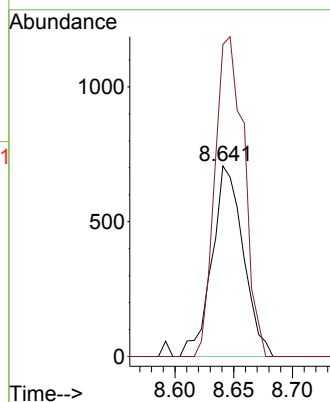

#55
1,1,2-Trichloroethane
Concen: 0.916 ug/l
RT: 9.098 min Scan# 1314
Delta R.T. -0.055 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35


Tgt Ion: 97 Resp: 1445
Ion Ratio Lower Upper
97 100
83 6.0 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#

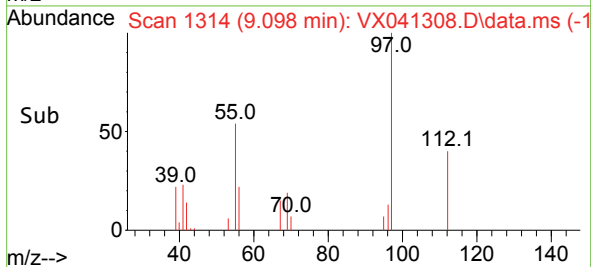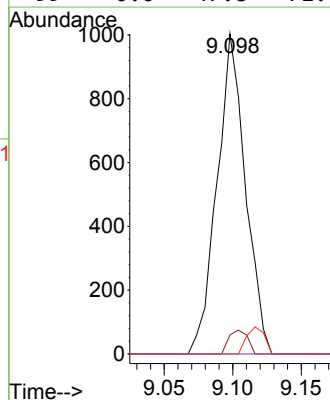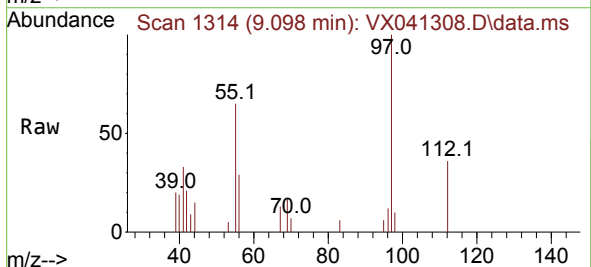






#62
4-Bromofluorobenzene
Concen: 52.225 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 95 Resp: 116287
Ion Ratio Lower Upper
95 100
174 96.5 0.0 135.6
176 95.1 0.0 131.0

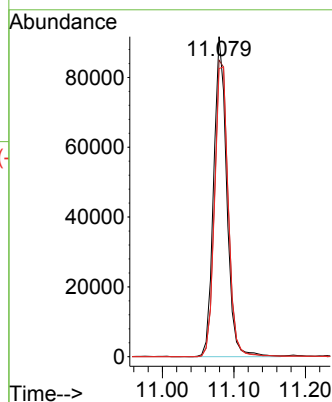

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 117 Resp: 252022
Ion Ratio Lower Upper
117 100
82 49.2 46.2 69.4
119 32.2 25.5 38.3

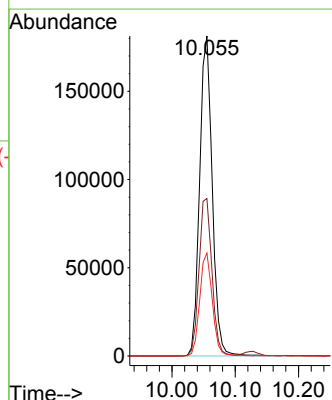



#69

o-Xylene

Concen: 0.277 ug/l

RT: 10.646 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:106 Resp: 896

Ion Ratio Lower Upper

106 100

91 234.5 108.9 326.8

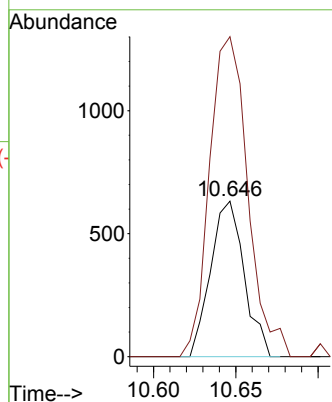

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35




Tgt Ion:152 Resp: 133438


Ion Ratio Lower Upper

152 100

115 53.7 43.3 129.9

150 156.6 0.0 345.0

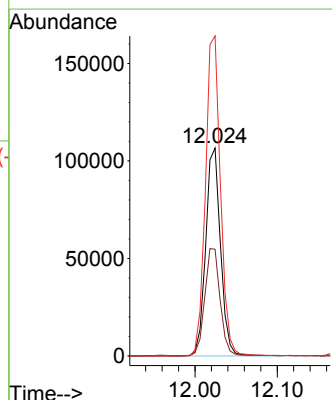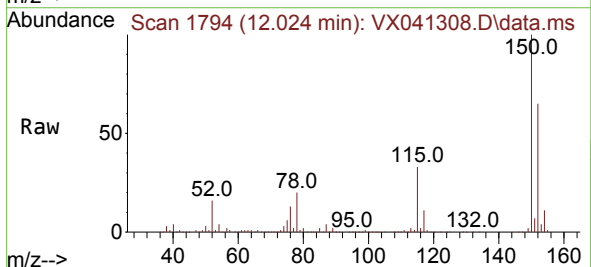



#73

Isopropylbenzene

Concen: 8.622 ug/l

RT: 10.964 min Scan# 1639

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 70230

Ion Ratio Lower Upper

105 100

120 26.6 12.9 38.6

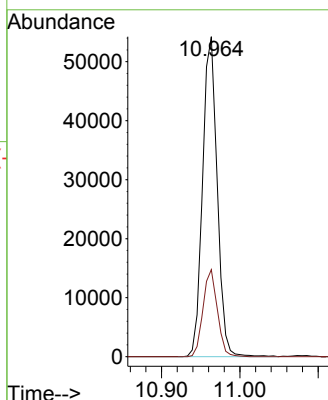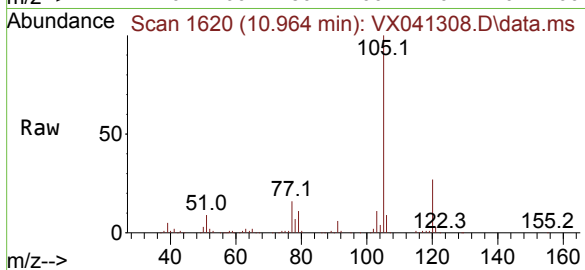

#76

1,2,3-Trichloropropane

Concen: 26.789 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 75 Resp: 58256

Ion Ratio Lower Upper

75 100

77 1.3 19.1 57.5#

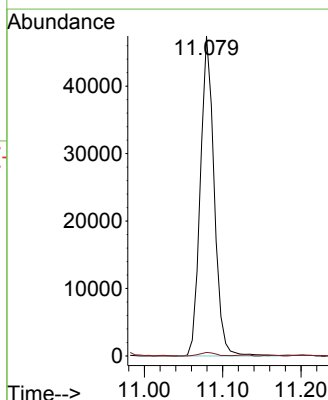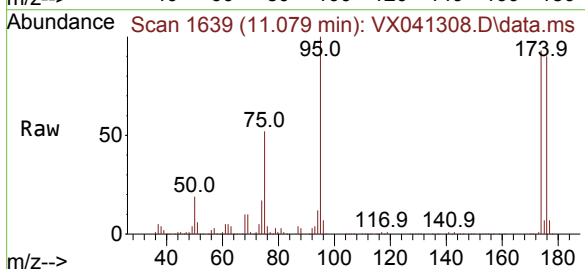



#78

n-propylbenzene

Concen: 1.749 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 14965

Ion Ratio Lower Upper

91 100

120 23.2 11.5 34.4

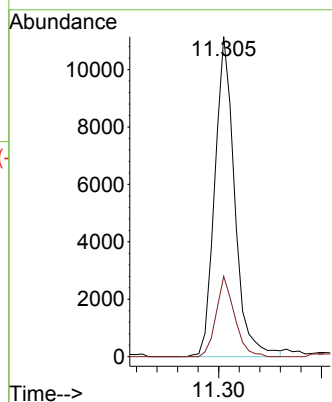

#79

2-Chlorotoluene

Concen: 2.715 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.061 min

Lab File: VX041308.D




Acq: 30 Apr 2024 18:35


Tgt Ion: 91 Resp: 14965

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#



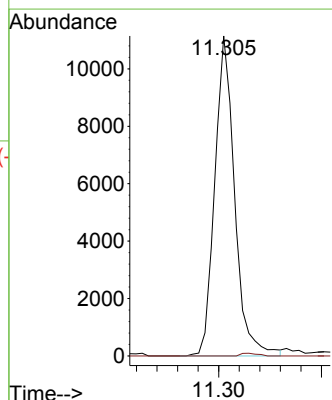





#81
trans-1,4-Dichloro-2-butene
Concen: 72.970 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 58256
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

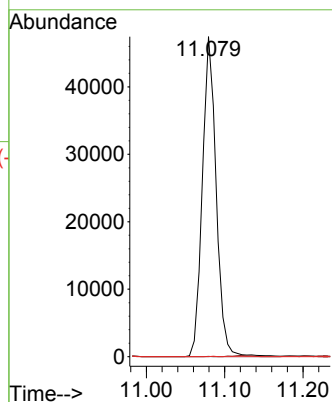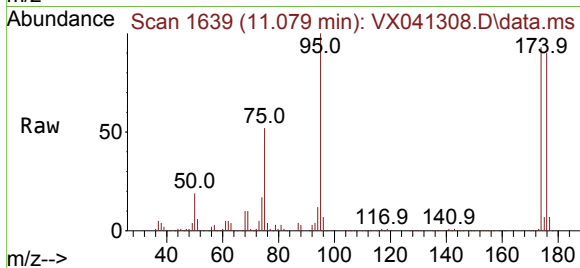

#82
4-Chlorotoluene
Concen: 2.391 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.146 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 91 Resp: 14965
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#

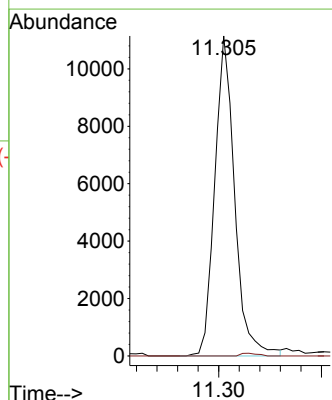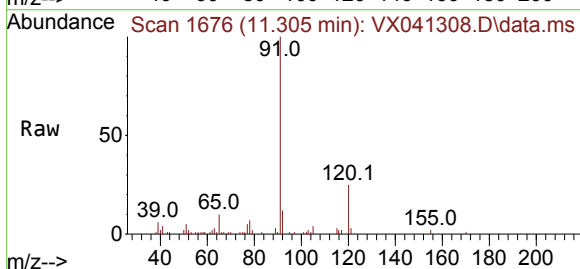



#83

tert-Butylbenzene

Concen: 2.261 ug/l

RT: 11.713 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX041308.D





Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:	119	Resp:	16075
Ion	Ratio	Lower	Upper
119	100		
91	63.0	31.2	93.6
134	25.8	11.7	35.0

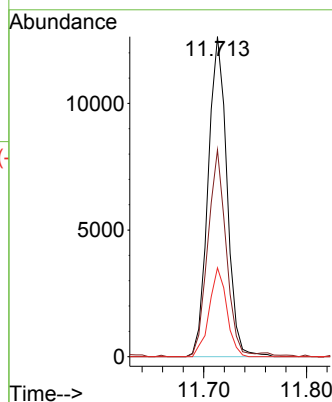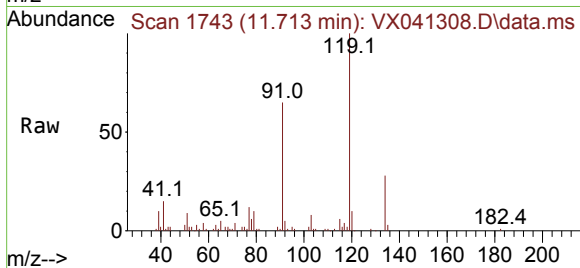

#84

1,2,4-Trimethylbenzene

Concen: 9.387 ug/l




RT: 11.890 min Scan# 1772


Delta R.T. 0.140 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Tgt Ion:	105	Resp:	62714
Ion	Ratio	Lower	Upper
105	100		
120	0.1	21.2	63.6#

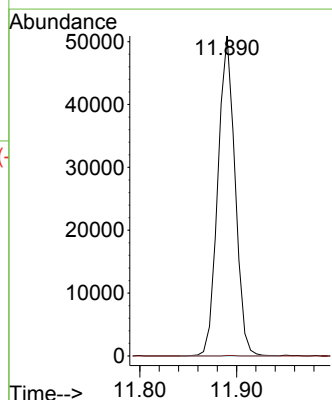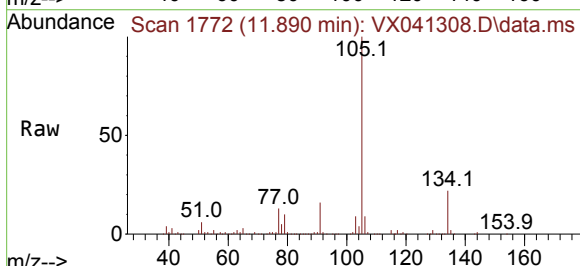



#85

sec-Butylbenzene

Concen: 7.696 ug/l

RT: 11.890 min Scan# 11

Delta R.T. 0.000 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 62714

Ion Ratio Lower Upper

105 100

134 30.9 9.8 29.4#

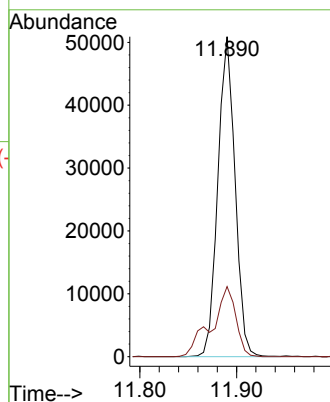

#86

p-Isopropyltoluene

Concen: 5.725 ug/l

RT: 12.177 min Scan# 1819

Delta R.T. 0.171 min

Lab File: VX041308.D

Acq: 30 Apr 2024 18:35




Tgt Ion:119 Resp: 41896


Ion Ratio Lower Upper

119 100

134 27.6 12.8 38.3

91 24.5 13.1 39.3



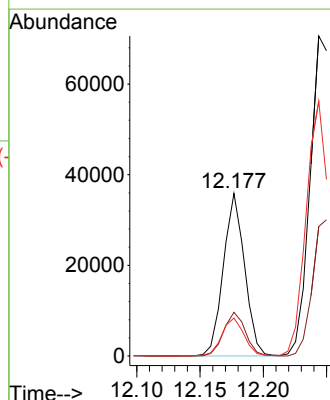





#89
n-Butylbenzene
Concen: 1.171 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. 0.000 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 6890
Ion Ratio Lower Upper
91 100
92 44.5 27.4 82.0
134 61.4 12.6 37.8#

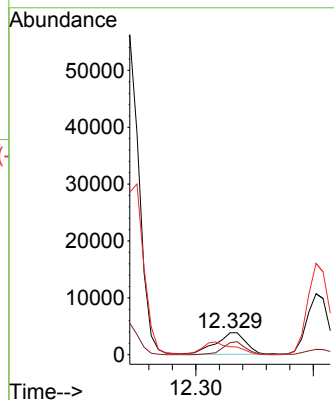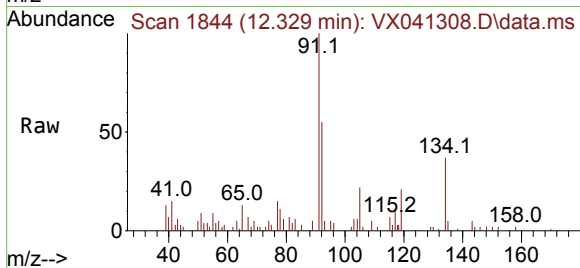

#90
Hexachloroethane
Concen: 28.211 ug/l
RT: 12.616 min Scan# 1891
Delta R.T. 0.079 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35


Tgt Ion: 117 Resp: 34527
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

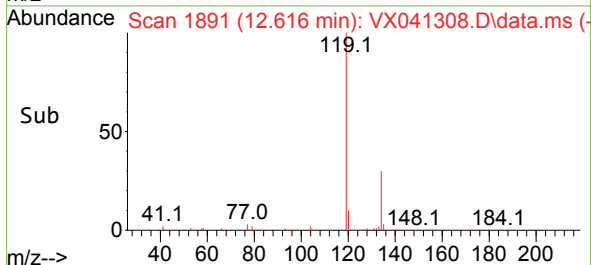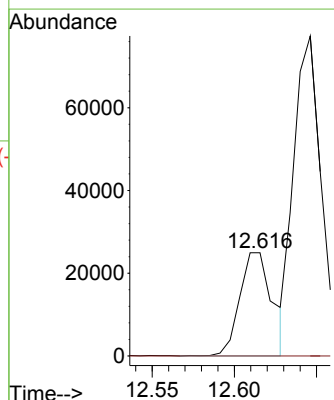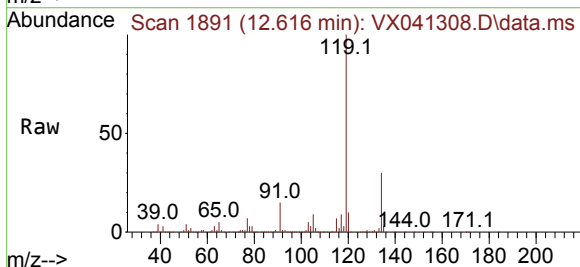






#92
1,2-Dibromo-3-Chloropropane
Concen: 4.092 ug/l
RT: 12.920 min Scan# 1941
Delta R.T. -0.018 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Instrument :
MSVOA_X
ClientSampleId :

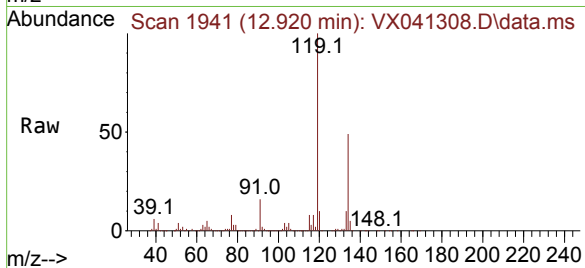

Tgt Ion: 75 Resp: 2524
Ion Ratio Lower Upper
75 100
155 2.1 36.1 108.5#
157 0.0 44.9 134.7#

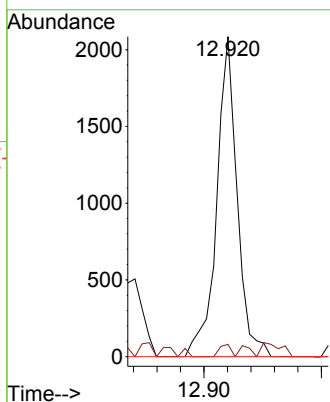

#95
Naphthalene
Concen: 0.284 ug/l
RT: 13.792 min Scan# 2084
Delta R.T. 0.018 min
Lab File: VX041308.D
Acq: 30 Apr 2024 18:35

Tgt Ion: 128 Resp: 2597
Ion Ratio Lower Upper
128 100
127 35.2 10.3 15.5#
129 77.1 8.8 13.2#

