
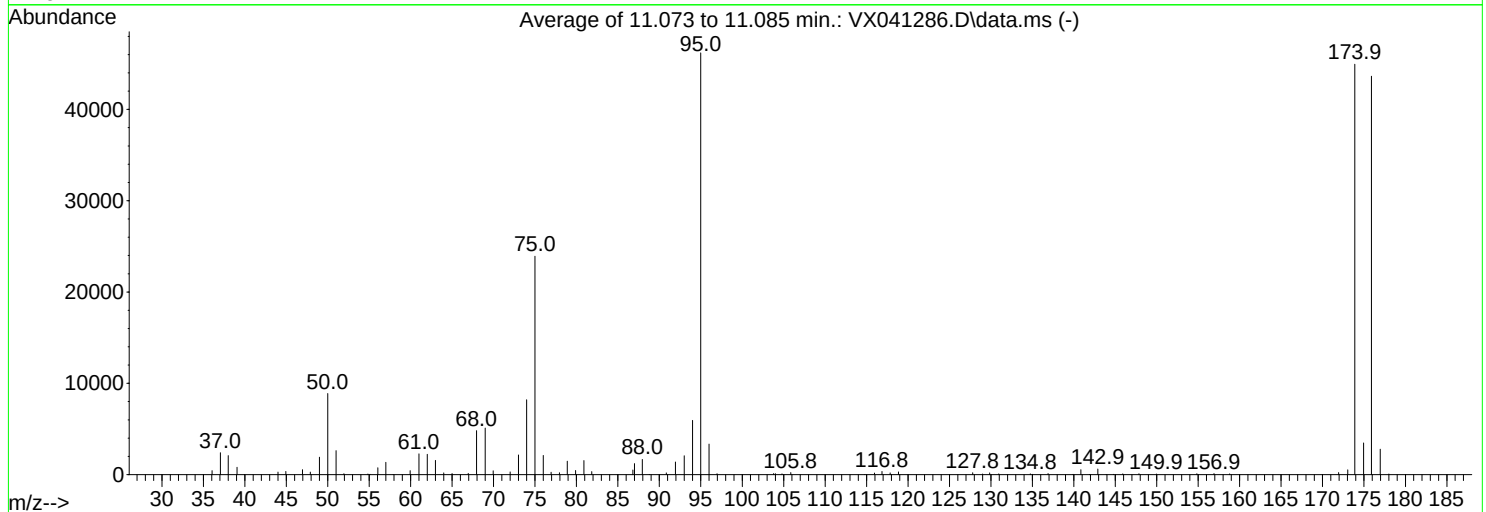


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043024\
Data File : VX041286.D
Acq On : 30 Apr 2024 08:14
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Title : SW846 8260
Last Update : Wed May 01 02:38:17 2024

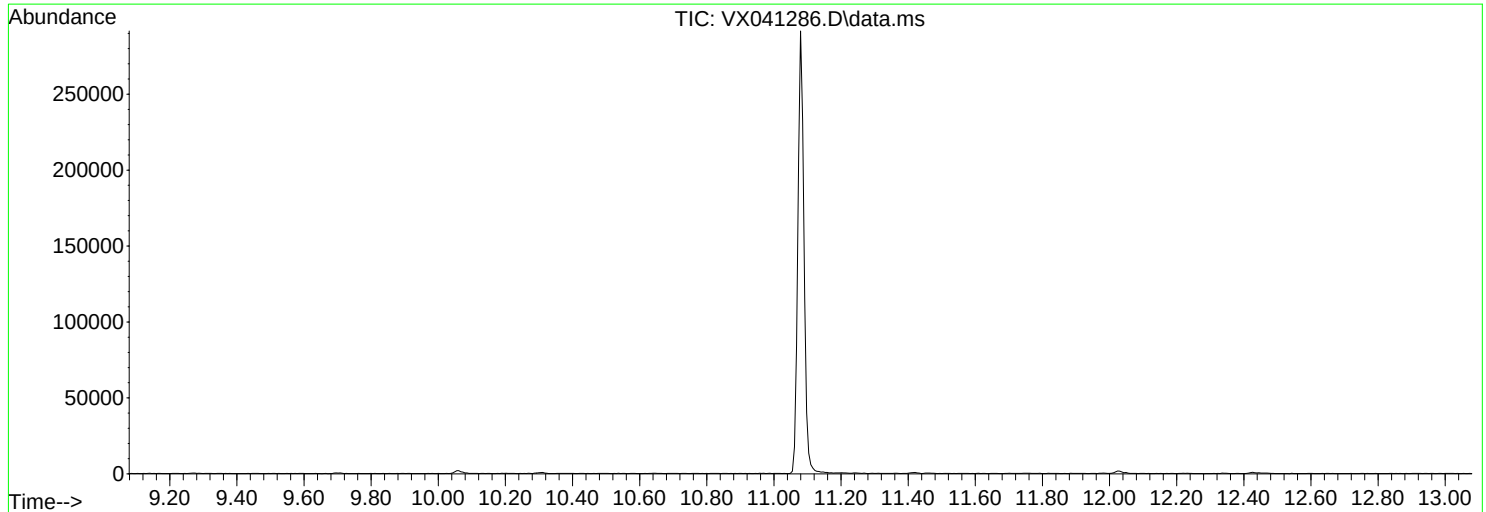

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.2	8878	PASS
75	95	30	60	51.8	23915	PASS
95	95	100	100	100.0	46195	PASS
96	95	5	9	7.2	3347	PASS
173	174	0.00	2	1.2	528	PASS
174	95	50	100	97.3	44944	PASS
175	174	5	9	7.7	3462	PASS
176	174	95	101	97.1	43640	PASS
177	176	5	9	6.4	2784	PASS