

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043025\
 Data File : VX045995.D
 Acq On : 30 Apr 2025 14:06
 Operator : JC/MD
 Sample : Q1915-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-04282025

Quant Time: May 01 03:37:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	56553	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	111268	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	107559	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	44562	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	58476	56.542	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 113.080%			
35) Dibromofluoromethane	5.379	113	43365	54.931	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 109.860%			
50) Toluene-d8	8.647	98	146921	53.320	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 106.640%			
62) 4-Bromofluorobenzene	11.079	95	53005	52.810	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 105.620%			
Target Compounds						Qvalue
6) Chloroethane	1.684	64	268	0.635	ug/l #	42
8) Diethyl Ether	2.136	74	100	0.251	ug/l #	1
11) Tert butyl alcohol	2.977	59	247	1.777	ug/l #	72
13) Acrolein	2.233	56	73	0.381	ug/l	85
16) Acetone	2.386	43	21932	51.644	ug/l	98
18) Methyl Acetate	2.703	43	1759	1.799	ug/l	96
20) Methylene Chloride	2.788	84	6417	8.071	ug/l	95
29) Tetrahydrofuran	5.031	42	153	0.380	ug/l #	60
31) Cyclohexane	5.543	56	1645	1.297	ug/l #	29
36) 1,1-Dichloropropene	5.550	75	5333	5.003	ug/l #	51
38) Carbon Tetrachloride	5.550	117	6820	5.920	ug/l #	15
41) Methacrylonitrile	5.031	41	142	0.200	ug/l #	40
43) Isopropyl Acetate	6.348	43	10089	4.956	ug/l	98
48) Methyl methacrylate	7.793	41	43939	41.800	ug/l #	50
51) 4-Methyl-2-Pentanone	8.549	43	36809	27.273	ug/l #	52
53) t-1,3-Dichloropropene	8.958	75	193	2.443	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	14160	12.101	ug/l #	68
57) 1,3-Dichloropropane	9.482	76	1344	0.983	ug/l #	42
59) 2-Hexanone	9.378	43	11437	11.443	ug/l #	28
68) m/p-Xylenes	10.299	106	400	0.267	ug/l	74
69) o-Xylene	10.640	106	827	0.561	ug/l	86
74) N-amyl acetate	10.780	43	1386	0.812	ug/l #	49
76) 1,2,3-Trichloropropane	11.079	75	31155	28.662	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.451	105	1814	0.615	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	31155	97.276	ug/l #	1
84) 1,2,4-Trimethylbenzene	11.756	105	3197	1.079	ug/l	94
89) n-Butylbenzene	12.323	91	588	0.229	ug/l #	29
90) Hexachloroethane	12.536	117	145	0.285	ug/l #	19
95) Naphthalene	13.780	128	995	0.322	ug/l #	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043025\
Data File : VX045995.D
Acq On : 30 Apr 2025 14:06
Operator : JC/MD
Sample : Q1915-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Quant Time: May 01 03:37:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration

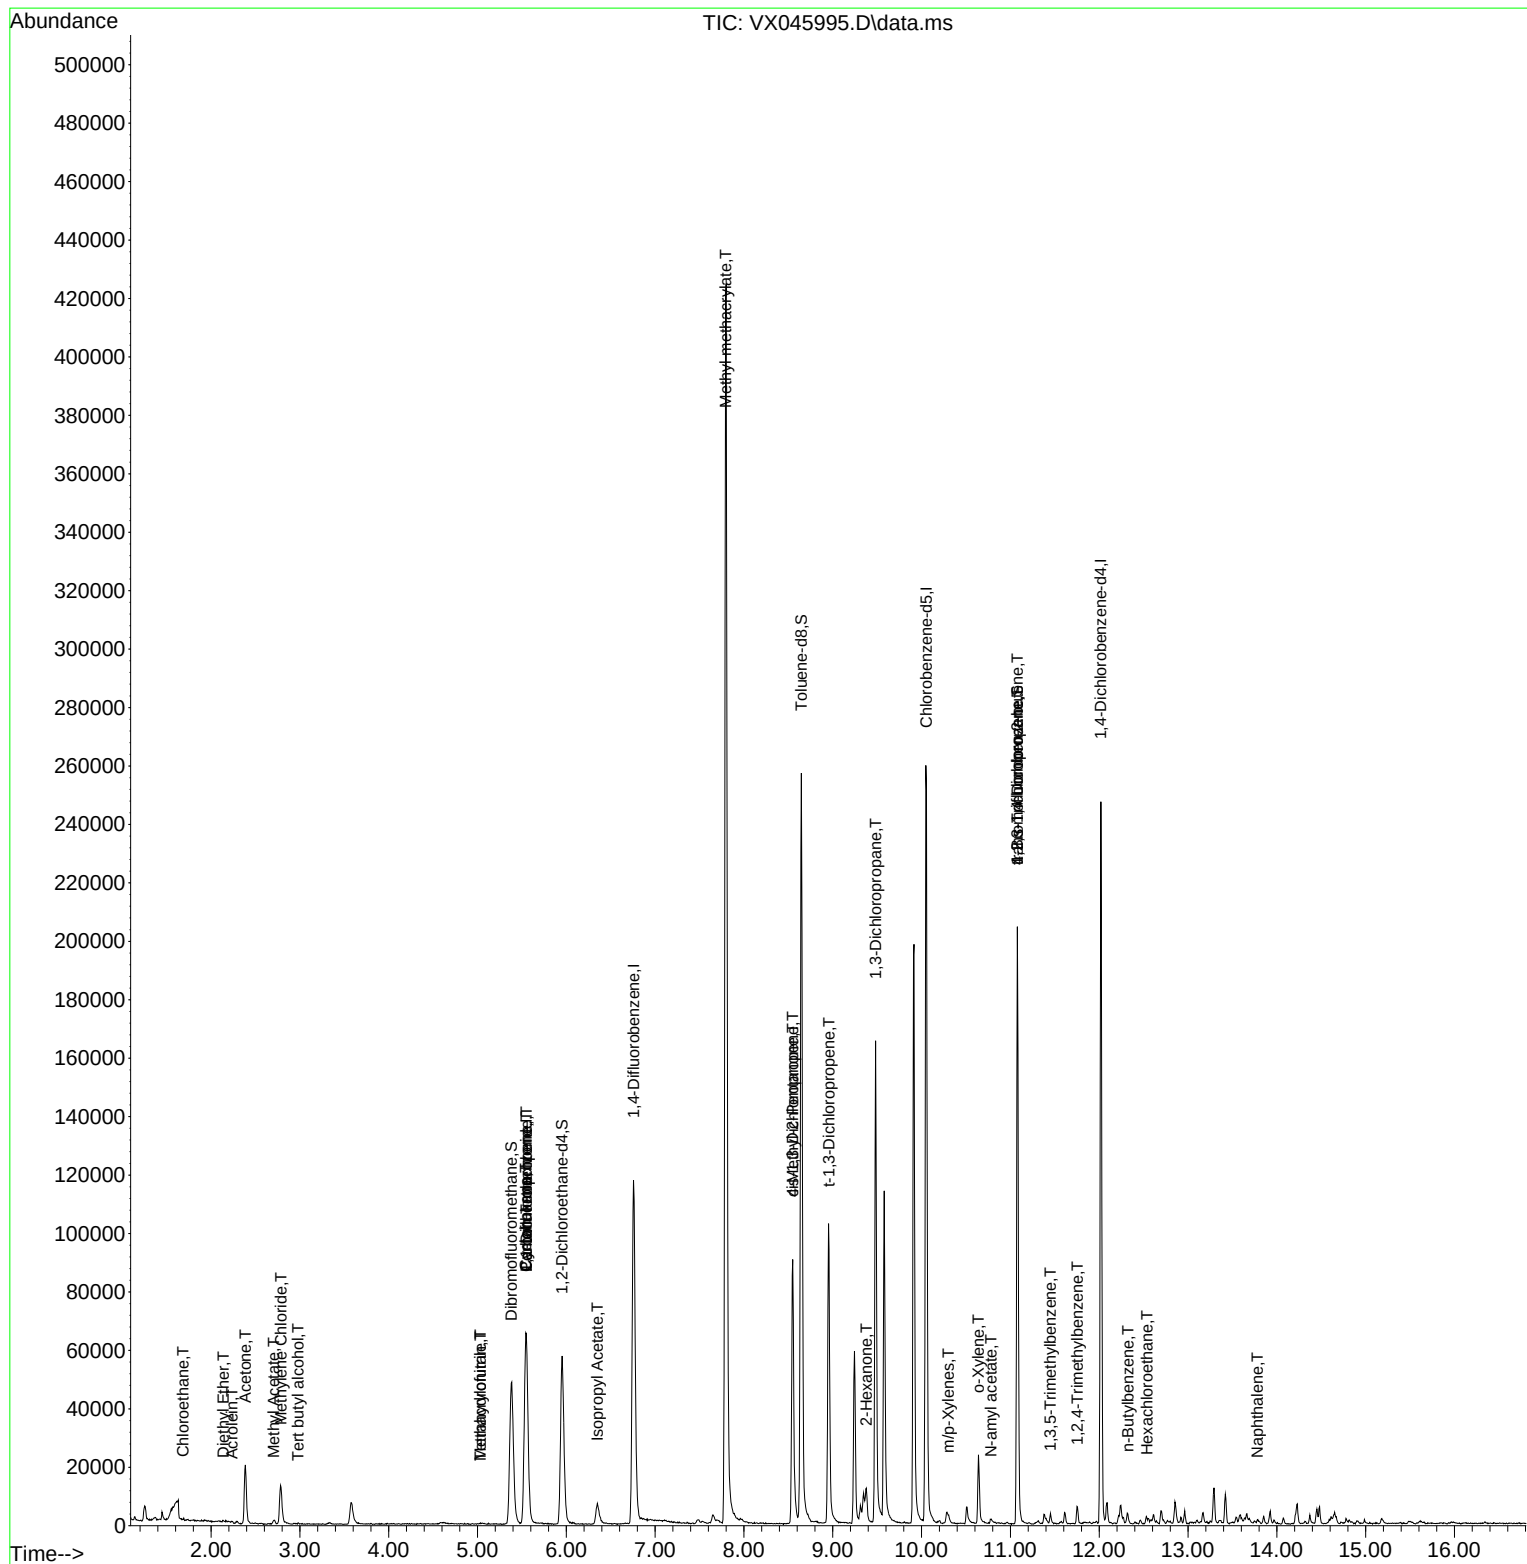






#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Instrument :
MSVOA_X
ClientSampleId :
WC-04282025



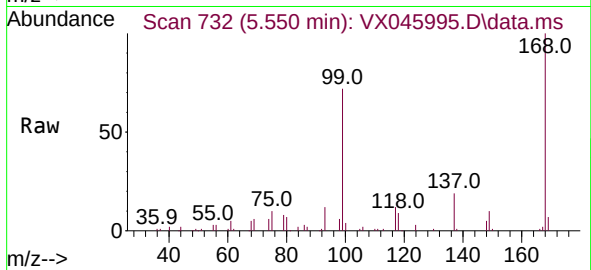



Tgt Ion:168 Resp: 56553
Ion Ratio Lower Upper
168 100
99 71.5 52.3 78.5

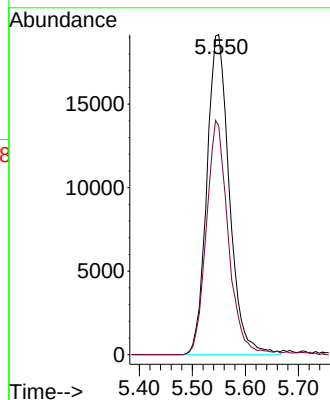

#6
Chloroethane
Concen: 0.635 ug/l
RT: 1.684 min Scan# 98
Delta R.T. 0.018 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 64 Resp: 268
Ion Ratio Lower Upper
64 100
66 0.0 26.3 39.5


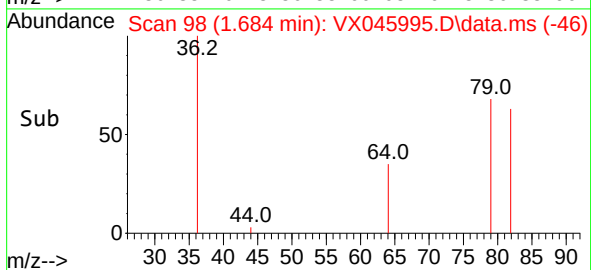
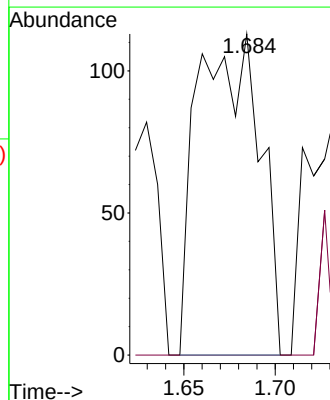
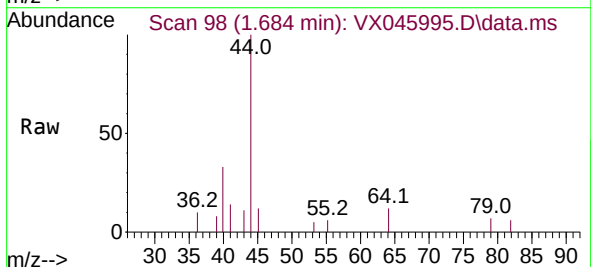




#8
Diethyl Ether
Concen: 0.251 ug/l
RT: 2.136 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 74 Resp: 100
Ion Ratio Lower Upper
74 100
45 305.0 53.0 159.1#

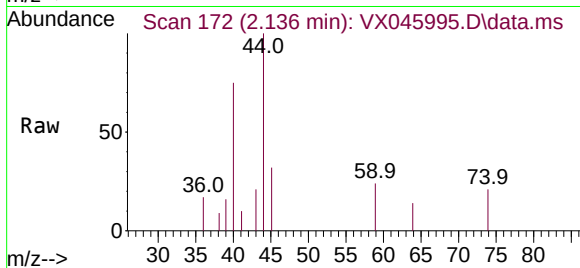

#11
Tert butyl alcohol
Concen: 1.777 ug/l
RT: 2.977 min Scan# 310
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 59 Resp: 247
Ion Ratio Lower Upper
59 100
57 0.0 8.6 12.8#


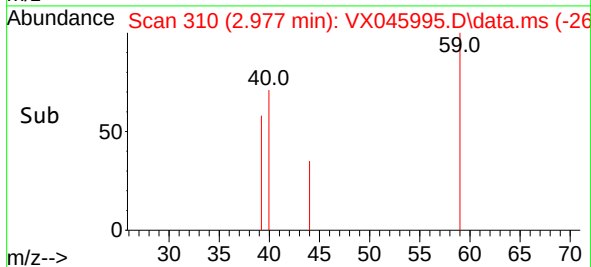

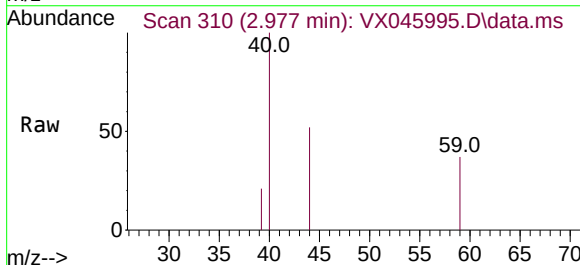


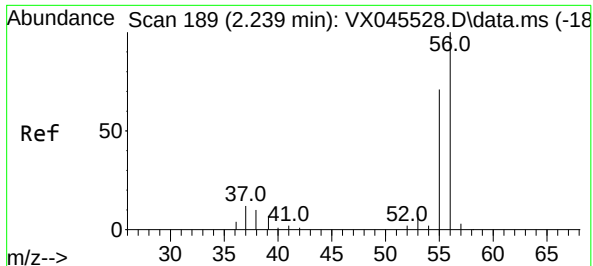

#13
Acrolein
Concen: 0.381 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 56 Resp: 73
Ion Ratio Lower Upper
56 100
55 57.5 56.2 84.2

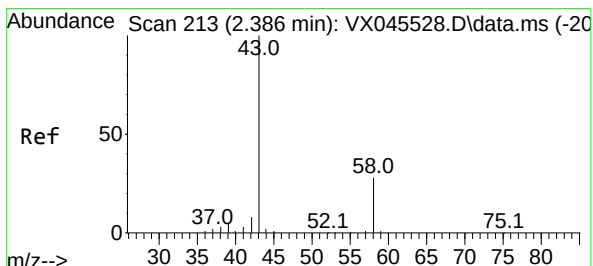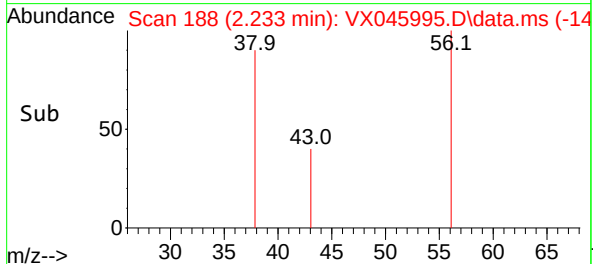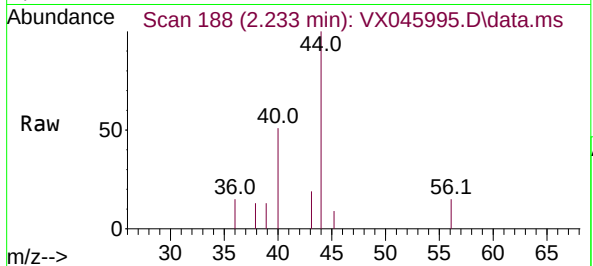

#16
Acetone
Concen: 51.644 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 43 Resp: 21932
Ion Ratio Lower Upper
43 100
58 28.8 22.3 33.5


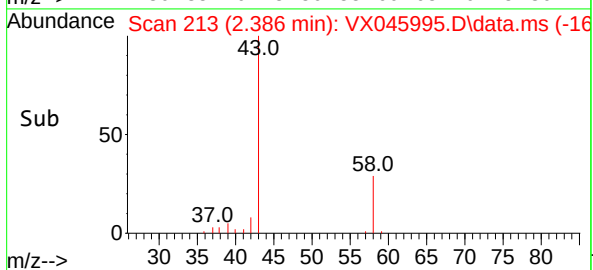

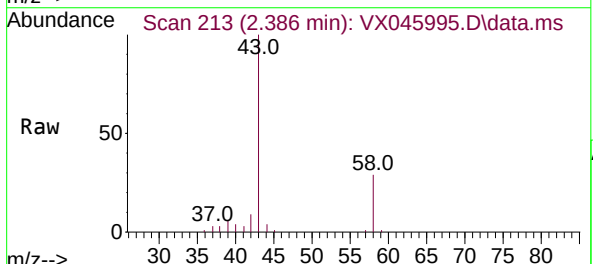




#18
Methyl Acetate
Concen: 1.799 ug/l
RT: 2.703 min Scan# 20
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 43 Resp: 1759
Ion Ratio Lower Upper
43 100
74 19.8 17.5 26.3

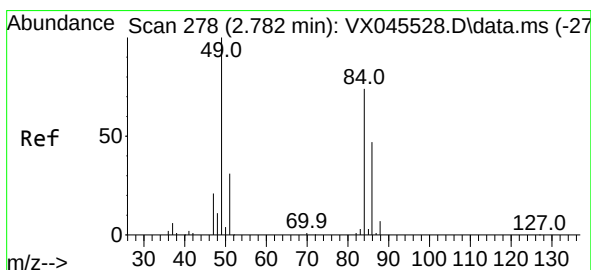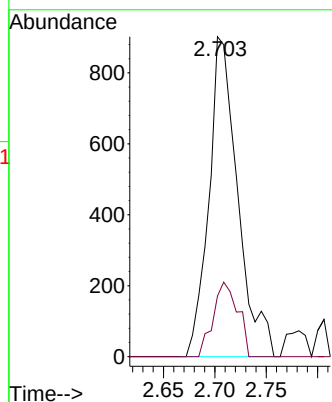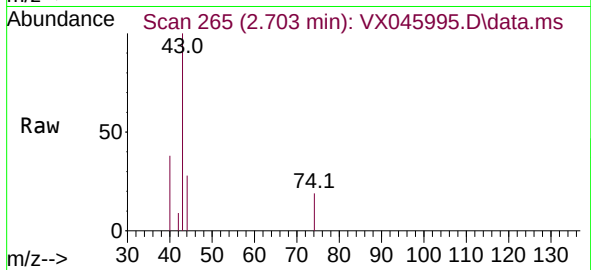

#20
Methylene Chloride
Concen: 8.071 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.006 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 84 Resp: 6417
Ion Ratio Lower Upper
84 100
49 127.4 107.5 161.3
51 42.4 33.0 49.6
86 66.4 50.1 75.1

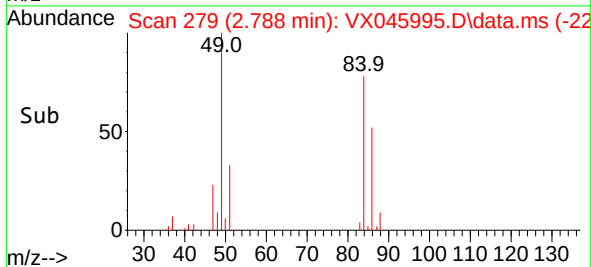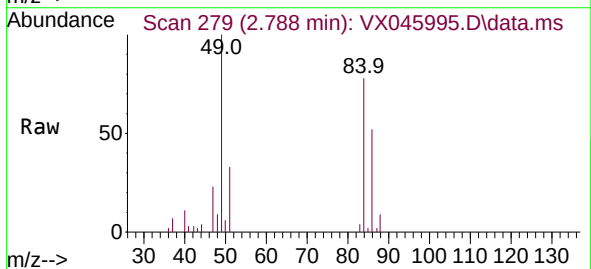

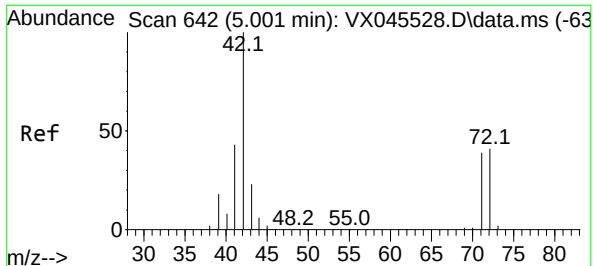

#29

Tetrahydrofuran

Concen: 0.380 ug/l

RT: 5.031 min Scan# 642

Delta R.T. 0.030 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :

WC-04282025





Tgt Ion: 42 Resp: 153

Ion Ratio Lower Upper

42 100

72 0.0 33.4 50.0#

71 31.4 31.4 47.0

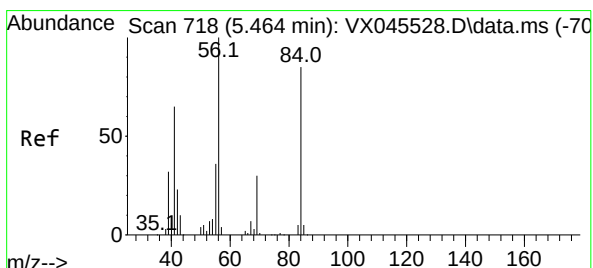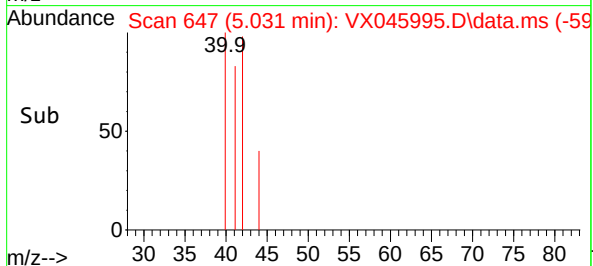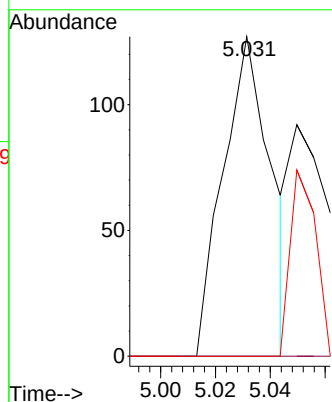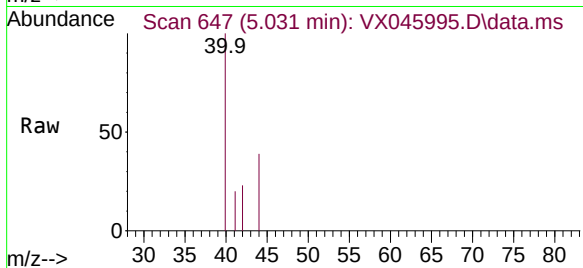

#31

Cyclohexane

Concen: 1.297 ug/l

RT: 5.543 min Scan# 731

Delta R.T. 0.079 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06




Tgt Ion: 56 Resp: 1645


Ion Ratio Lower Upper

56 100

69 149.8 23.6 35.4#

84 101.1 67.7 101.5

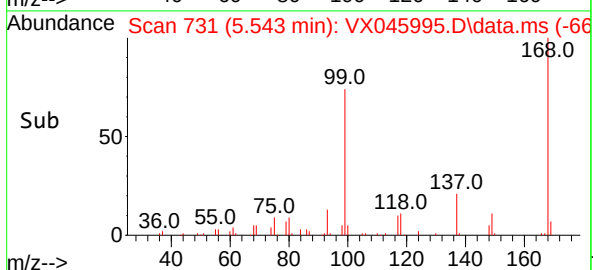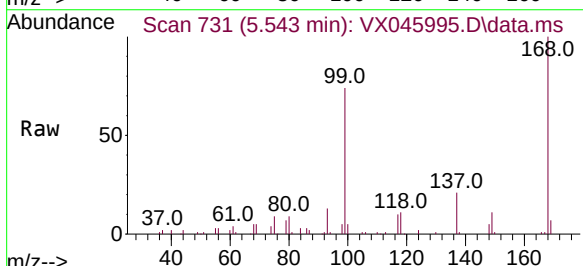



#33

1,2-Dichloroethane-d4

Concen: 56.542 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :





WC-04282025

Tgt Ion: 65 Resp: 58476

Ion Ratio Lower Upper

65 100

67 49.7 0.0 99.0

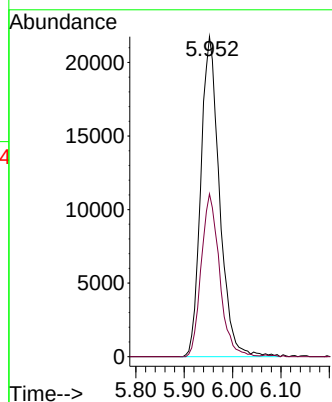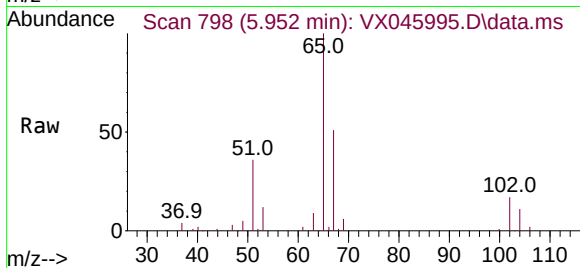

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06




Tgt Ion: 114 Resp: 111268


Ion Ratio Lower Upper

114 100

63 25.5 0.0 46.8

88 16.0 0.0 35.4

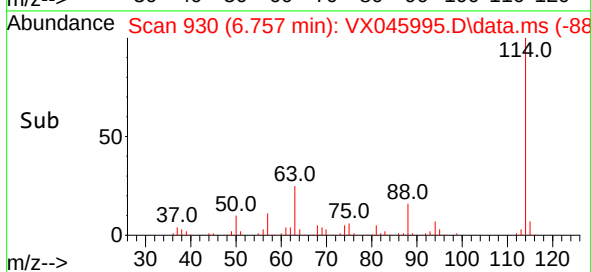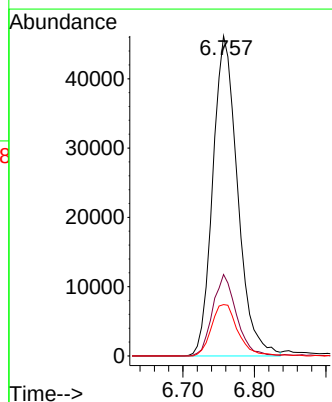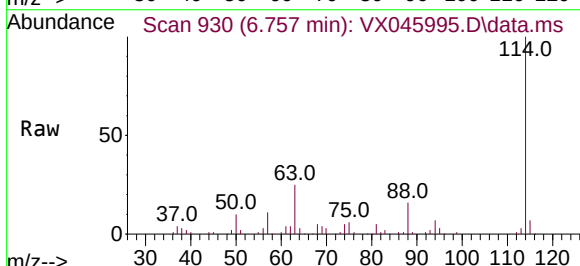

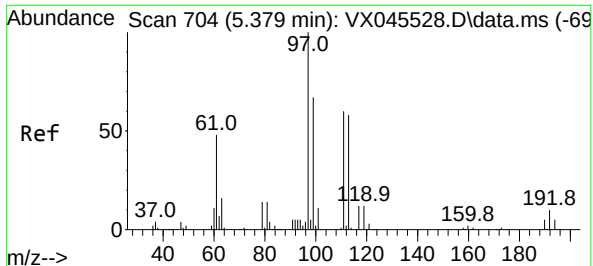

#35

Dibromofluoromethane

Concen: 54.931 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX045995.D


Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :

WC-04282025

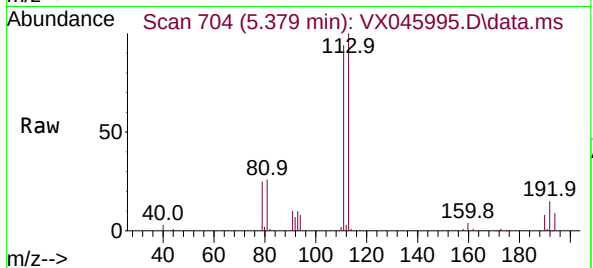




Tgt Ion:113 Resp: 43365

Ion Ratio Lower Upper

113 100

111 99.7 81.8 122.6

192 16.0 13.8 20.6

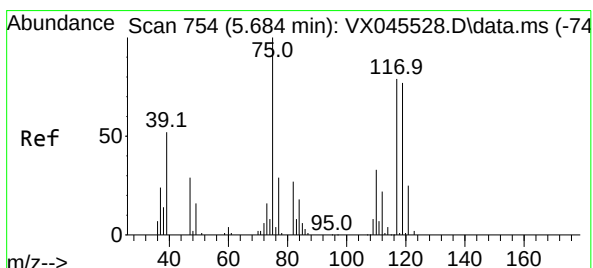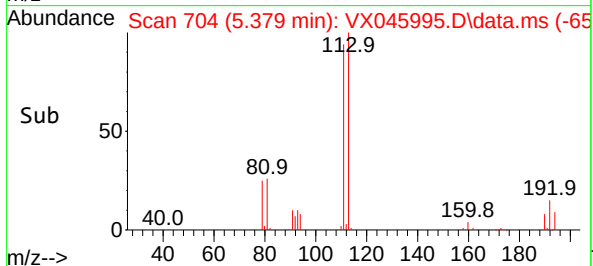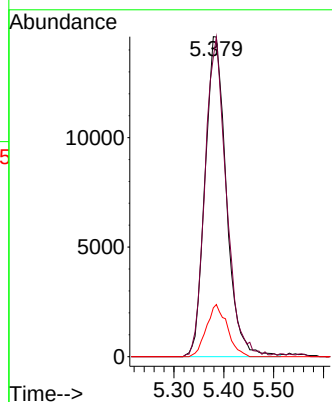

#36

1,1-Dichloropropene

Concen: 5.003 ug/l

RT: 5.550 min Scan# 732

Delta R.T. -0.134 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06




Tgt Ion: 75 Resp: 5333


Ion Ratio Lower Upper

75 100

110 9.2 16.9 50.6#


77 0.0 25.0 37.4#

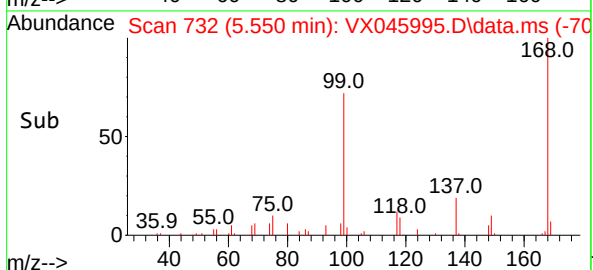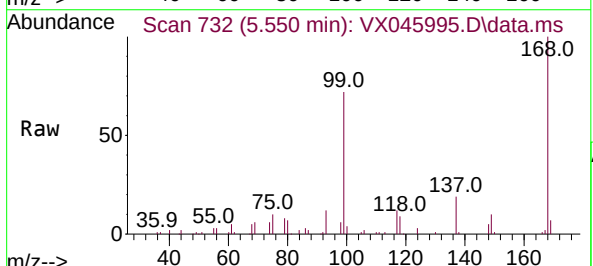






#38
Carbon Tetrachloride
Concen: 5.920 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.122 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Instrument :
MSVOA_X
ClientSampleId :
WC-04282025







Tgt Ion:117 Resp: 6820
Ion Ratio Lower Upper
117 100
119 3.9 76.9 115.3#
121 0.0 24.2 36.2#

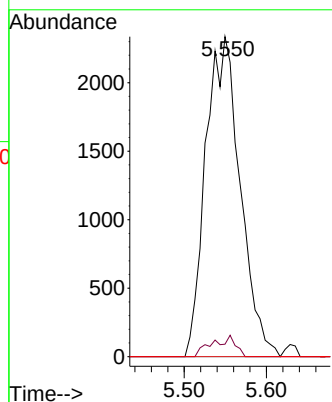

#41
Methacrylonitrile
Concen: 0.200 ug/l
RT: 5.031 min Scan# 647
Delta R.T. 0.110 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 41 Resp: 142
Ion Ratio Lower Upper
41 100
39 32.4 47.0 70.6#
67 0.0 53.2 79.8#
52 0.0 25.0 37.6#


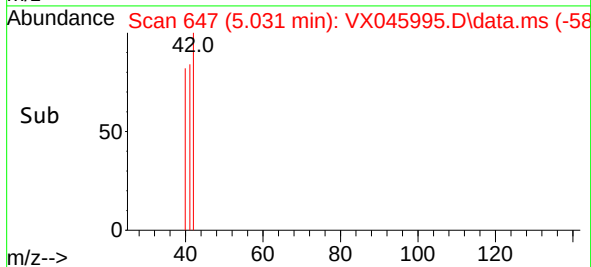

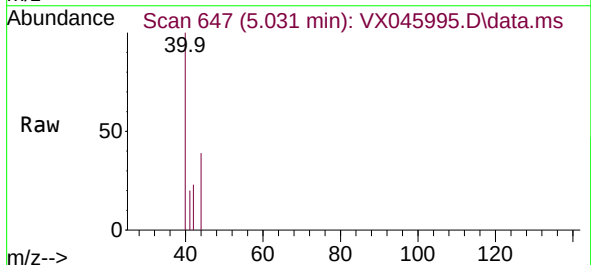




#43
Isopropyl Acetate
Concen: 4.956 ug/l
RT: 6.348 min Scan# 81
Delta R.T. 0.012 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 43 Resp: 10089
Ion Ratio Lower Upper
43 100
61 18.4 14.1 21.1
87 12.4 9.2 13.8



#48
Methyl methacrylate
Concen: 41.800 ug/l
RT: 7.793 min Scan# 1100
Delta R.T. 0.103 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 41 Resp: 43939
Ion Ratio Lower Upper
41 100
69 0.2 58.2 87.2#
39 59.3 53.6 80.4


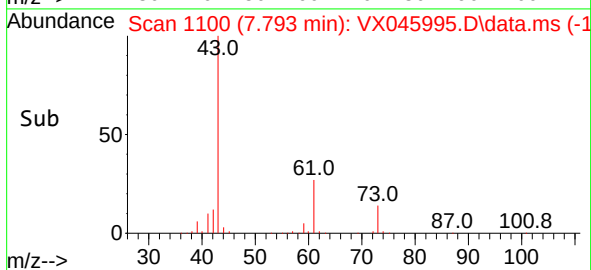




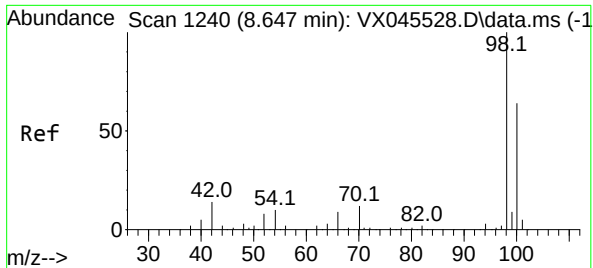

#50
Toluene-d8
Concen: 53.320 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 98 Resp: 146921
Ion Ratio Lower Upper
98 100
100 64.2 52.2 78.4

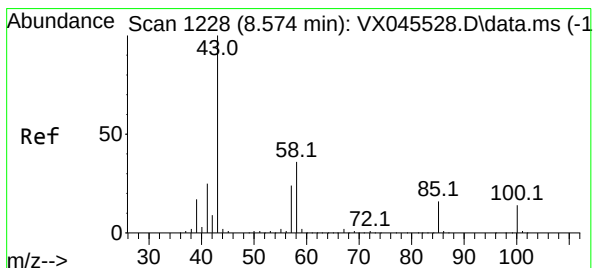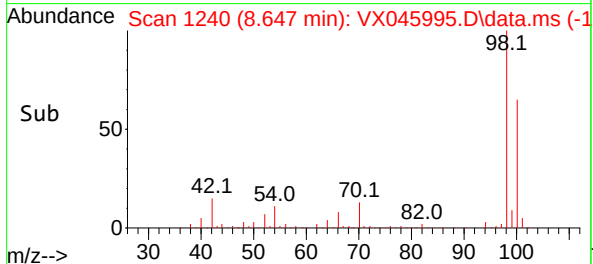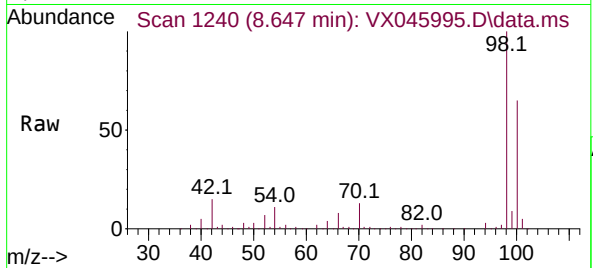

#51
4-Methyl-2-Pentanone
Concen: 27.273 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 43 Resp: 36809
Ion Ratio Lower Upper
43 100
58 7.2 28.5 42.7#

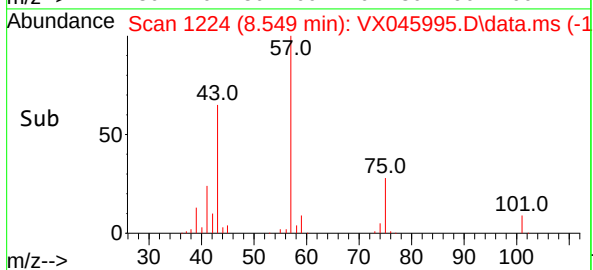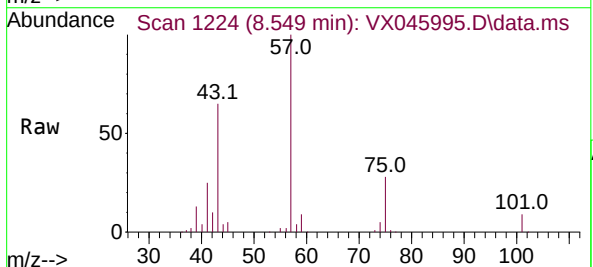

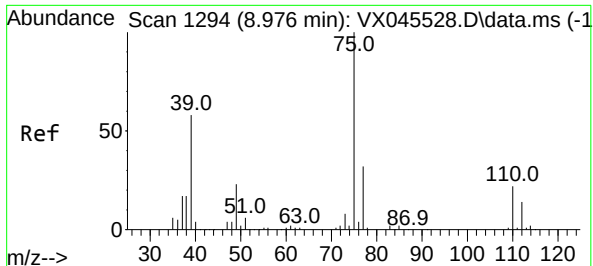

#53

t-1,3-Dichloropropene

Concen: 2.443 ug/l

RT: 8.958 min Scan# 11

Delta R.T. -0.018 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :





WC-04282025

Tgt Ion: 75 Resp: 193

Ion Ratio Lower Upper

75 100

77 0.0 25.4 38.0#

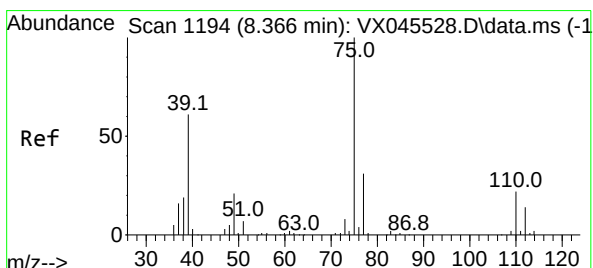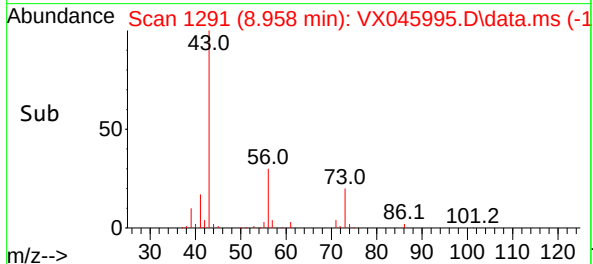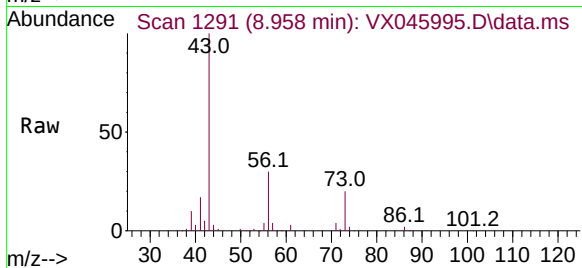

#54

cis-1,3-Dichloropropene

Concen: 12.101 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. 0.183 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06




Tgt Ion: 75 Resp: 14160


Ion Ratio Lower Upper

75 100

77 1.3 24.6 36.8#

39 44.6 48.4 72.6#

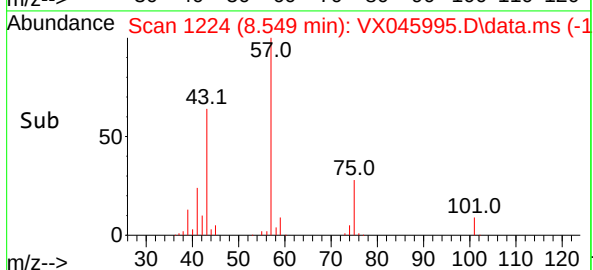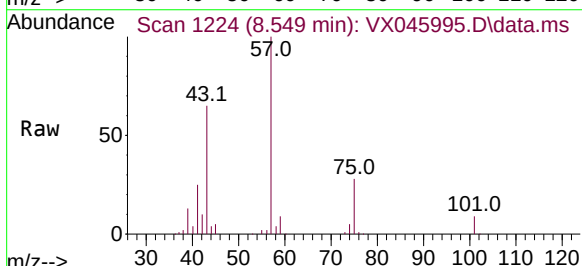



#57

1,3-Dichloropropane

Concen: 0.983 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :





WC-04282025

Tgt Ion: 76 Resp: 1344

Ion Ratio Lower Upper

76 100

78 0.0 26.0 39.0#

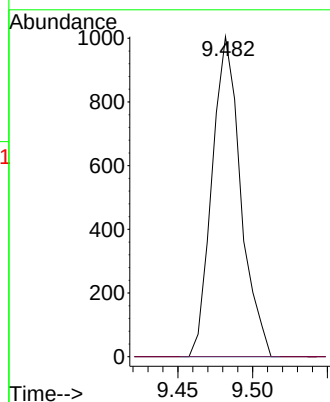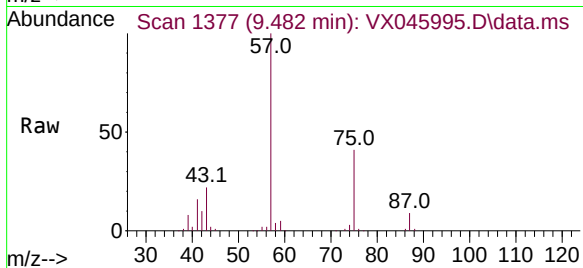

#59

2-Hexanone

Concen: 11.443 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.049 min

Lab File: VX045995.D




Acq: 30 Apr 2025 14:06


Tgt Ion: 43 Resp: 11437

Ion Ratio Lower Upper

43 100

58 0.0 24.9 74.6#


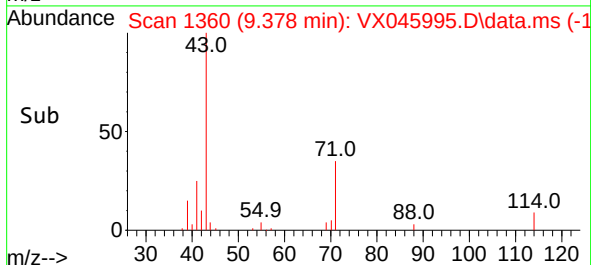
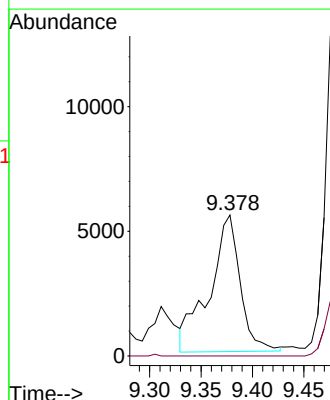
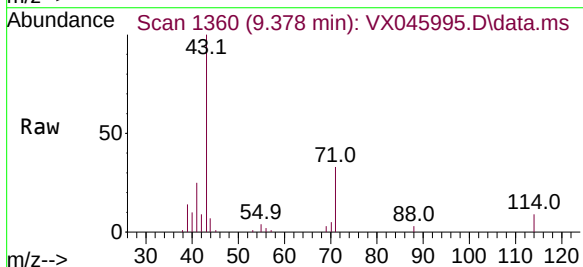




#62
4-Bromofluorobenzene
Concen: 52.810 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion: 95 Resp: 53005
Ion Ratio Lower Upper
95 100
174 68.1 0.0 135.8
176 66.0 0.0 131.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.006 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 117 Resp: 107559
Ion Ratio Lower Upper
117 100
82 59.5 49.2 73.8
119 33.1 25.1 37.7


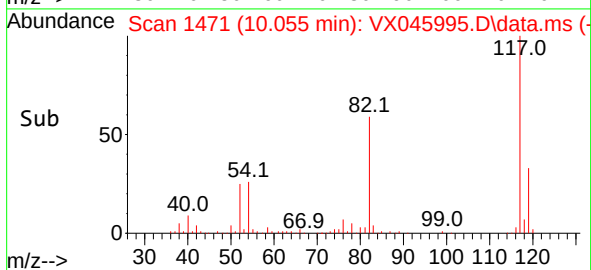






#68
m/p-Xylenes
Concen: 0.267 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion:106 Resp: 400
Ion Ratio Lower Upper
106 100
91 257.5 172.6 258.8

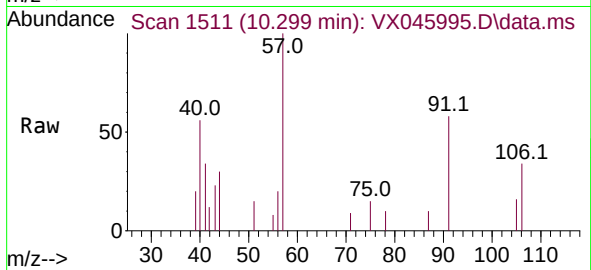

#69
o-Xylene
Concen: 0.561 ug/l
RT: 10.640 min Scan# 1567
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion:106 Resp: 827
Ion Ratio Lower Upper
106 100
91 249.5 113.6 340.6


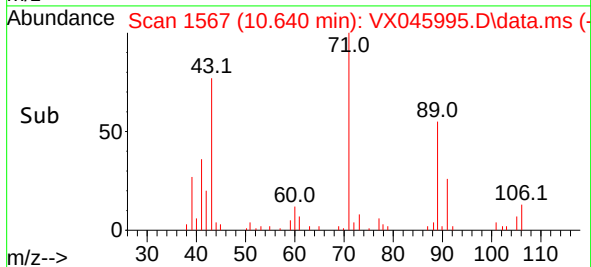

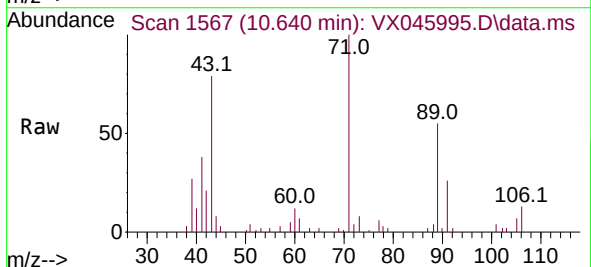




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06




Instrument :
MSVOA_X
ClientSampleId :
WC-04282025


Tgt Ion:152 Resp: 44562
Ion Ratio Lower Upper
152 100
115 64.3 46.9 140.7
150 155.0 0.0 349.4

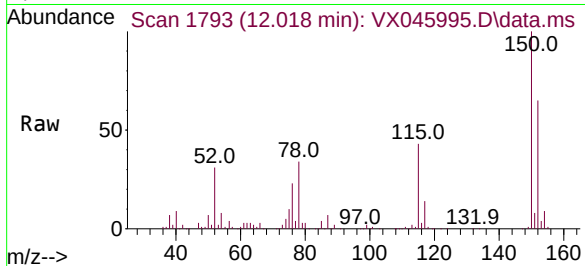

#74
N-ethyl acetate
Concen: 0.812 ug/l
RT: 10.780 min Scan# 1590
Delta R.T. -0.061 min
Lab File: VX045995.D
Acq: 30 Apr 2025 14:06

Tgt Ion: 43 Resp: 1386
Ion Ratio Lower Upper
43 100
70 0.0 30.1 45.1#
55 4.5 18.3 27.5#
61 0.0 17.5 26.3#

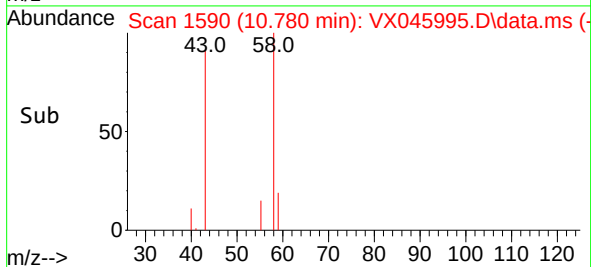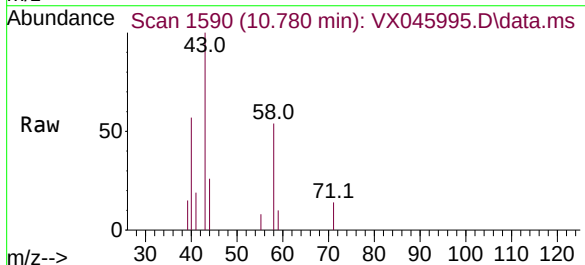



#76

1,2,3-Trichloropropane

Concen: 28.662 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.159 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :





WC-04282025

Tgt Ion: 75 Resp: 31155

Ion Ratio Lower Upper

75 100

77 1.1 20.0 59.9#

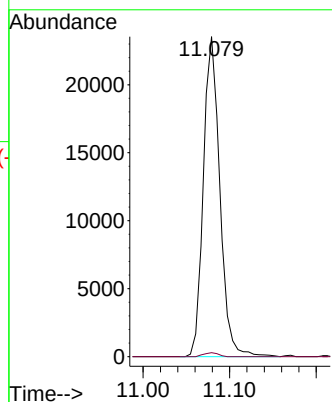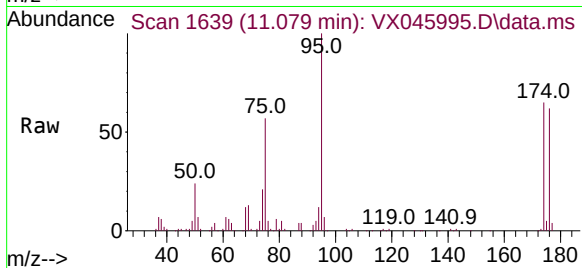

#80

1,3,5-Trimethylbenzene

Concen: 0.615 ug/l

RT: 11.451 min Scan# 1700

Delta R.T. -0.000 min

Lab File: VX045995.D




Acq: 30 Apr 2025 14:06


Tgt Ion:105 Resp: 1814

Ion Ratio Lower Upper

105 100

120 44.2 23.0 69.0


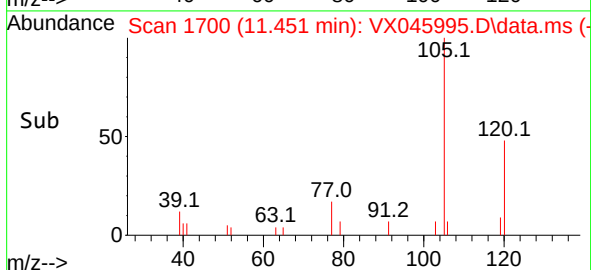

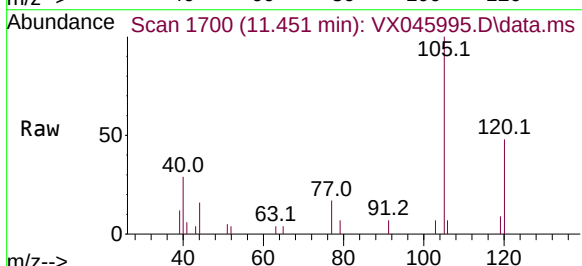




#81
 trans-1,4-Dichloro-2-butene
 Concen: 97.276 ug/l
 RT: 11.079 min Scan# 1
 Delta R.T. 0.061 min
 Lab File: VX045995.D
 Acq: 30 Apr 2025 14:06




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-04282025


Tgt Ion: 75 Resp: 31155
 Ion Ratio Lower Upper
 75 100
 53 0.0 101.8 152.6#
 89 0.0 37.2 55.8#

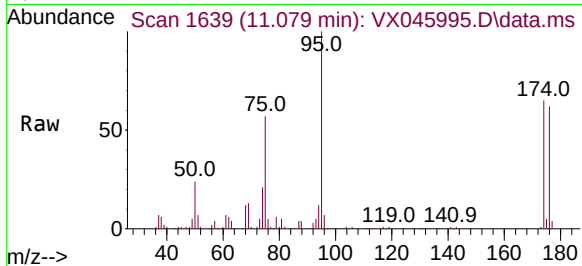

#84
 1,2,4-Trimethylbenzene
 Concen: 1.079 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. 0.006 min
 Lab File: VX045995.D
 Acq: 30 Apr 2025 14:06

Tgt Ion: 105 Resp: 3197
 Ion Ratio Lower Upper
 105 100
 120 39.1 21.4 64.3

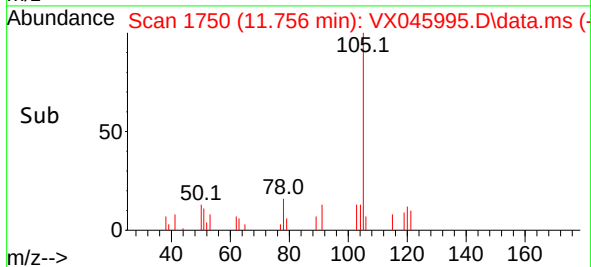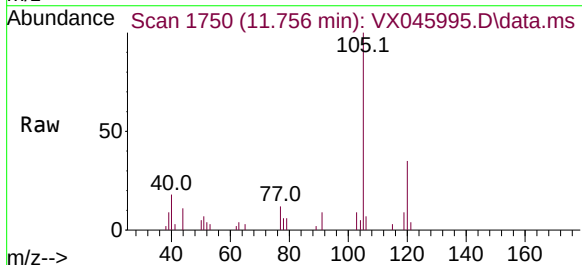



#89

n-Butylbenzene

Concen: 0.229 ug/l

RT: 12.323 min Scan# 11

Delta R.T. -0.006 min

Lab File: VX045995.D

Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :

WC-04282025





Tgt Ion: 91 Resp: 588

Ion Ratio Lower Upper

91 100

92 23.6 26.9 80.6#

134 91.0 11.9 35.7#

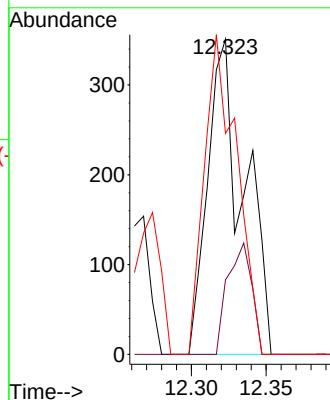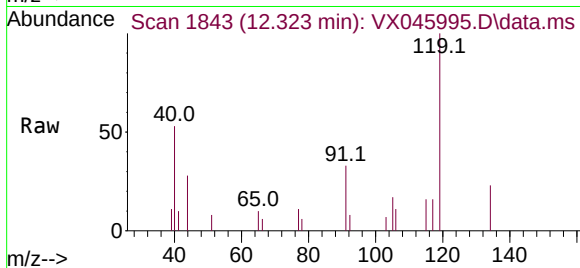

#90

Hexachloroethane

Concen: 0.285 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. -0.000 min

Lab File: VX045995.D




Acq: 30 Apr 2025 14:06


Tgt Ion: 117 Resp: 145

Ion Ratio Lower Upper

117 100

201 0.0 31.2 93.6#

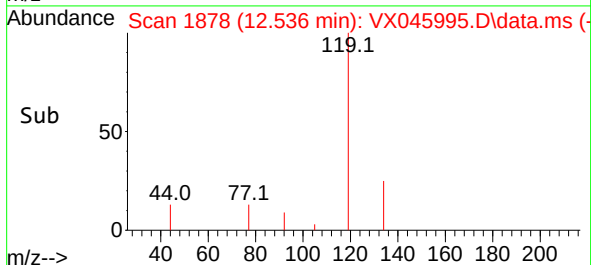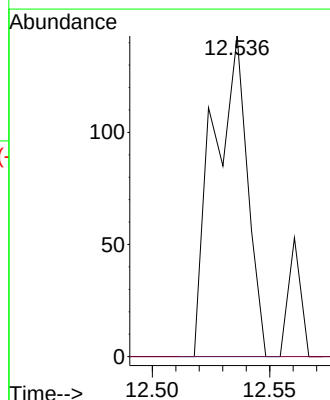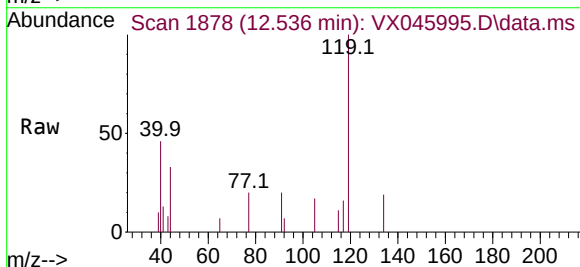



#95

Naphthalene

Concen: 0.322 ug/l

RT: 13.780 min Scan# 20

Delta R.T. 0.006 min

Lab File: VX045995.D


Acq: 30 Apr 2025 14:06

Instrument :

MSVOA_X

ClientSampleId :

WC-04282025

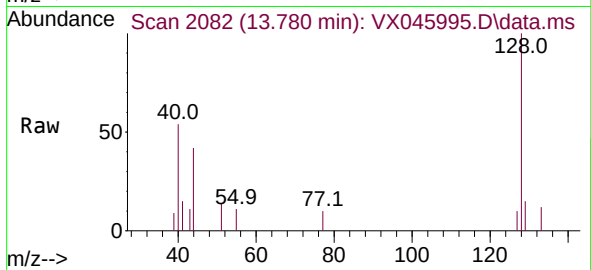

Tgt Ion:128 Resp: 995

Ion Ratio Lower Upper

128 100

127 8.0 10.3 15.5#

129 10.7 8.6 12.8

