

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043025\
 Data File : VX045986.D
 Acq On : 30 Apr 2025 10:32
 Operator : JC/MD
 Sample : VX0430MBL01
 Misc : 5.00g/10mL100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0430MBL01

Quant Time: May 01 03:35:22 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	64334	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.751	114	128575	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	118214	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50670	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	64222	54.587	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	109.180%
35) Dibromofluoromethane	5.373	113	47365	51.922	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.840%
50) Toluene-d8	8.647	98	159607	50.127	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.260%
62) 4-Bromofluorobenzene	11.079	95	60417	52.093	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX043025\
Data File : VX045986.D
Acq On : 30 Apr 2025 10:32
Operator : JC/MD
Sample : VX0430MBL01
Misc : 5.00g/10mL100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0430MBL01

Quant Time: May 01 03:35:22 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration




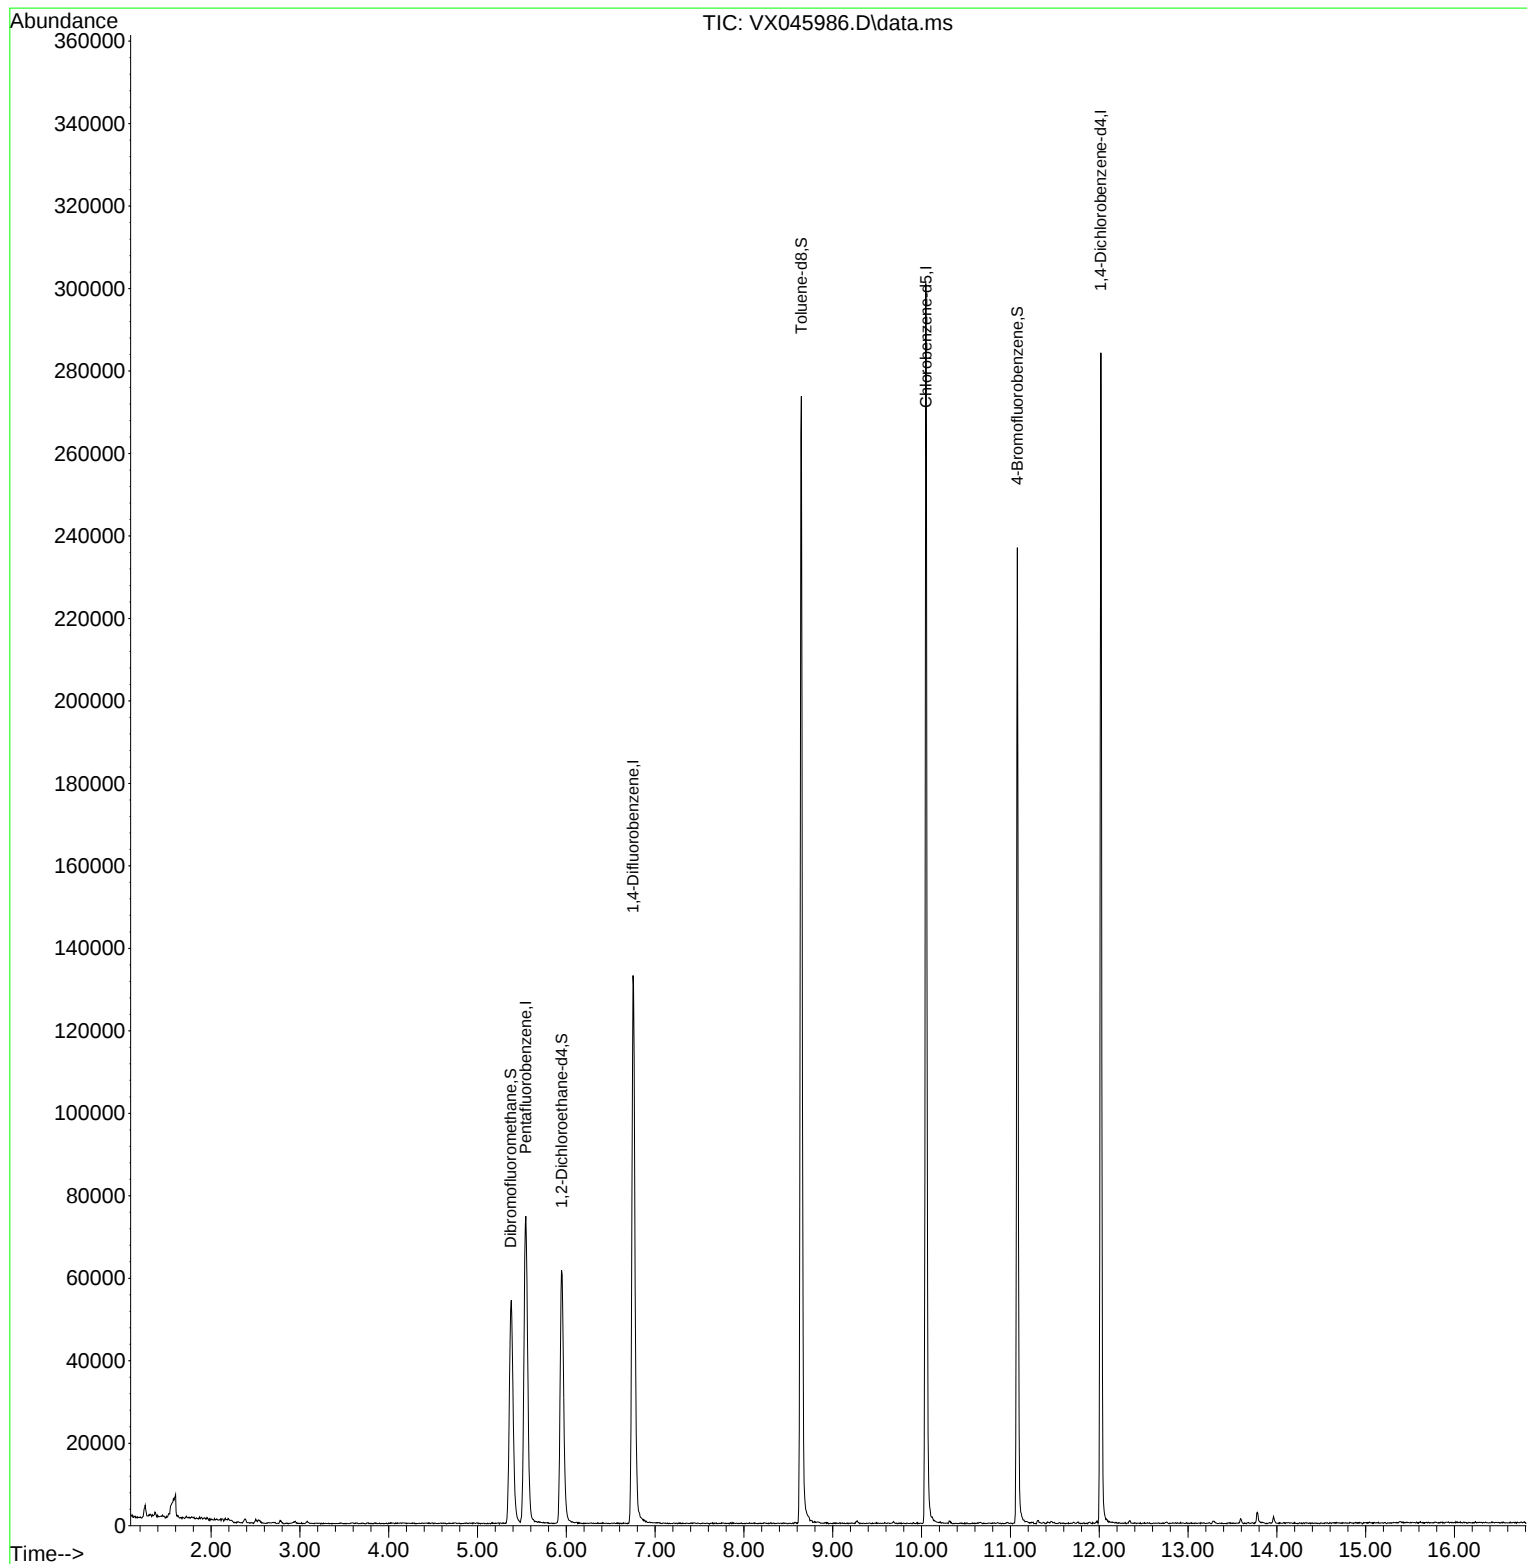


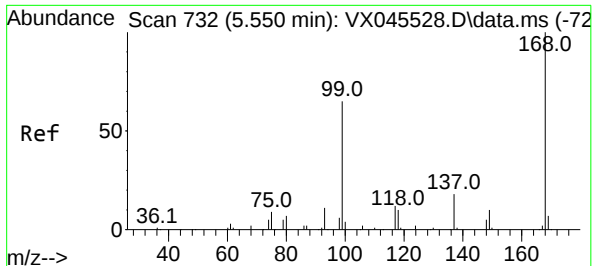

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.006 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0430MBL01


Tgt Ion:168 Resp: 64334
Ion Ratio Lower Upper
168 100
99 70.4 52.3 78.5

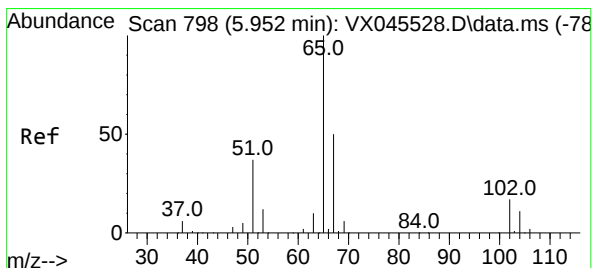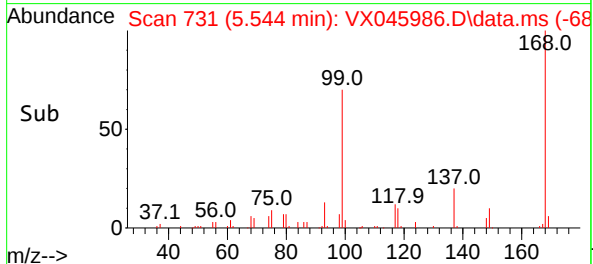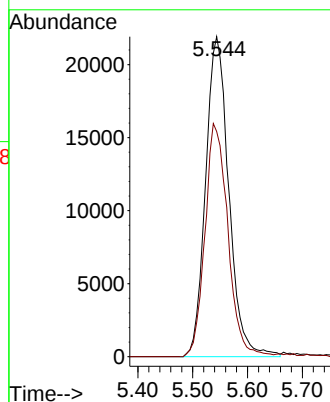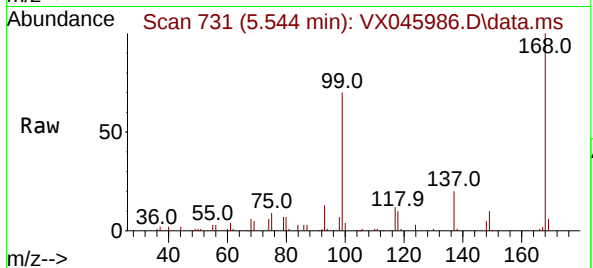

#33
1,2-Dichloroethane-d4
Concen: 54.587 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32

Tgt Ion: 65 Resp: 64222
Ion Ratio Lower Upper
65 100
67 48.1 0.0 99.0


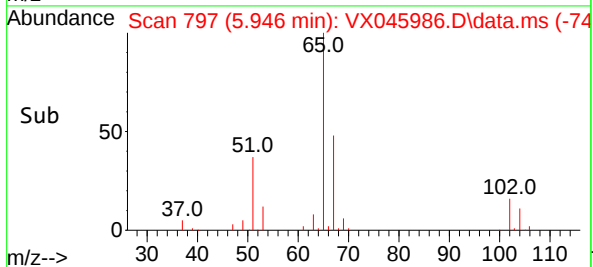
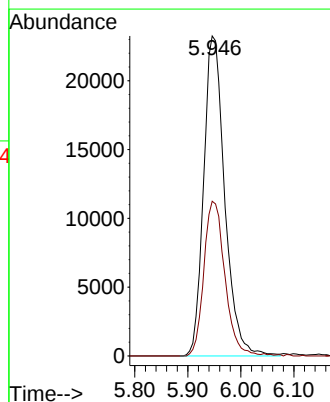
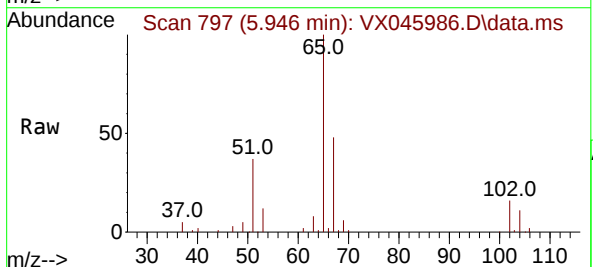


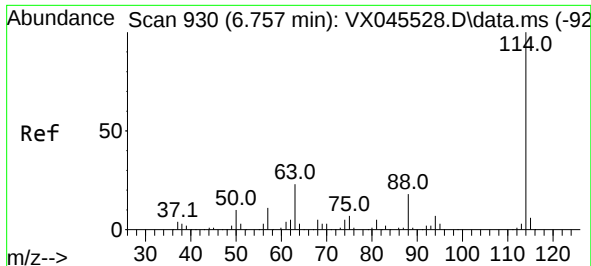

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.751 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0430MBL01


Tgt Ion:114 Resp: 128575
Ion Ratio Lower Upper
114 100
63 23.8 0.0 46.8
88 17.8 0.0 35.4

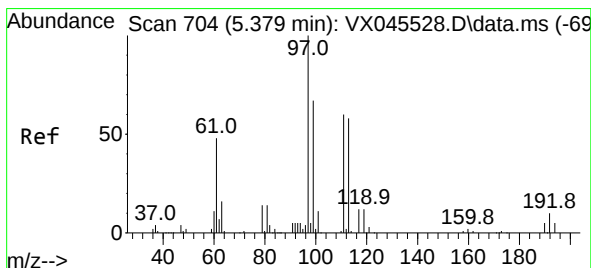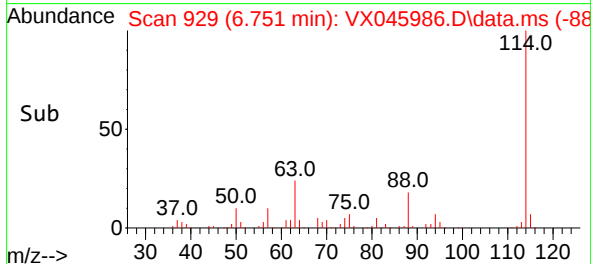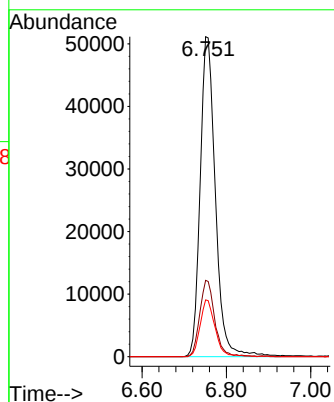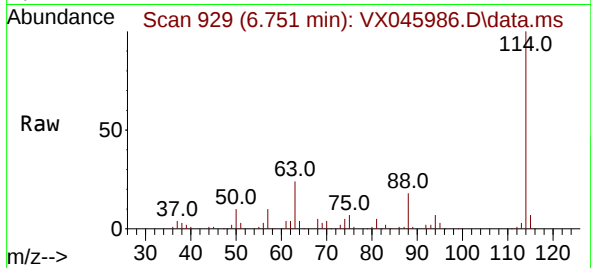

#35
Dibromofluoromethane
Concen: 51.922 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.006 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32

Tgt Ion:113 Resp: 47365
Ion Ratio Lower Upper
113 100
111 102.1 81.8 122.6
192 17.0 13.8 20.6


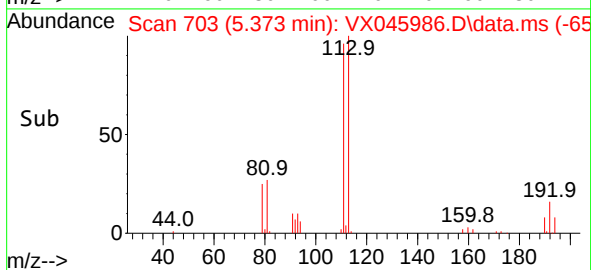
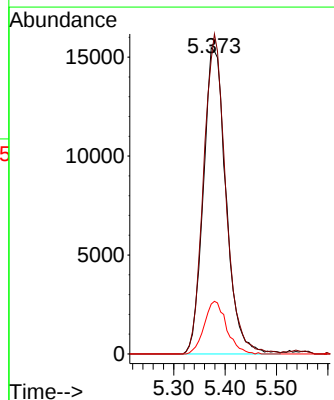
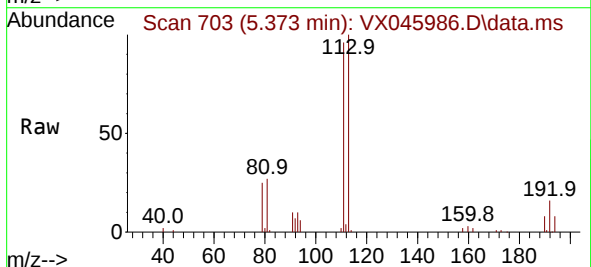


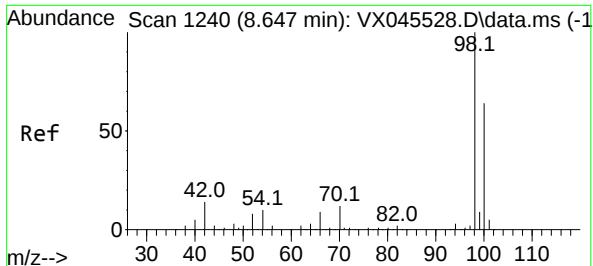

#50
Toluene-d8
Concen: 50.127 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0430MBL01


Tgt Ion: 98 Resp: 159607
Ion Ratio Lower Upper
98 100
100 63.5 52.2 78.4

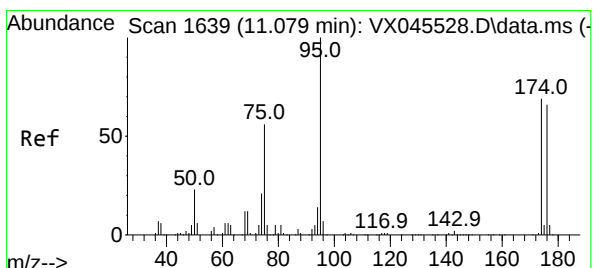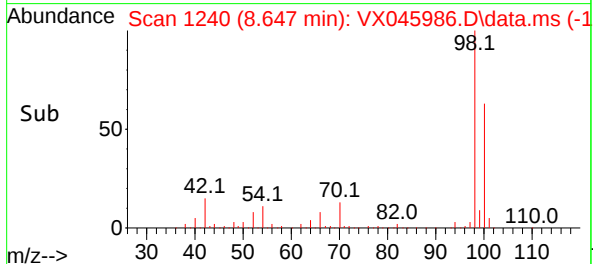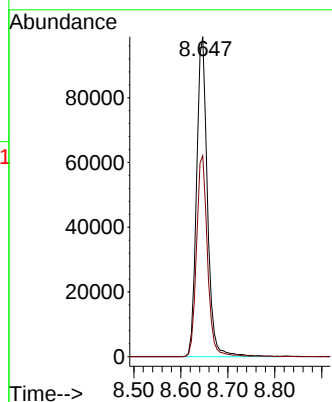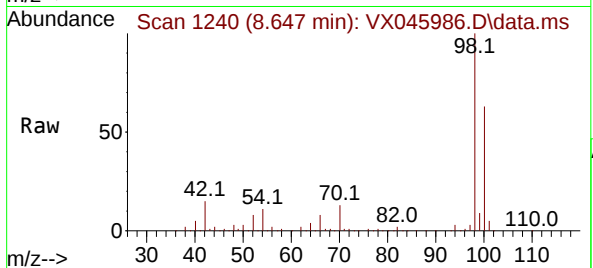

#62
4-Bromofluorobenzene
Concen: 52.093 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32

Tgt Ion: 95 Resp: 60417
Ion Ratio Lower Upper
95 100
174 68.5 0.0 135.8
176 65.7 0.0 131.4


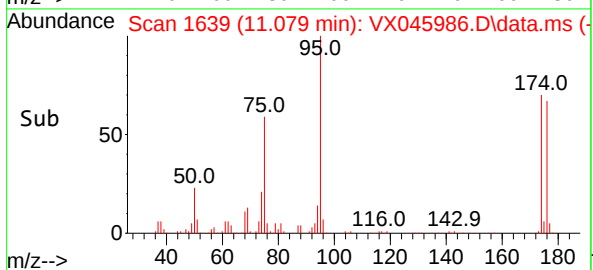
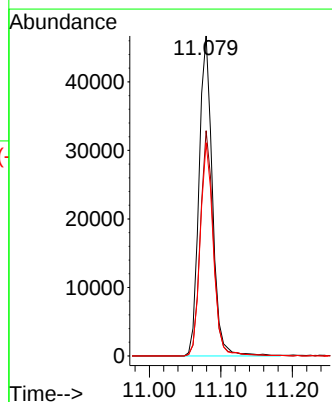
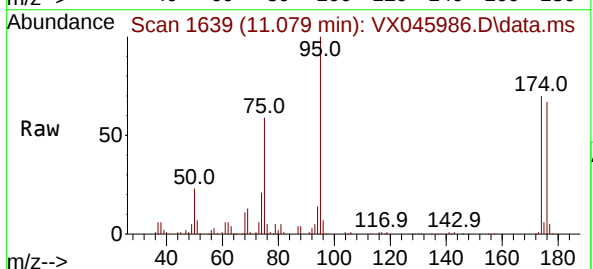


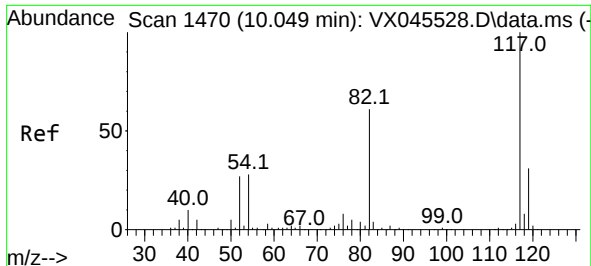

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32

Instrument :
MSVOA_X
ClientSampleId :
VX0430MBL01

Tgt Ion:117 Resp: 118214
Ion Ratio Lower Upper
117 100
82 62.0 49.2 73.8
119 34.0 25.1 37.7

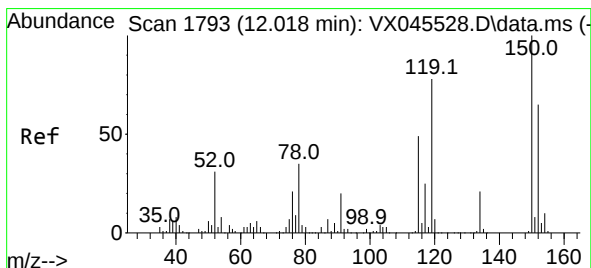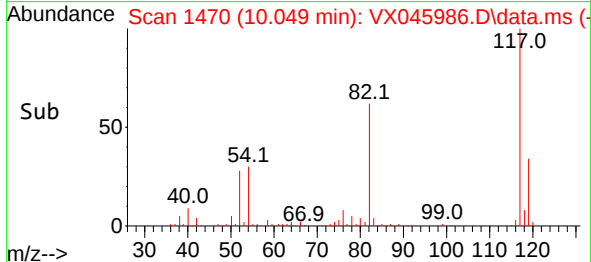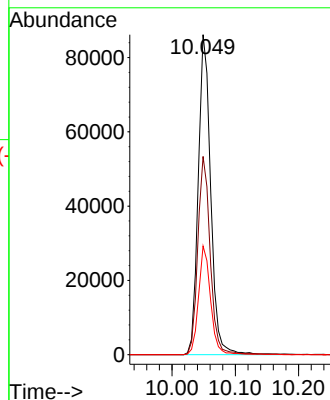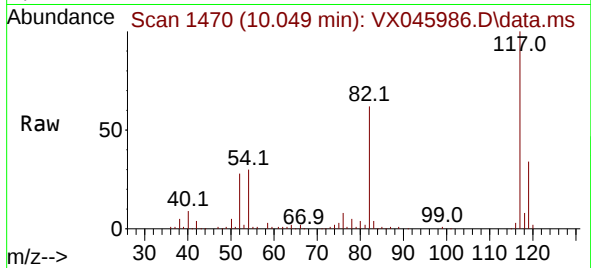

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX045986.D
Acq: 30 Apr 2025 10:32

Tgt Ion:152 Resp: 50670
Ion Ratio Lower Upper
152 100
115 67.2 46.9 140.7
150 156.5 0.0 349.4

