

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX050120\
 Data File : VX016005.D
 Acq On : 01 May 2020 12:18
 Operator : JC/SP
 Sample : VX0501WBL02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0501WBL02

Quant Time: May 02 07:21:17 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 28 17:30:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	286801	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	457087	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	432390	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	213245	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	177773	47.41	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.82%	
35) Dibromofluoromethane	5.46	113	136502	47.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.74%	
50) Toluene-d8	8.70	98	557030	52.25	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.50%	
62) 4-Bromofluorobenzene	11.12	95	216388	51.75	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.50%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX050120\
Data File : VX016005.D
Acq On : 01 May 2020 12:18
Operator : JC/SP
Sample : VX0501WBL02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0501WBL02

Quant Time: May 02 07:21:17 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 28 17:30:11 2020
Response via : Initial Calibration

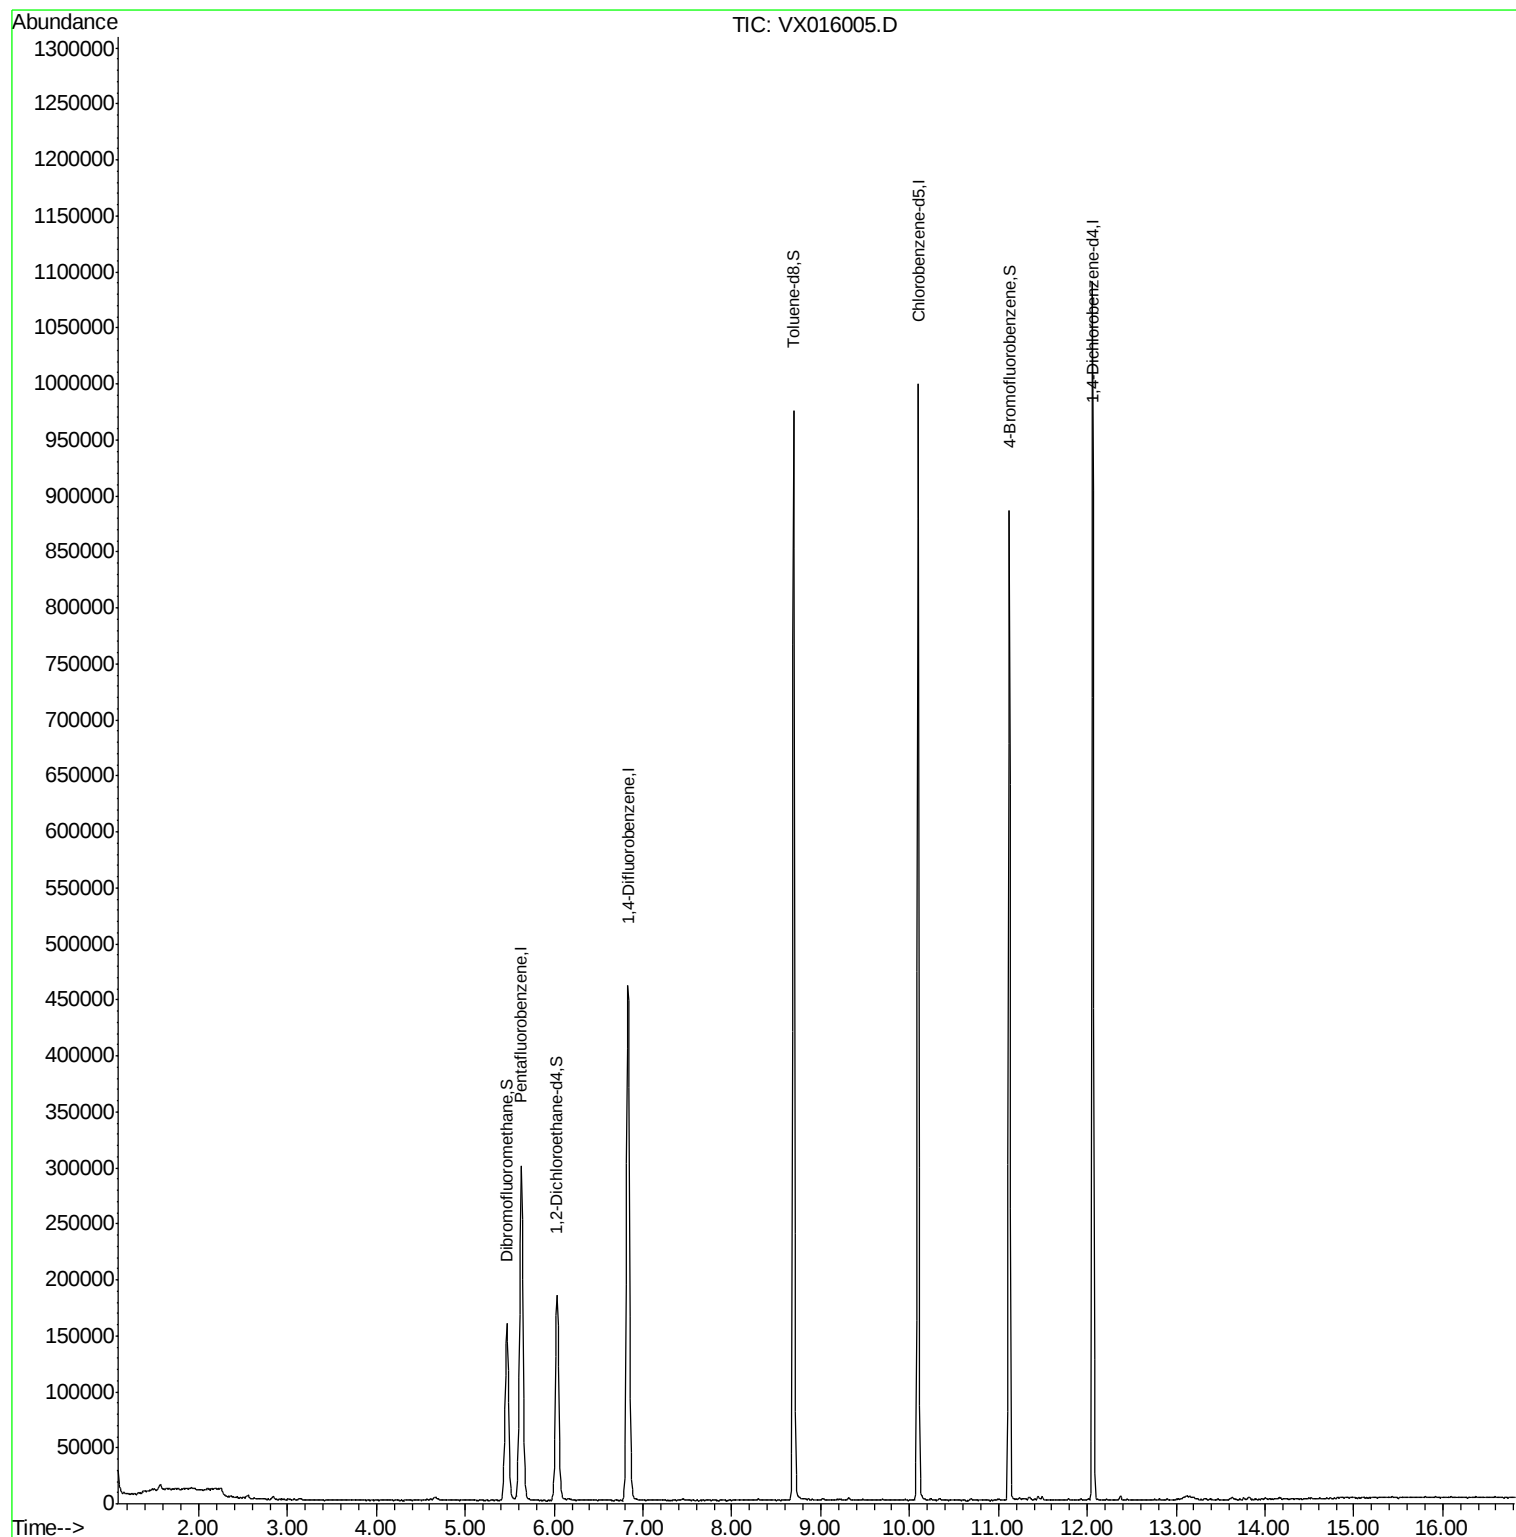

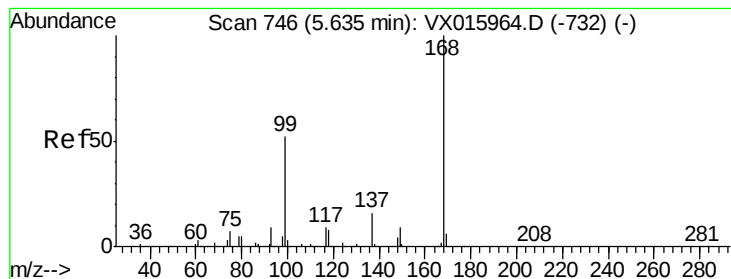

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 746

Delta R.T. 0.00 min

Lab File: VX016005.D

Acq: 01 May 2020 12:18

Instrument :

MSVOA_X

ClientSampleId :


VX0501WBL02

Tot Ion:168 Resp: 286801

Ion Ratio Lower Upper

168 100

99 53.7 41.7 62.5

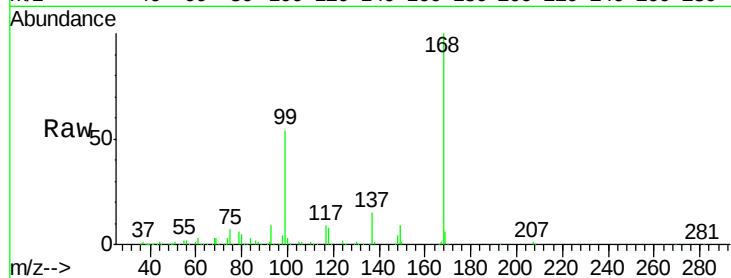

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.64

120000

100000

80000



60000

40000

20000

0

Time-->

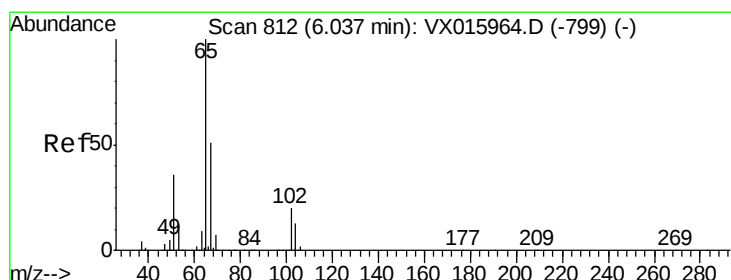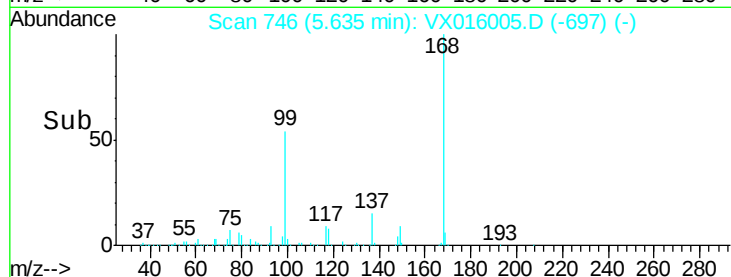

#33

1,2-Dichloroethane-d4

Concen: 47.408 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.01 min

Lab File: VX016005.D


Acq: 01 May 2020 12:18

Tgt Ion: 65 Resp: 177773

Ion Ratio Lower Upper

65 100

67 51.9 0.0 102.4

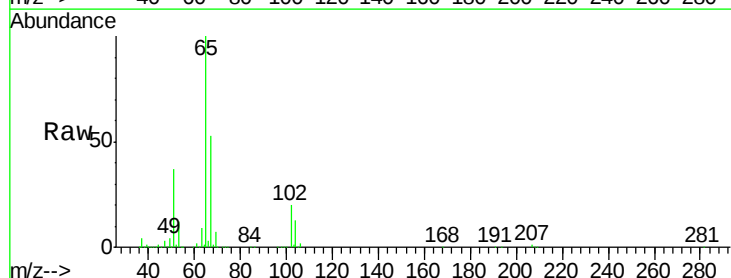

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03


60000


40000

20000

0

Time-->

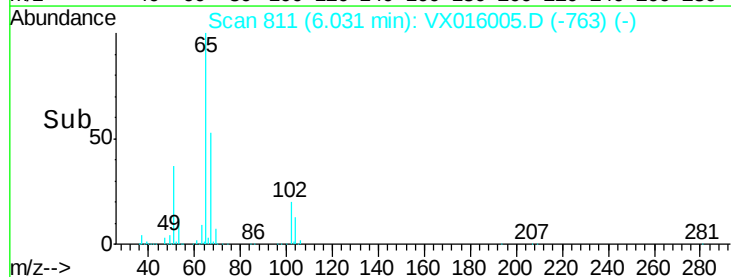

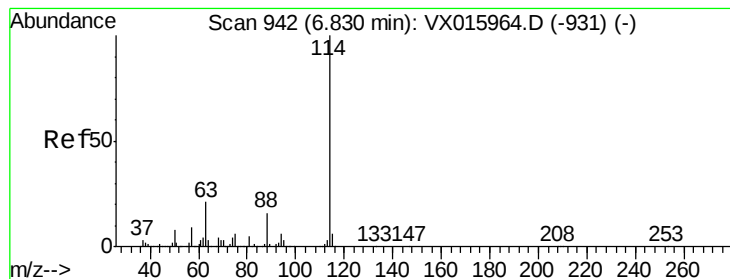

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. 0.00 min

Lab File: VX016005.D

Acq: 01 May 2020 12:18

Instrument :

MSVOA_X

ClientSampleId :

VX0501WBL02


Tot Ion:114 Resp: 457087

Ion Ratio Lower Upper

114 100

63 21.7 0.0 41.2




88 16.3 0.0 31.8

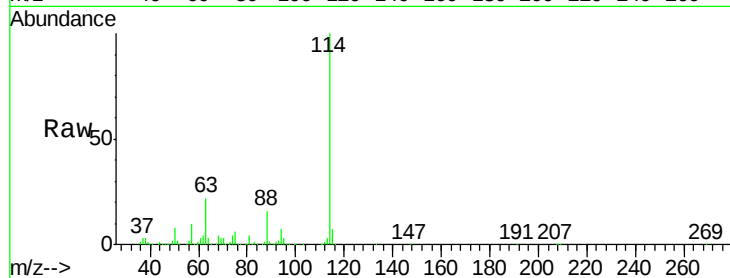

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

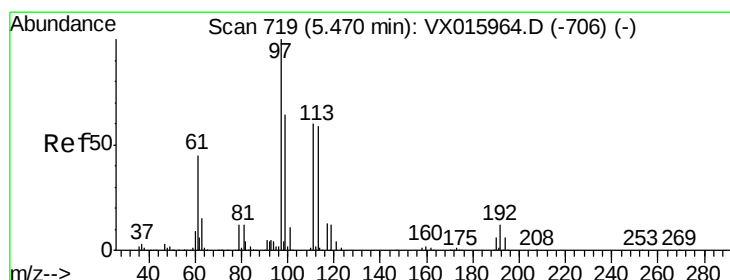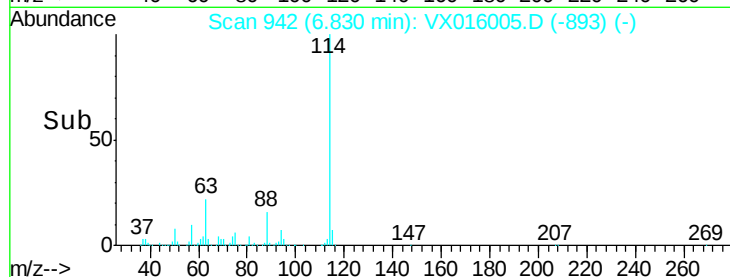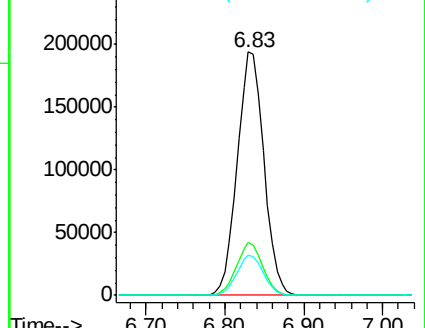

#35

Dibromofluoromethane

Concen: 47.873 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.01 min

Lab File: VX016005.D

Acq: 01 May 2020 12:18


Tgt Ion:113 Resp: 136502

Ion Ratio Lower Upper

113 100

111 101.0 81.8 122.8



192 20.8 16.8 25.2

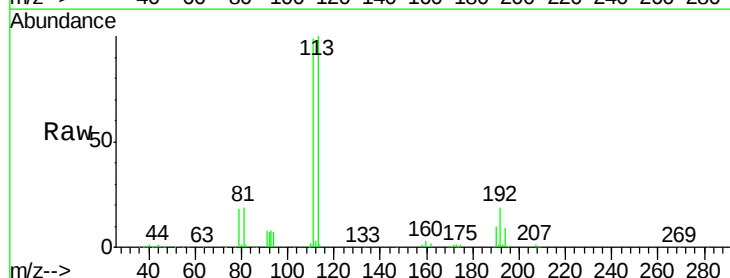


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

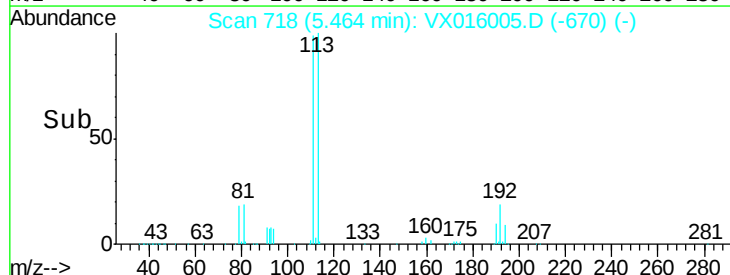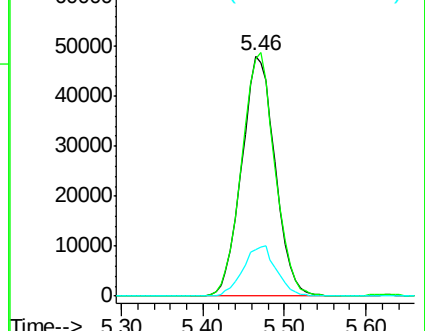

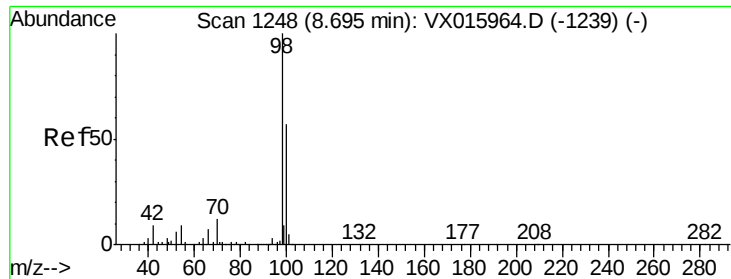

#50

Toluene-d8

Concen: 52.250 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. 0.00 min

Lab File: VX016005.D

Acq: 01 May 2020 12:18

Instrument :

MSVOA_X

ClientSampleId :





VX0501WBL02

Tot Ion: 98 Resp: 557030

Ion Ratio Lower Upper

98 100

100 66.7 53.1 79.7

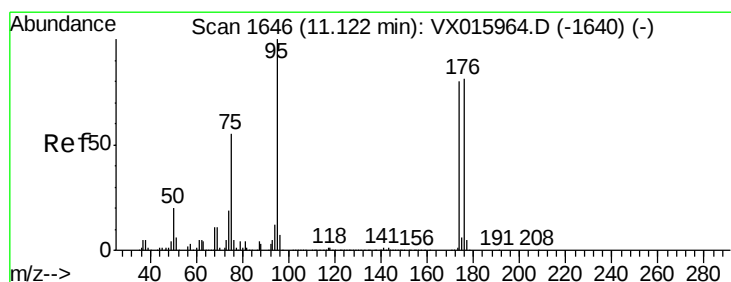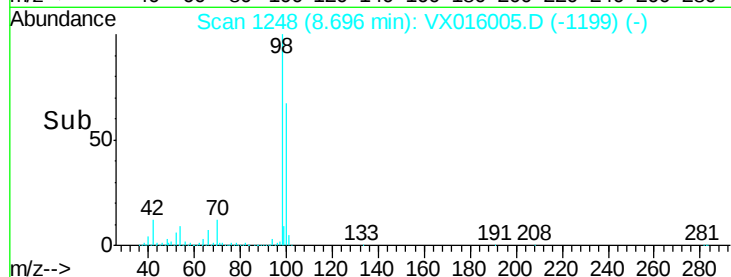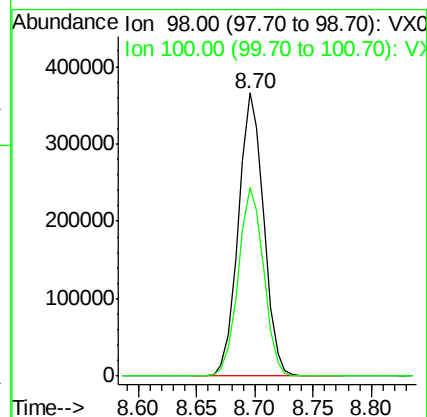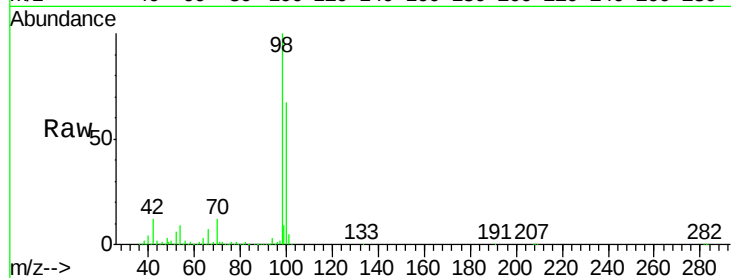

#62

4-Bromofluorobenzene

Concen: 51.751 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. 0.00 min

Lab File: VX016005.D

Acq: 01 May 2020 12:18




Tgt Ion: 95 Resp: 216388


Ion Ratio Lower Upper

95 100

174 80.7 0.0 165.0

176 79.5 0.0 163.2


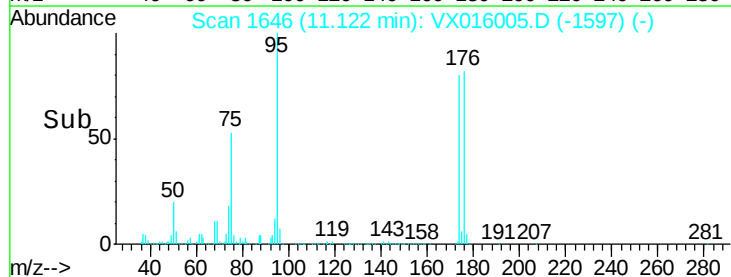
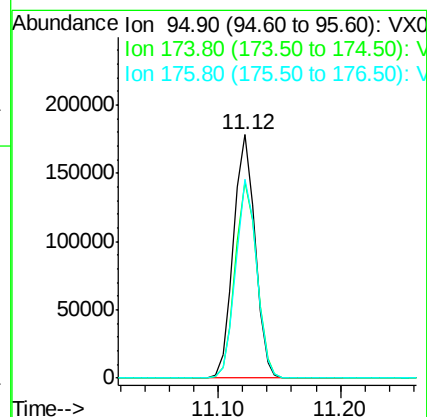
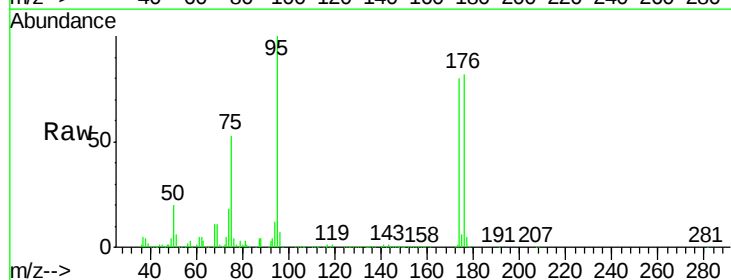


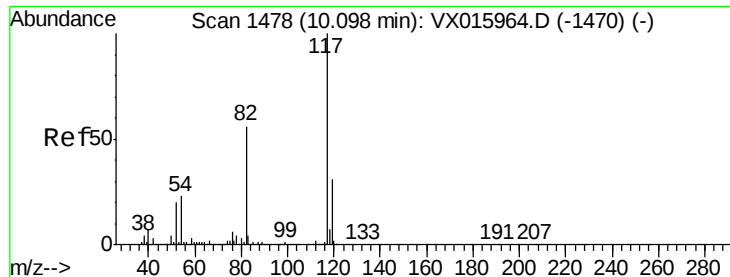

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. 0.00 min
Lab File: VX016005.D
Acq: 01 May 2020 12:18

Instrument :
MSVOA_X
ClientSampleId :
VX0501WBL02

Tot Ion:117 Resp: 432390
Ion Ratio Lower Upper
117 100
82 56.5 44.5 66.7
119 31.5 25.0 37.6

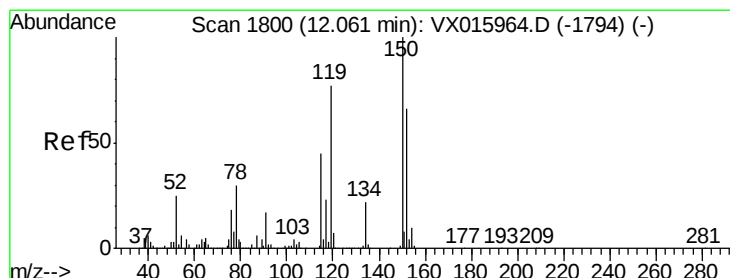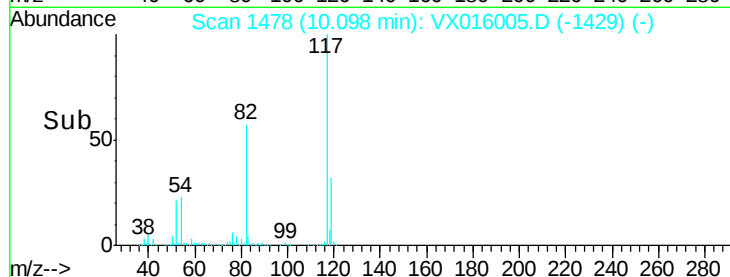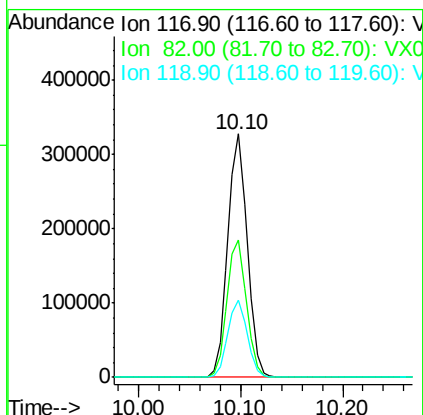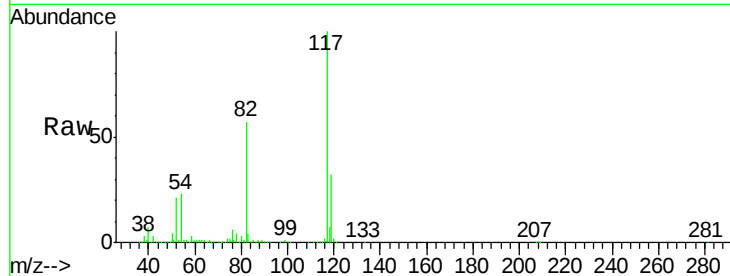

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. 0.00 min
Lab File: VX016005.D
Acq: 01 May 2020 12:18

Tgt Ion:152 Resp: 213245
Ion Ratio Lower Upper
152 100
115 58.1 40.9 122.7
150 155.1 0.0 342.4

