

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX050120\
 Data File : VX016017.D
 Acq On : 01 May 2020 17:25
 Operator : JC/SP
 Sample : L2469-03
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ187I-20200429

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.581	237	245	253	rBV	38772	77206	5.21%	0.895%
2	3.672	413	424	434	rBV	53048	126817	8.55%	1.470%
3	5.470	707	719	730	rBV	157957	450493	30.38%	5.222%
4	5.635	734	746	760	rVB	290919	810356	54.65%	9.393%
5	6.037	800	812	829	rBV	182629	484100	32.65%	5.611%
6	6.318	849	858	868	rBV3	9253	28722	1.94%	0.333%
7	6.836	932	943	955	rBV	445850	1060683	71.53%	12.294%
8	8.037	1129	1140	1145	rBV2	11179	23415	1.58%	0.271%
9	8.159	1153	1160	1169	rVB2	15194	31029	2.09%	0.360%
10	8.695	1241	1248	1264	rBV	936681	1482770	100.00%	17.187%
11	10.098	1472	1478	1489	rBV	1009903	1336422	90.13%	15.490%
12	10.640	1557	1567	1572	rBV8	6016	17009	1.15%	0.197%
13	11.122	1639	1646	1652	rBV	900061	1103633	74.43%	12.792%
14	11.933	1776	1779	1784	rVB	12224	15644	1.06%	0.181%
15	12.012	1786	1792	1795	rVV	11113	14972	1.01%	0.174%
16	12.061	1795	1800	1812	rVB	1122034	1446007	97.52%	16.761%
17	12.372	1849	1851	1858	rVB	19784	26411	1.78%	0.306%
18	12.878	1931	1934	1940	rVB	10710	15337	1.03%	0.178%
19	13.628	2053	2057	2061	rBV	32020	43439	2.93%	0.503%
20	13.701	2067	2069	2075	rVB	11494	15204	1.03%	0.176%
21	14.005	2116	2119	2124	rVB2	13208	17786	1.20%	0.206%


Sum of corrected areas: 8627455

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX050120\
Data File : VX016017.D
Acq On : 01 May 2020 17:25
Operator : JC/SP
Sample : L2469-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ187I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

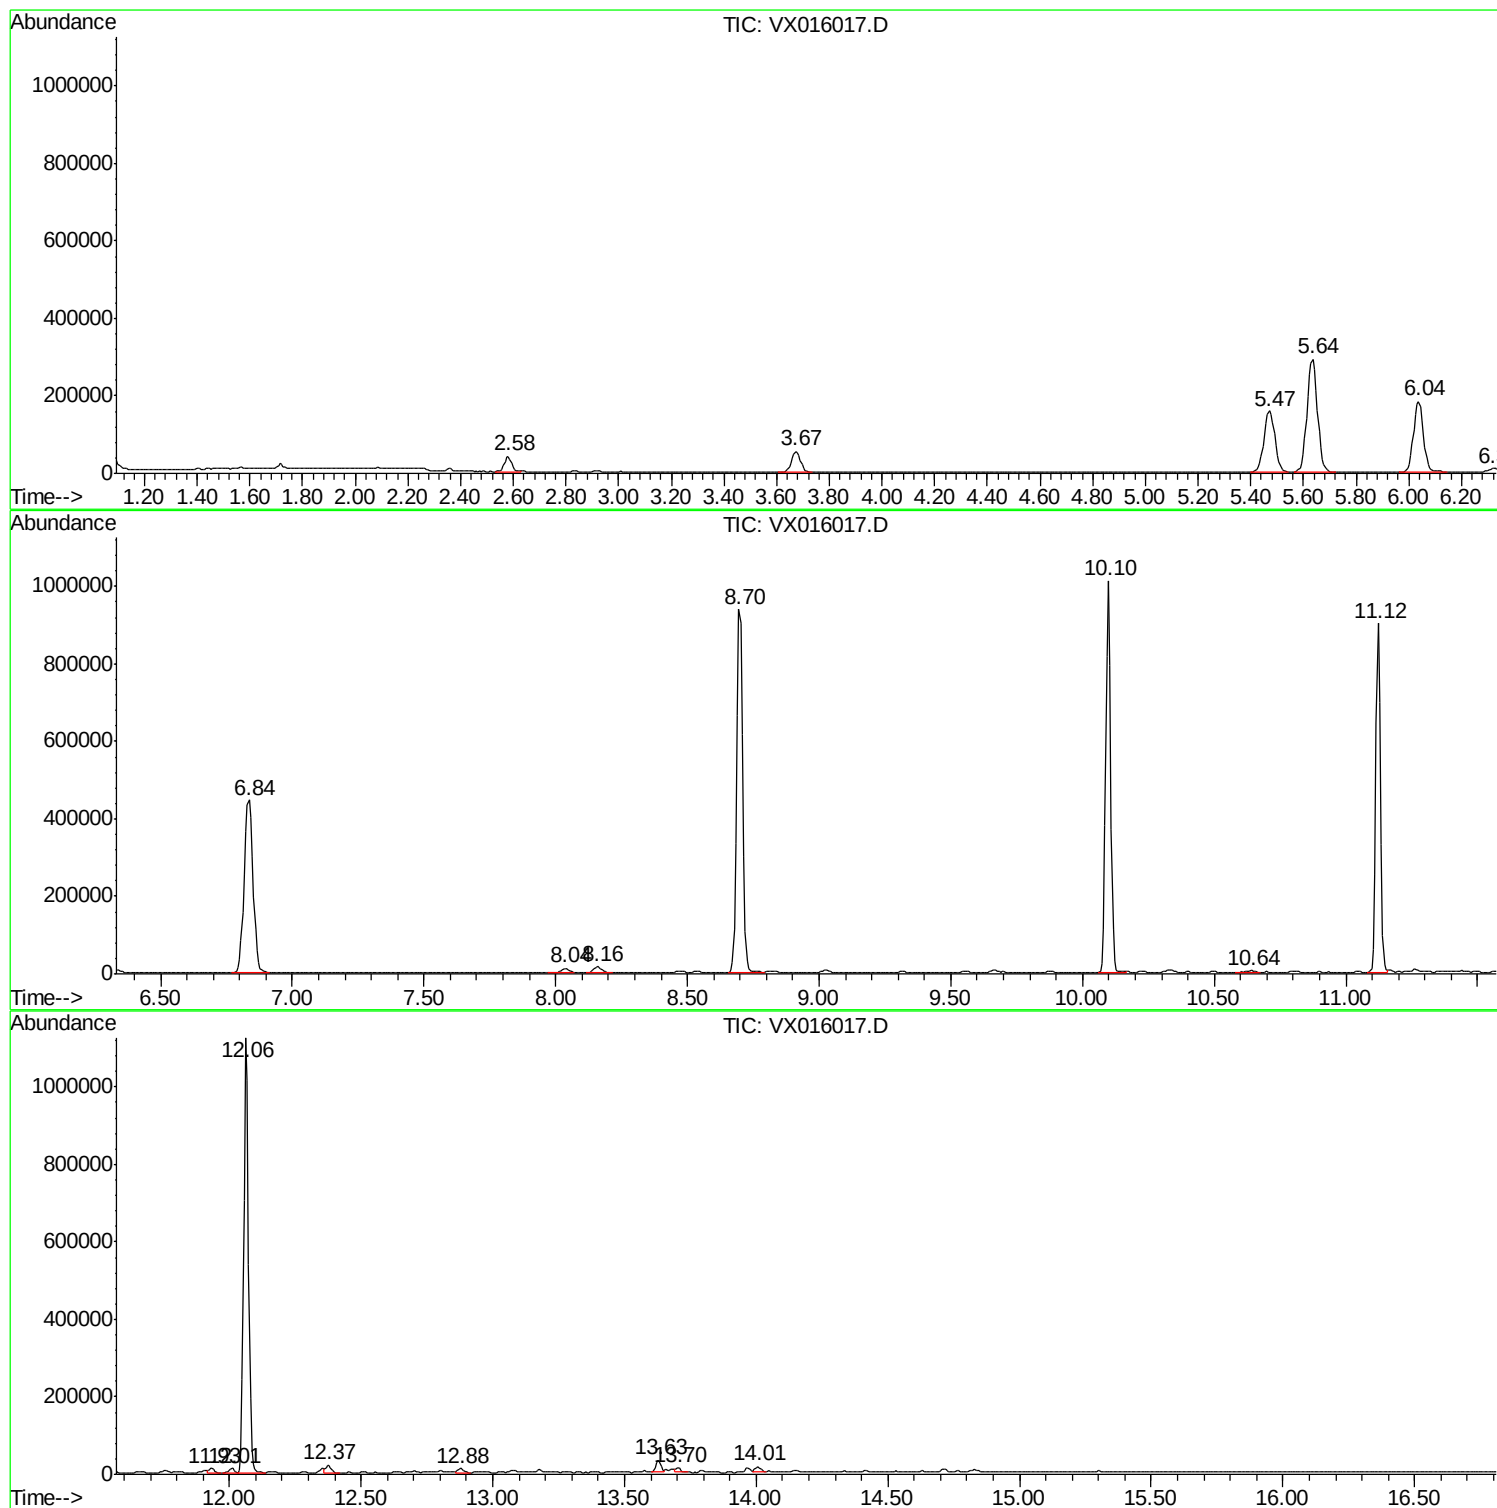

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX050120\
Data File : VX016017.D
Acq On : 01 May 2020 17:25
Operator : JC/SP
Sample : L2469-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ187I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX050120\
Data File : VX016017.D
Acq On : 01 May 2020 17:25
Operator : JC/SP
Sample : L2469-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ187I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc