

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX050120\
 Data File : VX016020.D
 Acq On : 01 May 2020 18:33
 Operator : JC/SP
 Sample : L2469-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SA-PZ190I-20200429

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.715	99	103	110	rVB	65863	78551	5.08%	0.791%
2	2.355	202	208	216	rBV	42535	68133	4.41%	0.686%
3	2.575	235	244	254	rBV	36419	73523	4.76%	0.740%
4	3.672	411	424	439	rBV	466751	1103255	71.42%	11.111%
5	5.471	705	719	733	rBV	171359	492769	31.90%	4.963%
6	5.635	733	746	761	rVB	285411	803080	51.99%	8.088%
7	6.038	800	812	822	rBV	183817	482876	31.26%	4.863%
8	6.836	931	943	955	rBV	447697	1055490	68.32%	10.630%
9	8.696	1241	1248	1258	rBV	936263	1467676	95.01%	14.782%
10	10.098	1472	1478	1491	rBV	1003359	1360203	88.05%	13.699%
11	10.323	1510	1515	1525	rVB5	8905	18056	1.17%	0.182%
12	11.122	1640	1646	1652	rBV	868423	1087963	70.43%	10.957%
13	11.756	1743	1750	1755	rBV	17320	23240	1.50%	0.234%
14	11.908	1770	1775	1776	rBV	13798	18913	1.22%	0.190%
15	11.933	1776	1779	1786	rVV	41038	49615	3.21%	0.500%
16	12.012	1786	1792	1795	rVV	24279	32843	2.13%	0.331%
17	12.067	1795	1801	1814	rVB	1100845	1544812	100.00%	15.558%
18	12.378	1843	1852	1856	rBV	31780	44001	2.85%	0.443%
19	12.878	1927	1934	1940	rVB	26023	39366	2.55%	0.396%
20	13.628	2053	2057	2060	rBV2	17883	24704	1.60%	0.249%
21	13.701	2066	2069	2075	rVB	28183	43944	2.84%	0.443%
22	14.146	2138	2142	2148	rVB4	12514	16111	1.04%	0.162%


Sum of corrected areas: 9929124

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX050120\
Data File : VX016020.D
Acq On : 01 May 2020 18:33
Operator : JC/SP
Sample : L2469-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ190I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

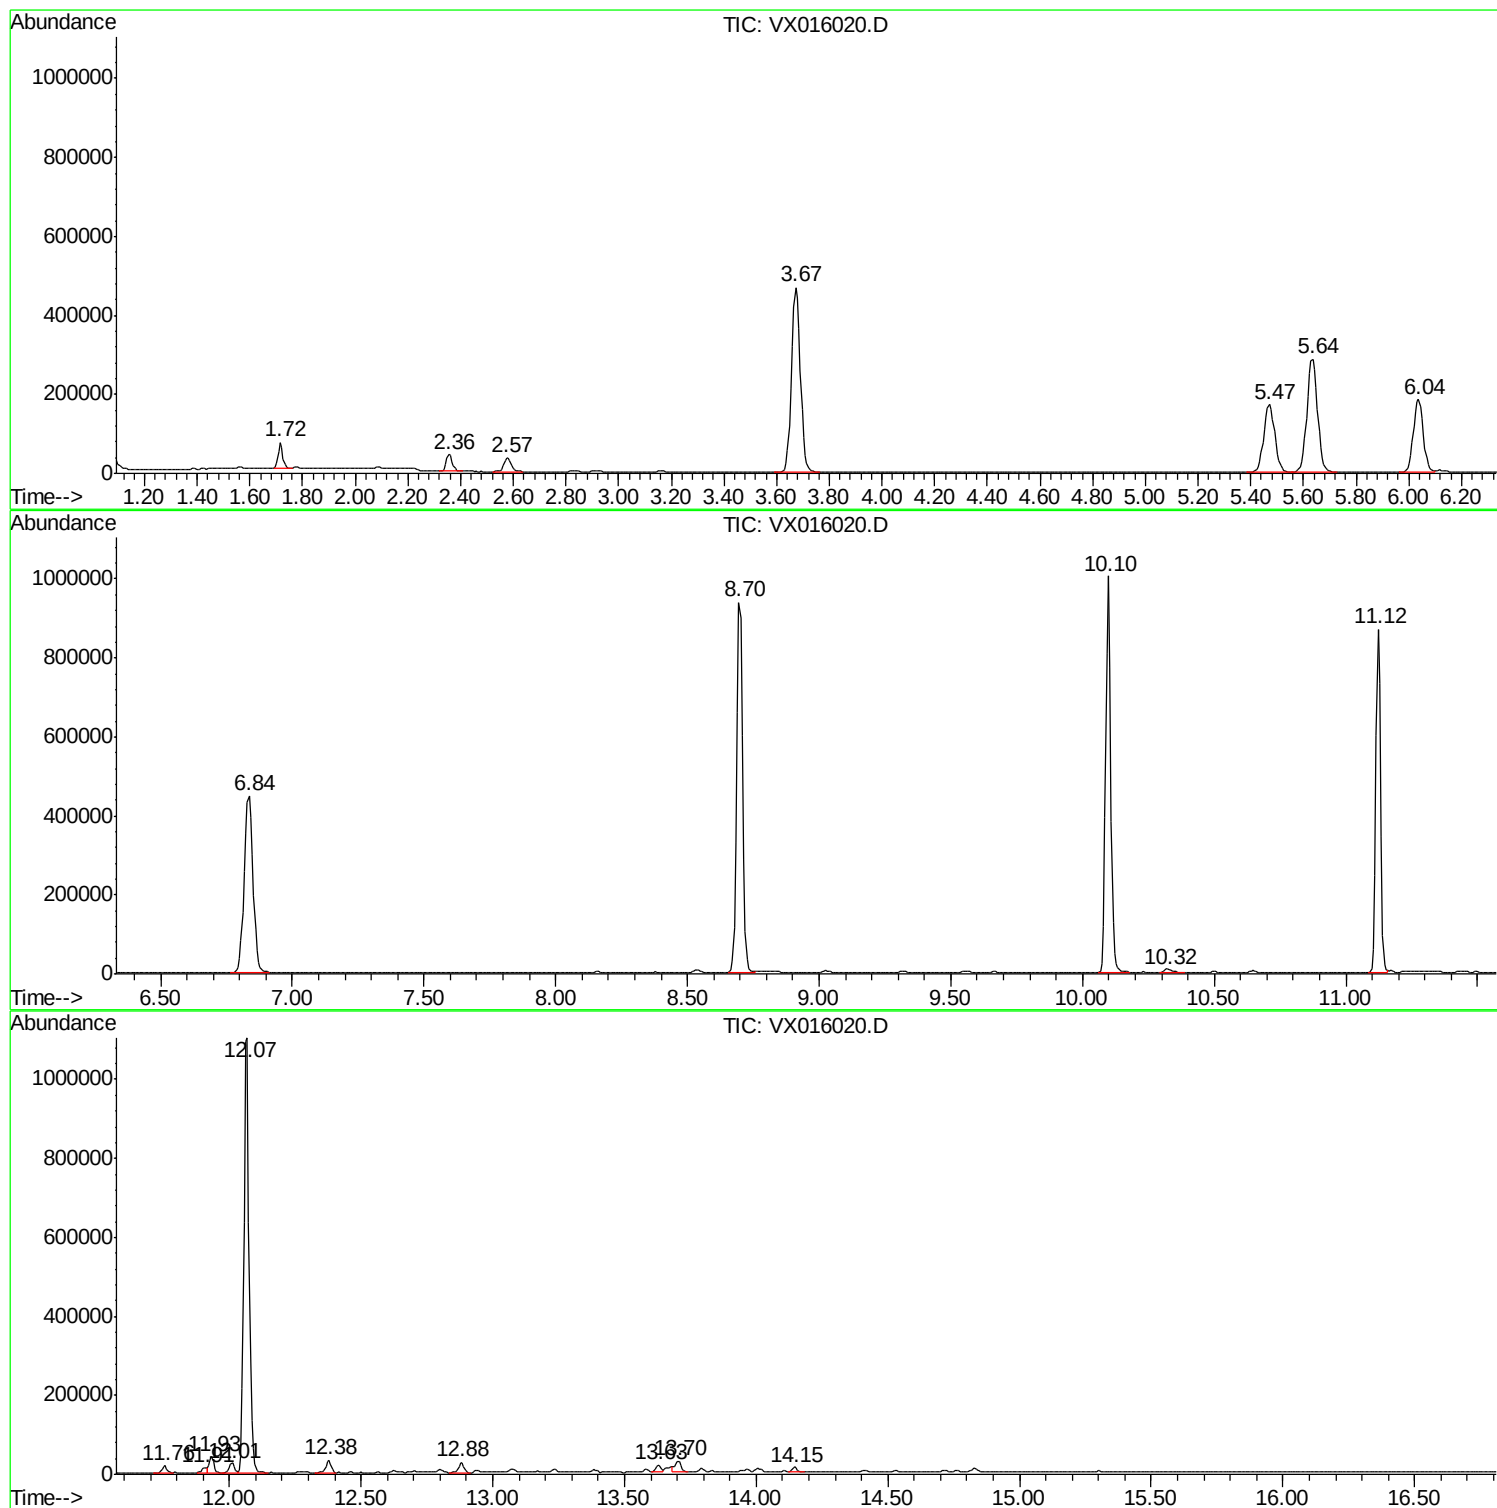

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX050120\
Data File : VX016020.D
Acq On : 01 May 2020 18:33
Operator : JC/SP
Sample : L2469-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ190I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX050120\
Data File : VX016020.D
Acq On : 01 May 2020 18:33
Operator : JC/SP
Sample : L2469-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SA-PZ190I-20200429

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X042820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc