

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
 Data File : VX035440.D
 Acq On : 01 May 2023 15:08
 Operator : JC/MD
 Sample : 02558-05
 Misc : 4.49g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-SS012-0006-01

Quant Time: May 02 00:00:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	237023	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	388045	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	360217	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	171813	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	141123	49.352	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.700%		
35) Dibromofluoromethane	5.379	113	109360	45.917	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	91.840%		
50) Toluene-d8	8.647	98	464147	51.660	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	103.320%		
62) 4-Bromofluorobenzene	11.085	95	177288	52.455	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	104.900%		
Target Compounds						Qvalue
13) Acrolein	1.989	56	142	0.277	ug/l #	20
16) Acetone	2.404	43	1875	1.510	ug/l	91
18) Methyl Acetate	2.715	43	3174	0.661	ug/l	96
20) Methylene Chloride	2.788	84	1397	0.491	ug/l #	84
25) 2-Butanone	4.611	43	2519	1.390	ug/l	93
29) Tetrahydrofuran	5.050	42	809	0.696	ug/l	97
36) 1,1-Dichloropropene	5.544	75	17662	4.749	ug/l #	50
38) Carbon Tetrachloride	5.544	117	23073	6.536	ug/l #	16
39) Methylcyclohexane	7.373	83	4013	0.886	ug/l	88
43) Isopropyl Acetate	6.361	43	1326	0.232	ug/l #	62
52) Toluene	8.720	92	4022	0.595	ug/l	99
55) 1,1,2-Trichloroethane	9.098	97	1300	0.482	ug/l #	18
59) 2-Hexanone	9.384	43	2628	0.998	ug/l #	26
67) Ethyl Benzene	10.195	91	17900	1.326	ug/l	99
68) m/p-Xylenes	10.299	106	31659	6.122	ug/l	100
69) o-Xylene	10.640	106	22067	4.351	ug/l	95
73) Isopropylbenzene	10.963	105	14043	1.118	ug/l	99
74) N-amyl acetate	10.854	43	11576	2.453	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.219	83	10589	2.716	ug/l #	26
76) 1,2,3-Trichloropropane	11.378	75	2831	0.826	ug/l #	1
78) n-propylbenzene	11.305	91	51684	3.583	ug/l	98
79) 2-Chlorotoluene	11.378	91	33861	3.757	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.451	105	154982	14.635	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.085	75	85849	81.128	ug/l #	10
83) tert-Butylbenzene	11.713	119	2872	0.270	ug/l	94
84) 1,2,4-Trimethylbenzene	11.756	105	423189	39.772	ug/l	99
85) sec-Butylbenzene	11.890	105	40853	3.134	ug/l	83
86) p-Isopropyltoluene	12.012	119	37777	3.408	ug/l	99
89) n-Butylbenzene	12.323	91	137102	14.651	ug/l #	24
90) Hexachloroethane	12.530	117	18645	10.988	ug/l #	16
92) 1,2-Dibromo-3-Chloropr...	12.963	75	3281	4.197	ug/l #	16
95) Naphthalene	13.780	128	440170	38.333	ug/l	97
96) 1,2,3-Trichlorobenzene	13.975	180	2492	0.664	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_X


ClientSampleId :


P001-SS012-0006-01

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
Data File : VX035440.D
Acq On : 01 May 2023 15:08
Operator : JC/MD
Sample : 02558-05
Misc : 4.49g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01

Quant Time: May 02 00:00:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration




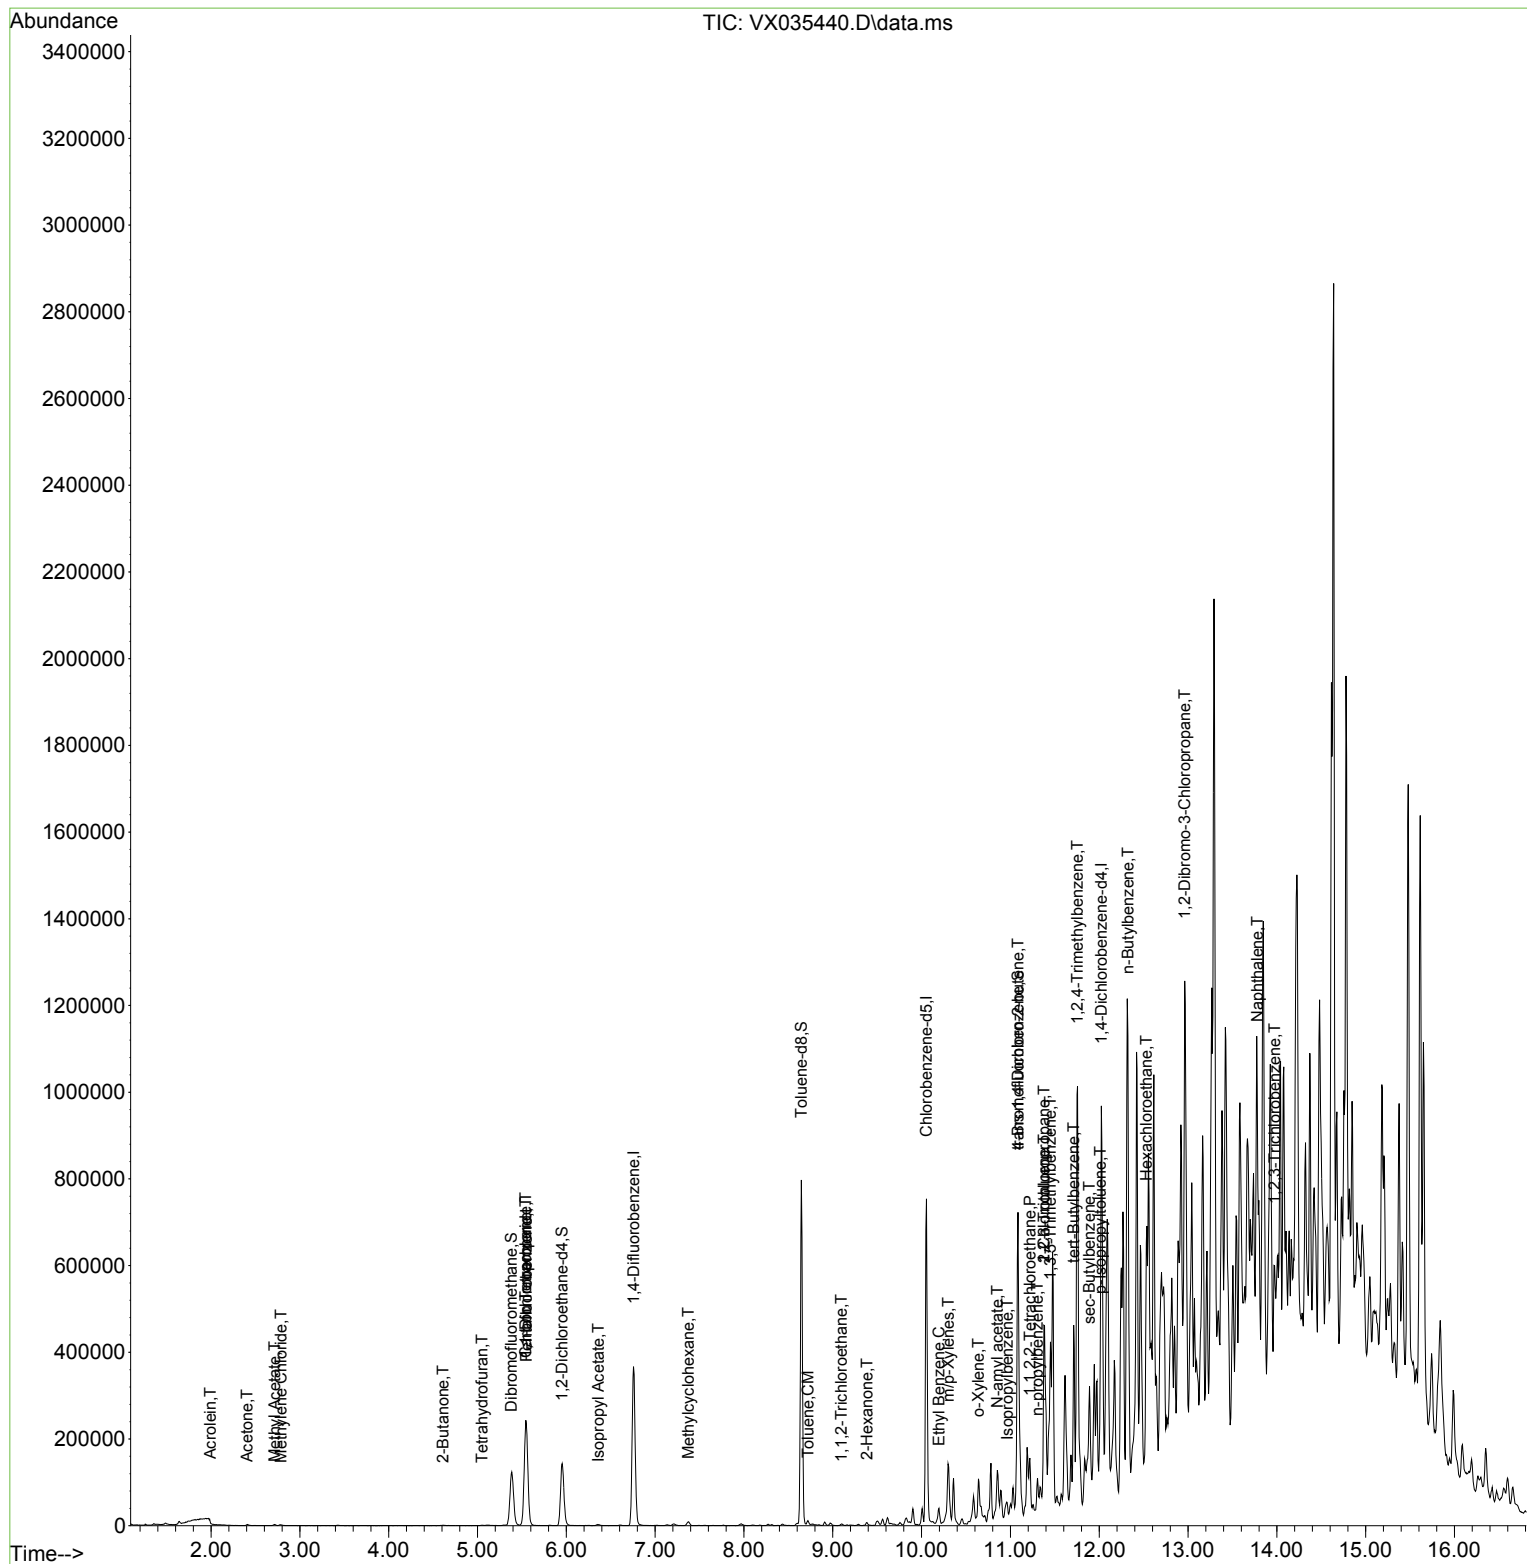




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion:168 Resp: 237023
Ion Ratio Lower Upper
168 100
99 55.3 45.7 68.5



#13
Acrolein
Concen: 0.277 ug/l
RT: 1.989 min Scan# 148
Delta R.T. -0.250 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 56 Resp: 142
Ion Ratio Lower Upper
56 100
55 136.6 56.6 85.0#


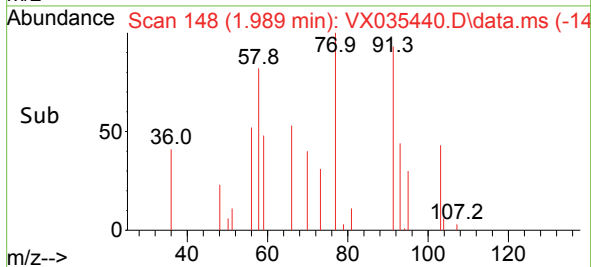

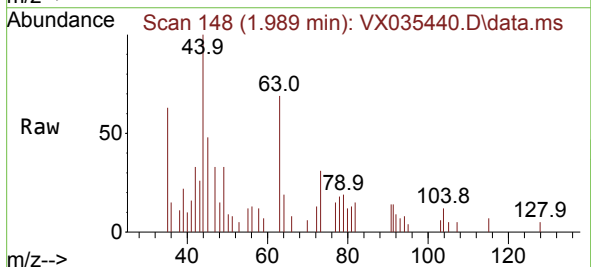




#16
Acetone
Concen: 1.510 ug/l
RT: 2.404 min Scan# 215
Delta R.T. 0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 43 Resp: 1875
Ion Ratio Lower Upper
43 100
58 35.8 24.7 37.1



#18
Methyl Acetate
Concen: 0.661 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.007 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 43 Resp: 3174
Ion Ratio Lower Upper
43 100
74 20.8 18.3 27.5





#20

Methylene Chloride

Concen: 0.491 ug/l

RT: 2.788 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX035440.D


Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01



Tgt Ion: 84 Resp: 1397




Ion Ratio Lower Upper

84 100

49 111.4 103.8 155.8

51 29.7 31.8 47.8#

86 77.6 51.4 77.2#

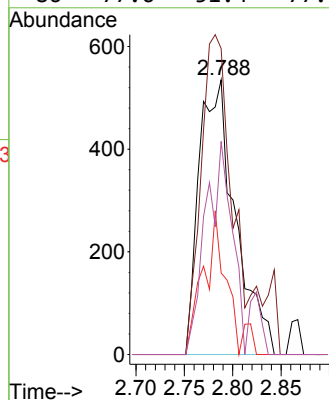

#25

2-Butanone

Concen: 1.390 ug/l

RT: 4.611 min Scan# 578

Delta R.T. 0.043 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 43 Resp: 2519

Ion Ratio Lower Upper

43 100

72 20.5 19.3 28.9

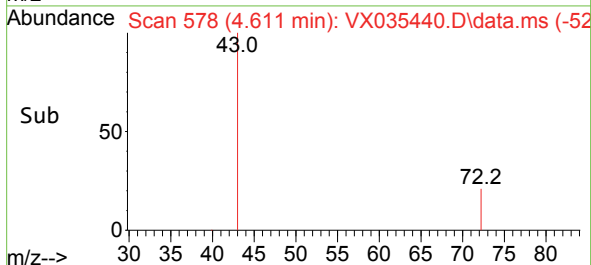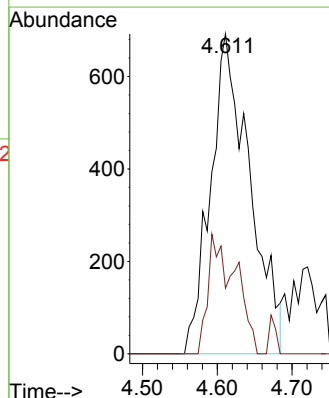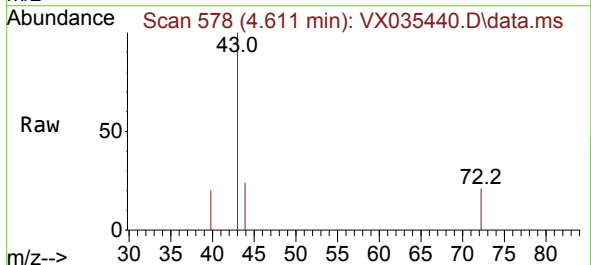



#29

Tetrahydrofuran

Concen: 0.696 ug/l

RT: 5.050 min Scan# 61

Delta R.T. 0.037 min

Lab File: VX035440.D


Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01






Tgt Ion: 42 Resp: 809

Ion Ratio Lower Upper

42 100

72 39.6 34.5 51.7

71 40.0 32.1 48.1

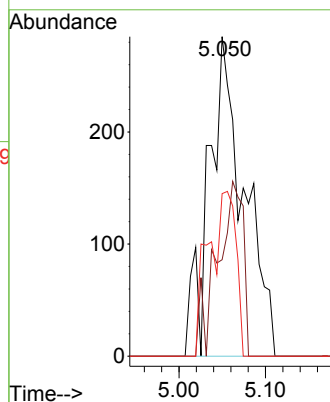

#33

1,2-Dichloroethane-d4

Concen: 49.352 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.006 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 65 Resp: 141123

Ion Ratio Lower Upper

65 100

67 52.2 0.0 104.0


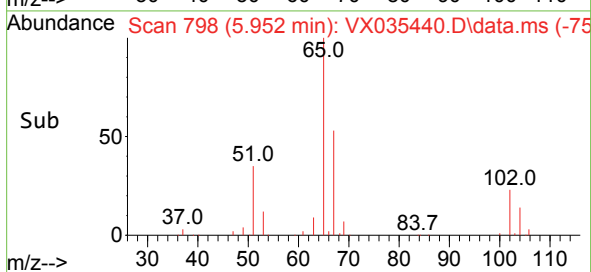
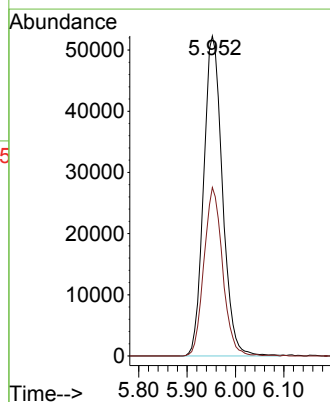





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion:114 Resp: 388045
Ion Ratio Lower Upper
114 100
63 19.2 0.0 42.2
88 16.7 0.0 33.2



#35
Dibromofluoromethane
Concen: 45.917 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion:113 Resp: 109360
Ion Ratio Lower Upper
113 100
111 103.3 83.7 125.5
192 20.6 15.4 23.2


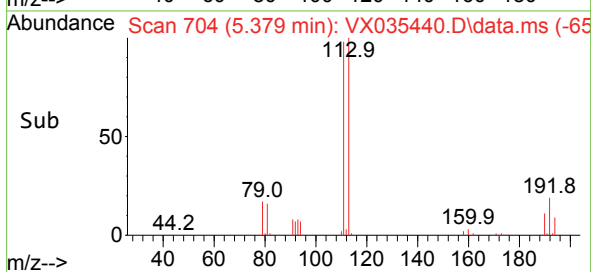






#36
1,1-Dichloropropene
Concen: 4.749 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.146 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 75 Resp: 17662
Ion Ratio Lower Upper
75 100
110 9.3 17.5 52.5#
77 0.0 24.3 36.5#



#38
Carbon Tetrachloride
Concen: 6.536 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.133 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 117 Resp: 23073
Ion Ratio Lower Upper
117 100
119 5.4 76.6 114.8#
121 0.0 23.8 35.6#

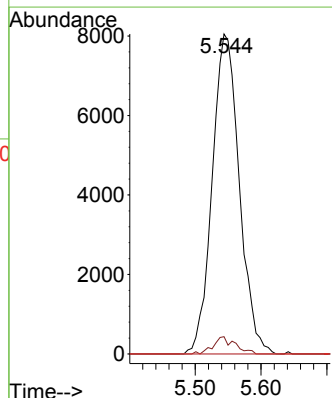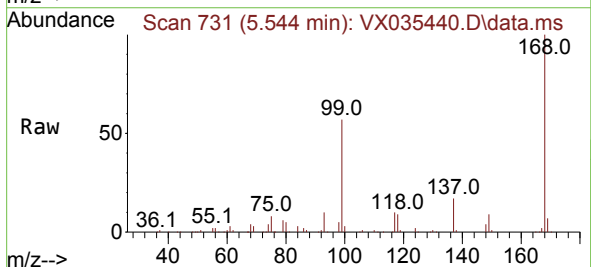



#39

Methylcyclohexane

Concen: 0.886 ug/l

RT: 7.373 min Scan# 1032

Delta R.T. -0.005 min

Lab File: VX035440.D


Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01

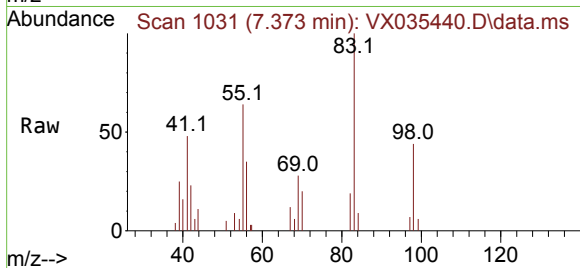




Tgt Ion: 83 Resp: 4013

Ion Ratio Lower Upper

83 100

55 64.4 60.5 90.7

98 43.5 40.4 60.6



#43

Isopropyl Acetate

Concen: 0.232 ug/l

RT: 6.361 min Scan# 865

Delta R.T. 0.025 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08




Tgt Ion: 43 Resp: 1326


Ion Ratio Lower Upper

43 100

61 0.0 15.2 22.8#

87 0.0 9.8 14.8#




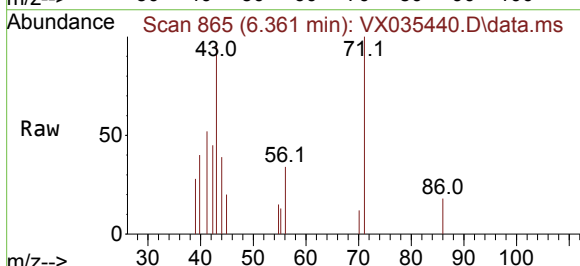




#50
Toluene-d8
Concen: 51.660 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.001 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 98 Resp: 464147
Ion Ratio Lower Upper
98 100
100 67.2 52.5 78.7



#52
Toluene
Concen: 0.595 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.000 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 92 Resp: 4022
Ion Ratio Lower Upper
92 100
91 169.6 136.8 205.2

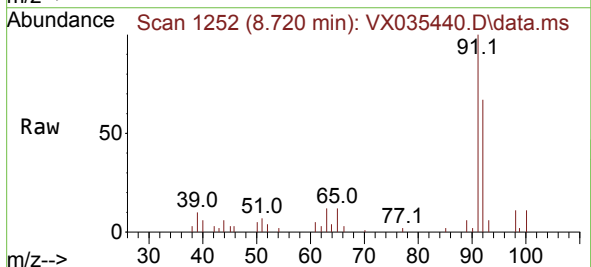



#55

1,1,2-Trichloroethane

Concen: 0.482 ug/l

RT: 9.098 min Scan# 1

Delta R.T. -0.054 min

Lab File: VX035440.D


Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01



Tgt Ion: 97 Resp: 1300




Ion Ratio Lower Upper

97 100

83 0.0 69.7 104.5#

85 7.3 43.7 65.5#

99 0.0 49.7 74.5#



#59

2-Hexanone

Concen: 0.998 ug/l

RT: 9.384 min Scan# 1361

Delta R.T. -0.049 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 43 Resp: 2628

Ion Ratio Lower Upper

43 100

58 0.0 26.3 78.9#









#62
4-Bromofluorobenzene
Concen: 52.455 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 95 Resp: 177288
Ion Ratio Lower Upper
95 100
174 79.6 0.0 147.4
176 75.9 0.0 140.6

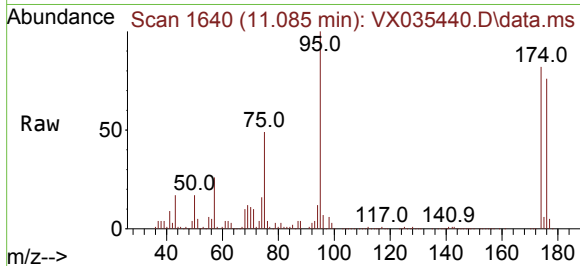

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 117 Resp: 360217
Ion Ratio Lower Upper
117 100
82 54.4 45.0 67.4
119 33.0 26.0 39.0

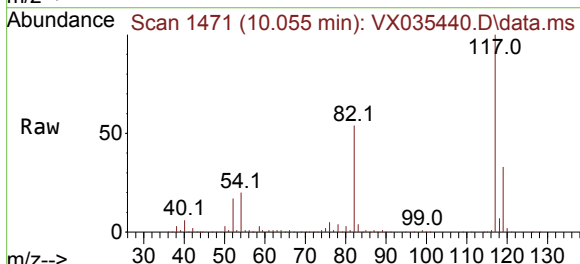



#67

Ethyl Benzene

Concen: 1.326 ug/l

RT: 10.195 min Scan# 1494

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :





P001-SS012-0006-01

Tgt Ion: 91 Resp: 17900

Ion Ratio Lower Upper

91 100

106 31.6 25.6 38.4

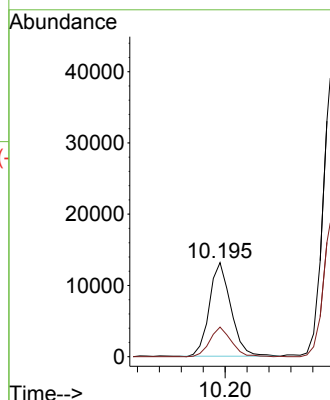

#68

m/p-Xylenes

Concen: 6.122 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 106 Resp: 31659

Ion Ratio Lower Upper

106 100

91 204.8 164.0 246.0

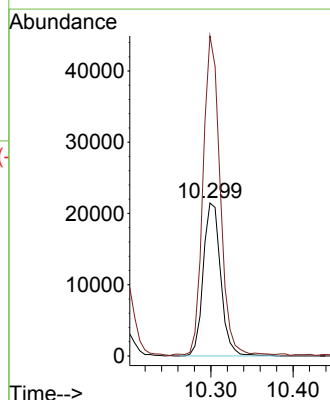



#69

o-Xylene

Concen: 4.351 ug/l

RT: 10.640 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :





P001-SS012-0006-01

Tgt Ion:106 Resp: 22067

Ion Ratio Lower Upper

106 100

91 209.2 108.5 325.3

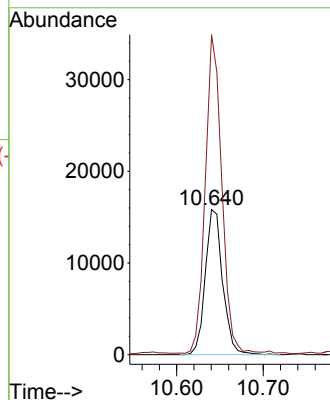

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.024 min Scan# 1794

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08




Tgt Ion:152 Resp: 171813


Ion Ratio Lower Upper

152 100

115 62.5 45.0 135.0

150 157.1 0.0 352.4


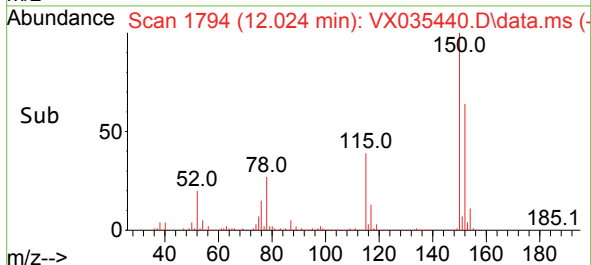
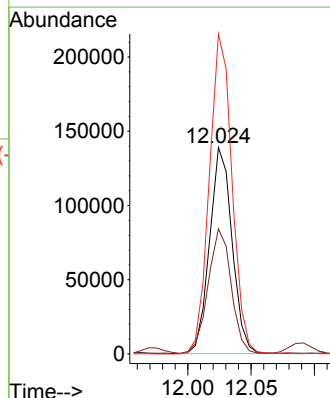
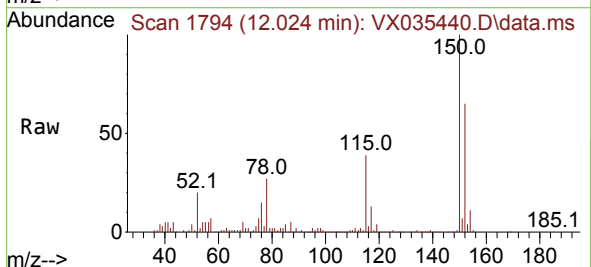


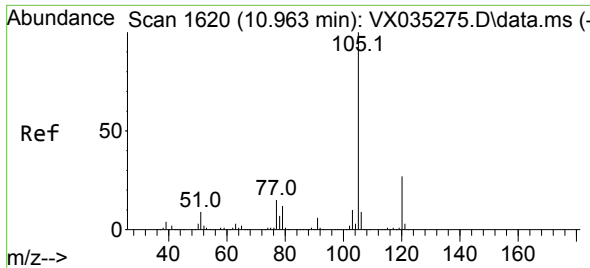

#73
Isopropylbenzene
Concen: 1.118 ug/l
RT: 10.963 min Scan# 1602
Delta R.T. 0.000 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion:105 Resp: 14043
Ion Ratio Lower Upper
105 100
120 27.4 13.3 39.9

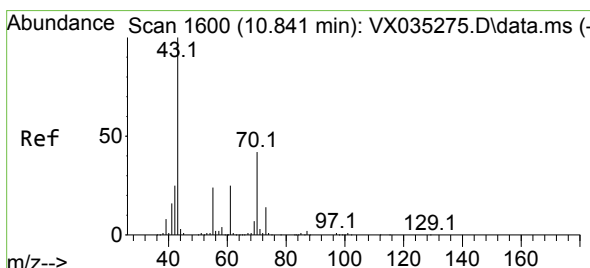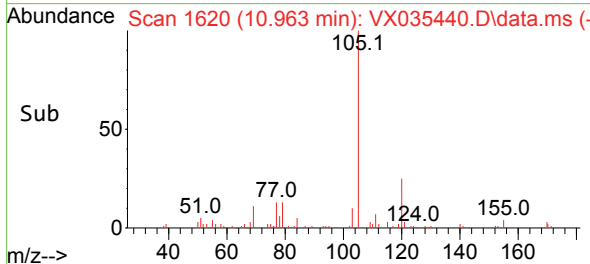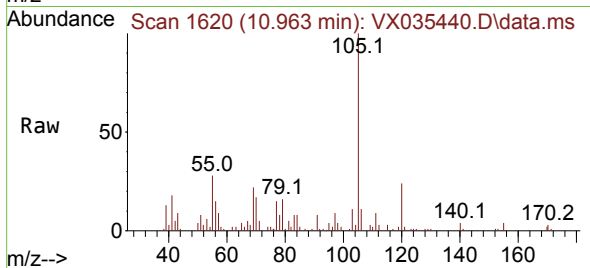

#74
N-ethyl acetate
Concen: 2.453 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.013 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 43 Resp: 11576
Ion Ratio Lower Upper
43 100
70 69.9 32.1 48.1#
55 218.2 18.3 27.5#
61 0.0 18.8 28.2#

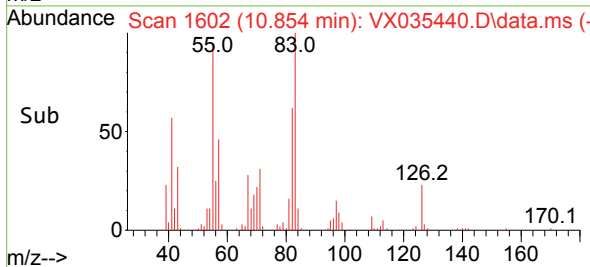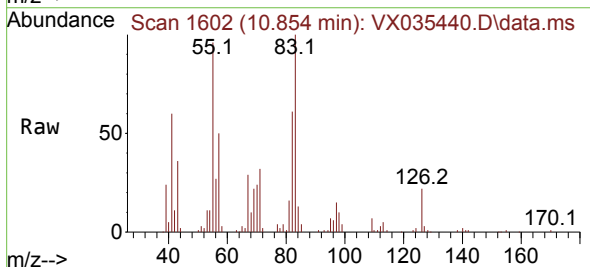



#75

1,1,2,2-Tetrachloroethane

Concen: 2.716 ug/l

RT: 11.219 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01





Tgt Ion: 83 Resp: 10589

Ion Ratio Lower Upper

83 100

131 0.6 4.8 14.3#

85 0.0 32.0 96.0#

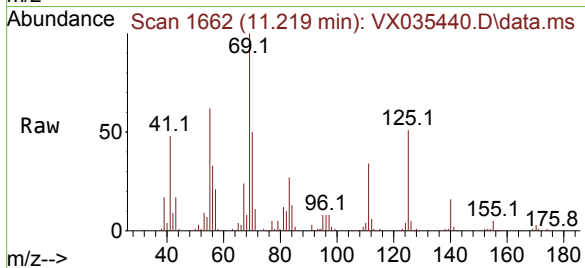

#76

1,2,3-Trichloropropane

Concen: 0.826 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.141 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 75 Resp: 2831

Ion Ratio Lower Upper

75 100

77 1223.8 21.6 64.8#

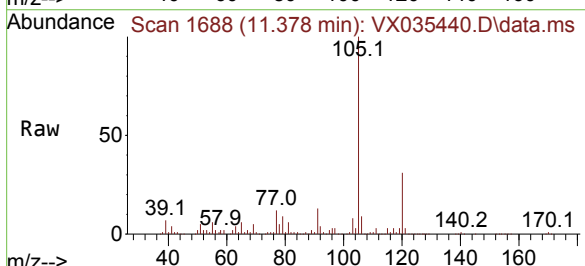



#78

n-propylbenzene

Concen: 3.583 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.001 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :





P001-SS012-0006-01

Tgt Ion: 91 Resp: 51684

Ion Ratio Lower Upper

91 100

120 22.2 11.5 34.5

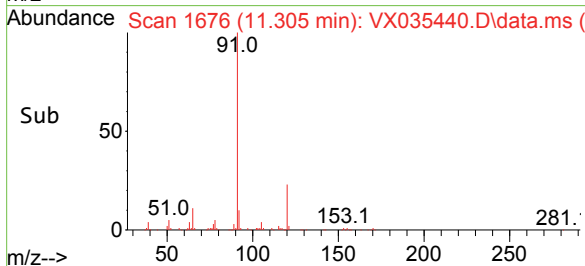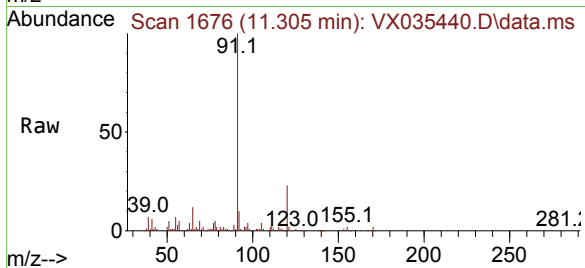

#79

2-Chlorotoluene

Concen: 3.757 ug/l

RT: 11.378 min Scan# 1688

Delta R.T. 0.013 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion: 91 Resp: 33861

Ion Ratio Lower Upper

91 100

126 1.2 16.3 48.9#

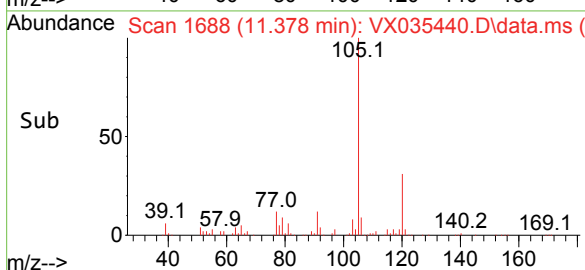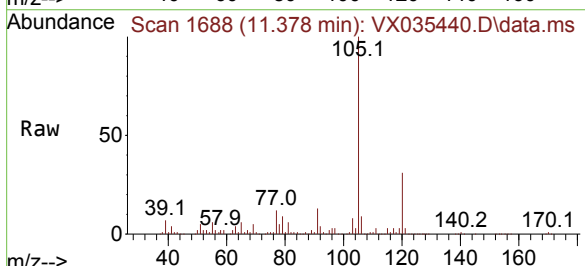



#80

1,3,5-Trimethylbenzene

Concen: 14.635 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :





P001-SS012-0006-01

Tgt Ion:105 Resp: 154982

Ion Ratio Lower Upper

105 100

120 49.1 23.7 71.1

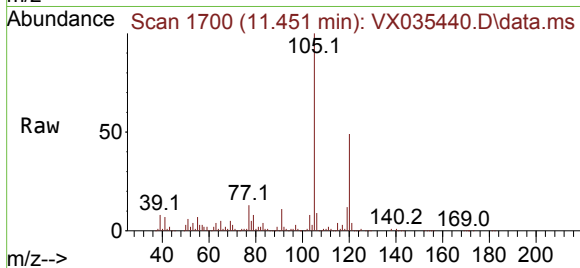

#81

trans-1,4-Dichloro-2-butene

Concen: 81.128 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.067 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08




Tgt Ion: 75 Resp: 85849


Ion Ratio Lower Upper

75 100

53 1.7 82.6 124.0#

89 0.0 36.9 55.3#

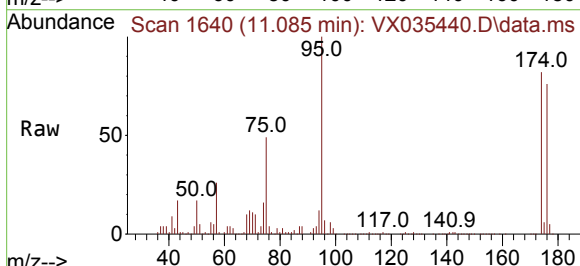



#83

tert-Butylbenzene

Concen: 0.270 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :

P001-SS012-0006-01





Tgt Ion:119 Resp: 2872

Ion Ratio Lower Upper

119 100

91 66.3 30.6 92.0

134 20.9 11.8 35.4

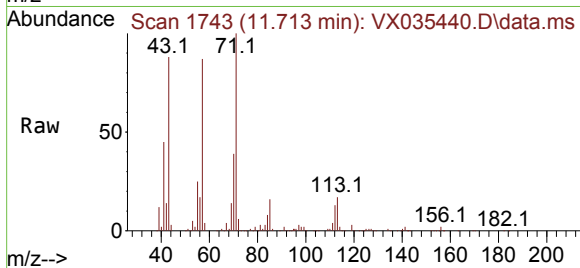

#84

1,2,4-Trimethylbenzene

Concen: 39.772 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.007 min

Lab File: VX035440.D




Acq: 01 May 2023 15:08


Tgt Ion:105 Resp: 423189

Ion Ratio Lower Upper

105 100

120 45.2 22.4 67.0

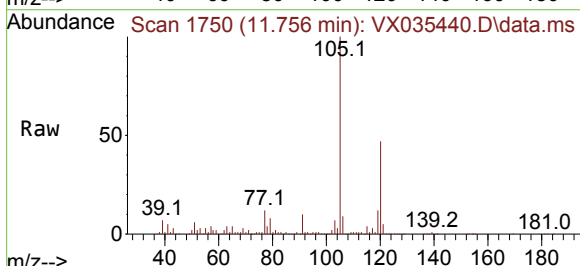

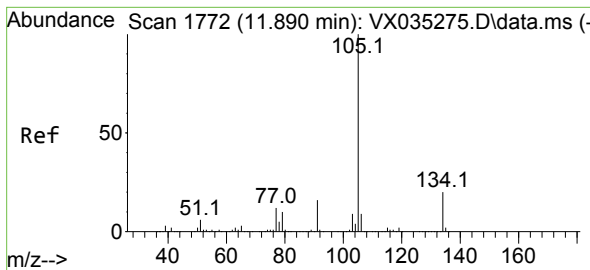

#85

sec-Butylbenzene

Concen: 3.134 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08

Instrument :

MSVOA_X

ClientSampleId :





P001-SS012-0006-01

Tgt Ion:105 Resp: 40853

Ion Ratio Lower Upper

105 100

134 28.4 10.2 30.4

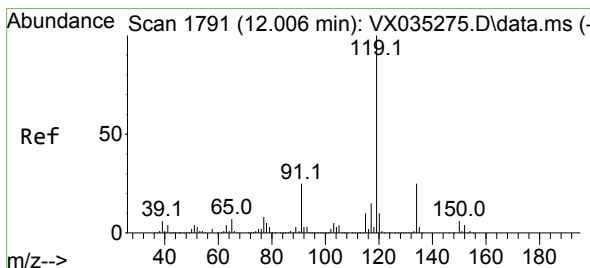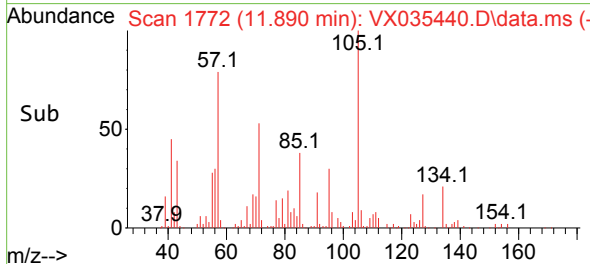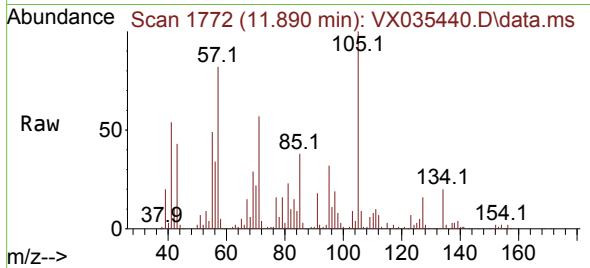

#86

p-Isopropyltoluene

Concen: 3.408 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX035440.D

Acq: 01 May 2023 15:08




Tgt Ion:119 Resp: 37777


Ion Ratio Lower Upper

119 100

134 26.6 13.2 39.5

91 24.6 12.9 38.7


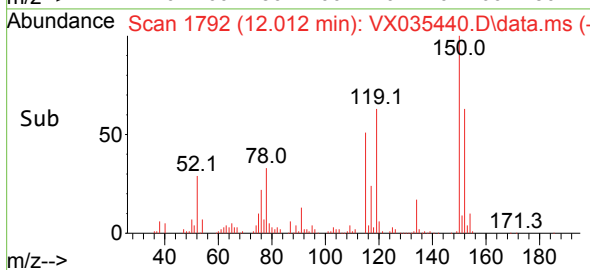

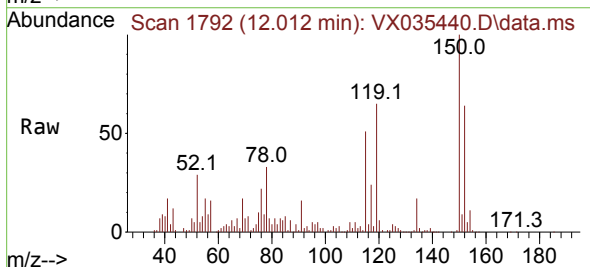




#89
n-Butylbenzene
Concen: 14.651 ug/l
RT: 12.323 min Scan# 1843
Delta R.T. -0.012 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 91 Resp: 137102
Ion Ratio Lower Upper
91 100
92 32.0 27.7 83.0
134 112.7 13.0 38.9#

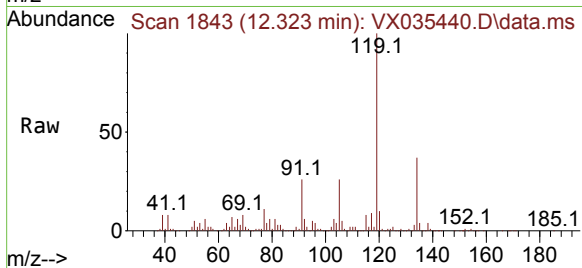

#90
Hexachloroethane
Concen: 10.988 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08

Tgt Ion: 117 Resp: 18645
Ion Ratio Lower Upper
117 100
201 0.7 34.4 103.1#


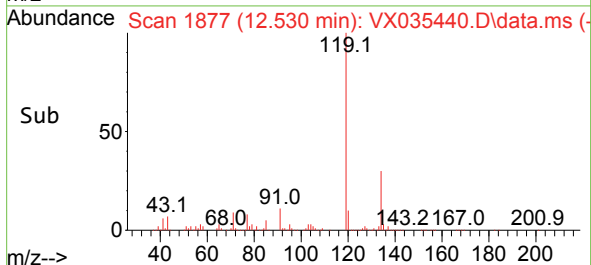

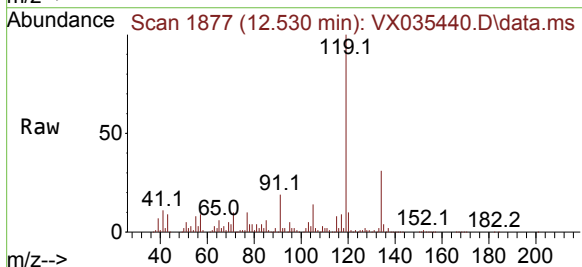


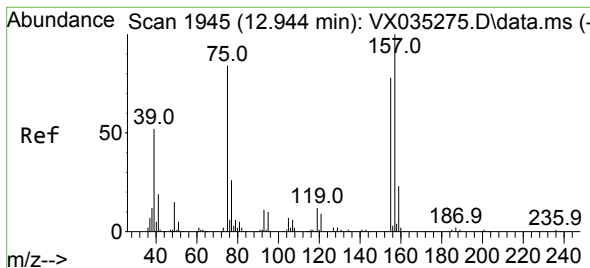

#92
1,2-Dibromo-3-Chloropropane
Concen: 4.197 ug/l
RT: 12.963 min Scan# 1948
Delta R.T. 0.019 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08




Instrument :
MSVOA_X
ClientSampleId :
P001-SS012-0006-01


Tgt Ion: 75 Resp: 3281
Ion Ratio Lower Upper
75 100
155 22.5 38.4 115.1#
157 0.6 49.9 149.7#

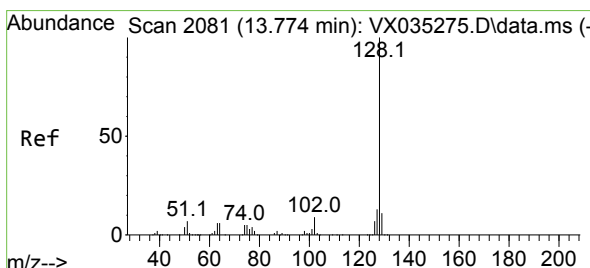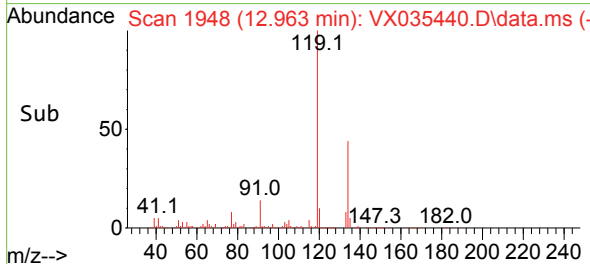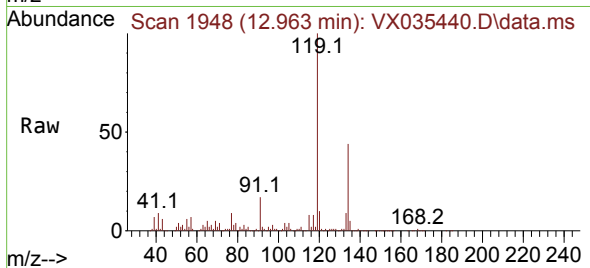

#95
Naphthalene
Concen: 38.333 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX035440.D
Acq: 01 May 2023 15:08


Tgt Ion: 128 Resp: 440170
Ion Ratio Lower Upper
128 100
127 13.2 10.2 15.4
129 12.6 8.6 13.0

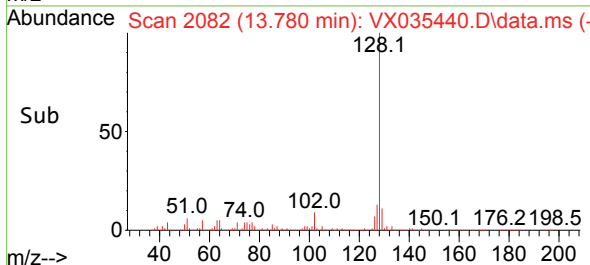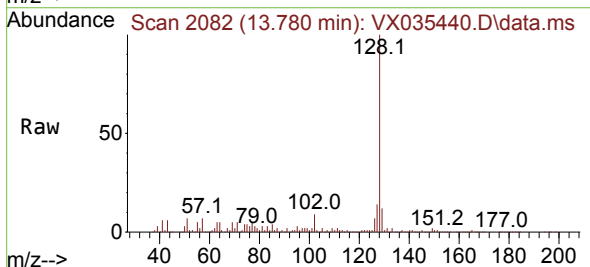



#96
 1,2,3-Trichlorobenzene
 Concen: 0.664 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX035440.D
 Acq: 01 May 2023 15:08

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-SS012-0006-01



Tgt Ion:180 Resp: 2492
 Ion Ratio Lower Upper
 180 100
 182 0.0 48.0 144.2#
 145 1936.8 17.7 53.1#

