

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
 Data File : VX035441.D
 Acq On : 01 May 2023 15:31
 Operator : JC/MD
 Sample : 02558-01
 Misc : 4.78g/10mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-SS011-0006-01

Quant Time: May 02 00:01:05 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	226579	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	365870	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	327397	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	148544	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	131866	48.240	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	96.480%		
35) Dibromofluoromethane	5.385	113	103236	45.973	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	91.940%		
50) Toluene-d8	8.647	98	438671	51.784	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	103.560%		
62) 4-Bromofluorobenzene	11.085	95	159265	49.978	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	99.960%		
Target Compounds						
					Qvalue	
5) Bromomethane	1.611	94	319	0.219	ug/l #	62
6) Chloroethane	1.739	64	324	0.253	ug/l #	82
16) Acetone	2.404	43	1729	1.456	ug/l #	86
18) Methyl Acetate	2.715	43	4470	0.974	ug/l	96
20) Methylene Chloride	2.776	84	1719	0.631	ug/l #	71
25) 2-Butanone	4.599	43	2357	1.360	ug/l	92
29) Tetrahydrofuran	5.050	42	797	0.717	ug/l #	63
31) Cyclohexane	5.537	56	4565	1.177	ug/l #	1
36) 1,1-Dichloropropene	5.537	75	16460	4.694	ug/l #	43
38) Carbon Tetrachloride	5.544	117	22932	6.889	ug/l #	15
39) Methylcyclohexane	7.385	83	1188	0.278	ug/l #	78
55) 1,1,2-Trichloroethane	9.104	97	1301	0.512	ug/l #	25
59) 2-Hexanone	9.378	43	2993	1.205	ug/l #	26
67) Ethyl Benzene	10.195	91	6456	0.526	ug/l	95
68) m/p-Xylenes	10.299	106	12600	2.681	ug/l	98
69) o-Xylene	10.646	106	8129	1.764	ug/l	97
73) Isopropylbenzene	10.963	105	6892	0.635	ug/l	99
74) N-amyl acetate	10.854	43	12974	3.179	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.219	83	12183	3.615	ug/l #	25
76) 1,2,3-Trichloropropane	11.085	75	77927	26.299	ug/l #	35
78) n-propylbenzene	11.305	91	24907	1.997	ug/l	99
79) 2-Chlorotoluene	11.378	91	19441	2.495	ug/l #	48
80) 1,3,5-Trimethylbenzene	11.451	105	84164	9.193	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.085	75	77927	85.178	ug/l #	9
82) 4-Chlorotoluene	11.616	91	8104	0.926	ug/l	77
84) 1,2,4-Trimethylbenzene	11.756	105	235013	25.546	ug/l	100
85) sec-Butylbenzene	11.890	105	26193	2.324	ug/l	79
86) p-Isopropyltoluene	12.012	119	28716	2.996	ug/l	99
89) n-Butylbenzene	12.329	91	126429	15.627	ug/l #	23
90) Hexachloroethane	12.536	117	17080	11.642	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	12.926	75	2110	3.122	ug/l #	6
95) Naphthalene	13.780	128	279399	28.144	ug/l #	96
96) 1,2,3-Trichlorobenzene	13.975	180	3136	0.966	ug/l #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
Data File : VX035441.D
Acq On : 01 May 2023 15:31
Operator : JC/MD
Sample : 02558-01
Misc : 4.78g/10mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01

Quant Time: May 02 00:01:05 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration




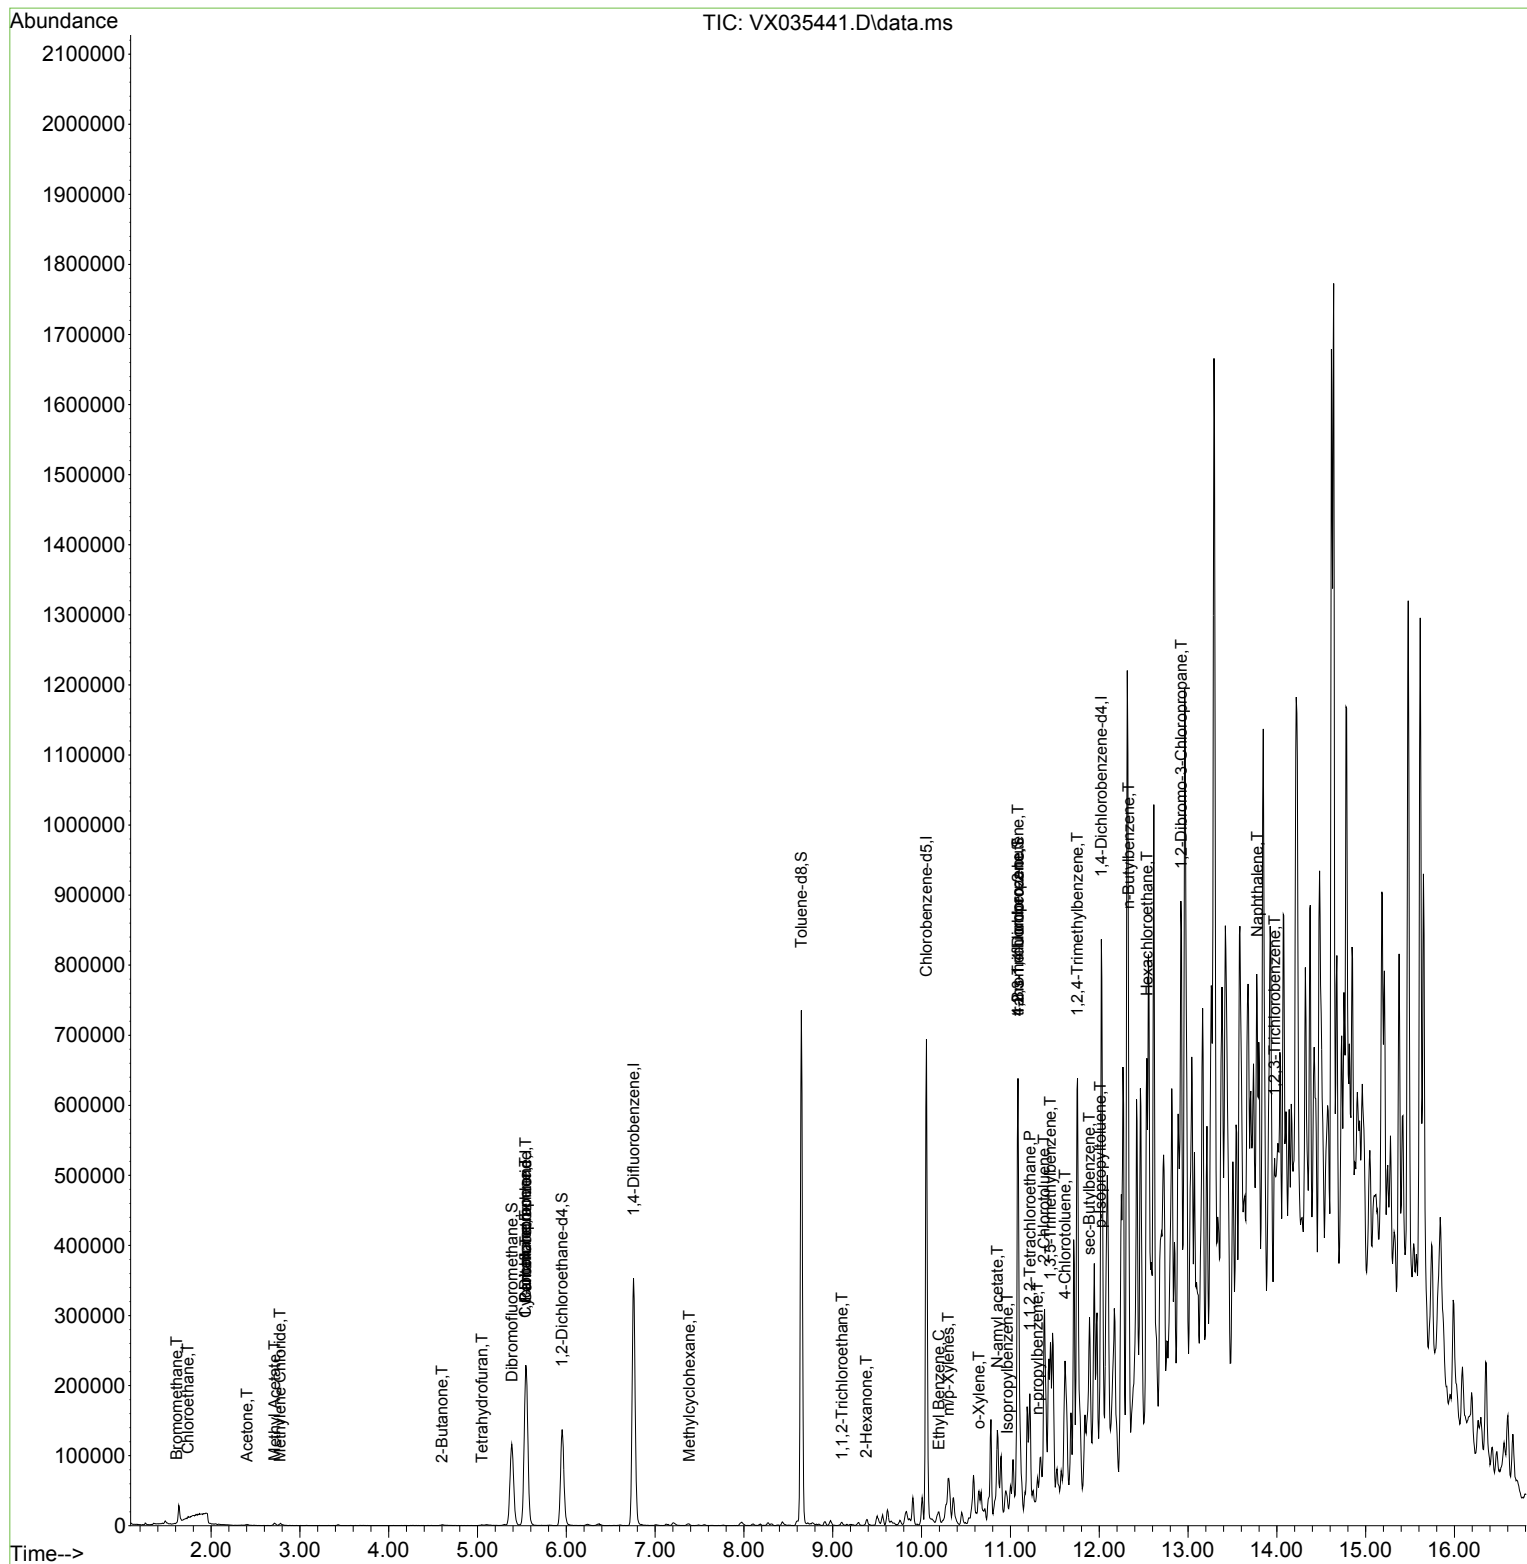




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.005 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion:168 Resp: 226579
Ion Ratio Lower Upper
168 100
99 56.6 45.7 68.5

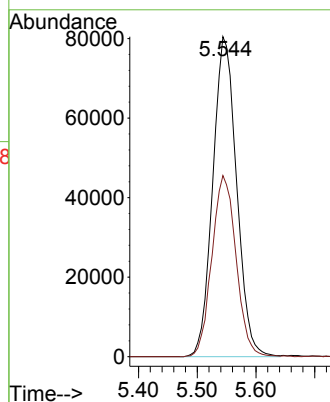

#5
Bromomethane
Concen: 0.219 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 94 Resp: 319
Ion Ratio Lower Upper
94 100
96 58.7 77.0 115.6#


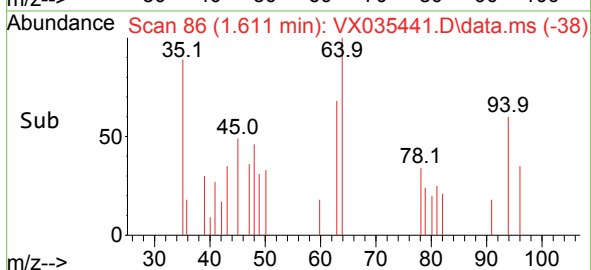
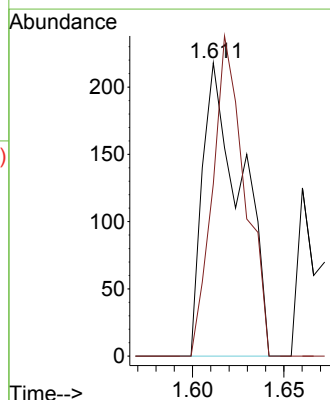
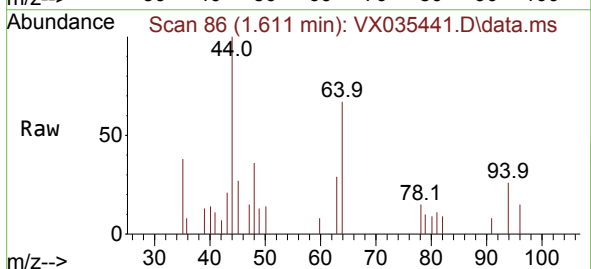


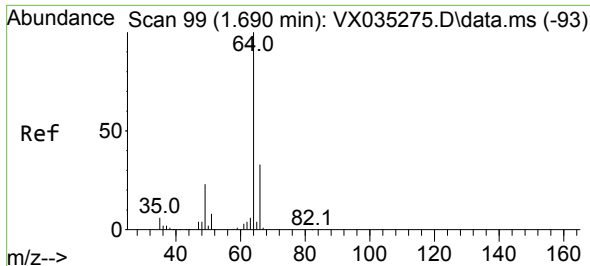

#6
Chloroethane
Concen: 0.253 ug/l
RT: 1.739 min Scan# 107
Delta R.T. 0.049 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 64 Resp: 324
Ion Ratio Lower Upper
64 100
66 22.4 26.2 39.4#

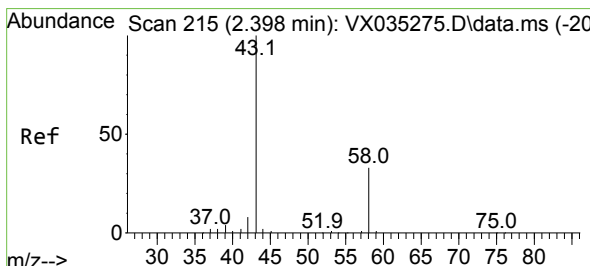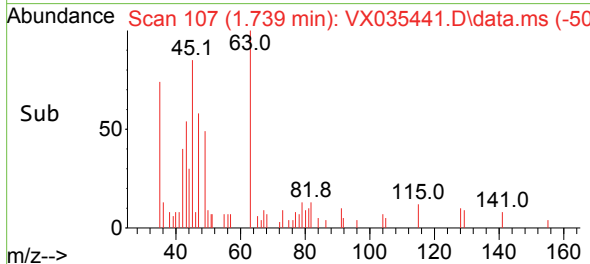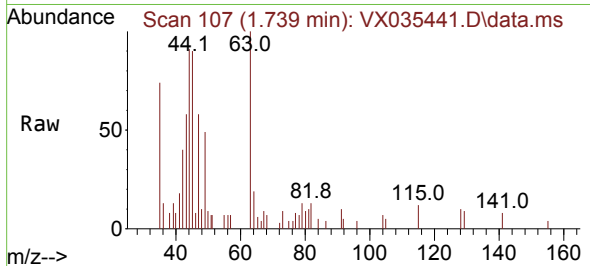

#16
Acetone
Concen: 1.456 ug/l
RT: 2.404 min Scan# 216
Delta R.T. 0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 43 Resp: 1729
Ion Ratio Lower Upper
43 100
58 23.0 24.7 37.1#


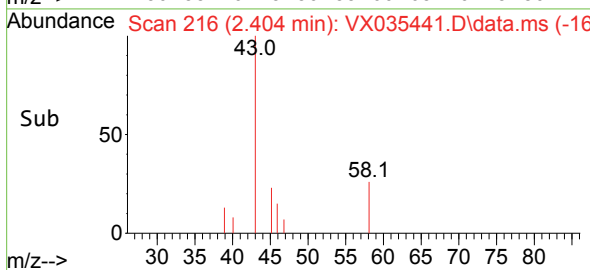

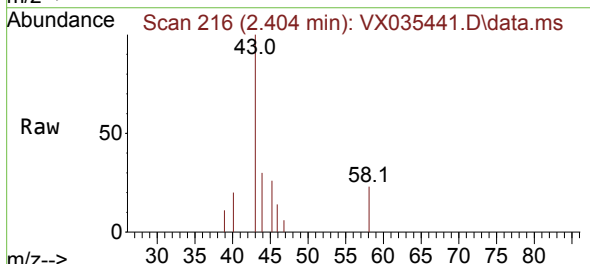




#18
Methyl Acetate
Concen: 0.974 ug/l
RT: 2.715 min Scan# 20
Delta R.T. 0.007 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 43 Resp: 4470
Ion Ratio Lower Upper
43 100
74 25.1 18.3 27.5

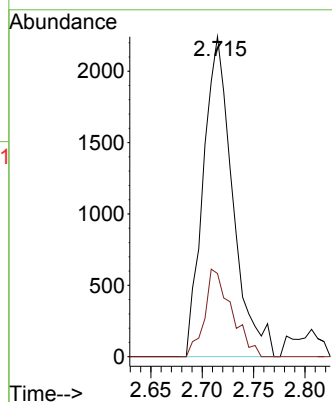

#20
Methylene Chloride
Concen: 0.631 ug/l
RT: 2.776 min Scan# 277
Delta R.T. -0.012 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 84 Resp: 1719
Ion Ratio Lower Upper
84 100
49 93.1 103.8 155.8#
51 17.8 31.8 47.8#
86 49.6 51.4 77.2#


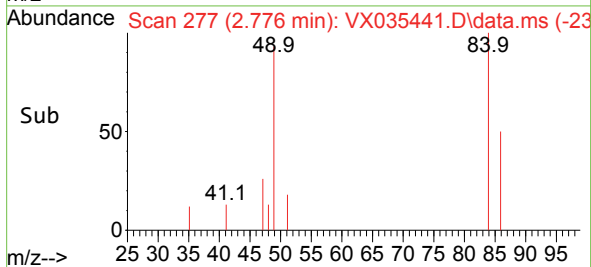

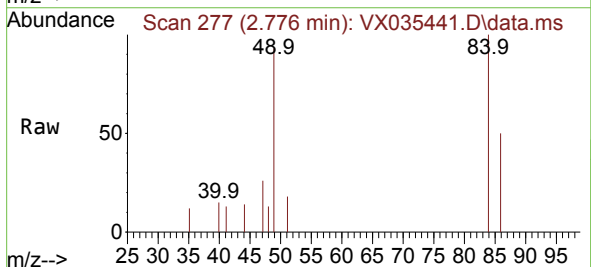




#25
2-Butanone
Concen: 1.360 ug/l
RT: 4.599 min Scan# 51
Delta R.T. 0.031 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 43 Resp: 2357
Ion Ratio Lower Upper
43 100
72 28.2 19.3 28.9

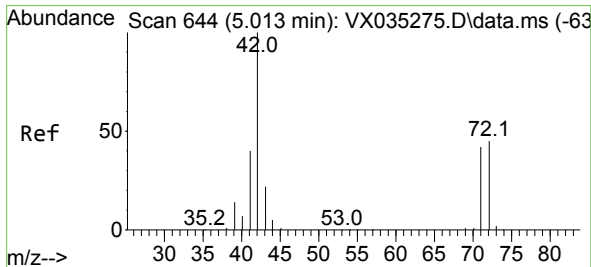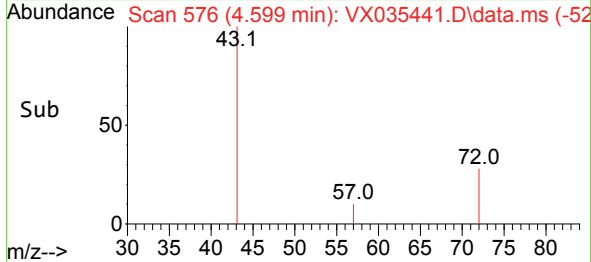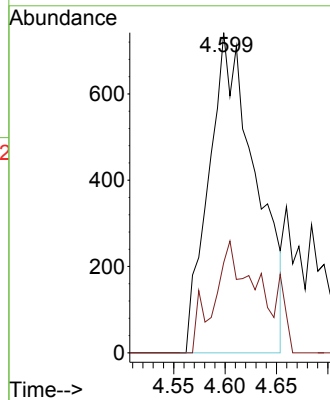

#29
Tetrahydrofuran
Concen: 0.717 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.037 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31


Tgt Ion: 42 Resp: 797
Ion Ratio Lower Upper
42 100
72 64.6 34.5 51.7#
71 14.6 32.1 48.1#

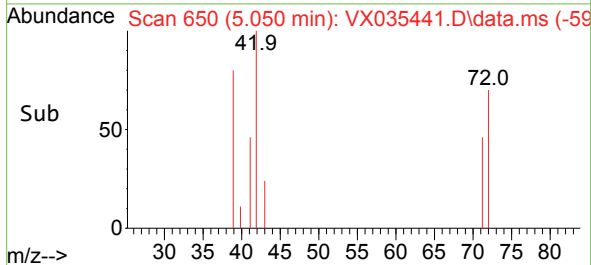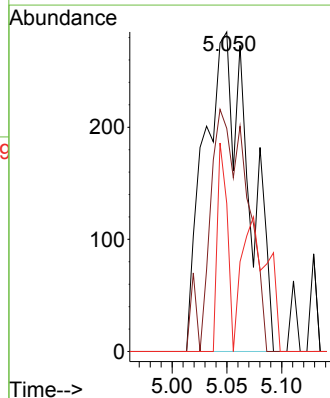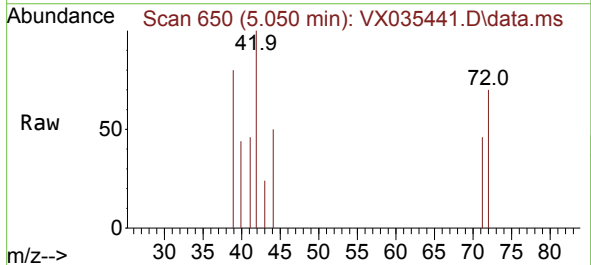






#31
Cyclohexane
Concen: 1.177 ug/l
RT: 5.537 min Scan# 719
Delta R.T. 0.067 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01







Tgt Ion: 56 Resp: 4565
Ion Ratio Lower Upper
56 100
69 182.2 23.7 35.5#
84 139.7 68.5 102.7#

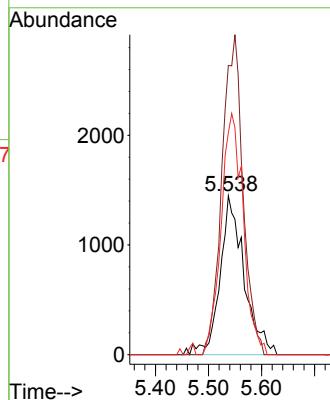

#33
1,2-Dichloroethane-d4
Concen: 48.240 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 65 Resp: 131866
Ion Ratio Lower Upper
65 100
67 52.6 0.0 104.0


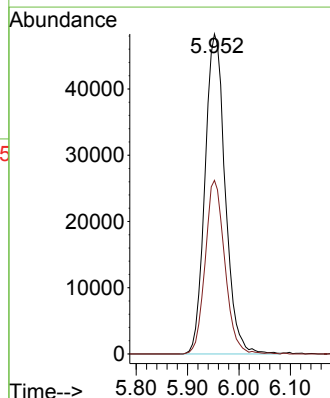






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion:114 Resp: 365870
Ion Ratio Lower Upper
114 100
63 19.6 0.0 42.2
88 16.7 0.0 33.2

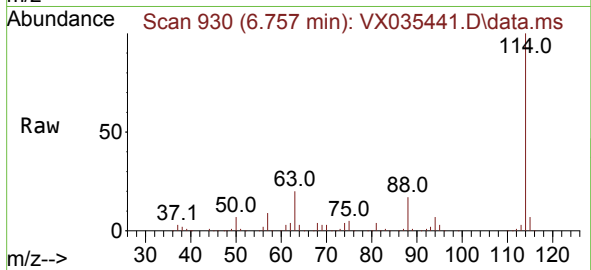

#35
Dibromofluoromethane
Concen: 45.973 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion:113 Resp: 103236
Ion Ratio Lower Upper
113 100
111 102.3 83.7 125.5
192 21.0 15.4 23.2


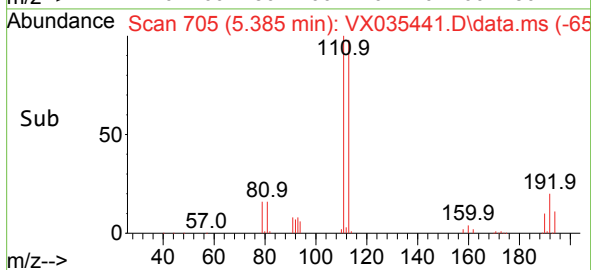

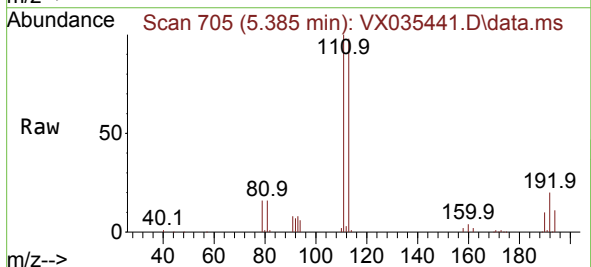




#36
1,1-Dichloropropene
Concen: 4.694 ug/l
RT: 5.537 min Scan# 710
Delta R.T. -0.153 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 75 Resp: 16460
Ion Ratio Lower Upper
75 100
110 1.7 17.5 52.5#
77 0.0 24.3 36.5#

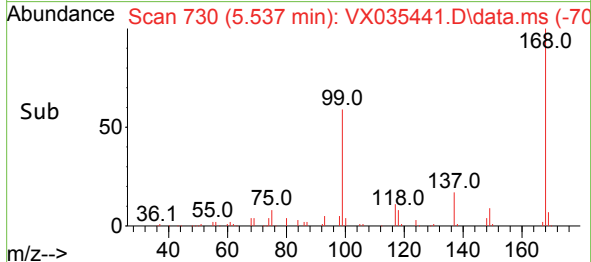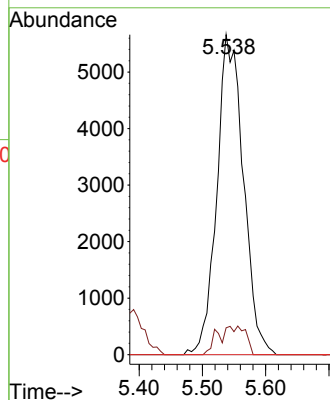

#38
Carbon Tetrachloride
Concen: 6.889 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.133 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 117 Resp: 22932
Ion Ratio Lower Upper
117 100
119 4.1 76.6 114.8#
121 0.0 23.8 35.6#

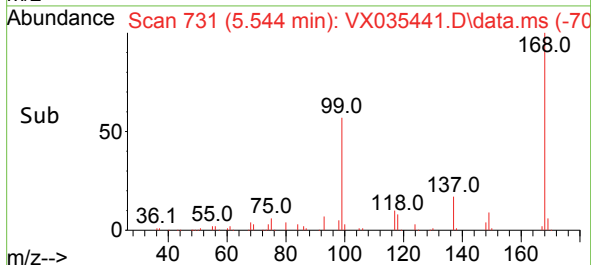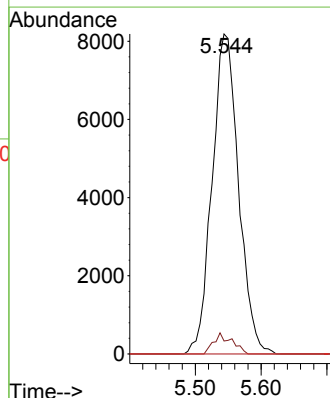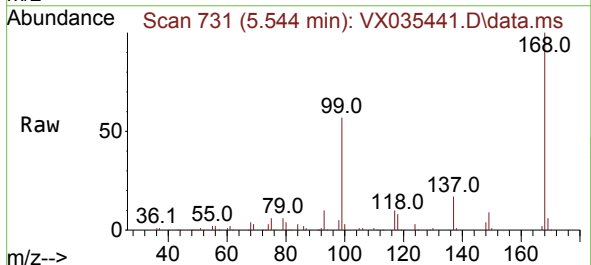



#39

Methylcyclohexane

Concen: 0.278 ug/l

RT: 7.385 min Scan# 1033

Delta R.T. 0.007 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :

P001-SS011-0006-01





Tgt Ion: 83 Resp: 1188

Ion Ratio Lower Upper

83 100

55 58.8 60.5 90.7#

98 32.6 40.4 60.6#

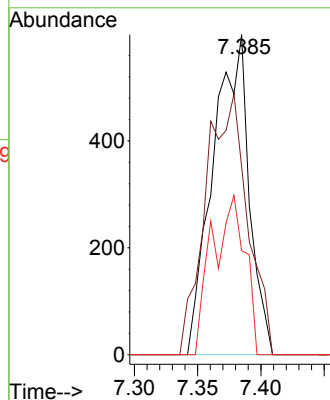

#50

Toluene-d8

Concen: 51.784 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.001 min

Lab File: VX035441.D




Acq: 01 May 2023 15:31


Tgt Ion: 98 Resp: 438671

Ion Ratio Lower Upper

98 100

100 66.3 52.5 78.7

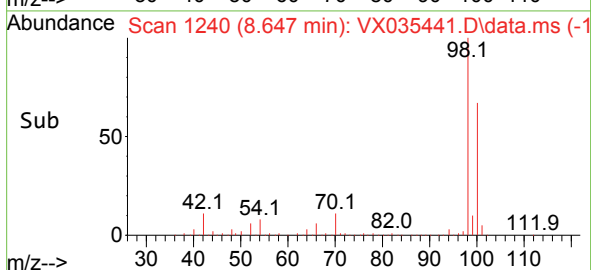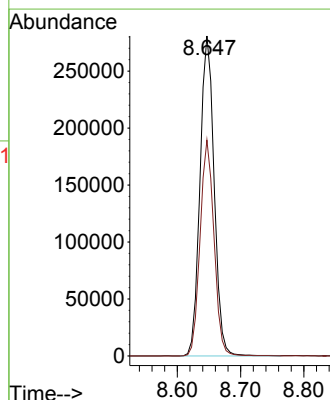



#55

1,1,2-Trichloroethane

Concen: 0.512 ug/l

RT: 9.104 min Scan# 1

Delta R.T. -0.048 min

Lab File: VX035441.D


Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :

P001-SS011-0006-01

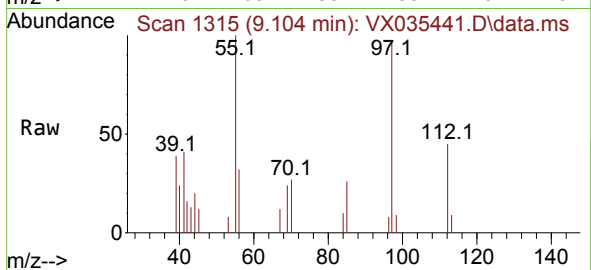

Tgt Ion: 97 Resp: 1301




Ion Ratio Lower Upper

97 100

83 0.0 69.7 104.5#

85 27.3 43.7 65.5#

99 0.0 49.7 74.5#



#59

2-Hexanone

Concen: 1.205 ug/l

RT: 9.378 min Scan# 1360

Delta R.T. -0.055 min

Lab File: VX035441.D




Acq: 01 May 2023 15:31


Tgt Ion: 43 Resp: 2993

Ion Ratio Lower Upper

43 100

58 0.0 26.3 78.9#


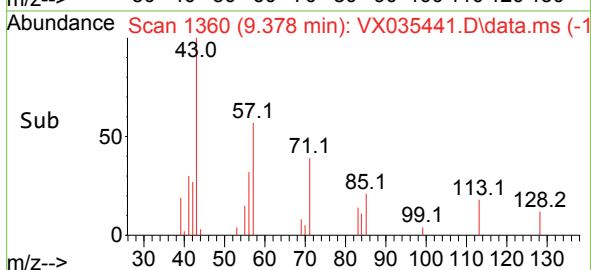






#62
4-Bromofluorobenzene
Concen: 49.978 ug/l
RT: 11.085 min Scan# 1
Delta R.T. 0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 95 Resp: 159265
Ion Ratio Lower Upper
95 100
174 79.4 0.0 147.4
176 75.9 0.0 140.6

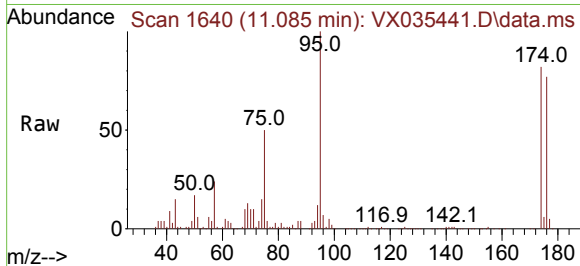

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 117 Resp: 327397
Ion Ratio Lower Upper
117 100
82 55.3 45.0 67.4
119 32.6 26.0 39.0



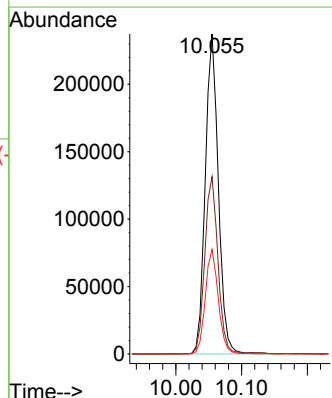
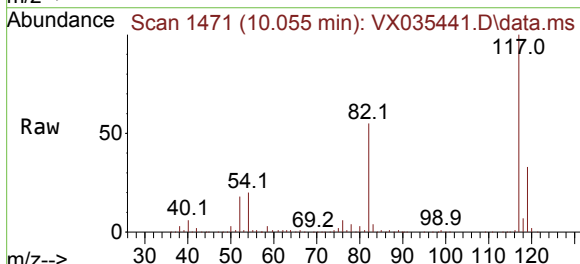




#67
Ethyl Benzene
Concen: 0.526 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 91 Resp: 6456
Ion Ratio Lower Upper
91 100
106 29.0 25.6 38.4



#68
m/p-Xylenes
Concen: 2.681 ug/l
RT: 10.299 min Scan# 1511
Delta R.T. -0.000 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 106 Resp: 12600
Ion Ratio Lower Upper
106 100
91 202.6 164.0 246.0


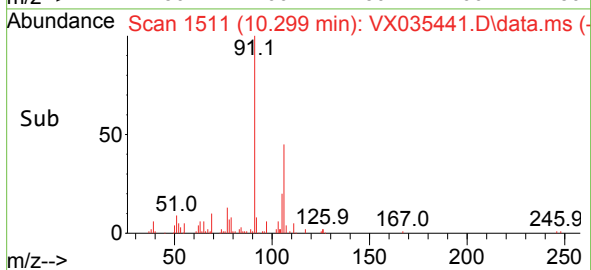






#69
o-Xylene
Concen: 1.764 ug/l
RT: 10.646 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion:106 Resp: 8129
Ion Ratio Lower Upper
106 100
91 222.3 108.5 325.3

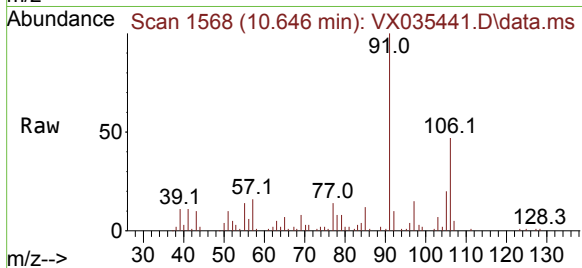

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion:152 Resp: 148544
Ion Ratio Lower Upper
152 100
115 62.4 45.0 135.0
150 159.9 0.0 352.4

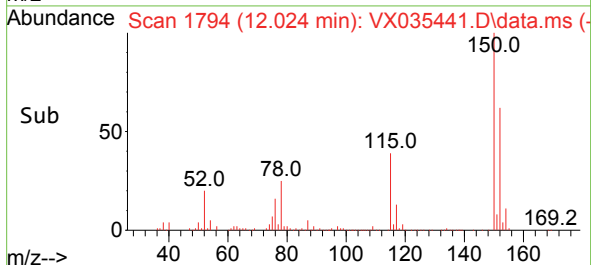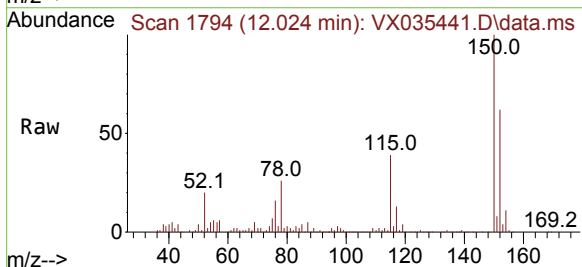



#73

Isopropylbenzene

Concen: 0.635 ug/l

RT: 10.963 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :





P001-SS011-0006-01

Tgt Ion:105 Resp: 6892

Ion Ratio Lower Upper

105 100

120 26.9 13.3 39.9



#74

N-ethyl acetate

Concen: 3.179 ug/l

RT: 10.854 min Scan# 1602

Delta R.T. 0.013 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Tgt Ion: 43 Resp: 12974




Ion Ratio Lower Upper


43 100

70 81.0 32.1 48.1#

55 267.4 18.3 27.5#

61 0.0 18.8 28.2#

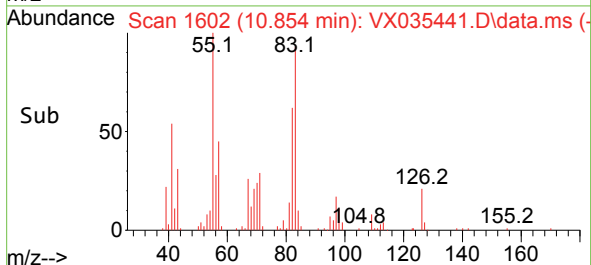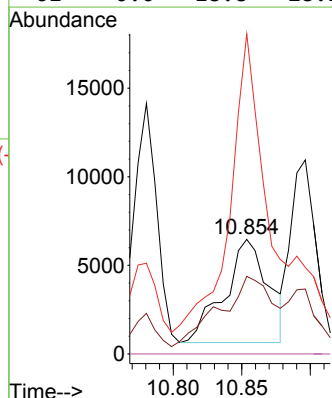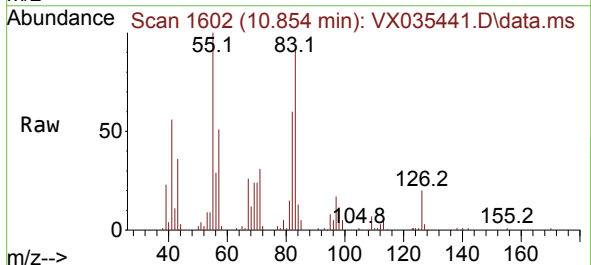



#75

1,1,2,2-Tetrachloroethane

Concen: 3.615 ug/l

RT: 11.219 min Scan# 1

Delta R.T. 0.006 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :

P001-SS011-0006-01





Tgt Ion: 83 Resp: 12183

Ion Ratio Lower Upper

83 100

131 0.0 4.8 14.3#

85 0.0 32.0 96.0#

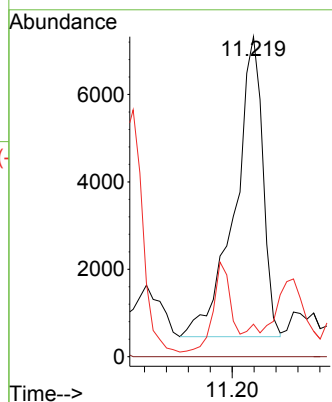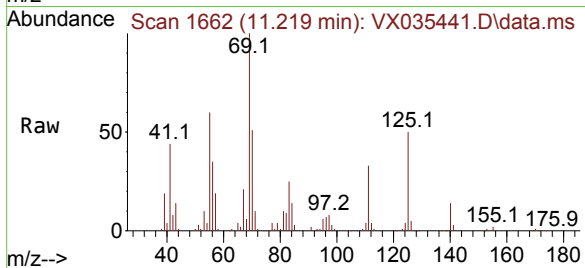

#76

1,2,3-Trichloropropane

Concen: 26.299 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. -0.152 min

Lab File: VX035441.D




Acq: 01 May 2023 15:31


Tgt Ion: 75 Resp: 77927

Ion Ratio Lower Upper

75 100

77 1.5 21.6 64.8#


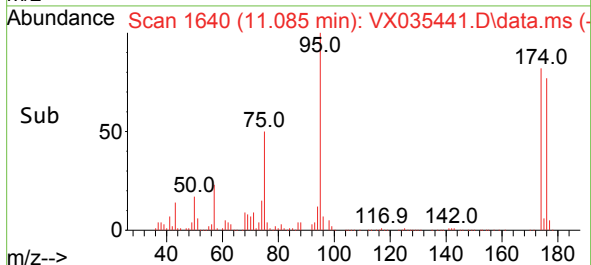

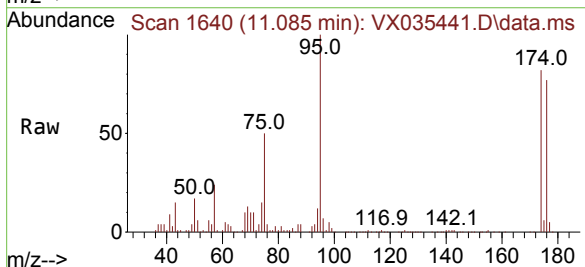


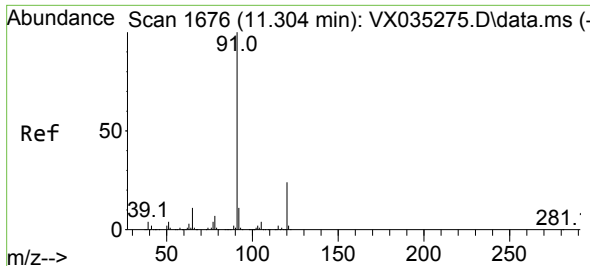

#78
n-propylbenzene
Concen: 1.997 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. 0.001 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 91 Resp: 24907
Ion Ratio Lower Upper
91 100
120 22.7 11.5 34.5

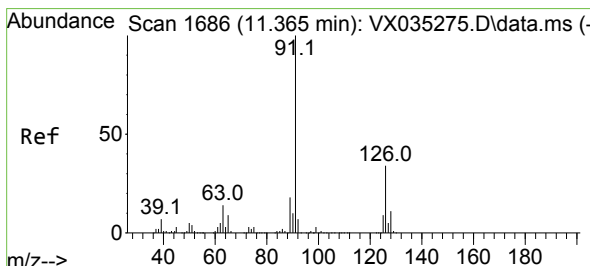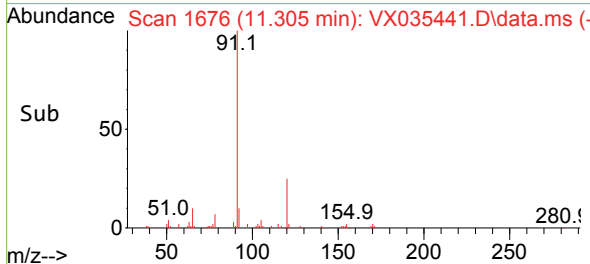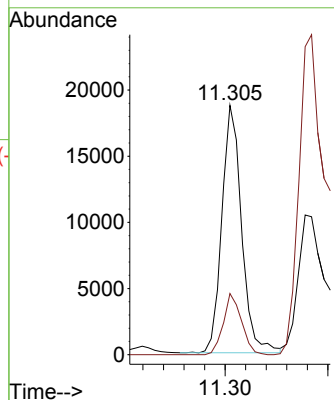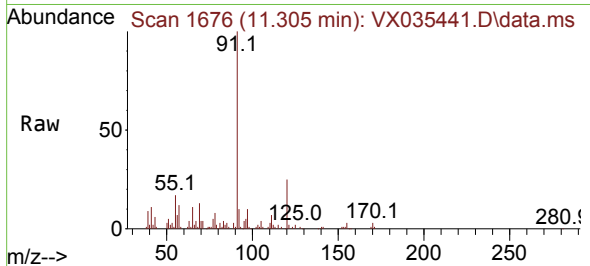

#79
2-Chlorotoluene
Concen: 2.495 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.013 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 91 Resp: 19441
Ion Ratio Lower Upper
91 100
126 3.2 16.3 48.9#

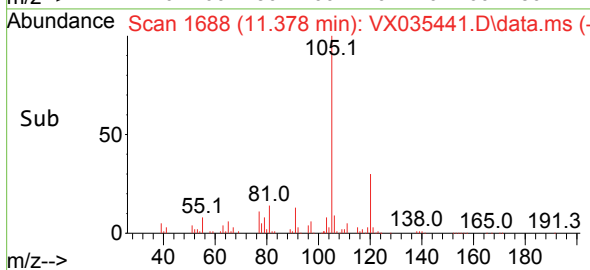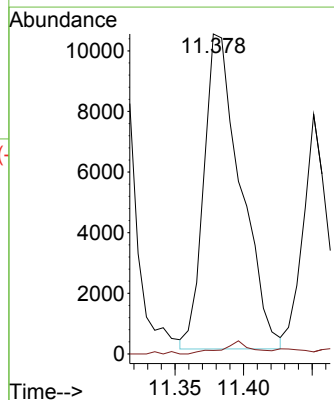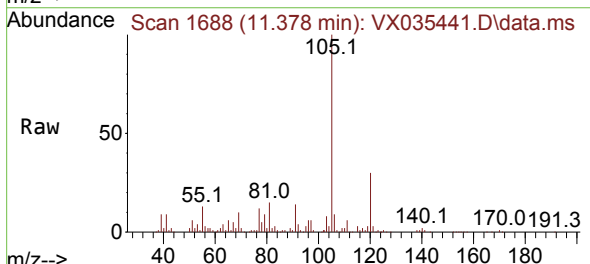



#80

1,3,5-Trimethylbenzene

Concen: 9.193 ug/l

RT: 11.451 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :





P001-SS011-0006-01

Tgt Ion:105 Resp: 84164

Ion Ratio Lower Upper

105 100

120 49.5 23.7 71.1

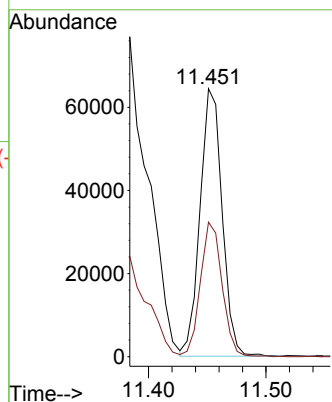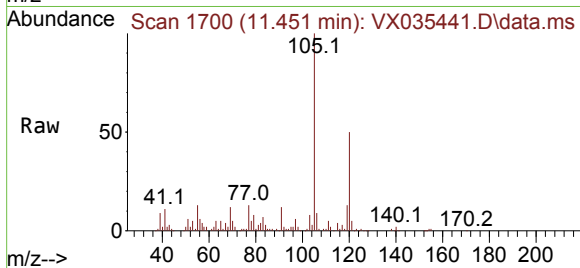

#81

trans-1,4-Dichloro-2-butene

Concen: 85.178 ug/l

RT: 11.085 min Scan# 1640

Delta R.T. 0.067 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31




Tgt Ion: 75 Resp: 77927


Ion Ratio Lower Upper

75 100

53 0.7 82.6 124.0#

89 0.0 36.9 55.3#


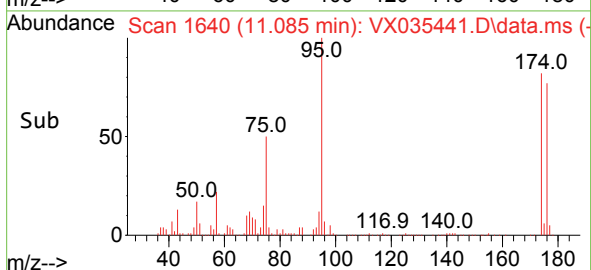

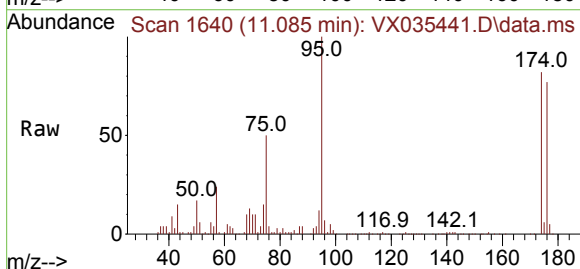




#82
4-Chlorotoluene
Concen: 0.926 ug/l
RT: 11.616 min Scan# 11
Delta R.T. 0.165 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 91 Resp: 8104
Ion Ratio Lower Upper
91 100
126 16.2 14.2 42.6

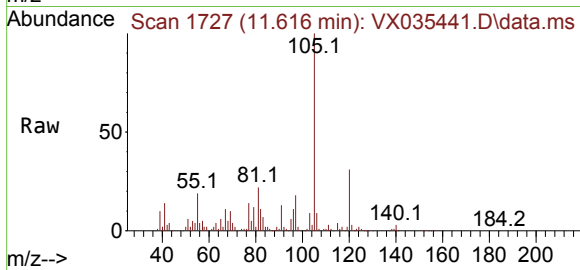

#84
1,2,4-Trimethylbenzene
Concen: 25.546 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.007 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31

Tgt Ion: 105 Resp: 235013
Ion Ratio Lower Upper
105 100
120 44.8 22.4 67.0

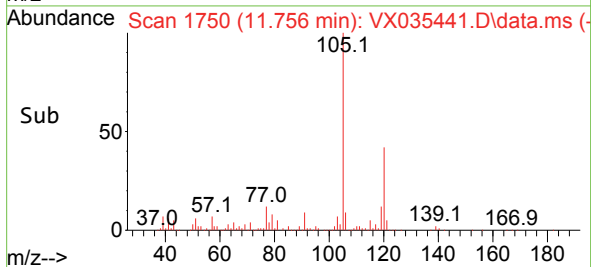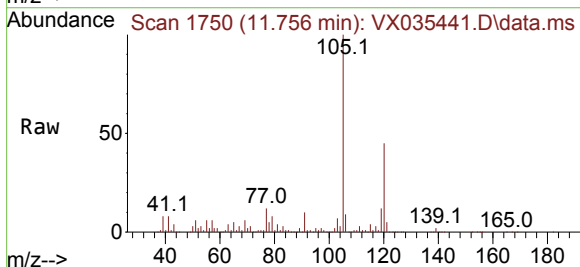



#85

sec-Butylbenzene

Concen: 2.324 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :





P001-SS011-0006-01

Tgt Ion:105 Resp: 26193

Ion Ratio Lower Upper

105 100

134 30.1 10.2 30.4

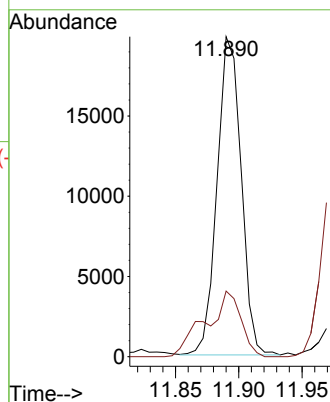

#86

p-Isopropyltoluene

Concen: 2.996 ug/l

RT: 12.012 min Scan# 1792

Delta R.T. 0.006 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31




Tgt Ion:119 Resp: 28716


Ion Ratio Lower Upper

119 100

134 27.0 13.2 39.5

91 26.5 12.9 38.7

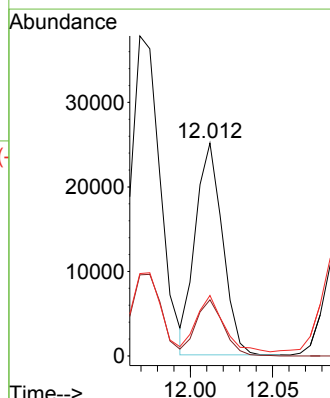



#89

n-Butylbenzene

Concen: 15.627 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. -0.006 min

Lab File: VX035441.D

Acq: 01 May 2023 15:31

Instrument :

MSVOA_X

ClientSampleId :

P001-SS011-0006-01





Tgt Ion: 91 Resp: 126429

Ion Ratio Lower Upper

91 100

92 31.6 27.7 83.0

134 113.4 13.0 38.9#

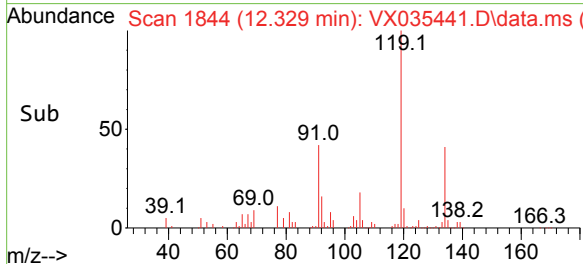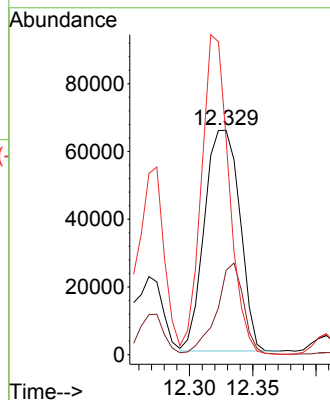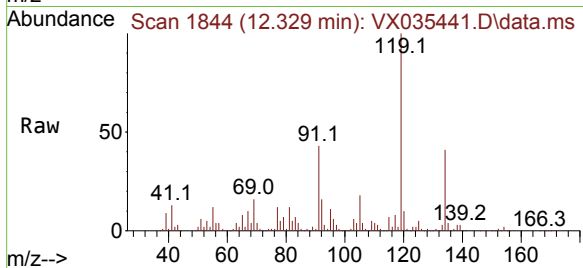

#90

Hexachloroethane

Concen: 11.642 ug/l

RT: 12.536 min Scan# 1878

Delta R.T. 0.000 min

Lab File: VX035441.D




Acq: 01 May 2023 15:31


Tgt Ion: 117 Resp: 17080

Ion Ratio Lower Upper

117 100

201 0.0 34.4 103.1#


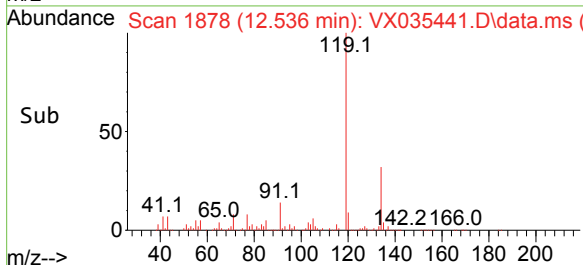
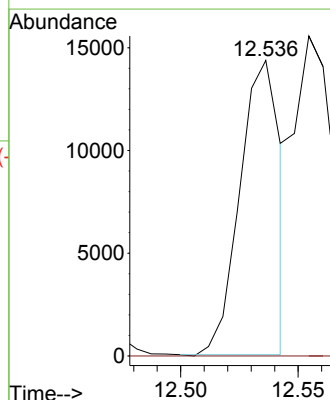
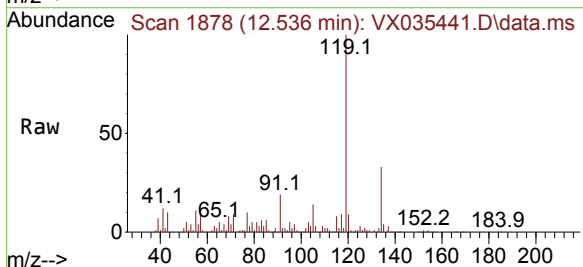


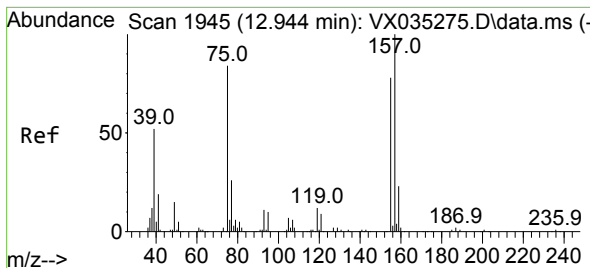

#92
1,2-Dibromo-3-Chloropropane
Concen: 3.122 ug/l
RT: 12.926 min Scan# 1942
Delta R.T. -0.018 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31




Instrument :
MSVOA_X
ClientSampleId :
P001-SS011-0006-01


Tgt Ion: 75 Resp: 2110
Ion Ratio Lower Upper
75 100
155 0.0 38.4 115.1#
157 2.9 49.9 149.7#

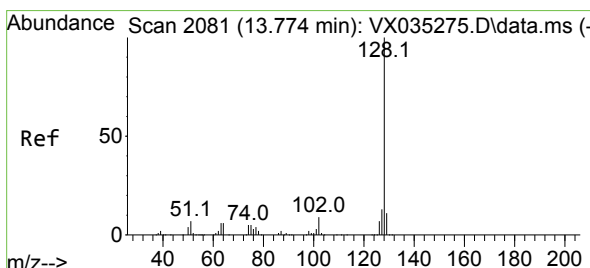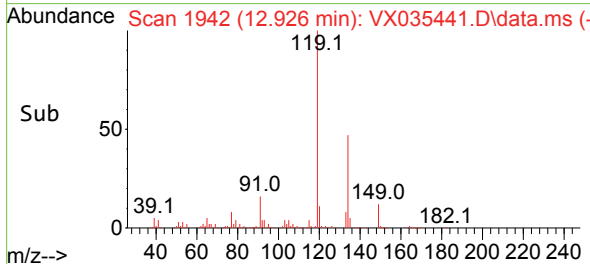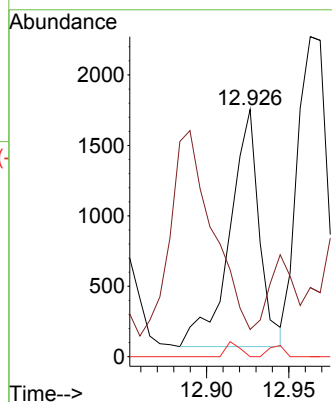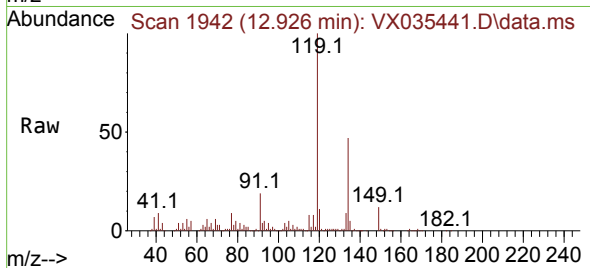

#95
Naphthalene
Concen: 28.144 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. 0.006 min
Lab File: VX035441.D
Acq: 01 May 2023 15:31


Tgt Ion:128 Resp: 279399
Ion Ratio Lower Upper
128 100
127 13.5 10.2 15.4
129 13.1 8.6 13.0#

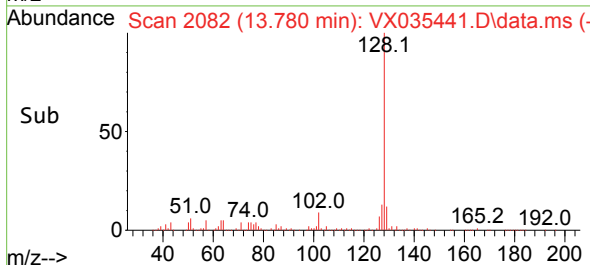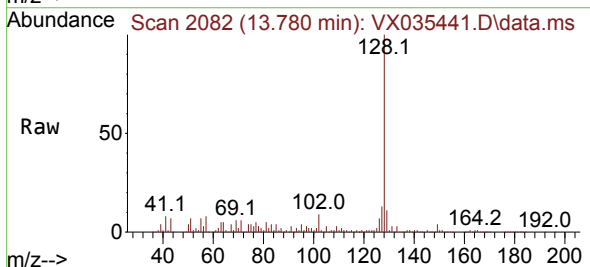



#96
 1,2,3-Trichlorobenzene
 Concen: 0.966 ug/l
 RT: 13.975 min Scan# 2114
 Delta R.T. 0.012 min
 Lab File: VX035441.D
 Acq: 01 May 2023 15:31

Instrument :
 MSVOA_X
 ClientSampleId :
 P001-SS011-0006-01

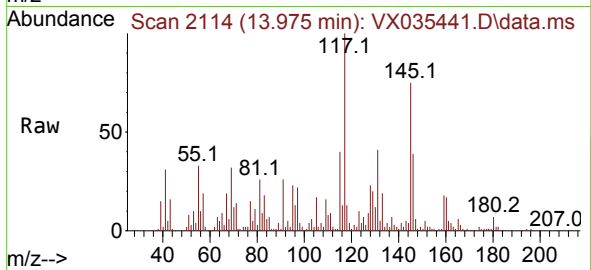

Tgt Ion:180 Resp: 3136
 Ion Ratio Lower Upper
 180 100
 182 0.0 48.0 144.2#
 145 1460.0 17.7 53.1#

