

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
 Data File : VX035446.D
 Acq On : 01 May 2023 17:28
 Operator : JC/MD
 Sample : 02522-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-16D

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Title : SW846 8260

Signal : TIC: VX035446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.300	31	35	42	rBV	5811	14851	1.21%	0.207%
2	2.392	208	214	226	rVB	6276	12939	1.06%	0.180%
3	5.099	647	658	672	rBV3	7136	21256	1.74%	0.297%
4	5.385	692	705	721	rBV	133325	394989	32.28%	5.510%
5	5.550	721	732	751	rVB2	244081	690338	56.42%	9.630%
6	5.958	790	799	818	rBV	146200	388039	31.71%	5.413%
7	6.763	921	931	948	rBV	373653	893980	73.06%	12.471%
8	8.647	1233	1240	1256	rBV	785331	1223676	100.00%	17.070%
9	9.275	1337	1343	1350	rVB	16803	25964	2.12%	0.362%
10	10.055	1465	1471	1486	rBV	787260	1073536	87.73%	14.975%
11	11.079	1634	1639	1654	rBV	658471	849929	69.46%	11.856%
12	11.750	1745	1749	1757	rVB	26144	33264	2.72%	0.464%
13	12.024	1788	1794	1801	rBV	820219	1037835	84.81%	14.477%
14	12.085	1801	1804	1809	rVB2	9214	12520	1.02%	0.175%
15	12.244	1825	1830	1838	rBV2	17839	24089	1.97%	0.336%
16	12.701	1899	1905	1912	rBV	9864	15357	1.25%	0.214%
17	13.170	1975	1982	1986	rBV	10235	13531	1.11%	0.189%
18	13.286	1992	2001	2007	rBV2	14032	22925	1.87%	0.320%
19	13.426	2020	2024	2028	rBV2	11416	14829	1.21%	0.207%
20	13.774	2077	2081	2090	rBV	92970	128158	10.47%	1.788%
21	14.640	2215	2223	2232	rBV	58820	91138	7.45%	1.271%
22	14.780	2241	2246	2251	rVB	54225	69497	5.68%	0.969%
23	15.213	2308	2317	2320	rBV6	7796	16888	1.38%	0.236%
24	15.377	2340	2344	2353	rVB5	12524	29609	2.42%	0.413%
25	15.481	2357	2361	2366	rBV3	12139	19637	1.60%	0.274%
26	15.609	2379	2382	2386	rVB2	12404	16433	1.34%	0.229%
27	16.328	2492	2500	2510	rBV3	13240	33421	2.73%	0.466%




Sum of corrected areas: 7168628

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
Data File : VX035446.D
Acq On : 01 May 2023 17:28
Operator : JC/MD
Sample : 02522-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

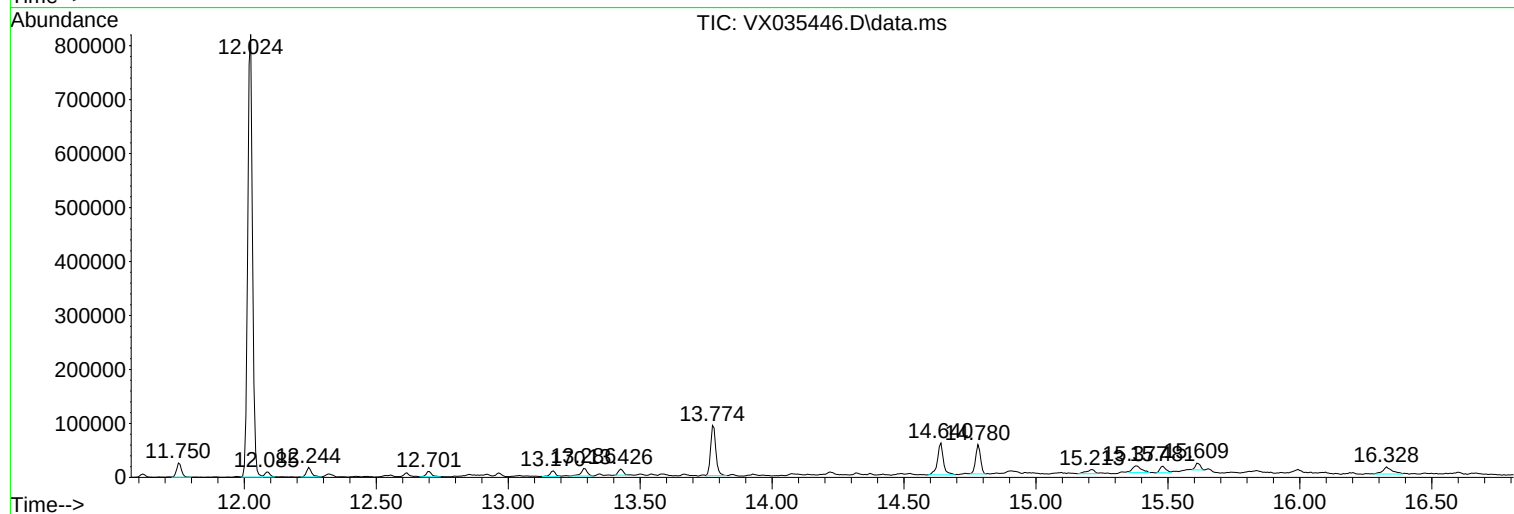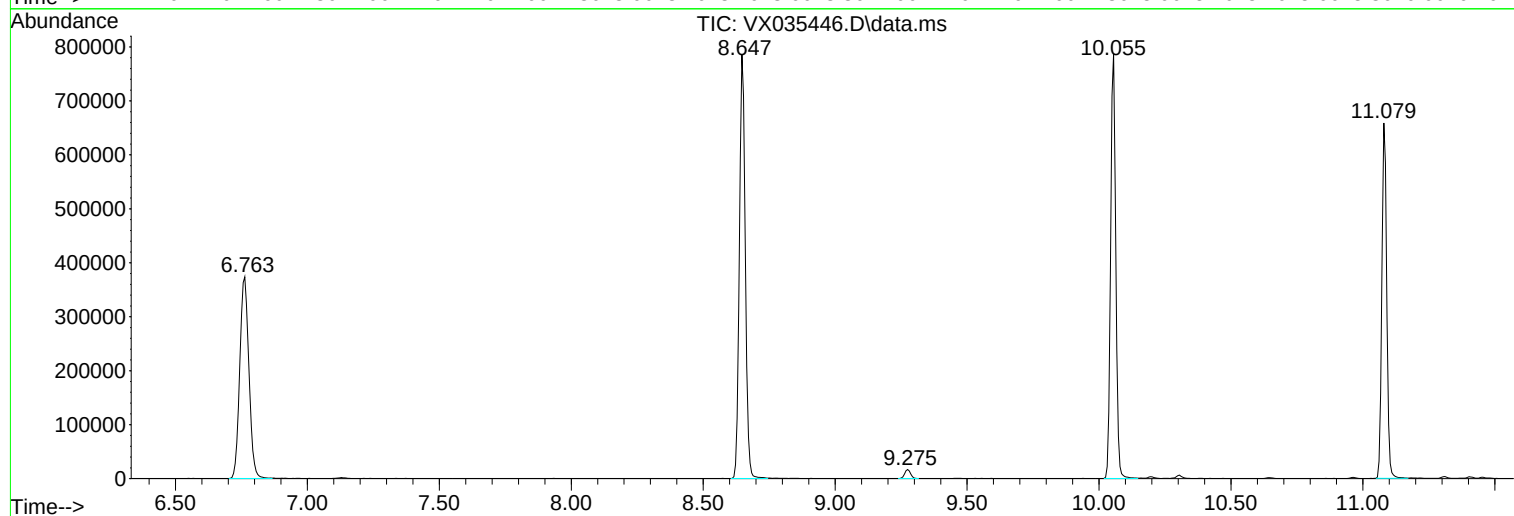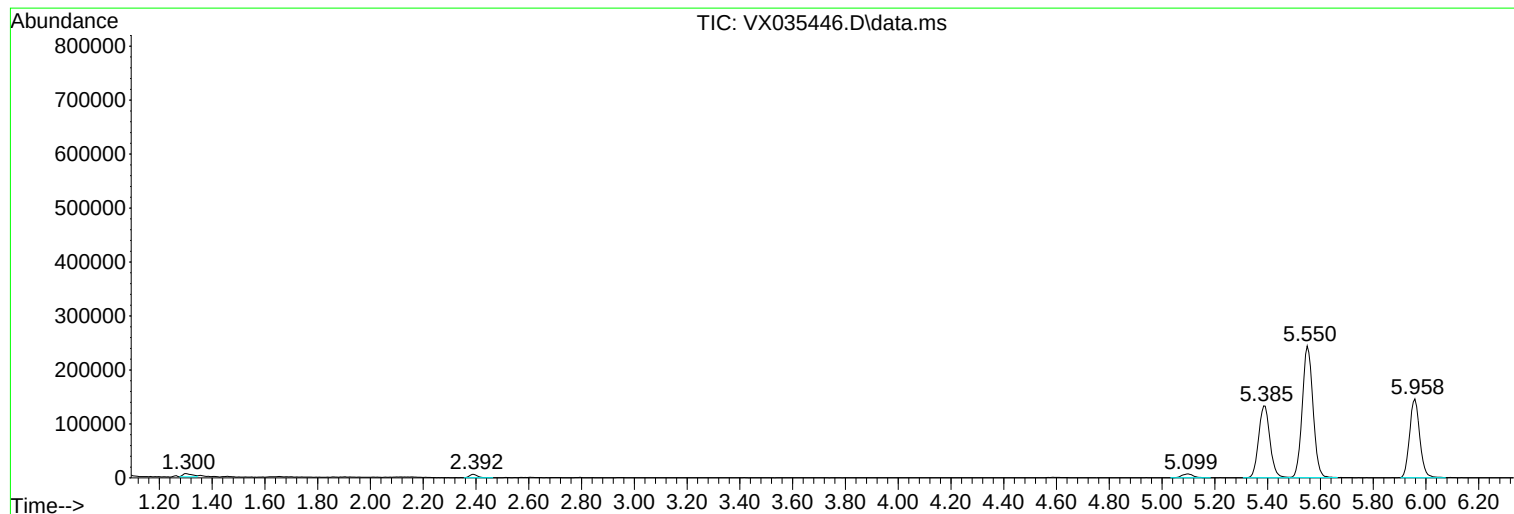

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
Data File : VX035446.D
Acq On : 01 May 2023 17:28
Operator : JC/MD
Sample : 02522-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050123\
Data File : VX035446.D
Acq On : 01 May 2023 17:28
Operator : JC/MD
Sample : 02522-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-16D

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------