

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
 Data File : VX041331.D
 Acq On : 01 May 2024 17:03
 Operator : JC/MD
 Sample : P2264-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 02 03:13:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 02:38:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	173565	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.763	114	253228	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	231515	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	138067	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	97681	51.697	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 103.400%	
35) Dibromofluoromethane	5.385	113	78524	45.759	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 91.520%	
50) Toluene-d8	8.647	98	285994	52.655	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 105.320%	
62) 4-Bromofluorobenzene	11.079	95	120684	57.399	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 114.800%	
Target Compounds						
					Qvalue	
5) Bromomethane	1.593	94	183	0.207	ug/l	# 48
6) Chloroethane	1.691	64	1337	2.047	ug/l	# 59
11) Tert butyl alcohol	3.001	59	2192	5.796	ug/l	99
13) Acrolein	2.203	56	179	0.597	ug/l	# 1
16) Acetone	2.392	43	8726	6.680	ug/l	93
19) Methyl tert-butyl Ether	3.117	73	12826	2.616	ug/l	94
20) Methylene Chloride	2.788	84	881	0.537	ug/l	# 79
31) Cyclohexane	5.464	56	5563	2.439	ug/l	94
36) 1,1-Dichloropropene	5.550	75	10708	5.218	ug/l	# 52
38) Carbon Tetrachloride	5.550	117	15596	6.635	ug/l	# 15
39) Methylcyclohexane	7.373	83	3914	1.624	ug/l	98
41) Methacrylonitrile	5.196	41	696	0.528	ug/l	# 1
48) Methyl methacrylate	7.653	41	460	0.261	ug/l	# 64
51) 4-Methyl-2-Pentanone	8.647	43	1359	0.588	ug/l	# 1
55) 1,1,2-Trichloroethane	9.098	97	911	0.611	ug/l	# 22
59) 2-Hexanone	9.250	43	1921	1.040	ug/l	72
68) m/p-Xylenes	10.305	106	2697	0.869	ug/l	96
73) Isopropylbenzene	10.963	105	12151	1.442	ug/l	98
76) 1,2,3-Trichloropropane	11.079	75	60281	26.791	ug/l	# 39
78) n-propylbenzene	11.305	91	4012	0.453	ug/l	98
79) 2-Chlorotoluene	11.305	91	4012	0.703	ug/l	# 42
81) trans-1,4-Dichloro-2-b...	11.079	75	60281	72.975	ug/l	# 5
82) 4-Chlorotoluene	11.305	91	4012	0.620	ug/l	# 46
83) tert-Butylbenzene	11.713	119	18549	2.521	ug/l	97
84) 1,2,4-Trimethylbenzene	11.616	105	6666	0.964	ug/l	83
85) sec-Butylbenzene	11.890	105	41239	4.891	ug/l	100
86) p-Isopropyltoluene	12.177	119	35515	4.690	ug/l	94
89) n-Butylbenzene	12.329	91	5858	0.962	ug/l	88
90) Hexachloroethane	12.646	117	79288	62.612	ug/l	# 17
92) 1,2-Dibromo-3-Chloropr...	12.920	75	1470	2.304	ug/l	# 9


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
Data File : VX041331.D
Acq On : 01 May 2024 17:03
Operator : JC/MD
Sample : P2264-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 02 03:13:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 01 02:38:17 2024
Response via : Initial Calibration

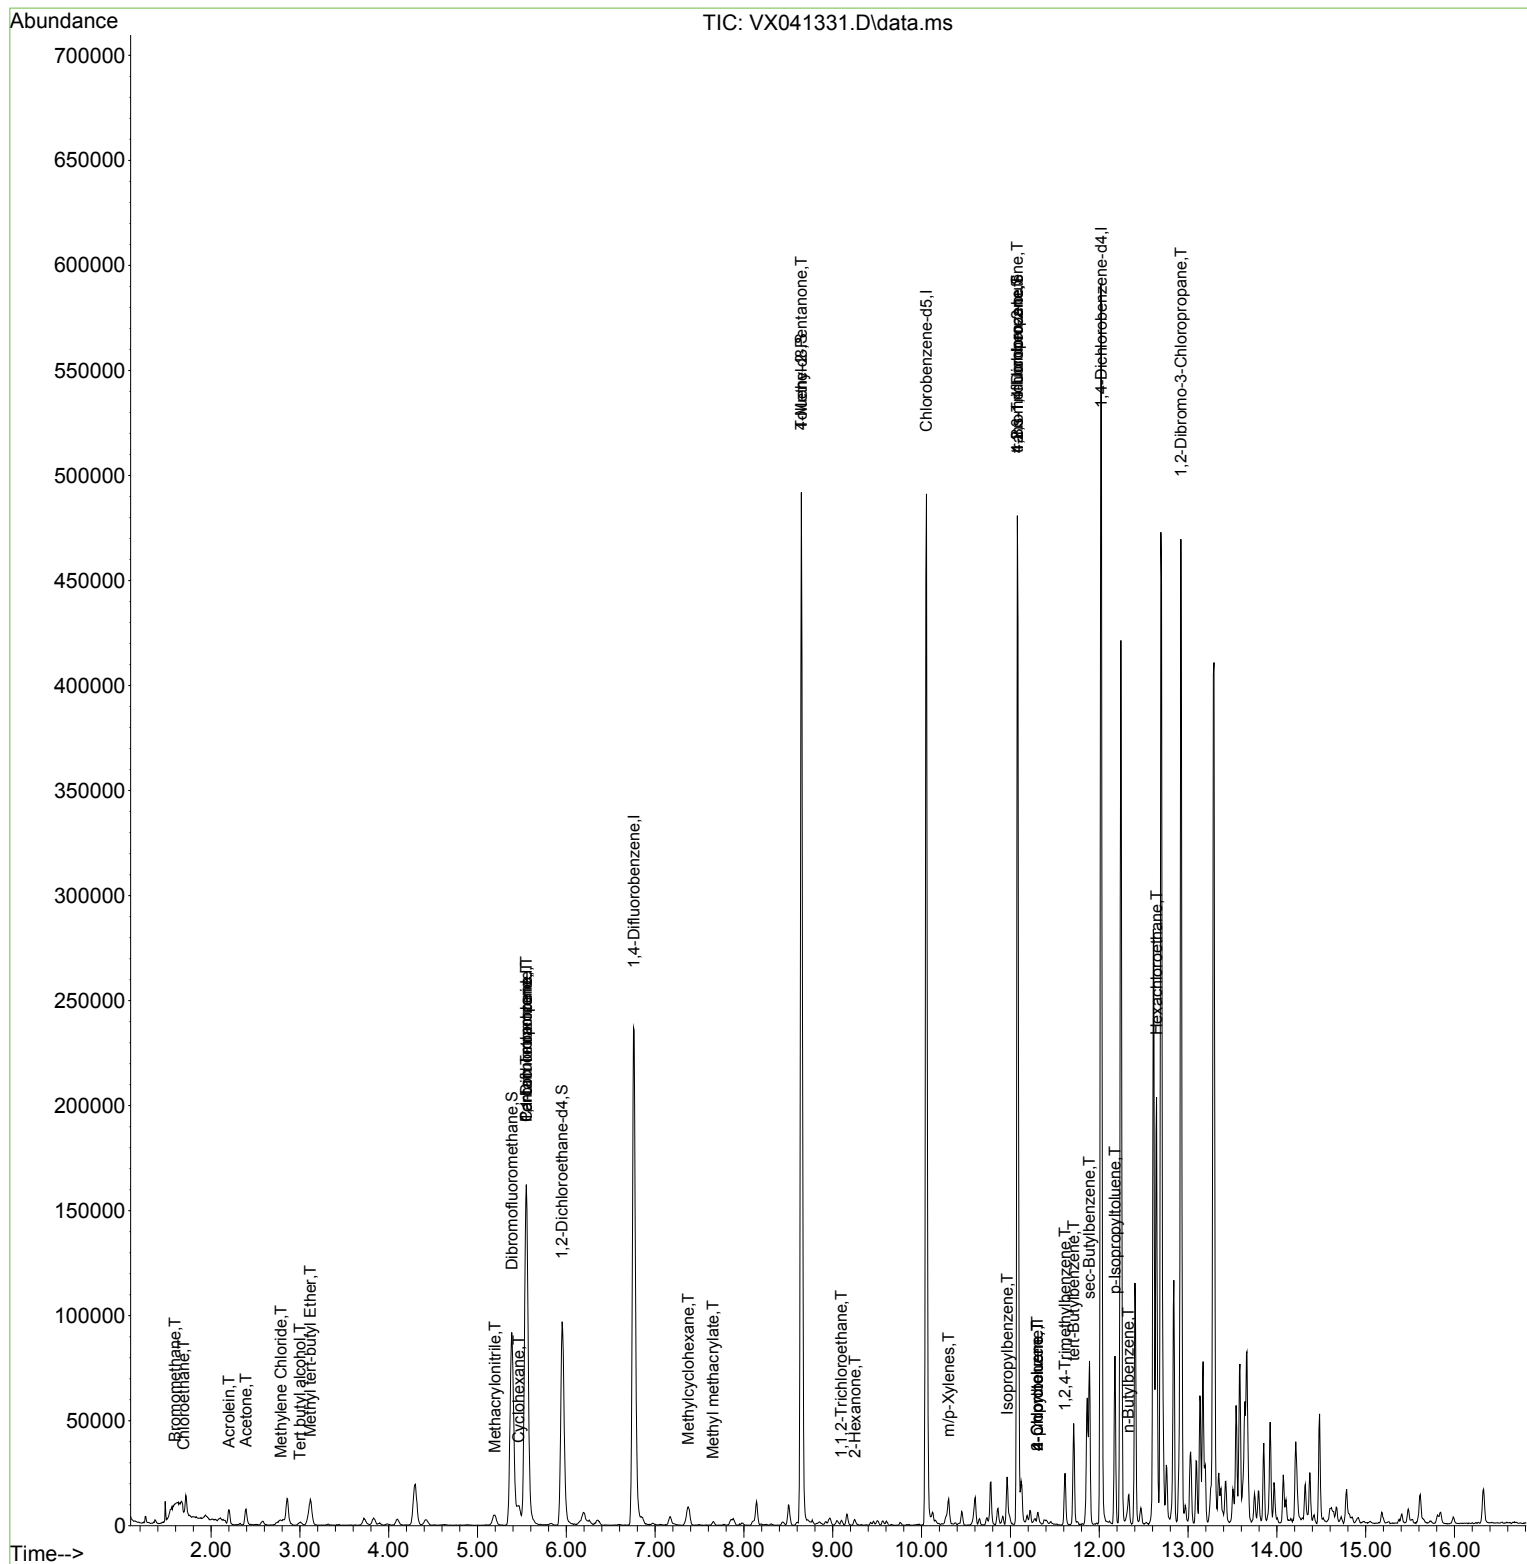



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.550 min Scan# 71

Delta R.T. -0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:168 Resp: 173565

Ion Ratio Lower Upper

168 100

99 47.6 56.6 85.0#

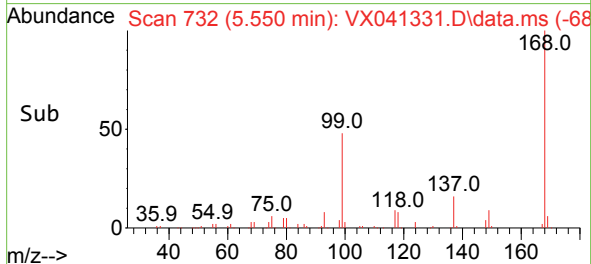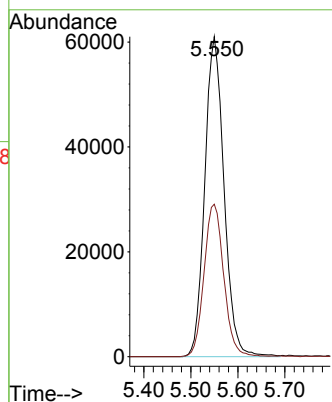

#5

Bromomethane

Concen: 0.207 ug/l

RT: 1.593 min Scan# 83

Delta R.T. -0.006 min

Lab File: VX041331.D




Acq: 01 May 2024 17:03


Tgt Ion: 94 Resp: 183

Ion Ratio Lower Upper

94 100

96 43.1 74.6 111.8#







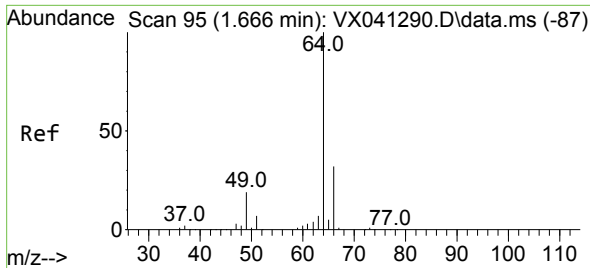

#6
Chloroethane
Concen: 2.047 ug/l
RT: 1.691 min Scan# 91
Delta R.T. 0.024 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 64 Resp: 1337
Ion Ratio Lower Upper
64 100
66 8.5 25.1 37.7#

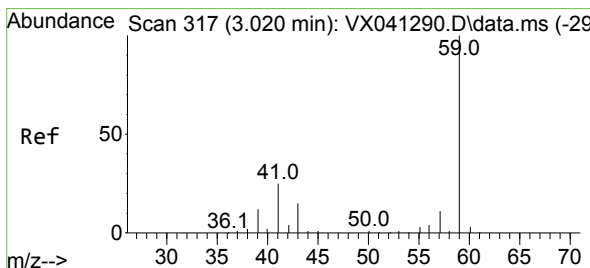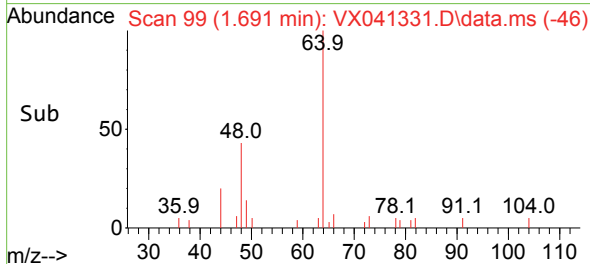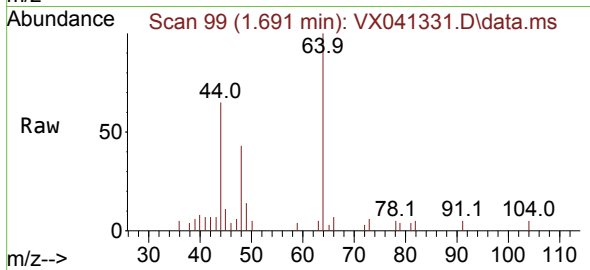

#11
Tert butyl alcohol
Concen: 5.796 ug/l
RT: 3.001 min Scan# 314
Delta R.T. -0.018 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion: 59 Resp: 2192
Ion Ratio Lower Upper
59 100
57 8.0 6.0 9.0

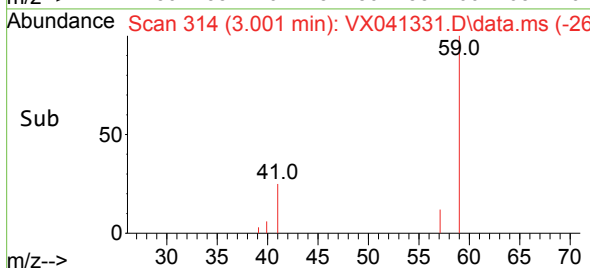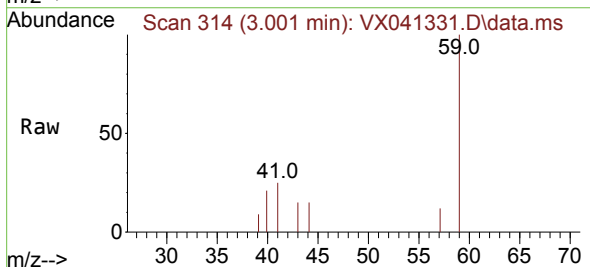

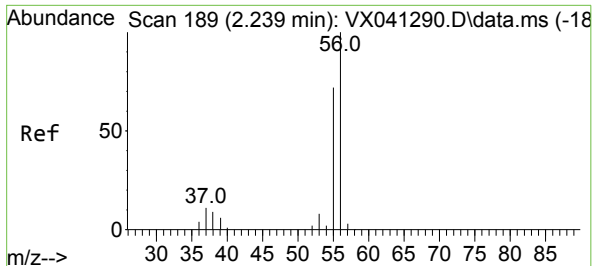

#13

Acrolein

Concen: 0.597 ug/l

RT: 2.203 min Scan# 189

Delta R.T. -0.037 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 56 Resp: 179

Ion Ratio Lower Upper

56 100

55 2013.4 57.1 85.7#

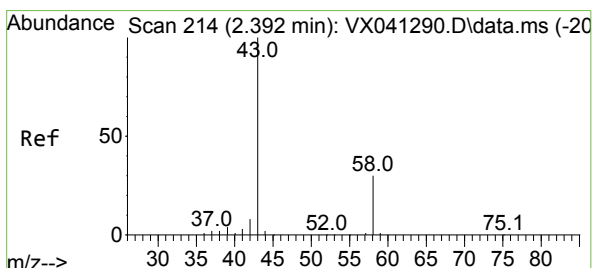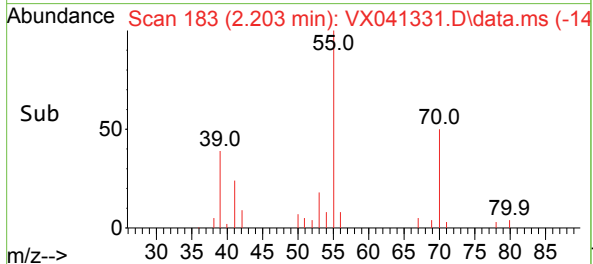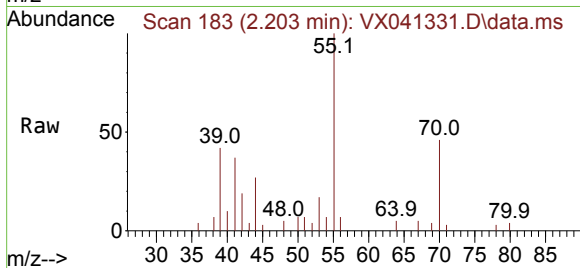

#16

Acetone

Concen: 6.680 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX041331.D




Acq: 01 May 2024 17:03


Tgt Ion: 43 Resp: 8726

Ion Ratio Lower Upper

43 100

58 31.2 21.9 32.9


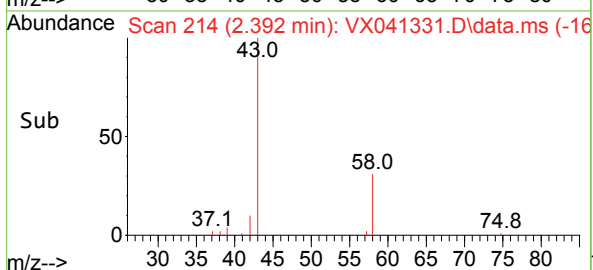

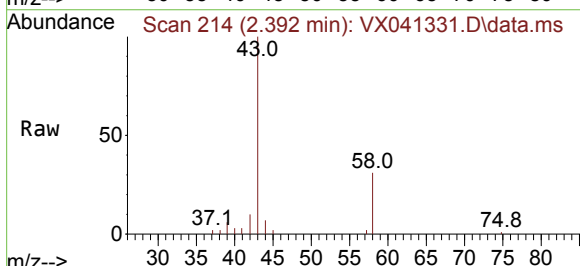




#19
Methyl tert-butyl Ether
Concen: 2.616 ug/l
RT: 3.117 min Scan# 31
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 73 Resp: 12826
Ion Ratio Lower Upper
73 100
57 24.3 17.3 25.9

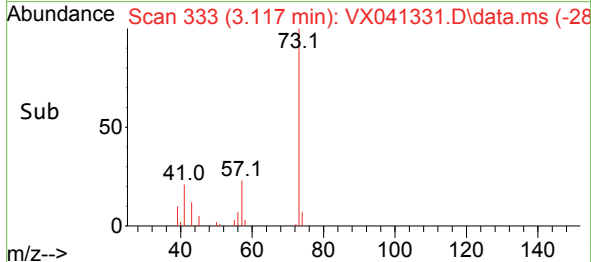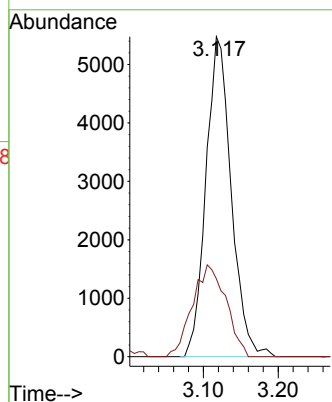

#20
Methylene Chloride
Concen: 0.537 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03


Tgt Ion: 84 Resp: 881
Ion Ratio Lower Upper
84 100
49 92.2 103.6 155.4#
51 31.2 33.8 50.6#
86 61.9 49.4 74.0

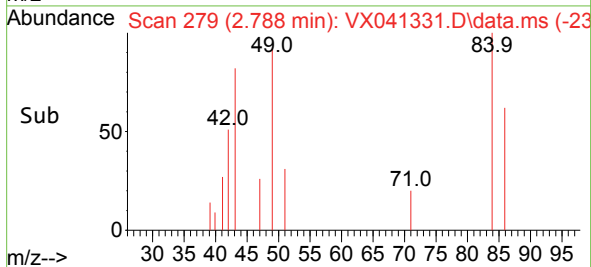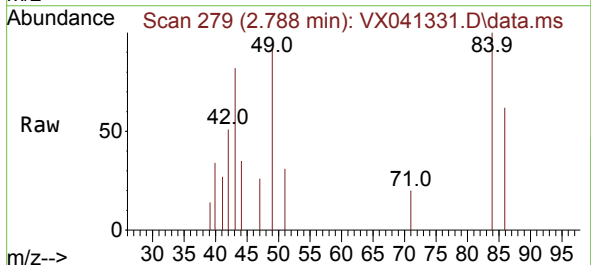






#31
Cyclohexane
Concen: 2.439 ug/l
RT: 5.464 min Scan# 718
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 56 Resp: 5563
Ion Ratio Lower Upper
56 100
69 32.6 23.4 35.2
84 87.4 65.9 98.9

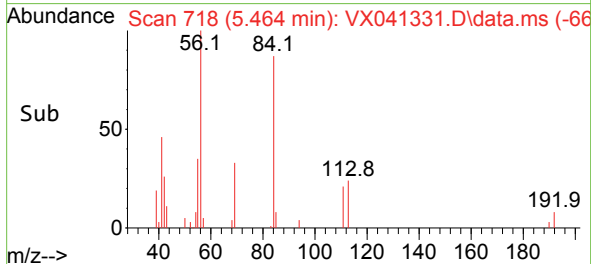

#33
1,2-Dichloroethane-d4
Concen: 51.697 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion: 65 Resp: 97681
Ion Ratio Lower Upper
65 100
67 50.0 0.0 100.2


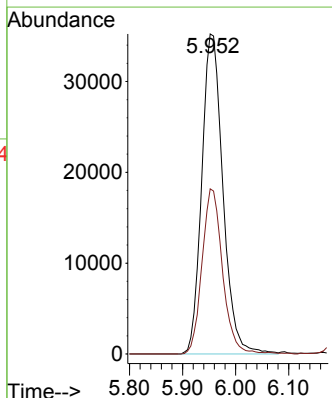
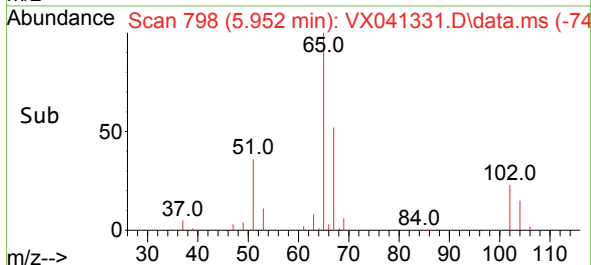
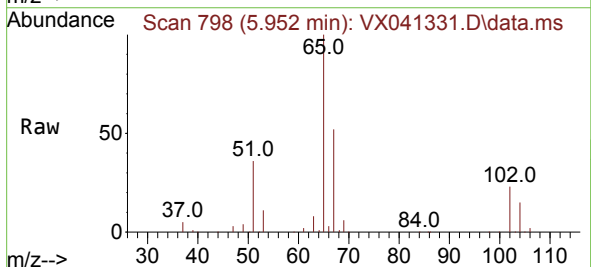


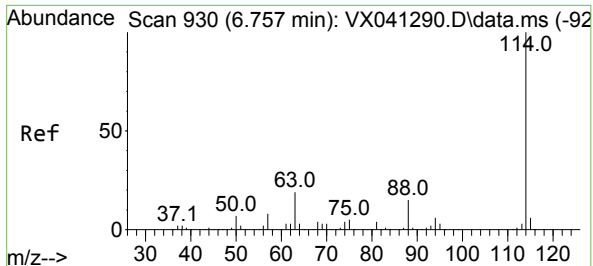

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.006 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 253228
Ion Ratio Lower Upper
114 100
63 18.3 0.0 45.0
88 15.0 0.0 36.6

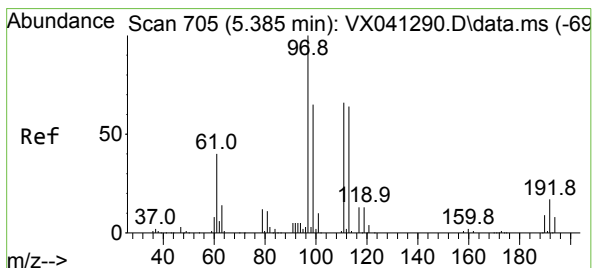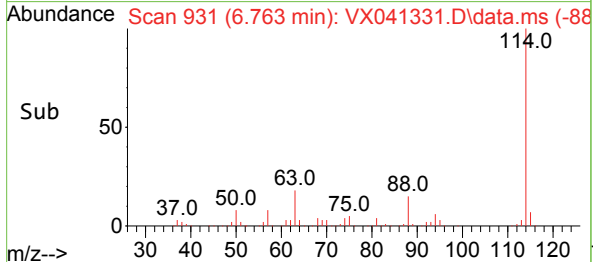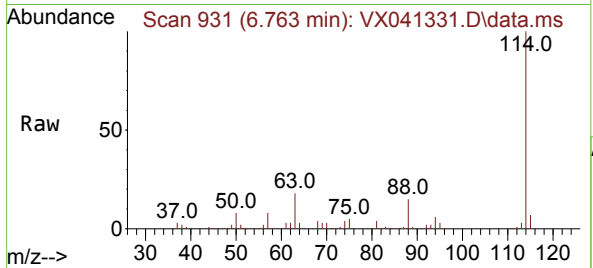

#35
Dibromofluoromethane
Concen: 45.759 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion:113 Resp: 78524
Ion Ratio Lower Upper
113 100
111 101.5 82.9 124.3
192 24.7 13.3 19.9#


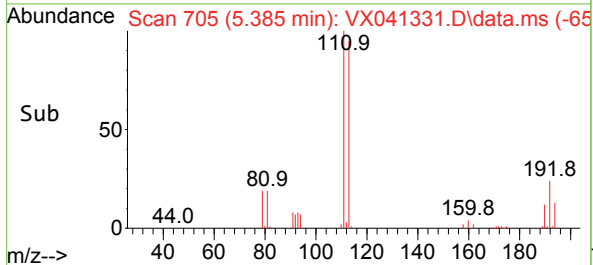

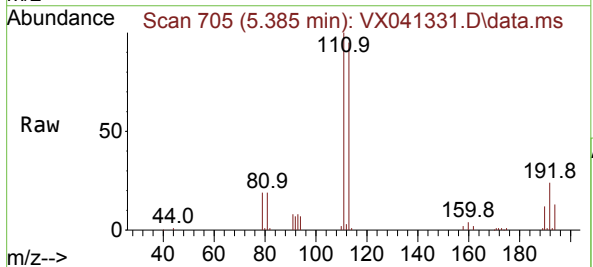




#36
1,1-Dichloropropene
Concen: 5.218 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 10708
Ion Ratio Lower Upper
75 100
110 10.3 17.0 50.9#
77 0.0 24.7 37.1#

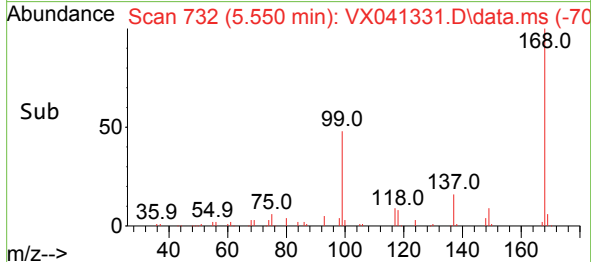

#38
Carbon Tetrachloride
Concen: 6.635 ug/l
RT: 5.550 min Scan# 732
Delta R.T. -0.122 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion: 117 Resp: 15596
Ion Ratio Lower Upper
117 100
119 5.3 78.2 117.2#
121 0.0 24.4 36.6#

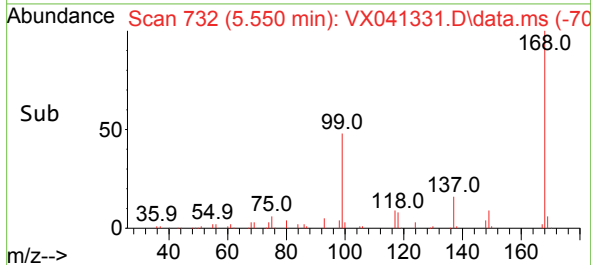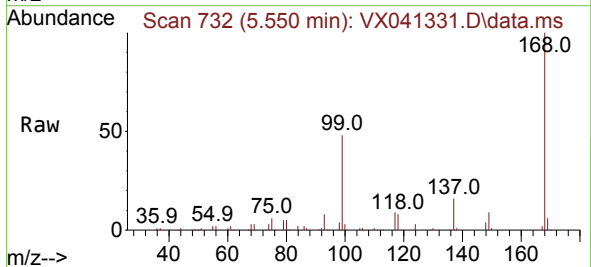



#39

Methylcyclohexane

Concen: 1.624 ug/l

RT: 7.373 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 83 Resp: 3914

Ion Ratio Lower Upper

83 100

55 82.9 64.6 97.0

98 46.5 36.7 55.1

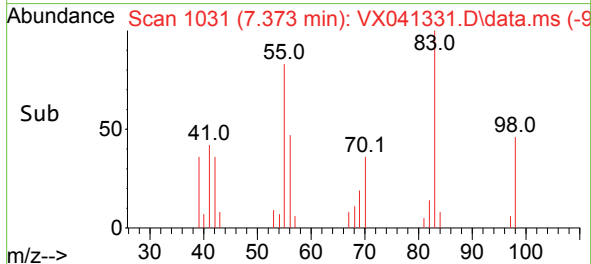

#41

Methacrylonitrile

Concen: 0.528 ug/l

RT: 5.196 min Scan# 674

Delta R.T. 0.268 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Tgt Ion: 41 Resp: 696




Ion Ratio Lower Upper


41 100

39 0.0 45.2 67.8#

67 703.2 52.6 78.8#

52 6.8 22.7 34.1#

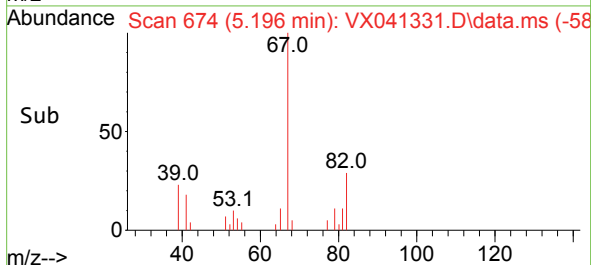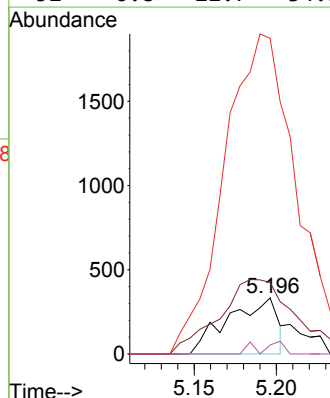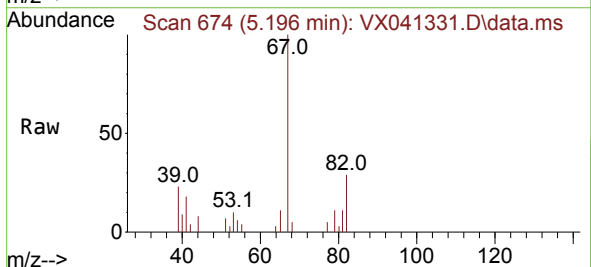



#48

Methyl methacrylate

Concen: 0.261 ug/l

RT: 7.653 min Scan# 1084

Delta R.T. -0.043 min

Lab File: VX041331.D





Acq: 01 May 2024 17:03

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 41	Resp: 460
Ion Ratio	Lower Upper
41	100
69	121.7 59.2 88.8#
39	52.2 47.7 71.5

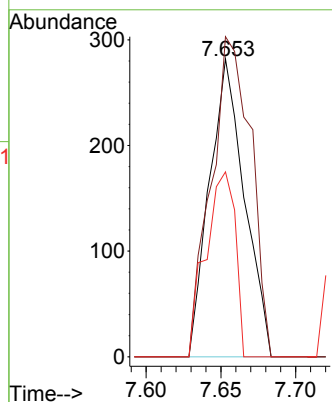

#50

Toluene-d8

Concen: 52.655 ug/l




RT: 8.647 min Scan# 1240


Delta R.T. 0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Tgt Ion: 98	Resp: 285994
Ion Ratio	Lower Upper
98	100
100	65.9 53.1 79.7




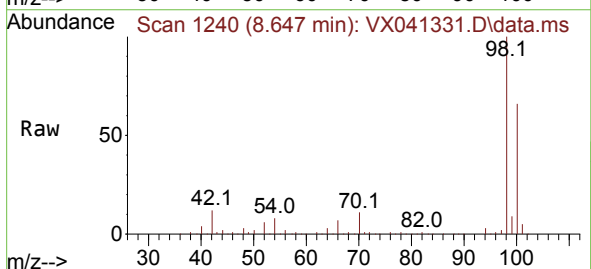




#51
4-Methyl-2-Pentanone
Concen: 0.588 ug/l
RT: 8.647 min Scan# 1314
Delta R.T. 0.067 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1359
Ion Ratio Lower Upper
43 100
58 168.4 30.4 45.6#

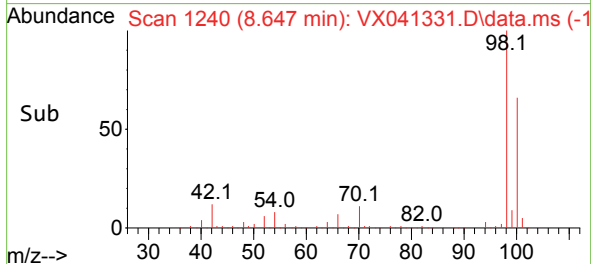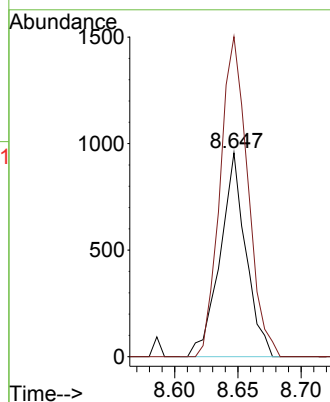

#55
1,1,2-Trichloroethane
Concen: 0.611 ug/l
RT: 9.098 min Scan# 1314
Delta R.T. -0.055 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion: 97 Resp: 911
Ion Ratio Lower Upper
97 100
83 10.4 65.8 98.8#
85 0.0 41.6 62.4#
99 0.0 47.8 71.8#


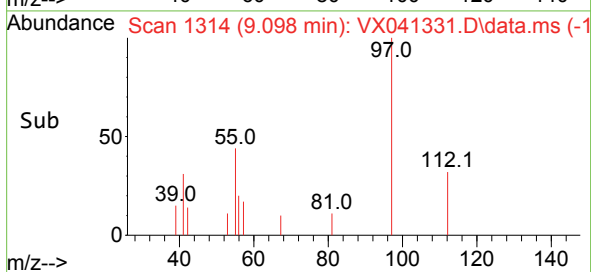

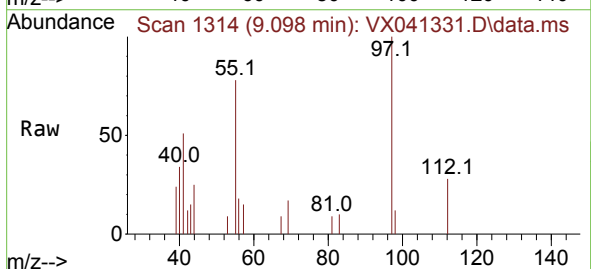




#59
2-Hexanone
Concen: 1.040 ug/l
RT: 9.250 min Scan# 11
Delta R.T. -0.183 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 1921
Ion Ratio Lower Upper
43 100
58 32.8 26.2 78.5

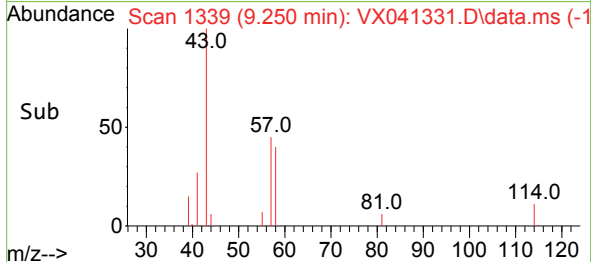

#62
4-Bromofluorobenzene
Concen: 57.399 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion: 95 Resp: 120684
Ion Ratio Lower Upper
95 100
174 98.0 0.0 135.6
176 96.4 0.0 131.0

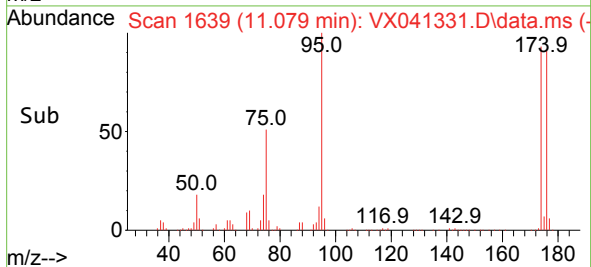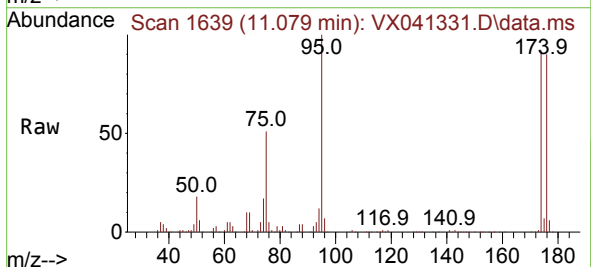



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:117 Resp: 231515

Ion Ratio Lower Upper

117 100

82 51.1 46.2 69.4

119 32.5 25.5 38.3

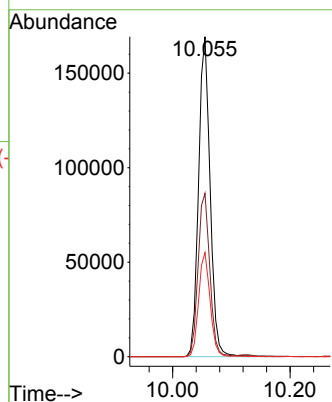

#68

m/p-Xylenes

Concen: 0.869 ug/l

RT: 10.305 min Scan# 1512

Delta R.T. 0.006 min

Lab File: VX041331.D




Acq: 01 May 2024 17:03


Tgt Ion:106 Resp: 2697

Ion Ratio Lower Upper

106 100

91 200.0 165.5 248.3









#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:152 Resp: 138067
Ion Ratio Lower Upper
152 100
115 53.3 43.3 129.9
150 154.9 0.0 345.0

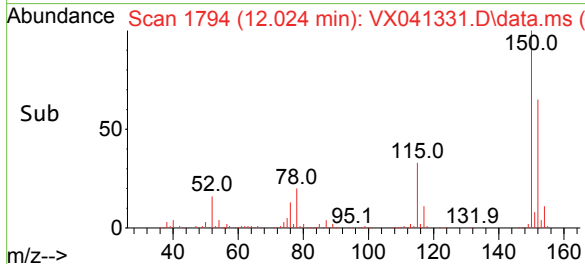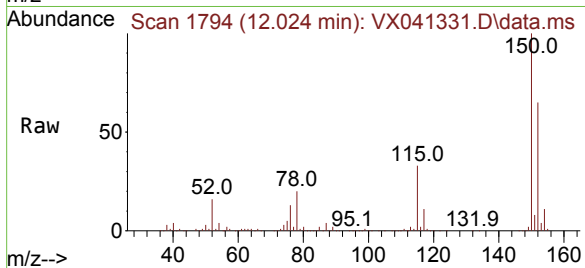

#73
Isopropylbenzene
Concen: 1.442 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. 0.000 min
Lab File: VX041331.D
Acq: 01 May 2024 17:03

Tgt Ion:105 Resp: 12151
Ion Ratio Lower Upper
105 100
120 26.6 12.9 38.6

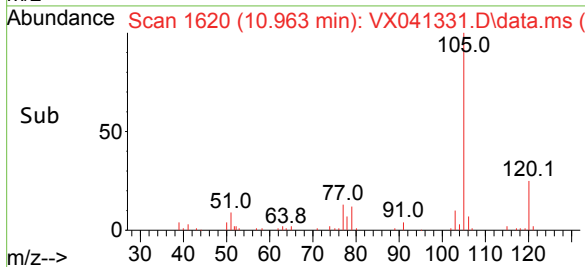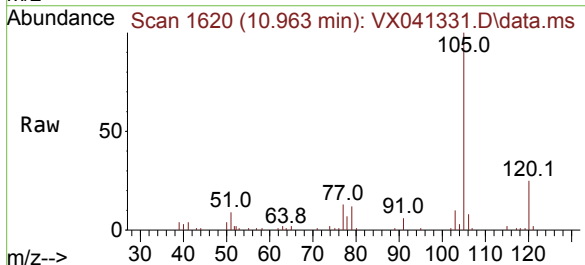



#76

1,2,3-Trichloropropane

Concen: 26.791 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 60281

Ion Ratio Lower Upper

75 100

77 1.1 19.1 57.5#

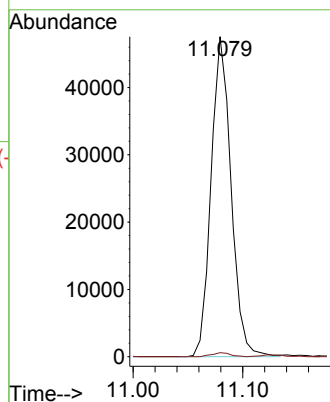

#78

n-propylbenzene

Concen: 0.453 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX041331.D




Acq: 01 May 2024 17:03


Tgt Ion: 91 Resp: 4012

Ion Ratio Lower Upper

91 100

120 24.0 11.5 34.4

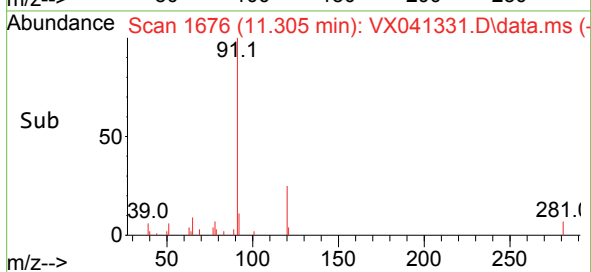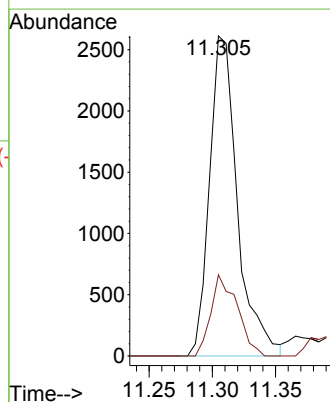



#79

2-Chlorotoluene

Concen: 0.703 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. -0.061 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 4012

Ion Ratio Lower Upper

91 100

126 0.0 16.3 48.8#

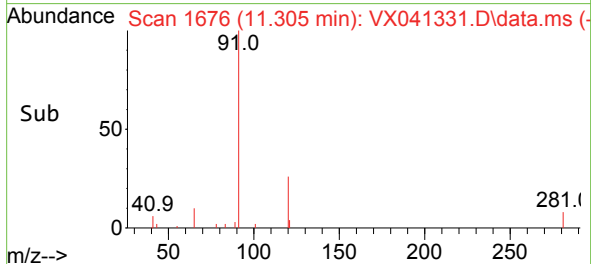

#81

trans-1,4-Dichloro-2-butene

Concen: 72.975 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03




Tgt Ion: 75 Resp: 60281


Ion Ratio Lower Upper

75 100

53 0.0 90.5 135.7#

89 0.0 36.9 55.3#

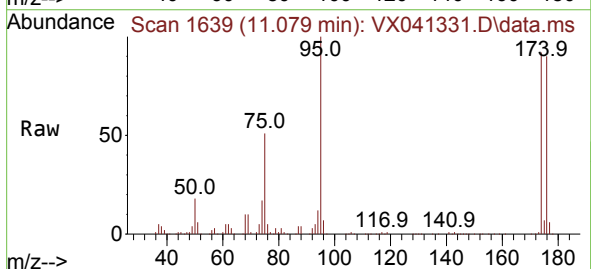



#82

4-Chlorotoluene

Concen: 0.620 ug/l

RT: 11.305 min Scan# 1

Delta R.T. -0.146 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 91 Resp: 4012

Ion Ratio Lower Upper

91 100

126 0.0 14.2 42.6#

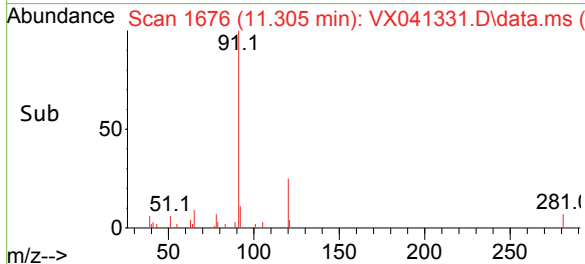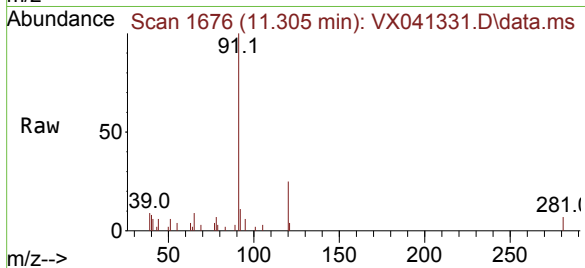

#83

tert-Butylbenzene

Concen: 2.521 ug/l

RT: 11.713 min Scan# 1743

Delta R.T. 0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03




Tgt Ion: 119 Resp: 18549


Ion Ratio Lower Upper

119 100

91 64.2 31.2 93.6

134 25.9 11.7 35.0

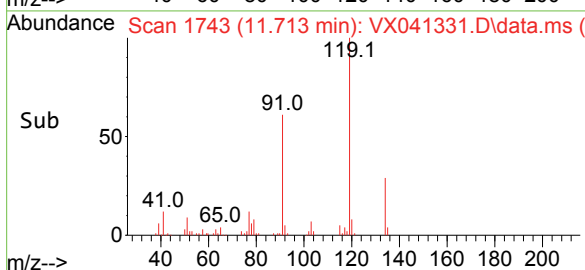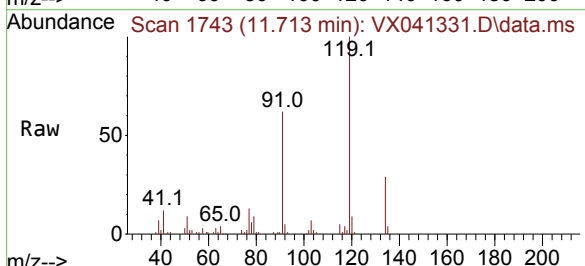



#84

1,2,4-Trimethylbenzene

Concen: 0.964 ug/l

RT: 11.616 min Scan# 1727

Delta R.T. -0.134 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:105 Resp: 6666

Ion Ratio Lower Upper

105 100

120 31.8 21.2 63.6

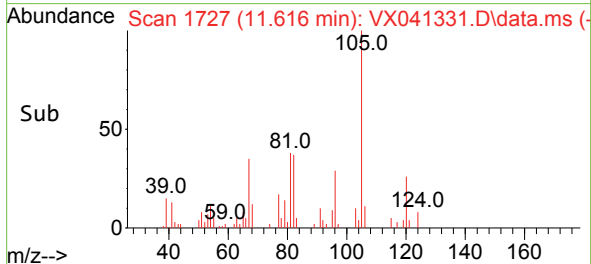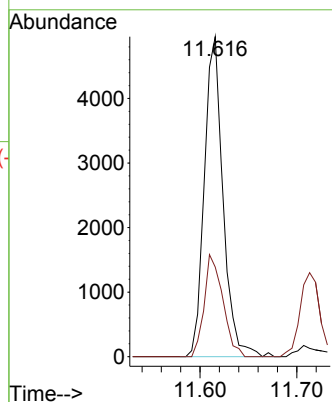

#85

sec-Butylbenzene

Concen: 4.891 ug/l

RT: 11.890 min Scan# 1772

Delta R.T. 0.000 min

Lab File: VX041331.D




Acq: 01 May 2024 17:03


Tgt Ion:105 Resp: 41239

Ion Ratio Lower Upper

105 100

134 19.7 9.8 29.4





#86

p-Isopropyltoluene

Concen: 4.690 ug/l

RT: 12.177 min Scan# 119

Delta R.T. 0.171 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:119 Resp: 35515

Ion Ratio Lower Upper

119 100

134 28.8 12.8 38.3

91 23.7 13.1 39.3

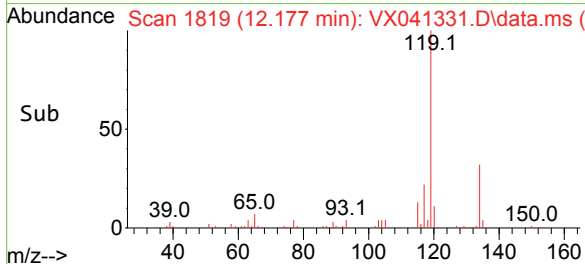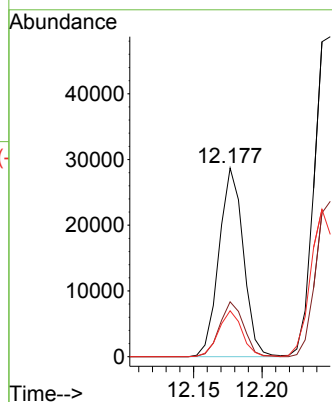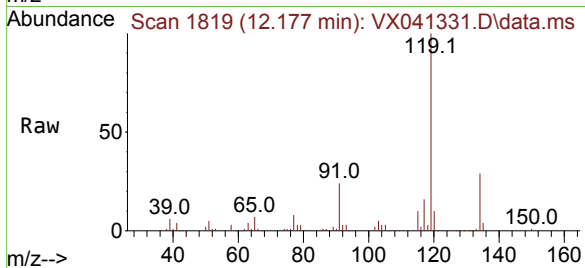

#89

n-Butylbenzene

Concen: 0.962 ug/l

RT: 12.329 min Scan# 1844

Delta R.T. 0.000 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03




Tgt Ion: 91 Resp: 5858


Ion Ratio Lower Upper

91 100

92 48.1 27.4 82.0

134 34.0 12.6 37.8

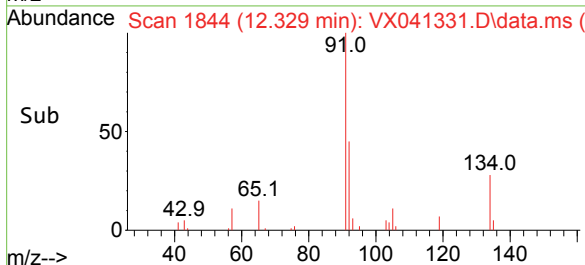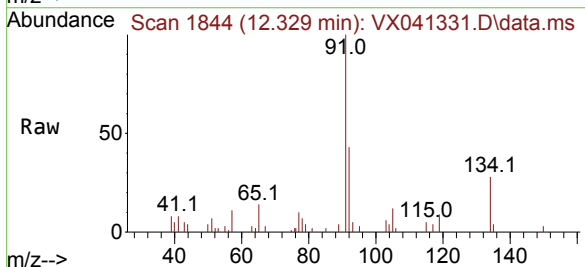



#90

Hexachloroethane

Concen: 62.612 ug/l

RT: 12.646 min Scan# 117

Delta R.T. 0.110 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion:117 Resp: 79288

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#

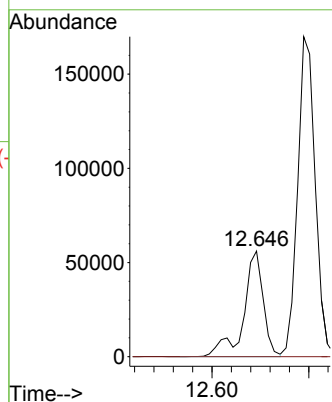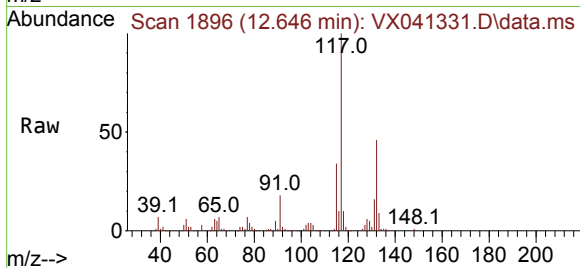

#92

1,2-Dibromo-3-Chloropropane

Concen: 2.304 ug/l

RT: 12.920 min Scan# 1941

Delta R.T. -0.018 min

Lab File: VX041331.D

Acq: 01 May 2024 17:03

Tgt Ion: 75 Resp: 1470

Ion Ratio Lower Upper

75 100

155 0.0 36.1 108.5#

157 0.0 44.9 134.7#

