

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
Data File : VX041332.D
Acq On : 01 May 2024 17:26
Operator : JC/MD
Sample : P2264-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-042324-01

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M

Title : SW846 8260

Signal : TIC: VX041332.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.563	69	78	79	rBV5	5219	11413	1.63%	0.278%
2	2.392	207	214	225	rBV	7890	14461	2.06%	0.352%
3	5.385	694	705	721	rBV2	90668	274567	39.20%	6.692%
4	5.550	721	732	748	rVV	152220	434074	61.97%	10.579%
5	5.952	788	798	817	rBV	97619	260383	37.17%	6.346%
6	6.757	921	930	956	rBV	241414	585934	83.65%	14.281%
7	8.647	1233	1240	1252	rBV	452010	700493	100.00%	17.073%
8	10.055	1465	1471	1487	rBV	450186	627505	89.58%	15.294%
9	11.079	1634	1639	1654	rBV	387903	511278	72.99%	12.461%
10	12.024	1788	1794	1808	rBV	503276	667138	95.24%	16.260%
11	12.244	1826	1830	1839	rVB5	4657	7193	1.03%	0.175%
12	13.292	1994	2002	2007	rBV3	5844	8573	1.22%	0.209%




Sum of corrected areas: 4103012

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
Data File : VX041332.D
Acq On : 01 May 2024 17:26
Operator : JC/MD
Sample : P2264-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-042324-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

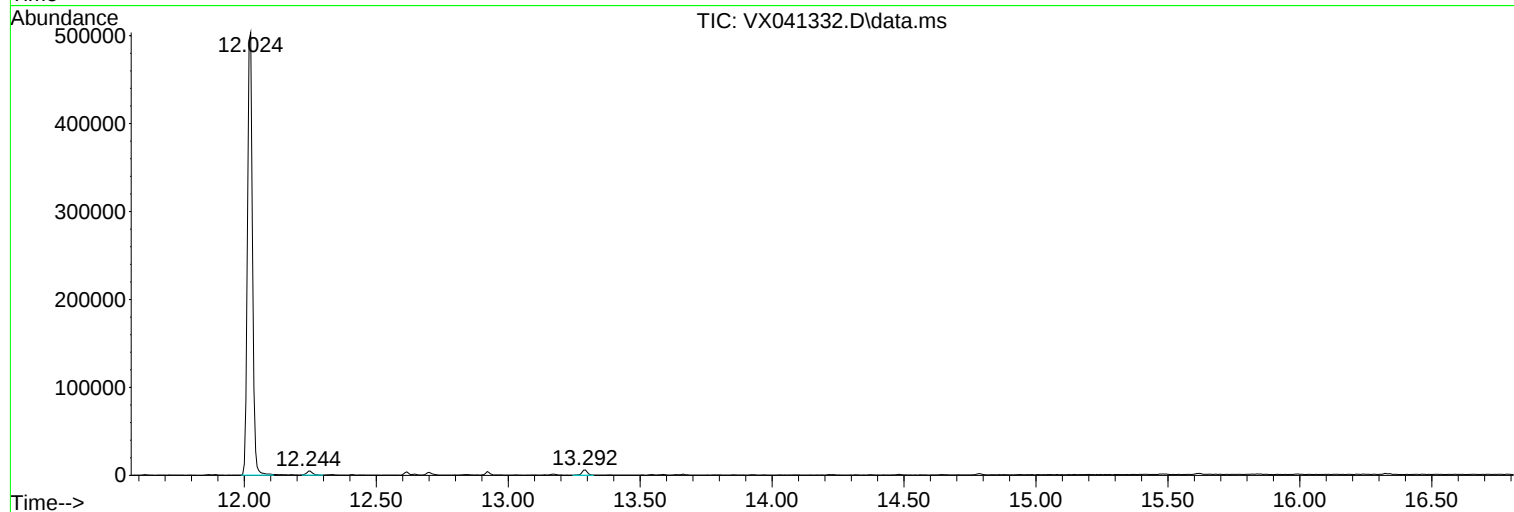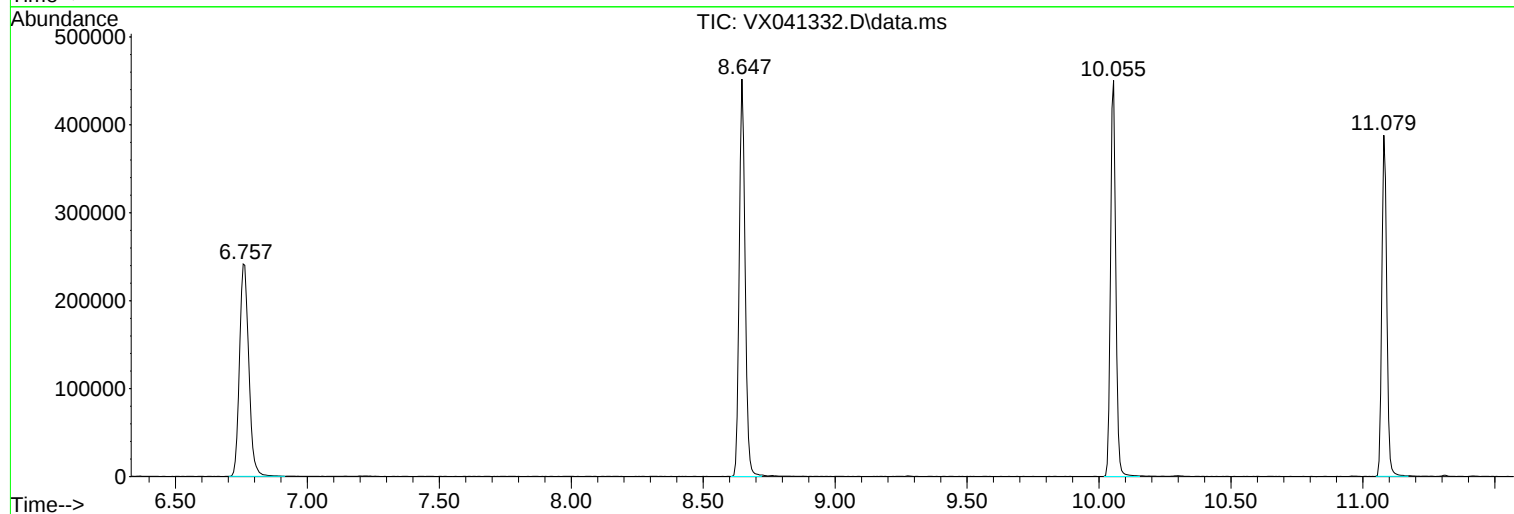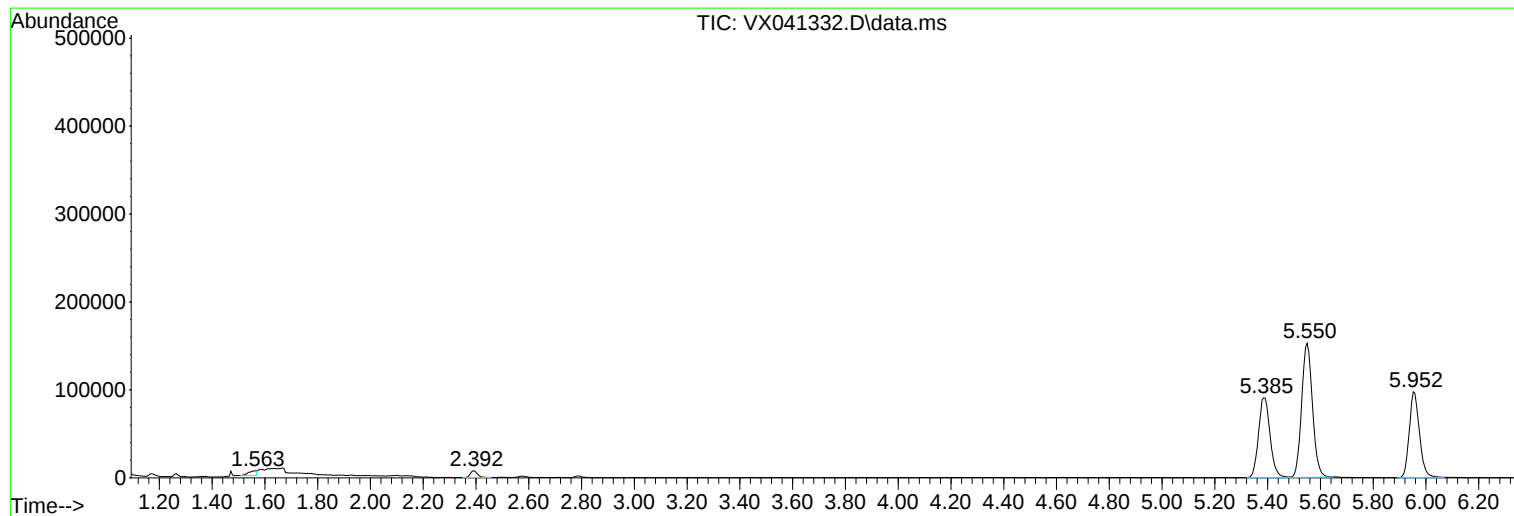

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
Data File : VX041332.D
Acq On : 01 May 2024 17:26
Operator : JC/MD
Sample : P2264-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-042324-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050124\
Data File : VX041332.D
Acq On : 01 May 2024 17:26
Operator : JC/MD
Sample : P2264-23
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP-042324-01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------