


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX050219\
Data File : VX009264.D
Acq On : 02 May 2019 09:14
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X050119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 02 06:46:57 2019

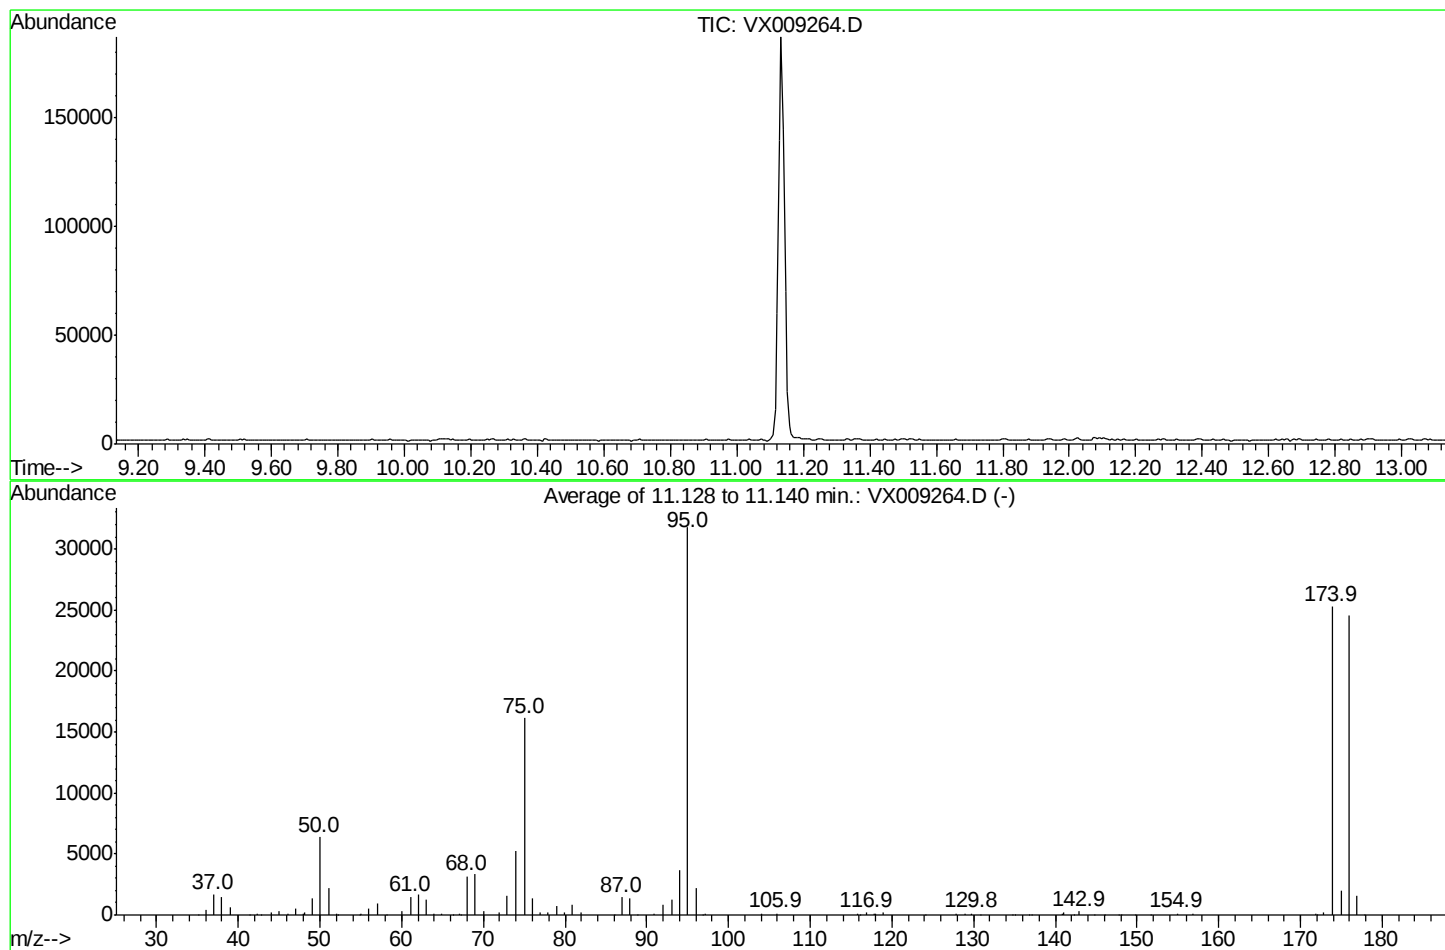

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	6394	PASS
75	95	30	60	50.7	16122	PASS
95	95	100	100	100.0	31773	PASS
96	95	5	9	6.9	2178	PASS
173	174	0.00	2	0.9	230	PASS
174	95	50	100	79.5	25258	PASS
175	174	5	9	8.0	2029	PASS
176	174	95	101	97.0	24506	PASS
177	176	5	9	6.3	1553	PASS