

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050222\
 Data File : VX028470.D
 Acq On : 02 May 2022 12:56
 Operator : JC/MD
 Sample : VX0502WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0502WBL01

Quant Time: May 03 04:50:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 19 13:38:04 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	415670	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	715236	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	696064	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	333692	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	283847	52.372	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 104.740%	
35) Dibromofluoromethane	5.391	113	263650	52.563	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 105.120%	
50) Toluene-d8	8.653	98	971436	50.425	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 100.840%	
62) 4-Bromofluorobenzene	11.079	95	352964	47.917	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 95.840%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050222\
Data File : VX028470.D
Acq On : 02 May 2022 12:56
Operator : JC/MD
Sample : VX0502WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0502WBL01

Quant Time: May 03 04:50:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 19 13:38:04 2022
Response via : Initial Calibration




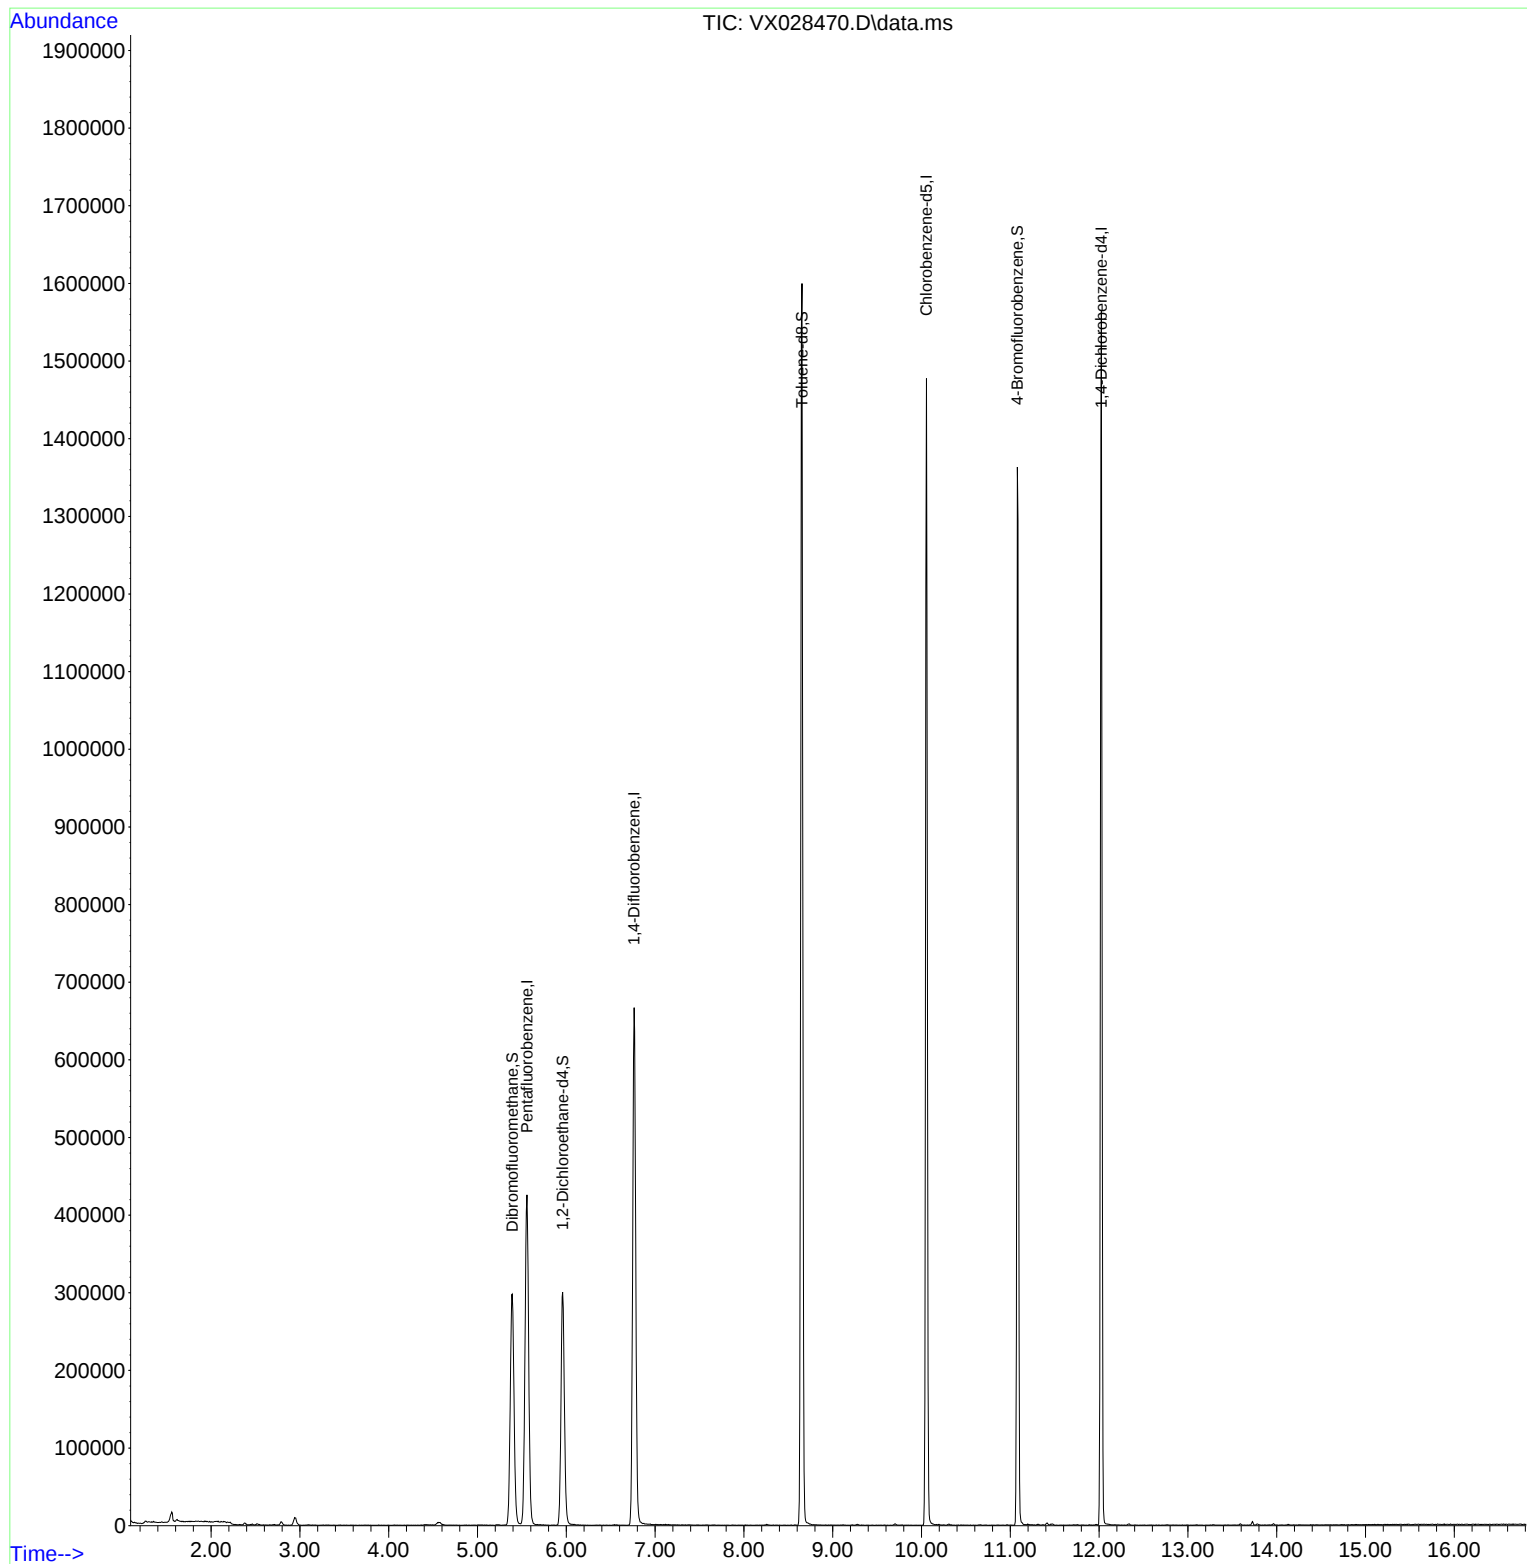




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 713
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56




Instrument :
MSVOA_X
ClientSampleId :
VX0502WBL01


Tgt Ion:168 Resp: 415670
Ion Ratio Lower Upper
168 100
99 54.5 41.7 62.5

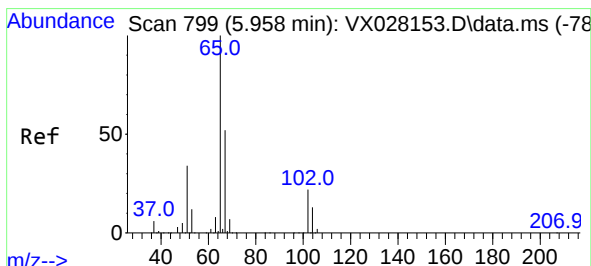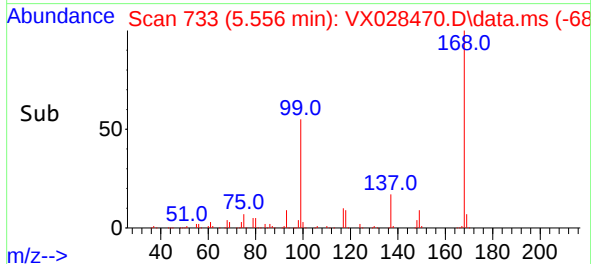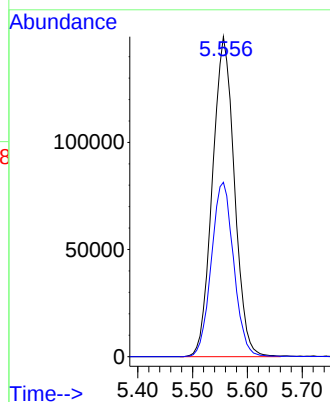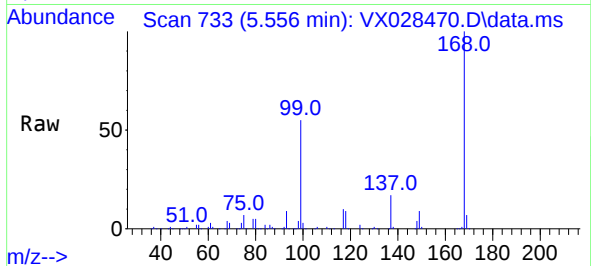

#33
1,2-Dichloroethane-d4
Concen: 52.372 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56


Tgt Ion: 65 Resp: 283847
Ion Ratio Lower Upper
65 100
67 52.1 0.0 107.4

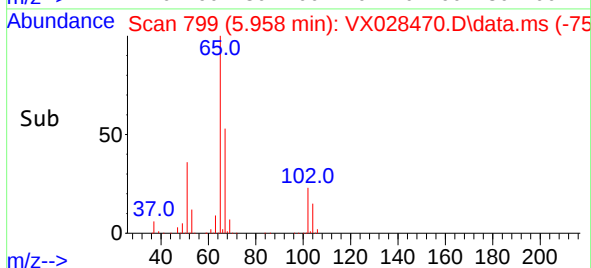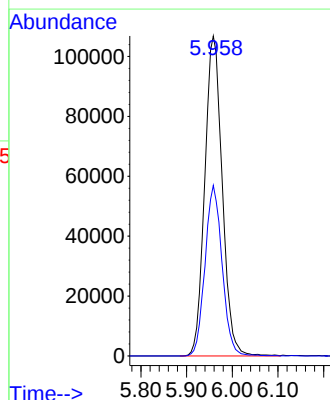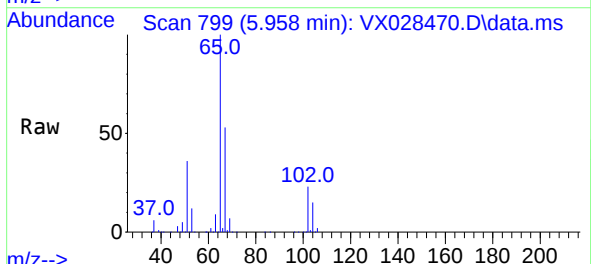



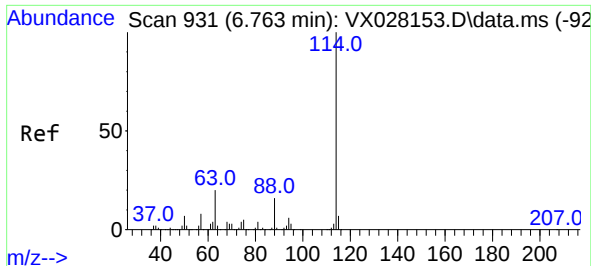


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56

Instrument :
MSVOA_X
ClientSampleId :
VX0502WBL01



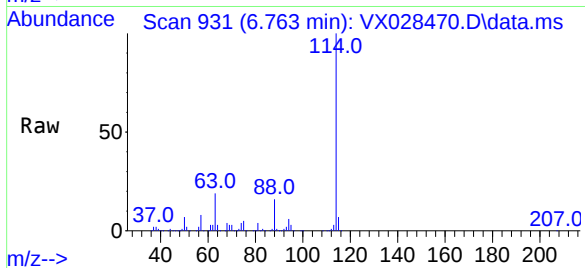


Tgt Ion:114 Resp: 715236
Ion Ratio Lower Upper
114 100
63 18.8 0.0 36.8
88 15.7 0.0 32.4

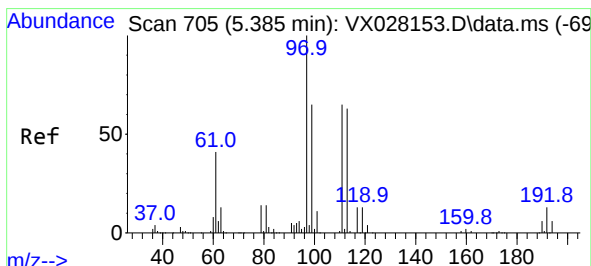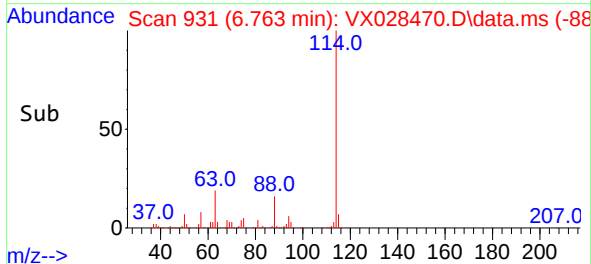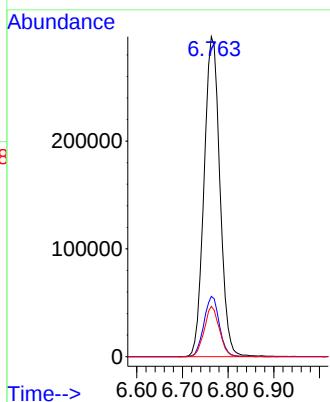

#35
Dibromofluoromethane
Concen: 52.563 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.006 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56

Tgt Ion:113 Resp: 263650
Ion Ratio Lower Upper
113 100
111 101.6 82.8 124.2
192 19.9 16.9 25.3


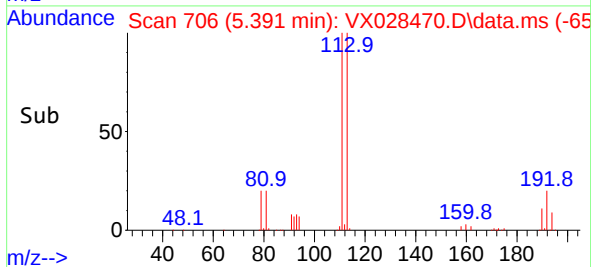
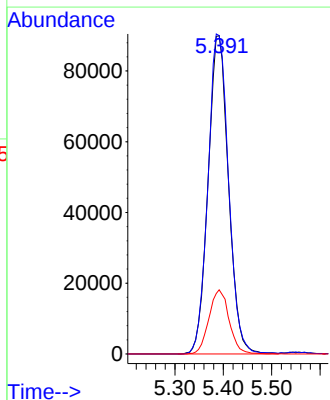
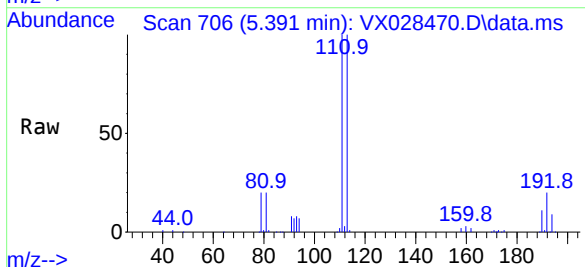




#50
Toluene-d8
Concen: 50.425 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56




Instrument :
MSVOA_X
ClientSampleId :
VX0502WBL01


Tgt Ion: 98 Resp: 971436
Ion Ratio Lower Upper
98 100
100 66.2 52.6 78.8

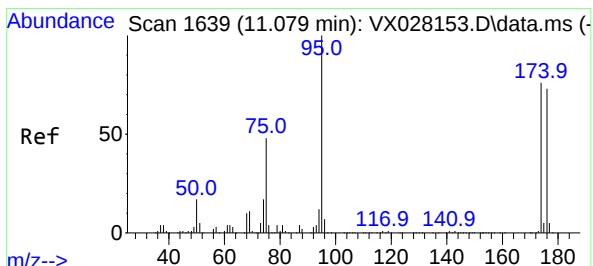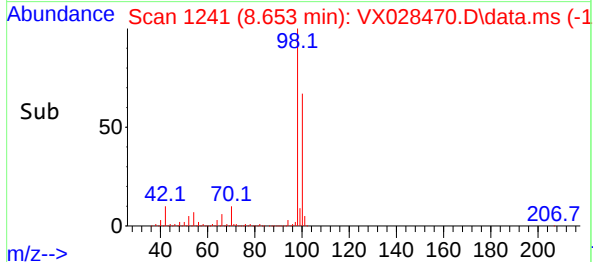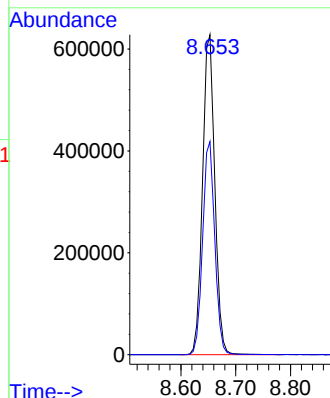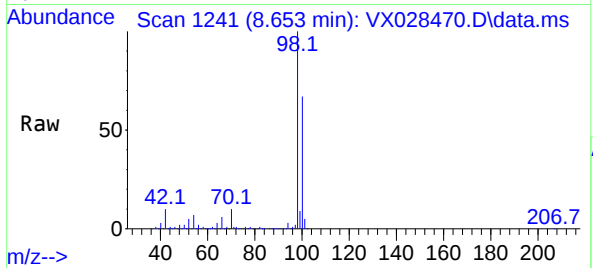

#62
4-Bromofluorobenzene
Concen: 47.917 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56

Tgt Ion: 95 Resp: 352964
Ion Ratio Lower Upper
95 100
174 85.8 0.0 163.0
176 83.5 0.0 155.0


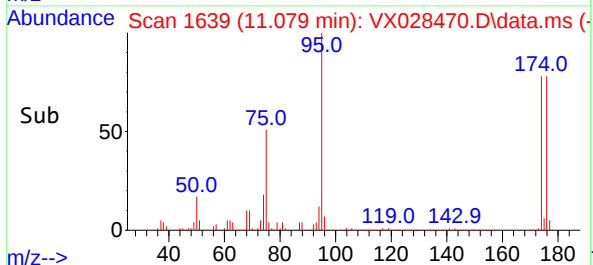
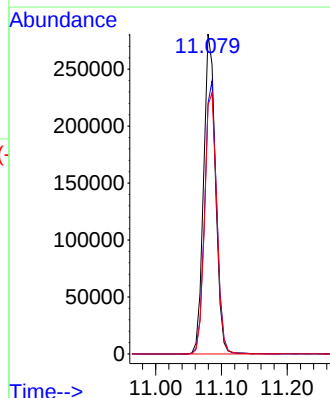
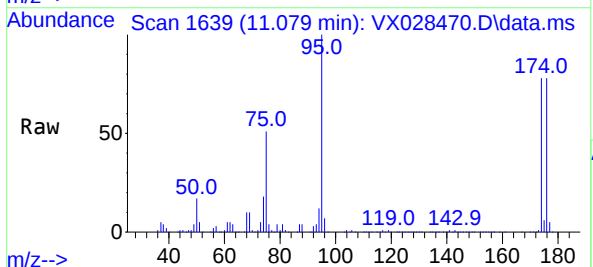


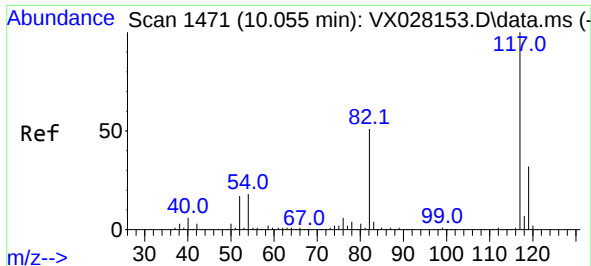

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56

Instrument :
MSVOA_X
ClientSampleId :
VX0502WBL01

Tgt Ion:117 Resp: 696064
Ion Ratio Lower Upper
117 100
82 52.2 41.8 62.8
119 32.3 24.8 37.2

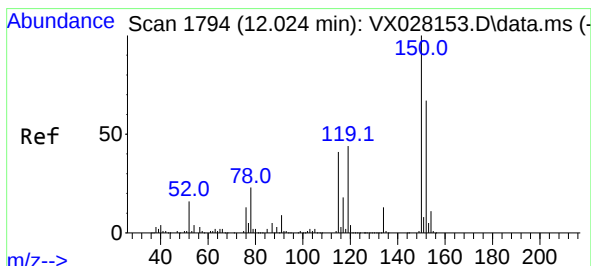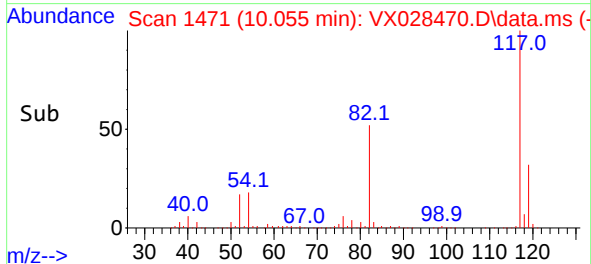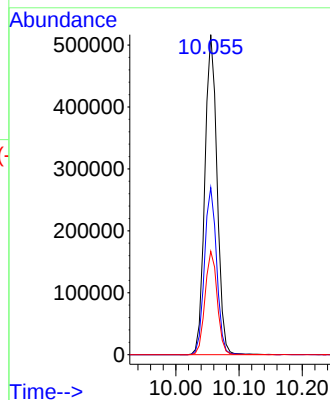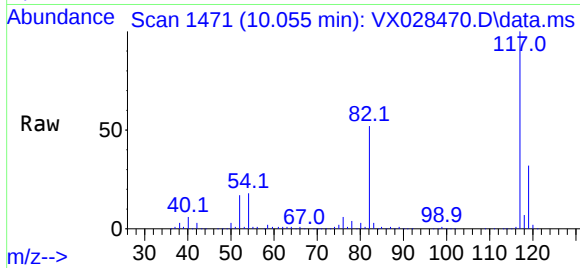

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX028470.D
Acq: 02 May 2022 12:56

Tgt Ion:152 Resp: 333692
Ion Ratio Lower Upper
152 100
115 58.2 37.5 112.7
150 158.2 0.0 338.2

