
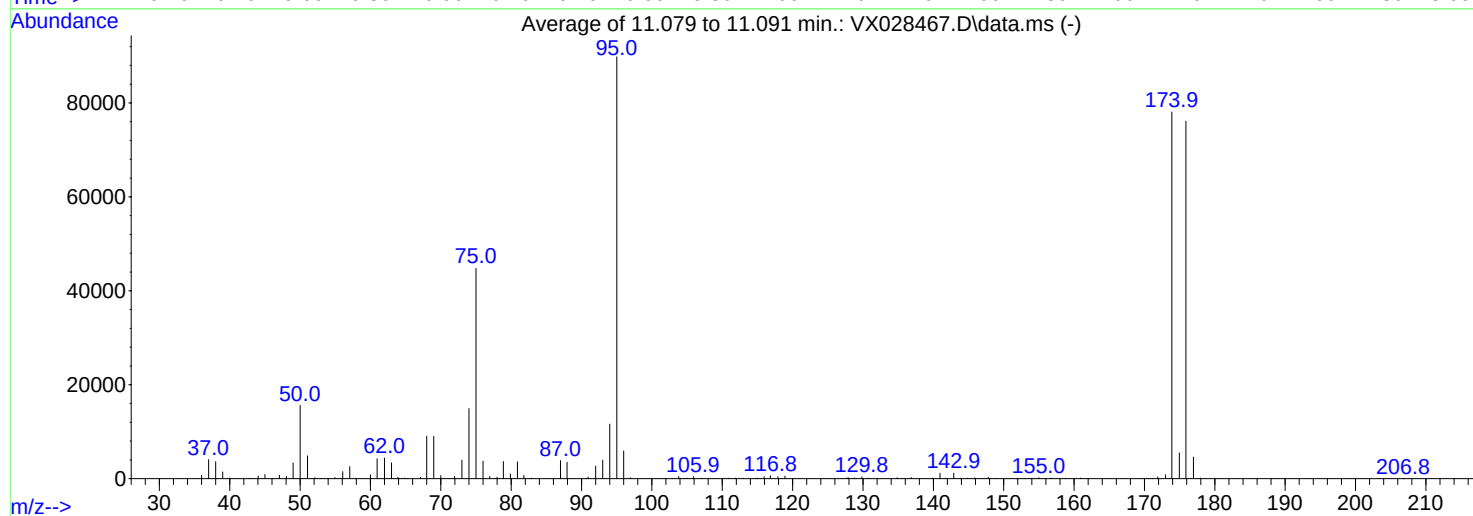


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050222\
 Data File : VX028467.D
 Acq On : 02 May 2022 09:49
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Title : SW846 8260
 Last Update : Tue Apr 19 13:38:04 2022

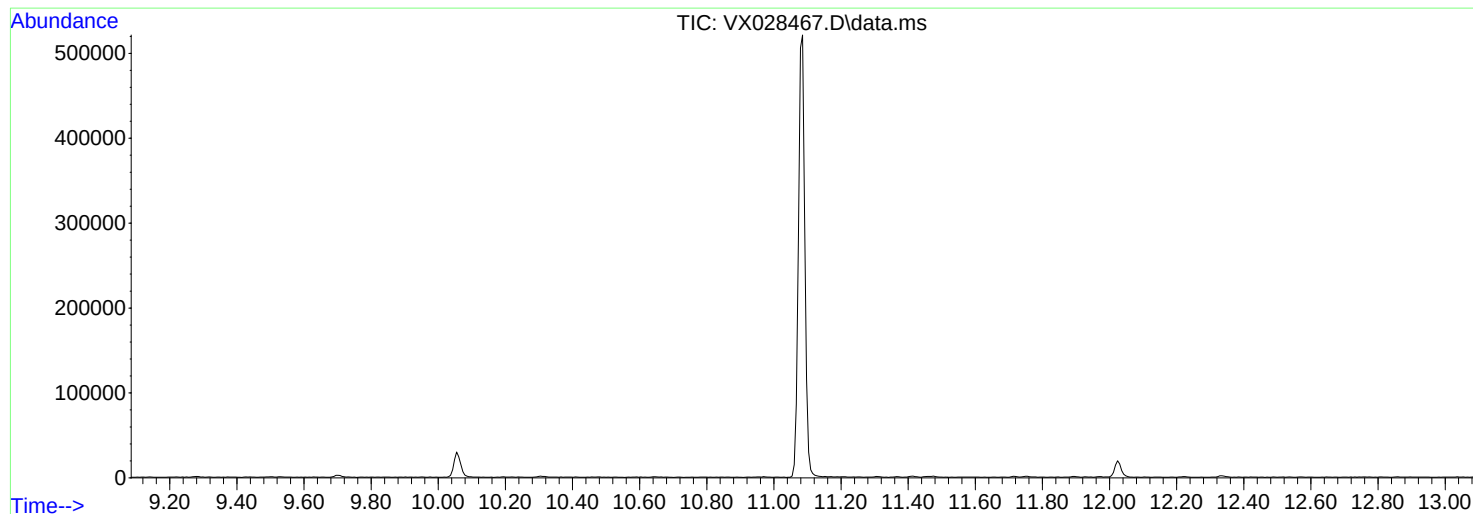

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	15595	PASS
75	95	30	60	49.9	44784	PASS
95	95	100	100	100.0	89819	PASS
96	95	5	9	6.6	5915	PASS
173	174	0.00	2	1.1	824	PASS
174	95	50	100	86.9	78072	PASS
175	174	5	9	7.0	5498	PASS
176	174	95	101	97.5	76101	PASS
177	176	5	9	6.0	4601	PASS