

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050224\
 Data File : VX041350.D
 Acq On : 02 May 2024 13:50
 Operator : JC/MD
 Sample : PB160645TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 03 01:37:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 02:38:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	185973	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	267979	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	282720	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	143605	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	98312	48.559	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.120%
35) Dibromofluoromethane	5.385	113	79545	43.802	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.600%
50) Toluene-d8	8.647	98	315301	54.856	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	109.720%
62) 4-Bromofluorobenzene	11.079	95	110298	49.572	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.140%
Target Compounds						
						Qvalue
3) Chloromethane	1.301	50	383	0.242	ug/l	# 43
5) Bromomethane	1.599	94	399	0.422	ug/l	93
6) Chloroethane	1.685	64	775	1.107	ug/l	# 52
11) Tert butyl alcohol	3.014	59	3662	9.037	ug/l	# 91
16) Acetone	2.392	43	26172	25.849	ug/l	93
18) Methyl Acetate	2.709	43	2563	1.237	ug/l	# 89
20) Methylene Chloride	2.788	84	6396	3.639	ug/l	88
25) 2-Butanone	4.580	43	19114	14.587	ug/l	95
29) Tetrahydrofuran	5.050	42	960	1.120	ug/l	# 59
31) Cyclohexane	5.538	56	3261	1.335	ug/l	# 14
36) 1,1-Dichloropropene	5.550	75	11508	5.300	ug/l	# 51
37) Ethyl Acetate	4.733	43	3176	1.172	ug/l	# 96
38) Carbon Tetrachloride	5.544	117	16331	6.565	ug/l	# 15
41) Methacrylonitrile	5.044	41	353	0.253	ug/l	# 52
43) Isopropyl Acetate	6.348	43	116245	28.535	ug/l	98
48) Methyl methacrylate	7.616	41	4514	2.417	ug/l	# 16
49) 1,4-Dioxane	7.805	88	142	3.517	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.549	43	90581	37.055	ug/l	# 50
52) Toluene	8.720	92	3828	0.935	ug/l	99
53) t-1,3-Dichloropropene	8.958	75	826	0.393	ug/l	# 43
54) cis-1,3-Dichloropropene	8.549	75	41260	17.689	ug/l	# 57
57) 1,3-Dichloropropane	9.482	76	5552	2.109	ug/l	# 42
59) 2-Hexanone	9.439	43	9001	4.605	ug/l	99
74) N-amyl acetate	10.774	43	3044	0.795	ug/l	# 51
76) 1,2,3-Trichloropropane	11.079	75	55489	23.710	ug/l	# 38
78) n-propylbenzene	11.305	91	6346	0.689	ug/l	97
79) 2-Chlorotoluene	11.305	91	6346	1.070	ug/l	# 42
81) trans-1,4-Dichloro-2-b...	11.079	75	55489	64.583	ug/l	# 5
82) 4-Chlorotoluene	11.305	91	6346	0.942	ug/l	# 46
90) Hexachloroethane	12.616	117	309	0.235	ug/l	# 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050224\
Data File : VX041350.D
Acq On : 02 May 2024 13:50
Operator : JC/MD
Sample : PB160645TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 03 01:37:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 01 02:38:17 2024
Response via : Initial Calibration




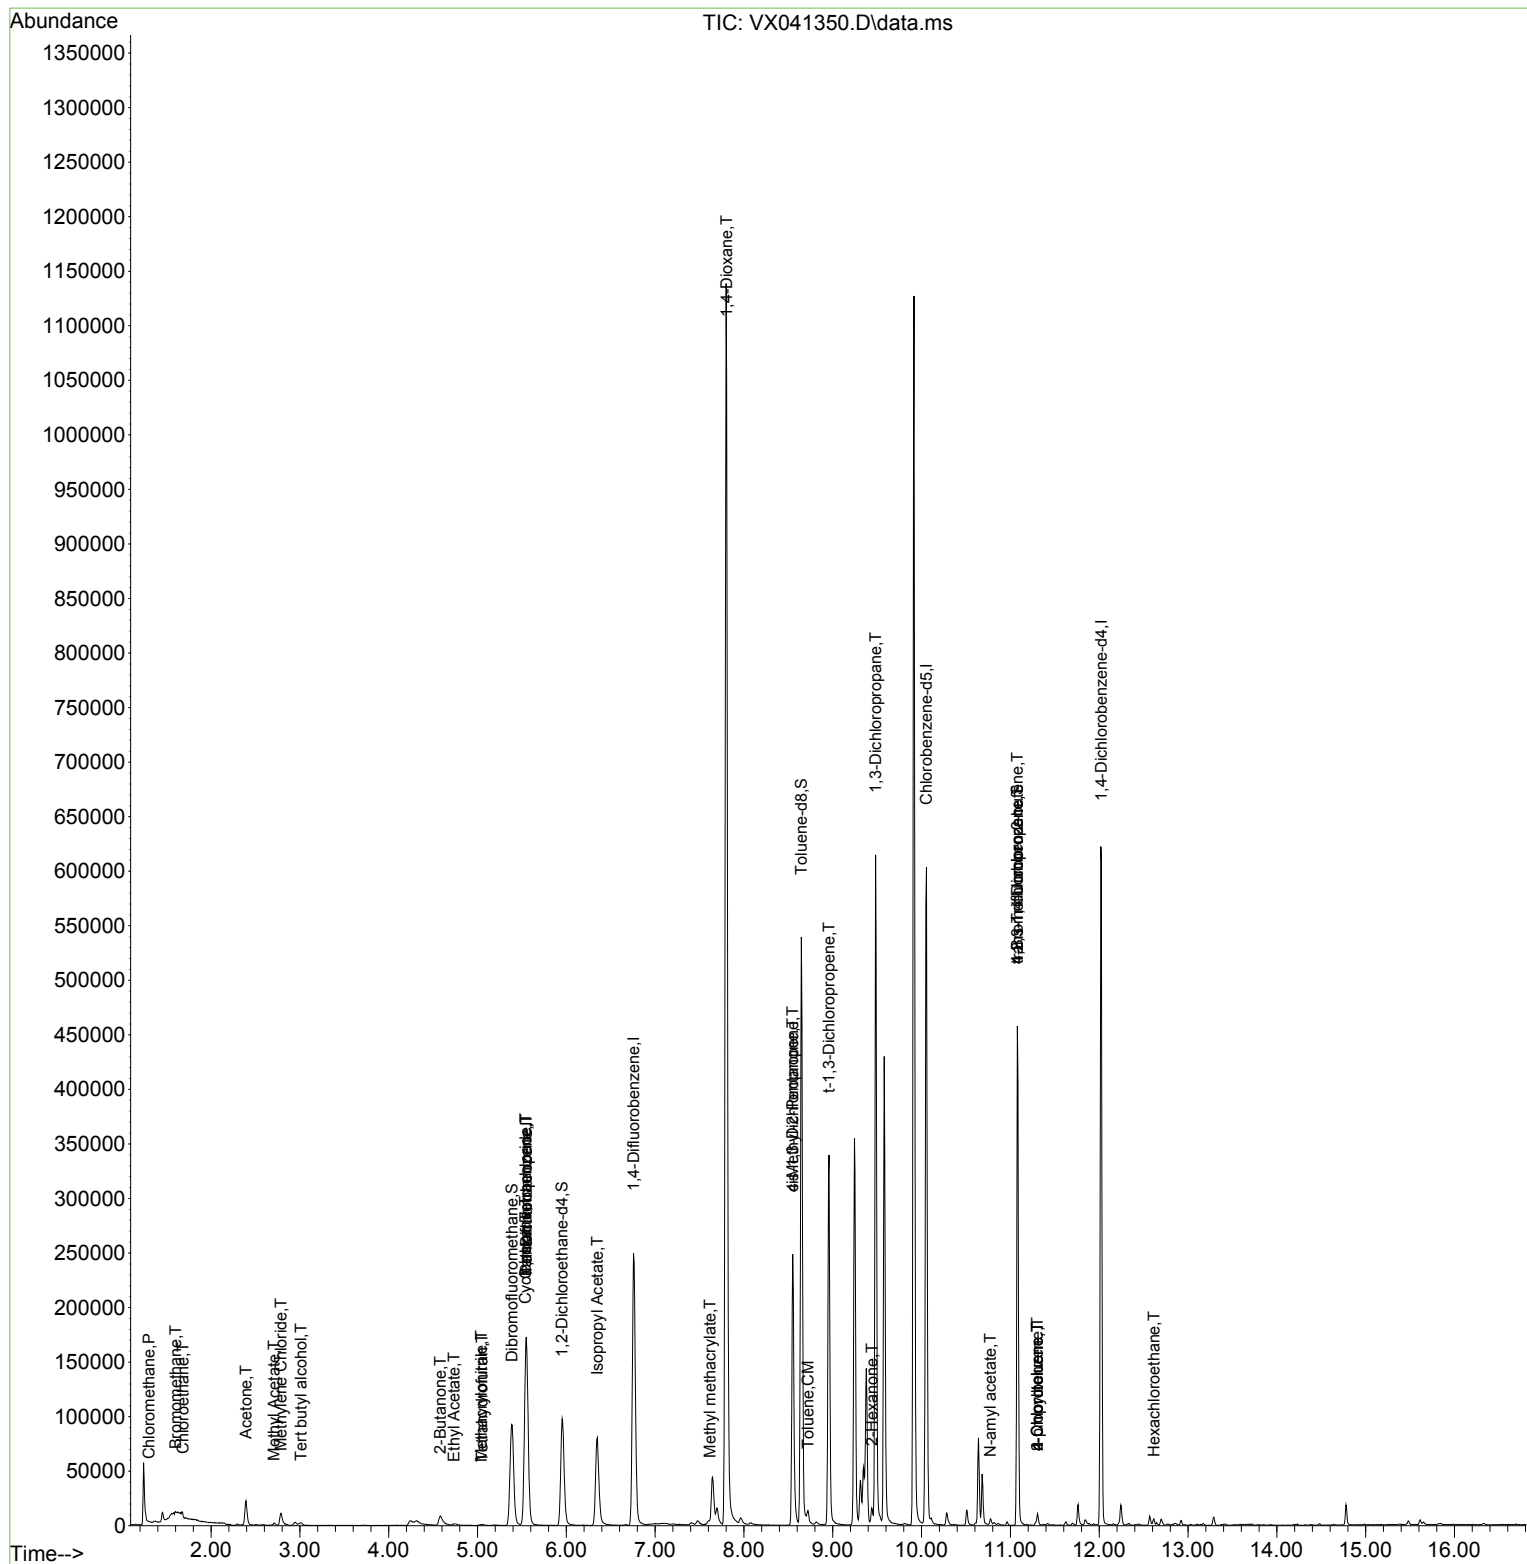




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 185973
Ion Ratio Lower Upper
168 100
99 47.7 56.6 85.0#

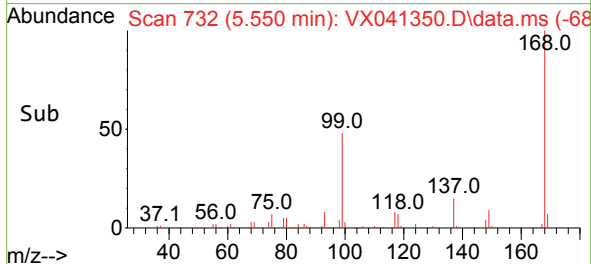

#3
Chloromethane
Concen: 0.242 ug/l
RT: 1.301 min Scan# 35
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 50 Resp: 383
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#


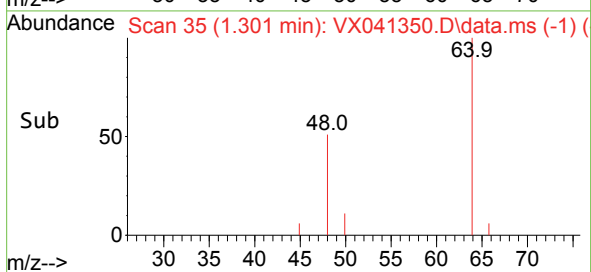




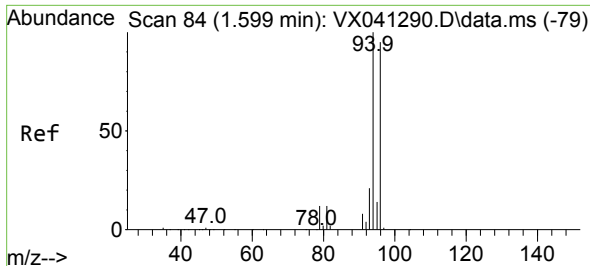

#5
Bromomethane
Concen: 0.422 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 94 Resp: 399
Ion Ratio Lower Upper
94 100
96 86.5 74.6 111.8

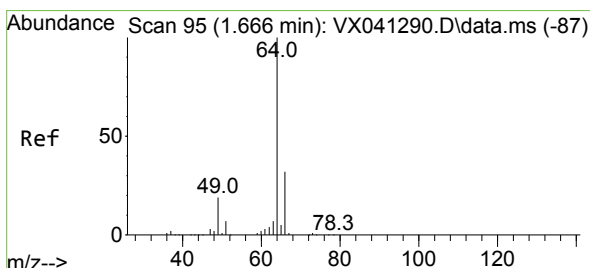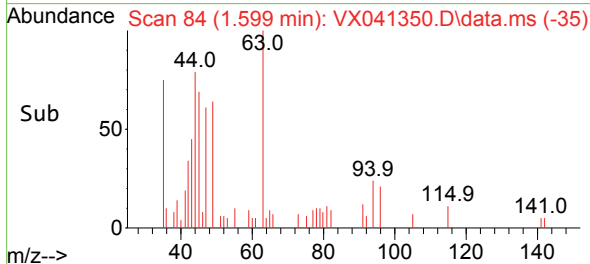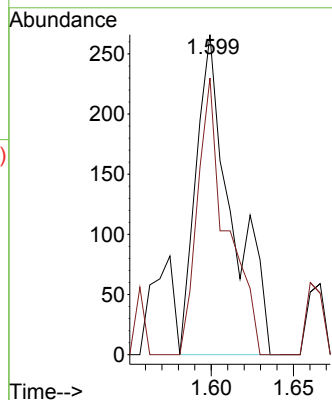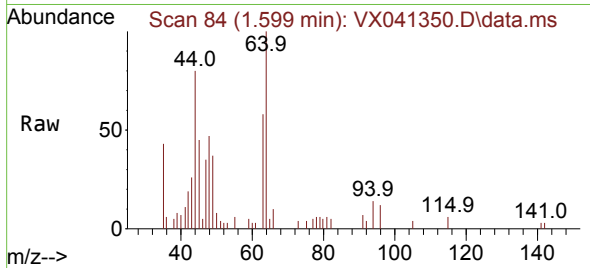

#6
Chloroethane
Concen: 1.107 ug/l
RT: 1.685 min Scan# 98
Delta R.T. 0.018 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 64 Resp: 775
Ion Ratio Lower Upper
64 100
66 4.6 25.1 37.7#

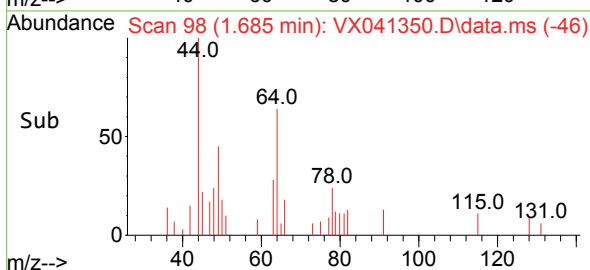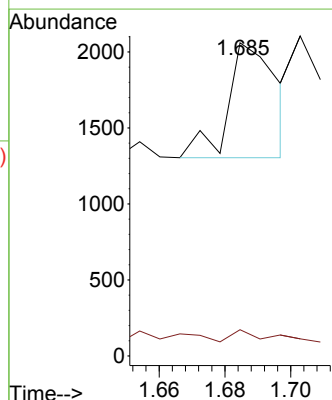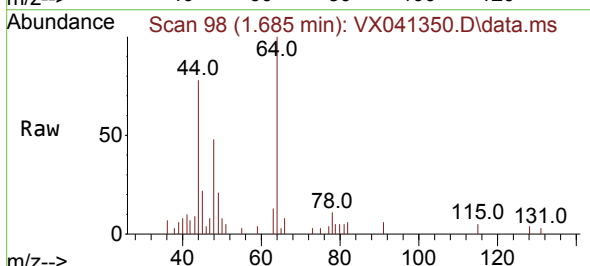



#11

Tert butyl alcohol

Concen: 9.037 ug/l

RT: 3.014 min Scan# 31

Delta R.T. -0.006 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 59 Resp: 3662

Ion Ratio Lower Upper

59 100

57 10.7 6.0 9.0#

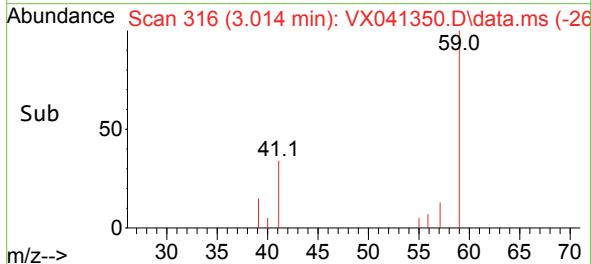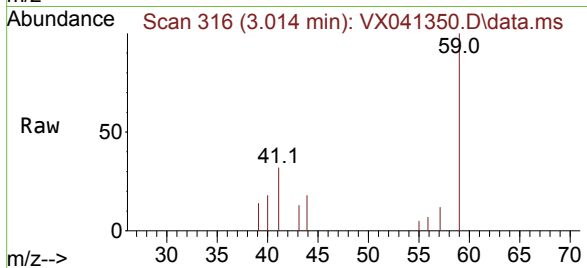

#16

Acetone

Concen: 25.849 ug/l

RT: 2.392 min Scan# 214

Delta R.T. -0.000 min

Lab File: VX041350.D




Acq: 02 May 2024 13:50


Tgt Ion: 43 Resp: 26172

Ion Ratio Lower Upper

43 100

58 31.3 21.9 32.9


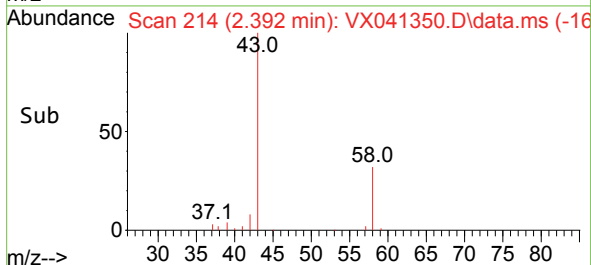
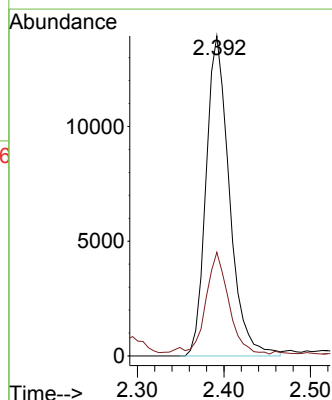
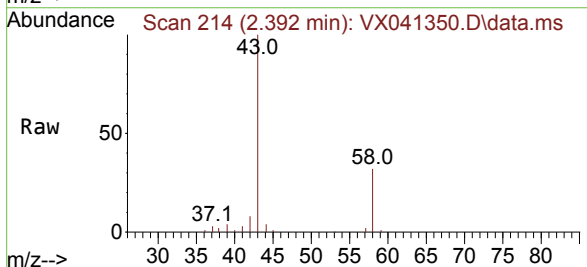




#18
Methyl Acetate
Concen: 1.237 ug/l
RT: 2.709 min Scan# 20
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 2563
Ion Ratio Lower Upper
43 100
74 27.5 17.8 26.8#

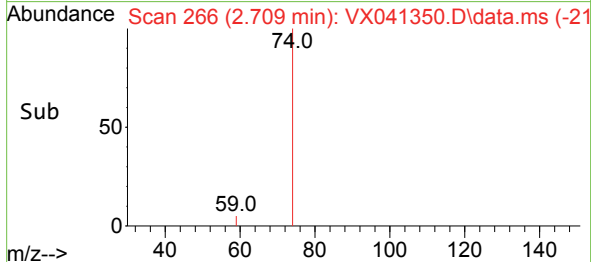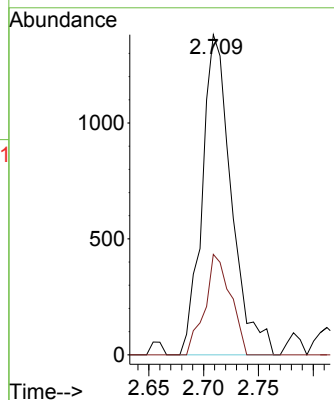

#20
Methylene Chloride
Concen: 3.639 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 84 Resp: 6396
Ion Ratio Lower Upper
84 100
49 115.2 103.6 155.4
51 36.4 33.8 50.6
86 71.1 49.4 74.0


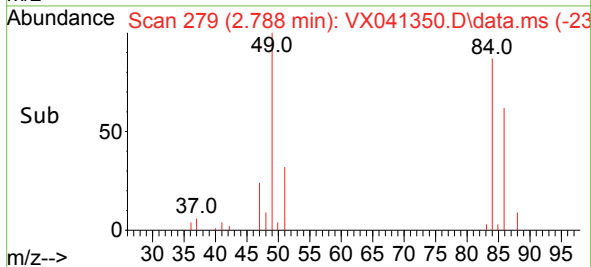
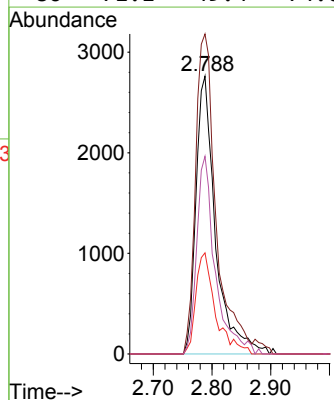
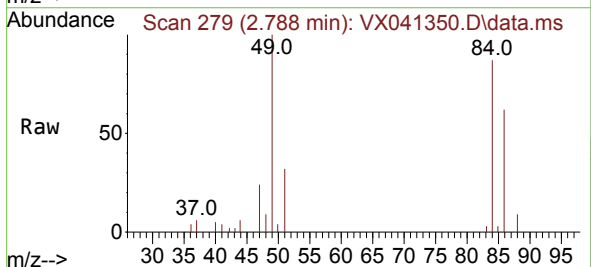


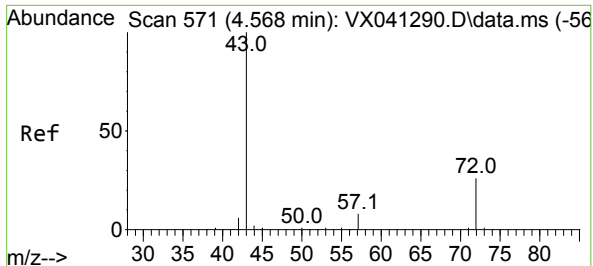

#25
2-Butanone
Concen: 14.587 ug/l
RT: 4.580 min Scan# 51
Delta R.T. 0.012 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 19114
Ion Ratio Lower Upper
43 100
72 26.9 19.4 29.2

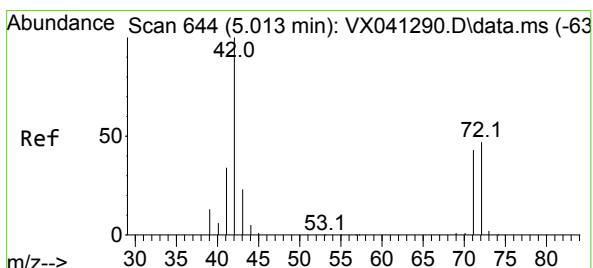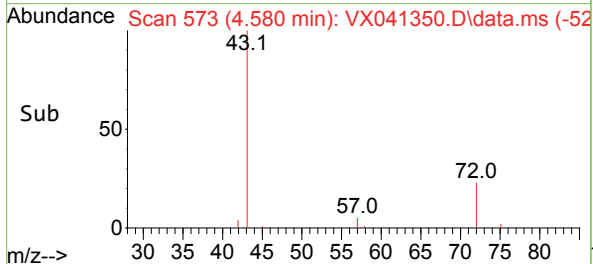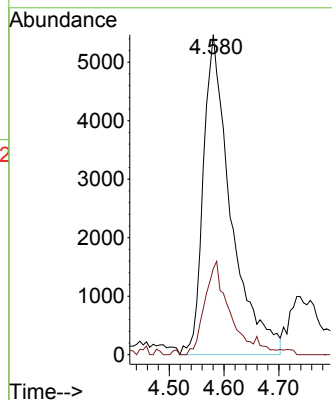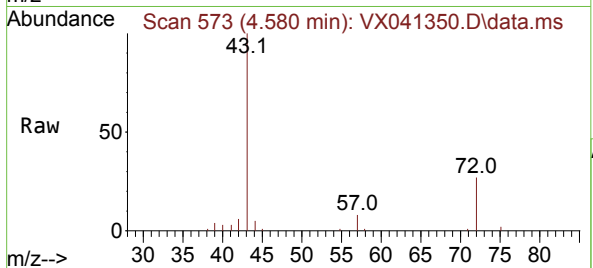

#29
Tetrahydrofuran
Concen: 1.120 ug/l
RT: 5.050 min Scan# 650
Delta R.T. 0.037 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50


Tgt Ion: 42 Resp: 960
Ion Ratio Lower Upper
42 100
72 15.4 34.2 51.4#
71 15.8 32.2 48.2#

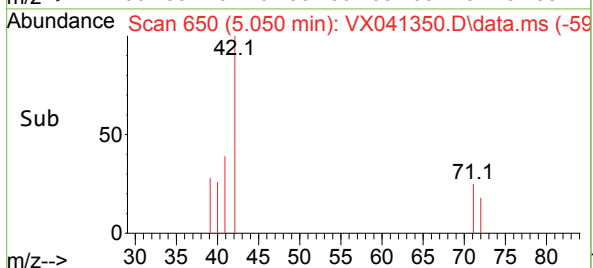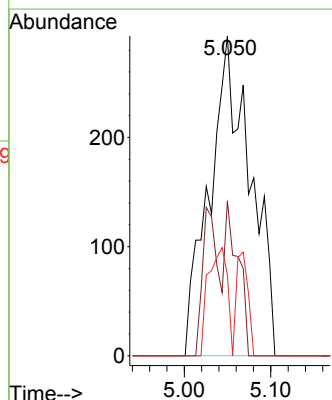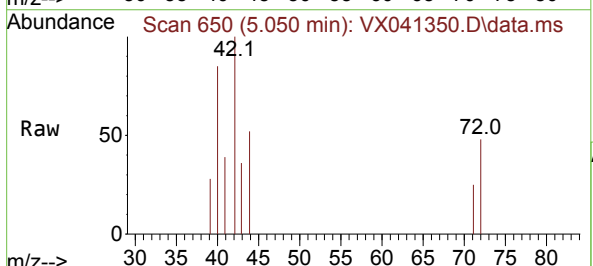



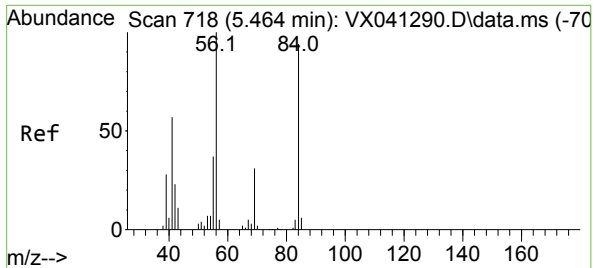


#31
Cyclohexane
Concen: 1.335 ug/l
RT: 5.538 min Scan# 718
Delta R.T. 0.073 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Instrument :
MSVOA_X
ClientSampleId :



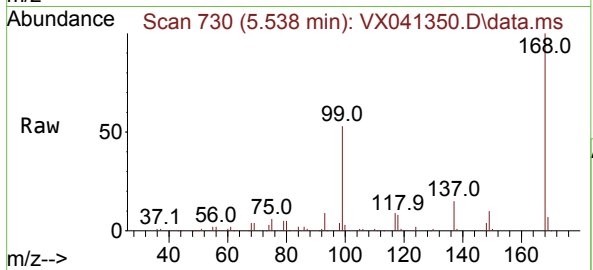



Tgt Ion: 56 Resp: 3261
Ion Ratio Lower Upper
56 100
69 182.5 23.4 35.2#
84 95.8 65.9 98.9

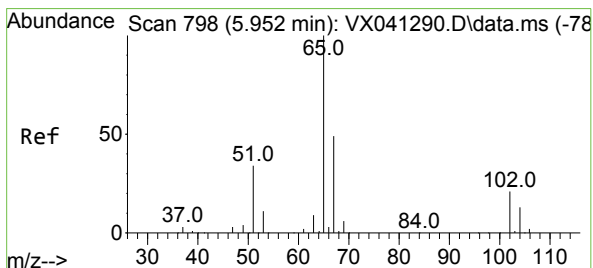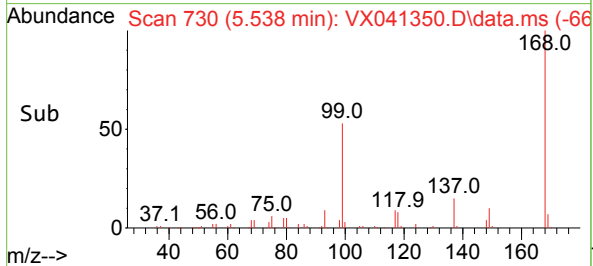

#33
1,2-Dichloroethane-d4
Concen: 48.559 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 65 Resp: 98312
Ion Ratio Lower Upper
65 100
67 50.9 0.0 100.2


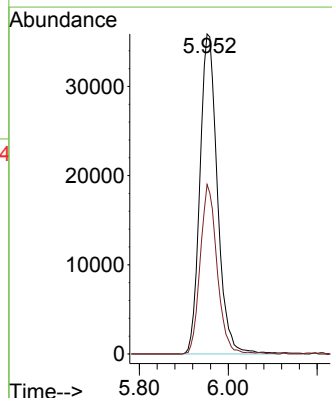
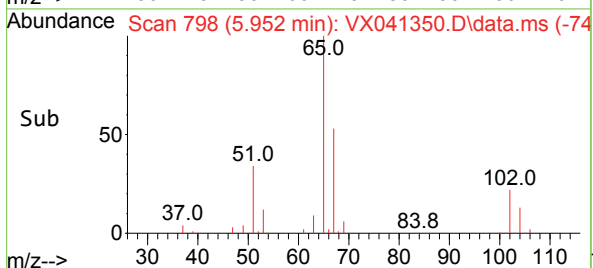
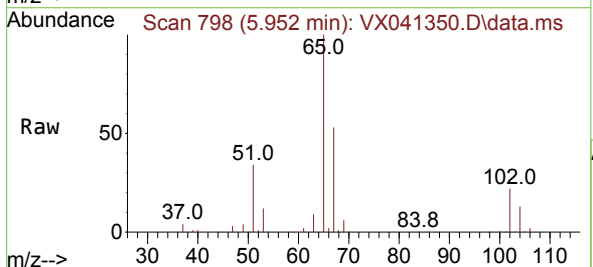


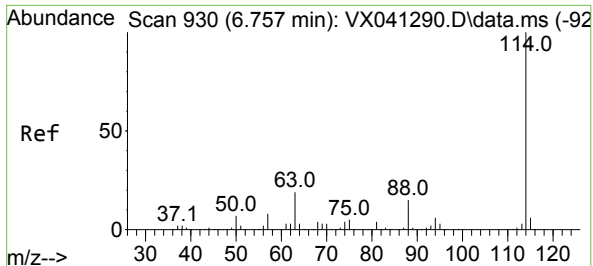

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:114 Resp: 267979
Ion Ratio Lower Upper
114 100
63 18.5 0.0 45.0
88 14.9 0.0 36.6

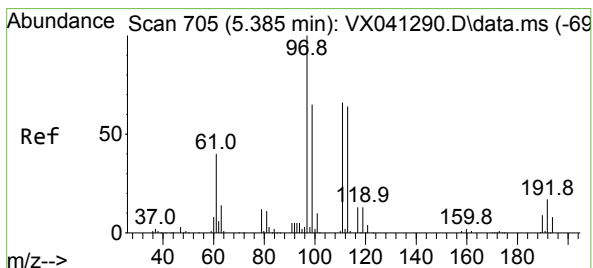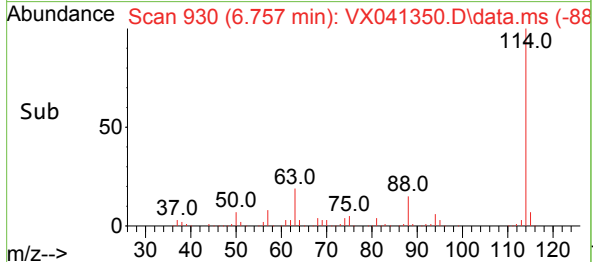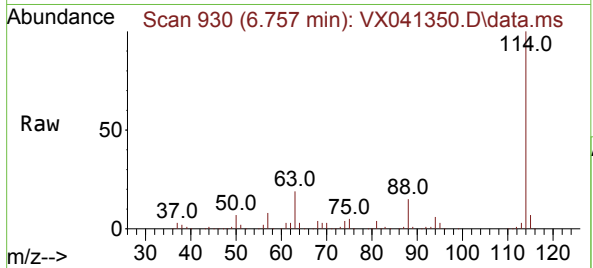

#35
Dibromofluoromethane
Concen: 43.802 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion:113 Resp: 79545
Ion Ratio Lower Upper
113 100
111 102.7 82.9 124.3
192 25.4 13.3 19.9#


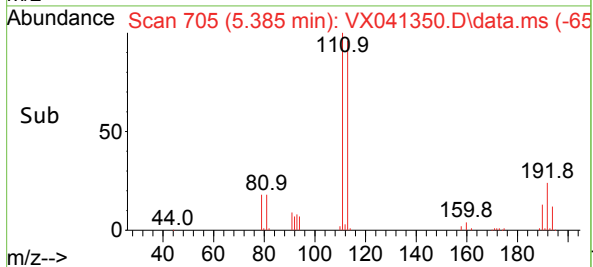

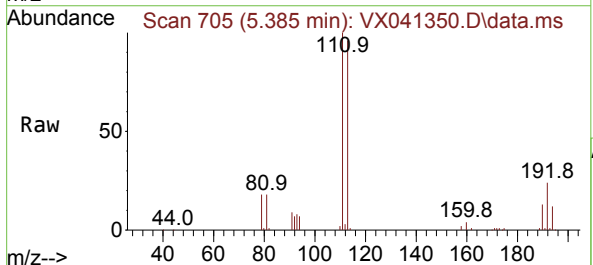




#36
1,1-Dichloropropene
Concen: 5.300 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 11508
Ion Ratio Lower Upper
75 100
110 9.3 17.0 50.9#
77 0.0 24.7 37.1#

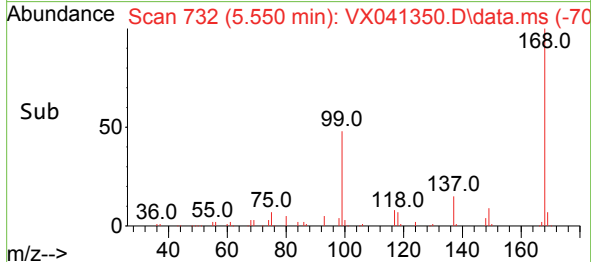

#37
Ethyl Acetate
Concen: 1.172 ug/l
RT: 4.733 min Scan# 598
Delta R.T. 0.012 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50


Tgt Ion: 43 Resp: 3176
Ion Ratio Lower Upper
43 100
61 12.2 10.6 16.0
70 8.1 8.3 12.5#

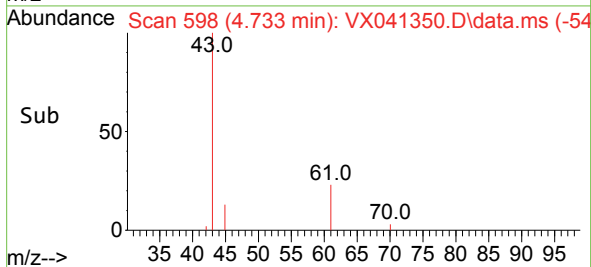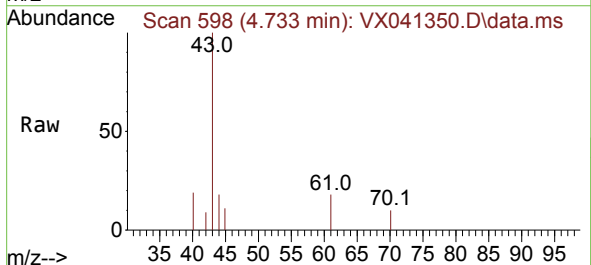






#38
Carbon Tetrachloride
Concen: 6.565 ug/l
RT: 5.544 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:117 Resp: 16331
Ion Ratio Lower Upper
117 100
119 5.1 78.2 117.2#
121 0.0 24.4 36.6#



#41
Methacrylonitrile
Concen: 0.253 ug/l
RT: 5.044 min Scan# 649
Delta R.T. 0.116 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 41 Resp: 353
Ion Ratio Lower Upper
41 100
39 59.5 45.2 67.8
67 0.0 52.6 78.8#
52 0.0 22.7 34.1#

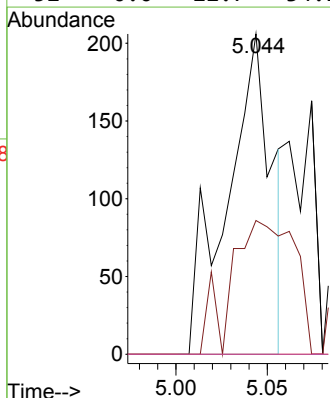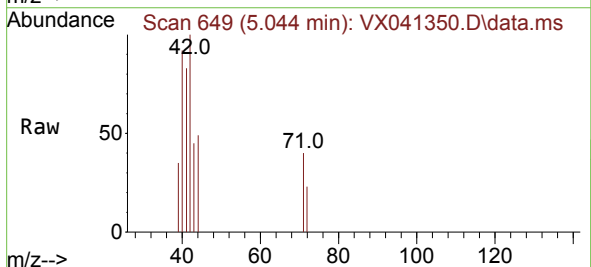



#43

Isopropyl Acetate

Concen: 28.535 ug/l

RT: 6.348 min Scan# 81

Delta R.T. 0.000 min


Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 43 Resp: 116245

Ion Ratio Lower Upper

43 100

61 19.5 15.2 22.8

87 13.2 9.8 14.6



#48

Methyl methacrylate

Concen: 2.417 ug/l

RT: 7.616 min Scan# 1071

Delta R.T. -0.079 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50




Tgt Ion: 41 Resp: 4514


Ion Ratio Lower Upper

41 100

69 0.0 59.2 88.8#

39 0.0 47.7 71.5#

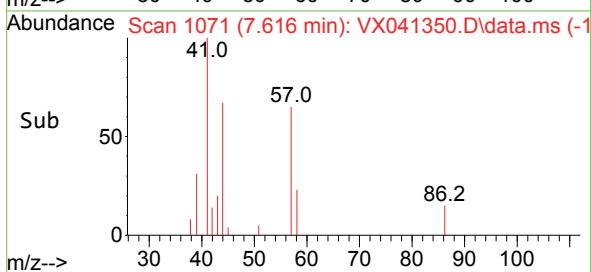



#49

1,4-Dioxane

Concen: 3.517 ug/l

RT: 7.805 min Scan# 1102

Delta R.T. 0.134 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 88 Resp: 142

Ion Ratio Lower Upper

88 100

43 768666.9 0.0 0.0#

58 3215.5 60.1 90.1#



#50

Toluene-d8

Concen: 54.856 ug/l

RT: 8.647 min Scan# 1240

Delta R.T. 0.000 min

Lab File: VX041350.D




Acq: 02 May 2024 13:50


Tgt Ion: 98 Resp: 315301

Ion Ratio Lower Upper

98 100

100 67.1 53.1 79.7


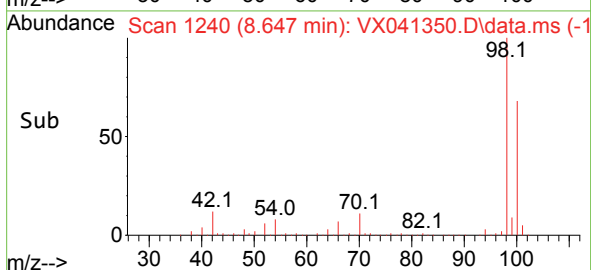
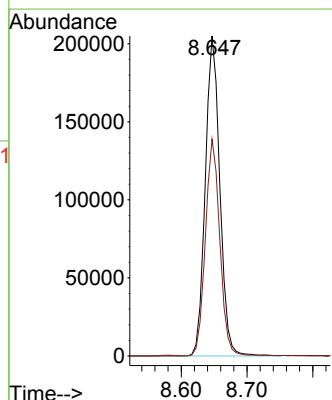





#51
4-Methyl-2-Pentanone
Concen: 37.055 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.030 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 90581
Ion Ratio Lower Upper
43 100
58 8.0 30.4 45.6#

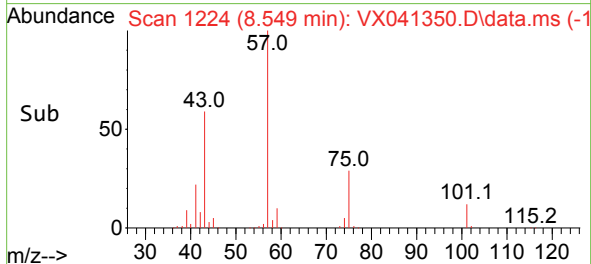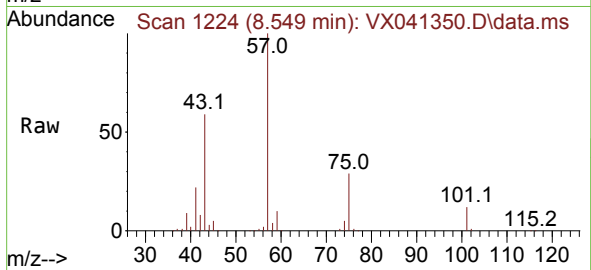

#52
Toluene
Concen: 0.935 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 92 Resp: 3828
Ion Ratio Lower Upper
92 100
91 169.7 134.2 201.2


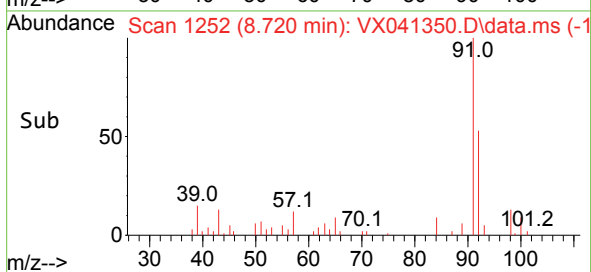

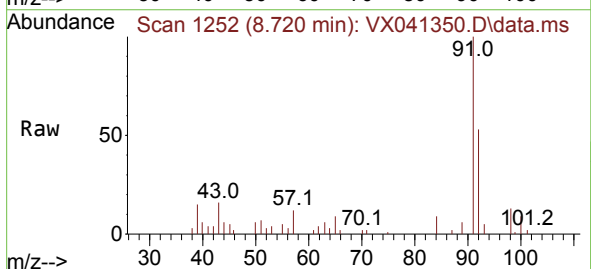




#53
 t-1,3-Dichloropropene
 Concen: 0.393 ug/l
 RT: 8.958 min Scan# 11
 Delta R.T. -0.018 min
 Lab File: VX041350.D
 Acq: 02 May 2024 13:50




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 826
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.7 38.5#

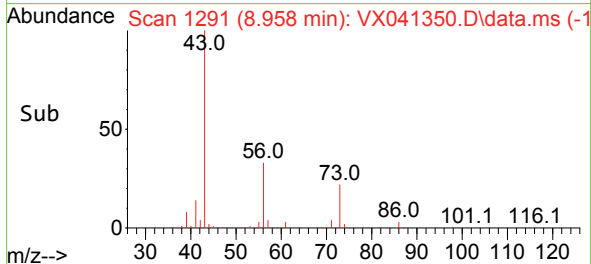

#54
 cis-1,3-Dichloropropene
 Concen: 17.689 ug/l
 RT: 8.549 min Scan# 1224
 Delta R.T. 0.183 min
 Lab File: VX041350.D
 Acq: 02 May 2024 13:50

Tgt Ion: 75 Resp: 41260
 Ion Ratio Lower Upper
 75 100
 77 0.7 25.3 37.9#
 39 31.3 46.7 70.1#

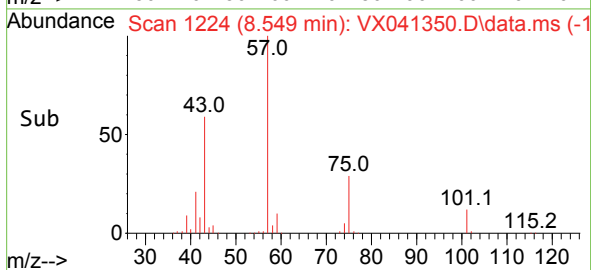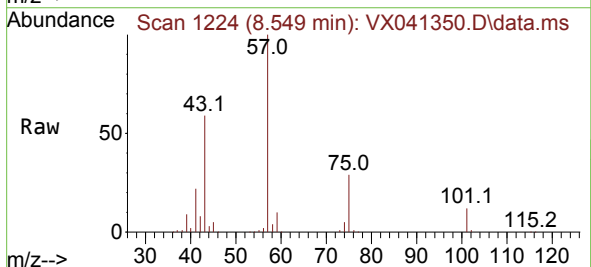



#57

1,3-Dichloropropane

Concen: 2.109 ug/l

RT: 9.482 min Scan# 1377

Delta R.T. 0.177 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 5552

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

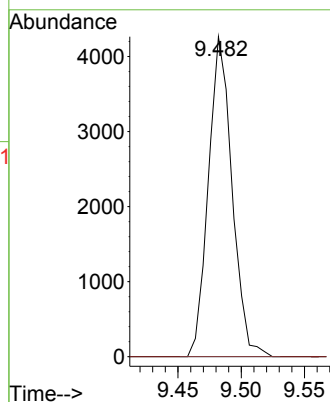

#59

2-Hexanone

Concen: 4.605 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VX041350.D




Acq: 02 May 2024 13:50


Tgt Ion: 43 Resp: 9001

Ion Ratio Lower Upper

43 100

58 51.3 26.2 78.5

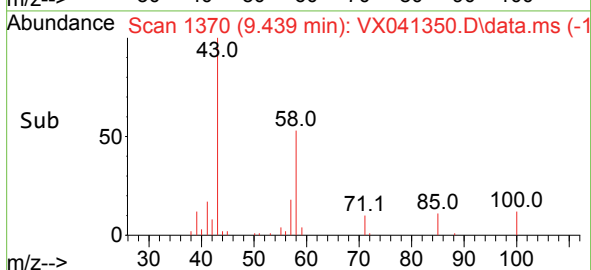



#62

4-Bromofluorobenzene

Concen: 49.572 ug/l

RT: 11.079 min Scan# 1

Delta R.T. 0.000 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 95 Resp: 110298

Ion Ratio Lower Upper

95 100

174 99.0 0.0 135.6

176 96.5 0.0 131.0

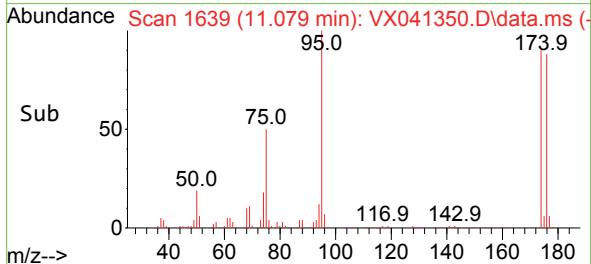

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50




Tgt Ion: 117 Resp: 282720


Ion Ratio Lower Upper

117 100

82 49.9 46.2 69.4


119 32.7 25.5 38.3

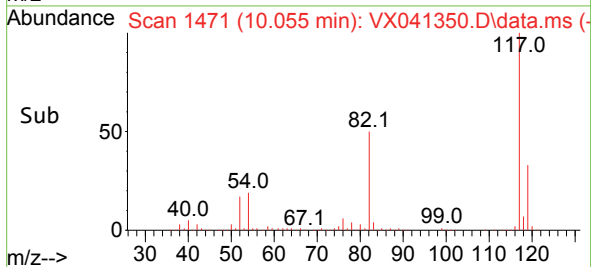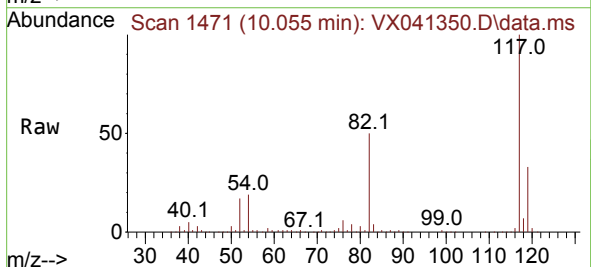






#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 12.024 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VX041350.D
 Acq: 02 May 2024 13:50


Instrument :
 MSVOA_X
 ClientSampleId :

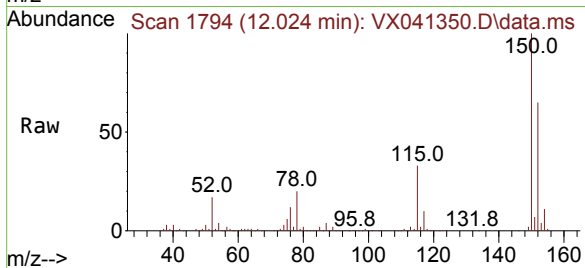



Tgt Ion:152 Resp: 143605
 Ion Ratio Lower Upper
 152 100
 115 54.0 43.3 129.9
 150 156.4 0.0 345.0




#74
 N-ethyl acetate
 Concen: 0.795 ug/l
 RT: 10.774 min Scan# 1589
 Delta R.T. -0.067 min
 Lab File: VX041350.D
 Acq: 02 May 2024 13:50

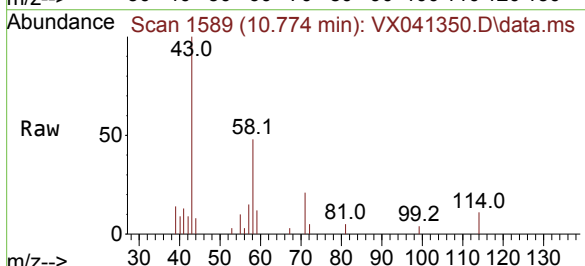

Tgt Ion: 43 Resp: 3044
 Ion Ratio Lower Upper
 43 100
 70 0.0 32.9 49.3#
 55 14.3 19.3 28.9#
 61 0.0 18.8 28.2#

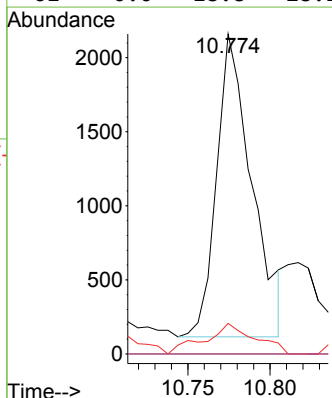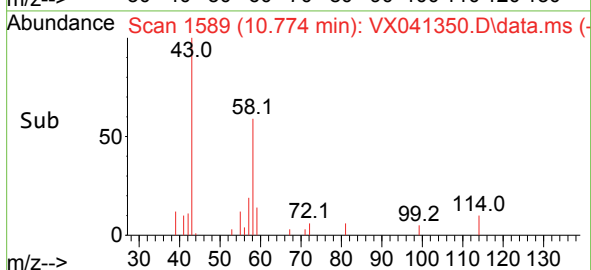



#76

1,2,3-Trichloropropane

Concen: 23.710 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.158 min

Lab File: VX041350.D

Acq: 02 May 2024 13:50

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 75 Resp: 55489

Ion Ratio Lower Upper

75 100

77 1.0 19.1 57.5#

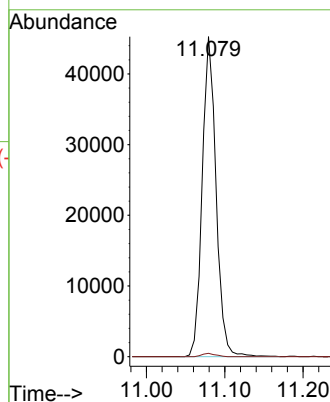

#78

n-propylbenzene

Concen: 0.689 ug/l

RT: 11.305 min Scan# 1676

Delta R.T. 0.000 min

Lab File: VX041350.D




Acq: 02 May 2024 13:50


Tgt Ion: 91 Resp: 6346

Ion Ratio Lower Upper

91 100

120 24.4 11.5 34.4


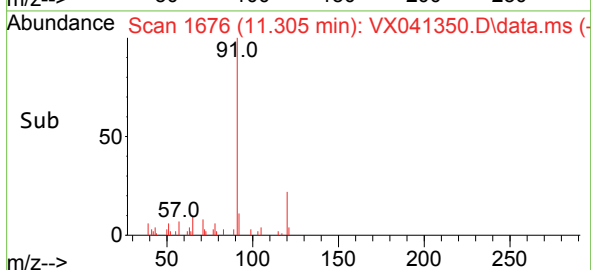






#79
2-Chlorotoluene
Concen: 1.070 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.061 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 91 Resp: 6346
Ion Ratio Lower Upper
91 100
126 0.0 16.3 48.8#

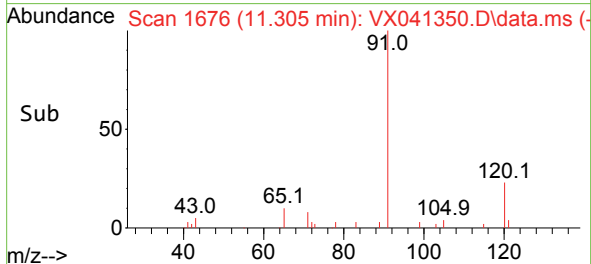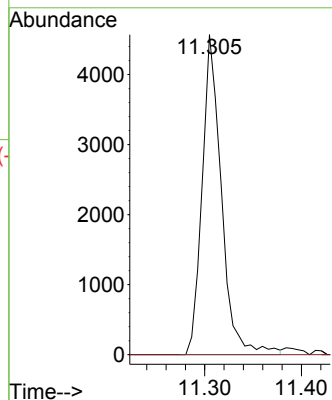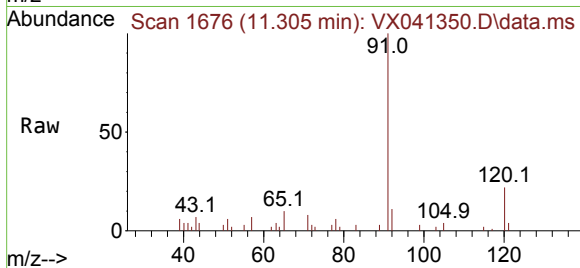

#81
trans-1,4-Dichloro-2-butene
Concen: 64.583 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 75 Resp: 55489
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#


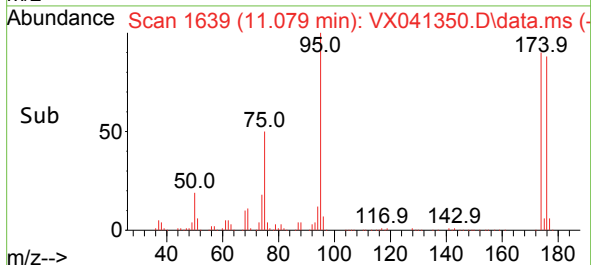
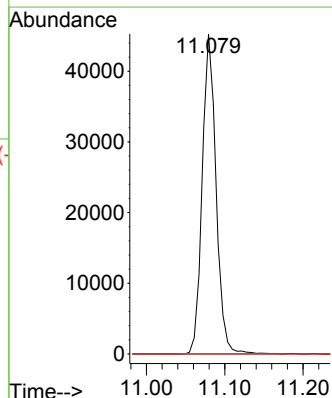
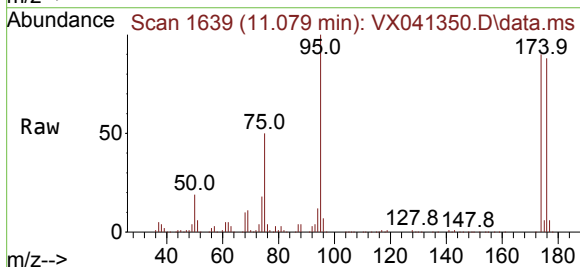




#82
4-Chlorotoluene
Concen: 0.942 ug/l
RT: 11.305 min Scan# 11
Delta R.T. -0.146 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 91 Resp: 6346
Ion Ratio Lower Upper
91 100
126 0.0 14.2 42.6#



#90
Hexachloroethane
Concen: 0.235 ug/l
RT: 12.616 min Scan# 1891
Delta R.T. 0.079 min
Lab File: VX041350.D
Acq: 02 May 2024 13:50

Tgt Ion: 117 Resp: 309
Ion Ratio Lower Upper
117 100
201 0.0 32.9 98.6#

