

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050225\
 Data File : VX046023.D
 Acq On : 02 May 2025 13:28
 Operator : JC/MD
 Sample : Q1925-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0068

Quant Time: May 02 23:14:43 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	67376	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	130527	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	124567	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	56427	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	65659	53.289	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 106.580%	
35) Dibromofluoromethane	5.385	113	47275	51.048	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.100%	
50) Toluene-d8	8.647	98	164948	51.029	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.060%	
62) 4-Bromofluorobenzene	11.079	95	65875	55.949	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 111.900%	


Target Compounds				Qvalue		
11) Tert butyl alcohol	2.983	59	1476	8.914	ug/l #	89
13) Acrolein	2.239	56	139	0.610	ug/l #	48
16) Acetone	2.386	43	30293	59.874	ug/l	98
17) Carbon Disulfide	2.501	76	1281	0.641	ug/l #	76
18) Methyl Acetate	2.703	43	2138	1.835	ug/l	97
20) Methylene Chloride	2.782	84	6742	7.118	ug/l	96
25) 2-Butanone	4.580	43	4350	5.874	ug/l #	82
29) Tetrahydrofuran	5.050	42	453	0.943	ug/l #	39
36) 1,1-Dichloropropene	5.544	75	6570	5.254	ug/l #	49
38) Carbon Tetrachloride	5.544	117	8061	5.965	ug/l #	14
40) Benzene	6.037	78	35012	9.168	ug/l	93
42) 1,2-Dichloroethane	6.031	62	373	0.236	ug/l #	78
43) Isopropyl Acetate	6.348	43	11832	4.954	ug/l	98
48) Methyl methacrylate	7.604	41	1683	1.365	ug/l #	15
51) 4-Methyl-2-Pentanone	8.549	43	39562	24.988	ug/l #	48
52) Toluene	8.714	92	22940	9.927	ug/l	99
53) t-1,3-Dichloropropene	8.951	75	212	2.433	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	13594	9.903	ug/l #	67
55) 1,1,2-Trichloroethane	9.012	97	204	0.222	ug/l #	14
57) 1,3-Dichloropropane	9.482	76	1339	0.835	ug/l #	42
59) 2-Hexanone	9.378	43	8346	7.119	ug/l #	28
67) Ethyl Benzene	10.195	91	3520	0.738	ug/l	94
68) m/p-Xylenes	10.299	106	6961	4.015	ug/l	95
69) o-Xylene	10.640	106	5967	3.493	ug/l	96
70) Styrene	10.658	104	2051	0.728	ug/l #	54
76) 1,2,3-Trichloropropane	11.079	75	36947	26.843	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.451	105	2506	0.670	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	36947	91.103	ug/l #	1
83) tert-Butylbenzene	11.756	119	802	0.217	ug/l #	41
84) 1,2,4-Trimethylbenzene	11.750	105	14131	3.767	ug/l	68
85) sec-Butylbenzene	11.750	105	14131	3.109	ug/l #	58
95) Naphthalene	13.774	128	357676	91.361	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050225\
Data File : VX046023.D
Acq On : 02 May 2025 13:28
Operator : JC/MD
Sample : Q1925-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068

Quant Time: May 02 23:14:43 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration



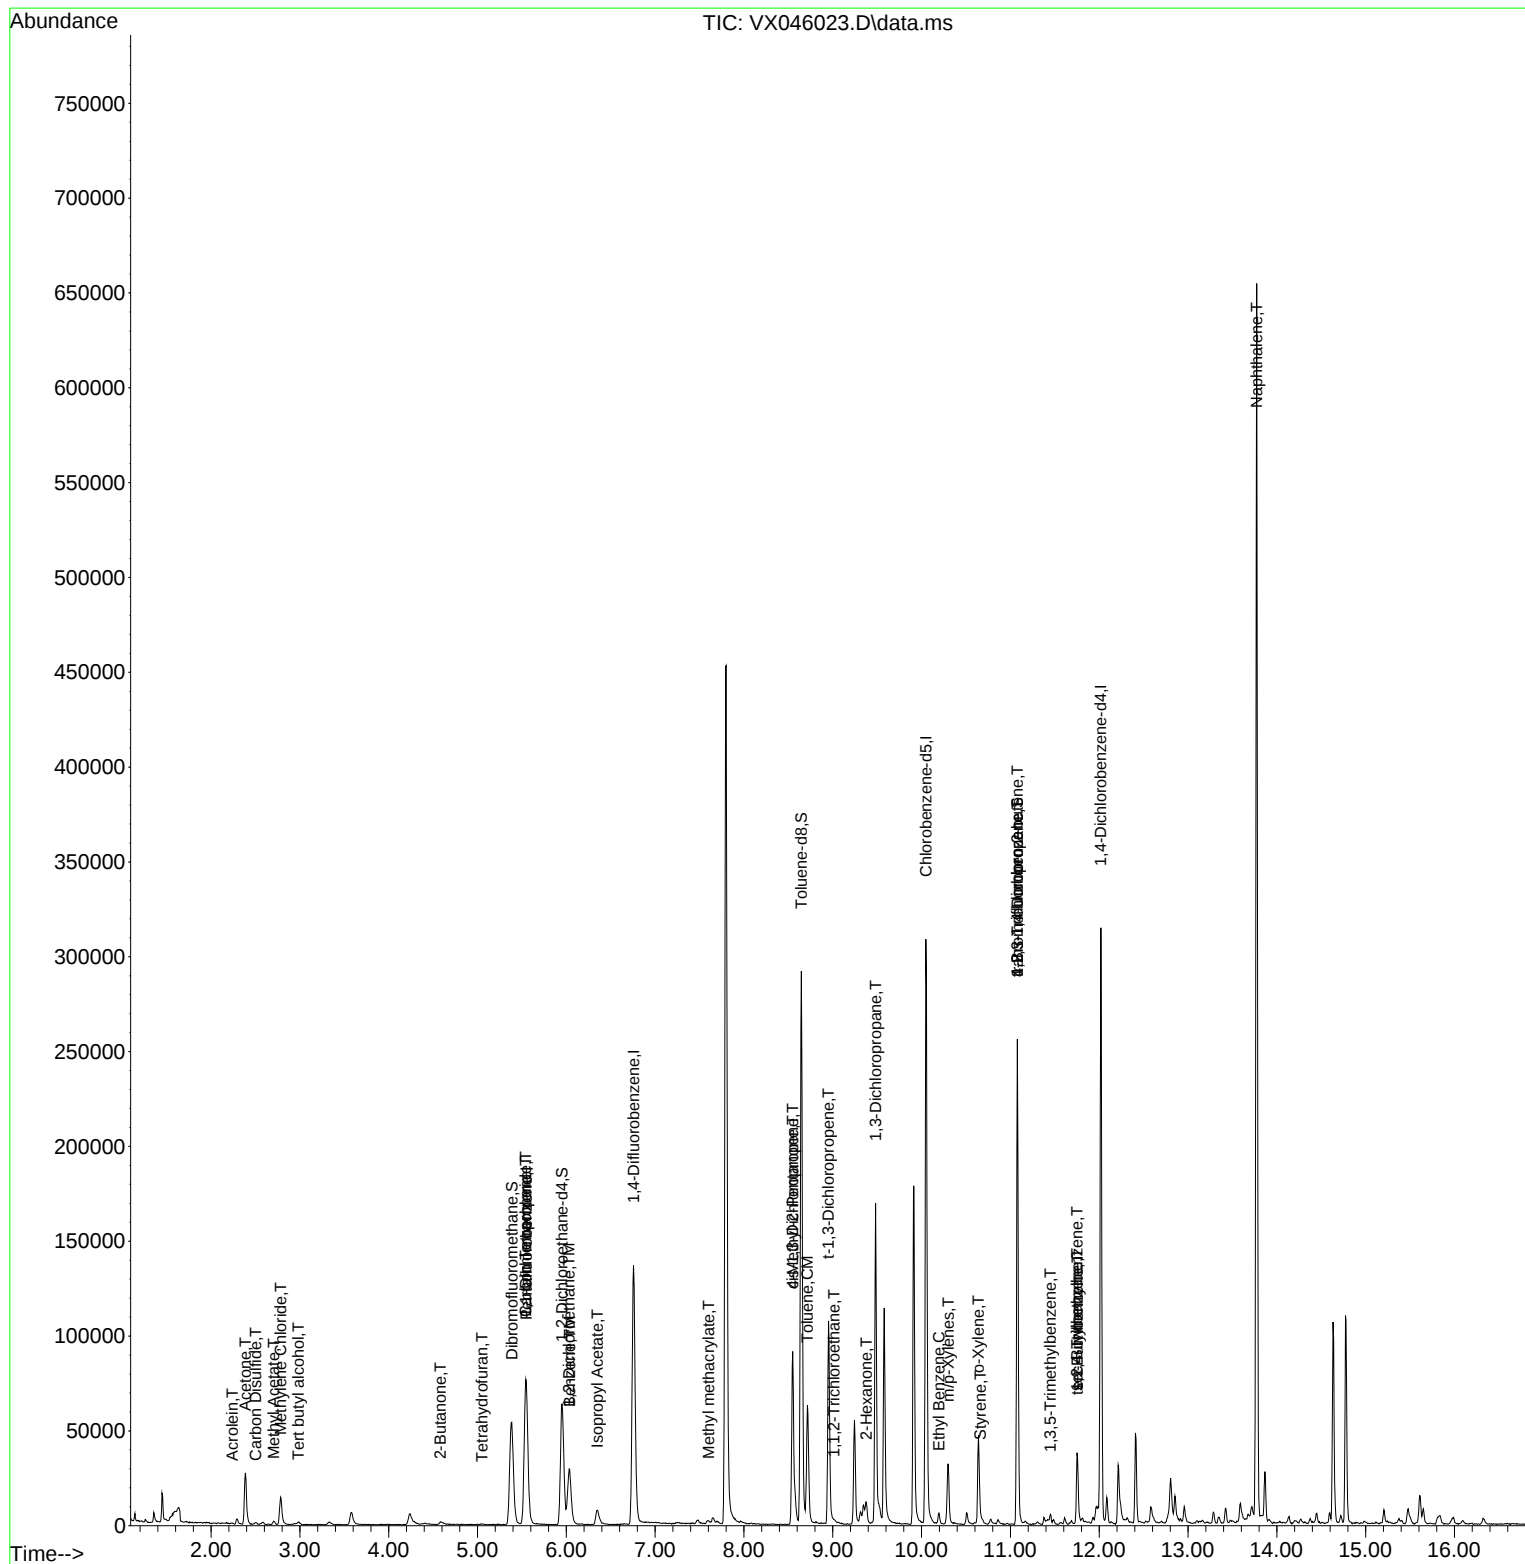




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion:168 Resp: 67376
Ion Ratio Lower Upper
168 100
99 68.8 52.3 78.5

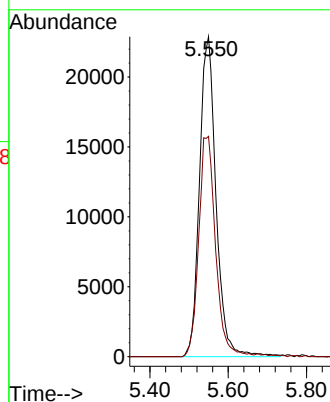

#11
Tert butyl alcohol
Concen: 8.914 ug/l
RT: 2.983 min Scan# 311
Delta R.T. 0.006 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 59 Resp: 1476
Ion Ratio Lower Upper
59 100
57 6.7 8.6 12.8#


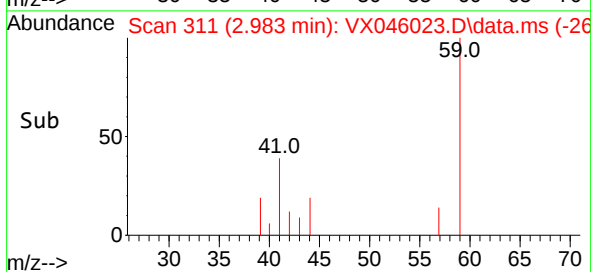
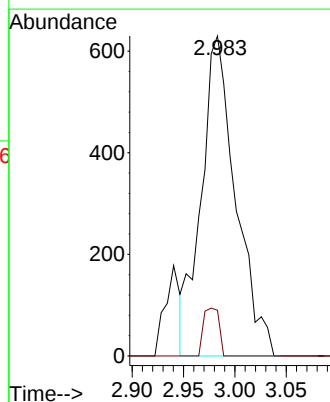





#13
Acrolein
Concen: 0.610 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 56 Resp: 139
Ion Ratio Lower Upper
56 100
55 112.9 56.2 84.2#

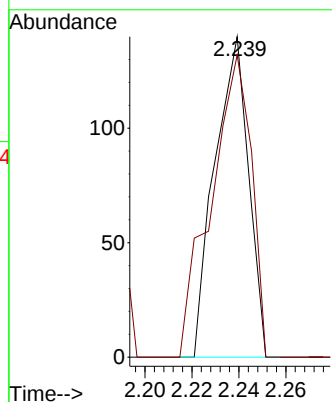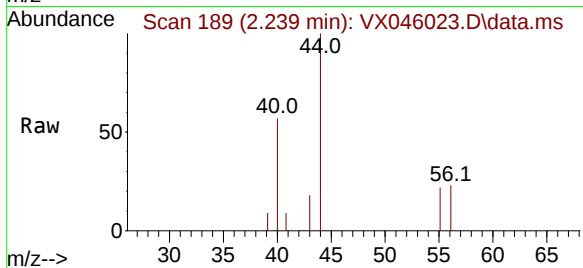

#16
Acetone
Concen: 59.874 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 43 Resp: 30293
Ion Ratio Lower Upper
43 100
58 27.0 22.3 33.5

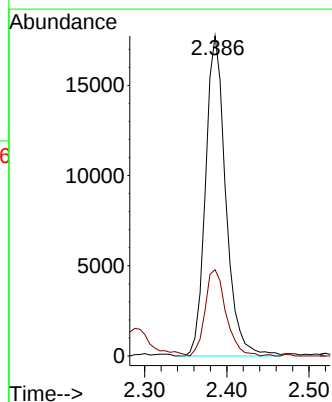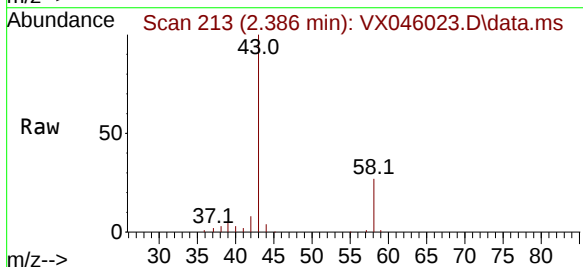



#17

Carbon Disulfide

Concen: 0.641 ug/l

RT: 2.501 min Scan# 21

Delta R.T. -0.006 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0068

Tgt Ion: 76 Resp: 1281

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.6#

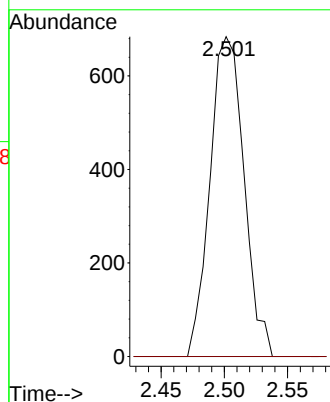

#18

Methyl Acetate

Concen: 1.835 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX046023.D




Acq: 02 May 2025 13:28


Tgt Ion: 43 Resp: 2138

Ion Ratio Lower Upper

43 100

74 20.6 17.5 26.3


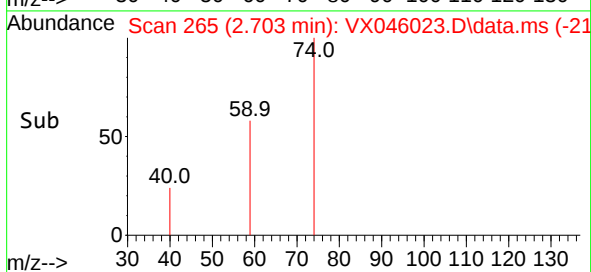
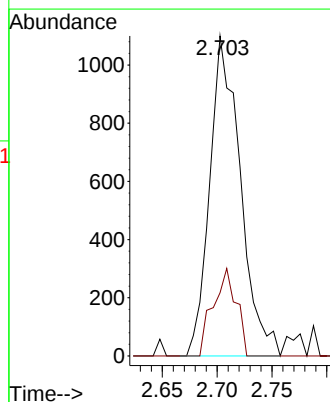





#20
Methylene Chloride
Concen: 7.118 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion:	84	Resp:	6742
Ion	Ratio	Lower	Upper
84	100		
49	128.8	107.5	161.3
51	46.9	33.0	49.6
86	63.1	50.1	75.1



#25
2-Butanone
Concen: 5.874 ug/l
RT: 4.580 min Scan# 573
Delta R.T. 0.024 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion:	43	Resp:	4350
Ion	Ratio	Lower	Upper
43	100		
72	32.0	18.6	28.0


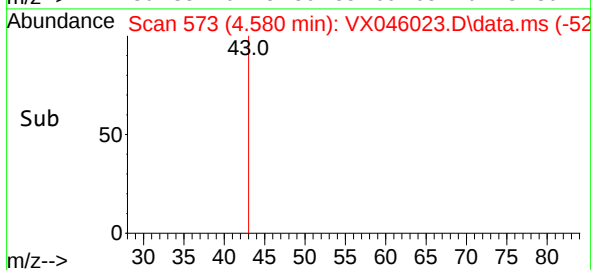






#29
Tetrahydrofuran
Concen: 0.943 ug/l
RT: 5.050 min Scan# 61
Delta R.T. 0.049 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 42 Resp: 453
Ion Ratio Lower Upper
42 100
72 5.5 33.4 50.0#
71 0.0 31.4 47.0#

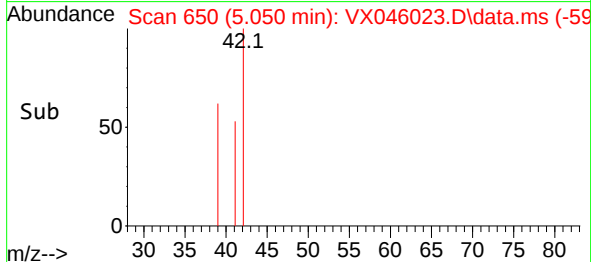

#33
1,2-Dichloroethane-d4
Concen: 53.289 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 65 Resp: 65659
Ion Ratio Lower Upper
65 100
67 48.8 0.0 99.0



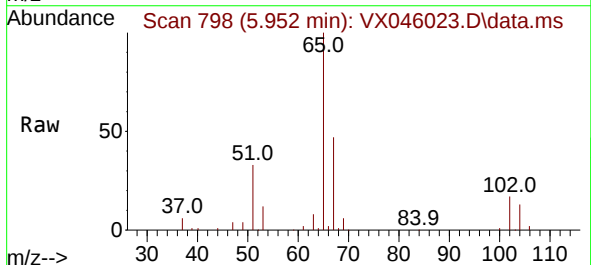




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion:114 Resp: 130527
Ion Ratio Lower Upper
114 100
63 24.9 0.0 46.8
88 17.5 0.0 35.4

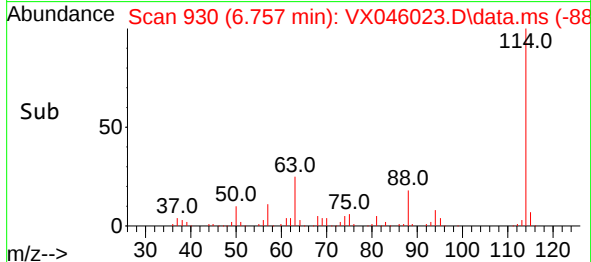

#35
Dibromofluoromethane
Concen: 51.048 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.006 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion:113 Resp: 47275
Ion Ratio Lower Upper
113 100
111 102.8 81.8 122.6
192 17.5 13.8 20.6




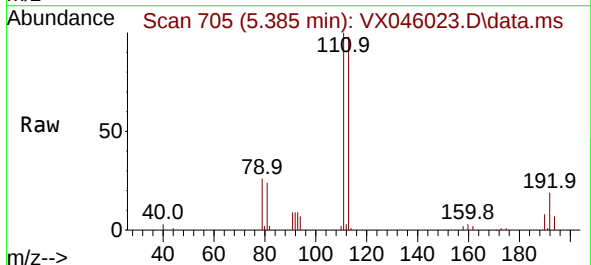




#36
1,1-Dichloropropene
Concen: 5.254 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.140 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 75 Resp: 6570
Ion Ratio Lower Upper
75 100
110 7.9 16.9 50.6#
77 0.0 25.0 37.4#

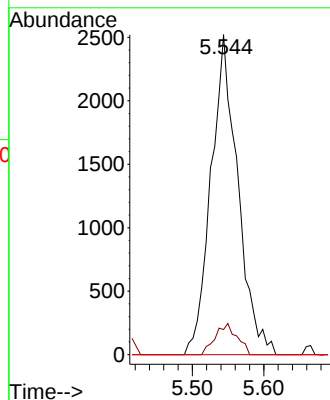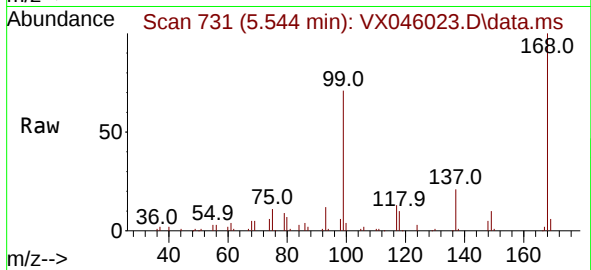

#38
Carbon Tetrachloride
Concen: 5.965 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.128 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 117 Resp: 8061
Ion Ratio Lower Upper
117 100
119 2.3 76.9 115.3#
121 0.0 24.2 36.2#

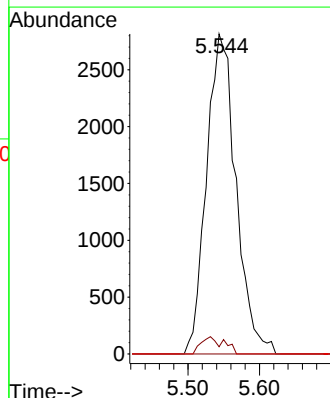



#40

Benzene

Concen: 9.168 ug/l

RT: 6.037 min Scan# 811

Delta R.T. 0.006 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0068

Tgt Ion: 78 Resp: 35012

Ion Ratio Lower Upper

78 100

77 27.1 19.0 28.6

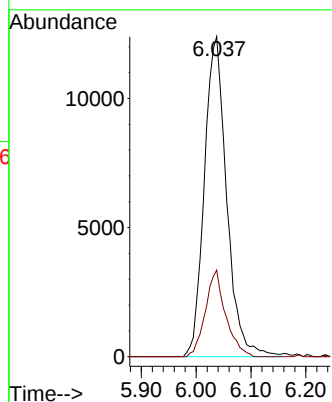

#42

1,2-Dichloroethane

Concen: 0.236 ug/l

RT: 6.031 min Scan# 811

Delta R.T. -0.049 min

Lab File: VX046023.D




Acq: 02 May 2025 13:28


Tgt Ion: 62 Resp: 373

Ion Ratio Lower Upper

62 100

98 0.0 0.0 15.2


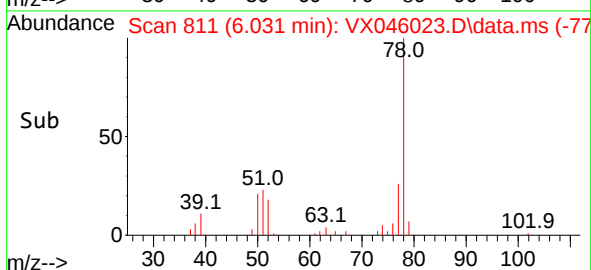






#43
Isopropyl Acetate
Concen: 4.954 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 43 Resp: 11832
Ion Ratio Lower Upper
43 100
61 17.4 14.1 21.1
87 10.1 9.2 13.8

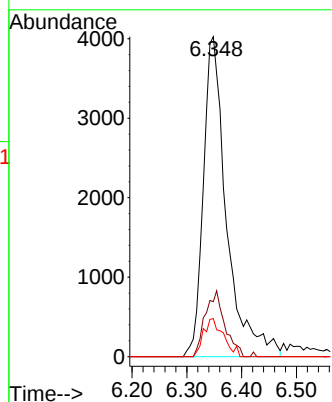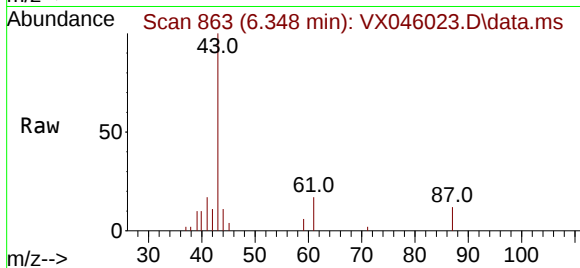

#48
Methyl methacrylate
Concen: 1.365 ug/l
RT: 7.604 min Scan# 1069
Delta R.T. -0.085 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 41 Resp: 1683
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 0.0 53.6 80.4#




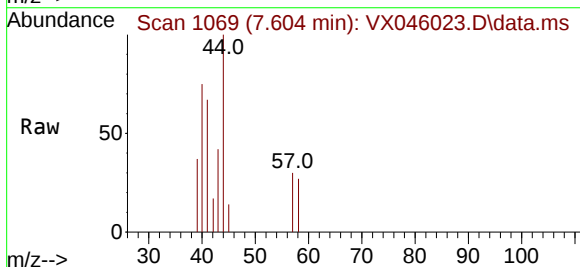




#50
Toluene-d8
Concen: 51.029 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 98 Resp: 164948
Ion Ratio Lower Upper
98 100
100 65.9 52.2 78.4

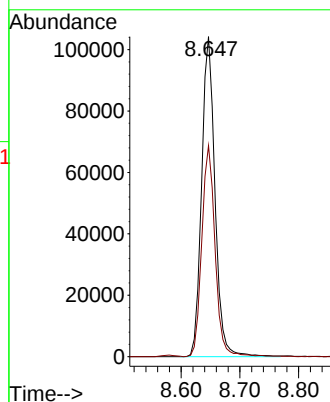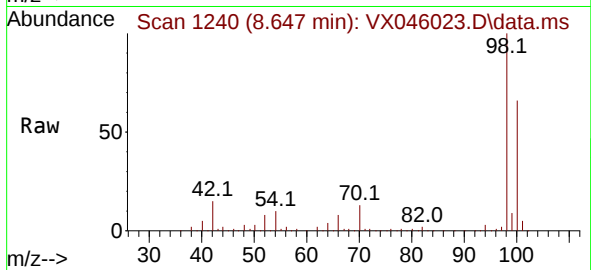

#51
4-Methyl-2-Pentanone
Concen: 24.988 ug/l
RT: 8.549 min Scan# 1224
Delta R.T. -0.025 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 43 Resp: 39562
Ion Ratio Lower Upper
43 100
58 5.0 28.5 42.7#


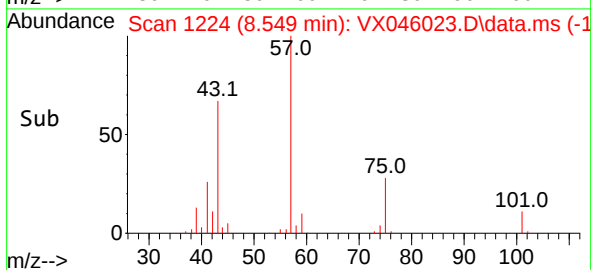
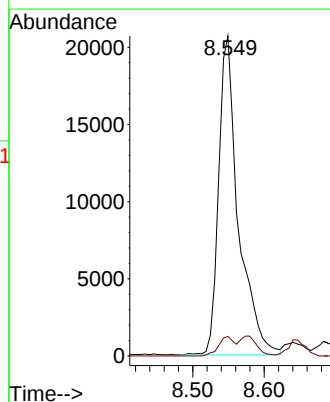



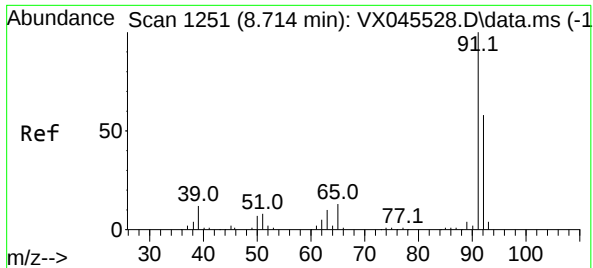

#52
Toluene
Concen: 9.927 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion: 92 Resp: 22940
Ion Ratio Lower Upper
92 100
91 171.8 138.7 208.1

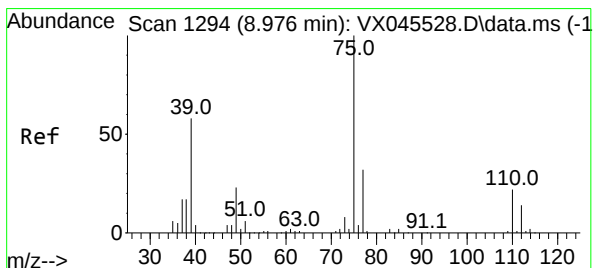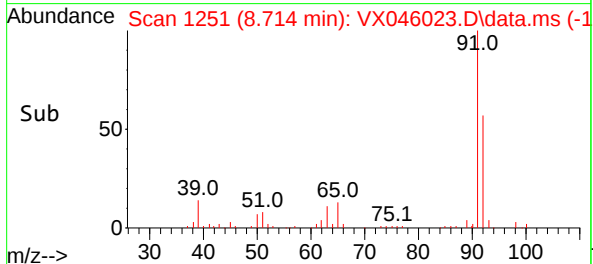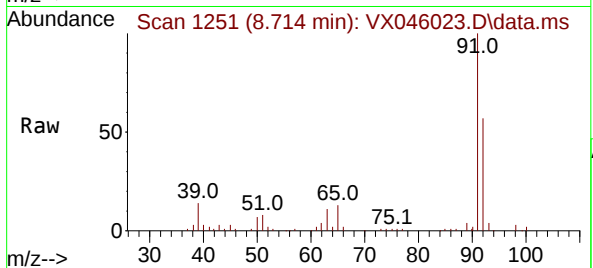

#53
t-1,3-Dichloropropene
Concen: 2.433 ug/l
RT: 8.951 min Scan# 1290
Delta R.T. -0.025 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 75 Resp: 212
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#


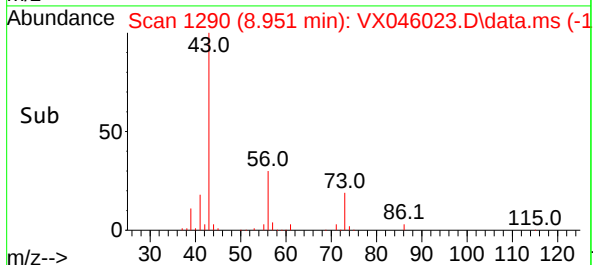
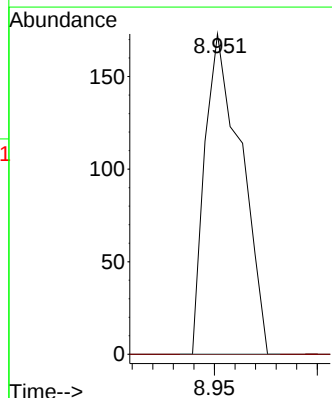
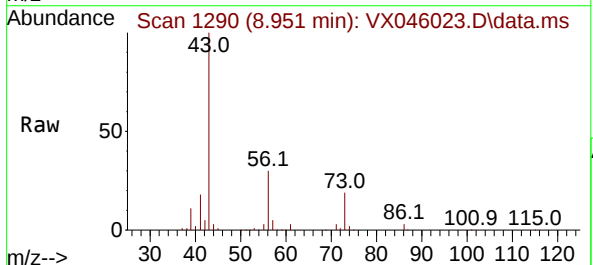




#54
 cis-1,3-Dichloropropene
 Concen: 9.903 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28




Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0068


Tgt Ion: 75 Resp: 13594
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.6 36.8#
 39 44.1 48.4 72.6#

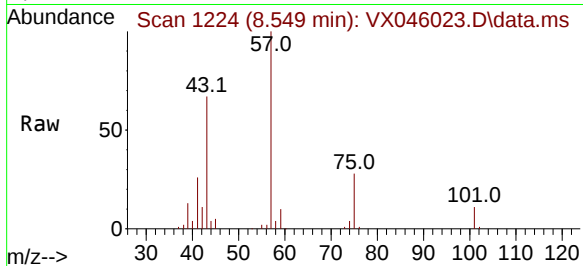

#55
 1,1,2-Trichloroethane
 Concen: 0.222 ug/l
 RT: 9.012 min Scan# 1300
 Delta R.T. -0.134 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28

Tgt Ion: 97 Resp: 204
 Ion Ratio Lower Upper
 97 100
 83 0.0 71.8 107.8#
 85 0.0 47.0 70.6#
 99 0.0 48.6 73.0#


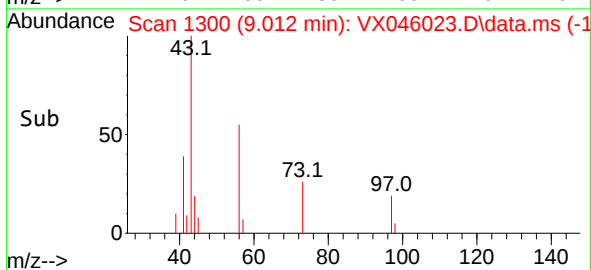

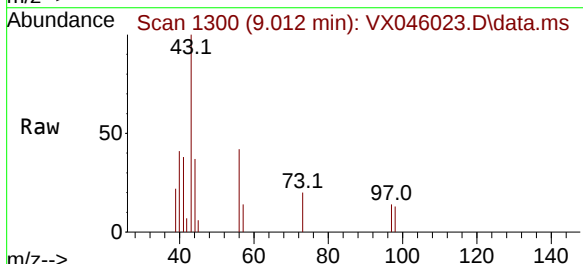




#57
 1,3-Dichloropropane
 Concen: 0.835 ug/l
 RT: 9.482 min Scan# 1339
 Delta R.T. 0.177 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28




Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0068


Tgt Ion: 76 Resp: 1339
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.0 39.0#

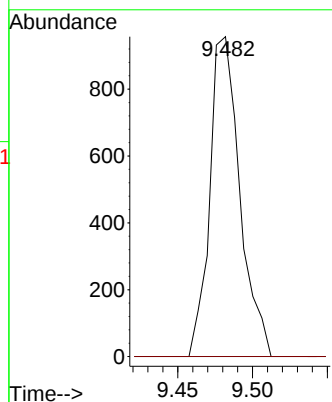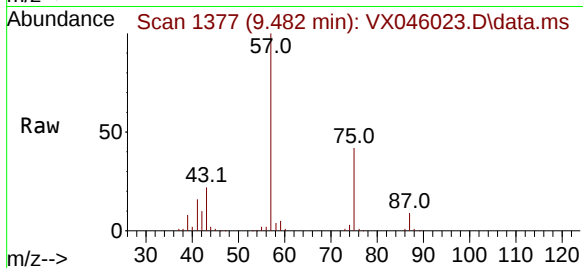

#59
 2-Hexanone
 Concen: 7.119 ug/l
 RT: 9.378 min Scan# 1360
 Delta R.T. -0.049 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28

Tgt Ion: 43 Resp: 8346
 Ion Ratio Lower Upper
 43 100
 58 0.0 24.9 74.6#

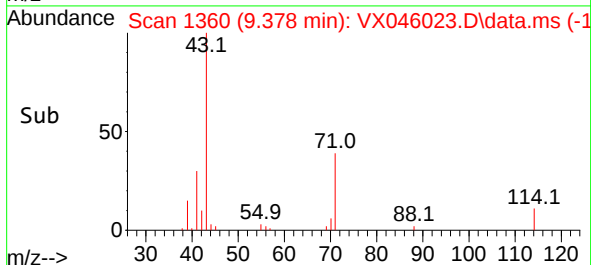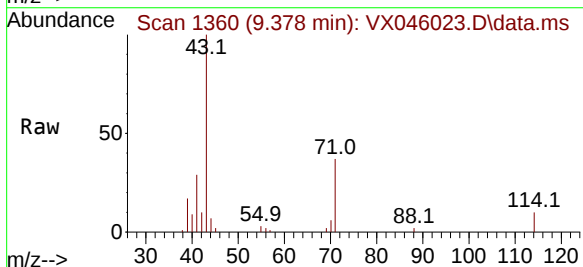



#62

4-Bromofluorobenzene

Concen: 55.949 ug/l

RT: 11.079 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0068





Tgt Ion: 95 Resp: 65875

Ion Ratio Lower Upper

95 100

174 65.8 0.0 135.8

176 63.9 0.0 131.4

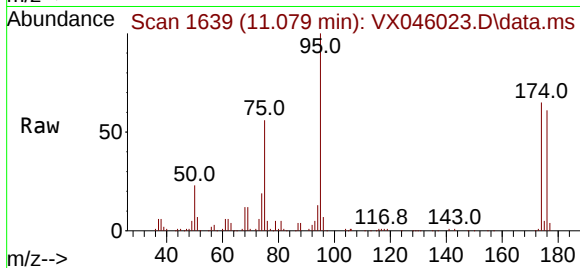

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.049 min Scan# 1470

Delta R.T. -0.000 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28




Tgt Ion: 117 Resp: 124567


Ion Ratio Lower Upper

117 100

82 63.2 49.2 73.8

119 32.4 25.1 37.7

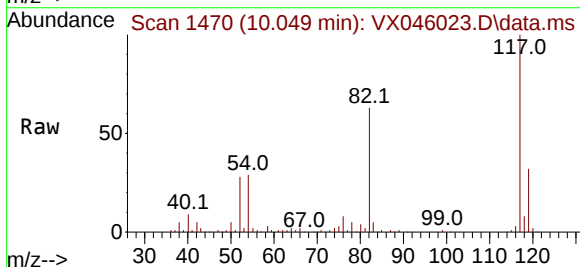



#67

Ethyl Benzene

Concen: 0.738 ug/l

RT: 10.195 min Scan# 1493

Delta R.T. 0.006 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0068

Tgt Ion: 91 Resp: 3520

Ion Ratio Lower Upper

91 100

106 32.8 23.7 35.5

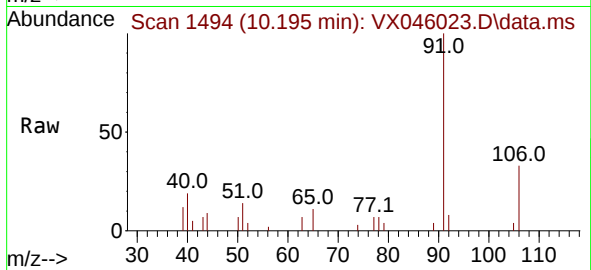

#68

m/p-Xylenes

Concen: 4.015 ug/l

RT: 10.299 min Scan# 1511

Delta R.T. -0.000 min

Lab File: VX046023.D




Acq: 02 May 2025 13:28


Tgt Ion: 106 Resp: 6961

Ion Ratio Lower Upper

106 100

91 223.0 172.6 258.8









#69
o-Xylene
Concen: 3.493 ug/l
RT: 10.640 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion:106 Resp: 5967
Ion Ratio Lower Upper
106 100
91 220.5 113.6 340.6

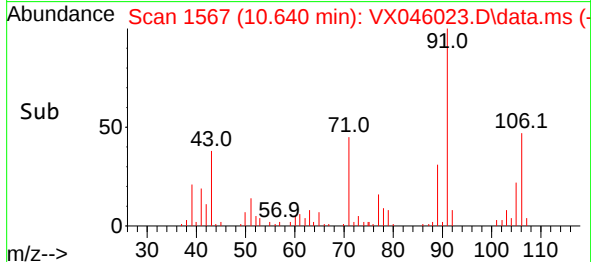

#70
Styrene
Concen: 0.728 ug/l
RT: 10.658 min Scan# 1570
Delta R.T. 0.006 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion:104 Resp: 2051
Ion Ratio Lower Upper
104 100
78 98.5 45.4 68.2#
103 79.4 43.8 65.8#

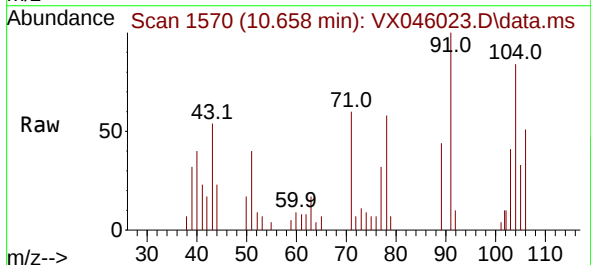



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0068





Tgt Ion:152 Resp: 56427

Ion Ratio Lower Upper

152 100

115 65.6 46.9 140.7

150 159.4 0.0 349.4

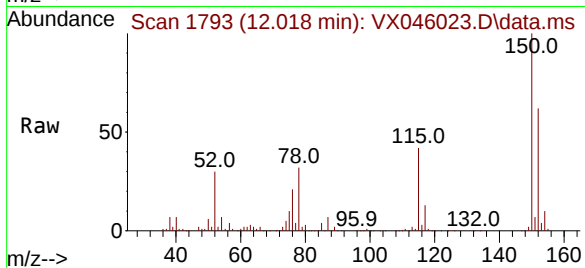

#76

1,2,3-Trichloropropane

Concen: 26.843 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX046023.D




Acq: 02 May 2025 13:28


Tgt Ion: 75 Resp: 36947

Ion Ratio Lower Upper

75 100

77 1.2 20.0 59.9#


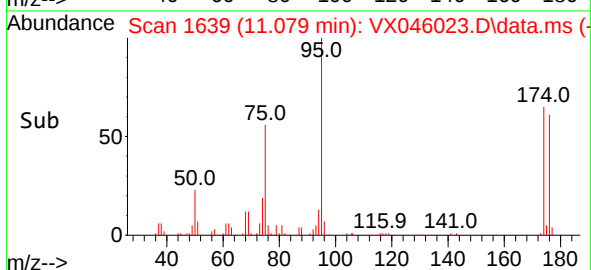

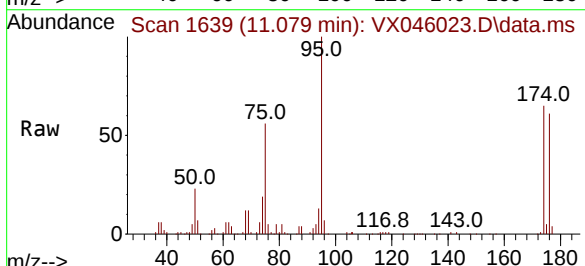




#80
1,3,5-Trimethylbenzene
Concen: 0.670 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0068


Tgt Ion:105 Resp: 2506
Ion Ratio Lower Upper
105 100
120 48.0 23.0 69.0

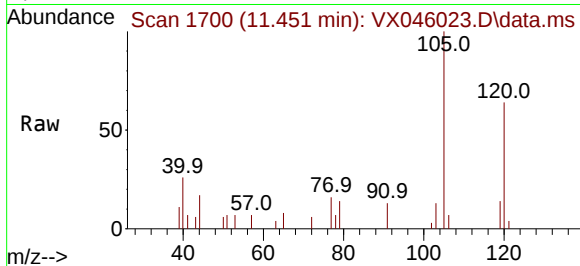

#81
trans-1,4-Dichloro-2-butene
Concen: 91.103 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046023.D
Acq: 02 May 2025 13:28

Tgt Ion: 75 Resp: 36947
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#

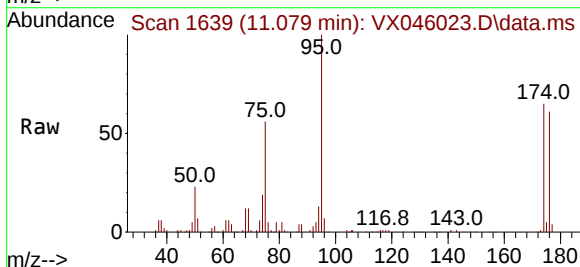



#83

tert-Butylbenzene

Concen: 0.217 ug/l

RT: 11.756 min Scan# 1743

Delta R.T. 0.043 min

Lab File: VX046023.D

Acq: 02 May 2025 13:28

Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0068





Tgt Ion:119 Resp: 802

Ion Ratio Lower Upper

119 100

91 115.0 32.4 97.2#

134 0.0 11.5 34.5#

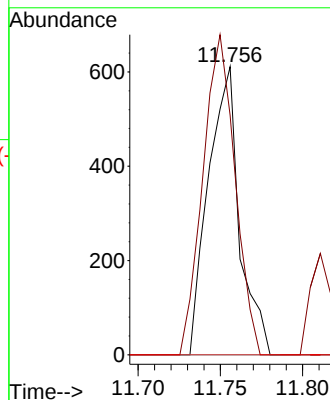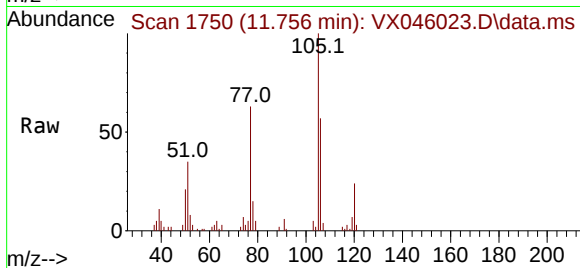

#84

1,2,4-Trimethylbenzene

Concen: 3.767 ug/l

RT: 11.750 min Scan# 1749

Delta R.T. -0.000 min

Lab File: VX046023.D




Acq: 02 May 2025 13:28


Tgt Ion:105 Resp: 14131

Ion Ratio Lower Upper

105 100

120 22.6 21.4 64.3


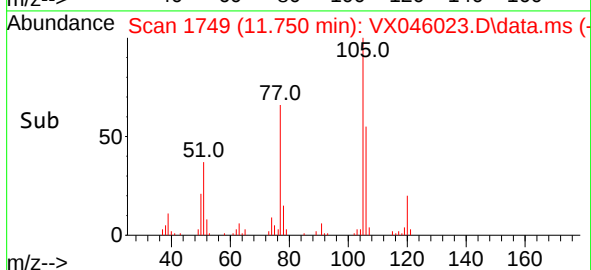
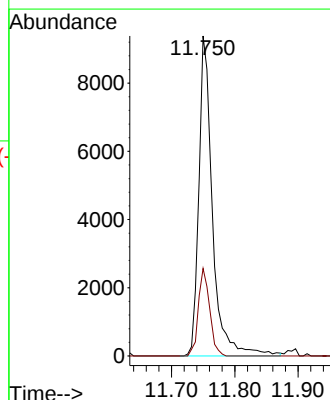
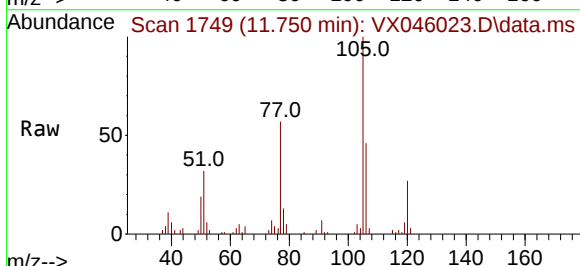




#85
 sec-Butylbenzene
 Concen: 3.109 ug/l
 RT: 11.750 min Scan# 11
 Delta R.T. -0.140 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0068

Tgt Ion:105 Resp: 14131
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.6 28.6#

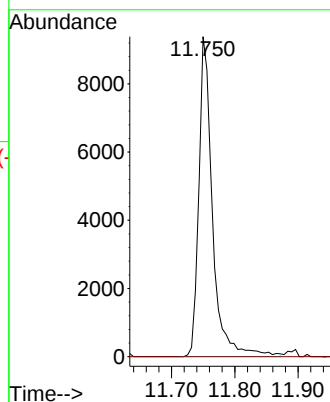

#95
 Naphthalene
 Concen: 91.361 ug/l
 RT: 13.774 min Scan# 2081
 Delta R.T. -0.000 min
 Lab File: VX046023.D
 Acq: 02 May 2025 13:28

Tgt Ion:128 Resp: 357676
 Ion Ratio Lower Upper
 128 100
 127 13.1 10.3 15.5
 129 11.0 8.6 12.8

