

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050225\
 Data File : VX046024.D
 Acq On : 02 May 2025 13:51
 Operator : JC/MD
 Sample : Q1925-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0069

Quant Time: May 02 23:15:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 02 03:11:43 2025
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	63181	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	122697	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	116875	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	53888	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	61162	52.935	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.880%	
35) Dibromofluoromethane	5.385	113	44698	51.345	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 102.700%	
50) Toluene-d8	8.647	98	155535	51.188	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 102.380%	
62) 4-Bromofluorobenzene	11.079	95	60672	54.819	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 109.640%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	2.995	59	1432	9.222	ug/l #	93
13) Acrolein	2.233	56	322	1.506	ug/l	95
16) Acetone	2.386	43	28725	60.544	ug/l	95
17) Carbon Disulfide	2.501	76	535	0.286	ug/l #	76
18) Methyl Acetate	2.709	43	2143	1.962	ug/l	95
20) Methylene Chloride	2.782	84	6784	7.638	ug/l	99
25) 2-Butanone	4.519	43	158	0.228	ug/l #	52
29) Tetrahydrofuran	5.025	42	106	0.235	ug/l #	35
31) Cyclohexane	5.544	56	1959	1.382	ug/l #	46
36) 1,1-Dichloropropene	5.544	75	6208	5.282	ug/l #	49
38) Carbon Tetrachloride	5.544	117	7144	5.624	ug/l #	15
40) Benzene	6.044	78	9877	2.751	ug/l	97
43) Isopropyl Acetate	6.348	43	11126	4.956	ug/l	96
48) Methyl methacrylate	7.598	41	1715	1.480	ug/l #	15
51) 4-Methyl-2-Pentanone	8.549	43	37716	25.342	ug/l #	48
52) Toluene	8.714	92	6554	3.017	ug/l	100
53) t-1,3-Dichloropropene	8.952	75	167	2.410	ug/l #	43
54) cis-1,3-Dichloropropene	8.549	75	13146	10.188	ug/l #	68
57) 1,3-Dichloropropane	9.482	76	1326	0.880	ug/l #	42
59) 2-Hexanone	9.378	43	11271	10.227	ug/l #	28
67) Ethyl Benzene	10.195	91	1245	0.278	ug/l	91
68) m/p-Xylenes	10.305	106	2076	1.276	ug/l	90
69) o-Xylene	10.646	106	1763	1.100	ug/l	86
70) Styrene	10.659	104	926	0.350	ug/l #	73
74) N-amyl acetate	10.854	43	732	0.355	ug/l #	55
76) 1,2,3-Trichloropropane	11.079	75	36241	27.571	ug/l #	37
80) 1,3,5-Trimethylbenzene	11.451	105	863	0.242	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.079	75	36241	93.573	ug/l #	1
90) Hexachloroethane	12.408	117	626	1.018	ug/l #	19
95) Naphthalene	13.774	128	93856	25.103	ug/l	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050225\
Data File : VX046024.D
Acq On : 02 May 2025 13:51
Operator : JC/MD
Sample : Q1925-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069

Quant Time: May 02 23:15:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X040225W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 02 03:11:43 2025
Response via : Initial Calibration



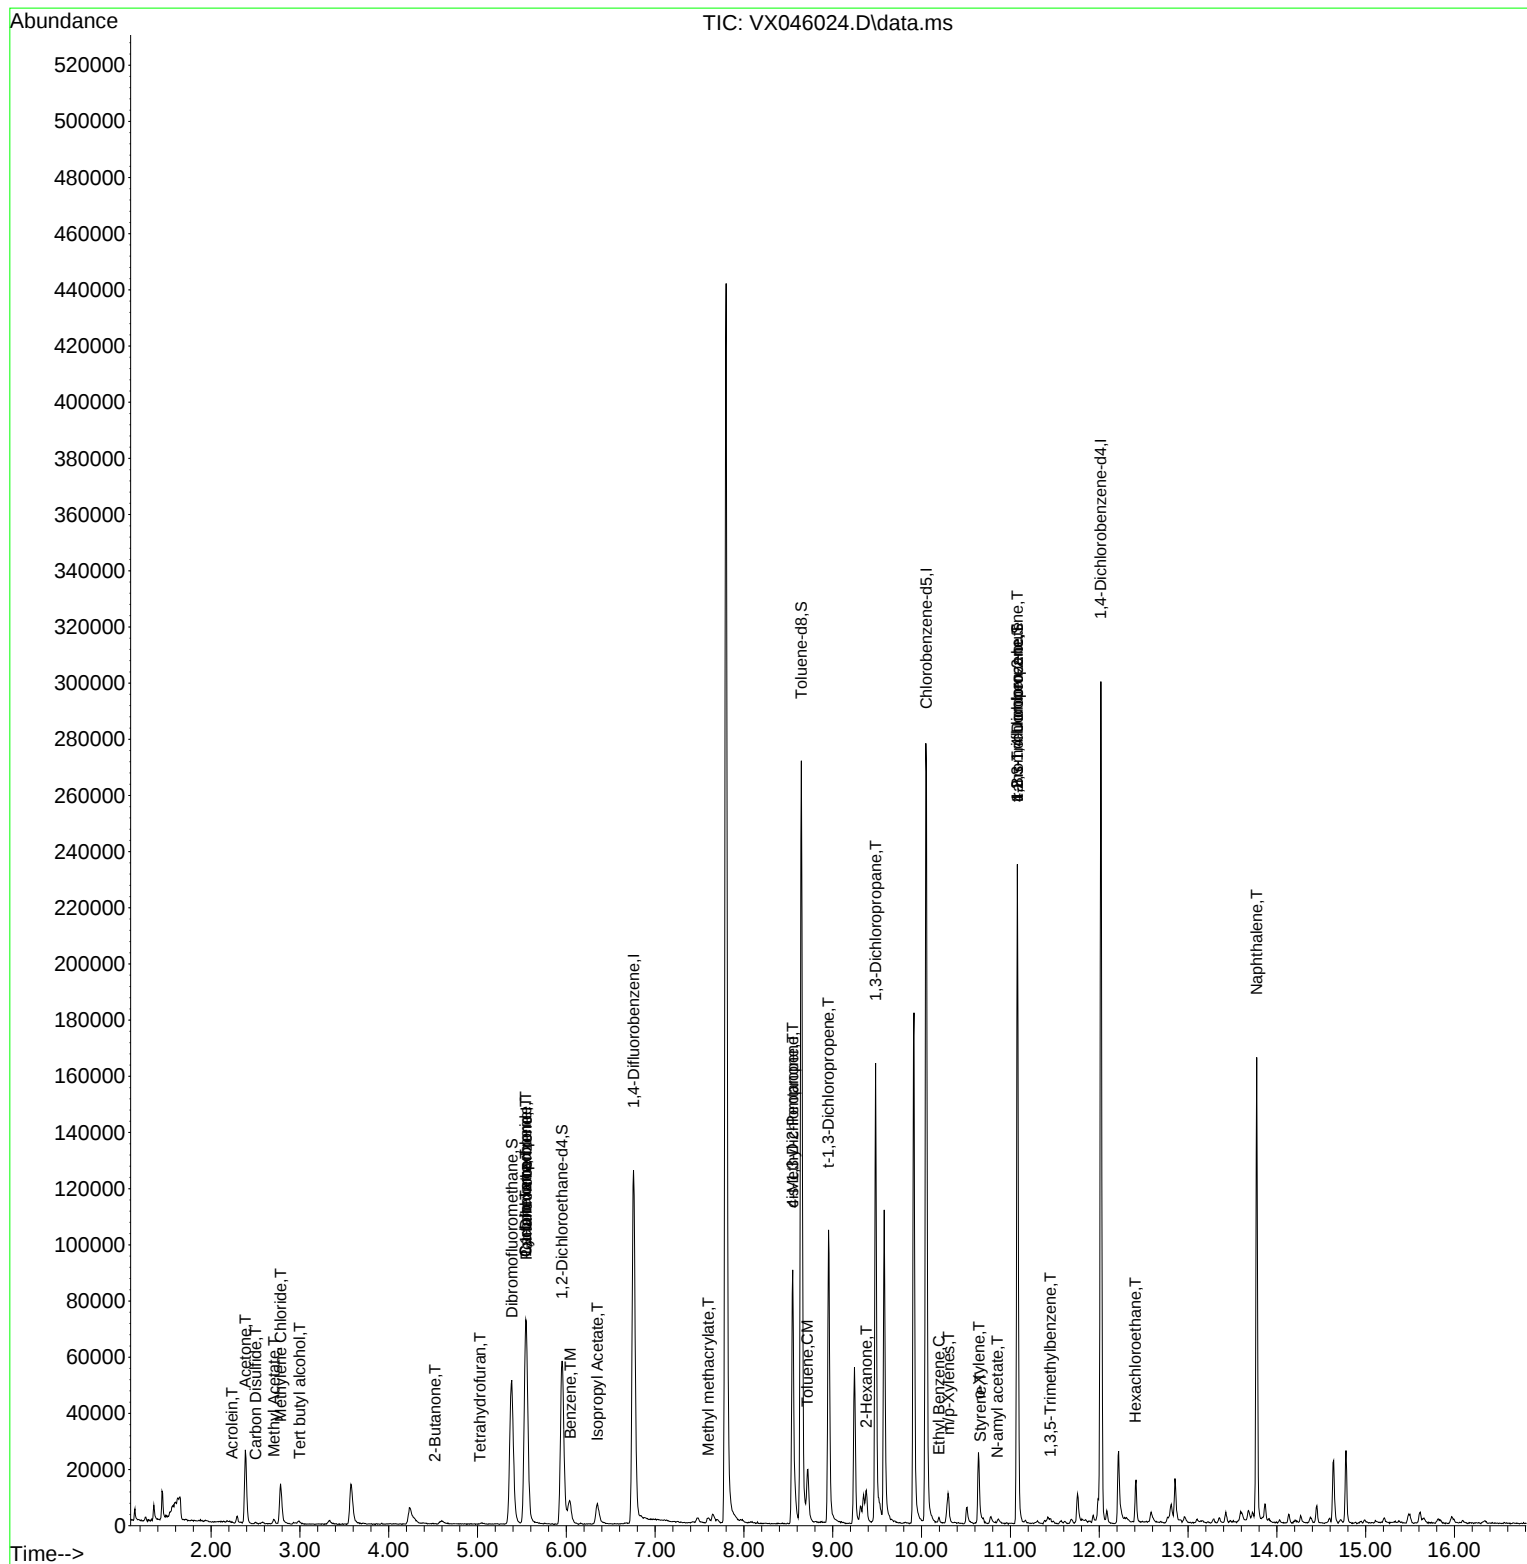




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion:168 Resp: 63181
Ion Ratio Lower Upper
168 100
99 64.7 52.3 78.5

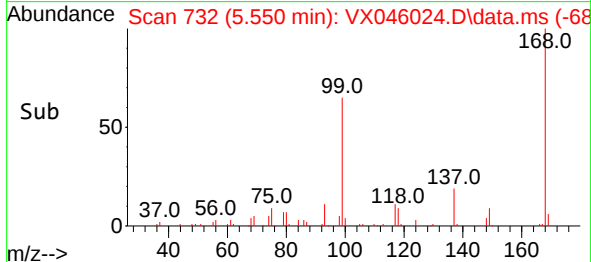

#11
Tert butyl alcohol
Concen: 9.222 ug/l
RT: 2.995 min Scan# 313
Delta R.T. 0.018 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 59 Resp: 1432
Ion Ratio Lower Upper
59 100
57 8.2 8.6 12.8#


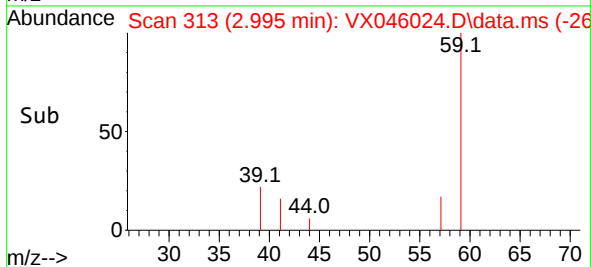

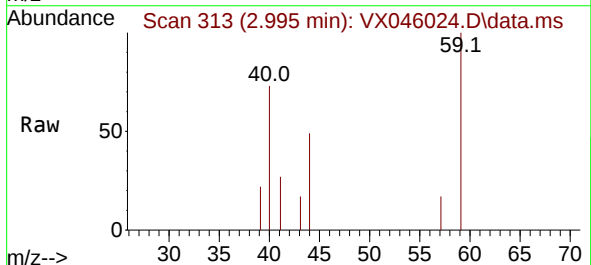


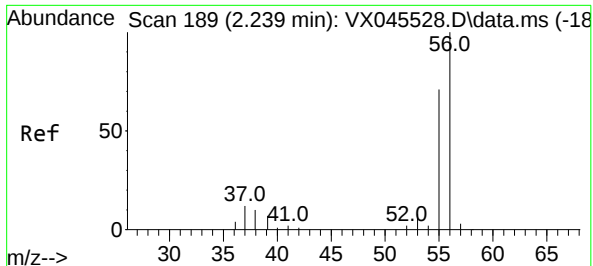

#13
Acrolein
Concen: 1.506 ug/l
RT: 2.233 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion: 56 Resp: 322
Ion Ratio Lower Upper
56 100
55 74.5 56.2 84.2

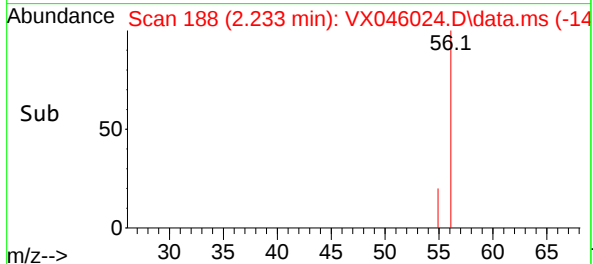

#16
Acetone
Concen: 60.544 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 43 Resp: 28725
Ion Ratio Lower Upper
43 100
58 25.4 22.3 33.5


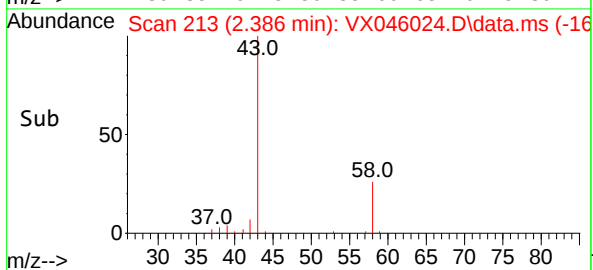

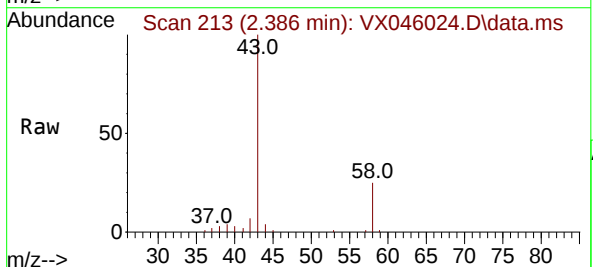


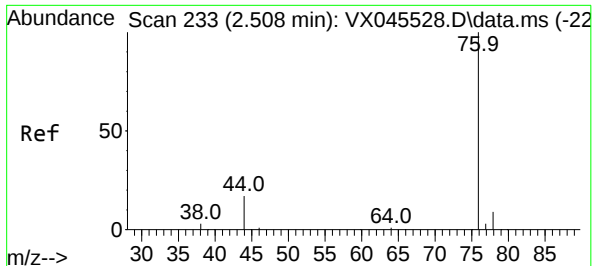

#17
Carbon Disulfide
Concen: 0.286 ug/l
RT: 2.501 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion: 76 Resp: 535
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.6#

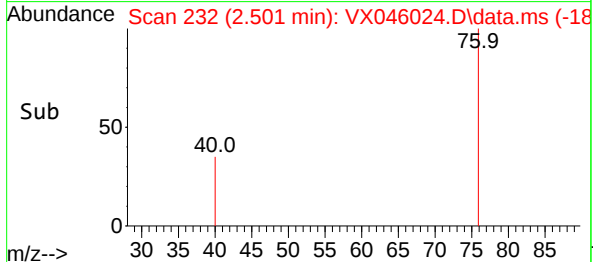

#18
Methyl Acetate
Concen: 1.962 ug/l
RT: 2.709 min Scan# 266
Delta R.T. 0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 43 Resp: 2143
Ion Ratio Lower Upper
43 100
74 19.3 17.5 26.3


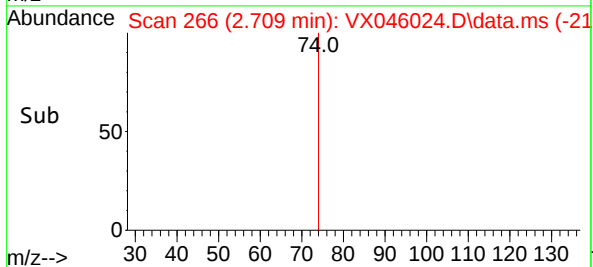

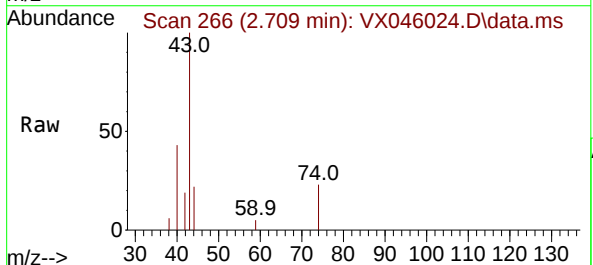




#20
Methylene Chloride
Concen: 7.638 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion:	84	Resp:	6784
Ion	Ratio	Lower	Upper
84	100		
49	132.7	107.5	161.3
51	42.6	33.0	49.6
86	63.4	50.1	75.1



#25
2-Butanone
Concen: 0.228 ug/l
RT: 4.519 min Scan# 563
Delta R.T. -0.037 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion:	43	Resp:	158
Ion	Ratio	Lower	Upper
43	100		
72	0.0	18.6	28.0#





#29

Tetrahydrofuran

Concen: 0.235 ug/l

RT: 5.025 min Scan# 642

Delta R.T. 0.024 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0069





Tgt Ion: 42 Resp: 106

Ion Ratio Lower Upper

42 100

72 0.0 33.4 50.0#

71 0.0 31.4 47.0#

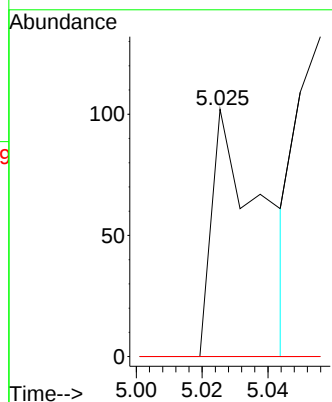

#31

Cyclohexane

Concen: 1.382 ug/l

RT: 5.544 min Scan# 731

Delta R.T. 0.079 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51




Tgt Ion: 56 Resp: 1959


Ion Ratio Lower Upper

56 100

69 132.9 23.6 35.4#

84 89.8 67.7 101.5





#33

1,2-Dichloroethane-d4

Concen: 52.935 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0069

Tgt Ion: 65 Resp: 61162

Ion Ratio Lower Upper

65 100

67 49.4 0.0 99.0

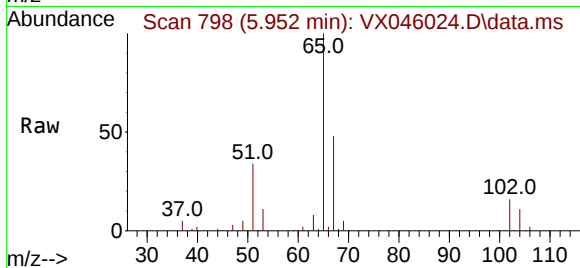

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51




Tgt Ion: 114 Resp: 122697


Ion Ratio Lower Upper

114 100

63 24.7 0.0 46.8

88 18.6 0.0 35.4


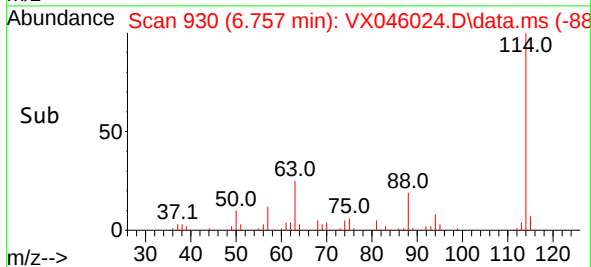

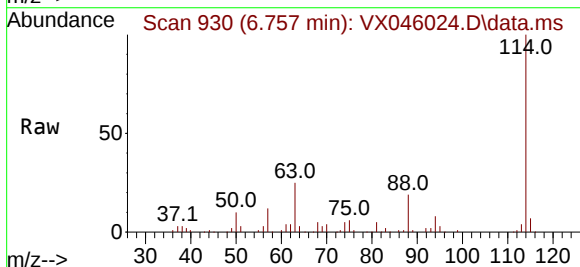


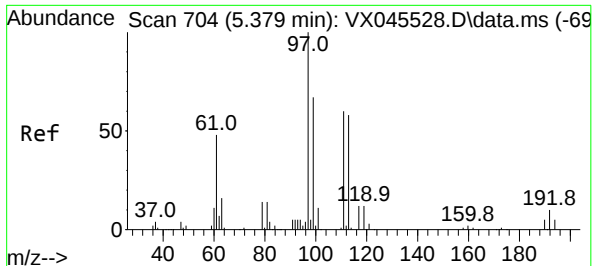

#35
Dibromofluoromethane
Concen: 51.345 ug/l
RT: 5.385 min Scan# 704
Delta R.T. 0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion:113 Resp: 44698
Ion Ratio Lower Upper
113 100
111 103.3 81.8 122.6
192 16.8 13.8 20.6

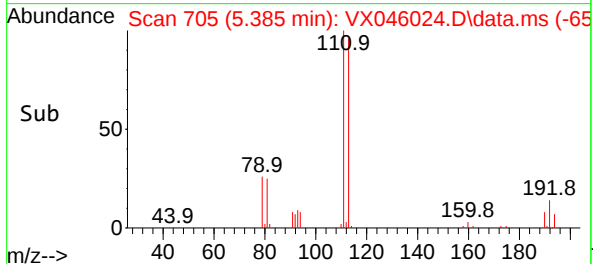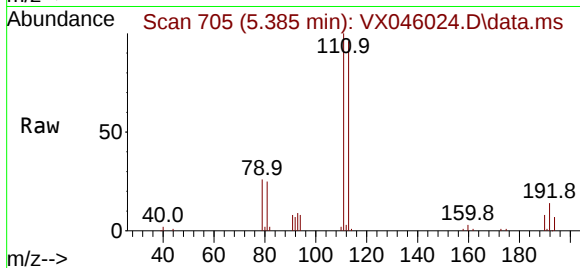

#36
1,1-Dichloropropene
Concen: 5.282 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.140 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51


Tgt Ion: 75 Resp: 6208
Ion Ratio Lower Upper
75 100
110 7.7 16.9 50.6#
77 0.0 25.0 37.4#

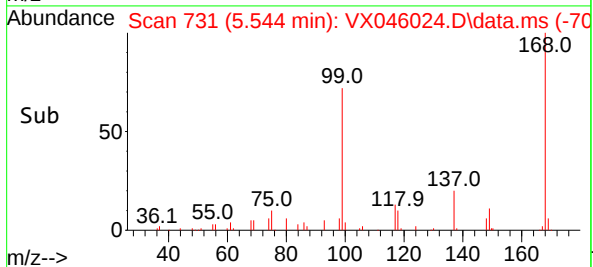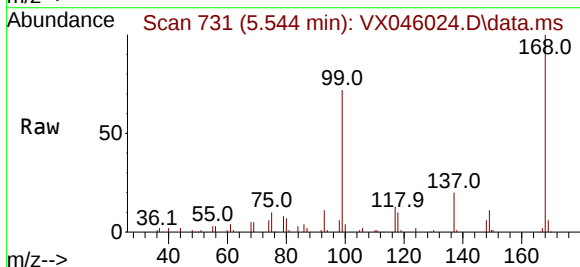






#38
Carbon Tetrachloride
Concen: 5.624 ug/l
RT: 5.544 min Scan# 711
Delta R.T. -0.128 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069







Tgt Ion:117 Resp: 7144
Ion Ratio Lower Upper
117 100
119 4.2 76.9 115.3#
121 0.0 24.2 36.2#



#40
Benzene
Concen: 2.751 ug/l
RT: 6.044 min Scan# 813
Delta R.T. 0.012 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 78 Resp: 9877
Ion Ratio Lower Upper
78 100
77 25.4 19.0 28.6




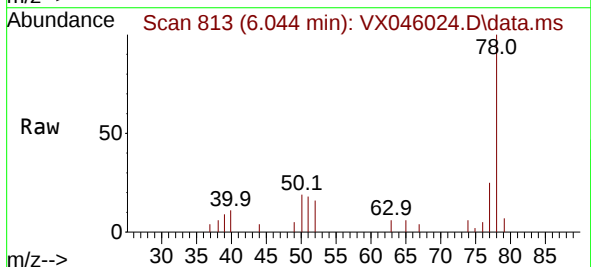




#43
Isopropyl Acetate
Concen: 4.956 ug/l
RT: 6.348 min Scan# 863
Delta R.T. 0.012 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion: 43 Resp: 11126
Ion Ratio Lower Upper
43 100
61 15.4 14.1 21.1
87 11.0 9.2 13.8

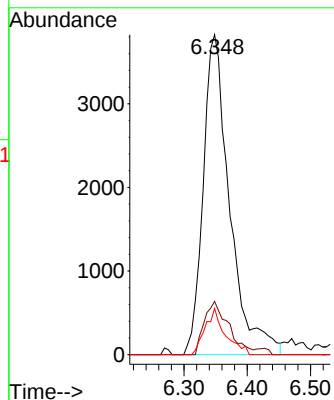

#48
Methyl methacrylate
Concen: 1.480 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.091 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 41 Resp: 1715
Ion Ratio Lower Upper
41 100
69 0.0 58.2 87.2#
39 0.0 53.6 80.4#

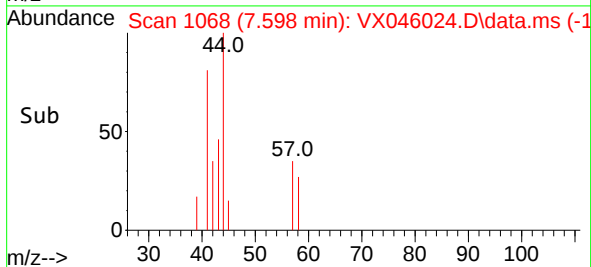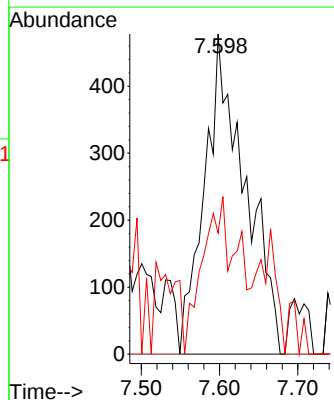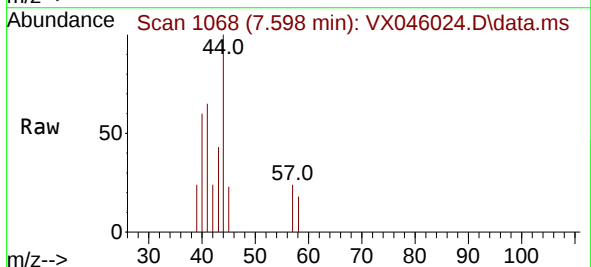

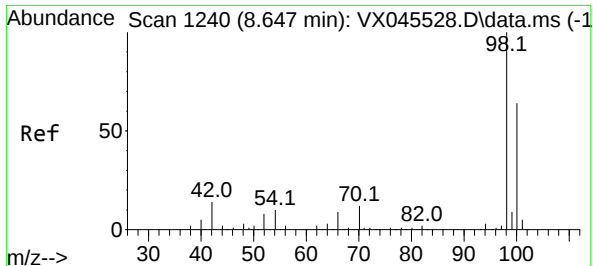

#50

Toluene-d8

Concen: 51.188 ug/l

RT: 8.647 min Scan# 11

Delta R.T. -0.000 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0069

Tgt Ion: 98 Resp: 155535

Ion Ratio Lower Upper

98 100

100 65.2 52.2 78.4

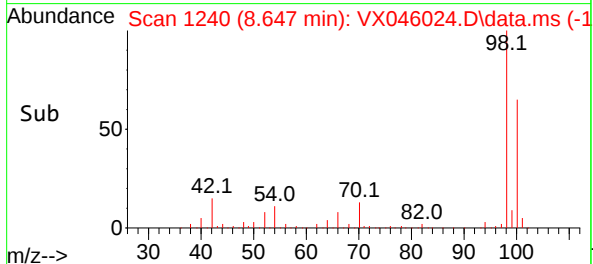

#51

4-Methyl-2-Pentanone

Concen: 25.342 ug/l

RT: 8.549 min Scan# 1224

Delta R.T. -0.024 min

Lab File: VX046024.D




Acq: 02 May 2025 13:51


Tgt Ion: 43 Resp: 37716

Ion Ratio Lower Upper

43 100

58 4.9 28.5 42.7#


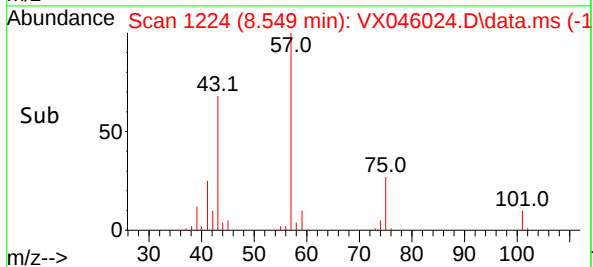

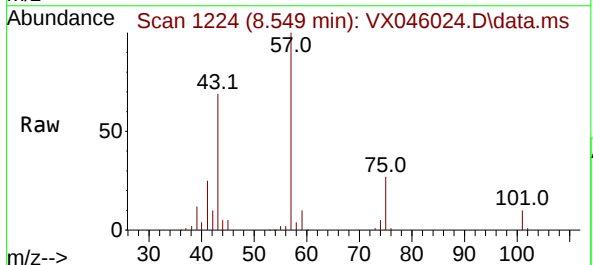


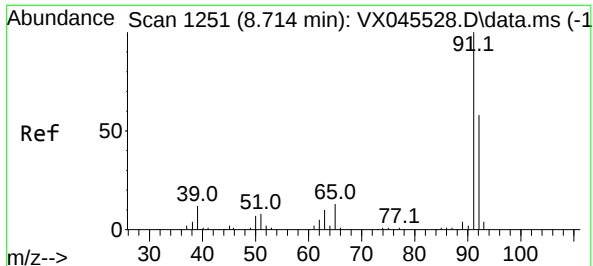

#52
Toluene
Concen: 3.017 ug/l
RT: 8.714 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion: 92 Resp: 6554
Ion Ratio Lower Upper
92 100
91 173.8 138.7 208.1

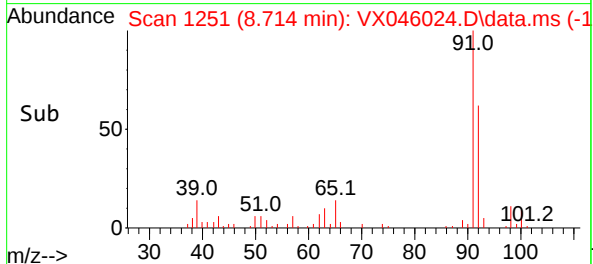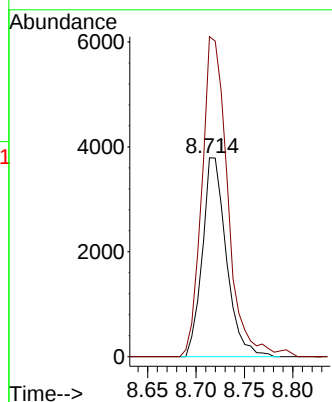

#53
t-1,3-Dichloropropene
Concen: 2.410 ug/l
RT: 8.952 min Scan# 1290
Delta R.T. -0.024 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 75 Resp: 167
Ion Ratio Lower Upper
75 100
77 0.0 25.4 38.0#


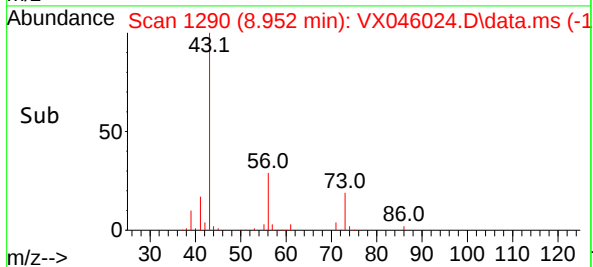
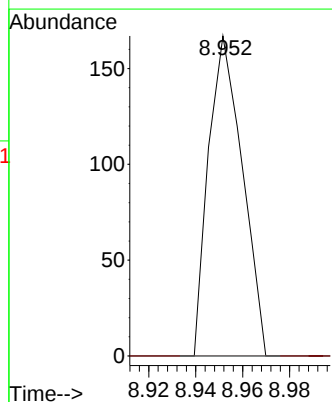
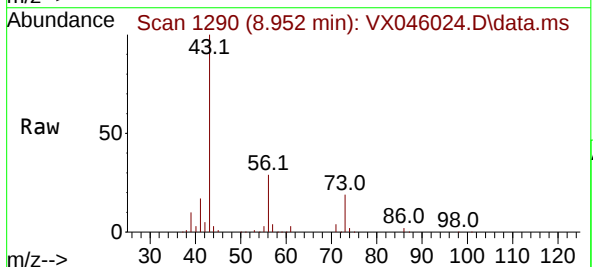




#54
 cis-1,3-Dichloropropene
 Concen: 10.188 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX046024.D
 Acq: 02 May 2025 13:51




Instrument :
 MSVOA_X
 ClientSampleId :
 AUD-25-0069


Tgt Ion: 75 Resp: 13146
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.6 36.8#
 39 45.2 48.4 72.6#



#57
 1,3-Dichloropropane
 Concen: 0.880 ug/l
 RT: 9.482 min Scan# 1377
 Delta R.T. 0.177 min
 Lab File: VX046024.D
 Acq: 02 May 2025 13:51

Tgt Ion: 76 Resp: 1326
 Ion Ratio Lower Upper
 76 100
 78 0.0 26.0 39.0#







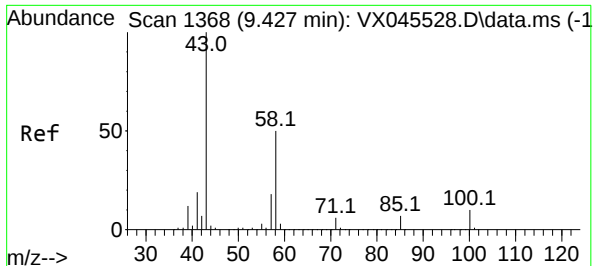

#59
2-Hexanone
Concen: 10.227 ug/l
RT: 9.378 min Scan# 11
Delta R.T. -0.049 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion: 43 Resp: 11271
Ion Ratio Lower Upper
43 100
58 0.0 24.9 74.6#

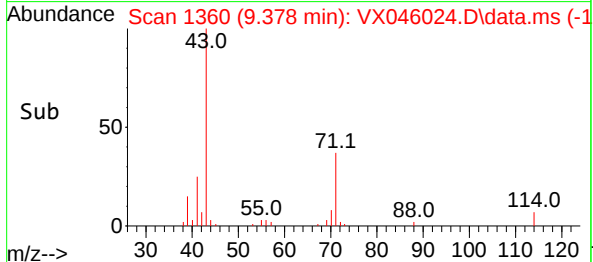

#62
4-Bromofluorobenzene
Concen: 54.819 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 95 Resp: 60672
Ion Ratio Lower Upper
95 100
174 67.9 0.0 135.8
176 66.1 0.0 131.4


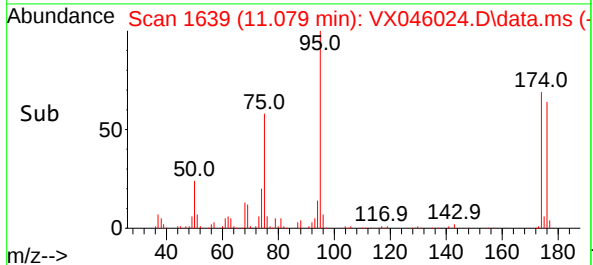

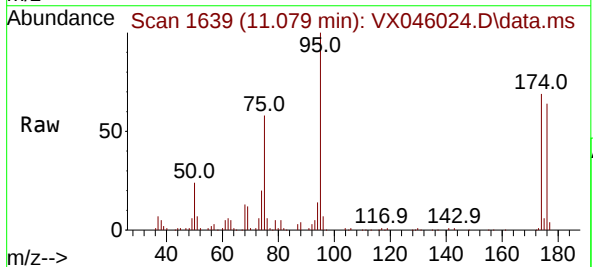




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1470
Delta R.T. 0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion:117 Resp: 116875
Ion Ratio Lower Upper
117 100
82 61.6 49.2 73.8
119 32.2 25.1 37.7

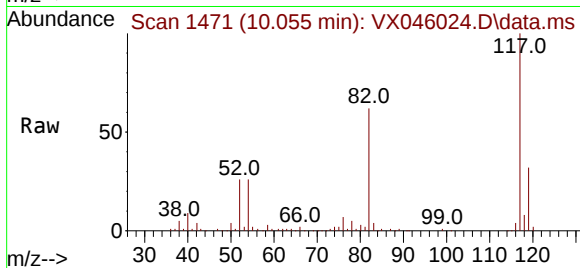

#67
Ethyl Benzene
Concen: 0.278 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.006 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 91 Resp: 1245
Ion Ratio Lower Upper
91 100
106 24.6 23.7 35.5

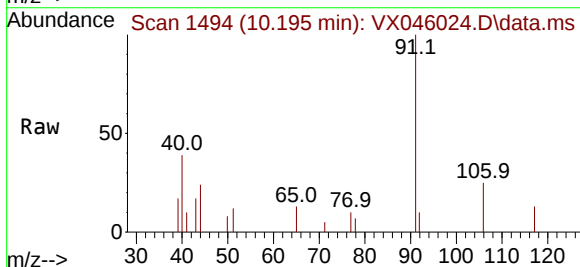



#68

m/p-Xylenes

Concen: 1.276 ug/l

RT: 10.305 min Scan# 1511

Delta R.T. 0.006 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Instrument :

MSVOA_X

ClientSampleId :





AUD-25-0069

Tgt Ion:106 Resp: 2076

Ion Ratio Lower Upper

106 100

91 231.2 172.6 258.8

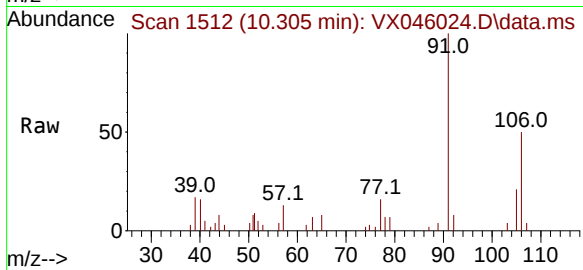

#69

o-Xylene

Concen: 1.100 ug/l

RT: 10.646 min Scan# 1568

Delta R.T. 0.006 min

Lab File: VX046024.D




Acq: 02 May 2025 13:51


Tgt Ion:106 Resp: 1763

Ion Ratio Lower Upper

106 100

91 204.7 113.6 340.6

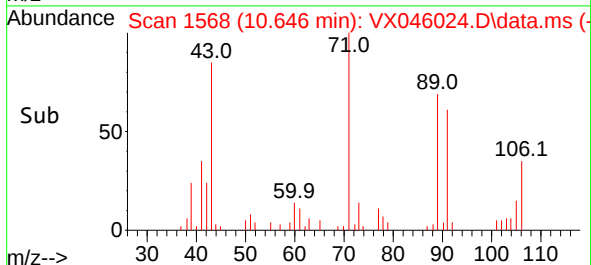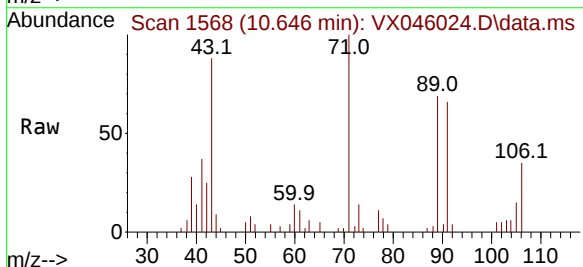



#70

Styrene

Concen: 0.350 ug/l

RT: 10.659 min Scan# 1569

Delta R.T. 0.006 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51





Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0069

Tgt Ion:104	Resp:	926
Ion Ratio	Lower	Upper
104	100	
78	83.9	45.4 68.2#
103	66.6	43.8 65.8#

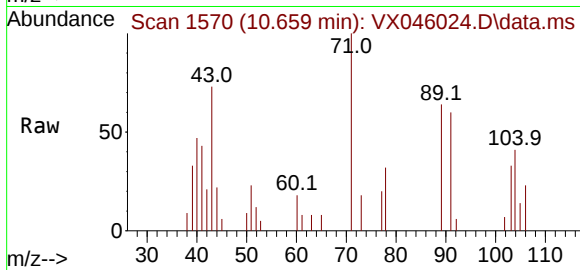

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 12.018 min Scan# 1793


Delta R.T. -0.000 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Tgt Ion:152	Resp:	53888
Ion Ratio	Lower	Upper
152	100	
115	64.0	46.9 140.7
150	157.7	0.0 349.4

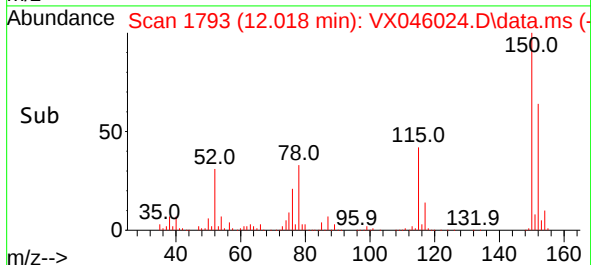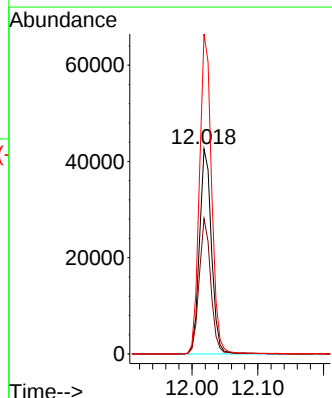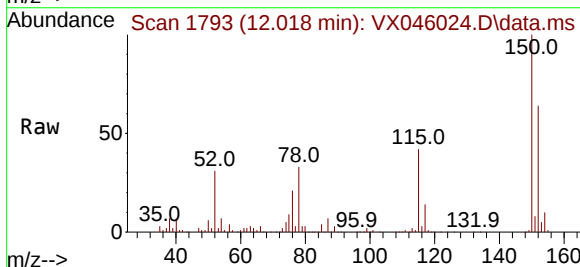



#74

N-amy1 acetate

Concen: 0.355 ug/l

RT: 10.854 min Scan# 1602

Delta R.T. 0.012 min

Lab File: VX046024.D

Acq: 02 May 2025 13:51

Instrument :

MSVOA_X

ClientSampleId :

AUD-25-0069

Tgt Ion: 43 Resp: 732





Ion Ratio Lower Upper

43 100

70 44.4 30.1 45.1

55 71.3 18.3 27.5#

61 0.0 17.5 26.3#

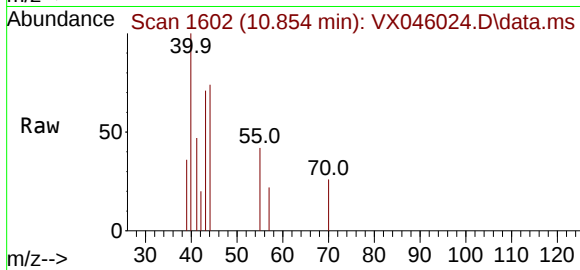

#76

1,2,3-Trichloropropane

Concen: 27.571 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.159 min

Lab File: VX046024.D




Acq: 02 May 2025 13:51


Tgt Ion: 75 Resp: 36241

Ion Ratio Lower Upper

75 100

77 0.9 20.0 59.9#




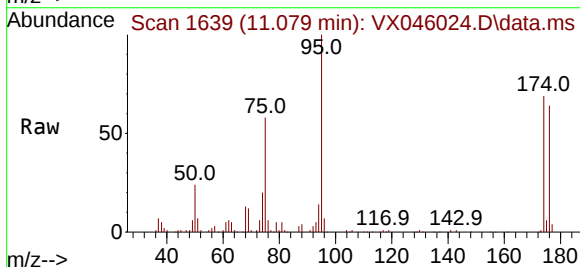




#80
1,3,5-Trimethylbenzene
Concen: 0.242 ug/l
RT: 11.451 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51




Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069


Tgt Ion:105 Resp: 863
Ion Ratio Lower Upper
105 100
120 47.9 23.0 69.0

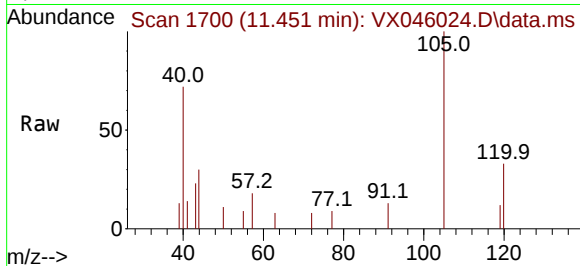

#81
trans-1,4-Dichloro-2-butene
Concen: 93.573 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion: 75 Resp: 36241
Ion Ratio Lower Upper
75 100
53 0.0 101.8 152.6#
89 0.0 37.2 55.8#


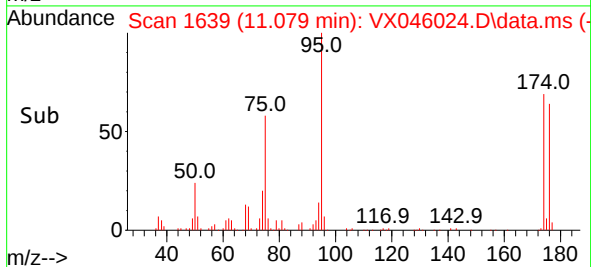

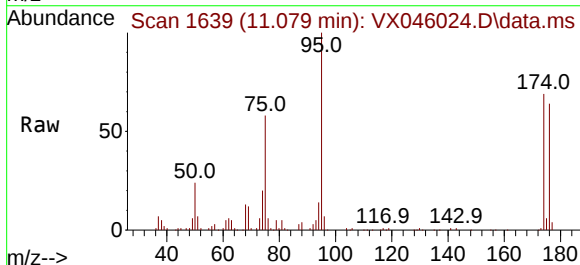




#90
Hexachloroethane
Concen: 1.018 ug/l
RT: 12.408 min Scan# 117
Delta R.T. -0.128 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Instrument :
MSVOA_X
ClientSampleId :
AUD-25-0069

Tgt Ion:117 Resp: 626
Ion Ratio Lower Upper
117 100
201 0.0 31.2 93.6#

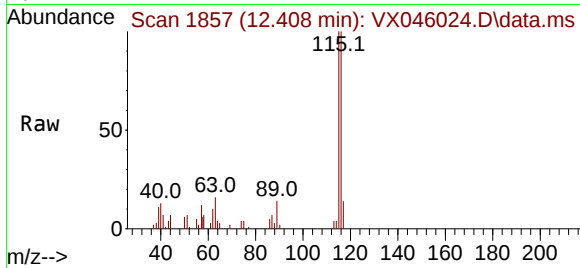

#95
Naphthalene
Concen: 25.103 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.000 min
Lab File: VX046024.D
Acq: 02 May 2025 13:51

Tgt Ion:128 Resp: 93856
Ion Ratio Lower Upper
128 100
127 13.1 10.3 15.5
129 10.7 8.6 12.8

