

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX050319\
 Data File : VX009301.D
 Acq On : 03 May 2019 10:27
 Operator : JC/SP
 Sample : VX0503WBL01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0503WBL01

Quant Time: May 03 14:11:46 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X050119W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu May 02 06:46:57 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	5.01	128	30565	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	6.85	114	177797	30.00	ug/l	0.00
57) Chlorobenzene-d5	10.11	117	151647	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	6.06	65	77102	30.41	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	101.37%
60) 4-Bromofluorobenzene	11.13	95	70043	27.18	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	90.60%
63) Toluene-d8	8.71	98	217489	30.25	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	100.83%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX050319\
Data File : VX009301.D
Acq On : 03 May 2019 10:27
Operator : JC/SP
Sample : VX0503WBL01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0503WBL01

Quant Time: May 03 14:11:46 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X050119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu May 02 06:46:57 2019
Response via : Initial Calibration

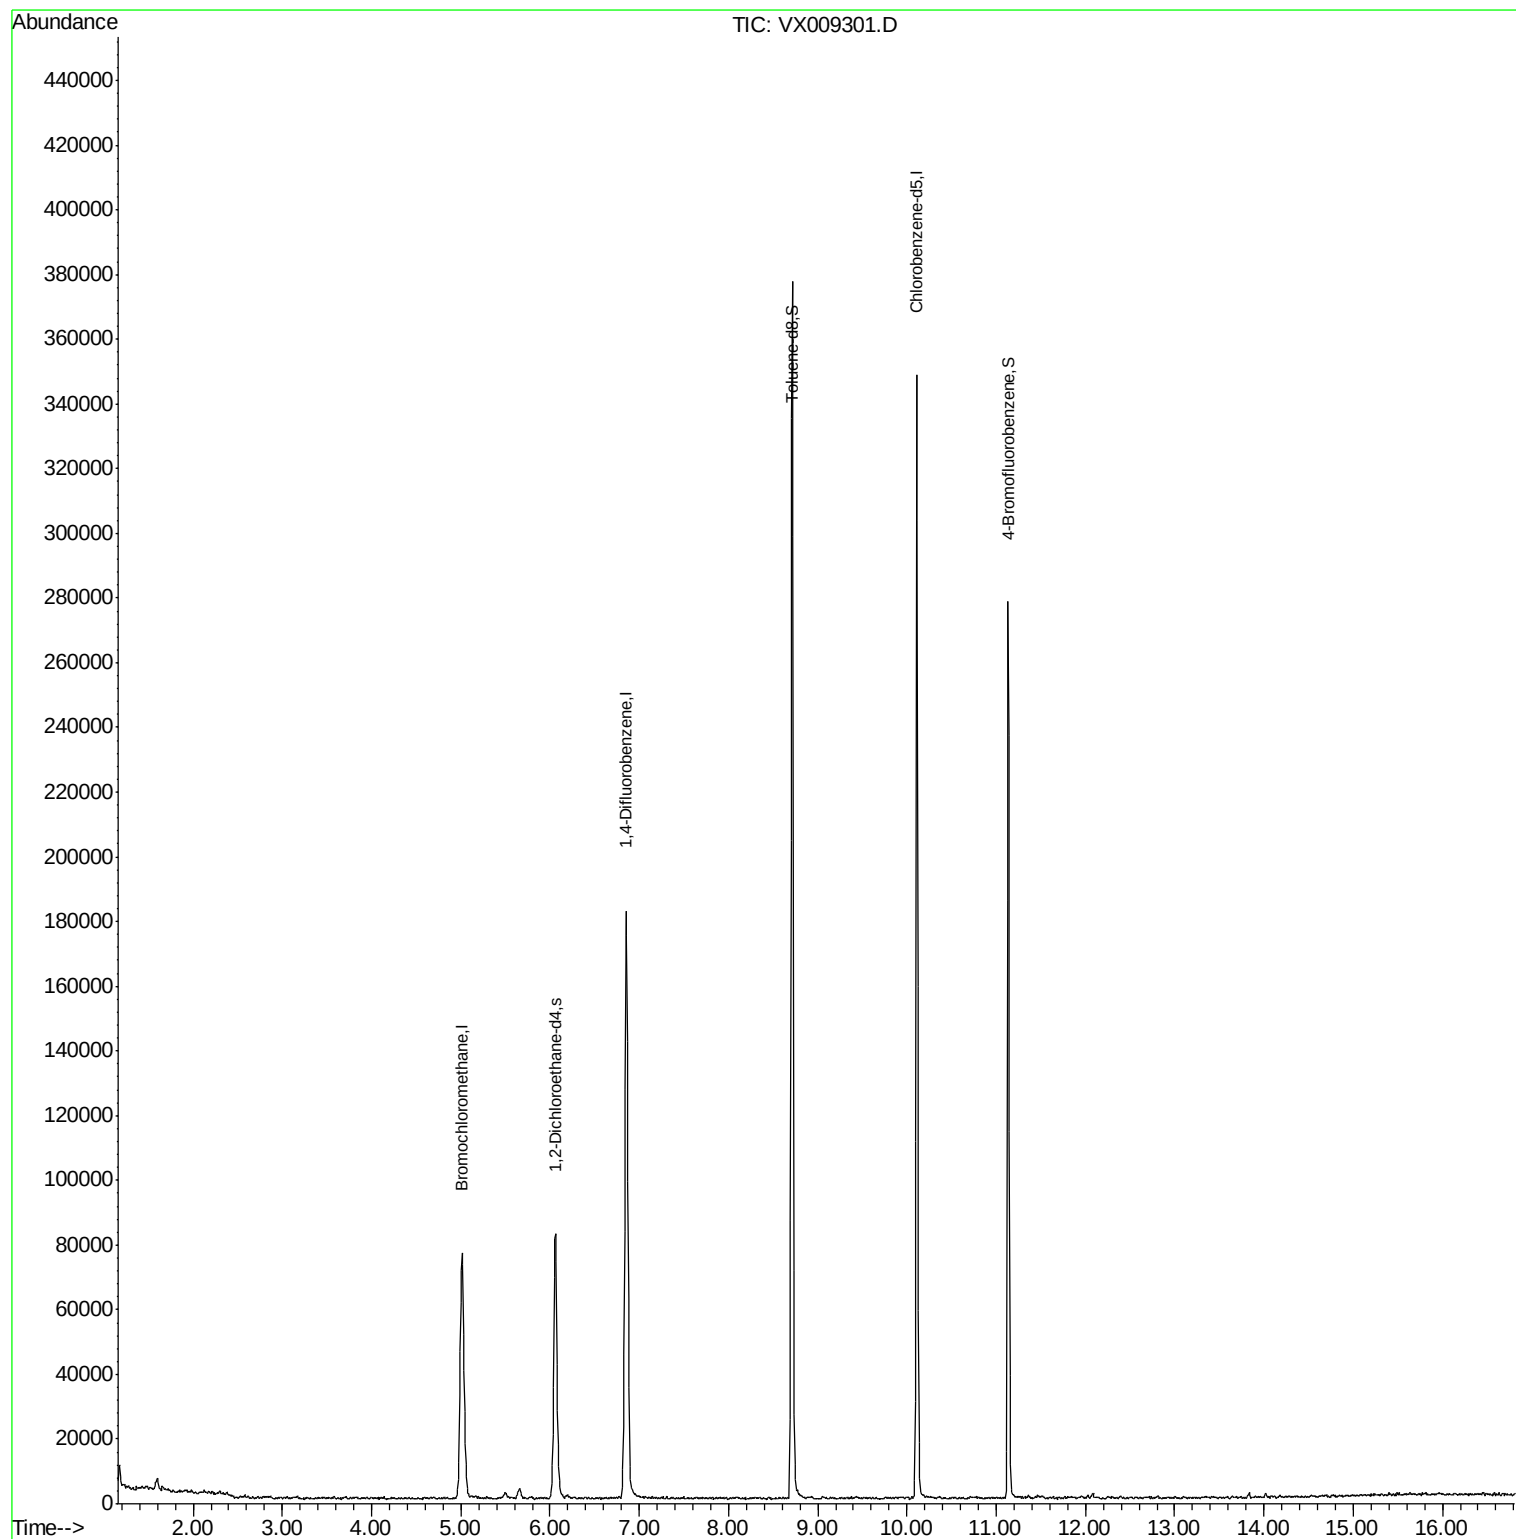

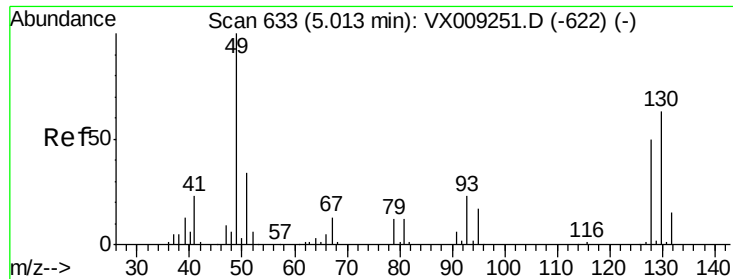

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 5.01 min Scan# 633

Delta R.T. -0.00 min

Lab File: VX009301.D

Acq: 03 May 2019 10:27

Instrument :

MSVOA_X

ClientSampled :

VX0503WBL01


Tot Ion:128 Resp: 30565

Ion Ratio Lower Upper

128 100

49 202.2 0.0 515.0




130 129.9 0.0 323.3

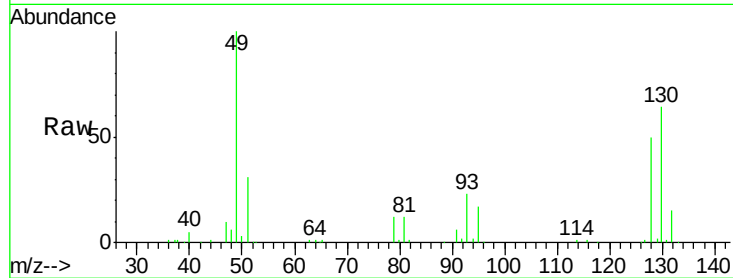

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VX0

Ion 130.00 (129.70 to 130.70): V

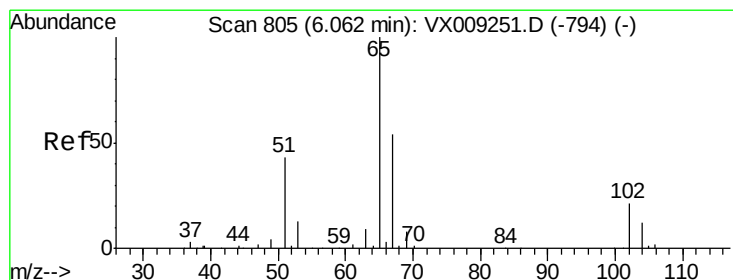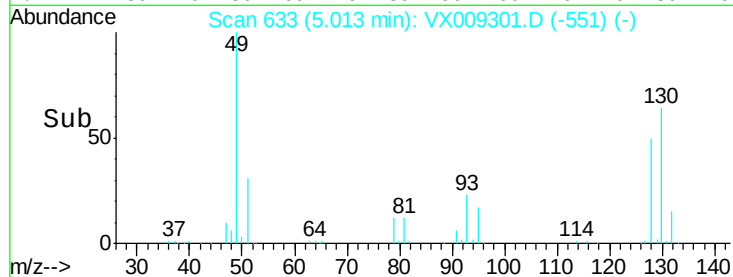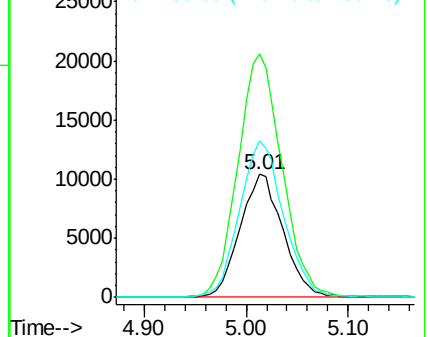

#27

1,2-Dichloroethane-d4

Concen: 30.409 ug/l

RT: 6.06 min Scan# 805

Delta R.T. -0.00 min

Lab File: VX009301.D


Acq: 03 May 2019 10:27

Tgt Ion: 65 Resp: 77102

Ion Ratio Lower Upper



65 100


67 53.5 43.1 64.7

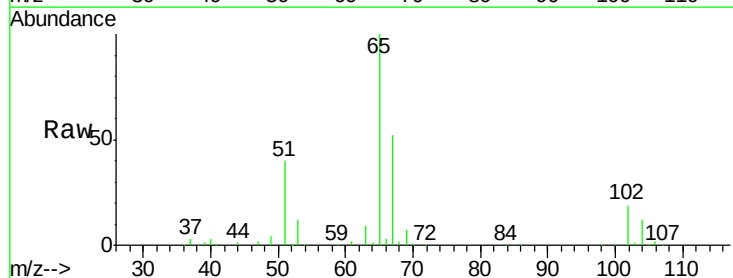

Abundance Ion 65.00 (64.70 to 65.70): VX0

Ion 67.00 (66.70 to 67.70): VX0



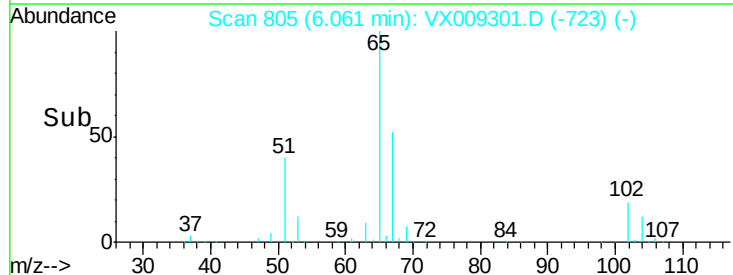
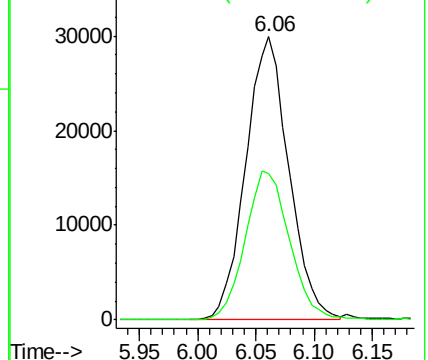


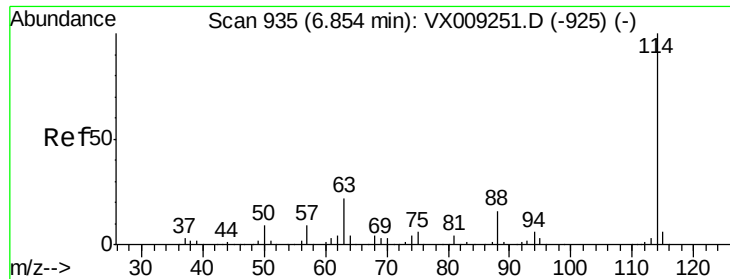

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 6.85 min Scan# 935
 Delta R.T. -0.00 min
 Lab File: VX009301.D
 Acq: 03 May 2019 10:27




Instrument :
 MSVOA_X
 ClientSampleId :
 VX0503WBL01


Tot Ion:114 Resp: 177797
 Ion Ratio Lower Upper
 114 100
 63 23.2 18.0 27.0
 88 16.1 13.4 20.0

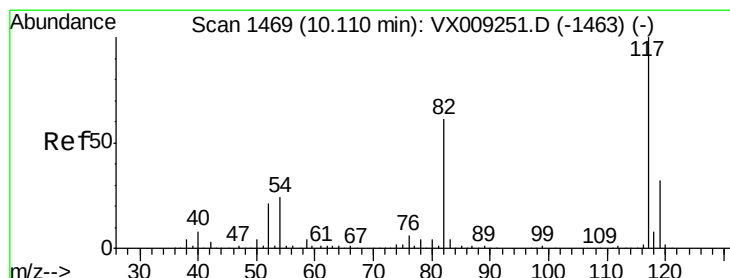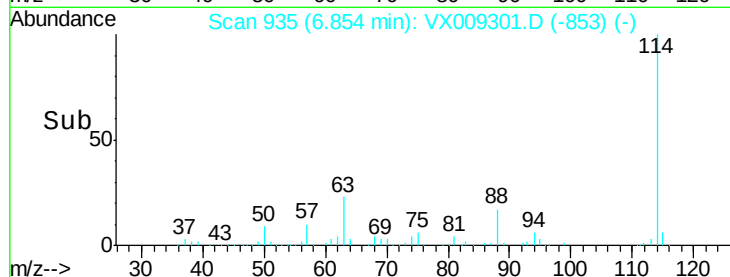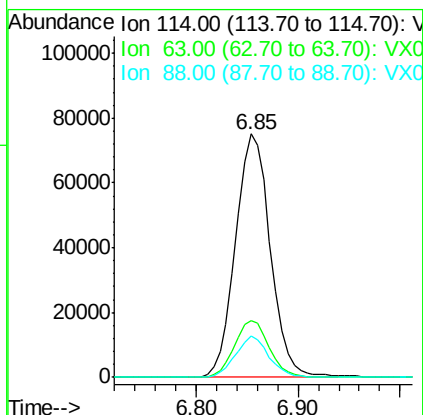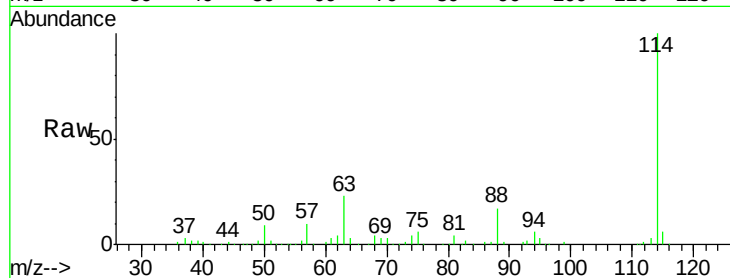

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 10.11 min Scan# 1469
 Delta R.T. -0.00 min
 Lab File: VX009301.D
 Acq: 03 May 2019 10:27

Tgt Ion:117 Resp: 151647
 Ion Ratio Lower Upper
 117 100
 82 58.6 47.8 71.8
 119 32.0 25.6 38.4

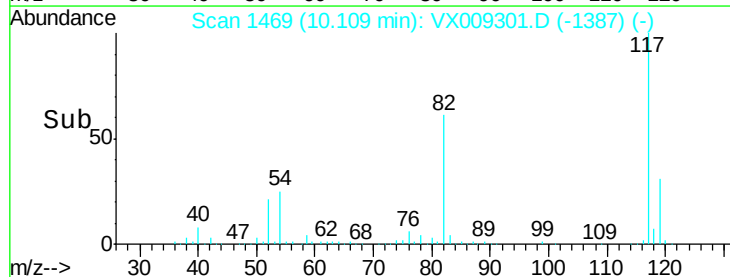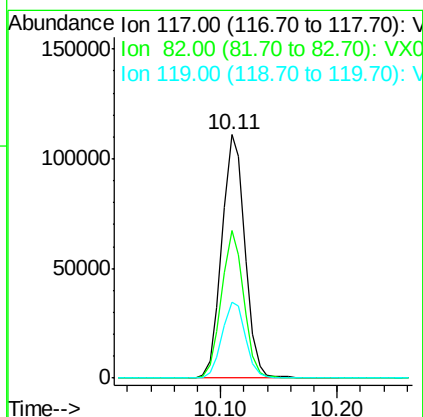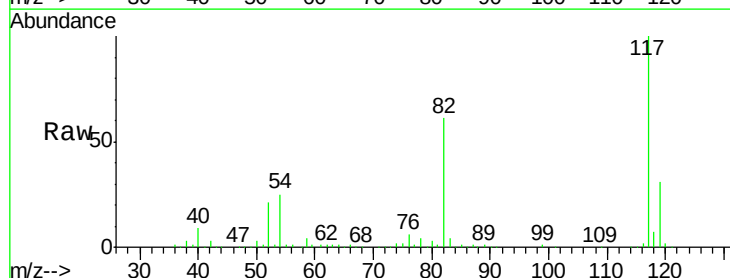


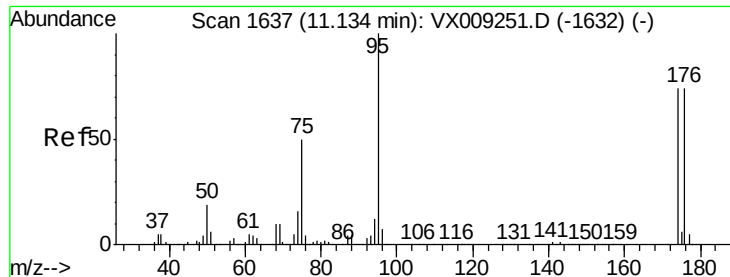




#60
 4-Bromofluorobenzene
 Concen: 27.182 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.00 min
 Lab File: VX009301.D
 Acq: 03 May 2019 10:27

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0503WBL01

Tot Ion: 95 Resp: 70043
 Ion Ratio Lower Upper
 95 100
 174 83.7 63.6 95.4
 176 79.5 62.4 93.6

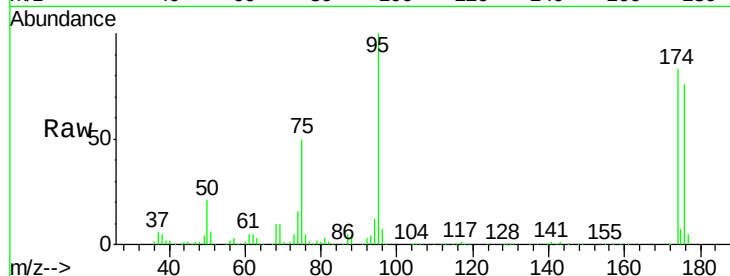


Abundance Ion 95.00 (94.70 to 95.70): VX0
 Ion 174.00 (173.70 to 174.70): V
 Ion 176.00 (175.70 to 176.70): V

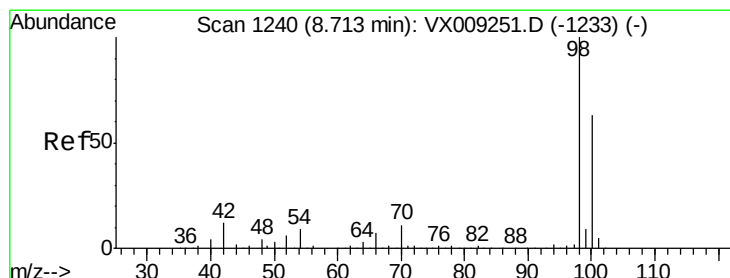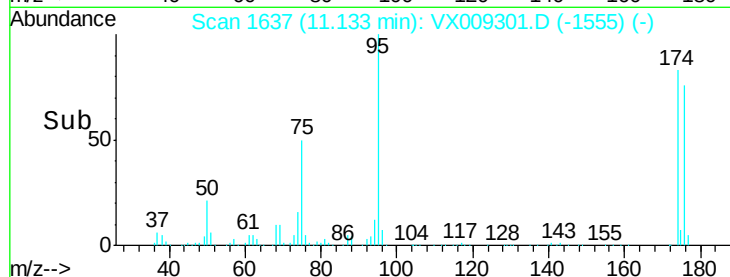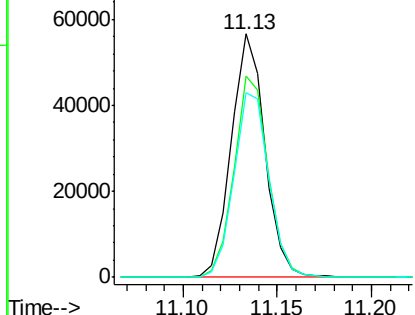

#63
 Toluene-d8
 Concen: 30.250 ug/l
 RT: 8.71 min Scan# 1240
 Delta R.T. -0.00 min
 Lab File: VX009301.D
 Acq: 03 May 2019 10:27

Tgt Ion: 98 Resp: 217489
 Ion Ratio Lower Upper
 98 100
 100 65.1 52.3 78.5

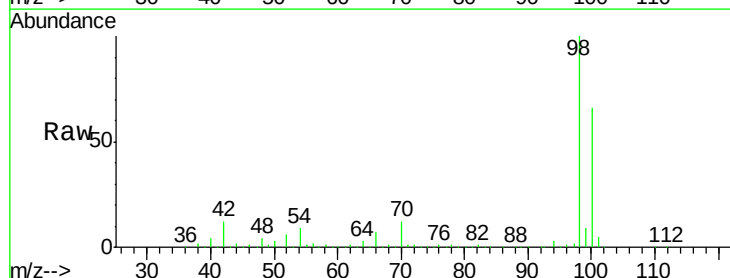

Abundance Ion 98.00 (97.70 to 98.70): VX0
 Ion 100.00 (99.70 to 100.70): V

