


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX050319\
Data File : VX009308.D
Acq On : 03 May 2019 14:08
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X042919W.M
Title : SW846 8260
Last Update : Sat May 04 07:18:36 2019

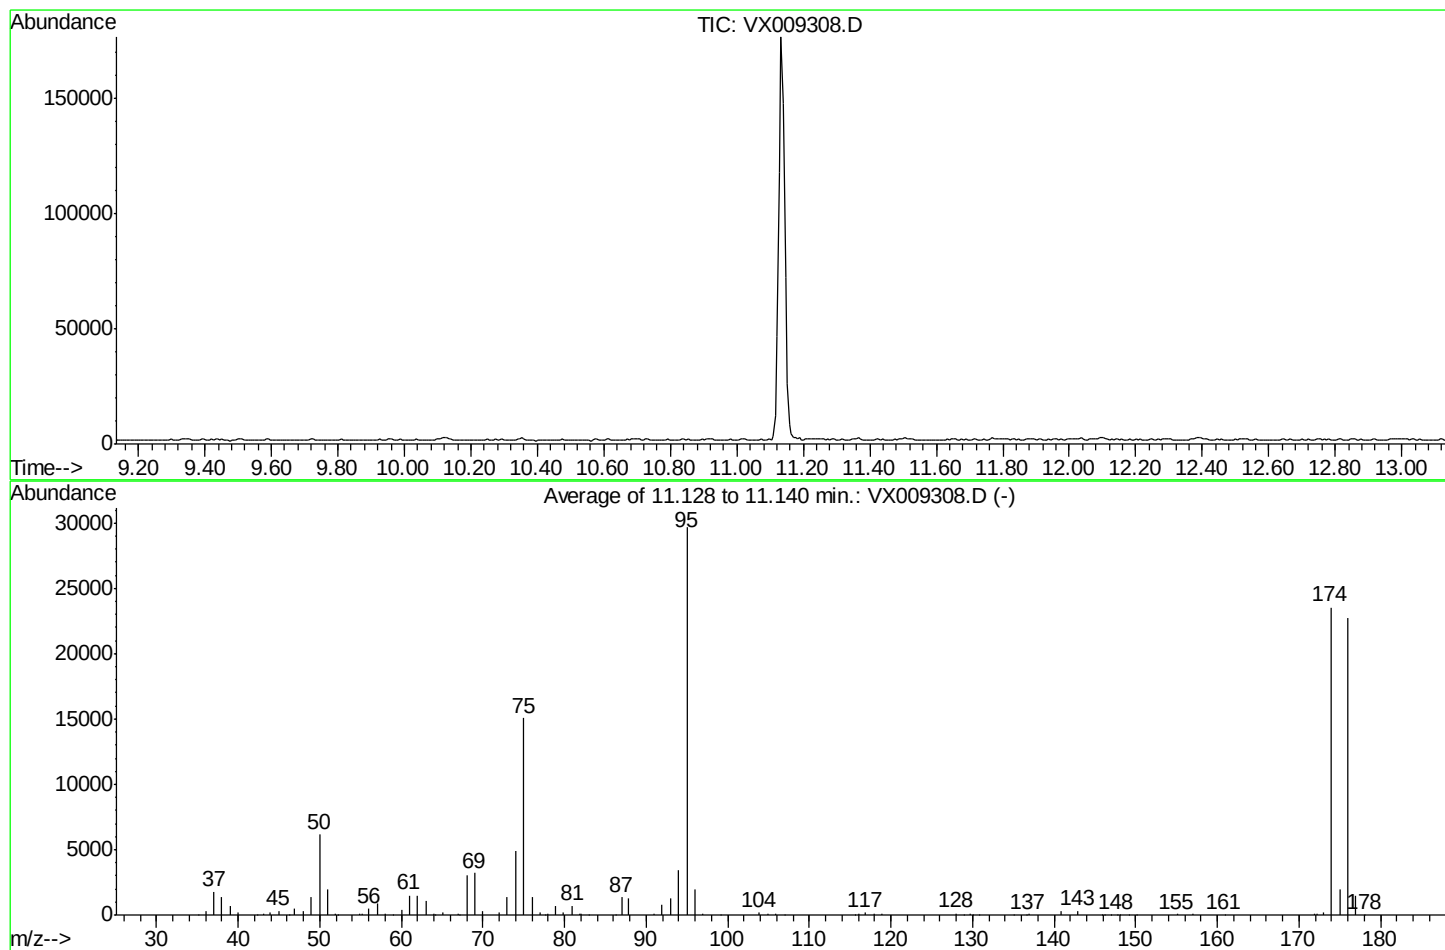

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	6130	PASS
75	95	30	60	50.7	15048	PASS
95	95	100	100	100.0	29661	PASS
96	95	5	9	6.5	1923	PASS
173	174	0.00	2	0.8	177	PASS
174	95	50	100	79.4	23556	PASS
175	174	5	9	8.3	1959	PASS
176	174	95	101	96.5	22733	PASS
177	176	5	9	6.6	1491	PASS