
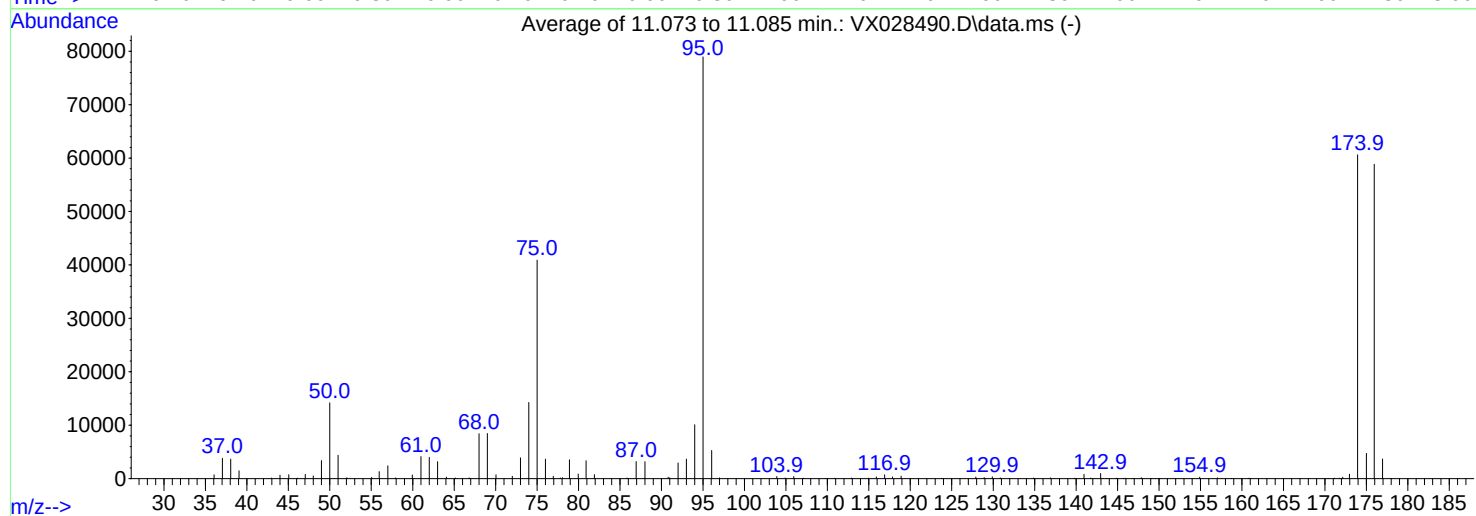


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050322\
 Data File : VX028490.D
 Acq On : 03 May 2022 09:42
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X041922W.M
 Title : SW846 8260
 Last Update : Tue Apr 19 13:38:04 2022

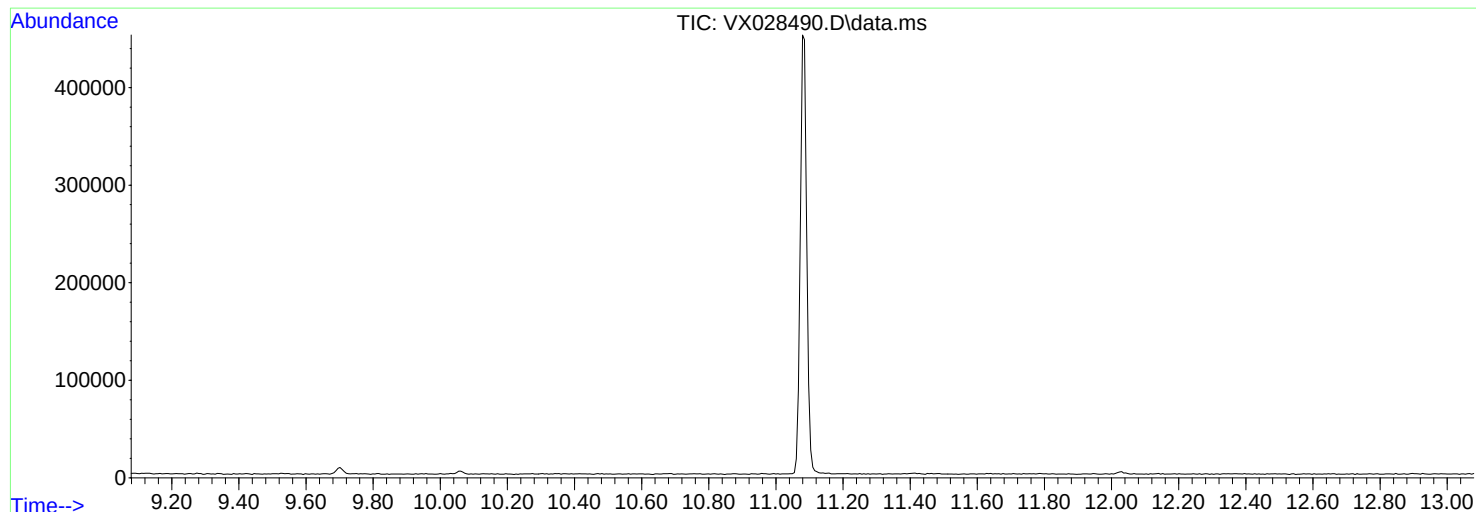

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	14209	PASS
75	95	30	60	51.8	40899	PASS
95	95	100	100	100.0	78949	PASS
96	95	5	9	6.7	5261	PASS
173	174	0.00	2	1.4	843	PASS
174	95	50	100	76.8	60605	PASS
175	174	5	9	7.8	4741	PASS
176	174	95	101	97.1	58843	PASS
177	176	5	9	6.3	3685	PASS