

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050323\
 Data File : VX035506.D
 Acq On : 03 May 2023 13:51
 Operator : JC/MD
 Sample : 02583-01
 Misc : 18.36g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 CF-21

Quant Time: May 04 03:56:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 25 16:31:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	219094	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	359394	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	328561	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	153507	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	129270	48.906	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	97.820%
35) Dibromofluoromethane	5.385	113	102210	46.336	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.680%
50) Toluene-d8	8.647	98	420475	50.530	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	101.060%
62) 4-Bromofluorobenzene	11.085	95	162784	52.003	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	104.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050323\
Data File : VX035506.D
Acq On : 03 May 2023 13:51
Operator : JC/MD
Sample : 02583-01
Misc : 18.36g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
CF-21

Quant Time: May 04 03:56:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X042523W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 25 16:31:40 2023
Response via : Initial Calibration




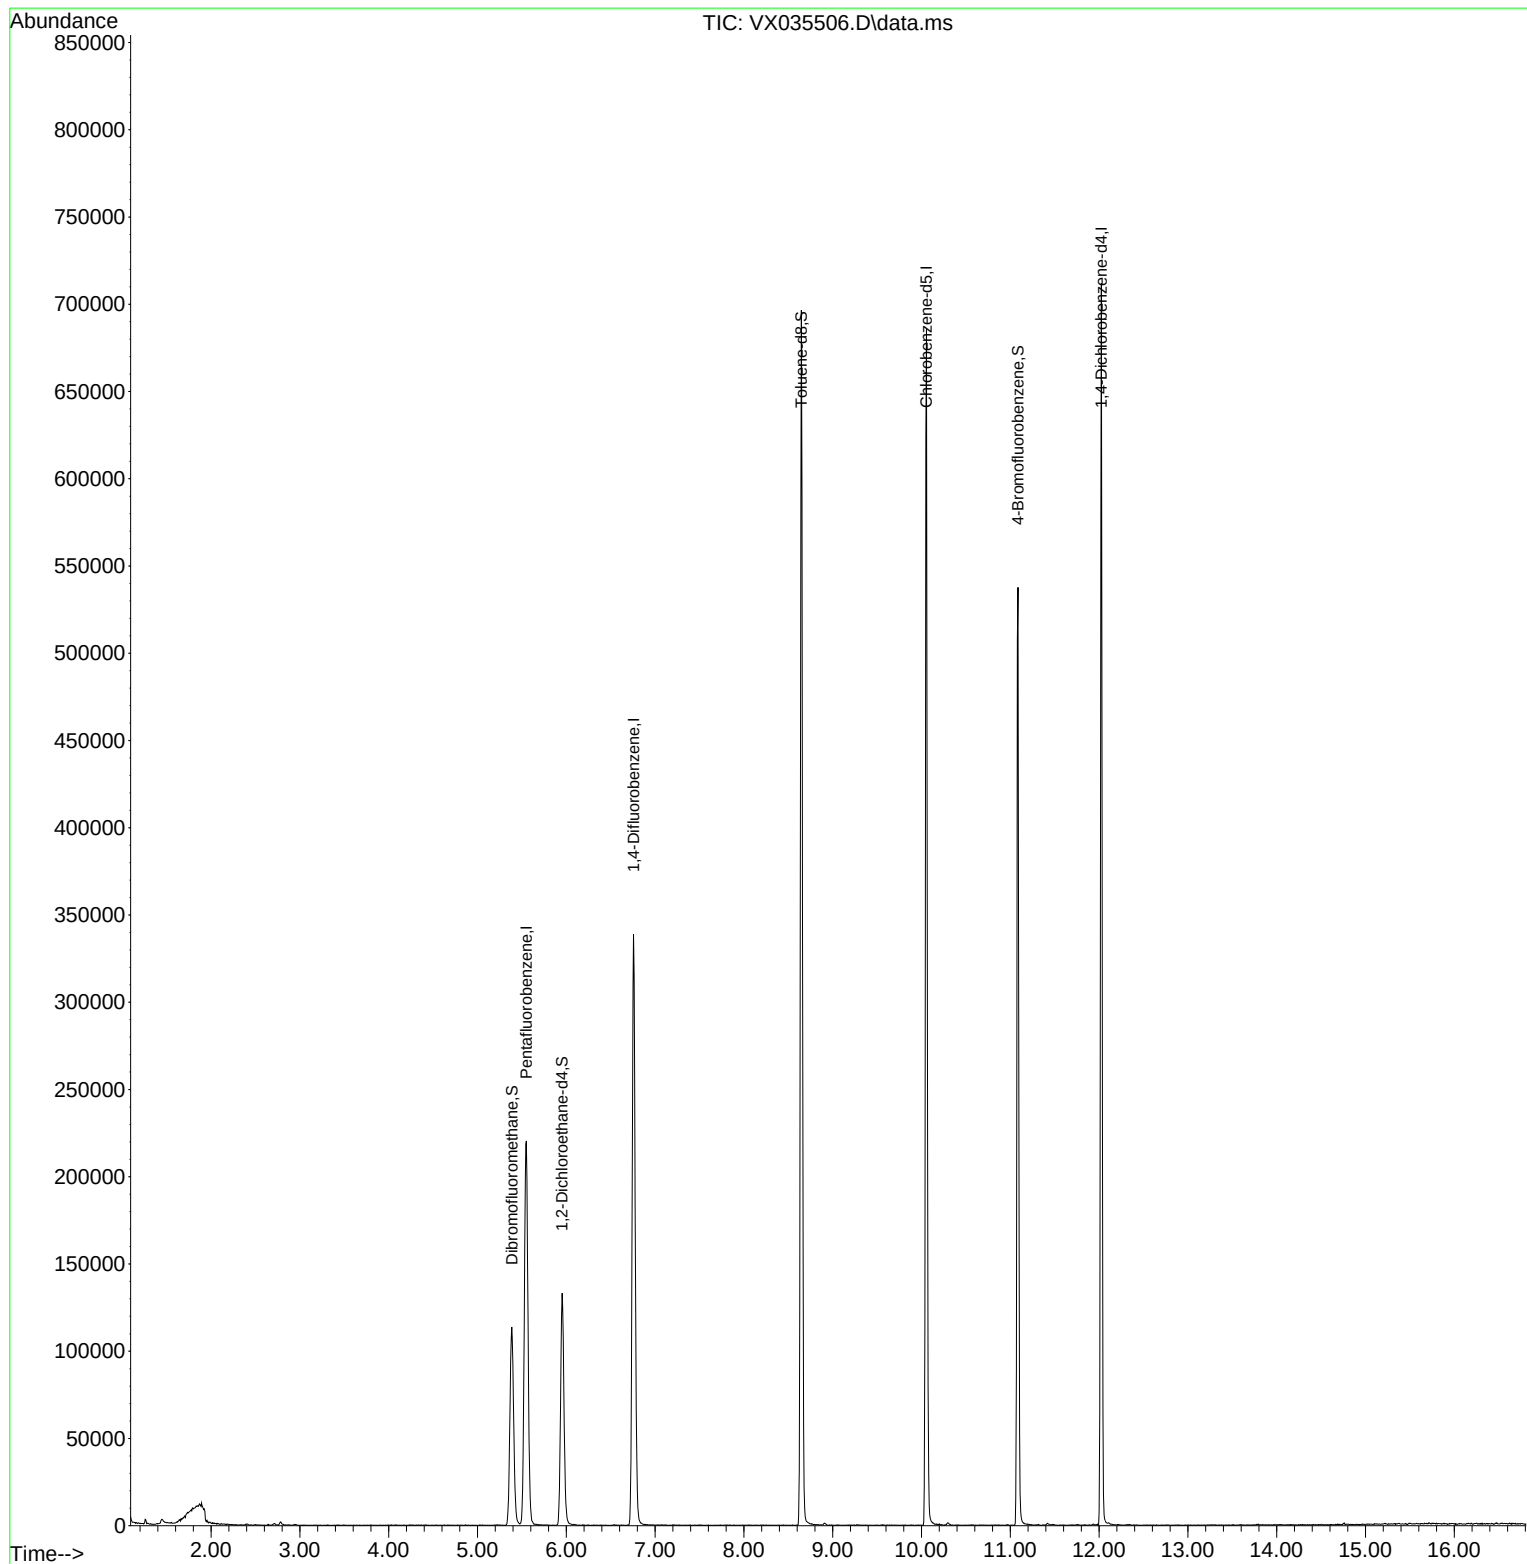


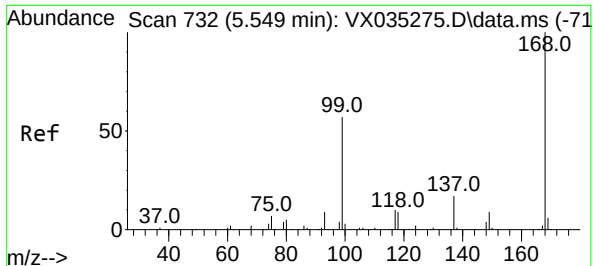

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.001 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51




Instrument :
MSVOA_X
ClientSampleId :
CF-21


Tgt Ion:168 Resp: 219094
Ion Ratio Lower Upper
168 100
99 55.6 45.7 68.5

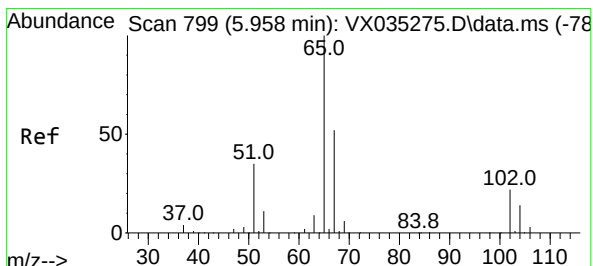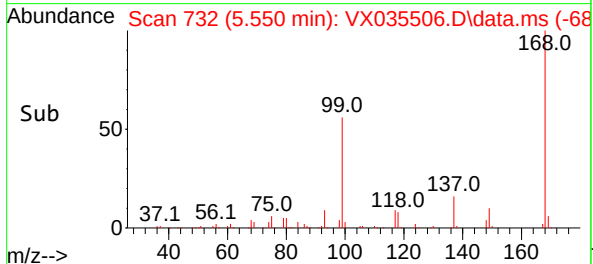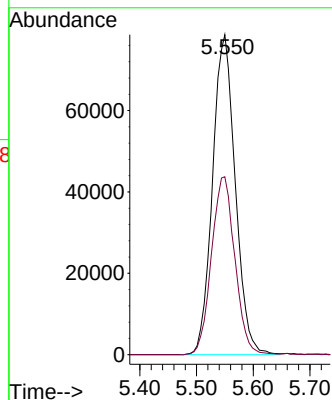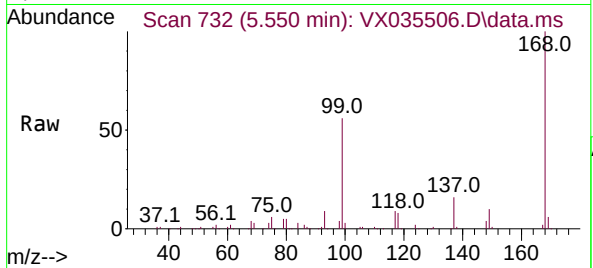

#33
1,2-Dichloroethane-d4
Concen: 48.906 ug/l
RT: 5.952 min Scan# 798
Delta R.T. -0.006 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51

Tgt Ion: 65 Resp: 129270
Ion Ratio Lower Upper
65 100
67 51.5 0.0 104.0


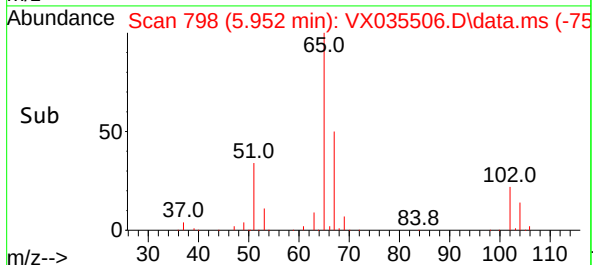
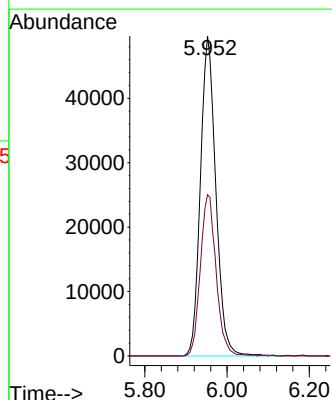
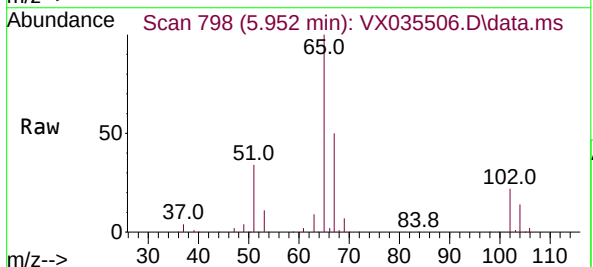


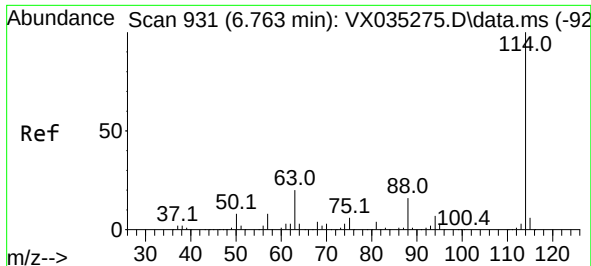

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. -0.006 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51




Instrument :
MSVOA_X
ClientSampleId :
CF-21


Tgt Ion:114 Resp: 359394
Ion Ratio Lower Upper
114 100
63 19.5 0.0 42.2
88 16.1 0.0 33.2

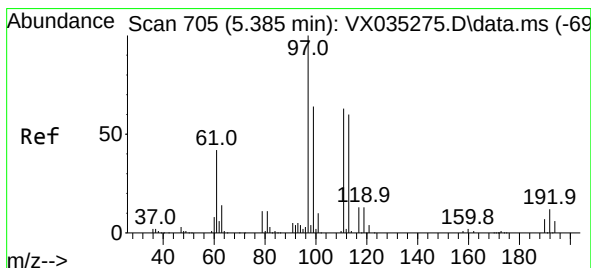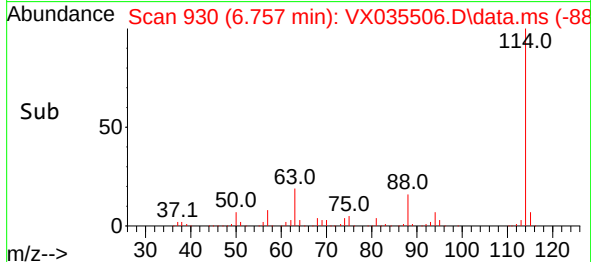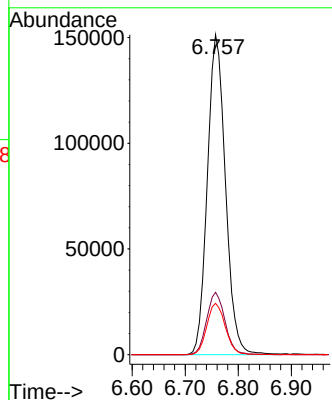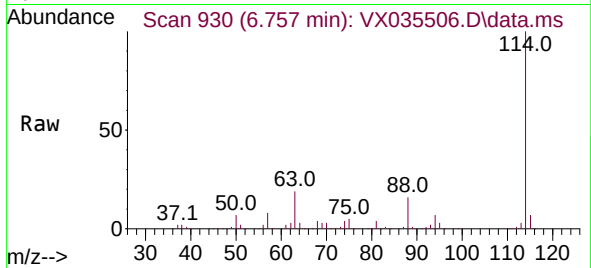

#35
Dibromofluoromethane
Concen: 46.336 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51

Tgt Ion:113 Resp: 102210
Ion Ratio Lower Upper
113 100
111 102.0 83.7 125.5
192 20.7 15.4 23.2


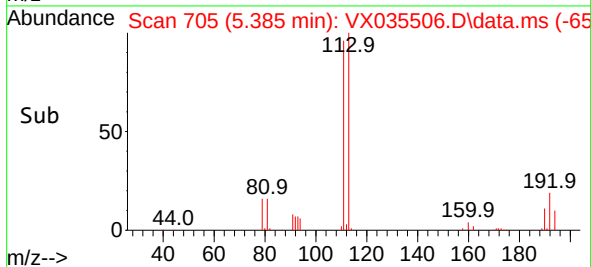
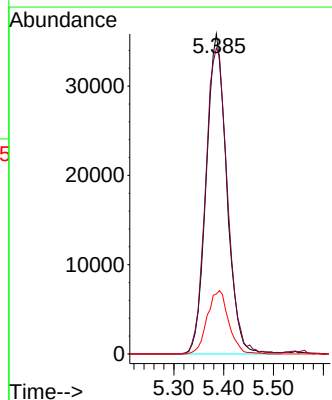
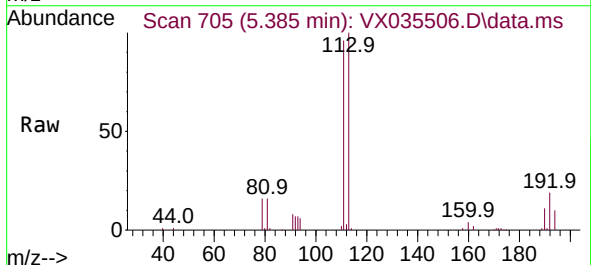


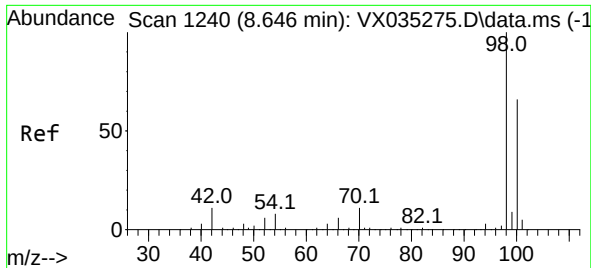

#50
Toluene-d8
Concen: 50.530 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.001 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51




Instrument :
MSVOA_X
ClientSampleId :
CF-21


Tgt Ion: 98 Resp: 420475
Ion Ratio Lower Upper
98 100
100 66.8 52.5 78.7

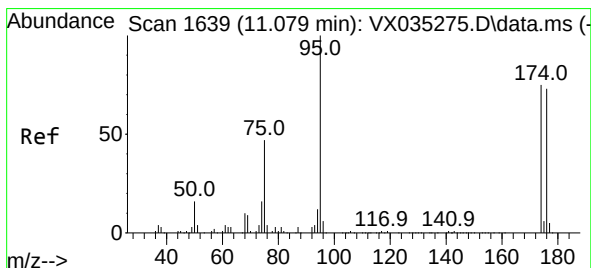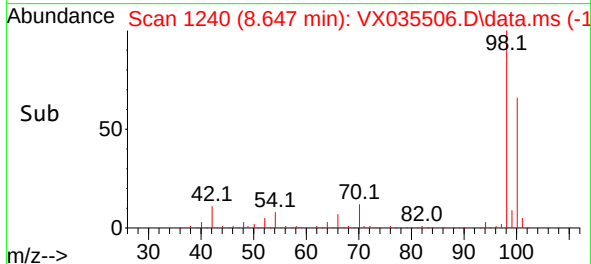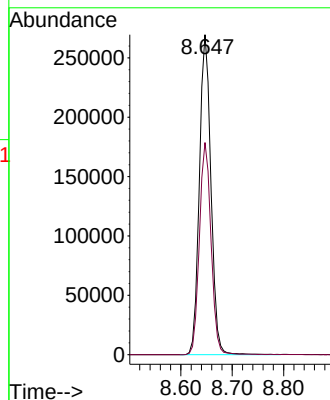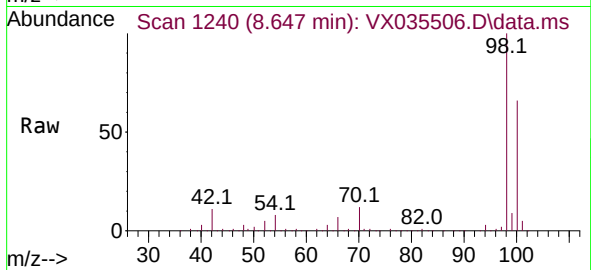

#62
4-Bromofluorobenzene
Concen: 52.003 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.006 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51

Tgt Ion: 95 Resp: 162784
Ion Ratio Lower Upper
95 100
174 79.0 0.0 147.4
176 76.6 0.0 140.6


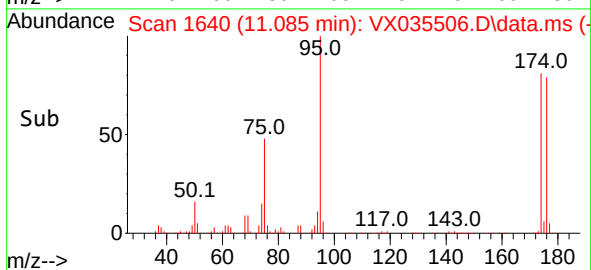
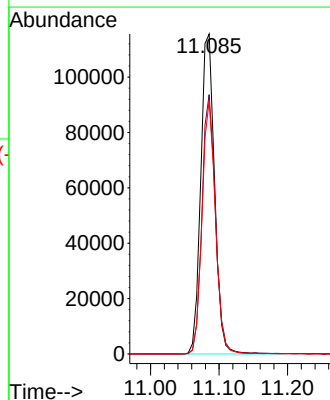
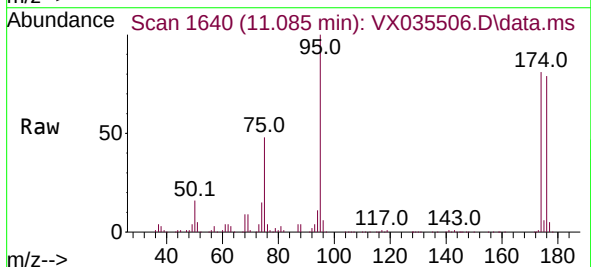


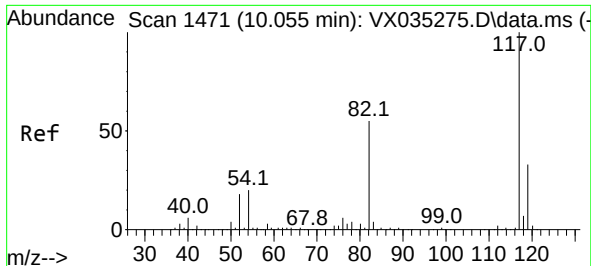

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51

Instrument :
MSVOA_X
ClientSampleId :
CF-21

Tgt Ion:117 Resp: 328561
Ion Ratio Lower Upper
117 100
82 55.7 45.0 67.4
119 33.2 26.0 39.0

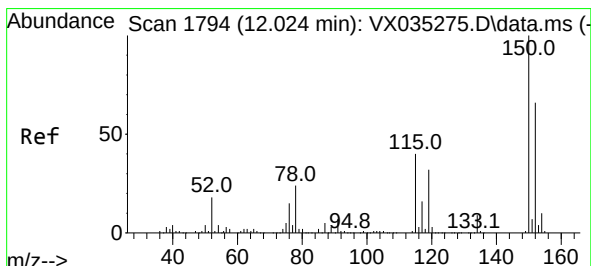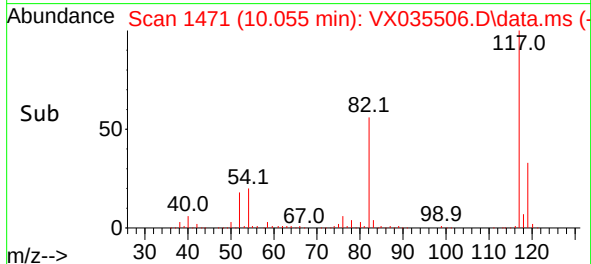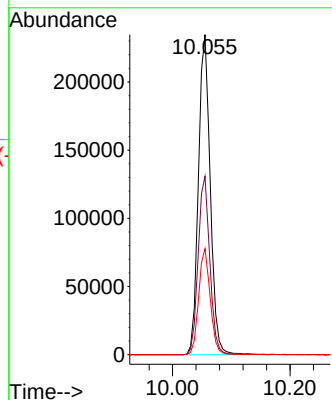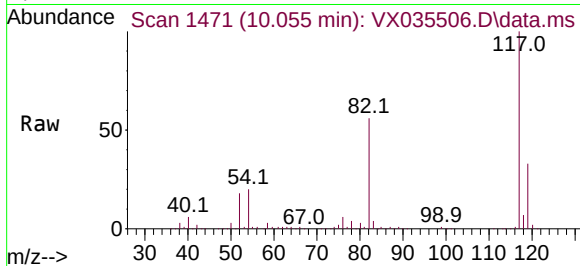

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX035506.D
Acq: 03 May 2023 13:51

Tgt Ion:152 Resp: 153507
Ion Ratio Lower Upper
152 100
115 60.1 45.0 135.0
150 158.8 0.0 352.4

