
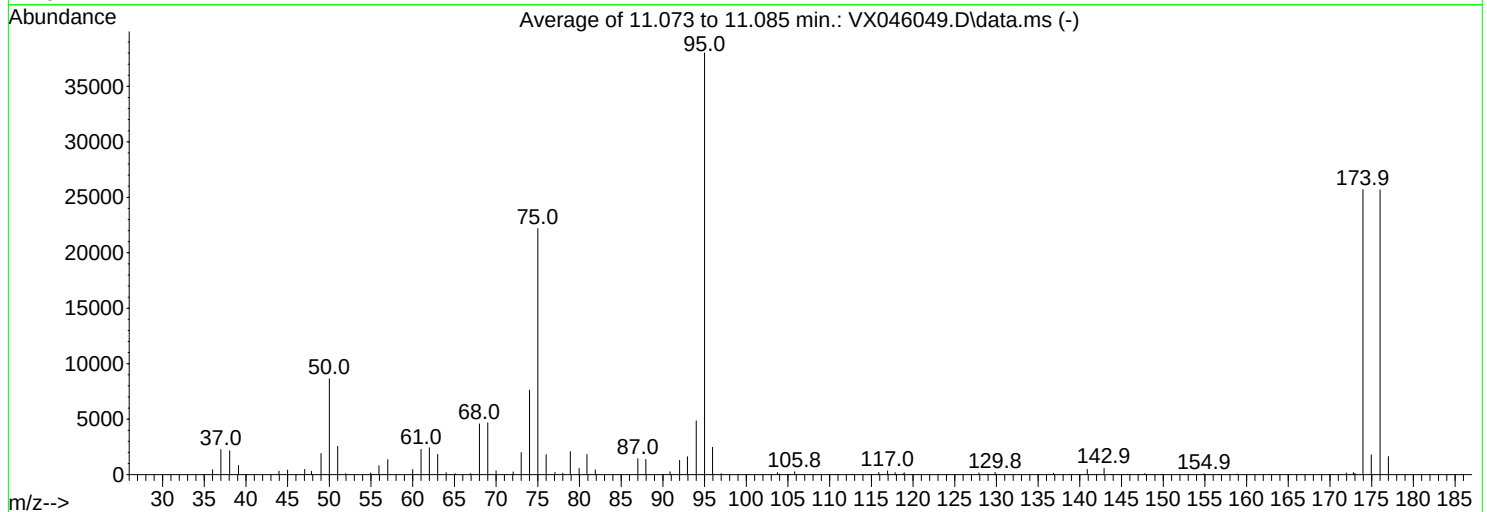


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050625\
Data File : VX046049.D
Acq On : 06 May 2025 09:07
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Title : SW846 8260
Last Update : Tue May 06 07:12:22 2025

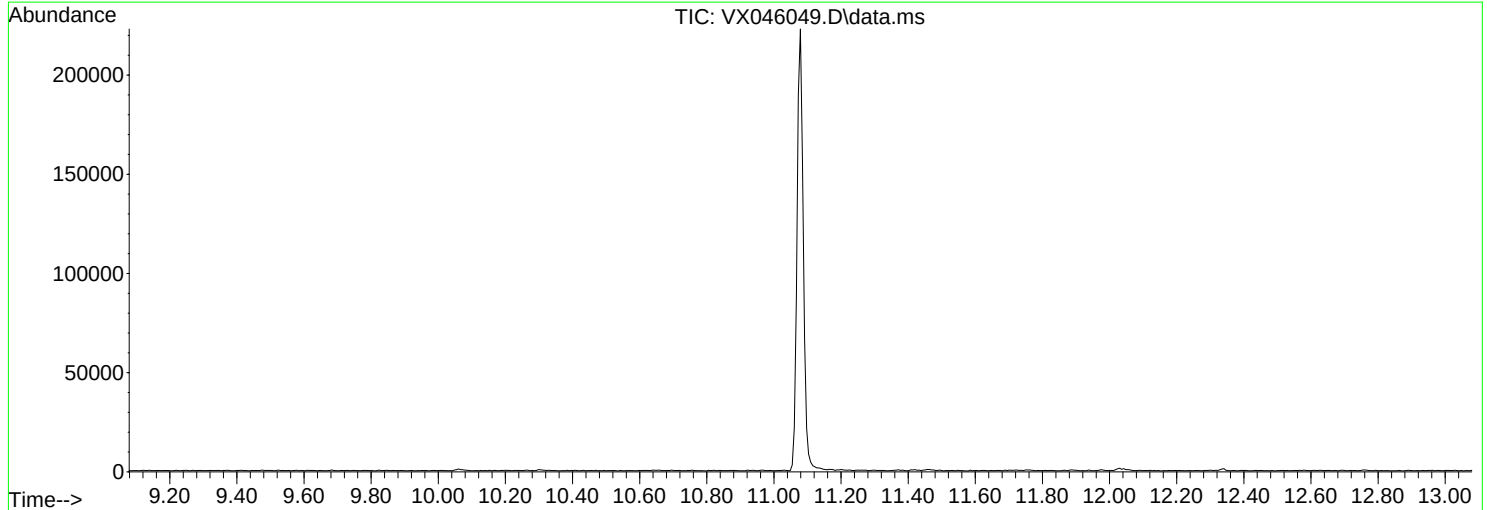

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.7	8636	PASS
75	95	30	60	58.3	22187	PASS
95	95	100	100	100.0	38024	PASS
96	95	5	9	6.5	2473	PASS
173	174	0.00	2	0.7	186	PASS
174	95	50	100	67.6	25701	PASS
175	174	5	9	6.9	1783	PASS
176	174	95	101	99.9	25680	PASS
177	176	5	9	6.3	1624	PASS