


Acrolein

Response Ratio

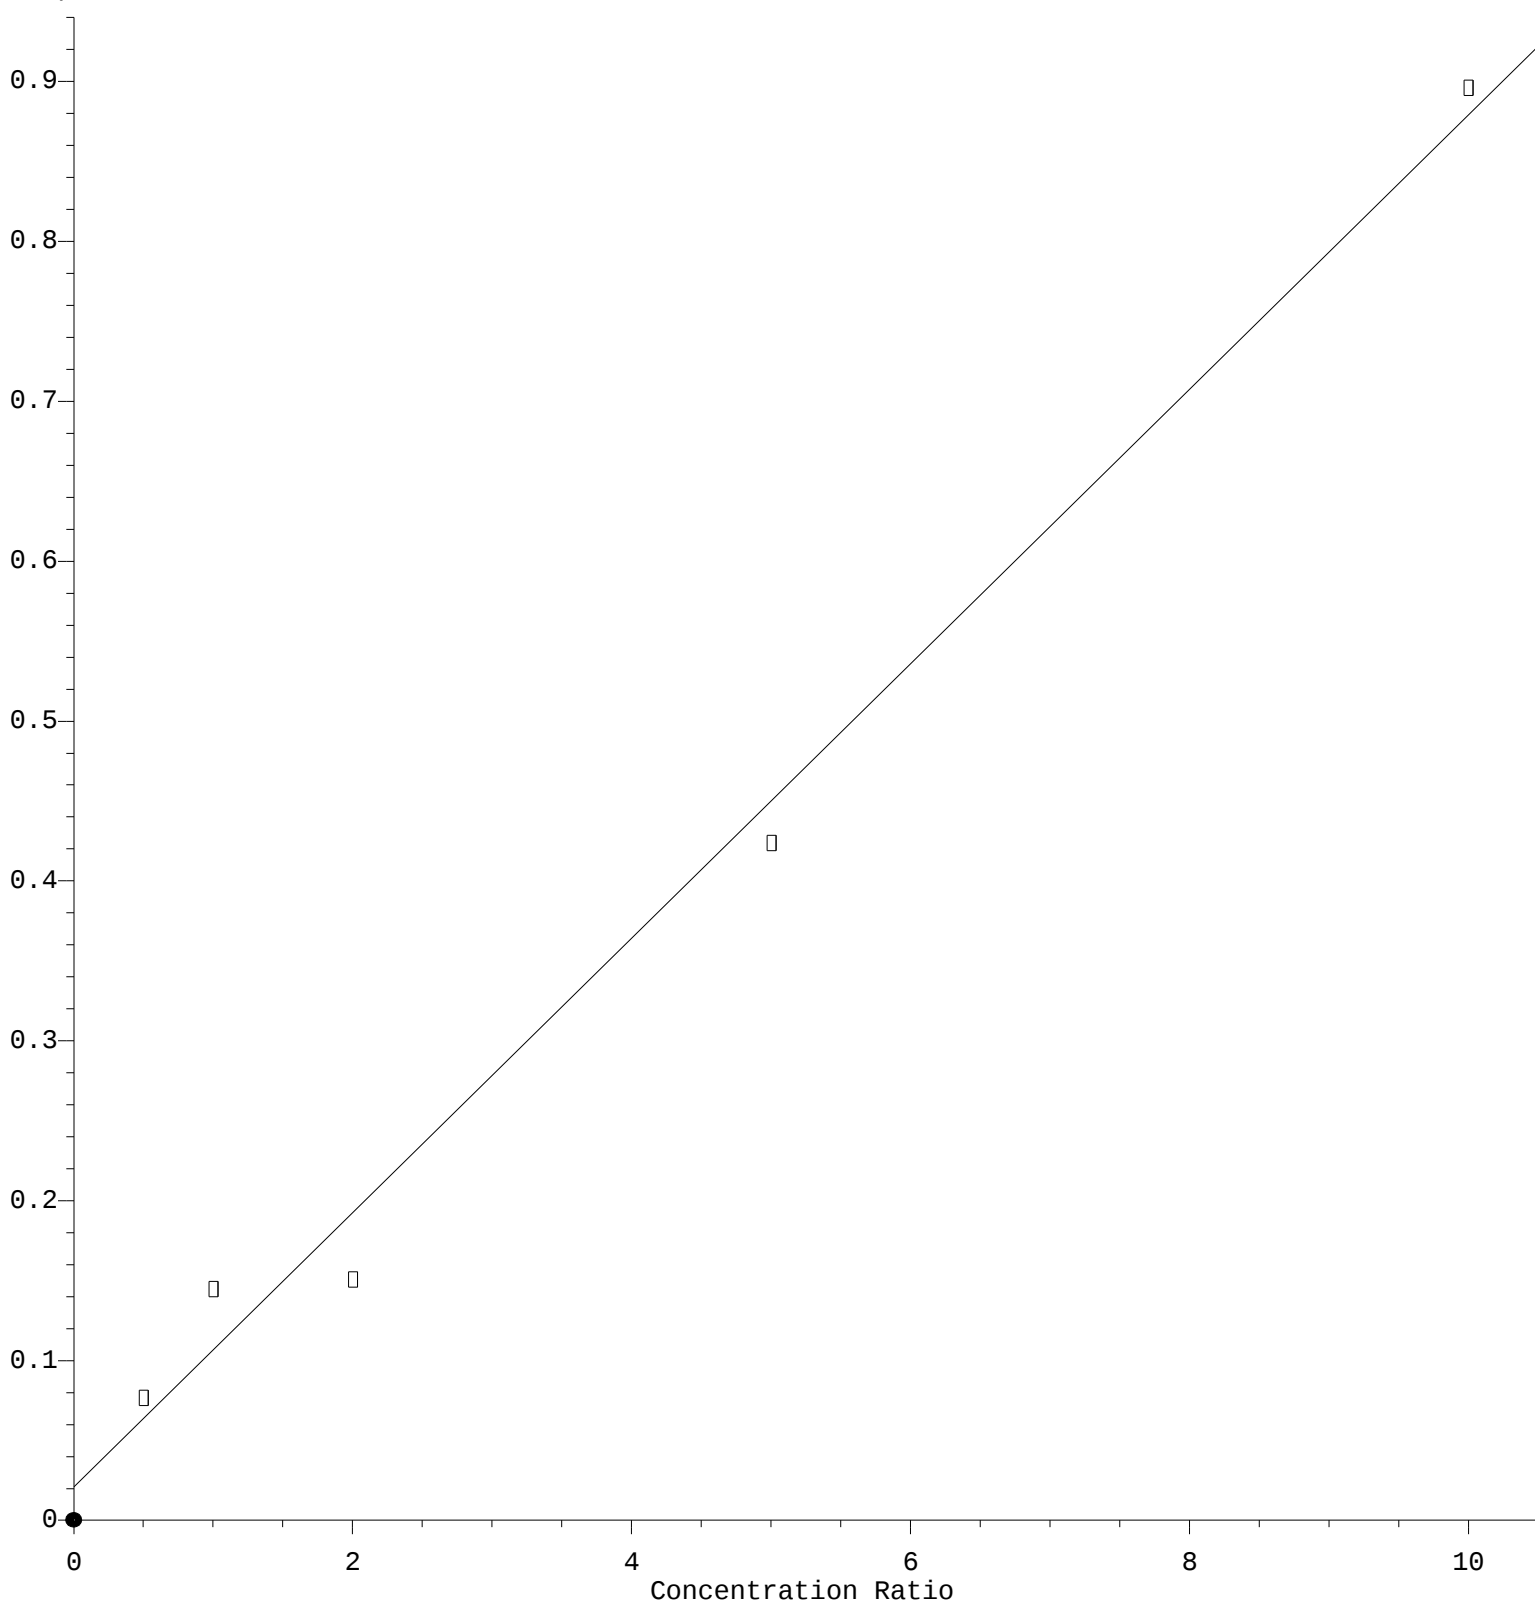

$$\text{Response} = 8.582\text{e-}002 * \text{Amt} + 2.081\text{e-}002$$


Coef of Det (r^2) = 0.990547 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M

Calibration Table Last Updated: Sat May 08 05:38:18 2021

Methylene Chloride

Response Ratio

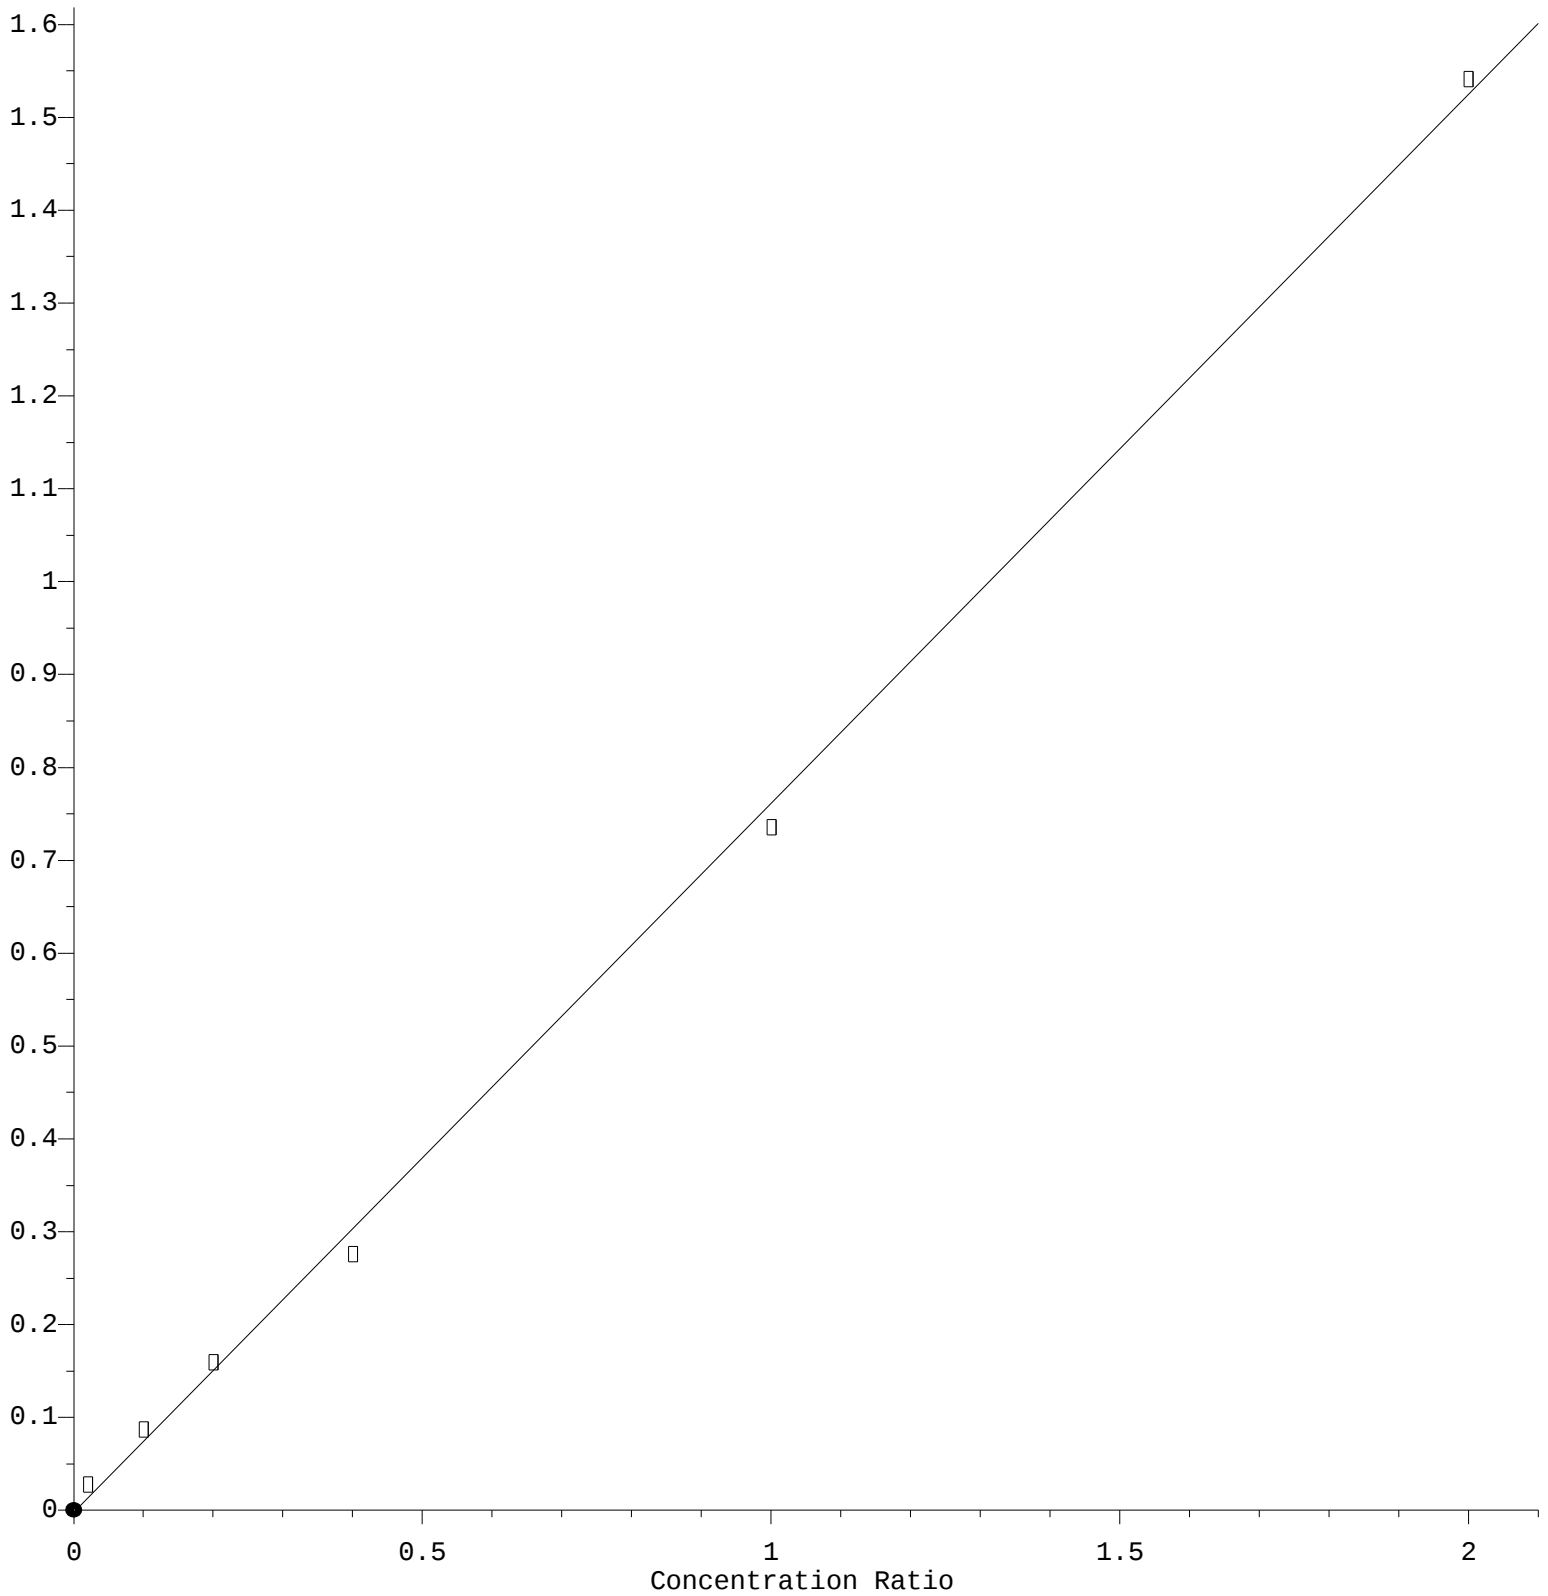


$$\text{Response} = 7.633\text{e-}001 * \text{Amt} - 2.233\text{e-}003$$

Coef of Det (r^2) = 0.998729 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M

Calibration Table Last Updated: Sat May 08 05:38:18 2021

1,2-Dibromo-3-Chloropropane

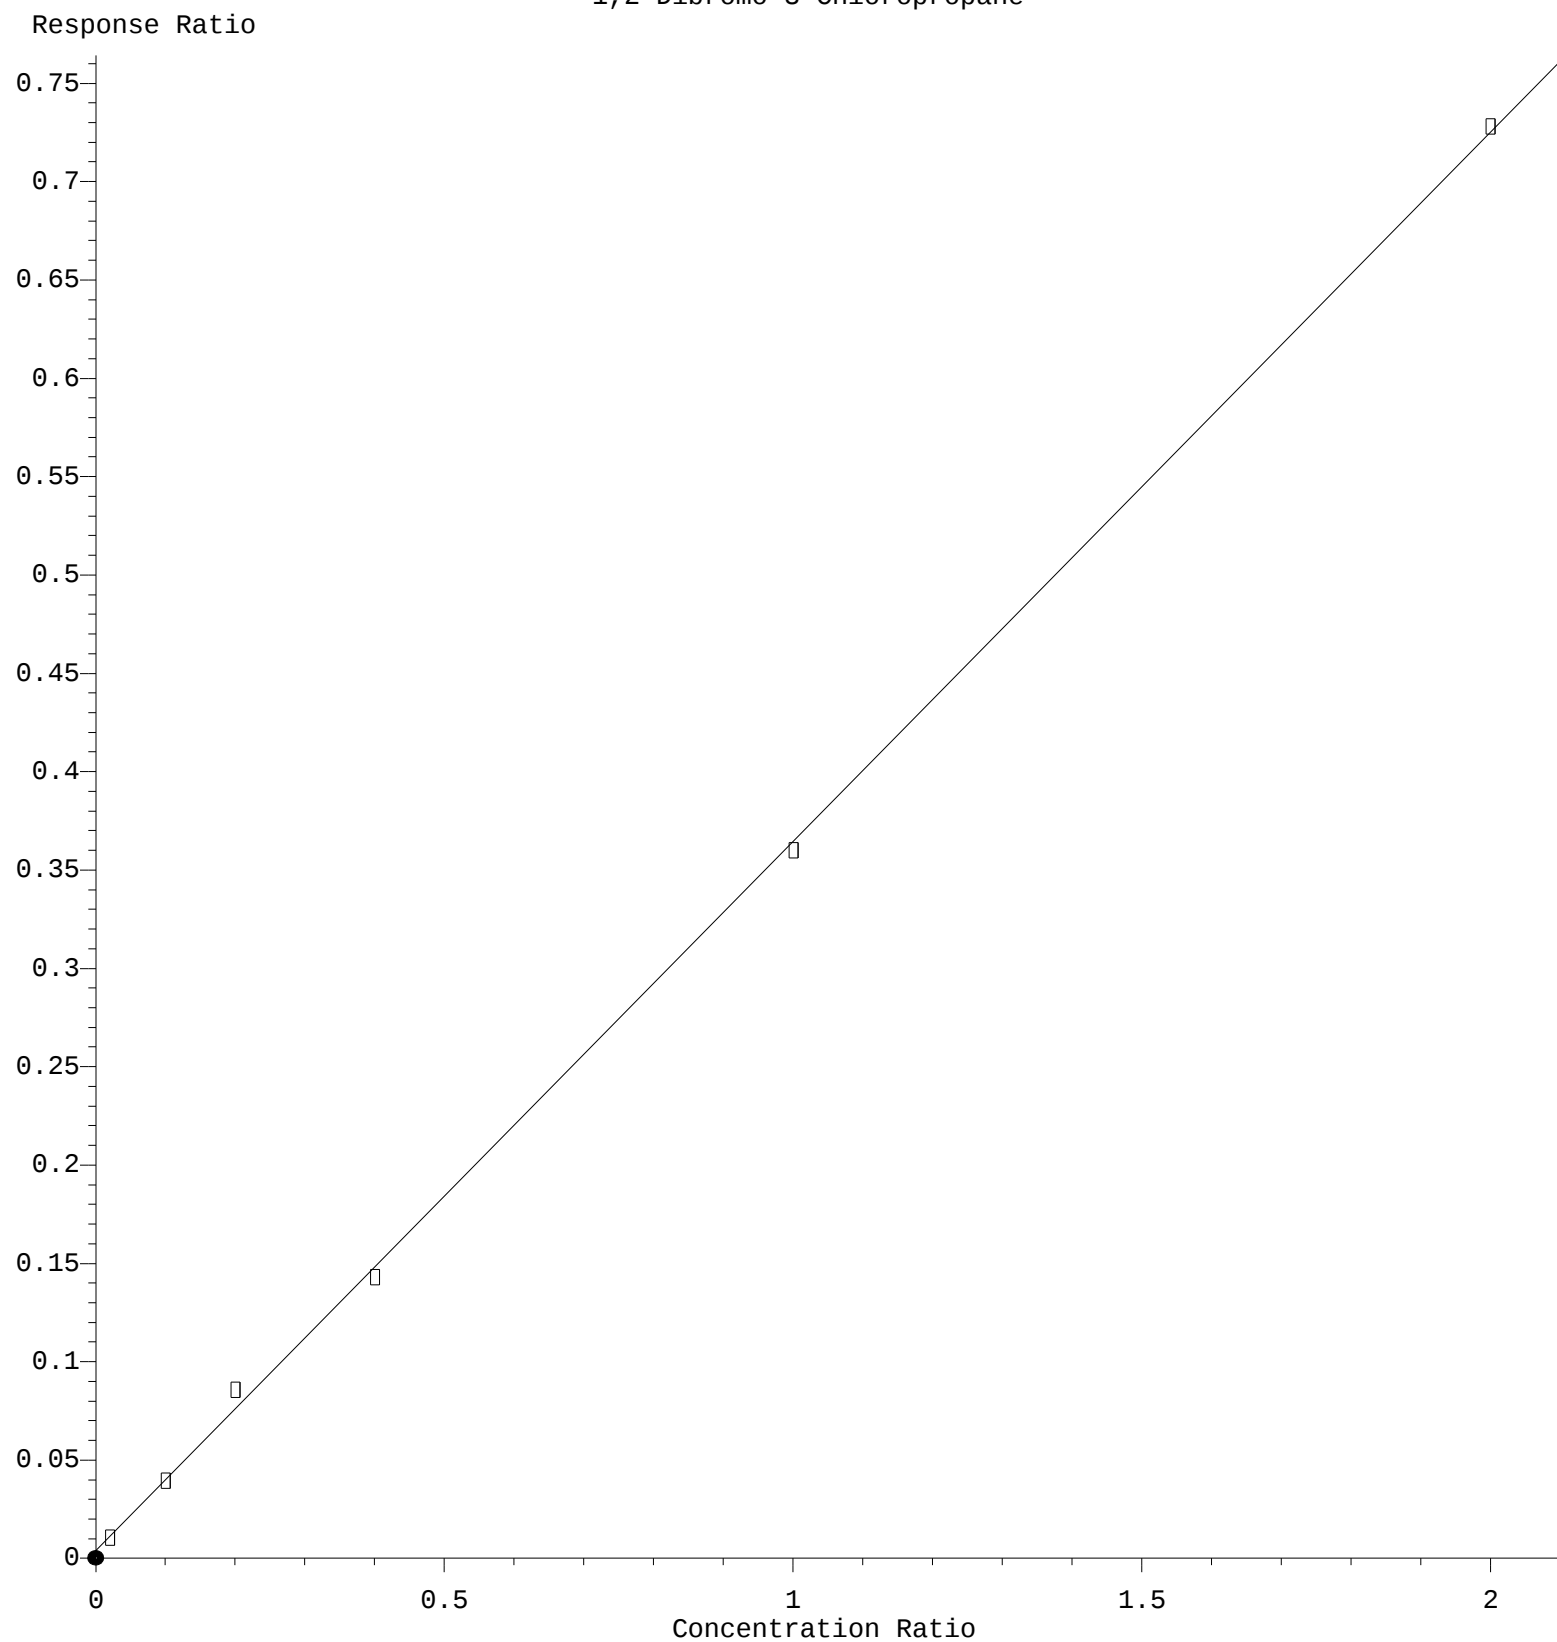

Response = $3.606 \times 10^{-1} \times \text{Amt} + 4.096 \times 10^{-3}$
 Coef of Det (r^2) = 0.999608 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050721W.M
 Calibration Table Last Updated: Sat May 08 05:38:18 2021