

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
 Data File : VX041398.D
 Acq On : 07 May 2024 11:47
 Operator : JC/MD
 Sample : P2354-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: May 08 01:57:02 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 01 02:38:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	182766	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.757	114	270416	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	265597	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	138443	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	98006	49.258	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	98.520%		
35) Dibromofluoromethane	5.379	113	80633	44.001	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.000%		
50) Toluene-d8	8.647	98	306696	52.878	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	105.760%		
62) 4-Bromofluorobenzene	11.079	95	118693	52.864	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	105.720%		
Target Compounds						
						Qvalue
5) Bromomethane	1.599	94	616	0.663	ug/l	99
10) Methyl Iodide	2.447	142	377	0.244	ug/l	# 80
11) Tert butyl alcohol	3.007	59	2866	7.197	ug/l	# 95
13) Acrolein	2.239	56	76	0.241	ug/l	# 50
14) Allyl chloride	2.660	41	513	0.216	ug/l	# 46
15) Acrylonitrile	3.081	53	251	0.276	ug/l	# 61
16) Acetone	2.386	43	18986	18.040	ug/l	96
17) Carbon Disulfide	2.501	76	1452	0.436	ug/l	# 87
18) Methyl Acetate	2.709	43	1789	0.879	ug/l	98
20) Methylene Chloride	2.782	84	4847	2.806	ug/l	89
25) 2-Butanone	4.568	43	13612	10.570	ug/l	99
29) Tetrahydrofuran	5.025	42	1536	1.824	ug/l	# 59
31) Cyclohexane	5.537	56	3068	1.278	ug/l	# 1
36) 1,1-Dichloropropene	5.544	75	11332	5.171	ug/l	# 51
37) Ethyl Acetate	4.568	43	13612	4.979	ug/l	# 69
38) Carbon Tetrachloride	5.544	117	15659	6.238	ug/l	# 15
41) Methacrylonitrile	5.025	41	980	0.696	ug/l	# 31
43) Isopropyl Acetate	6.342	43	58834	14.312	ug/l	98
48) Methyl methacrylate	7.622	41	1469	0.780	ug/l	# 10
51) 4-Methyl-2-Pentanone	8.549	43	49556	20.090	ug/l	# 48
52) Toluene	8.720	92	1886	0.456	ug/l	95
54) cis-1,3-Dichloropropene	8.549	75	21289	9.045	ug/l	# 57
56) Ethyl methacrylate	9.238	69	626	0.254	ug/l	# 1
57) 1,3-Dichloropropane	9.488	76	723	0.272	ug/l	# 42
59) 2-Hexanone	9.439	43	6775	3.435	ug/l	96
76) 1,2,3-Trichloropropane	11.079	75	60061	26.621	ug/l	# 38
81) trans-1,4-Dichloro-2-b...	11.079	75	60061	72.511	ug/l	# 5
84) 1,2,4-Trimethylbenzene	11.750	105	3016	0.435	ug/l	92
89) n-Butylbenzene	12.317	91	1235	0.202	ug/l	# 9
90) Hexachloroethane	12.554	117	622	0.490	ug/l	# 17
93) 1,2,4-Trichlorobenzene	13.597	180	647	0.202	ug/l	89
95) Naphthalene	13.780	128	20334	2.144	ug/l	99
96) 1,2,3-Trichlorobenzene	13.963	180	692	0.212	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041398.D
Acq On : 07 May 2024 11:47
Operator : JC/MD
Sample : P2354-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: May 08 01:57:02 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260
QLast Update : Wed May 01 02:38:17 2024
Response via : Initial Calibration




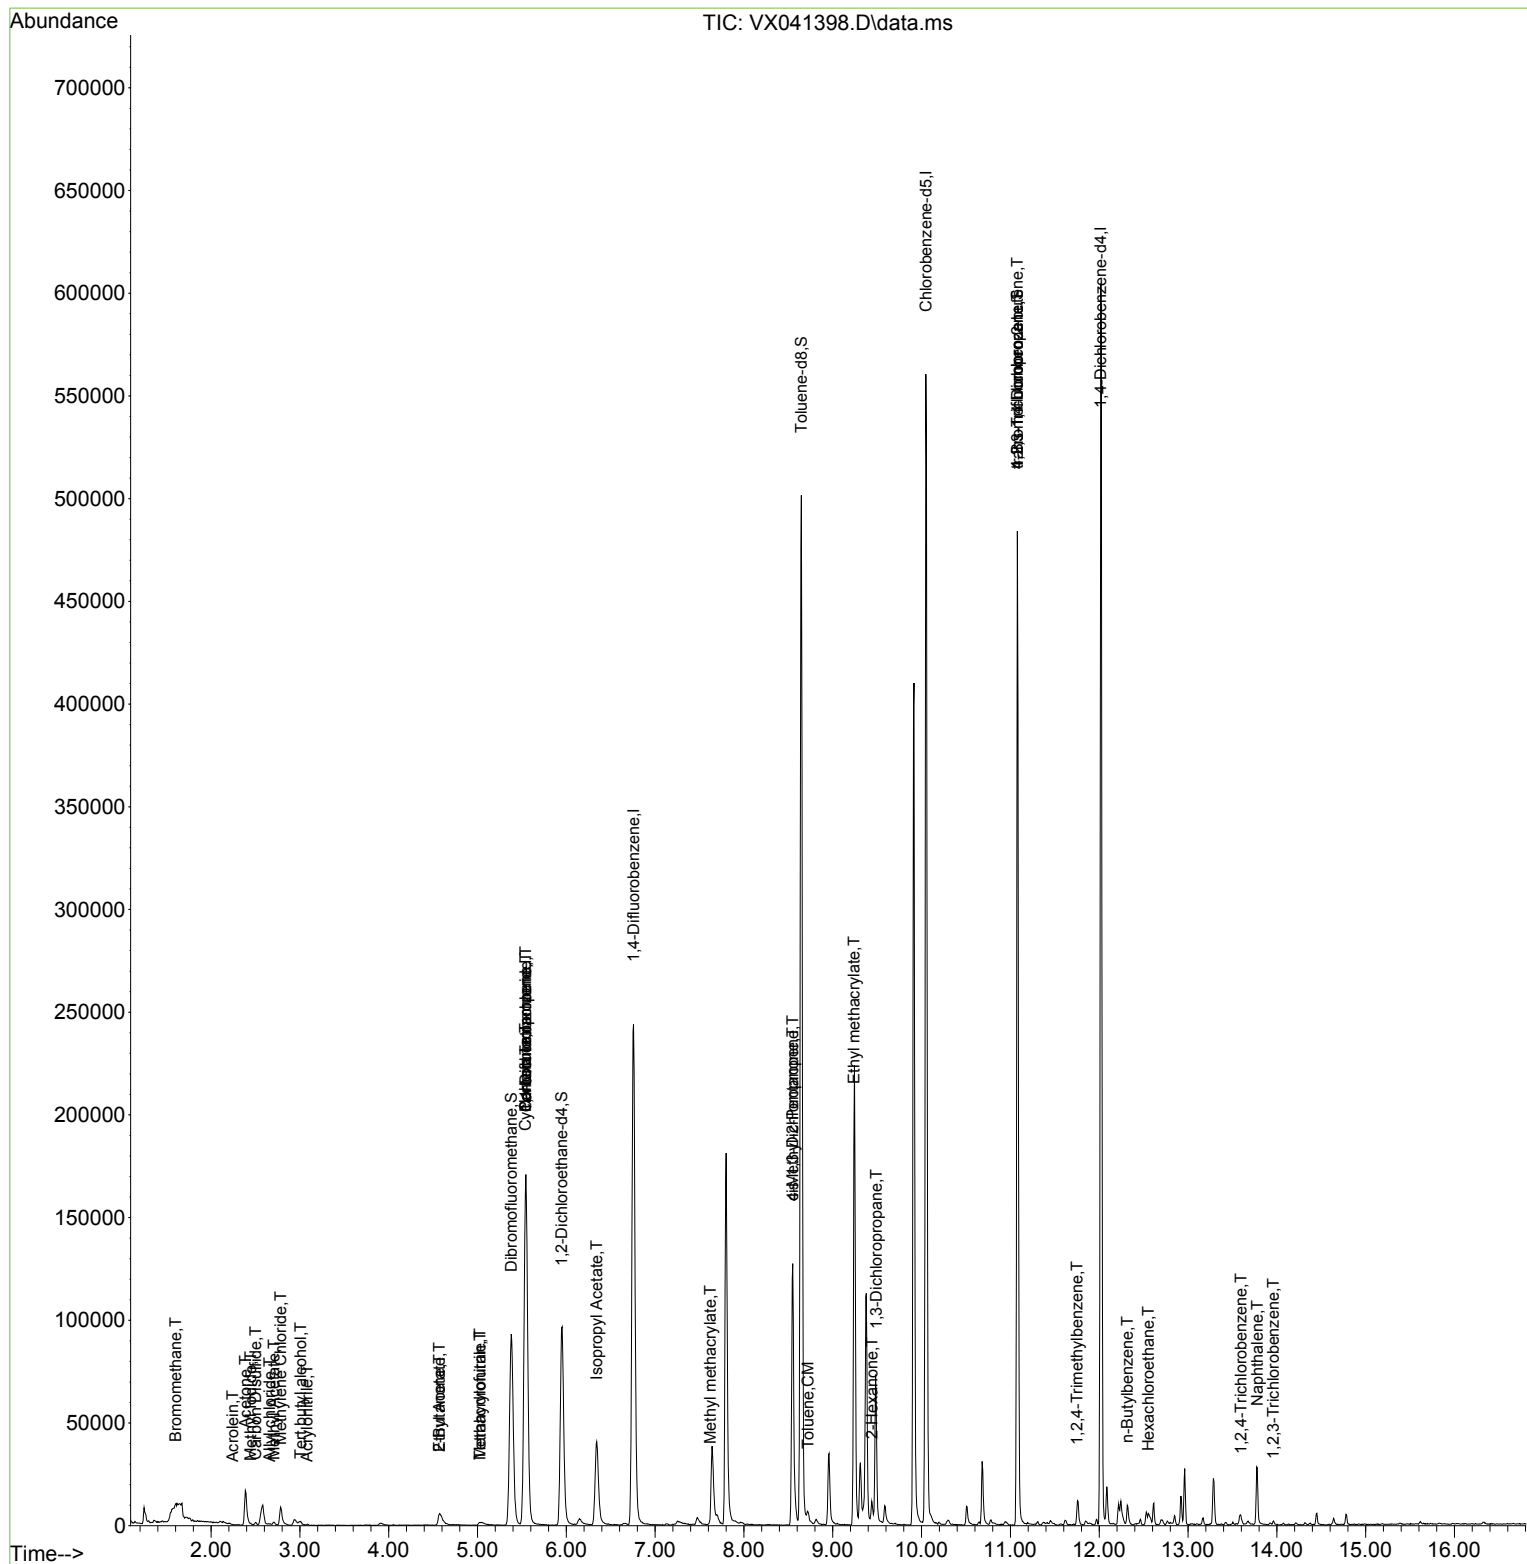




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion:168 Resp: 182766
Ion Ratio Lower Upper
168 100
99 49.3 56.6 85.0#



#5
Bromomethane
Concen: 0.663 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47


Tgt Ion: 94 Resp: 616
Ion Ratio Lower Upper
94 100
96 93.9 74.6 111.8








#10
Methyl Iodide
Concen: 0.244 ug/l
RT: 2.447 min Scan# 21
Delta R.T. -0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion:142 Resp: 377
Ion Ratio Lower Upper
142 100
127 40.8 41.6 62.4#
141 0.0 11.6 17.4#

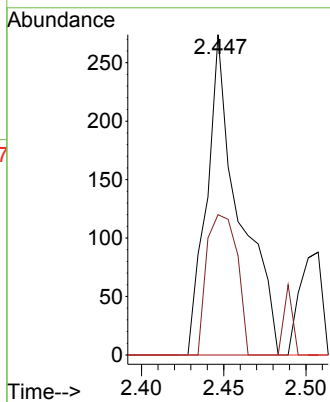

#11
Tert butyl alcohol
Concen: 7.197 ug/l
RT: 3.007 min Scan# 315
Delta R.T. -0.012 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion: 59 Resp: 2866
Ion Ratio Lower Upper
59 100
57 9.3 6.0 9.0#

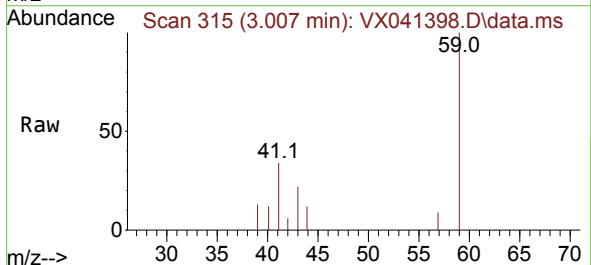



#13

Acrolein

Concen: 0.241 ug/l

RT: 2.239 min Scan# 189

Delta R.T. -0.000 min


Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 56 Resp: 76

Ion Ratio Lower Upper

56 100

55 30.3 57.1 85.7#

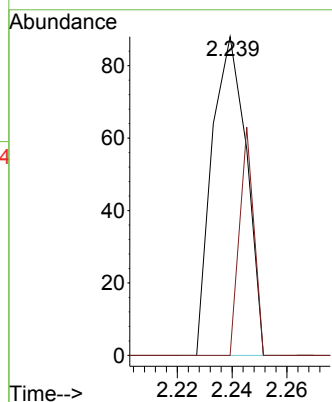

#14

Allyl chloride

Concen: 0.216 ug/l

RT: 2.660 min Scan# 258

Delta R.T. -0.000 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47




Tgt Ion: 41 Resp: 513


Ion Ratio Lower Upper

41 100

39 26.1 55.8 83.6#

76 0.0 24.3 36.5#

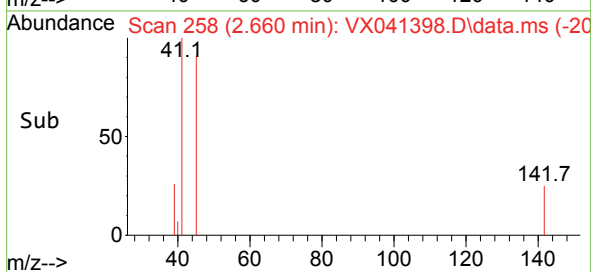



#15

Acrylonitrile

Concen: 0.276 ug/l

RT: 3.081 min Scan# 31

Delta R.T. 0.006 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 53 Resp: 251

Ion Ratio Lower Upper

53 100

52 56.6 66.0 99.0#

51 0.0 29.8 44.6#

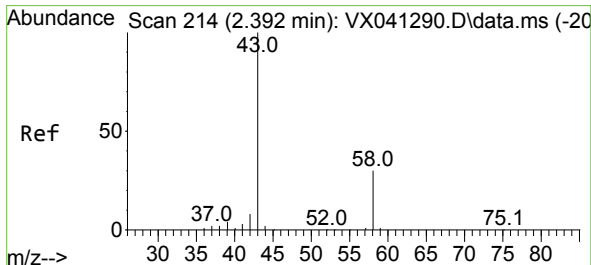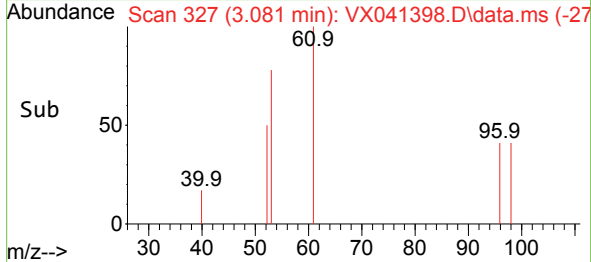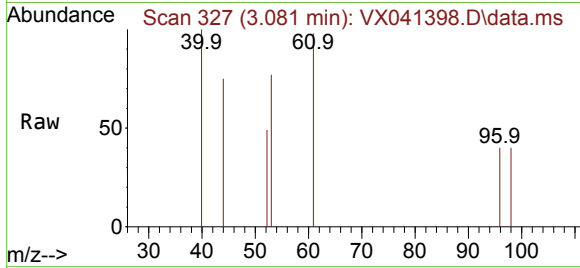

#16

Acetone

Concen: 18.040 ug/l

RT: 2.386 min Scan# 213

Delta R.T. -0.006 min

Lab File: VX041398.D




Acq: 07 May 2024 11:47


Tgt Ion: 43 Resp: 18986

Ion Ratio Lower Upper

43 100

58 29.6 21.9 32.9



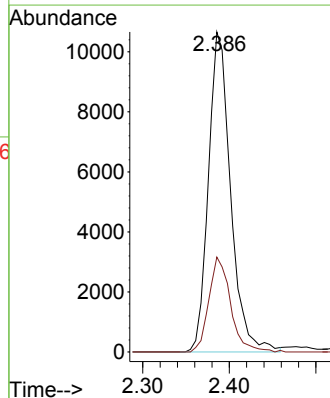
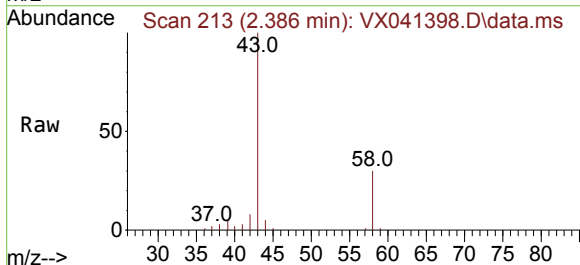


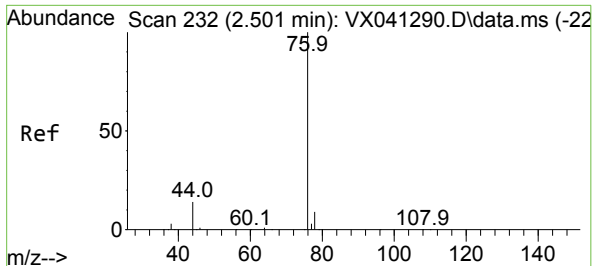

#17
Carbon Disulfide
Concen: 0.436 ug/l
RT: 2.501 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 76 Resp: 1452
Ion Ratio Lower Upper
76 100
78 13.4 7.0 10.6#

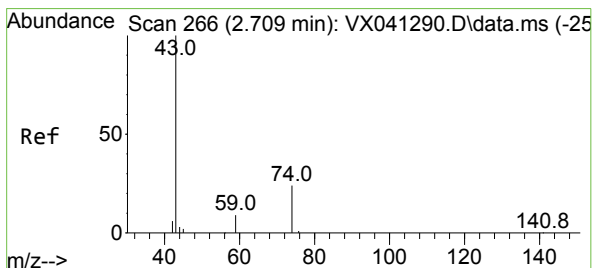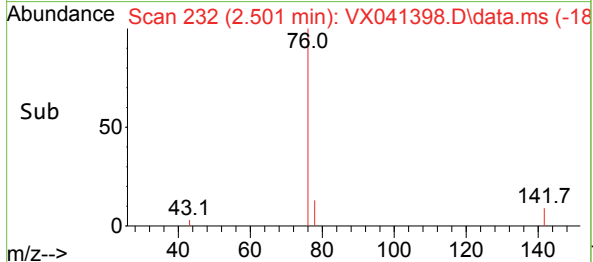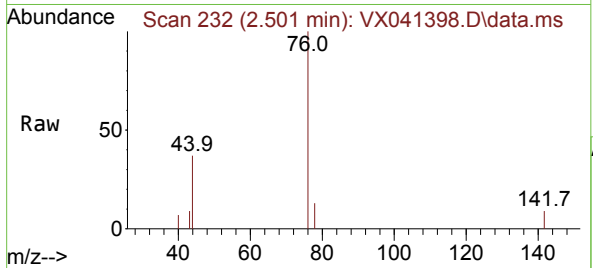

#18
Methyl Acetate
Concen: 0.879 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47


Tgt Ion: 43 Resp: 1789
Ion Ratio Lower Upper
43 100
74 21.4 17.8 26.8

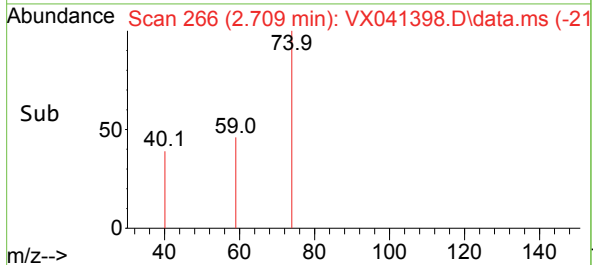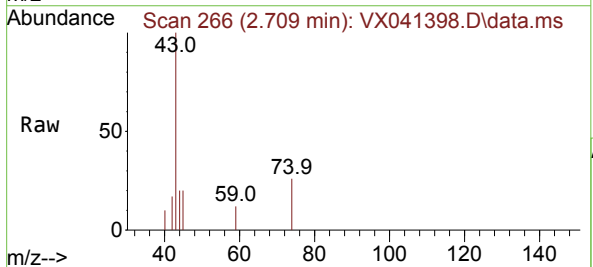





#20
Methylene Chloride
Concen: 2.806 ug/l
RT: 2.782 min Scan# 21
Delta R.T. -0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 84	Resp: 4847
Ion Ratio	Lower Upper
84 100	
49 108.7	103.6 155.4
51 39.7	33.8 50.6
86 60.2	49.4 74.0



#25
2-Butanone
Concen: 10.570 ug/l
RT: 4.568 min Scan# 571
Delta R.T. -0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion: 43	Resp: 13612
Ion Ratio	Lower Upper
43 100	
72 23.9	19.4 29.2





#29

Tetrahydrofuran

Concen: 1.824 ug/l

RT: 5.025 min Scan# 64

Delta R.T. 0.012 min


Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :






Tgt Ion: 42 Resp: 1536

Ion Ratio Lower Upper

42 100

72 16.7 34.2 51.4#

71 14.6 32.2 48.2#

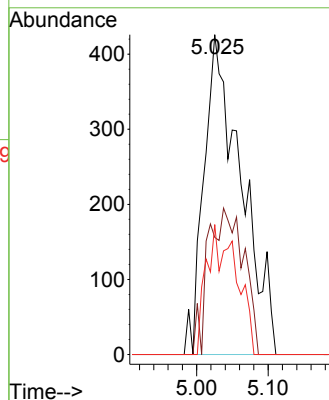

#31

Cyclohexane

Concen: 1.278 ug/l

RT: 5.537 min Scan# 730

Delta R.T. 0.073 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47




Tgt Ion: 56 Resp: 3068


Ion Ratio Lower Upper

56 100

69 161.4 23.4 35.2#

84 124.3 65.9 98.9#

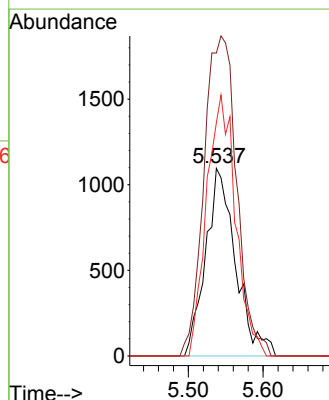



#33

1,2-Dichloroethane-d4

Concen: 49.258 ug/l

RT: 5.946 min Scan# 798

Delta R.T. -0.006 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 65 Resp: 98006

Ion Ratio Lower Upper

65 100

67 50.4 0.0 100.2



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47




Tgt Ion: 114 Resp: 270416


Ion Ratio Lower Upper

114 100

63 18.3 0.0 45.0

88 15.6 0.0 36.6



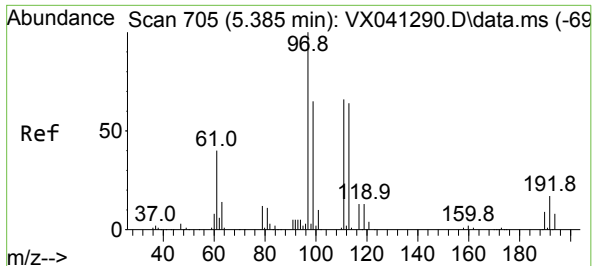

#35

Dibromofluoromethane

Concen: 44.001 ug/l

RT: 5.379 min Scan# 705

Delta R.T. -0.006 min

Lab File: VX041398.D





Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion:113 Resp: 80633
 Ion Ratio Lower Upper
 113 100
 111 101.8 82.9 124.3
 192 25.2 13.3 19.9#

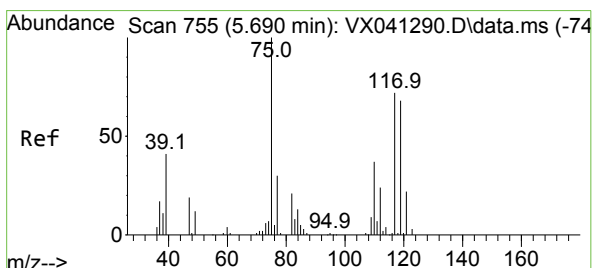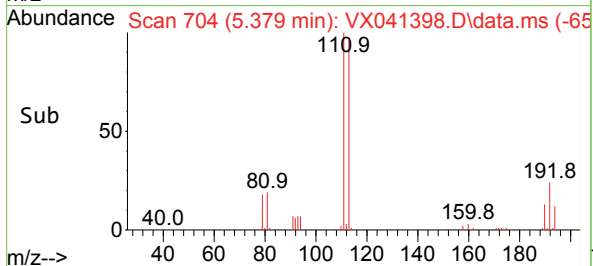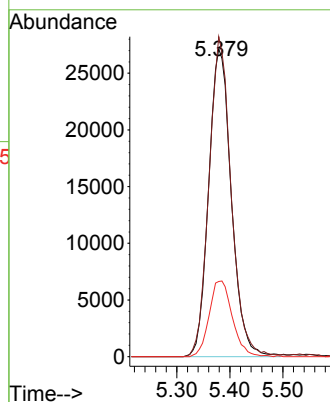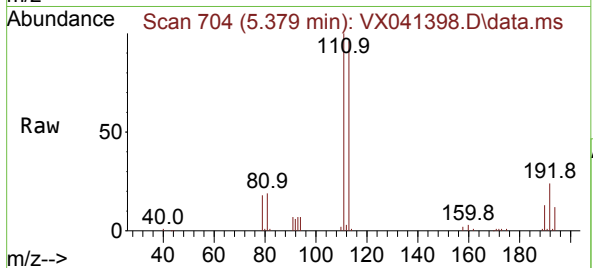

#36

1,1-Dichloropropene

Concen: 5.171 ug/l




RT: 5.544 min Scan# 731


Delta R.T. -0.146 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Tgt Ion: 75 Resp: 11332
 Ion Ratio Lower Upper
 75 100
 110 9.9 17.0 50.9#
 77 0.0 24.7 37.1#

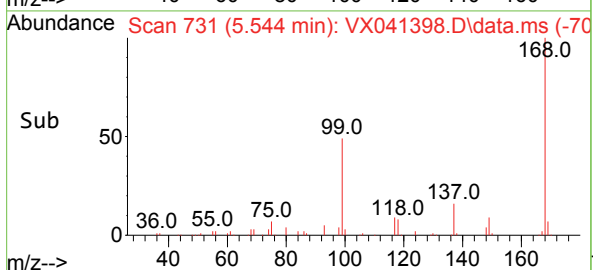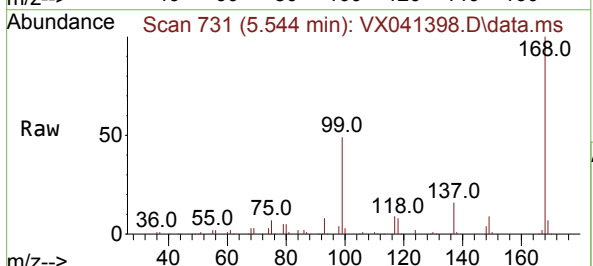



#37

Ethyl Acetate

Concen: 4.979 ug/l

RT: 4.568 min Scan# 51

Delta R.T. -0.152 min


Lab File: VX041398.D

Acq: 07 May 2024 11:47




Instrument :

MSVOA_X

ClientSampleId :



Tgt Ion: 43	Resp: 13612
Ion Ratio	Lower Upper
43	100
61	0.0 10.6 16.0#
70	0.0 8.3 12.5#

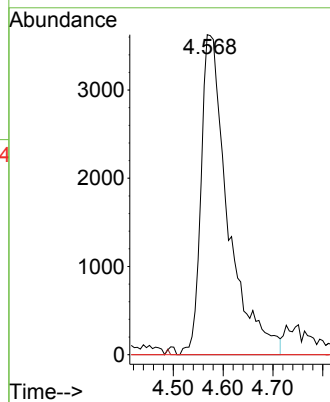

#38

Carbon Tetrachloride

Concen: 6.238 ug/l




RT: 5.544 min Scan# 731


Delta R.T. -0.128 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47


Tgt Ion: 117	Resp: 15659
Ion Ratio	Lower Upper
117	100
119	4.8 78.2 117.2#
121	0.0 24.4 36.6#








#41
Methacrylonitrile
Concen: 0.696 ug/l
RT: 5.025 min Scan# 646
Delta R.T. 0.097 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Instrument :
MSVOA_X
ClientSampleId :







Tgt Ion: 41	Resp: 980
Ion Ratio	Lower Upper
41 100	
39 11.9	45.2 67.8#
67 0.0	52.6 78.8#
52 0.0	22.7 34.1#



#43
Isopropyl Acetate
Concen: 14.312 ug/l
RT: 6.342 min Scan# 862
Delta R.T. -0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion: 43	Resp: 58834
Ion Ratio	Lower Upper
43 100	
61 19.6	15.2 22.8
87 13.9	9.8 14.6





#48

Methyl methacrylate

Concen: 0.780 ug/l

RT: 7.622 min Scan# 1084

Delta R.T. -0.073 min

Lab File: VX041398.D





Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :

Tgt Ion: 41	Resp: 1469
Ion Ratio	Lower Upper
41	100
69	0.0 59.2 88.8#
39	130.3 47.7 71.5#

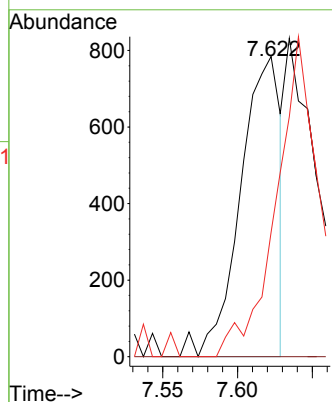

#50

Toluene-d8

Concen: 52.878 ug/l




RT: 8.647 min Scan# 1240


Delta R.T. -0.000 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Tgt Ion: 98	Resp: 306696
Ion Ratio	Lower Upper
98	100
100	66.0 53.1 79.7


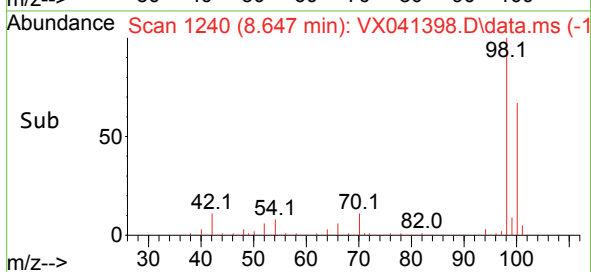
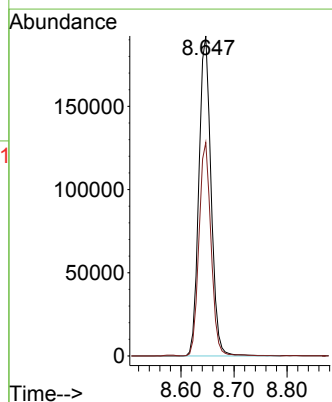





#51
4-Methyl-2-Pentanone
Concen: 20.090 ug/l
RT: 8.549 min Scan# 11
Delta R.T. -0.031 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 43 Resp: 49556
Ion Ratio Lower Upper
43 100
58 6.5 30.4 45.6#



#52
Toluene
Concen: 0.456 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. 0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion: 92 Resp: 1886
Ion Ratio Lower Upper
92 100
91 160.3 134.2 201.2









#54
 cis-1,3-Dichloropropene
 Concen: 9.045 ug/l
 RT: 8.549 min Scan# 1194
 Delta R.T. 0.183 min
 Lab File: VX041398.D
 Acq: 07 May 2024 11:47




Instrument :
 MSVOA_X
 ClientSampleId :


Tgt Ion: 75 Resp: 21289
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.3 37.9#
 39 32.1 46.7 70.1#

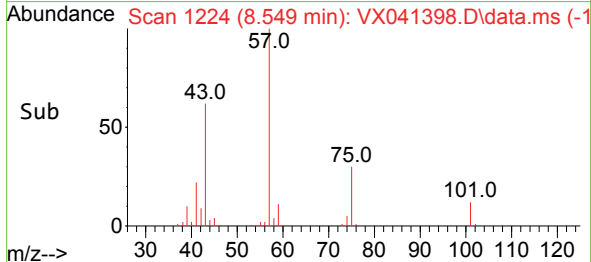

#56
 Ethyl methacrylate
 Concen: 0.254 ug/l
 RT: 9.238 min Scan# 1337
 Delta R.T. 0.122 min
 Lab File: VX041398.D
 Acq: 07 May 2024 11:47

Tgt Ion: 69 Resp: 626
 Ion Ratio Lower Upper
 69 100
 41 5674.0 56.8 85.2#
 39 2351.8 32.0 48.0#





#57

1,3-Dichloropropane

Concen: 0.272 ug/l

RT: 9.488 min Scan# 11

Delta R.T. 0.183 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X





ClientSampleId :

Tgt Ion: 76 Resp: 723

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#



#59

2-Hexanone

Concen: 3.435 ug/l

RT: 9.439 min Scan# 1370

Delta R.T. 0.006 min

Lab File: VX041398.D




Acq: 07 May 2024 11:47


Tgt Ion: 43 Resp: 6775

Ion Ratio Lower Upper

43 100

58 49.6 26.2 78.5









#62
4-Bromofluorobenzene
Concen: 52.864 ug/l
RT: 11.079 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 95 Resp: 118693
Ion Ratio Lower Upper
95 100
174 97.5 0.0 135.6
176 96.3 0.0 131.0



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47


Tgt Ion: 117 Resp: 265597
Ion Ratio Lower Upper
117 100
82 53.8 46.2 69.4
119 32.1 25.5 38.3








#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Instrument :
MSVOA_X
ClientSampleId :



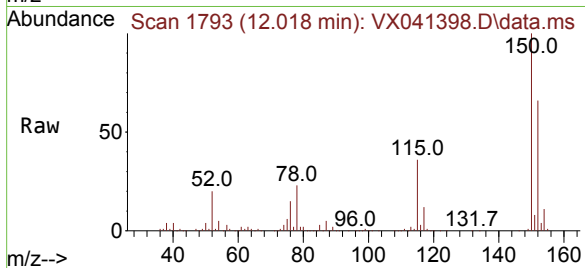



Tgt Ion:152 Resp: 138443
Ion Ratio Lower Upper
152 100
115 53.4 43.3 129.9
150 153.8 0.0 345.0

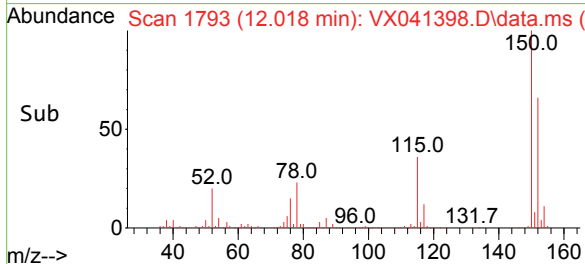

#76
1,2,3-Trichloropropane
Concen: 26.621 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.159 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion: 75 Resp: 60061
Ion Ratio Lower Upper
75 100
77 1.0 19.1 57.5#


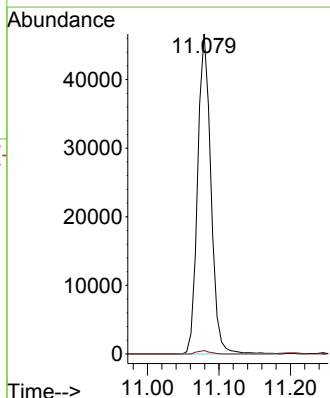
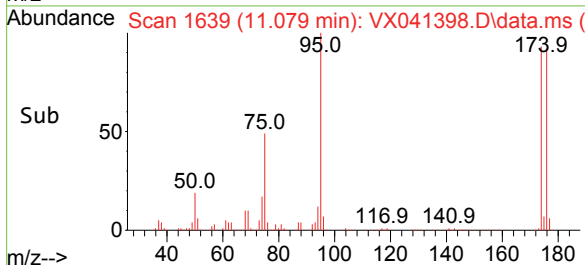
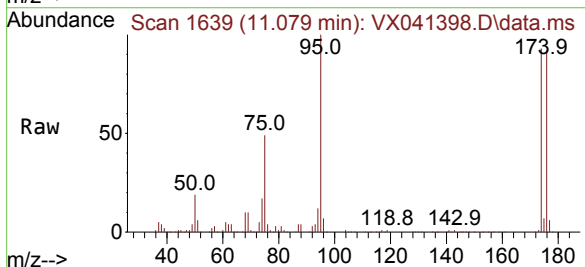




#81
trans-1,4-Dichloro-2-butene
Concen: 72.511 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 75 Resp: 60061
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 36.9 55.3#

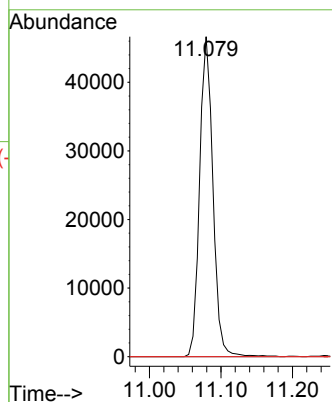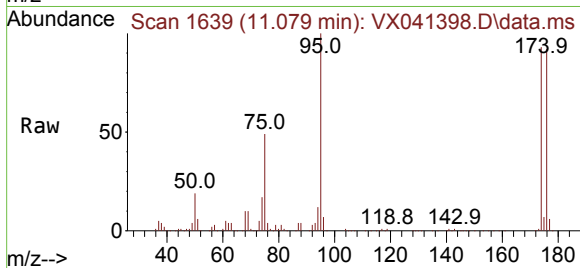

#84
1,2,4-Trimethylbenzene
Concen: 0.435 ug/l
RT: 11.750 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VX041398.D
Acq: 07 May 2024 11:47

Tgt Ion:105 Resp: 3016
Ion Ratio Lower Upper
105 100
120 47.2 21.2 63.6

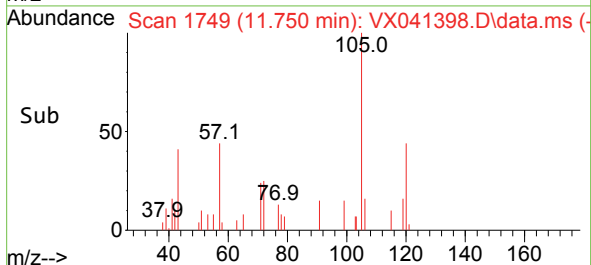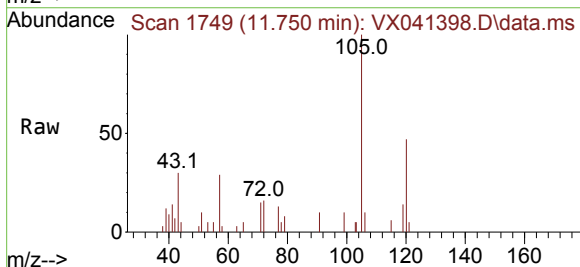



#89

n-Butylbenzene

Concen: 0.202 ug/l

RT: 12.317 min Scan# 11

Delta R.T. -0.012 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion: 91 Resp: 1235

Ion Ratio Lower Upper

91 100

92 25.2 27.4 82.0#

134 125.6 12.6 37.8#



#90

Hexachloroethane

Concen: 0.490 ug/l

RT: 12.554 min Scan# 1881

Delta R.T. 0.018 min

Lab File: VX041398.D




Acq: 07 May 2024 11:47


Tgt Ion: 117 Resp: 622

Ion Ratio Lower Upper

117 100

201 0.0 32.9 98.6#





#93

1,2,4-Trichlorobenzene

Concen: 0.202 ug/l

RT: 13.597 min Scan# 2050

Delta R.T. 0.012 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47

Instrument :

MSVOA_X

ClientSampleId :





Tgt Ion:180 Resp: 647

Ion Ratio Lower Upper

180 100

182 86.4 48.3 144.8

145 28.4 18.0 54.0

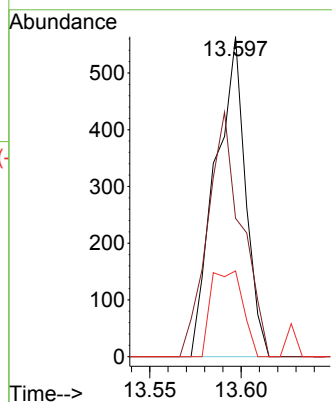

#95

Naphthalene

Concen: 2.144 ug/l

RT: 13.780 min Scan# 2082

Delta R.T. 0.006 min

Lab File: VX041398.D

Acq: 07 May 2024 11:47




Tgt Ion:128 Resp: 20334


Ion Ratio Lower Upper

128 100

127 13.3 10.3 15.5


129 11.1 8.8 13.2





#96
 1,2,3-Trichlorobenzene
 Concen: 0.212 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VX041398.D
 Acq: 07 May 2024 11:47

Instrument :
 MSVOA_X
 ClientSampleId :



Tgt Ion:	180	Resp:	692
Ion	Ratio	Lower	Upper
180	100		
182	86.3	46.9	140.6
145	30.2	17.8	53.5

