

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
 Data File : VX041401.D
 Acq On : 07 May 2024 13:08
 Operator : JC/MD
 Sample : P2393-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-7

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M

Title : SW846 8260

Signal : TIC: VX041401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.246	22	26	37	rBV2	7797	16333	1.04%	0.219%
2	1.581	66	81	82	rBV7	7397	22023	1.40%	0.295%
3	2.995	298	313	324	rBV	562923	1524207	96.88%	20.394%
4	3.117	324	333	358	rVB	666733	1573324	100.00%	21.051%
5	3.763	430	439	456	rVB	22083	59479	3.78%	0.796%
6	5.385	694	705	721	rBV	93404	273583	17.39%	3.660%
7	5.550	721	732	751	rVB	174467	501972	31.91%	6.716%
8	5.952	788	798	815	rBV	88946	240031	15.26%	3.212%
9	6.251	836	847	859	rBV4	25905	92066	5.85%	1.232%
10	6.757	921	930	946	rBV	231724	561029	35.66%	7.506%
11	7.982	1124	1131	1139	rVB	9794	19434	1.24%	0.260%
12	8.647	1233	1240	1255	rBV	456704	713636	45.36%	9.548%
13	10.055	1465	1471	1484	rVB	453607	645948	41.06%	8.643%
14	11.079	1634	1639	1650	rBV	438914	555937	35.34%	7.438%
15	12.018	1788	1793	1805	rBV	520363	674967	42.90%	9.031%




Sum of corrected areas: 7473969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041401.D
Acq On : 07 May 2024 13:08
Operator : JC/MD
Sample : P2393-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

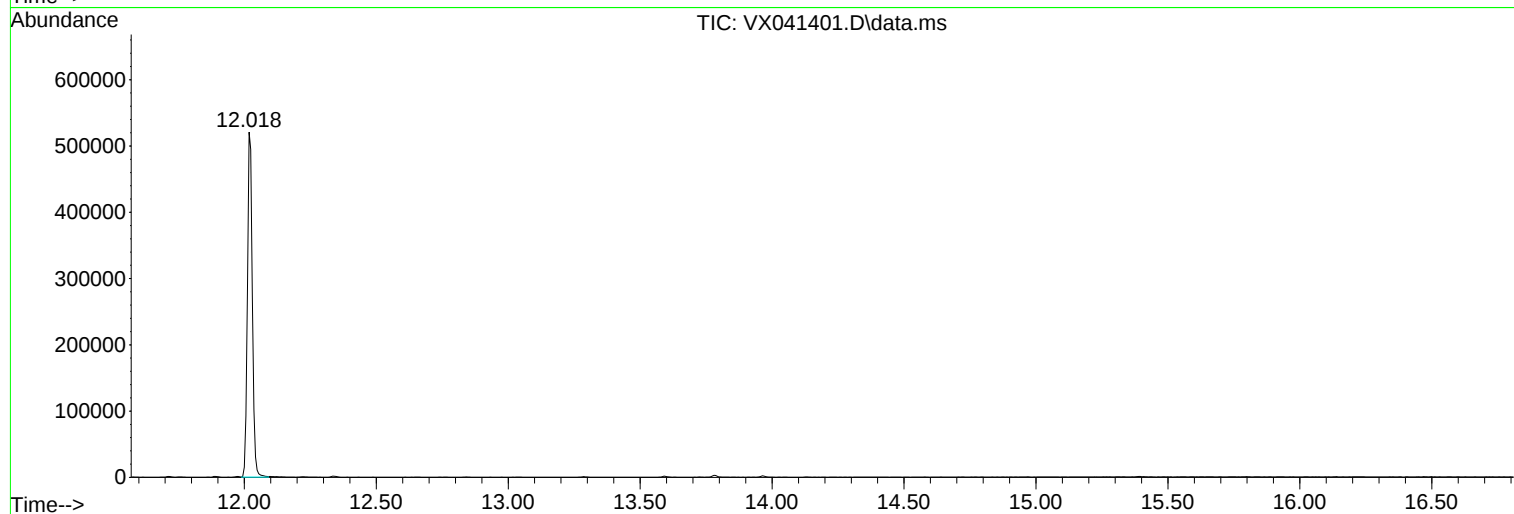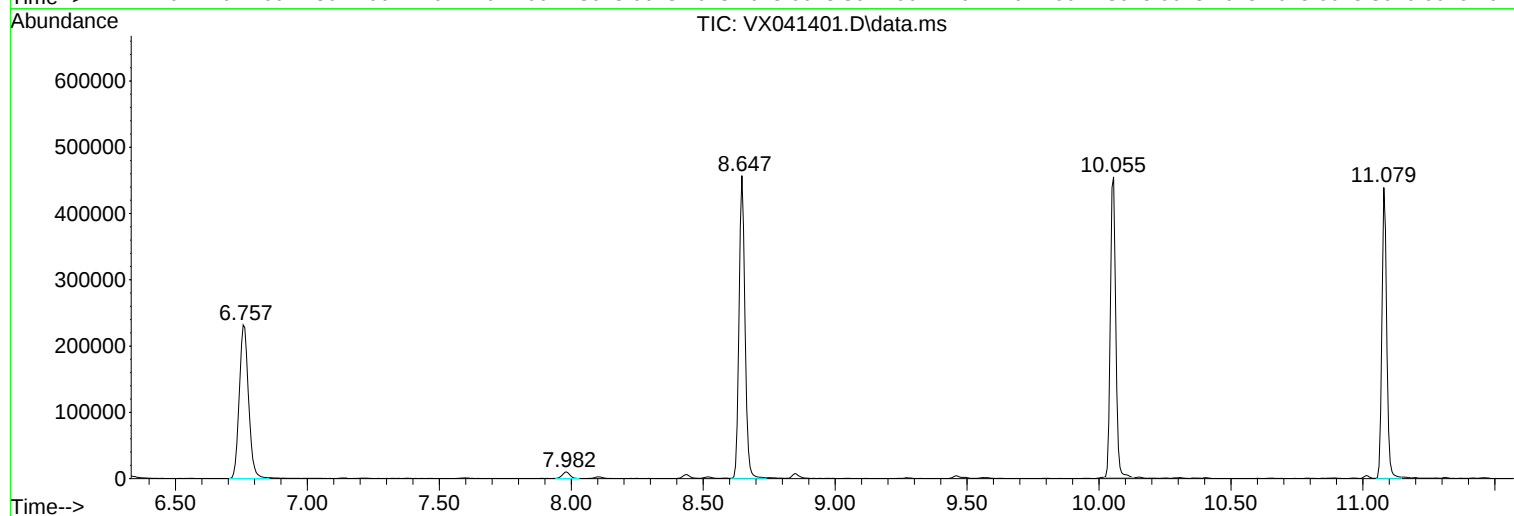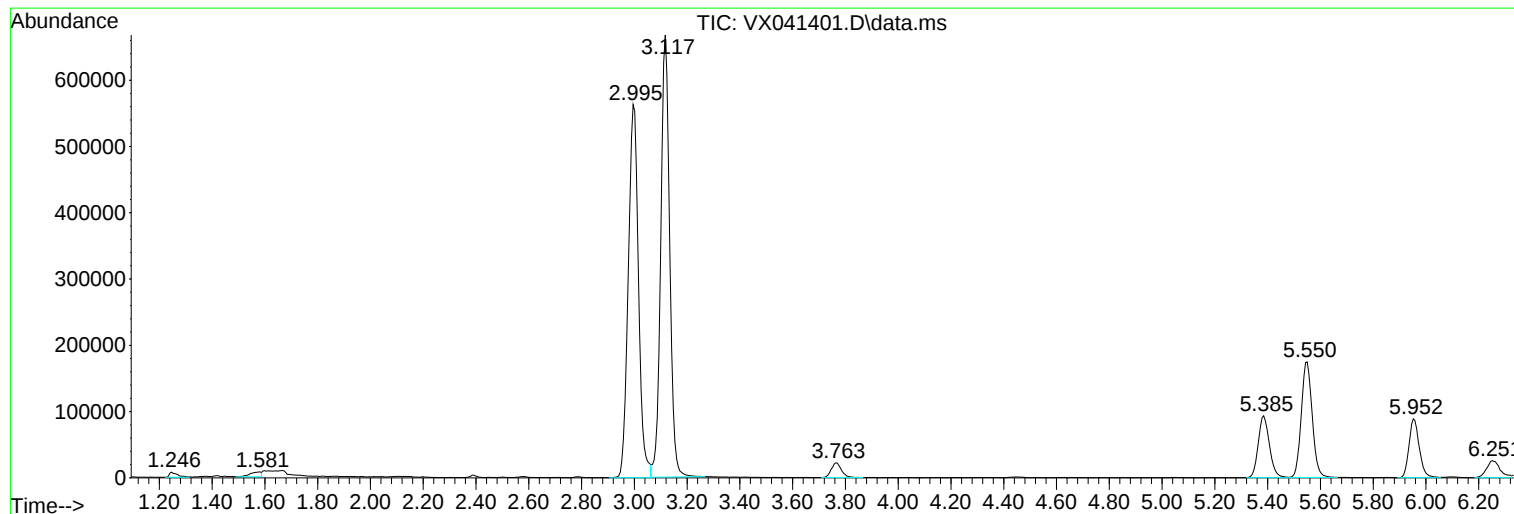

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041401.D
Acq On : 07 May 2024 13:08
Operator : JC/MD
Sample : P2393-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Amylene hydrate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.251	8.21 ug/l	92066	1,4-Difluorobenzene	6.757

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Amylene hydrate	88	C5H12O	000075-85-4	59
2			N,N-Dimethylformamide-di-t-butyl...	203	C11H25NO2	036805-97-7	59
3			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	50
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	42
5			Formic acid, 1,1-dimethylethyl e...	102	C5H10O2	000762-75-4	42

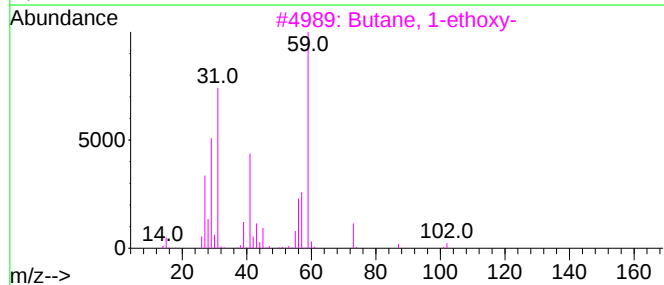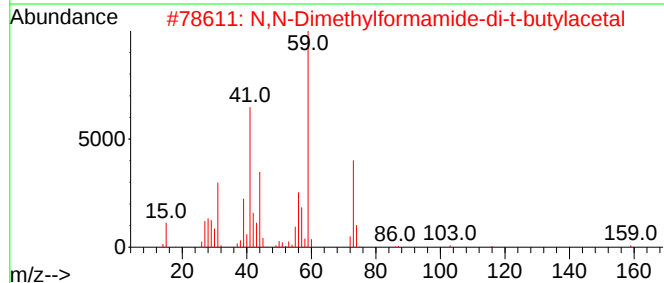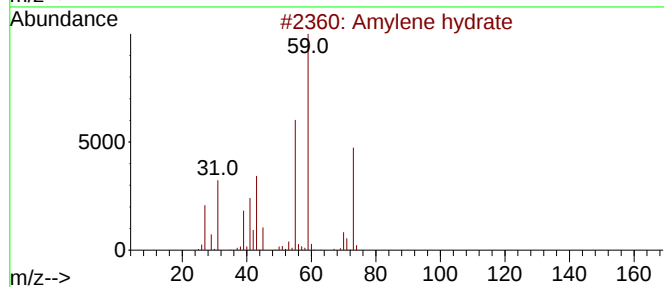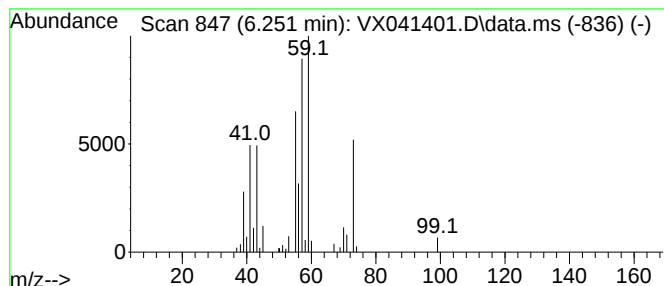

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041401.D
Acq On : 07 May 2024 13:08
Operator : JC/MD
Sample : P2393-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Amylene hydrate	6.251	8.2	ug/l	92066	2	6.757	561029	50.0