

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
 Data File : VX041405.D
 Acq On : 07 May 2024 14:40
 Operator : JC/MD
 Sample : P2389-02 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 1401

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
 Title : SW846 8260

Signal : TIC: VX041405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	35	rBV3	4477	10293	1.09%	0.192%
2	1.453	56	60	63	rBV	778742	941974	100.00%	17.597%
3	1.483	63	65	82	rVB	147533	289674	30.75%	5.411%
4	2.081	158	163	170	rBV	42884	67052	7.12%	1.253%
5	2.294	193	198	202	rBV	11257	18197	1.93%	0.340%
6	2.947	295	305	317	rBV	7562	18119	1.92%	0.338%
7	4.239	507	517	534	rBV3	5815	21022	2.23%	0.393%
8	5.385	687	705	721	rBV	88515	265222	28.16%	4.955%
9	5.550	721	732	749	rVV	168363	466285	49.50%	8.711%
10	5.952	789	798	821	rBV	89542	244757	25.98%	4.572%
11	6.763	920	931	944	rBV	203782	497057	52.77%	9.286%
12	6.879	944	950	967	rVB2	14434	38458	4.08%	0.718%
13	7.214	999	1005	1015	rBV3	9232	23105	2.45%	0.432%
14	8.647	1233	1240	1250	rBV	415857	648493	68.84%	12.115%
15	10.055	1465	1471	1488	rBV	452736	631327	67.02%	11.794%
16	10.311	1505	1513	1523	rVB2	15415	23277	2.47%	0.435%
17	11.079	1634	1639	1661	rBV	387299	505530	53.67%	9.444%
18	12.018	1788	1793	1804	rBV	473355	614508	65.24%	11.480%
19	12.219	1819	1826	1833	rBV2	6661	12886	1.37%	0.241%
20	12.414	1853	1858	1866	rBV	12114	15737	1.67%	0.294%




Sum of corrected areas: 5352973

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041405.D
Acq On : 07 May 2024 14:40
Operator : JC/MD
Sample : P2389-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

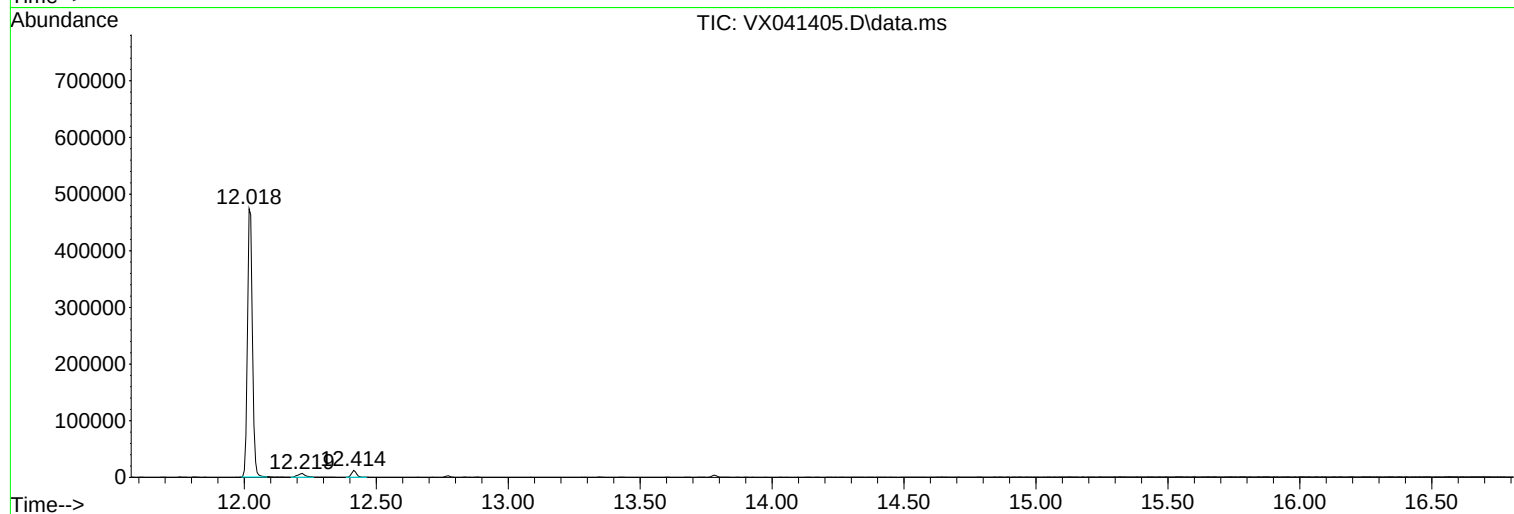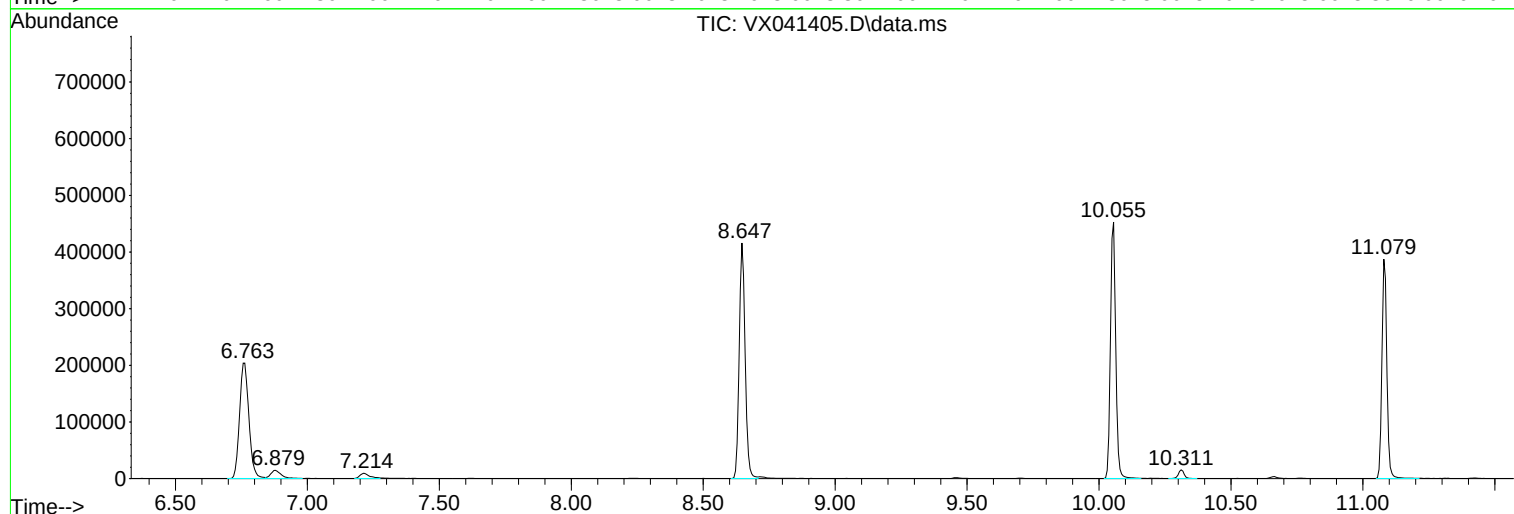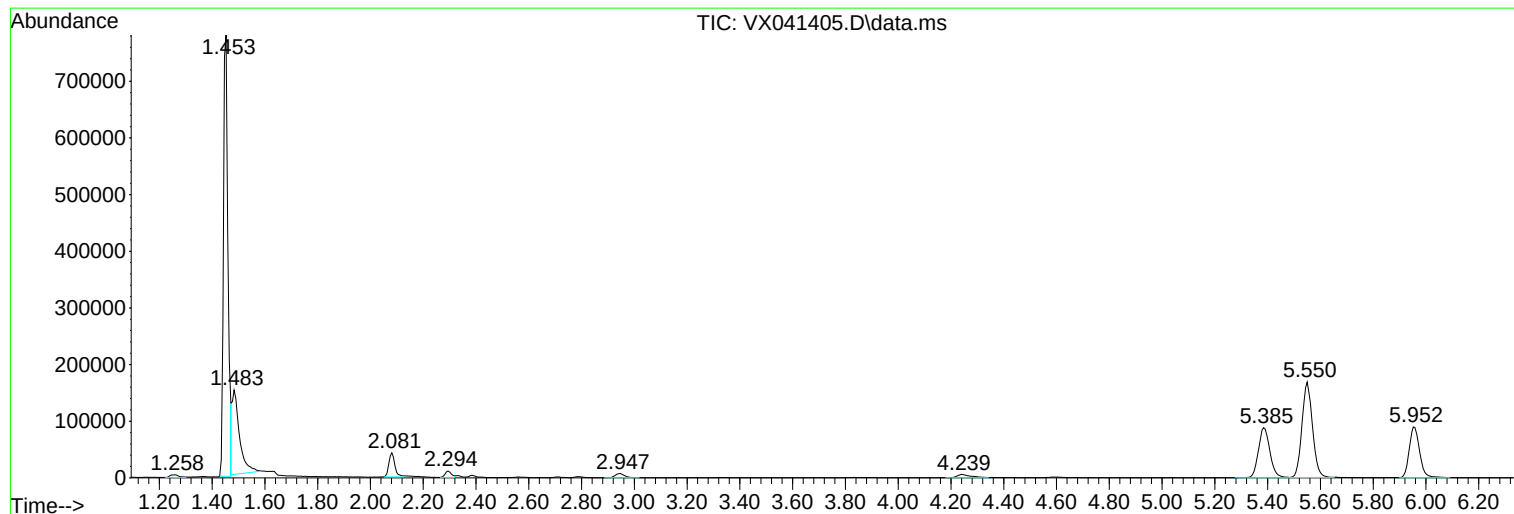

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041405.D
Acq On : 07 May 2024 14:40
Operator : JC/MD
Sample : P2389-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050724\
Data File : VX041405.D
Acq On : 07 May 2024 14:40
Operator : JC/MD
Sample : P2389-02 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
1401

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X043024W.M
Quant Title : SW846 8260

TIC Library :
TIC Integration Parameters: RTEINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------