

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050725\
 Data File : VX046070.D
 Acq On : 07 May 2025 10:32
 Operator : JC/MD
 Sample : VX0507WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0507WBL01

Quant Time: May 08 01:46:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.544	168	65914	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	130814	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	121214	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	50569	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	66342	53.987	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.980%
35) Dibromofluoromethane	5.379	113	48880	51.890	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.780%
50) Toluene-d8	8.647	98	163501	50.148	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	100.300%
62) 4-Bromofluorobenzene	11.079	95	60261	48.184	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	96.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX050725\
Data File : VX046070.D
Acq On : 07 May 2025 10:32
Operator : JC/MD
Sample : VX0507WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0507WBL01

Quant Time: May 08 01:46:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




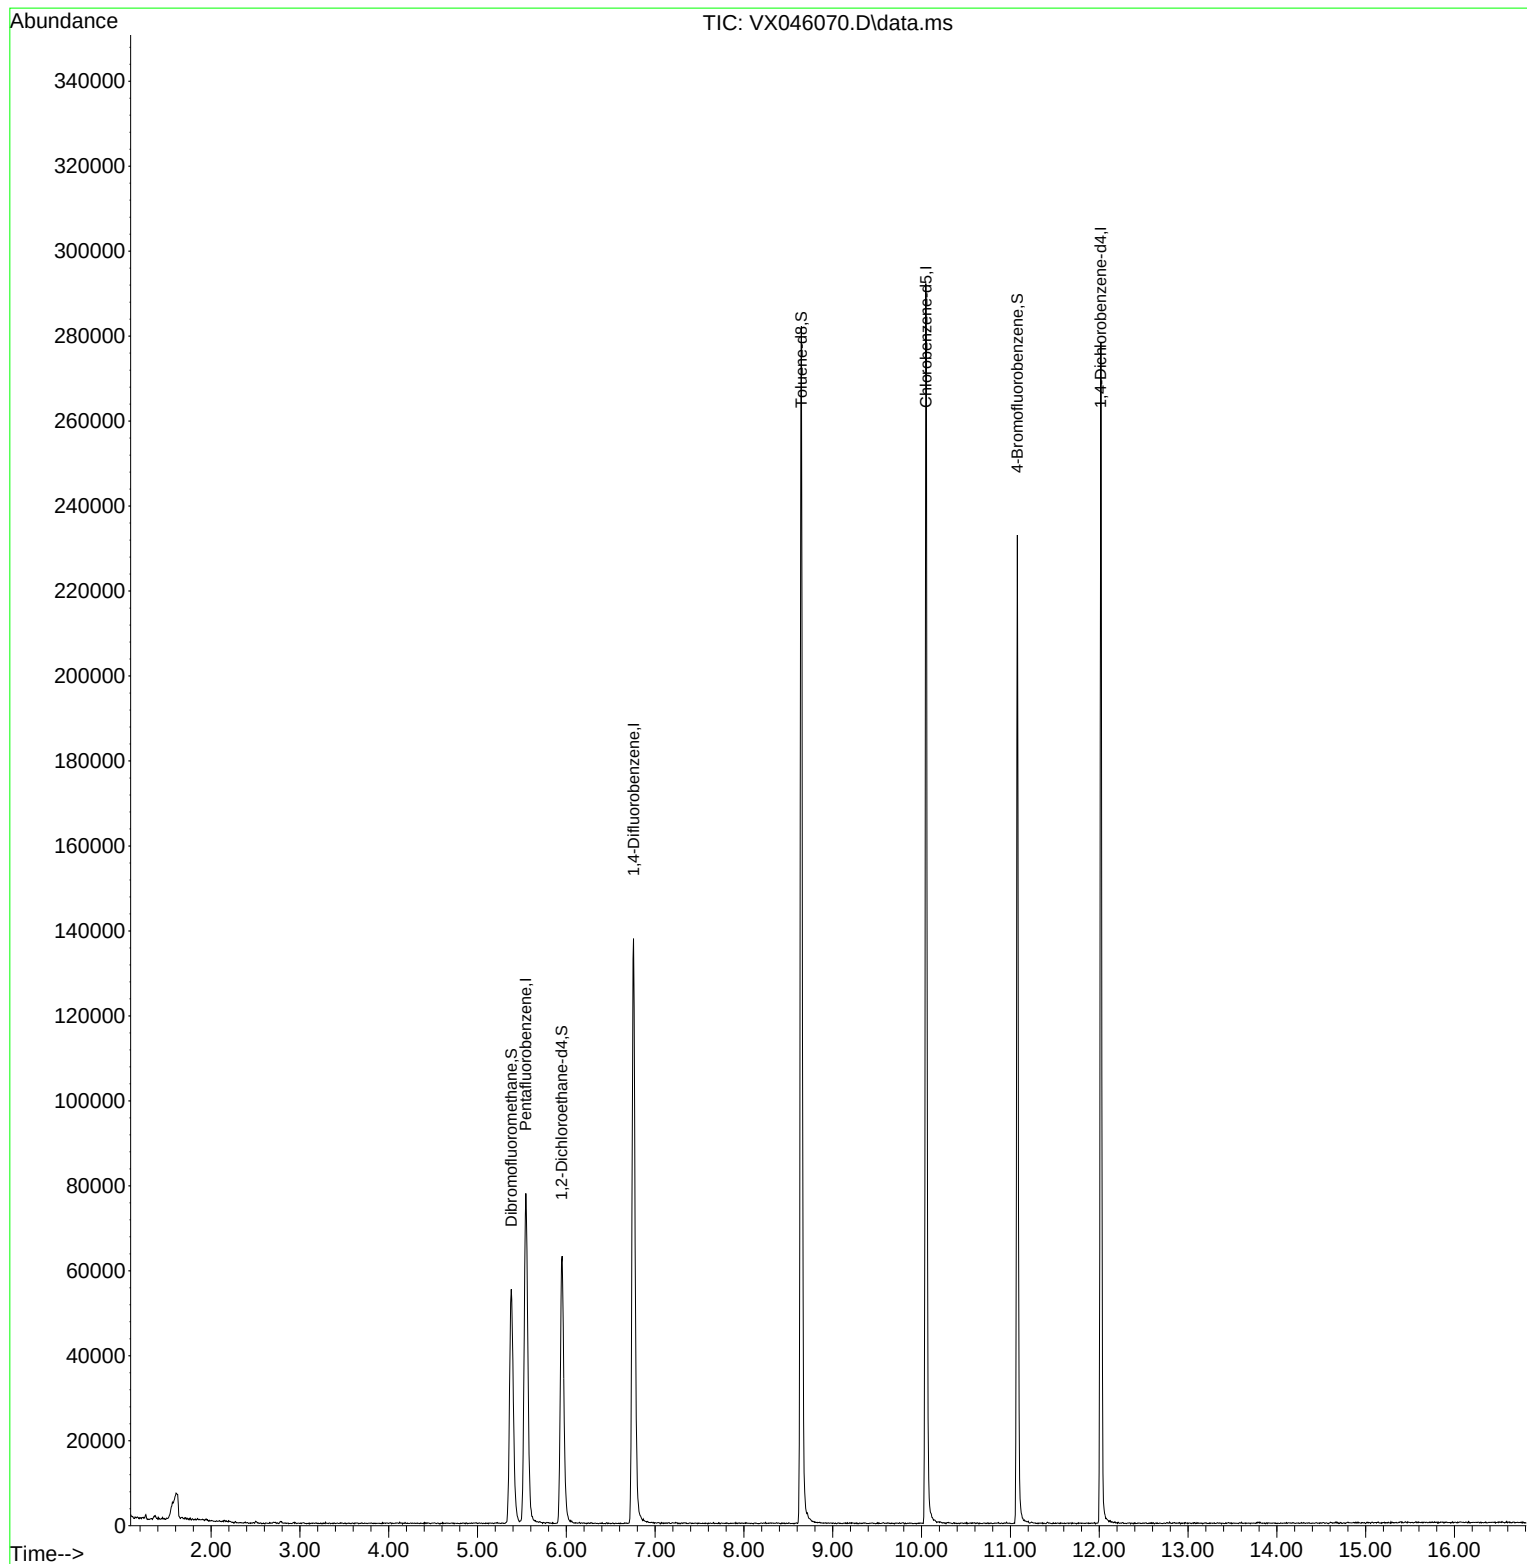


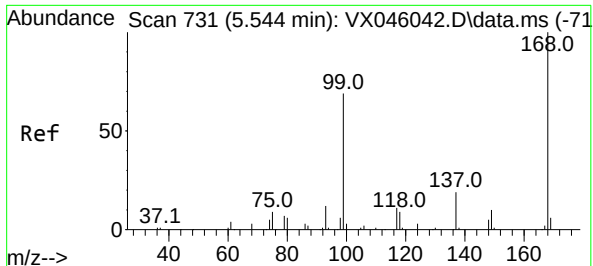

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0507WBL01


Tgt Ion:168 Resp: 65914
Ion Ratio Lower Upper
168 100
99 74.9 54.9 82.3

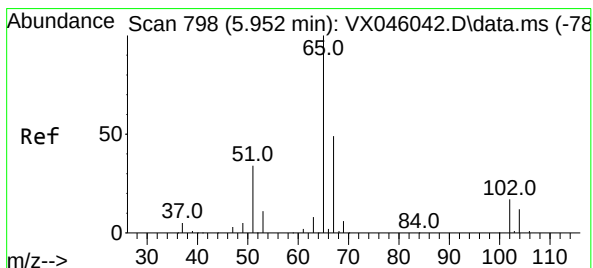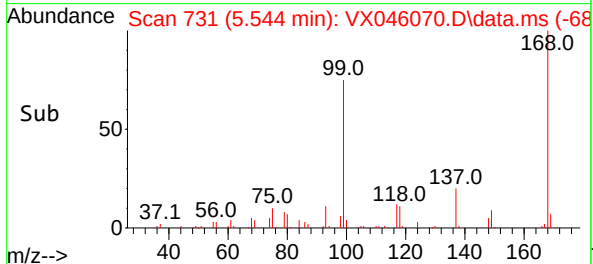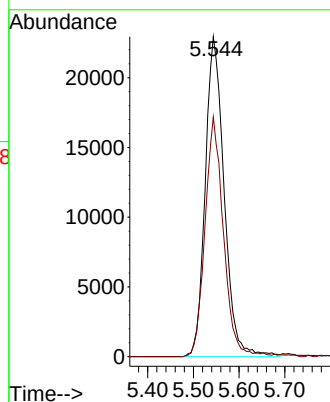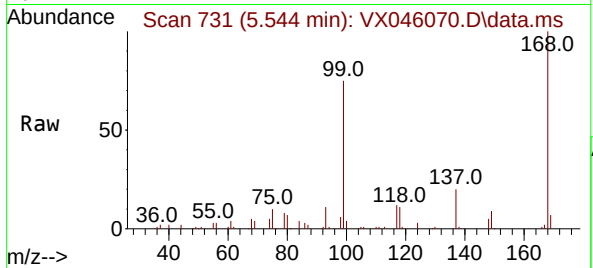

#33
1,2-Dichloroethane-d4
Concen: 53.987 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32

Tgt Ion: 65 Resp: 66342
Ion Ratio Lower Upper
65 100
67 48.8 0.0 99.0


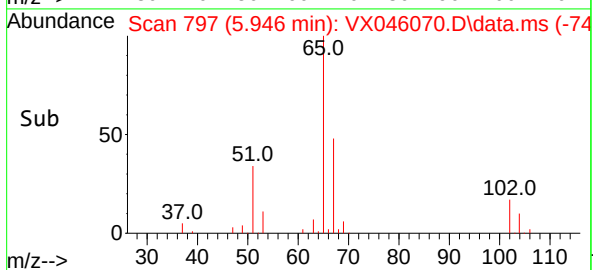
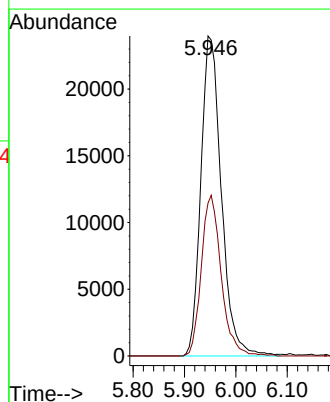
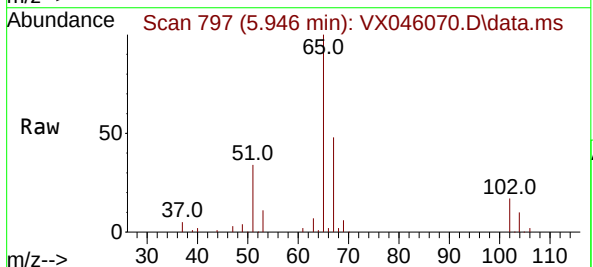


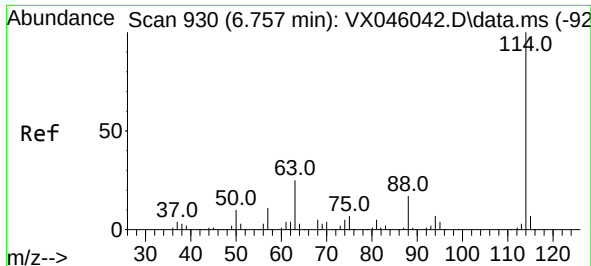

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 91
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0507WBL01


Tgt Ion:114 Resp: 130814
Ion Ratio Lower Upper
114 100
63 23.7 0.0 49.2
88 16.2 0.0 33.6

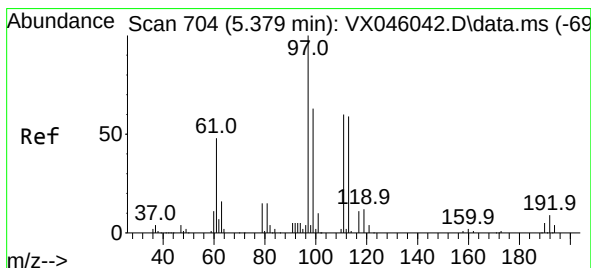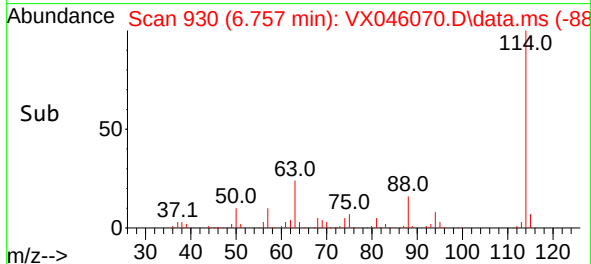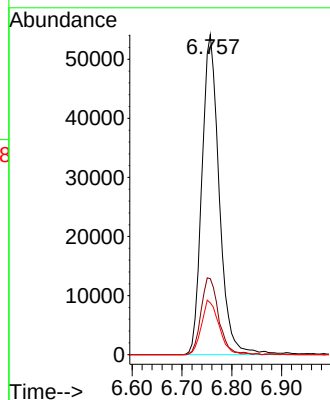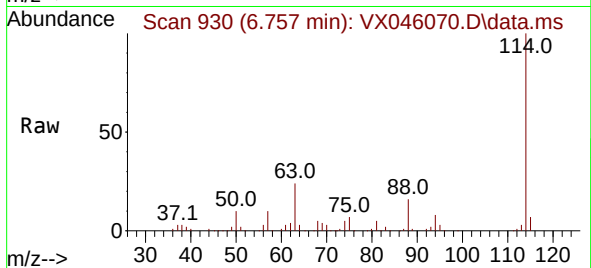

#35
Dibromofluoromethane
Concen: 51.890 ug/l
RT: 5.379 min Scan# 704
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32

Tgt Ion:113 Resp: 48880
Ion Ratio Lower Upper
113 100
111 101.5 83.1 124.7
192 16.2 13.3 19.9


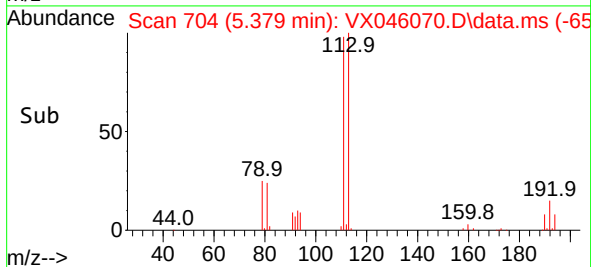
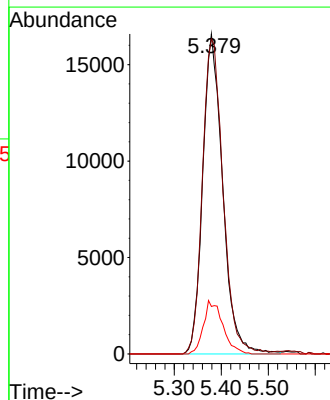
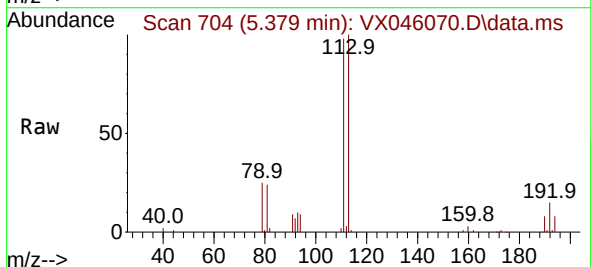


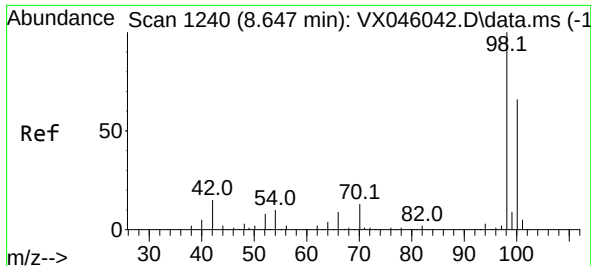

#50
Toluene-d8
Concen: 50.148 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32




Instrument :
MSVOA_X
ClientSampleId :
VX0507WBL01


Tgt Ion: 98 Resp: 163501
Ion Ratio Lower Upper
98 100
100 65.4 53.5 80.3

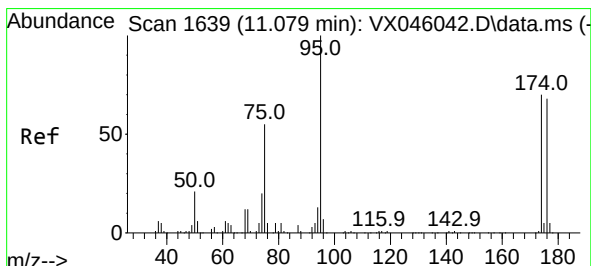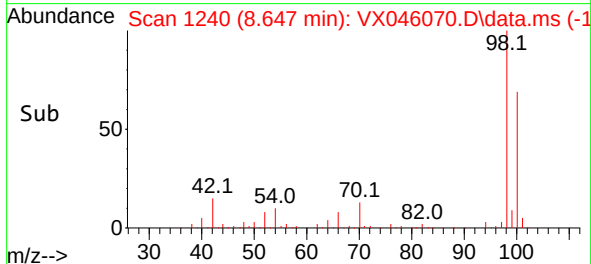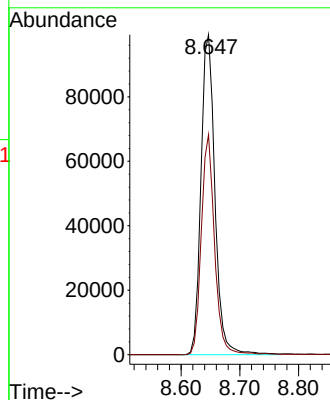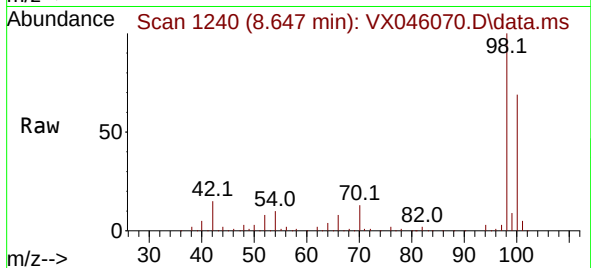

#62
4-Bromofluorobenzene
Concen: 48.184 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32

Tgt Ion: 95 Resp: 60261
Ion Ratio Lower Upper
95 100
174 68.0 0.0 135.8
176 65.2 0.0 131.4


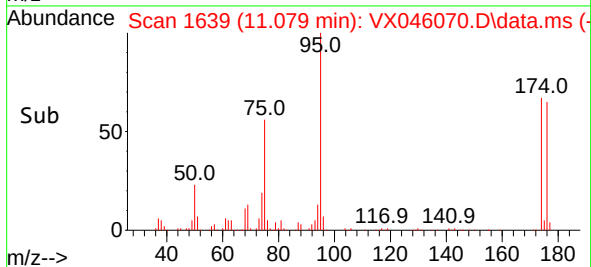
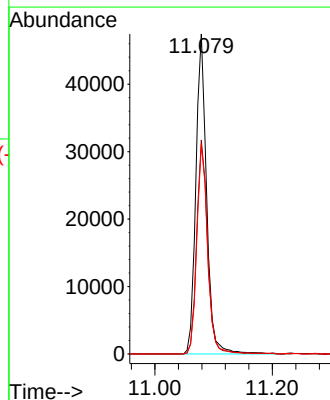
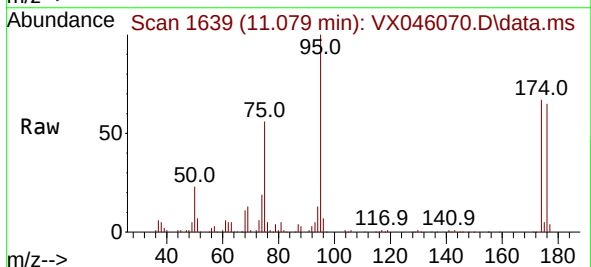


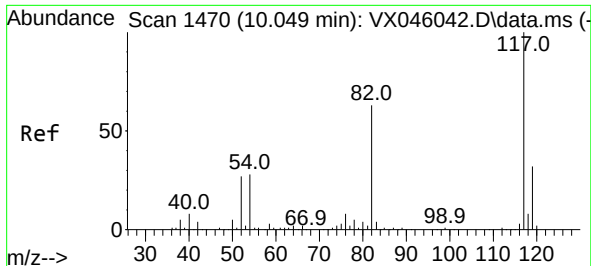

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32

Instrument :
MSVOA_X
ClientSampleId :
VX0507WBL01

Tgt Ion:117 Resp: 121214
Ion Ratio Lower Upper
117 100
82 64.2 50.6 76.0
119 32.4 25.8 38.6

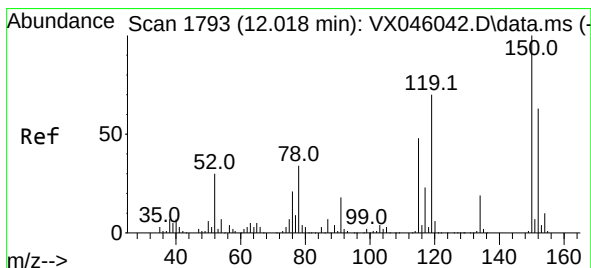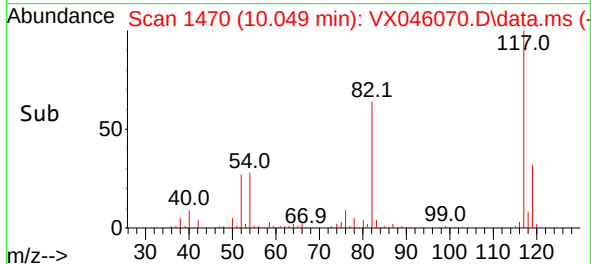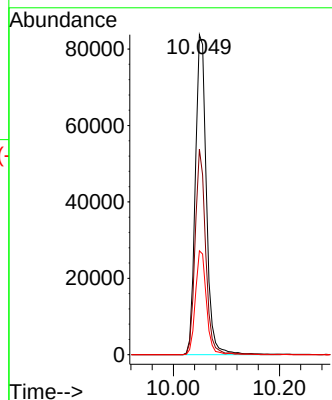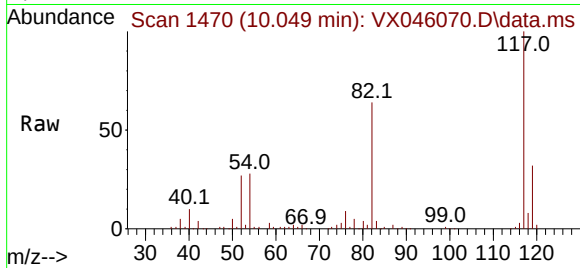

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046070.D
Acq: 07 May 2025 10:32

Tgt Ion:152 Resp: 50569
Ion Ratio Lower Upper
152 100
115 65.4 46.9 140.7
150 157.8 0.0 351.0

